
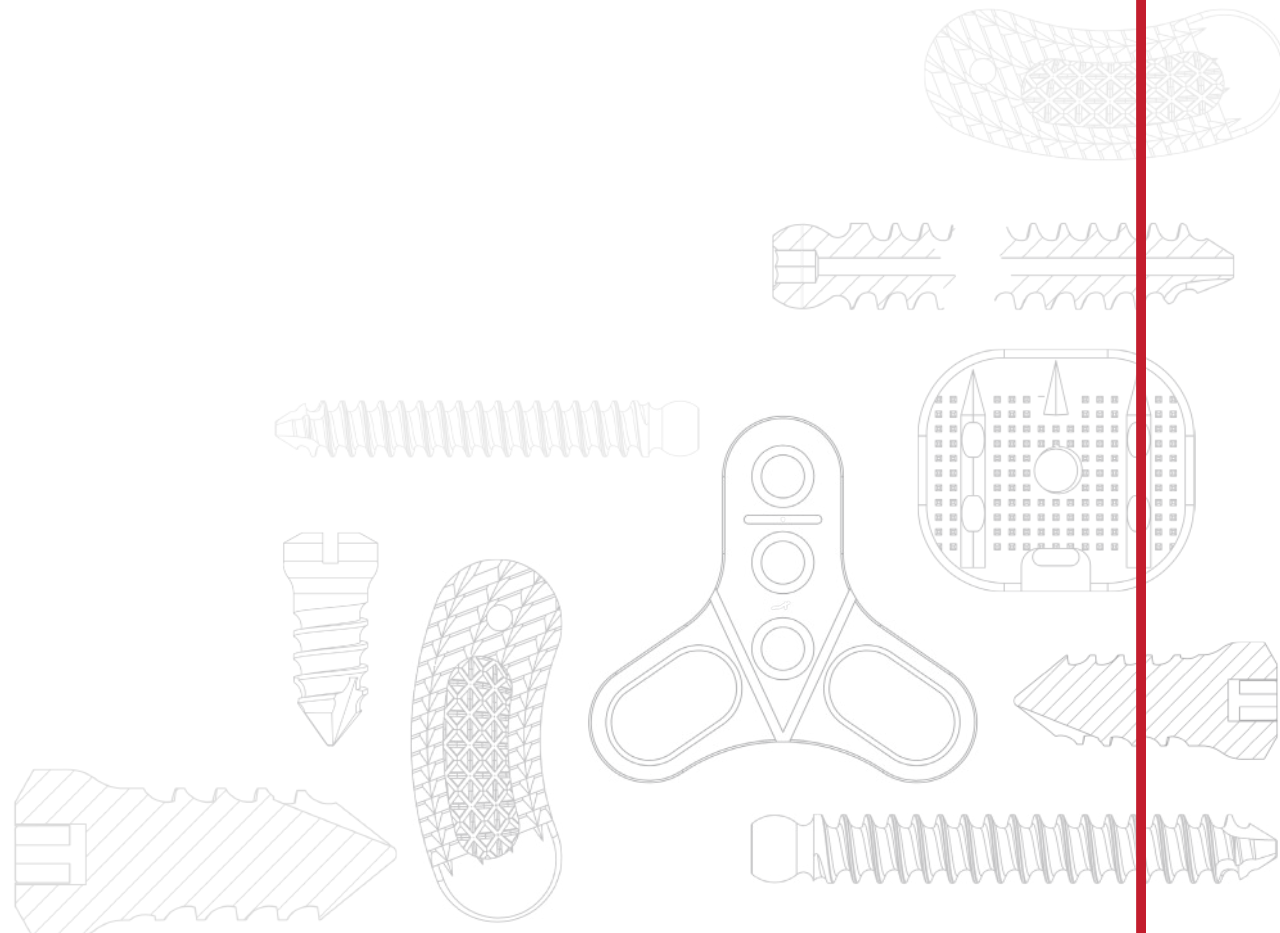


SPINAL PRODUCT CATALOG

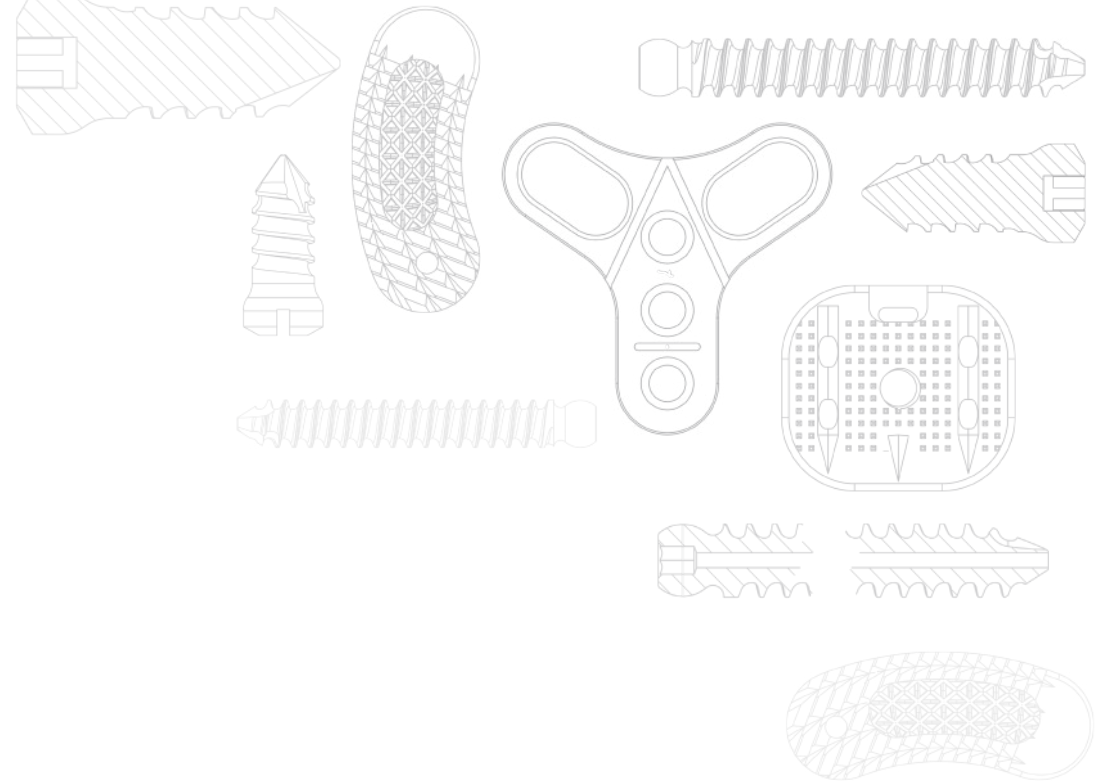

normmed
A Piece of You







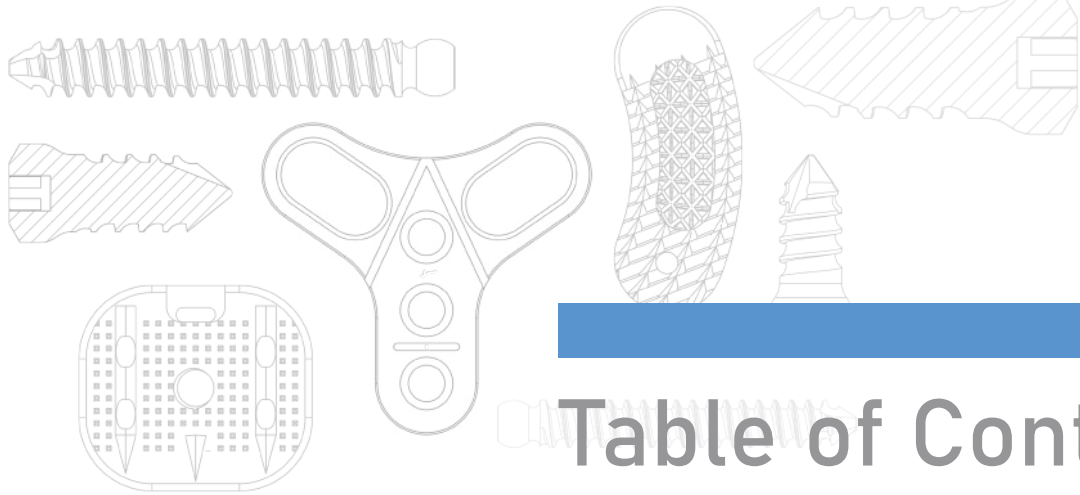



Table of Contents

05-43 **Implant Types**

44-54 **Instrument Sets**

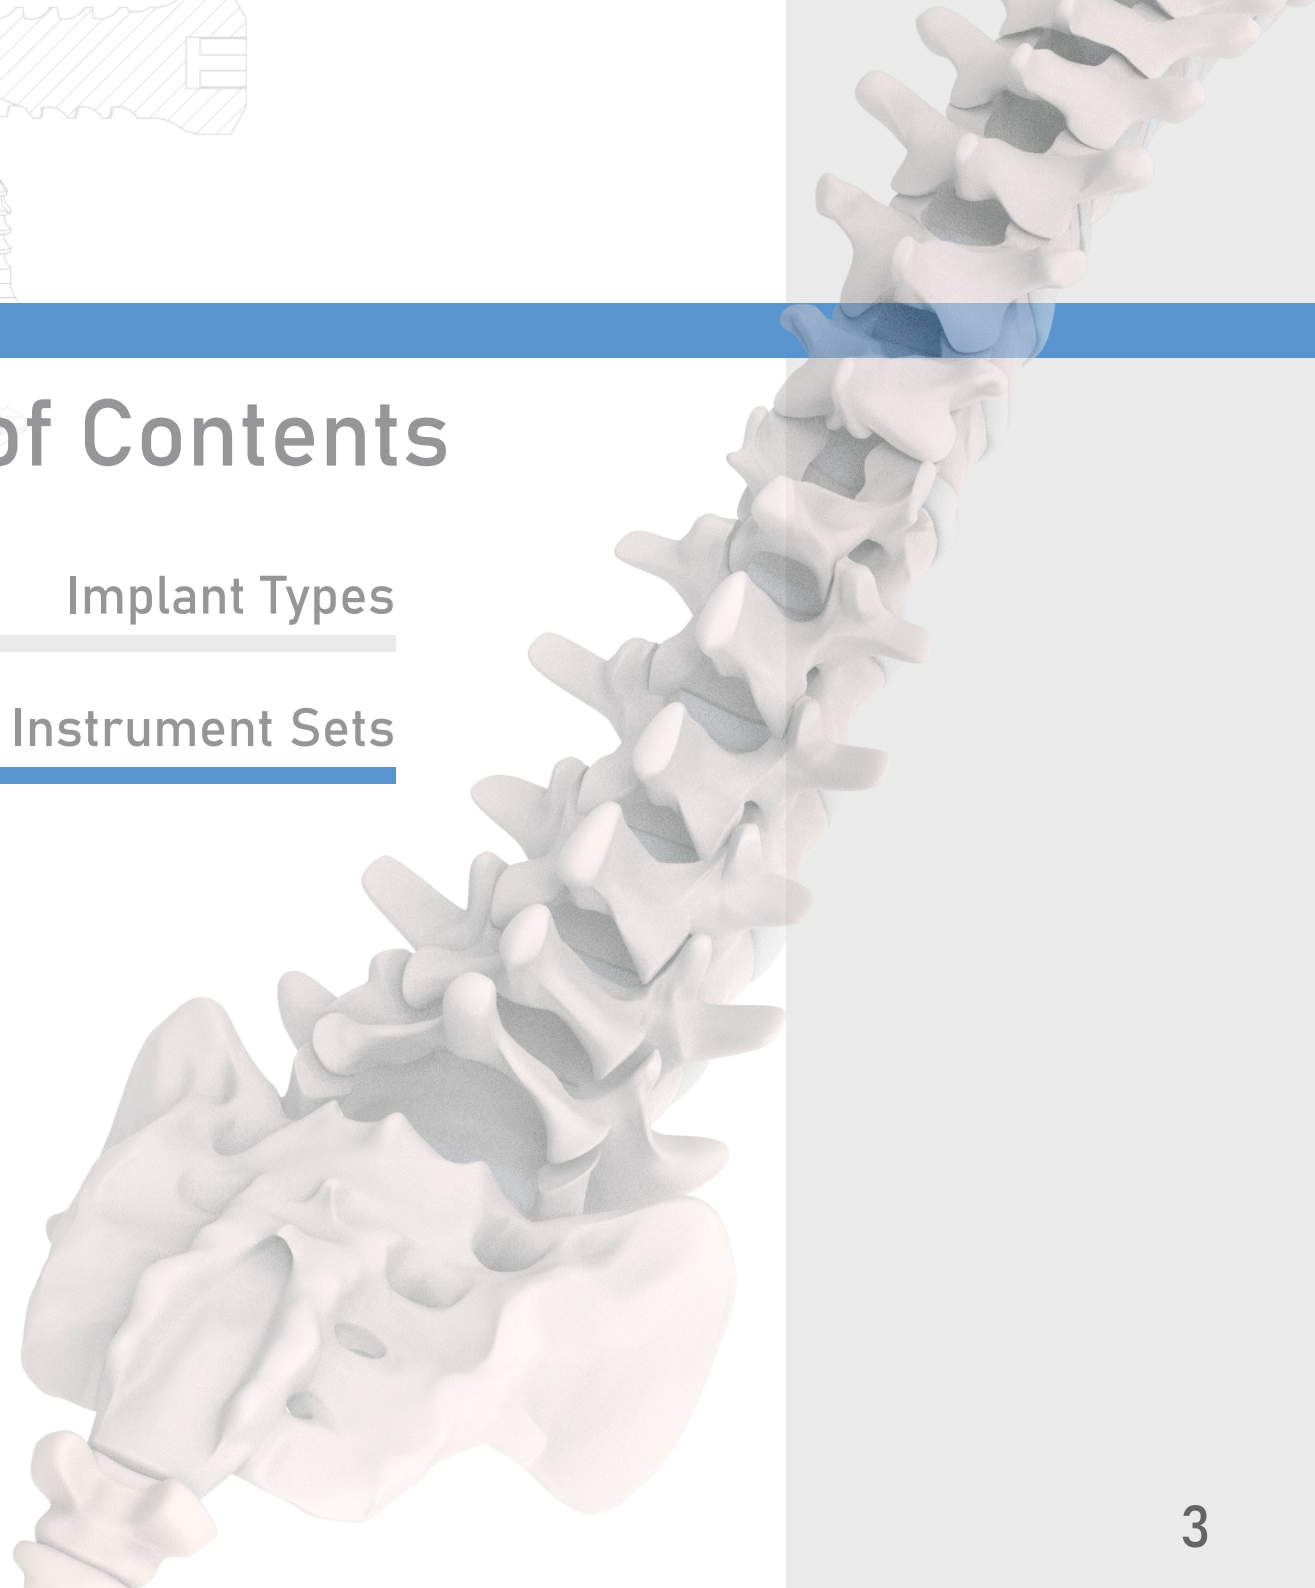

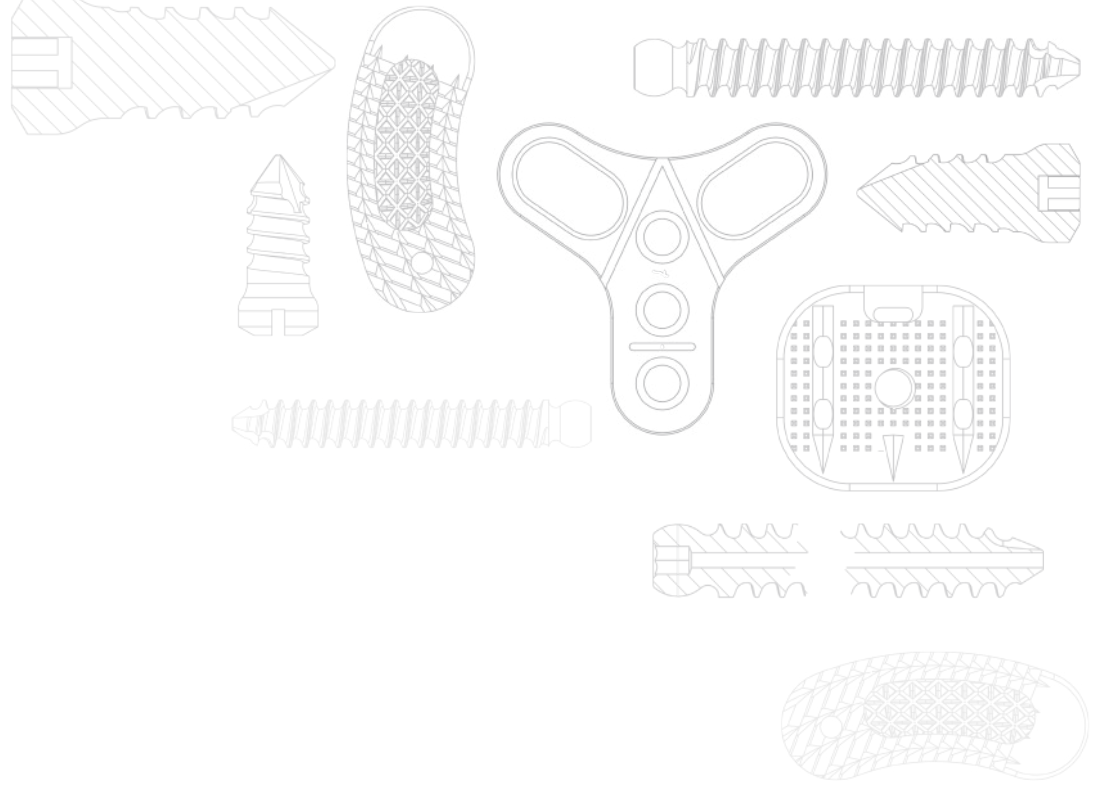

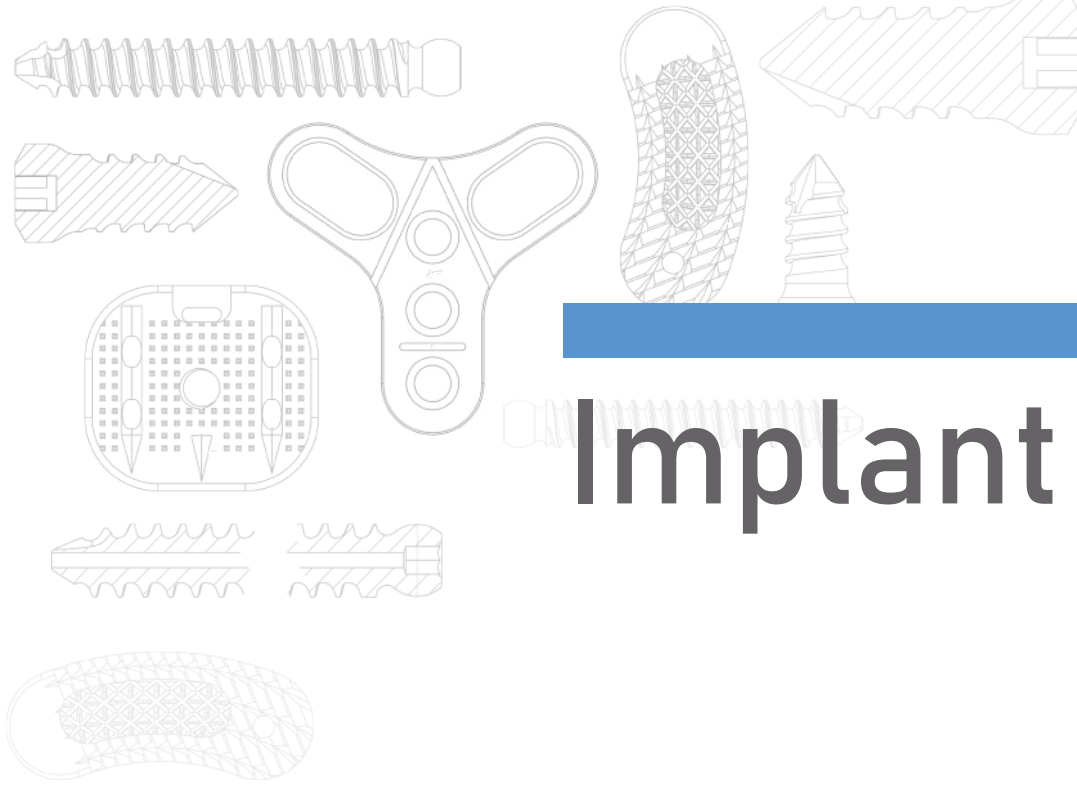

Implant Types






POLAR

Cervical Peek Cage




This implant system used with Polar and Polar-B Cervical Peek Cage Instrument Set
(Set Code: NM-SS-013)

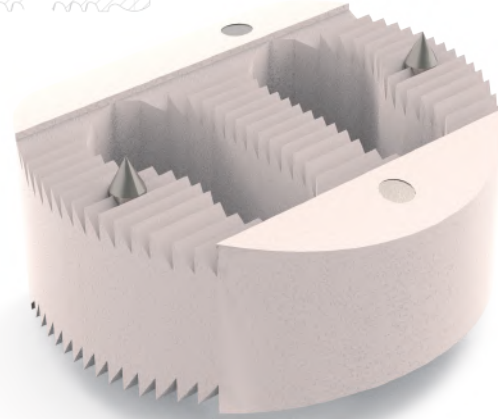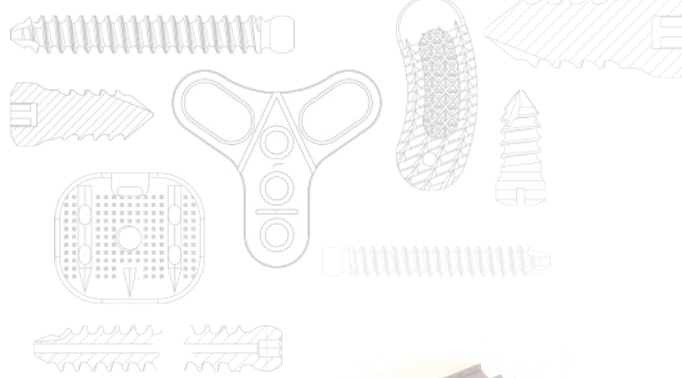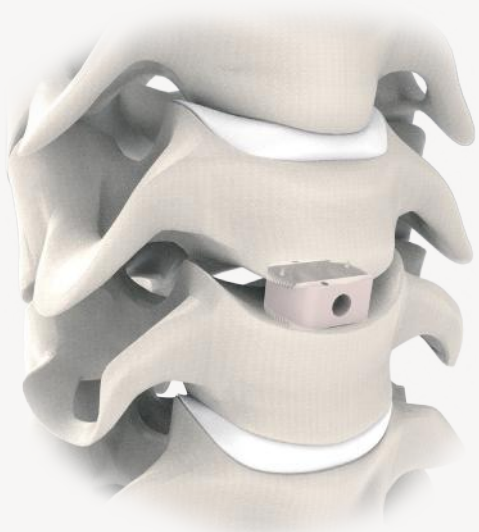

Polar Cervical Peek Cage

Product Code H(mm) L(mm) W(mm) Piece

NMPC041214	4	12	14	
NMPC041216	4	12	16	
NMPC041414	4	14	14	
NMPC041416	4	14	16	
NMPC051214	5	12	14	
NMPC051216	5	12	16	
NMPC051414	5	14	14	
NMPC051416	5	14	16	
NMPC061214	6	12	14	
NMPC061216	6	12	16	
NMPC061414	6	14	14	
NMPC061416	6	14	16	
NMPC071214	7	12	14	
NMPC071216	7	12	16	
NMPC071414	7	14	14	
NMPC071416	7	14	16	
NMPC081214	8	12	14	
NMPC081216	8	12	16	
NMPC081414	8	14	14	
NMPC081416	8	14	16	



H: Height(mm), L: Length(mm), W: Width(mm)

Features;


- Not lesion persistent that produced by peek material compatible with MR
- Best fit with anatomic structure
- Tantalum marker
- Strong fixation by superior and inferior area with threaded surface and two titanium pins

POLAR-B


Cervical Bladed Peek Cage



This implant system used with Polar and Polar-B Cervical Peek Cage Instrument Set
(Set Code: NM-SS-013)

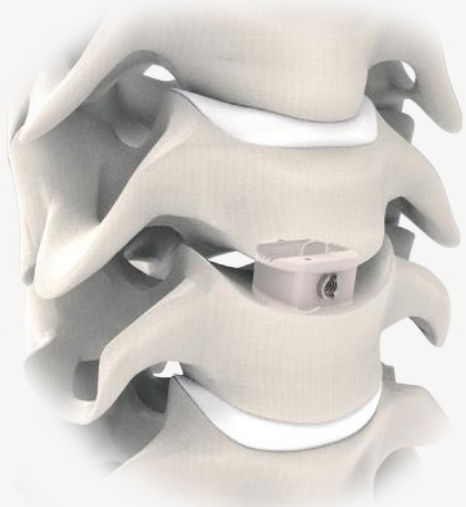


Bladed fixation

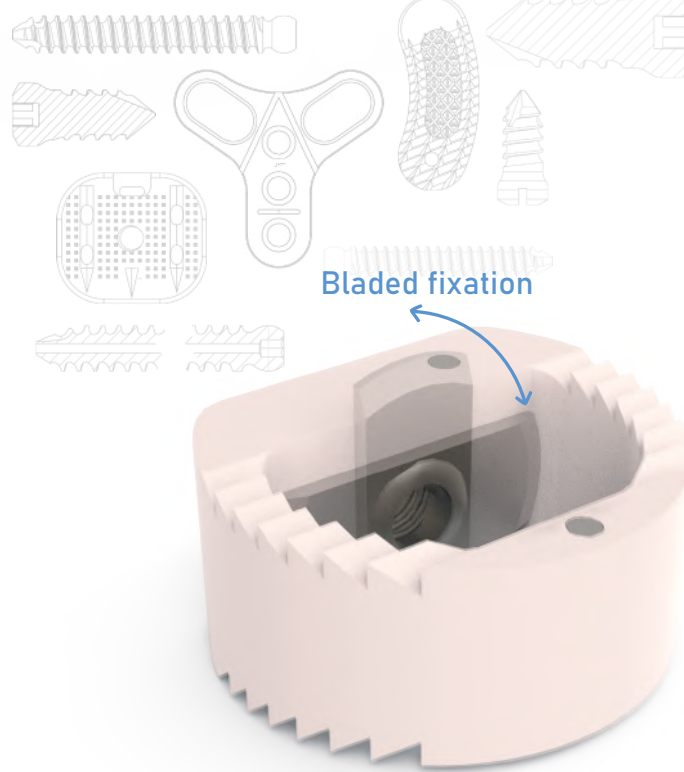

Polar-B Cervical Bladed Peek Cage

Product Code	H(mm)	L(mm)	W(mm)	Piece
NMPCB41214	4	12	14	
NMPCB41216	4	12	16	
NMPCB41414	4	14	14	
NMPCB41416	4	14	16	
NMPCB51214	5	12	14	
NMPCB51216	5	12	16	
NMPCB51414	5	14	14	
NMPCB51416	5	14	16	
NMPCB61214	6	12	14	
NMPCB61216	6	12	16	
NMPCB61414	6	14	14	
NMPCB61416	6	14	16	
NMPCB71214	7	12	14	
NMPCB71216	7	12	16	
NMPCB71414	7	14	14	
NMPCB71416	7	14	16	
NMPCB81214	8	12	14	
NMPCB81216	8	12	16	
NMPCB81414	8	14	14	
NMPCB81416	8	14	16	



NMPCB41214	4	12	14	
NMPCB41216	4	12	16	
NMPCB41414	4	14	14	
NMPCB41416	4	14	16	
NMPCB51214	5	12	14	
NMPCB51216	5	12	16	
NMPCB51414	5	14	14	
NMPCB51416	5	14	16	
NMPCB61214	6	12	14	
NMPCB61216	6	12	16	
NMPCB61414	6	14	14	
NMPCB61416	6	14	16	
NMPCB71214	7	12	14	
NMPCB71216	7	12	16	
NMPCB71414	7	14	14	
NMPCB71416	7	14	16	
NMPCB81214	8	12	14	
NMPCB81216	8	12	16	
NMPCB81414	8	14	14	
NMPCB81416	8	14	16	



H: Height(mm), L: Length(mm), W: Width(mm)

Features;




- Locking blade mechanism
- Tantalum marker
- Threaded surface
- Large graft area

CARSTEN

Carsten Trabecular Stand Alone Cage




This implant system used with Carsten Stand Alone Cage (CLIF) Instrument Set
(Set Code: NM-SS-025)

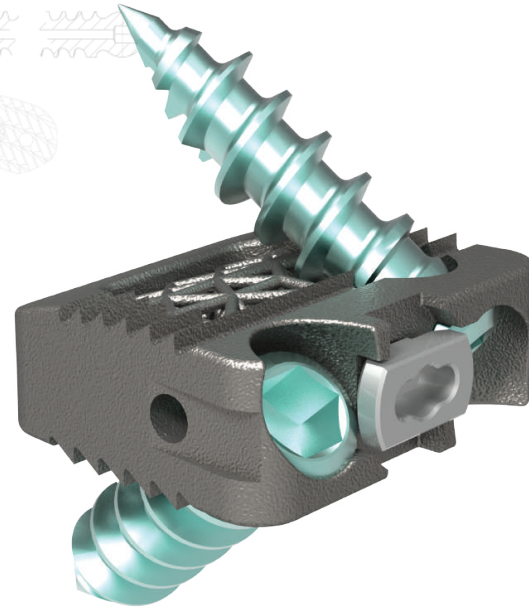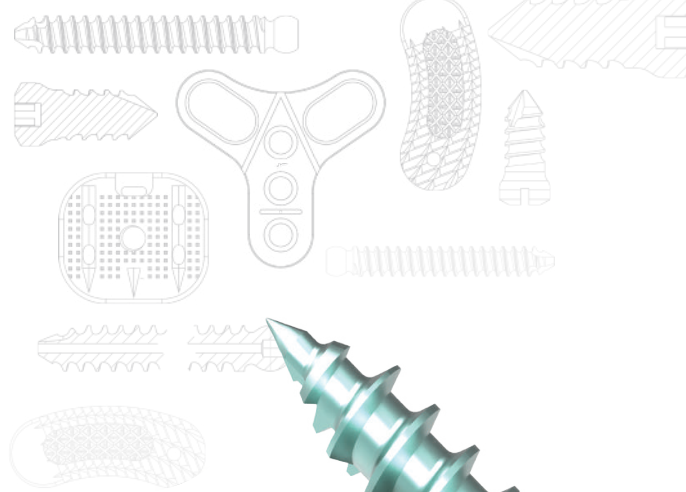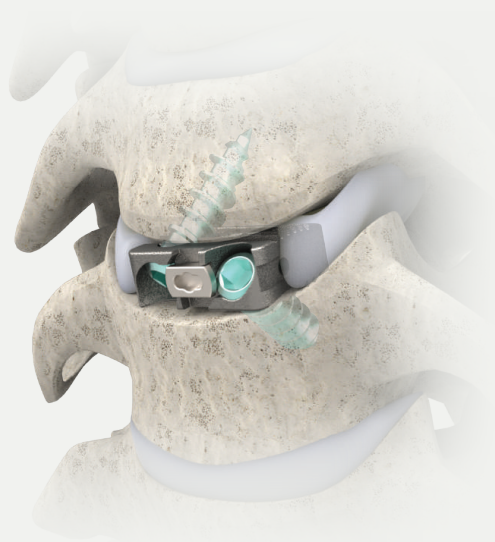

Carsten Stand Alone Cage

Product Code H(mm) L(mm) W(mm)


NM-TTC051214	5	12	14	
NM-TTC061214	6	12	14	
NM-TTC071214	7	12	14	
NM-TTC081214	8	12	14	
NM-TTC051414	5	14	14	
NM-TTC061414	6	14	14	
NM-TTC071414	7	14	14	
NM-TTC081414	8	14	14	
NM-TTC051416	5	14	16	
NM-TTC061416	6	14	16	
NM-TTC071416	7	14	16	
NM-TTC081416	8	14	16	



Carsten Stand Alone Cage Screw

Product Code D(mm) L(mm)

NMCAPS12	3,5	12	
NMCAPS14	3,5	14	
NMCAPS16	3,5	16	
NMCAPS18	3,5	18	
NMCAPS20	3,5	20	
NMCAPSR12	4	12	
NMCAPSR14	4	14	
NMCAPSR16	4	16	
NMCAPSR18	4	18	
NMCAPSR20	4	20	



D: Diameter(mm), H: Height(mm), L: Length(mm), W: Width(mm)

Features;

- 3D printed metal technology
- Best fit with anatomic structure
- Best fusion

TRIMI

Anterior Cervical Plate System



This implant system used with Trimi Anterior Cervical Plate Instrument Set
(Set Code: NM-SS-024)



Cervical Anterior Plate Screw Revision

Product Code	D(mm)	L(mm)	Piece
NMCAPSR12	4.0	12	<input type="checkbox"/>
NMCAPSR14	4.0	14	<input type="checkbox"/>
NMCAPSR16	4.0	16	<input type="checkbox"/>
NMCAPSR18	4.0	18	<input type="checkbox"/>
NMCAPSR20	4.0	20	<input type="checkbox"/>



Cervical Anterior Plate Screw

Product Code	D(mm)	L(mm)	Piece
NMCAPS12	3.5	12	<input type="checkbox"/>
NMCAPS14	3.5	14	<input type="checkbox"/>
NMCAPS16	3.5	16	<input type="checkbox"/>
NMCAPS18	3.5	18	<input type="checkbox"/>
NMCAPS20	3.5	20	<input type="checkbox"/>



Trimi Anterior Cervical Plate System

Product Code Hole L(mm) T(mm) Piece

NMCAP17	4	17	2	<input type="checkbox"/>
NMCAP20	4	20	2	<input type="checkbox"/>
NMCAP22	4	22	2	<input type="checkbox"/>
NMCAP24	4	24	2	<input type="checkbox"/>
NMCAP26	4	26	2	<input type="checkbox"/>
NMCAP28	4	28	2	<input type="checkbox"/>
NMCAP30	4	30	2	<input type="checkbox"/>
NMCAP32	6	32	2	<input type="checkbox"/>
NMCAP34	6	34	2	<input type="checkbox"/>
NMCAP36	6	36	2	<input type="checkbox"/>
NMCAP39	6	39	2	<input type="checkbox"/>
NMCAP42	6	42	2	<input type="checkbox"/>
NMCAP45	6	45	2	<input type="checkbox"/>
NMCAP48	6	48	2	<input type="checkbox"/>
NMCAP51	6	51	2	<input type="checkbox"/>
NMCAP55	6	55	2	<input type="checkbox"/>
NMCAP60	8	60	2	<input type="checkbox"/>
NMCAP65	8	65	2	<input type="checkbox"/>
NMCAP70	8	70	2	<input type="checkbox"/>
NMCAP74	8	74	2	<input type="checkbox"/>
NMCAP80	10	80	2.1	<input type="checkbox"/>



D: Diameter(mm), L: Length(mm), T: Thickness(mm)

Features;


- Provide high strength with low thickness
- Provide effective and simple use
- Low profile (totally 2 mm)
- Flexible blocking system securely to the screw

VERTELIFT-C

Anterior Cervical Corpectomy Cage



This implant system used with Vertelift-C Corpectomy Cage Instrument Set
(Set Code: NM-SS-006)

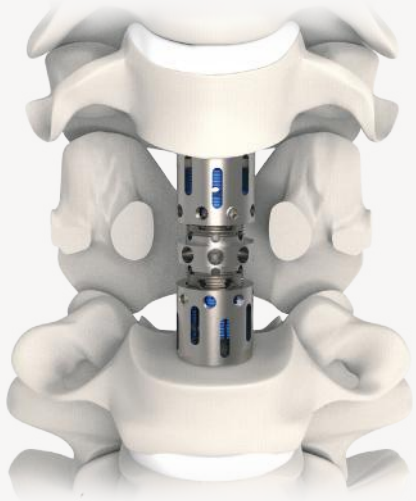

Vertelift-C Corpectomy Cage

Product Code D(mm) CL(mm) OL(mm) Angle Piece

NMCTC101013	10	10	13	-	
NMCTC101317	10	13	17	-	
NMCTC101625	10	16	25	-	
NMCTC121013	12	10	13	-	
NMCTC121317	12	13	17	-	
NMCTC121625	12	16	25	-	
NMCTC1216256	12	16	25	6°	
NMCTC122440	12	24	40	-	
NMCTC1224406	12	24	40	6°	
NMCTC123965	12	39	65	-	
NMCTC1239656	12	39	65	6°	
NMCTC141013	14	10	13	-	
NMCTC141317	14	13	17	-	
NMCTC141625	14	16	25	-	
NMCTC1416256	14	16	25	6°	
NMCTC142440	14	24	40	-	
NMCTC1424406	14	24	40	6°	
NMCTC143965	14	39	65	-	
NMCTC1439656	14	39	65	6°	
NMCTC161013	16	10	13	-	
NMCTC161317	16	13	17	-	
NMCTC161625	16	16	25	-	
NMCTC162440	16	24	40	-	
NMCTC163965	16	39	65	-	
NMCTC201013	20	10	13	-	
NMCTC201317	20	13	17	-	
NMCTC201625	20	16	25	-	



D: Diameter(mm), CL: Closed Length(mm), OL: Opened Length(mm)

Features;

- Allowing a complete contact with vertebral surface
- Provide a secure fixation with the feature of threaded surface
- Efficient grafting space before distraction
- Provide one stage locking mechanism


OXIS PLUS



Occipitocervical Fixation System





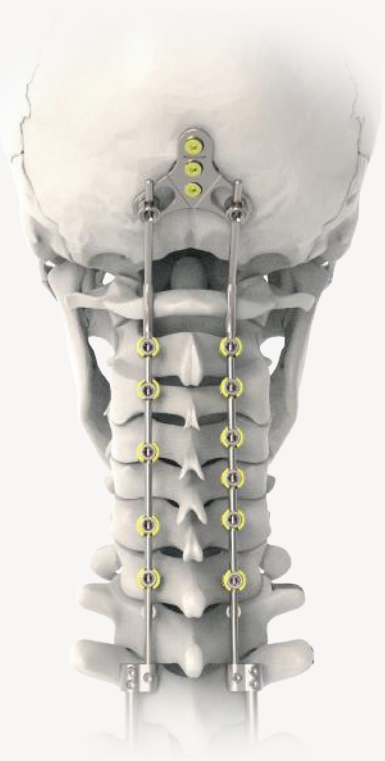



This implant system used with Oxis-PLUS Instrument Set

(Set Code: NM-SS-005)




Oxis Polyaxial Screw		(2 mm increments)	
Product Code	Diameter(mm)	XX/L(mm)	
NMPCSS35XX	3.5	8-32	
NMPCSS40XX	4.0	8-32	

Oxis Occipital Plate Screw		(2 mm increments)	
Product Code	Diameter(mm)	XX/L(mm)	
NMPCTOS35XX	3.5	6-20	
NMPCTOS40XX	4.0	6-20	

Oxis Rod			
Product Code	D(mm)	L(mm)	Piece
NMPCTR12	3.5	120	
NMPCTR14	3.5	140	
NMPCTR18	3.5	180	
NMPCTR24	3.5	240	

Oxis Transverse Link		
Product Code	L(mm)	Piece
NMPCTL40	40	
NMPCTL50	50	
NMPCTL60	60	
NMPCTL70	70	

Oxis Transverse Link Hook	
Product Code	Piece
NMPCTLH	

D: Diameter(mm), L: Length(mm)

Features;

- Provide high strength with low thickness
- Provide effective and simple use
- Flexible blocking system securely lock screw

Oxis Domino Rod Connector

Product Code **Diameter(mm)** **Piece**

NMPCRC3560 3.5 6.0



Oxis Lateral Connectors

Product Code **Length(mm)** **Piece**


NMPCLC10 10
 NMPCLC12 12



Oxis Laminar Hook

Product Code **Width(mm)** **Length(mm)** **Piece**

NMPCLH0405 4 5
 NMPCLH0406 4 6
 NMPCLH0407 4 7



Oxis Hybrid Rod

Product Code **Diameter(mm)** **Length(mm)** **Piece**

NMSHYR 150 3.5 6.0 150
 NMSHYR250 3.5 6.0 250
 NMSHYR350 3.5 6.0 350
 NMSHYR500 3.5 6.0 500



Oxis Occipital Rod/45° Angled

Product Code **Length(mm)** **Piece**

NMPCORA 150



Oxis Occipital Plate

Product Code **Length(mm)** **Piece**

NMPCHFS 45
 NMPCHFM 50
 NMPCHFL 55



Oxis Multiaxial Connector

Optional Implant **Length(mm)** **Piece**

30-35
 35-43
 44-61





This implant system used with
Oxis-PLUS Instrument Set
 (Set Code: NM-SS-005)

OXIS PLUS
 Posterior Cervical Occipitocervical
 Fixation System

D-FLEX Titanium Cervical Silicone Disc Prosthesis




This implant system used with Cervical Disc Prosthesis Instrument Set (Set Code: NM-SS-021)

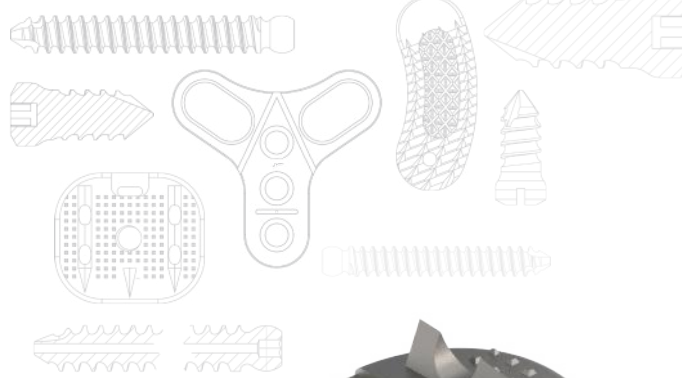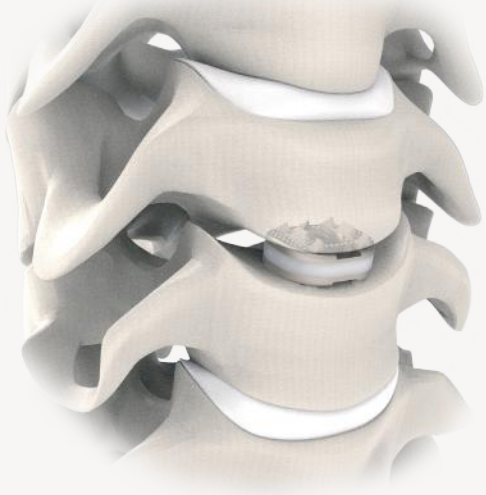

D-Flex Titanium Cervical Silicone Disc Prosthesis
Product Code H(mm) L(mm) W(mm) Piece

NMCDSI12-04	4	12	14	
NMCDSI14-04	4	14	14	
NMCDSI16-04	4	14	16	
NMCDSI12-05	5	12	14	
NMCDSI14-05	5	14	14	
NMCDSI16-05	5	14	16	
NMCDSI12-06	6	12	14	
NMCDSI14-06	6	14	14	
NMCDSI16-06	6	14	16	
NMCDSI12-07	7	12	14	
NMCDSI14-07	7	14	14	
NMCDSI16-07	7	14	16	
NMCDSI12-08	8	12	14	
NMCDSI14-08	8	14	14	
NMCDSI16-08	8	14	16	
NMCDSI18-08	8	16	18	
NMCDSI20-08	8	18	20	
NMCDSI18-09	9	16	18	
NMCDSI20-09	9	18	20	



H: Height(mm), L: Length(mm), W: Width(mm)




Features;

- Comprise titanium endplates with core manufacture from flexible silicone
- Allow lateral bending, axial rotations, flexion and extension, shock absorption
- This product is one part so it is a great advantage for ease of use.
- Anatomical structure and high biomechanical performance

D-MOTION Peek Cervical Disc Prosthesis




This implant system used with Cervical Disc Prosthesis Instrument Set (Set Code: NM-SS-021)

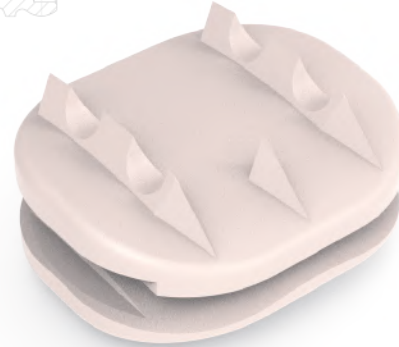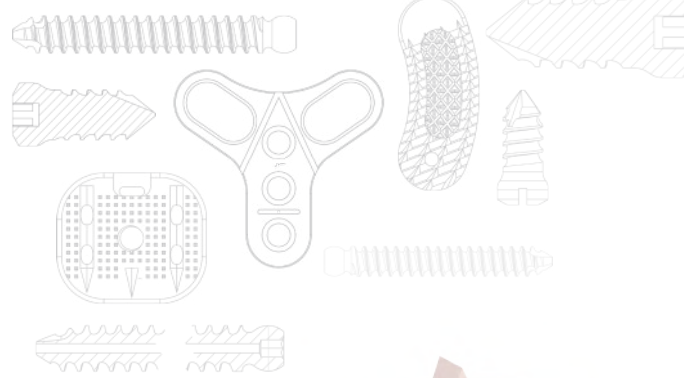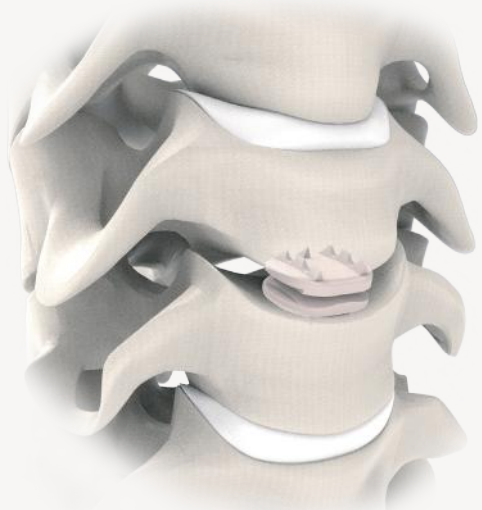

D-Motion Peek Cervical Disc Prosthesis

Product Code H(mm) L(mm) W(mm) Piece

NMCDP1205	5	12	14	
NMCDP1405	5	14	14	
NMCDP1605	5	14	16	
NMCDP1206	6	12	14	
NMCDP1406	6	14	14	
NMCDP1606	6	14	16	
NMCDP1207	7	12	14	
NMCDP1407	7	14	14	
NMCDP1607	7	14	16	
NMCDP1208	8	12	14	
NMCDP1408	8	14	14	
NMCDP1608	8	14	16	



H: Height(mm), L: Length(mm), W: Width(mm)

Features;

- D-Motion is made from a radiolucent polymer (PEEK) for imaging compatibility
- Anatomical structure
- Permits a physiological range of motion in flexion, extension, rotation and lateral bending


SILVER

Posterior Thoracolumbar Fixation System



This implant system used with Plexus & Silver Posterior Spinal Instrument Set

(Set Code: NM-SS-001)

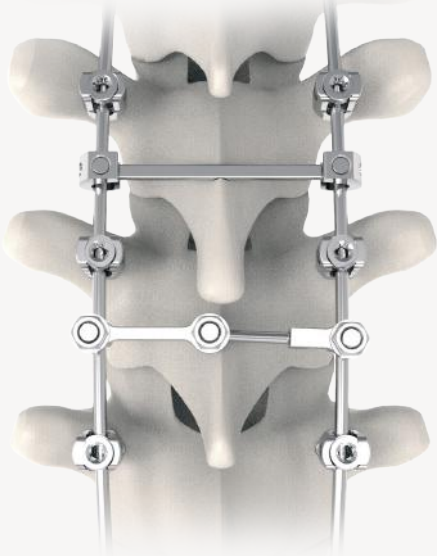

Silver Ion Coated Rapidfix Dual Lead Polyaxial Screw (5 mm increments)

Product Code	Diameter(mm)	XX/L(mm)
AB-NMSPA45XX	4.5	20-45
AB-NMSPA50XX	5.0	25-50
AB-NMSPA55XX	5.5	20-55
AB-NMSPA60XX	6.0	30-55
AB-NMSPA65XX	6.5	25-60
AB-NMSPA70XX	7.0	30-55
AB-NMSPA75XX	7.5	25-100
AB-NMSPA80XX	8.0	25-100



Silver Ion Coated Rapidfix Dual Lead Polyaxial Reduction Screw (5 mm increments)

Product Code	Diameter(mm)	XX/L(mm)
AB-NMSPRS45XX	4.5	25-45
AB-NMSPRS50XX	5.0	25-50
AB-NMSPRS55XX	5.5	20-55
AB-NMSPRS60XX	6.0	30-55
AB-NMSPRS65XX	6.5	25-60
AB-NMSPRS70XX	7.0	30-55
AB-NMSPRS75XX	7.5	25-100
AB-NMSPRS80XX	8.0	25-100



L: Length(mm)

Features;

- The feature of coating with nanoparticulate silver ions
- Reducing the infection rate and risk
- Decrease hospitalization period
- Antibacterial characteristic

Silver Ion Coated Rapidfix Dual Lead Monoaxial Screw (5 mm increments)
Product Code D(mm) XX/L(mm)

AB-NMSMA040XX	4.0	20-45
AB-NMSMA045XX	4.5	20-45
AB-NMSMA050XX	5.0	25-50
AB-NMSMA055XX	5.5	20-55
AB-NMSMA060XX	6.0	30-55
AB-NMSMA065XX	6.5	25-60
AB-NMSMA070XX	7.0	30-55
AB-NMSMA075XX	7.5	25-100
AB-NMSMA080XX	8.0	25-100



Silver Ion Coated Rapidfix Dual Lead Reduction Monoaxial Screw (5 mm increments)
Product Code D(mm) XX/L(mm)

AB-NMSMRS045XX	4.5	20-45
AB-NMSMRS050XX	5.0	25-50
AB-NMSMRS055XX	5.5	20-55
AB-NMSMRS060XX	6.0	30-55
AB-NMSMRS065XX	6.5	25-60
AB-NMSMRS070XX	7.0	30-55
AB-NMSMRS075XX	7.5	25-100
AB-NMSMRS080XX	8.0	25-100



Silver Ion Coated Rapidfix Dual Lead Cannulated Fenestrated Polyaxial Screw (5 mm increments)
Product Code D(mm) XX/L(mm)

AB-NMSPA055XX	5.5	30-55
AB-NMSPA060XX	6.0	30-55
AB-NMSPA065XX	6.5	30-55
AB-NMSPA070XX	7.0	30-55
AB-NMSPA075XX	7.5	30-55
AB-NMSPA080XX	8.0	30-55



Silver Ion Coated Rod
Product Code D(mm) L(mm) Piece

AB-NMSR1604	6.0	40
AB-NMSR1605	6.0	50
AB-NMSR1606	6.0	60
AB-NMSR1607	6.0	70
AB-NMSR1608	6.0	80
AB-NMSR1609	6.0	90
AB-NMSR1610	6.0	100
AB-NMSR1611	6.0	110
AB-NMSR1612	6.0	120
AB-NMSR1613	6.0	130
AB-NMSR1614	6.0	140
AB-NMSR1615	6.0	150
AB-NMSR1616	6.0	160
AB-NMSR1617	6.0	170
AB-NMSR1618	6.0	180
AB-NMSR1619	6.0	190
AB-NMSR1620	6.0	200
AB-NMSR1621	6.0	210
AB-NMSR1622	6.0	220
AB-NMSR1623	6.0	230
AB-NMSR1624	6.0	240
AB-NMSR1625	6.0	250
AB-NMSR1626	6.0	260
AB-NMSR1627	6.0	270
AB-NMSR1628	6.0	280
AB-NMSR1629	6.0	290
AB-NMSR1630	6.0	300
AB-NMSR1640	6.0	400
AB-NMSR1648	6.0	480
AB-NMSR1650	6.0	500
AB-NMSR1660	6.0	600



Silver Dynamic Rod
Product Code D(mm) L(mm) Piece

AB-NMDNR6050	6.0	50
AB-NMDNR6060	6.0	60
AB-NMDNR6070	6.0	70
AB-NMDNR6080	6.0	80
AB-NMDNR6090	6.0	90
AB-NMDNR6010	6.0	100
AB-NMDNR60200	6.0	200



Silver Ion Coated Lateral Extension Connector
Product Code L(mm) Piece

AB-NMSLCNT15	15
AB-NMSLCNT20	20
AB-NMSLCNT25	25
AB-NMSLCNT30	30
AB-NMSLCNT40	40



Silver Ion Coated Lateral-Extension Connector extend
Product Code L(mm) Piece

AB-NMSECNT01	30
AB-NMSECNT02	30



Silver Ion Coated Transverse Link Multiaxial
Product Code L(mm) Piece

AB-NMSATL2040	20-40
AB-NMSATL4060	40-60
AB-NMSATL6080	60-80
AB-NMSATL80100	80-100



D: Diameter(mm), L: Length(mm)

Cannulated and Fenestrated screws are used with a 3.5 hex screwdriver.



This implant system used with Plexus & Silver Posterior Spinal Instrument Set
 (Set Code: NM-SS-001)

SILVER
 Posterior Thoracolumbar
 Fixation System

Silver Ion Coated Laminar Hook

Product Code W(mm)L(mm) Piece

AB-NMPLH0505	5	5	<input type="checkbox"/>
AB-NMPLH0507	5	7	<input type="checkbox"/>
AB-NMPLH0509	5	9	<input type="checkbox"/>
AB-NMPLH0706	7	6	<input type="checkbox"/>
AB-NMPLH0707	7	7	<input type="checkbox"/>
AB-NMPLH0709	7	9	<input type="checkbox"/>
AB-NMPLH0711	7	11	<input type="checkbox"/>



Silver Ion Coated Laminar Angle 20° Left & Right Hook

Product Code W(mm)L(mm) Piece

AB-NMPLHLA709	7	9	<input type="checkbox"/>
AB-NMPLHLA711	7	11	<input type="checkbox"/>
AB-NMPLHRA709	7	9	<input type="checkbox"/>
AB-NMPLHRA711	7	11	<input type="checkbox"/>



Silver Ion Coated Laminar Flexible Hook

Product Code W(mm)L(mm) Piece

AB-NMLHF0505	5	5	<input type="checkbox"/>
AB-NMLHF0507	5	7	<input type="checkbox"/>



Silver Ion Coated Pedicle Flexible Hook

Product Code W(mm)L(mm) Piece

AB-NMPHF0505	5	5	<input type="checkbox"/>
AB-NMPHF0507	5	7	<input type="checkbox"/>



Silver Ion Coated Transverse Link

Product Code L(mm) Piece

AB-NMSTL140	40	<input type="checkbox"/>
AB-NMSTL150	50	<input type="checkbox"/>
AB-NMSTL160	60	<input type="checkbox"/>
AB-NMSTL170	70	<input type="checkbox"/>
AB-NMSTL180	80	<input type="checkbox"/>



Silver Ion Coated Transverse Link Hook

Product Code Piece

AB-NMSTLH	<input type="checkbox"/>
-----------	--------------------------



Silver Ion Coated Pedicular Hook

Product Code W(mm)L(mm) Piece

AB-NMPPH0505	5	5	<input type="checkbox"/>
AB-NMPPH0507	5	7	<input type="checkbox"/>
AB-NMPPH0805	8	5	<input type="checkbox"/>
AB-NMPPH0807	8	7	<input type="checkbox"/>
AB-NMPPH0809	8	9	<input type="checkbox"/>



D: Diameter(mm), L: Length(mm)




This implant system used with Plexus & Silver Posterior Spinal Instrument Set
(Set Code: NM-SS-001)

SILVER
Posterior Thoracolumbar
Fixation System

Posterior Thoracolumbar MIS Screw System



This implant system used with Ares MIS Screw System Instrument Set
(Set Code: NM-SS-004)

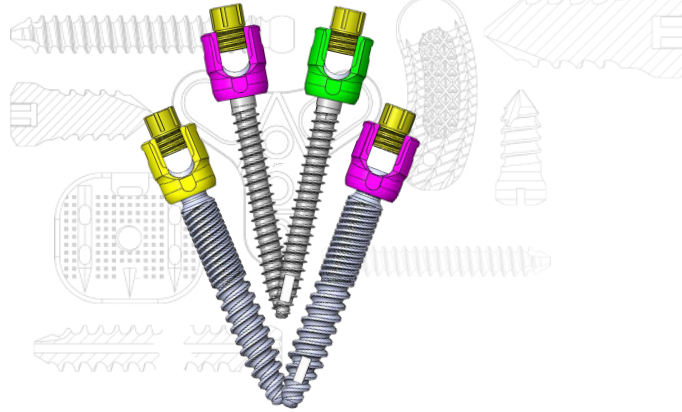

Ares MIS Ø5,5 Straight Rod (10 mm increments)
Product Code Diameter(mm) XXX/L(mm)

NMSR155XS 5.5 045-150




Ares MIS Ø5.5 Curved Rod (10 mm increments)
Product Code Diameter(mm) XXX/L(mm)

NMSR155XC 5.5 040-90




Locking Cap
Product Code

NMLN




Ares MIS Dual Lead Cannulated Polyaxial Screw (5 mm increments)
Product Code Diameter(mm) XX/L(mm)
NMLMIS55XX 5.5 30-50
NMLMIS65XX 6.5 30-55
NMLMIS75XX 7.5 30-50



Ares MIS Cannulated Polyaxial Fenestrated Dual Lead Polyaxial Screw (5 mm increments)
Product Code Diameter(mm) XX/L(mm)
NMLMIS57XX 5.7 30-50
NMLMIS67XX 6.7 30-55
NMLMIS77XX 7.7 30-50



Ares MIS Cannulated Quad Lead Polyaxial Screw (5 mm increments)
Product Code Diameter(mm) XX/L(mm)
NMQCPS55XX 5.5 30-50
NMQCPS65XX 6.5 30-55
NMQCPS75XX 7.5 30-50



Ares MIS Cannulated Fenestrated Quad Lead Polyaxial Screw (5 mm increments)
Product Code Diameter(mm) XX/L(mm)
NMQCPS57XX 5.5 30-50
NMQCPS67XX 6.5 30-55
NMQCPS77XX 7.5 30-50

L: Length(mm)

Features;

- The Ares MIS Spinal System is a thoracolumbar system designed to facilitate percutaneous screw and rod placement.
- The cannulated pedicle screws and extended reduction tabs allow for easy rod placement and minimal tissue disruption


Rapidfix

Dual Lead Thoracolumbar Screws



These screws are used with
Tower Fix Scoliosis
Deformity Instrument Set
and Plexus & Silver
Posterior Spinal Instrument
Set

(Set Code: NM-SS-002, Set Code: NM-SS-001)

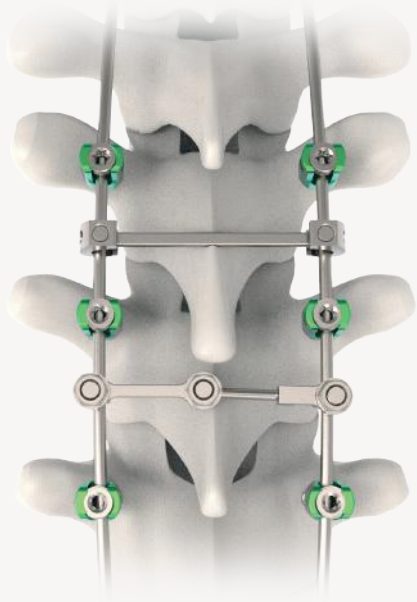

Rapidfix Dual Lead Polyaxial Screw

(5 mm increments)

Product Code	Diameter(mm)	XX/L(mm)
NMSPAK45XX	4.5	20-45
NMSPAK50XX	5.0	25-50
NMSPAK55XX	5.5	20-55
NMSPAK60XX	6.0	30-55
NMSPAK65XX	6.5	25-60
NMSPAK70XX	7.0	30-55
NMSPAK75XX	7.5	25-100
NMSPAK80XX	8.0	25-100



Rapidfix Dual Lead Reduction Polyaxial Screw

(5 mm increments)

Product Code	Diameter(mm)	XX/L(mm)
NMSPAKR45XX	4.5	25-45
NMSPAKR50XX	5.0	25-50
NMSPAKR55XX	5.5	20-55
NMSPAKR60XX	6.0	30-55
NMSPAKR65XX	6.5	25-60
NMSPAKR70XX	7.0	30-55
NMSPAKR75XX	7.5	25-100
NMSPAKR80XX	8.0	25-100



L: Length(mm)

Features;

- Rapidfix Dual Lead screw design displays a superior pullout compared to competitor design fast and controlled Insertion
- Combination of two threads having the same form of a double threaded.
- Excellent tactile feedback on bone purchase of screw thanks to combination of double lead

Rapidfix Dual Lead Cannulated Fenestrated Polyaxial Screw (5 mm increments)
Product Code D(mm) XX/L(mm)

NMSPAKH55XX	5.5	30-55
NMSPAKH60XX	6.0	30-55
NMSPAKH65XX	6.5	30-55
NMSPAKH70XX	7.0	30-55
NMSPAKH75XX	7.5	30-55
NMSPAKH80XX	8.0	30-55



Rapidfix Dual Lead Monoaxial Screw (5 mm increments)
Product Code D(mm) XX/L(mm)

NMSMAK40XX	4.0	20-45
NMSMAK45XX	4.5	20-45
NMSMAK50XX	5.0	25-50
NMSMAK55XX	5.5	20-55
NMSMAK60XX	6.0	30-55
NMSMAK65XX	6.5	25-60
NMSMAK70XX	7.0	30-55
NMSMAK75XX	7.5	25-100
NMSMAK80XX	8.0	25-100



Rapidfix Dual Lead Reduction Monoaxial Screw (5 mm increments)
Product Code D(mm) XX/L(mm)

NMSMAKR45XX	4.5	20-45
NMSMAKR50XX	5.0	25-50
NMSMAKR55XX	5.5	20-55
NMSMAKR60XX	6.0	30-55
NMSMAKR65XX	6.5	25-60
NMSMAKR70XX	7.0	30-55
NMSMAKR75XX	7.5	25-100
NMSMAKR80XX	8.0	25-100



Plexus Rod
Product Code D(mm) L(mm) Piece

NMSR1604	6.0	40	<input type="checkbox"/>
NMSR1605	6.0	50	<input type="checkbox"/>
NMSR1606	6.0	60	<input type="checkbox"/>
NMSR1607	6.0	70	<input type="checkbox"/>
NMSR1608	6.0	80	<input type="checkbox"/>
NMSR1609	6.0	90	<input type="checkbox"/>
NMSR1610	6.0	100	<input type="checkbox"/>
NMSR1611	6.0	110	<input type="checkbox"/>
NMSR1612	6.0	120	<input type="checkbox"/>
NMSR1613	6.0	130	<input type="checkbox"/>
NMSR1614	6.0	140	<input type="checkbox"/>
NMSR1615	6.0	150	<input type="checkbox"/>
NMSR1616	6.0	160	<input type="checkbox"/>
NMSR1617	6.0	170	<input type="checkbox"/>
NMSR1618	6.0	180	<input type="checkbox"/>
NMSR1619	6.0	190	<input type="checkbox"/>
NMSR1620	6.0	200	<input type="checkbox"/>
NMSR1621	6.0	210	<input type="checkbox"/>
NMSR1622	6.0	220	<input type="checkbox"/>



Rod
Product Code D(mm) L(mm) Piece

NMSR1623	6.0	230	<input type="checkbox"/>
NMSR1624	6.0	240	<input type="checkbox"/>
NMSR1625	6.0	250	<input type="checkbox"/>
NMSR1626	6.0	260	<input type="checkbox"/>
NMSR1627	6.0	270	<input type="checkbox"/>
NMSR1628	6.0	280	<input type="checkbox"/>
NMSR1629	6.0	290	<input type="checkbox"/>
NMSR1630	6.0	300	<input type="checkbox"/>
NMSR1631	6.0	310	<input type="checkbox"/>
NMSR1632	6.0	320	<input type="checkbox"/>
NMSR1640	6.0	400	<input type="checkbox"/>
NMSR1648	6.0	480	<input type="checkbox"/>
NMSR1650	6.0	500	<input type="checkbox"/>
NMSR1660	6.0	600	<input type="checkbox"/>



Cr-Co Rod
Product Code D(mm) L(mm) Piece

NMSCRR1604	6.0	40	<input type="checkbox"/>
NMSCRR1605	6.0	50	<input type="checkbox"/>

Dual Lead Polyaxial Reduction Fenestrated Screw
Product Code D(mm) L(mm) Piece

NMOPA45XX	4.5	25-45	<input type="checkbox"/>
NMOPA50XX	5.0	25-50	<input type="checkbox"/>
NMOPA55XX	5.5	20-55	<input type="checkbox"/>
NMOPA60XX	6.0	30-55	<input type="checkbox"/>
NMOPA65XX	6.5	25-60	<input type="checkbox"/>
NMOPA70XX	7.0	30-55	<input type="checkbox"/>
NMOPA75XX	7.5	25-100	<input type="checkbox"/>
NMOPA80XX	8.0	25-100	<input type="checkbox"/>



Dual Lead Monoaxial Reduction Fenestrated Screw
Product Code D(mm) L(mm) Piece

NMOMAS45XX	4.5	20-45	<input type="checkbox"/>
NMOMAS50XX	5.0	25-50	<input type="checkbox"/>
NMOMAS55XX	5.5	20-55	<input type="checkbox"/>
NMOMAS60XX	6.0	30-55	<input type="checkbox"/>
NMOMAS65XX	6.5	25-60	<input type="checkbox"/>
NMOMAS70XX	7.0	30-55	<input type="checkbox"/>
NMOMAS75XX	7.5	25-100	<input type="checkbox"/>
NMOMAS80XX	8.0	25-100	<input type="checkbox"/>



D: Diameter(mm), L: Length(mm)

Cannulated and Fenestrated screws are used with a 3.5 hex screwdriver.



This implant system used with **Tower Fix Scoliosis Deformity Instrument Set** and **Plexus & Silver Posterior Spinal Instrument Set**
 (Set Code: NM-SS-002, Set Code: NM-SS-001)

Rapidfix
 Dual Lead Thracolumbar
 Screws

Cr-Co Rod

Product Code D(mm) L(mm) Piece

NMSCRR1606	6.0	60	<input type="checkbox"/>
NMSCRR1607	6.0	70	<input type="checkbox"/>
NMSCRR1608	6.0	80	<input type="checkbox"/>
NMSCRR1609	6.0	90	<input type="checkbox"/>
NMSCRR1610	6.0	100	<input type="checkbox"/>
NMSCRR1611	6.0	110	<input type="checkbox"/>
NMSCRR1612	6.0	120	<input type="checkbox"/>
NMSCRR1613	6.0	130	<input type="checkbox"/>
NMSCRR1614	6.0	140	<input type="checkbox"/>
NMSCRR1615	6.0	150	<input type="checkbox"/>
NMSCRR1616	6.0	160	<input type="checkbox"/>
NMSCRR1617	6.0	170	<input type="checkbox"/>
NMSCRR1618	6.0	180	<input type="checkbox"/>
NMSCRR1619	6.0	190	<input type="checkbox"/>
NMSCRR1620	6.0	200	<input type="checkbox"/>
NMSCRR1621	6.0	210	<input type="checkbox"/>
NMSCRR1622	6.0	220	<input type="checkbox"/>
NMSCRR1623	6.0	230	<input type="checkbox"/>
NMSCRR1624	6.0	240	<input type="checkbox"/>
NMSCRR1625	6.0	250	<input type="checkbox"/>
NMSCRR1626	6.0	260	<input type="checkbox"/>
NMSCRR1627	6.0	270	<input type="checkbox"/>
NMSCRR1628	6.0	280	<input type="checkbox"/>
NMSCRR1629	6.0	290	<input type="checkbox"/>
NMSCRR1630	6.0	300	<input type="checkbox"/>
NMSCRR1631	6.0	310	<input type="checkbox"/>
NMSCRR1632	6.0	320	<input type="checkbox"/>
NMSCRR1640	6.0	400	<input type="checkbox"/>
NMSCRR1648	6.0	480	<input type="checkbox"/>
NMSCRR1650	6.0	500	<input type="checkbox"/>
NMSCRR1660	6.0	600	<input type="checkbox"/>



Laminar Hook

Product Code W(mm)L(mm) Piece

NMPLH0505	5	5	<input type="checkbox"/>
NMPLH0507	5	7	<input type="checkbox"/>
NMPLH0509	5	9	<input type="checkbox"/>
NMPLH0706	7	6	<input type="checkbox"/>
NMPLH0707	7	7	<input type="checkbox"/>
NMPLH0709	7	9	<input type="checkbox"/>
NMPLH0711	7	11	<input type="checkbox"/>



Pedicular Hook

Product Code W(mm)L(mm) Piece

NMPPH0505	5	5	<input type="checkbox"/>
NMPPH0507	5	7	<input type="checkbox"/>
NMPPH0805	8	5	<input type="checkbox"/>
NMPPH0807	8	7	<input type="checkbox"/>
NMPPH0809	8	9	<input type="checkbox"/>



Laminar Flexible Hook

Product Code W(mm)L(mm) Piece

NMLHF0505	5	5	<input type="checkbox"/>
NMLHF0507	5	7	<input type="checkbox"/>



Pedicle Flexible Hook

Product Code W(mm)L(mm) Piece

NMPHF0505	5	5	<input type="checkbox"/>
NMPHF0507	5	7	<input type="checkbox"/>



Laminar Angle 20° Left & Right Hook

Product Code W(mm)L(mm) Piece

NMPLHLA709	7	9	<input type="checkbox"/>
NMPLHLA711	7	11	<input type="checkbox"/>
NMPLHRA709	7	9	<input type="checkbox"/>
NMPLHRA711	7	11	<input type="checkbox"/>



Domino Rod Connector

Product Code D(mm) Piece

NMNSECNT01	5.5	<input type="checkbox"/>
NMNSECNT02	6.0	<input type="checkbox"/>



Dynamic Rod

Product Code D(mm) L(mm) Piece

NMDNR6050	6.0	50	<input type="checkbox"/>
NMDNR6060	6.0	60	<input type="checkbox"/>
NMDNR6070	6.0	70	<input type="checkbox"/>
NMDNR6080	6.0	80	<input type="checkbox"/>
NMDNR6090	6.0	90	<input type="checkbox"/>
NMDNR6010	6.0	100	<input type="checkbox"/>



Lateral Extension Connector

Product Code L(mm) Piece


NMSLCNT15	15	<input type="checkbox"/>
NMSLCNT20	20	<input type="checkbox"/>
NMSLCNT25	25	<input type="checkbox"/>
NMSLCNT30	30	<input type="checkbox"/>
NMSLCNT40	40	<input type="checkbox"/>



Transverse Link Multiaxial

Product Code L(mm) Piece

NMSATL2040	20-40	<input type="checkbox"/>
NMSATL4060	40-60	<input type="checkbox"/>
NMSATL6080	60-80	<input type="checkbox"/>
NMSATL80100	80-100	<input type="checkbox"/>

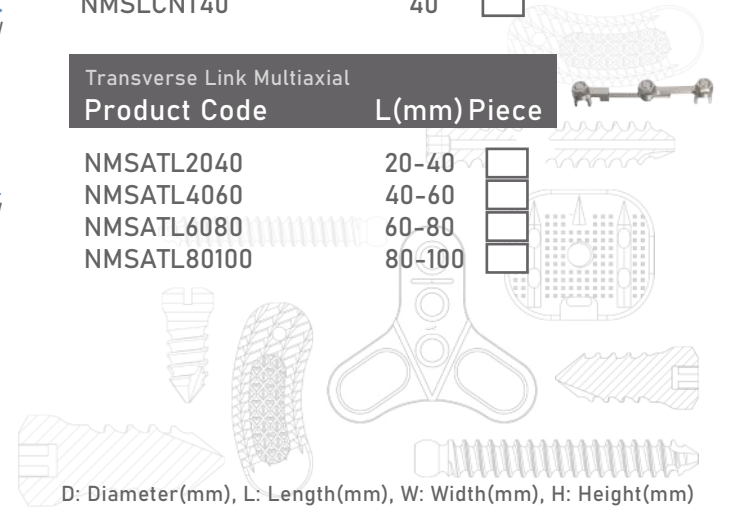

D: Diameter(mm), L: Length(mm), W: Width(mm), H: Height(mm)



This implant system used with **Tower Fix Scoliosis Deformity Instrument Set** and **Plexus & Silver Posterior Spinal Instrument Set**
 (Set Code: NM-SS-002, Set Code: NM-SS-001)

Rapidfix
 Dual Lead Thracolumbar
 Screws

Transverse Link

Product Code	L(mm)	Piece
NMSTL140	40	<input type="checkbox"/>
NMSTL150	50	<input type="checkbox"/>
NMSTL160	60	<input type="checkbox"/>
NMSTL170	70	<input type="checkbox"/>
NMSTL180	80	<input type="checkbox"/>



Transverse Link Hook

Product Code	Piece
NMSTLH	<input type="checkbox"/>



Sacral Connector

Product Code	L(mm)	Piece
NMSSC15	15	<input type="checkbox"/>
NMSSC20	20	<input type="checkbox"/>



Plexus Sacroiliac Polyaxial Screw

Product Code	D(mm)	XX/L(mm)
NMSICS80XX	8.0	70-120



L: Length(mm)



This implant system used with **Tower Fix Scoliosis Deformity Instrument Set** and **Plexus & Silver Posterior Spinal Instrument Set**
 (Set Code: NM-SS-002, Set Code: NM-SS-001)

Rapidfix
 Dual Lead Thracolumbar
 Screws


Quatro

Quad Lead Thoracolumbar Screws



These screws are used with Tower Fix Scoliosis Deformity Instrument Set and Plexus & Silver Posterior Spinal Instrument Set

(Set Code: NM-SS-002, Set Code: NM-SS-001)

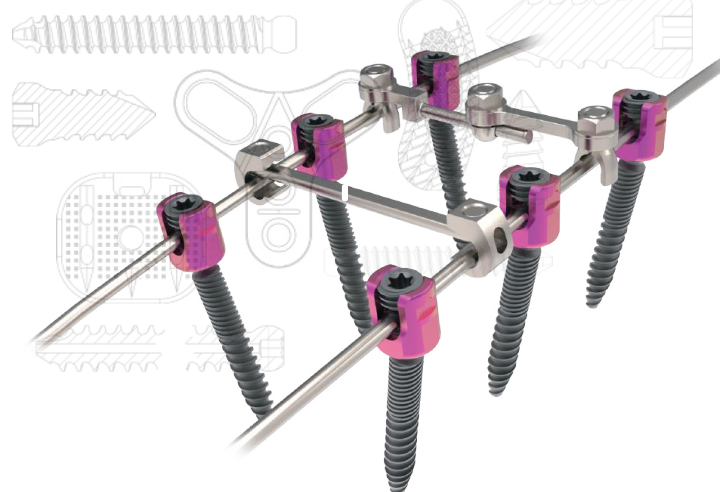

Quatro Quad Lead Polyaxial Reduction Fenestrated Screw (5 mm increments)		
Product Code	Diameter(mm)	XX/L(mm)
NMOPALS40XX	4.0	20-45
NMOPALS45XX	4.5	20-50
NMOPALS50XX	5.0	25-55
NMOPALS55XX	5.5	20-55
NMOPALS60XX	6.0	30-55
NMOPALS65XX	6.5	30-60
NMOPALS70XX	7.0	30-55
NMOPALS75XX	7.5	25-100



Quatro Quad Lead Polyaxial Screw (5 mm increments)		
Product Code	Diameter(mm)	XX/L(mm)
NMQSPA45XX	4.5	20-45
NMQSPA50XX	5.0	25-50
NMQSPA55XX	5.5	20-55
NMQSPA60XX	6.0	30-55
NMQSPA65XX	6.5	25-60
NMQSPA70XX	7.0	30-55
NMQSPA75XX	7.5	25-100



Quatro Quad Lead Cannulated Fenestrated Polyaxial Screw (5 mm increments)		
Product Code	Diameter(mm)	XX/L(mm)
NMQSPAH55XX	5.5	30-55
NMQSPAH60XX	6.0	30-55
NMQSPAH65XX	6.5	30-55
NMQSPAH70XX	7.0	30-55
NMQSPAH75XX	7.5	30-55



Quatro Quad Lead Polyaxial Reduction Screw (5 mm increments)		
Product Code	Diameter(mm)	XX/L(mm)
NMQSPAR40XX	4.0	20-45
NMQSPAR45XX	4.5	20-55
NMQSPAR50XX	5.0	25-55
NMQSPAR55XX	5.5	20-55
NMQSPAR60XX	6.0	30-55
NMQSPAR65XX	6.5	30-60
NMQSPAR70XX	7.0	30-55
NMQSPAR75XX	7.5	25-100



L: Length(mm)

Cannulated and Fenestrated screws are used with a 3.5 hex screwdriver.

Features;

- Distal tip teeth to enable insertion without pedicle prop
- Constant thread lead
- Cortical thread form support enhanced pedicle fixation
- Best pullout performance


PEDIFIX

Posterior Thoracolumbar Fixation System



This implant system used with Pedifix Instrument Set

(Set Code: NM-SS-020)

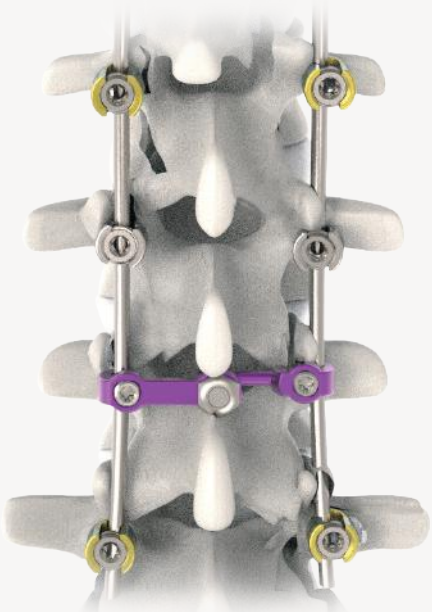

Pedifix Polyaxial Screw (5 mm increments)

Product Code	Diameter(mm)	XX/L(mm)
NMPXPS40XX	4.0	20-40
NMPXPS45XX	4.5	25-50
NMPXPS50XX	5.0	25-50
NMPXPS55XX	5.5	25-50
NMPXPS60XX	6.0	30-50



Pedifix Polyaxial Reduction Screw (5 mm increments)

Product Code	Diameter(mm)	XX/L(mm)
NMPXPRS45XX	4.5	20-50
NMPXPRS55XX	5.5	25-50
NMPXPRS60XX	6.0	30-50



Pedifix Monoaxial Screw (5 mm increments)

Product Code	Diameter(mm)	XX/L(mm)
NMPXMS40XX	4.0	20-40
NMPXMS45XX	4.5	25-45
NMPXMS50XX	5.0	25-50
NMPXMS55XX	5.5	25-50
NMPXMS60XX	6.0	30-50



L: Length(mm)

Features;

- Low profile tulip head (12.3mm) allows you to more directly visualize the surgical site
- Thread pattern optimized for cortical bone at the proximal end and cancellous bone at the distal end
- Designed to treat a wide range of deformities including adolescent idiopathic scoliosis (AIS) congenital scoliosis, neuromuscular scoliosis

Pedifix Monoblock Cross Connectors		
Product Code	L(mm)	Piece
NMPXMC12	12	<input type="checkbox"/>
NMPXMC13	13	<input type="checkbox"/>
NMPXMC14	14	<input type="checkbox"/>
NMPXMC15	15	<input type="checkbox"/>
NMPXMC16	16	<input type="checkbox"/>
NMPXMC17	17	<input type="checkbox"/>
NMPXMC18	18	<input type="checkbox"/>
NMPXMC19	19	<input type="checkbox"/>
NMPXMC20	20	<input type="checkbox"/>
NMPXMC21	21	<input type="checkbox"/>
NMPXMC22	22	<input type="checkbox"/>
NMPXMC23	23	<input type="checkbox"/>
NMPXMC24	24	<input type="checkbox"/>



Pedifix Dual Staple Caudal		
Product Code	Size	Piece
NMPXDSC(L)	Large	<input type="checkbox"/>
NMPXDSC(S)	Small	<input type="checkbox"/>



Pedifix Dual Staple Rostral		
Product Code	Size	Piece
NMPXDSR(L)		<input type="checkbox"/>
NMPXDSR(S)		<input type="checkbox"/>



Pedifix Pedicle Hook		
Product Code	Size	Piece
NMPXPH(L)	Large	<input type="checkbox"/>
NMPXPH(S)	Small	<input type="checkbox"/>



Pedifix Transverse Proses Hook		
Product Code	Side	Piece
NMPXTHL	Left	<input type="checkbox"/>
NMPXTHR	Right	<input type="checkbox"/>



Pedifix Thoracic Hook Offset		
Product Code	Side	Piece
NMPXTHOL	Left	<input type="checkbox"/>
NMPXTHOR	Right	<input type="checkbox"/>



Pedifix Supralaminar Thoracic Hook		
Product Code	Side	Piece
NMPXSH(L)	Left	<input type="checkbox"/>
NMPXSH(R)	Right	<input type="checkbox"/>



Pedifix Rod			
Product Code	L(mm)	Diameter (mm)	Piece
NMPXR030	30	4.5	<input type="checkbox"/>
NMPXR040	40	4.5	<input type="checkbox"/>
NMPXR050	50	4.5	<input type="checkbox"/>
NMPXR060	60	4.5	<input type="checkbox"/>
NMPXR070	70	4.5	<input type="checkbox"/>
NMPXR080	80	4.5	<input type="checkbox"/>
NMPXR090	90	4.5	<input type="checkbox"/>
NMPXR100	100	4.5	<input type="checkbox"/>
NMPXR200	200	4.5	<input type="checkbox"/>
NMPXR480	480	4.5	<input type="checkbox"/>



Pedifix Laminar Hook		
Product Code	Size	Piece
NMPXLH(L)	Large	<input type="checkbox"/>
NMPXLH(M)	Medium	<input type="checkbox"/>
NMPXLH(S)	Small	<input type="checkbox"/>



Pedifix Laminar Hook Angled Blade		
Product Code	Size	Piece
NMPXLHA		<input type="checkbox"/>



Pedifix Thoracic Laminar Hook Ramped	
Product Code	Piece
NMPXLHR	<input type="checkbox"/>



Pedifix Extended Body Laminar Hook	
Product Code	Piece
NMPXLHE	<input type="checkbox"/>



Pedifix Rod to Rod Connector		
Product Code	D(mm)	Piece
NMPXPDC4535	4.5-3.5	<input type="checkbox"/>
NMPXPDC4545	4.5-4.5	<input type="checkbox"/>
NMPXPDC4560	4.5-6.0	<input type="checkbox"/>




Pedifix Rod to Rod Connector			
Product Code	D(mm)	Size	Piece
NMPXPDCS4545	4.5-4.5	Small	<input type="checkbox"/>
NMPXPDCS4560	4.5-6.0	Small	<input type="checkbox"/>
NMPXPDCL4545	4.5-4.5	Large	<input type="checkbox"/>
NMPXPDCL4560	4.5-6.0	Large	<input type="checkbox"/>



Pedifix Single Staple	
Product Code	Piece
NMPXSS	<input type="checkbox"/>



D: Diameter(mm), L: Length(mm), W: Width(mm), H: Height(mm)

 This implant system used with
Pedifix Instrument Set
 (Set Code: NM-SS-020)

PEDIFIX
 Posterior Thoracolumbar
 Fixation System

Pedifix Offset Connector

Product Code **L(mm)** **Piece**

NMPXOC30	30	<input type="checkbox"/>
NMPXOC70	70	<input type="checkbox"/>



Pedifix Extended Connector

Product Code **L(mm)** **Side** **Piece**

NMPXEC(S)	30	Small	<input type="checkbox"/>
NMPXEC(L)	60	Large	<input type="checkbox"/>



Pedifix Parallel Connector

Product Code **Angle** **Piece**

NMPXIC00		<input type="checkbox"/>
----------	--	--------------------------



Pedifix Iliac Connector

Product Code **Angle** **Piece**

NMPXIC15	15°	<input type="checkbox"/>
NMPXIC25	25°	<input type="checkbox"/>
NMPXIC35	35°	<input type="checkbox"/>
NMPXIC45	45°	<input type="checkbox"/>



Pedifix Polyaxial Cross Connector

Product Code **L(mm)** **Side** **Piece**

NMPXPC2430	24-30	Small	<input type="checkbox"/>
NMPXPC3036	30-36	Medium	<input type="checkbox"/>
NMPXPC3645	36-45	Large	<input type="checkbox"/>
NMPXPC4560	45-60	X-Large	<input type="checkbox"/>



L: Length(mm)



This implant system used with
Pedifix Instrument Set
 (Set Code: NM-SS-020)


PEDIFIX
 Posterior Thoracolumbar
 Fixation System

ZEK

Anterior Thoracolumbar Corpectomy Cage



This implant system used with Vertelift - T Instrument Set
(Set Code: NM-SS-007)

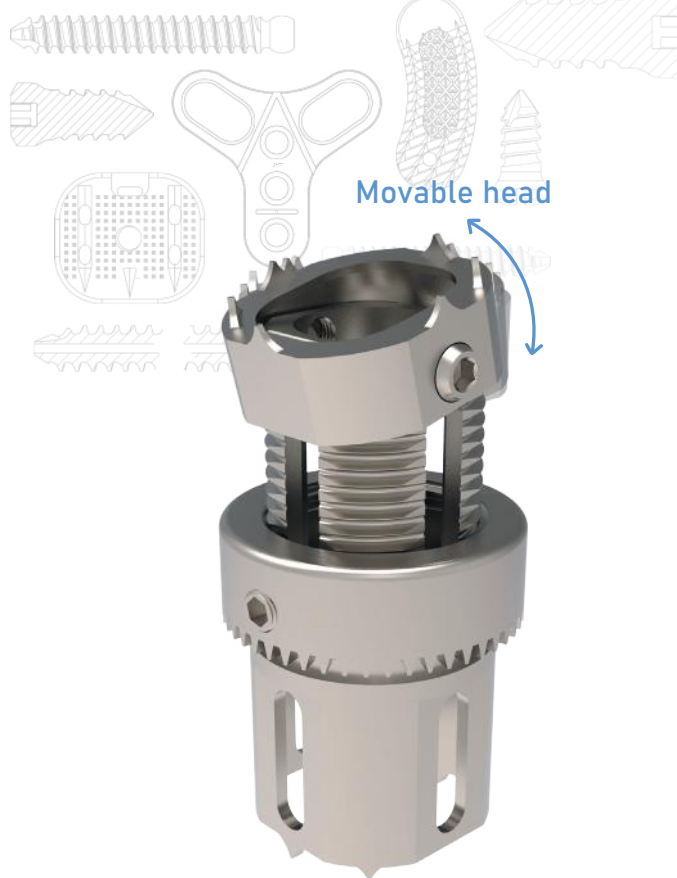

Zek Corpectomy Cage				
Product Code	D(mm)	CL(mm)	OL(mm)	Piece
NMVTCZ203244	20	32	44	
NMVTCZ204258	20	42	58	
NMVTCZ205684	20	56	84	
NMVTCZ242840	24	28	40	
NMVTCZ243854	24	38	54	
NMVTCZ245276	24	52	76	
NMVTCZ2474114	24	74	114	
NMVTCZ283244	28	32	44	
NMVTCZ284258	28	42	58	
NMVTCZ285684	28	56	84	



D: Diameter(mm), CL: Closed Length(mm), OL: Opened Length(mm)

Features;


- Full contact, full fusion through unique movable head technology
- Fit with the anatomy of patient
- Adjustable easily with threaded mechanism
- Adjustable easily with threaded surface

VERTELIFT-T

Anterior Thoracolumbar Corpectomy Cage



This implant system used with Vertelift - T Instrument Set
(Set Code: NM-SS-007)

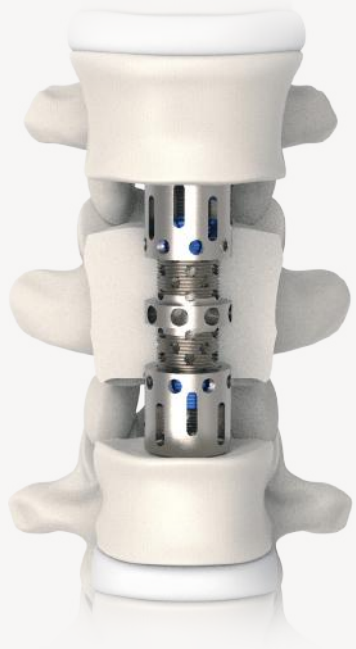

Vertelift-T Corpectomy Cage - Angled

Product Code D(mm) CL(mm) OL(mm) Angle Piece

NMVTCD202534	20	25	34	-	
NMVTCD203244	20	32	44	-	
NMVTCD204258	20	42	58	-	
NMVTCD205684	20	56	84	-	
NMVTCA202534	20	25	34	6°	
NMVTCA203244	20	32	44	6°	
NMVTCA204258	20	42	58	6°	
NMVTCA205684	20	56	84	6°	
NMVTCD242329	24	23	29	-	
NMVTCD242840	24	28	40	-	
NMVTCD243854	24	38	54	-	
NMVTCD245276	24	52	76	-	
NMVTCD2474114	24	74	114	-	
NMVTCA242329	24	23	29	6°	
NMVTCA242840	24	28	40	6°	
NMVTCA243854	24	38	54	6°	
NMVTCA245276	24	52	76	6°	
NMVTCA2474114	24	74	114	6°	
NMVTCD283244	28	32	44	-	
NMVTCD284258	28	42	58	-	
NMVTCD285684	28	56	84	-	
NMVTCD2882130	28	82	130	-	
NMVTCD28100140	28	100	140	-	
NMVTCA283244	28	32	44	6°	
NMVTCA284258	28	42	58	6°	
NMVTCA285684	28	56	84	6°	
NMVTCA2882130	28	82	130	6°	
NMVTCA28100140	28	100	140	6°	



D: Diameter(mm), CL: Closed Length(mm), OL: Opened Length(mm)

Features;

- Dual distractable thoracolumbar system
- Angled inferior and superior area allow a complete contact with vertebral surface
- Composed by one piece
- Provide a secure fixation with the feature of threaded surface



U-DEVICE

Interspinous Stabilisation Device




This implant system used with U-Device Instrument Set

(Set Code: NM-SS-018)

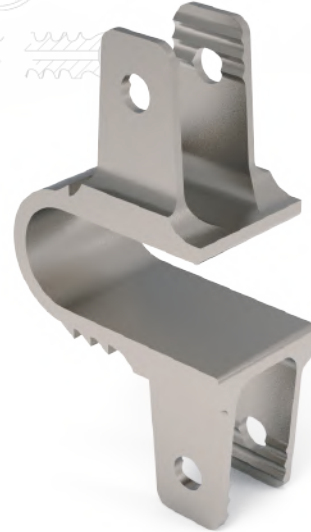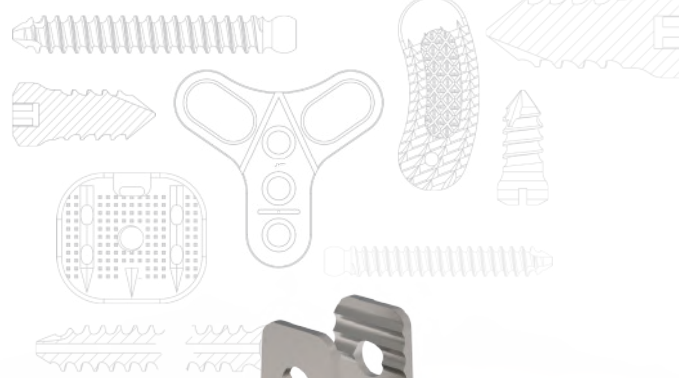

U-Device Interspinous System Stabilisation Device

Product Code	Width(mm)	Piece
NMSUD-SI-08	8	
NMSUD-SI-10	10	
NMSUD-SI-12	12	
NMSUD-SI-14	14	
NMSUD-SI-16	16	



Features;



- Dynamic fixation and stabilisation.
- Reduces stresses at the facet joints
- Prevent unfolding ligamentum flavum

Twisty TLIF Peek Cage



This implant system used with **Twisty TLIF Instrument Set**

(Set Code: NM-SS-016)

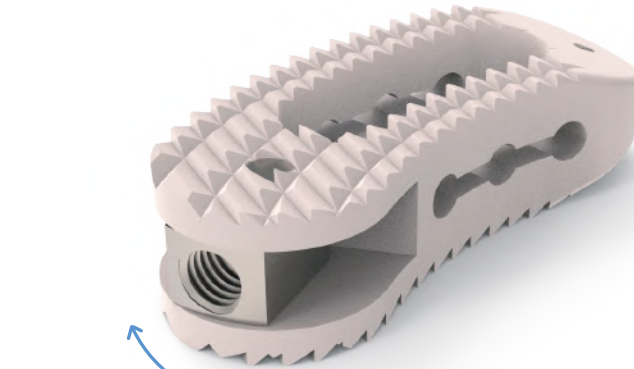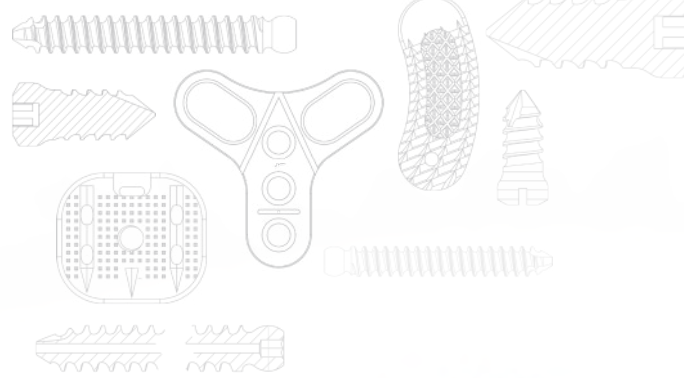


Movable titanium head

Twisty TLIF Peek Cage

Product Code H(mm) L(mm) W(mm) Piece

NMBC2407	7	24	10	
NMBC2807	7	28	10	
NMBC3207	7	32	10	
NMBC2408	8	24	10	
NMBC2808	8	28	10	
NMBC3208	8	32	10	
NMBC2409	9	24	10	
NMBC2809	9	28	10	
NMBC3209	9	32	10	
NMBC2410	10	24	10	
NMBC2810	10	28	10	
NMBC3210	10	32	10	
NMBC2411	11	24	10	
NMBC2811	11	28	10	
NMBC3211	11	32	10	
NMBC2412	12	24	10	
NMBC2812	12	28	10	
NMBC3212	12	32	10	
NMBC2413	13	24	10	
NMBC2813	13	28	10	
NMBC3213	13	32	10	



H: Height(mm), L: Length(mm), W: Width(mm)

Features;

- The cage and the holder are initially lined up to facilitate entry
- The wedge like profile makes the cage insertion process a straight forward and easy task
- The biocompatibility and mechanical properties are perfectly suited for interbody applications
- The cage is moved to its final location with minimal effort with movable titanium part
- Allow for a higher volume of bone grafting material resulting in good fusion

Twisty TLIF Peek Cage Angled

Product Code H(mm) L(mm) W(mm) Angle Piece

NMBCA24074	7	24	10	4°	<input type="checkbox"/>
NMBCA28074	7	28	10	4°	<input type="checkbox"/>
NMBCA32074	7	32	10	4°	<input type="checkbox"/>
NMBCA24084	8	24	10	4°	<input type="checkbox"/>
NMBCA24088	8	24	10	8°	<input type="checkbox"/>
NMBCA28084	8	28	10	4°	<input type="checkbox"/>
NMBCA28088	8	28	10	8°	<input type="checkbox"/>
NMBCA32084	8	32	10	4°	<input type="checkbox"/>
NMBCA32088	8	32	10	8°	<input type="checkbox"/>
NMBCA24094	9	24	10	4°	<input type="checkbox"/>
NMBCA24098	9	24	10	8°	<input type="checkbox"/>
NMBCA28094	9	28	10	4°	<input type="checkbox"/>
NMBCA28098	9	28	10	8°	<input type="checkbox"/>
NMBCA32094	9	32	10	4°	<input type="checkbox"/>
NMBCA32098	9	32	10	8°	<input type="checkbox"/>
NMBCA24104	10	24	10	4°	<input type="checkbox"/>
NMBCA24108	10	24	10	8°	<input type="checkbox"/>
NMBCA28104	10	28	10	4°	<input type="checkbox"/>
NMBCA28108	10	28	10	8°	<input type="checkbox"/>
NMBCA32104	10	32	10	4°	<input type="checkbox"/>
NMBCA32108	10	32	10	8°	<input type="checkbox"/>
NMBCA24114	11	24	10	4°	<input type="checkbox"/>
NMBCA24118	11	24	10	8°	<input type="checkbox"/>
NMBCA28114	11	28	10	4°	<input type="checkbox"/>
NMBCA28118	11	28	10	8°	<input type="checkbox"/>
NMBCA32114	11	32	10	4°	<input type="checkbox"/>
NMBCA32118	11	32	10	8°	<input type="checkbox"/>
NMBCA24124	12	24	10	4°	<input type="checkbox"/>
NMBCA24128	12	24	10	8°	<input type="checkbox"/>
NMBCA28124	12	28	10	4°	<input type="checkbox"/>
NMBCA28128	12	28	10	8°	<input type="checkbox"/>
NMBCA32124	12	32	10	4°	<input type="checkbox"/>
NMBCA32128	12	32	10	8°	<input type="checkbox"/>

A°/2



A°/2

Twisty TLIF Peek Cage Angled

Product Code H(mm) L(mm) W(mm) Angle Piece

NMBCA24134	13	24	10	4°	<input type="checkbox"/>
NMBCA24138	13	24	10	8°	<input type="checkbox"/>
NMBCA28134	13	28	10	4°	<input type="checkbox"/>
NMBCA28138	13	28	10	8°	<input type="checkbox"/>
NMBCA32134	13	32	10	4°	<input type="checkbox"/>
NMBCA32138	13	32	10	8°	<input type="checkbox"/>

A°/2



A°/2



L: Length(mm), W: Width(mm), H: Height(mm)






This implant system used with
Twisty TLIF Instrument Set
(Set Code: NM-SS-016)

Twisty
TLIF Peek Cage

Alligator PLIF Peek Cage




This implant system used with Alligator and Alligator-Exp PLIF Instrument Set
(Set Code: NM-SS-015)

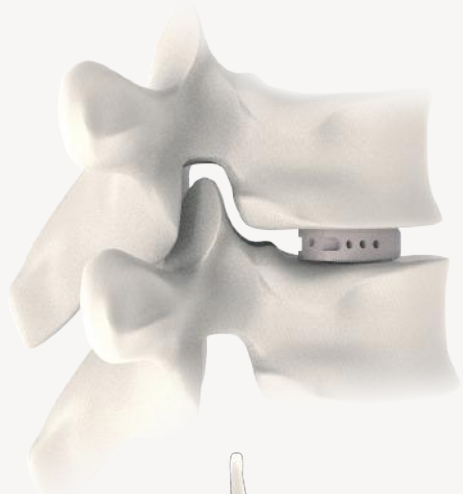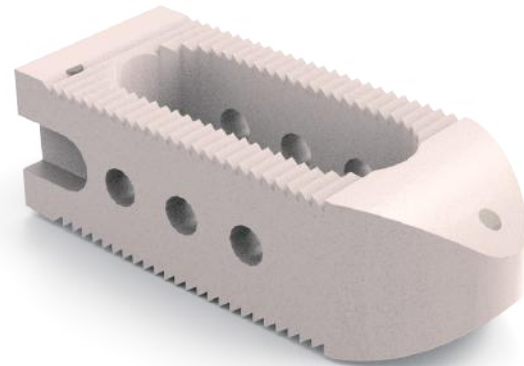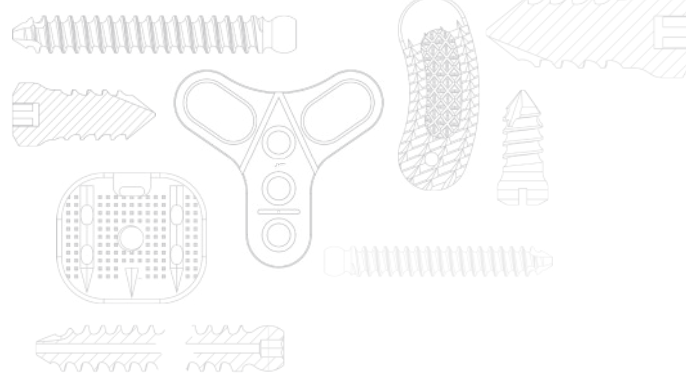

Alligator PLIF Peek Cage
Product Code H(mm) L(mm) W(mm) Piece

NMVPCD2206	6	22	10	
NMVPCD2406	6	24	10	
NMVPCD2207	7	22	10	
NMVPCD2407	7	24	10	
NMVPCD2208	8	22	10	
NMVPCD2408	8	24	10	
NMVPCD2209	9	22	10	
NMVPCD2409	9	24	10	
NMVPCD2210	10	22	10	
NMVPCD2410	10	24	10	
NMVPCD2211	11	22	10	
NMVPCD2411	11	24	10	
NMVPCD2212	12	22	10	
NMVPCD2412	12	24	10	



H: Height(mm), L: Length(mm), W: Width(mm)



Features;

- Tantalum marker
- Bulleted anterior profile facilitates cage insertion into the intervertebral space
- Open design of the upper and lower surfaces allows optimum graft surface to improve bone fusion

Alligator-exp PLIF Expandable Peek Cage




This implant system used with Alligator and Alligator-Exp PLIF Instrument Set
(Set Code: NM-SS-015)

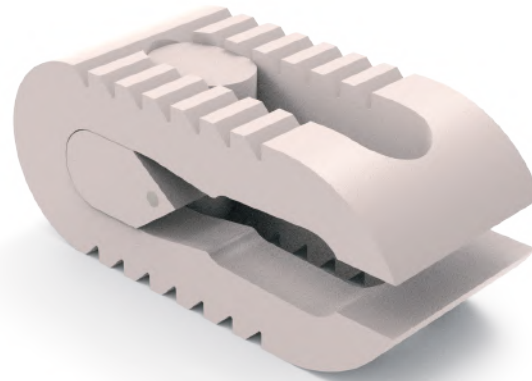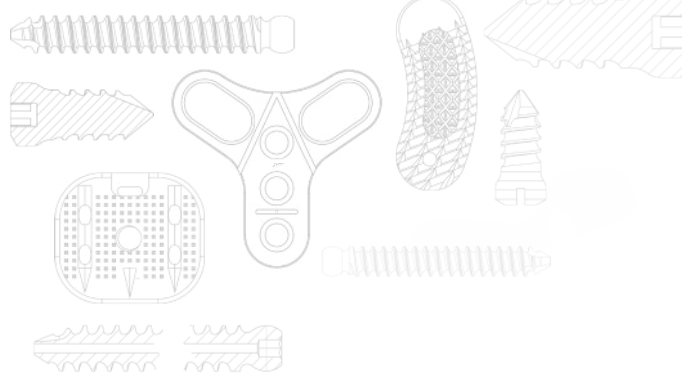

Alligator-Exp PLIF Expandable Peek Cage

Product Code H(mm) L(mm) W(mm) Piece

NMEPC1007	7	24	10	
NMEPC1008	8	24	10	
NMEPC1009	9	24	10	
NMEPC1010	10	24	10	
NMEPC1011	11	24	10	
NMEPC1012	12	24	10	



H: Height(mm), L: Length(mm), W: Width(mm)

Features;



- Don't allow any lesional problems
- Threaded surface feature facilities a strong fixation by superior and inferior area
- Height can be increased by 1 mm at least

Tra-Ti Trabecular TLIF Cage




This implant system used with **Twisty TLIF Instrument Set**

(Set Code: NM-SS-016)

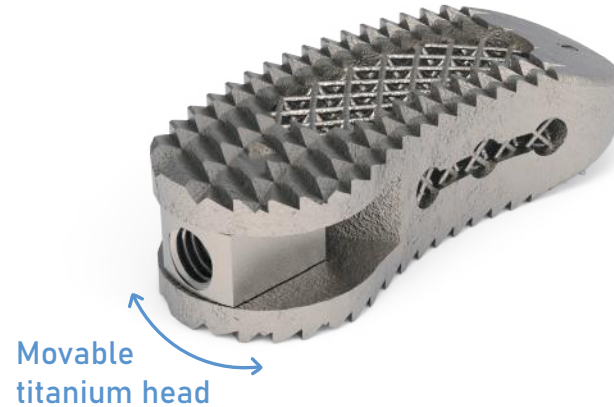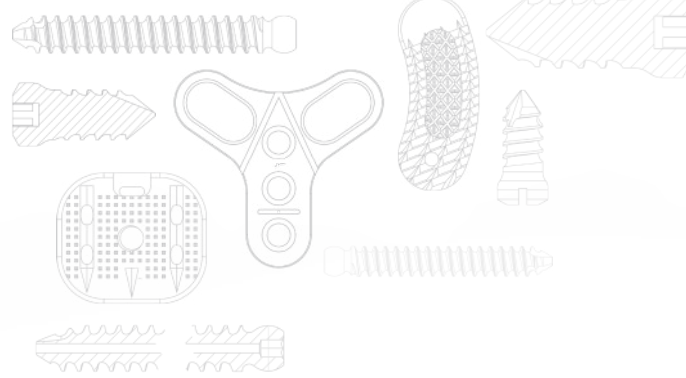

Tra-Ti Trabecular TLIF Cage
Product Code H(mm) L(mm) W(mm) Piece

NM-TTT2407	7	24	10	
NM-TTT2807	7	28	10	
NM-TTT3207	7	32	10	
NM-TTT2408	8	24	10	
NM-TTT2808	8	28	10	
NM-TTT3208	8	32	10	
NM-TTT2409	9	24	10	
NM-TTT2809	9	28	10	
NM-TTT3209	9	32	10	
NM-TTT2410	10	24	10	
NM-TTT2810	10	28	10	
NM-TTT3210	10	32	10	
NM-TTT2411	11	24	10	
NM-TTT2811	11	28	10	
NM-TTT3211	11	32	10	
NM-TTT2412	12	24	10	
NM-TTT2812	12	28	10	
NM-TTT3212	12	32	10	
NM-TTT2413	13	24	10	
NM-TTT2813	13	28	10	
NM-TTT3213	13	32	10	



H: Height(mm), L: Length(mm), W: Width(mm)

Features;

- Smooth wedge nose to facilitate insertion
- Solid-tipped, precisely angled serrations on the superior and inferior surfaces designed for bidirectional fixation and to maximize surface area for endplate contact with the implant

Tra-Ti Trabecular TLIF Cage Angled

Product Code H(mm) L(mm) W(mm) Angle Piece

NM-TTTA24074	7	24	10	4°	<input type="checkbox"/>
NM-TTTA28074	7	28	10	4°	<input type="checkbox"/>
NM-TTTA32074	7	32	10	4°	<input type="checkbox"/>
NM-TTTA24084	8	24	10	4°	<input type="checkbox"/>
NM-TTTA24088	8	24	10	8°	<input type="checkbox"/>
NM-TTTA28084	8	28	10	4°	<input type="checkbox"/>
NM-TTTA28088	8	28	10	8°	<input type="checkbox"/>
NM-TTTA32084	8	32	10	4°	<input type="checkbox"/>
NM-TTTA32088	8	32	10	8°	<input type="checkbox"/>
NM-TTTA24094	9	24	10	4°	<input type="checkbox"/>
NM-TTTA24098	9	24	10	8°	<input type="checkbox"/>
NM-TTTA28094	9	28	10	4°	<input type="checkbox"/>
NM-TTTA28098	9	28	10	8°	<input type="checkbox"/>
NM-TTTA32094	9	32	10	4°	<input type="checkbox"/>
NM-TTTA32098	9	32	10	8°	<input type="checkbox"/>
NM-TTTA24104	10	24	10	4°	<input type="checkbox"/>
NM-TTTA24108	10	24	10	8°	<input type="checkbox"/>
NM-TTTA28104	10	28	10	4°	<input type="checkbox"/>
NM-TTTA28108	10	28	10	8°	<input type="checkbox"/>
NM-TTTA32104	10	32	10	4°	<input type="checkbox"/>
NM-TTTA32108	10	32	10	8°	<input type="checkbox"/>
NM-TTTA24114	11	24	10	4°	<input type="checkbox"/>
NM-TTTA24118	11	24	10	8°	<input type="checkbox"/>
NM-TTTA28114	11	28	10	4°	<input type="checkbox"/>
NM-TTTA28118	11	28	10	8°	<input type="checkbox"/>
NM-TTTA32114	11	32	10	4°	<input type="checkbox"/>
NM-TTTA32118	11	32	10	8°	<input type="checkbox"/>
NM-TTTA24124	12	24	10	4°	<input type="checkbox"/>
NM-TTTA24128	12	24	10	8°	<input type="checkbox"/>
NM-TTTA28124	12	28	10	4°	<input type="checkbox"/>
NM-TTTA28128	12	28	10	8°	<input type="checkbox"/>
NM-TTTA32124	12	32	10	4°	<input type="checkbox"/>
NM-TTTA32128	12	32	10	8°	<input type="checkbox"/>

A°/2



A°/2

Tra-Ti Trabecular TLIF Cage Angled


Product Code H(mm) L(mm) W(mm) Angle Piece

NM-TTTA24134	13	24	10	4°	<input type="checkbox"/>
NM-TTTA24138	13	24	10	8°	<input type="checkbox"/>
NM-TTTA28134	13	28	10	4°	<input type="checkbox"/>
NM-TTTA28138	13	28	10	8°	<input type="checkbox"/>
NM-TTTA32134	13	32	10	4°	<input type="checkbox"/>
NM-TTTA32138	13	32	10	8°	<input type="checkbox"/>

A°/2



A°/2

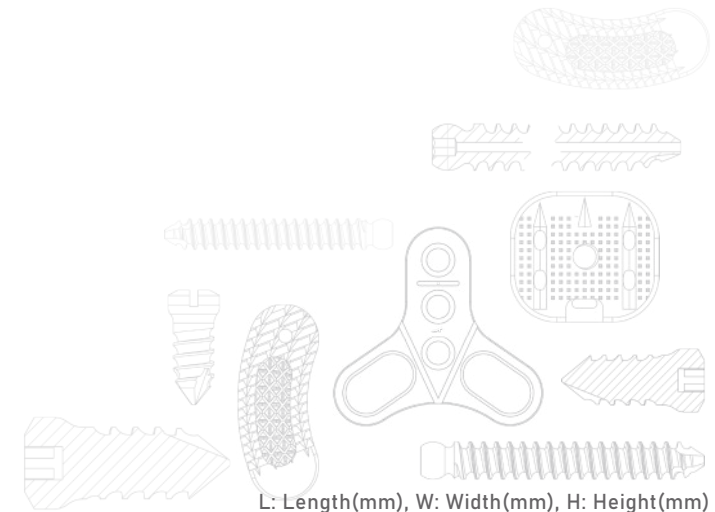


This implant system used with
Twisty TLIF Instrument Set
 (Set Code: NM-SS-016)

Twisty
 TLIF Peek Cage

Tra-Ti Trabecular PLIF Cage




This implant system used with Alligator and Alligator-Exp PLIF Instrument Set
(Set Code: NM-SS-015)

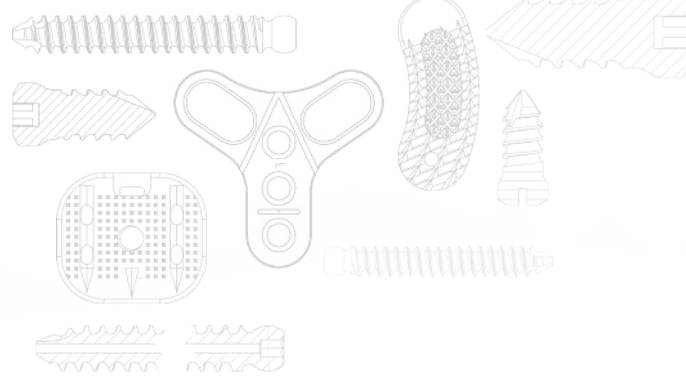

Tra-Ti Trabecular PLIF Cage
Product Code H(mm) L(mm) W(mm) Piece

NM-TTP2407	7	24	10	
NM-TTP2807	7	28	10	
NM-TTP3207	7	32	10	
NM-TTP2408	8	24	10	
NM-TTP2808	8	28	10	
NM-TTP3208	8	32	10	
NM-TTP2409	9	24	10	
NM-TTP2809	9	28	10	
NM-TTP3209	9	32	10	
NM-TTP2410	10	24	10	
NM-TTP2810	10	28	10	
NM-TTP3210	10	32	10	
NM-TTP2411	11	24	10	
NM-TTP2811	11	28	10	
NM-TTP3211	11	32	10	
NM-TTP2412	12	24	10	
NM-TTP2812	12	28	10	
NM-TTP3212	12	32	10	
NM-TTP2413	13	24	10	
NM-TTP2813	13	28	10	
NM-TTP3213	13	32	10	



H: Height(mm), L: Length(mm), W: Width(mm)

Features;


- Anatomical surface
- Smooth wedge nose to facilitate insertion
- Highly porous titanium alloy on top and bottom of implant and all sides of internal graft window

ESA ALIF Peek Cage



This implant system used with ALIF Peek Cage Instrument Set


(Set Code: NM-SS-023)

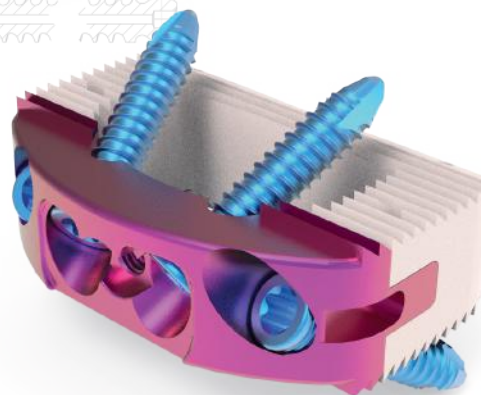

ESA Alif Peek Cage

Product Code H(mm) L(mm) W(mm) Angle Piece

NMALC25351004	10	25	35	4°	
NMALC25351009	10	25	35	9°	
NMALC25351014	10	25	35	14°	
NMALC29401004	10	29	40	4°	
NMALC29401009	10	29	40	9°	
NMALC29401014	10	29	40	14°	
NMALC25351204	12	25	35	4°	
NMALC25351209	12	25	35	9°	
NMALC25351214	12	25	35	14°	
NMALC29401204	12	29	40	4°	
NMALC29401209	12	29	40	9°	
NMALC29401214	12	29	40	14°	
NMALC25351404	14	25	35	4°	
NMALC25351409	14	25	35	9°	
NMALC25351414	14	25	35	14°	
NMALC29401404	14	29	40	4°	
NMALC29401409	14	29	40	9°	
NMALC29401414	14	29	40	14°	
NMALC25351604	16	25	35	4°	
NMALC25351609	16	25	35	9°	
NMALC25351614	16	25	35	14°	
NMALC29401604	16	29	40	4°	
NMALC29401609	16	29	40	9°	
NMALC29401614	16	29	40	14°	



L: Length(mm), W: Width(mm), H: Height(mm)


Features;

- Full contact, full fusion through unique movable head technology
- Fit with the anatomy of patient
- Adjustable easily with threaded mechanism
- Adjustable easily with threaded surface

ESA Alif Peek Cage













Product Code H(mm) L(mm) W(mm) Angle Piece

NMALC25351804	18	25	35	4°	<input type="checkbox"/>
NMALC25351809	18	25	35	9°	<input type="checkbox"/>
NMALC25351814	18	25	35	14°	<input type="checkbox"/>
NMALC29401804	18	29	40	4°	<input type="checkbox"/>
NMALC29401809	18	29	40	9°	<input type="checkbox"/>
NMALC29401814	18	29	40	14°	<input type="checkbox"/>
NMALC25352004	20	25	35	4°	<input type="checkbox"/>
NMALC25352009	20	25	35	9°	<input type="checkbox"/>
NMALC25352014	20	25	35	14°	<input type="checkbox"/>
NMALC29402004	20	29	40	4°	<input type="checkbox"/>
NMALC29402009	20	29	40	9°	<input type="checkbox"/>
NMALC29402014	20	29	40	14°	<input type="checkbox"/>



ESA Alif Screw

Product Code Diameter(mm) Length(mm) Piece

NMALCS4020	4.0	20	<input type="checkbox"/>	
NMALCS4025	4.0	25	<input type="checkbox"/>	
NMALCS4030	4.0	30	<input type="checkbox"/>	
NMALCS4320	4.3	20	<input type="checkbox"/>	
NMALCS4325	4.3	25	<input type="checkbox"/>	
NMALCS4330	4.3	30	<input type="checkbox"/>	
NMALCSF4020	4.0	20	<input type="checkbox"/>	
NMALCSF4025	4.0	25	<input type="checkbox"/>	
NMALCSF4030	4.0	30	<input type="checkbox"/>	
NMALCSF4320	4.3	20	<input type="checkbox"/>	
NMALCSF4325	4.3	25	<input type="checkbox"/>	
NMALCSF4330	4.3	30	<input type="checkbox"/>	



Fine Type



Blunt Type



D: Diameter(mm), L: Length(mm), W: Width(mm), H: Height(mm)



This implant system used with
ALIF Peek Cage Instrument Set
(Set Code: NM-SS-023)

ESA
ALIF Peek Cage




TOWERfix

Scoliosis Deformity Instrument Set



Tower Fix Scoliosis Deformity Instrument Set used with thoracolumbar screws

(Set Code: NM-SS-002)

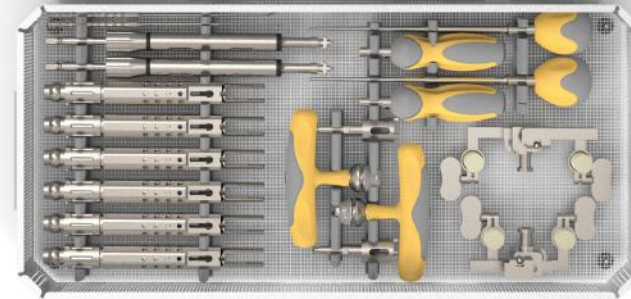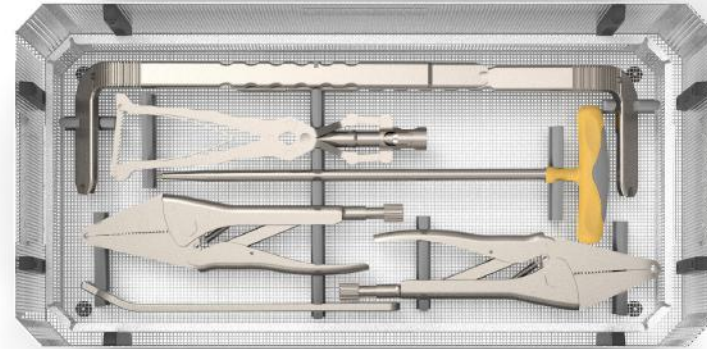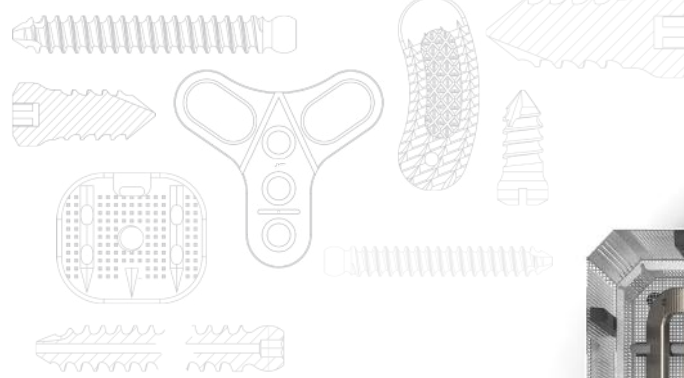

Features;



- The Towerfix Deformity Correction System offers even greater options for surgeons treating patients with spinal deformity. When surgically treating a variety of thoracolumbar pathologies, the Towerfix Deformity Correction System offers additional implant and instrument options to the Towerfix Spinal Fixation System needed to perform complex spine procedures.

Osteotomy & Curette System



Osteotomy Instrument Set
used with **Plexus & Silver**
Posterior Spinal Instrument
Set

(Set Code: NM-SS-003, Set Code: NM-SS-001)

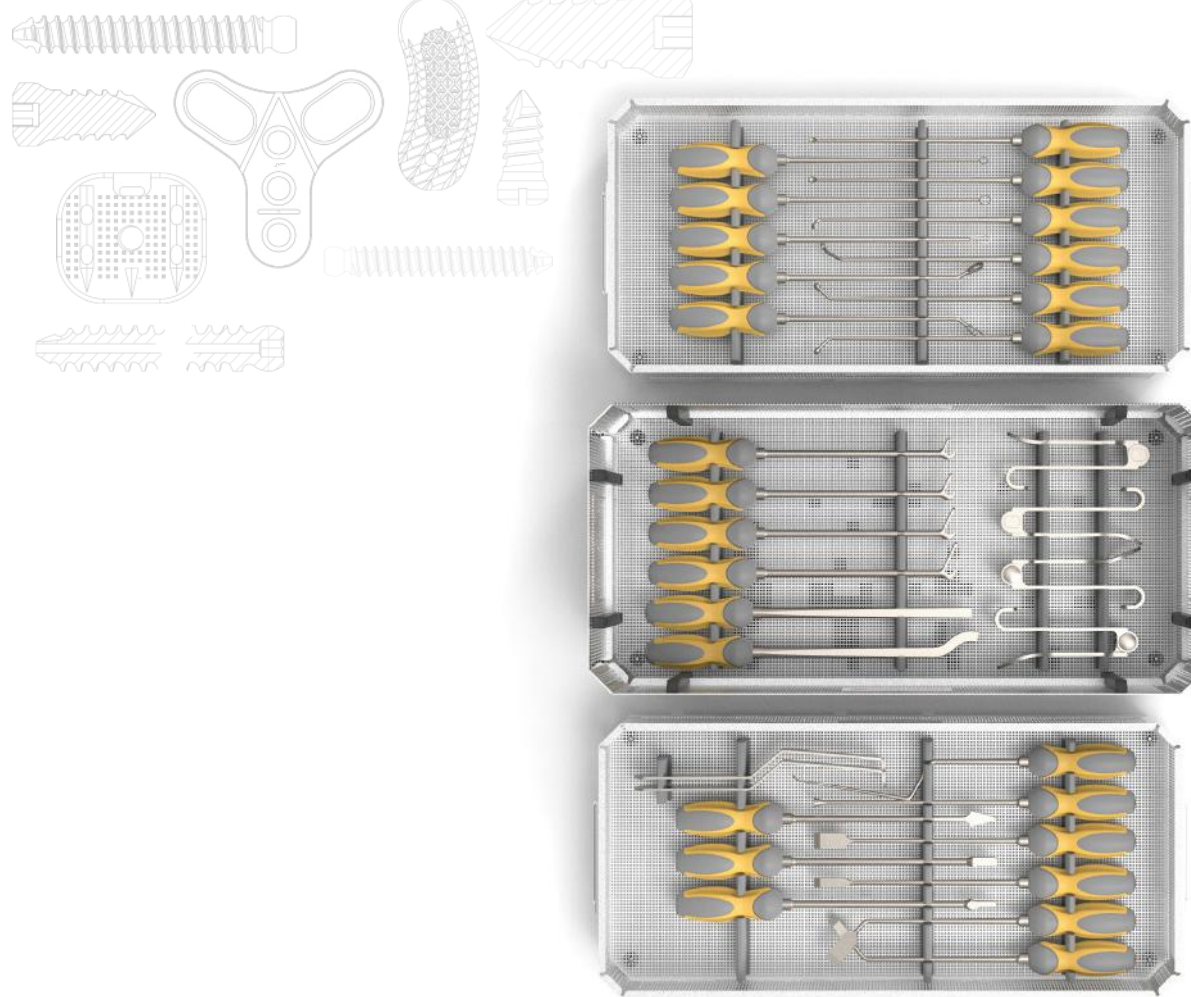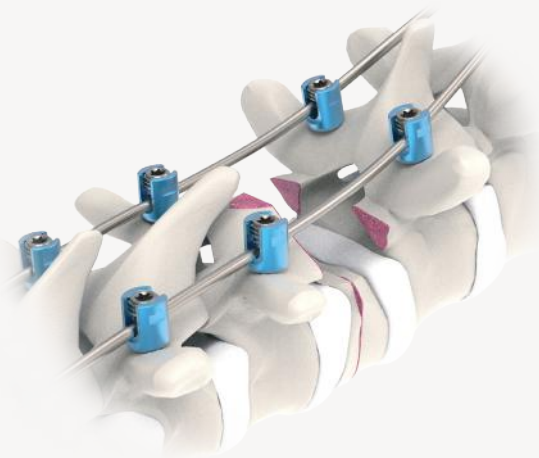


Features;

- Provide effective and simple use
- Include a wide selection of specialized instrumentation
- A truly complete set with dedicated instruments for corrective osteotomies
- Accommodate surgical preferences and anatomical variations
- Soft tissue retraction and protection

Nova-Reinforce


Kyphoplasty Vertebroplasty System

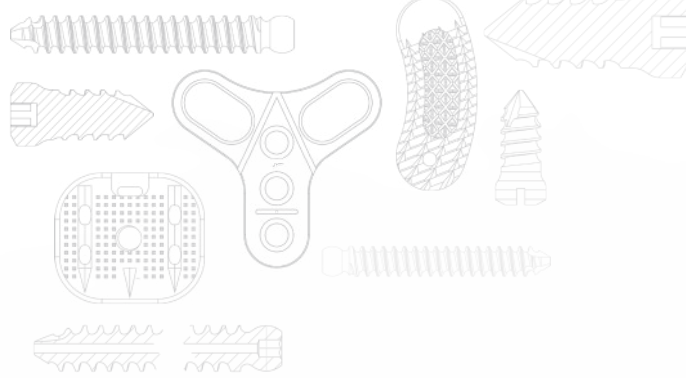

Features;

- Kyphoplasty is a minimally invasive surgery used to treat a spinal compression fracture
- Reduce pain from the fracture
- Stabilize the vertebra
- Restore the vertebra back to its normal height with balloon system

Spinal Bone Cement

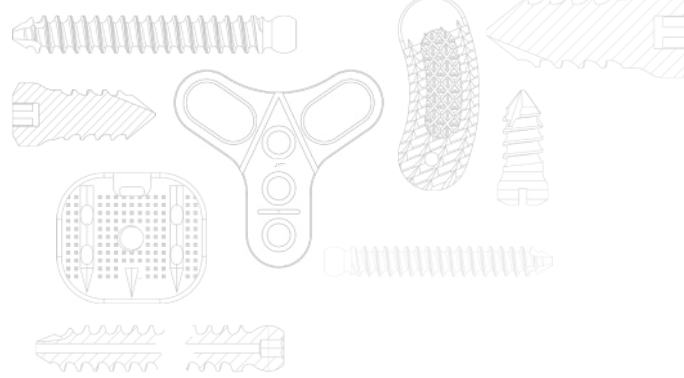

Spinal Bone Cement		
Product Code	Weight(gram)	Piece
NMBES-20	20	<input type="checkbox"/>
NMBES-40	40	<input type="checkbox"/>
NMBES-60	60	<input type="checkbox"/>

Spinal High Viscosity Bone Cement		
Product Code	Weight(gram)	Piece
NMHV-20	20	<input type="checkbox"/>
NMHV-40	40	<input type="checkbox"/>
NMHV-60	60	<input type="checkbox"/>

Spinal Low Viscosity Bone Cement		
Product Code	Weight(gram)	Piece
NMLV-20	20	<input type="checkbox"/>
NMLV-40	40	<input type="checkbox"/>
NMLV-60	60	<input type="checkbox"/>



This graft materials are used with **Vertebroplasty System**




Features;

- An ideal bone graft substitute should be biomechanically stable, able to degrade within an appropriate time frame, exhibit osteoconductive, osteogenic and osteoinductive properties and provide a favourable environment for invading blood vessels and bone forming cells.



Instrument Sets


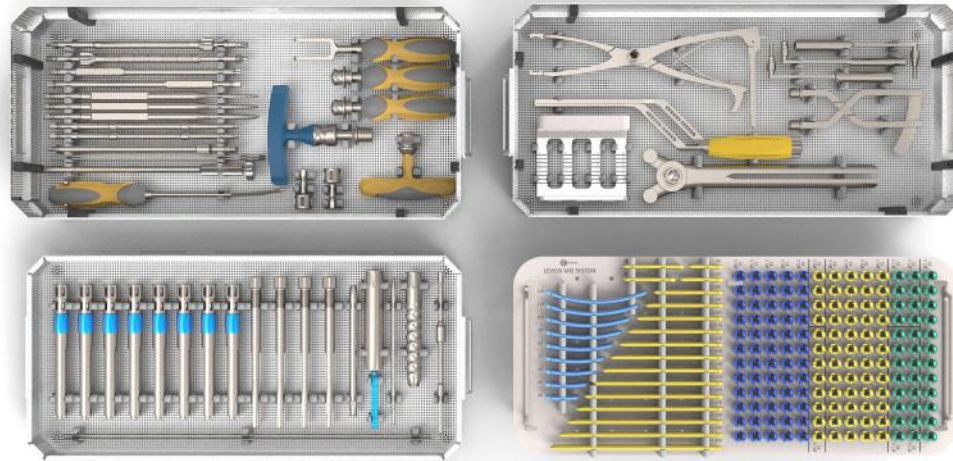


Polar and Polar-B Cervical Peek Cage Instrument Set

(Set Code: NM-SS-013)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

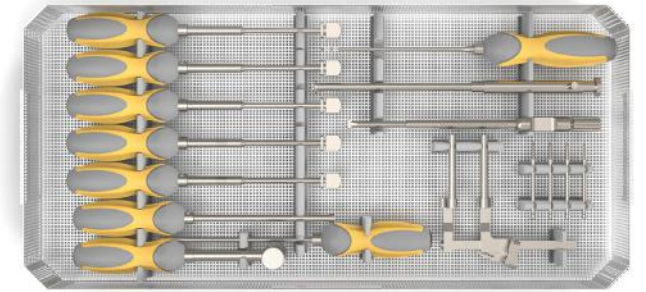
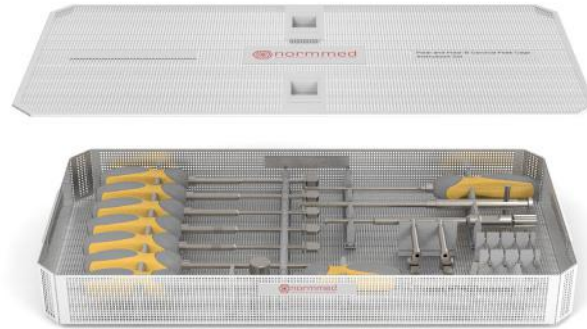


Trimi Anterior Cervical Plate Instrument Set

(Set Code: NM-SS-024)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

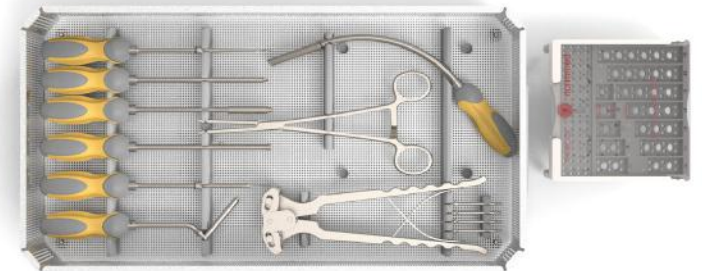
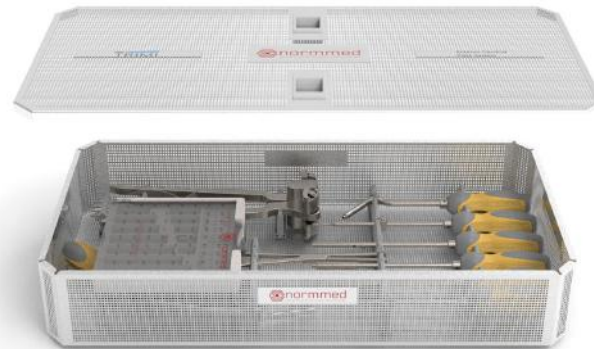


Vertelift-C Corpectomy Cage Instrument Set

(Set Code: NM-SS-006)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

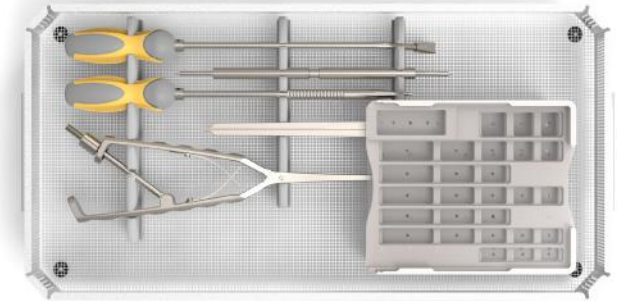
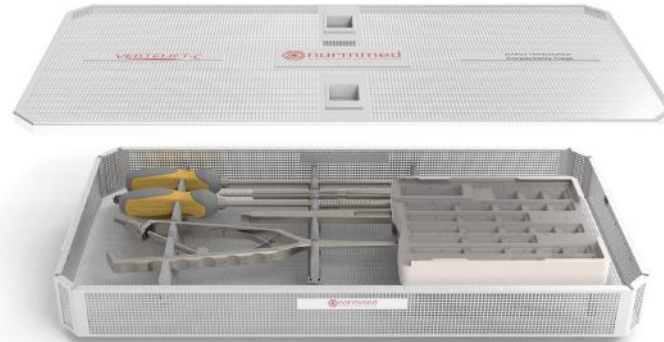


Laminoplasty Plate Instrument Set

(Set Code: NM-SS-019)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

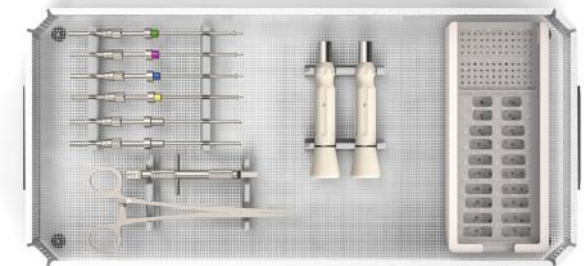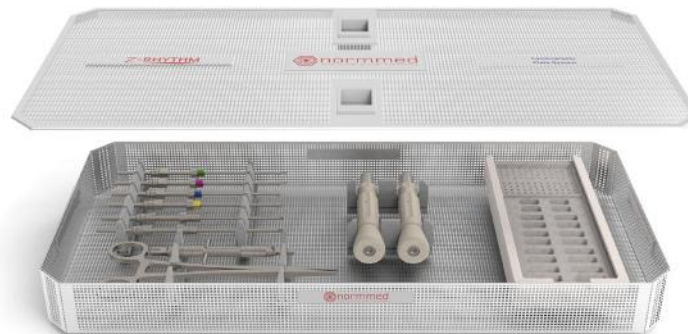


Oxis-PLUS Instrument Set

(Set Code: NM-SS-005)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

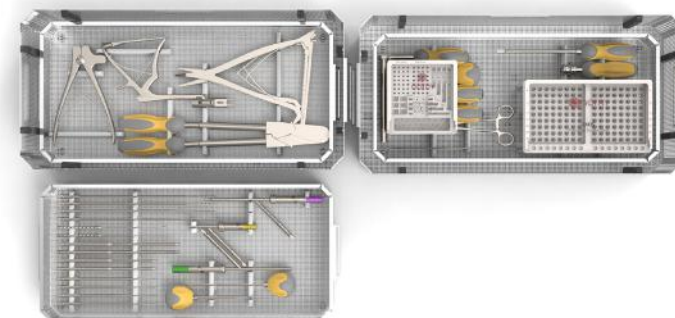


Cervical Disc Prosthesis Instrument Set

(Set Code: NM-SS-021)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

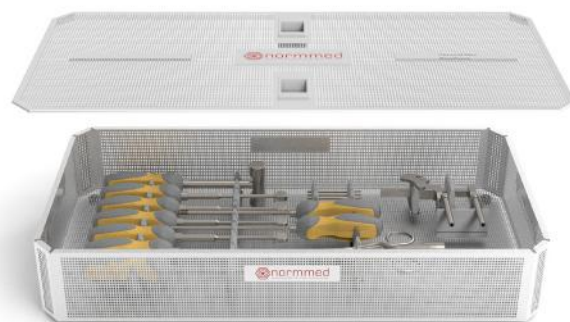


Plexus & Silver Posterior Spinal Instrument Set

(Set Code: NM-SS-001)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.


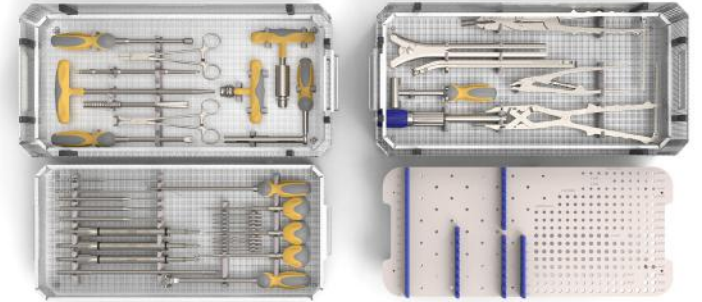


Ares MIS Screw System Instrument Set

(Set Code: NM-SS-004)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

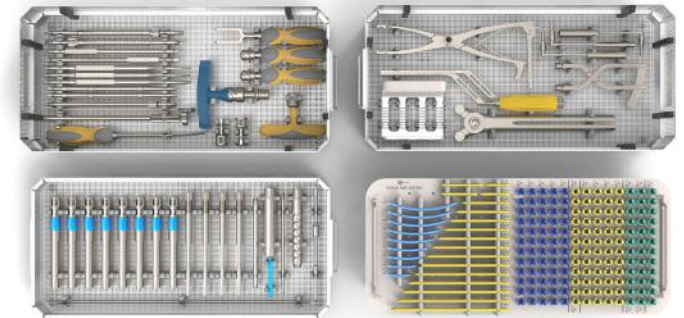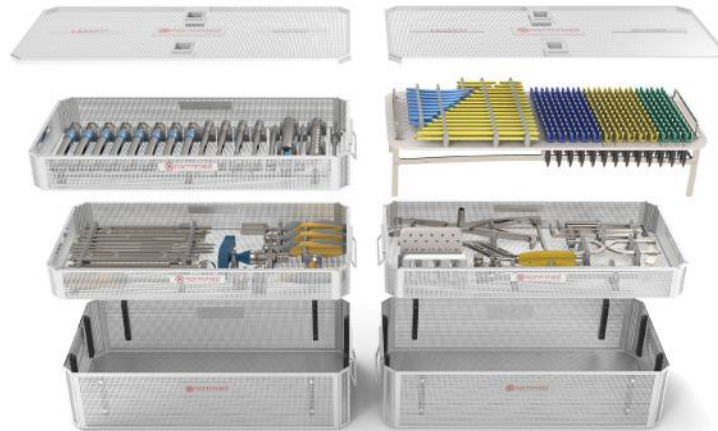


Tower Fix Scoliosis Deformity Instrument Set

(Set Code: NM-SS-002)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

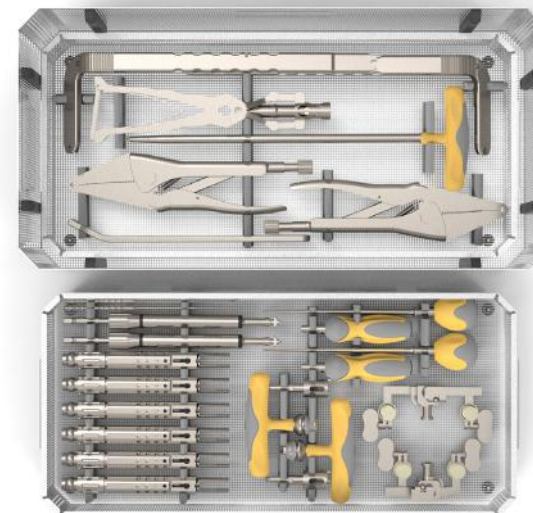


Pedifix Instrument Set

(Set Code: NM-SS-020)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.


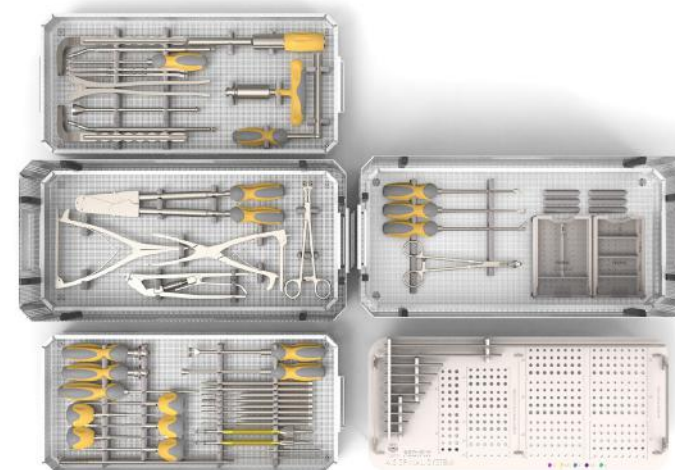


Vertelift - T Instrument Set

(Set Code: NM-SS-007)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

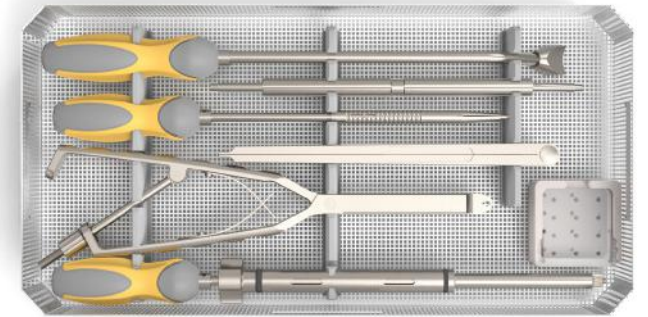
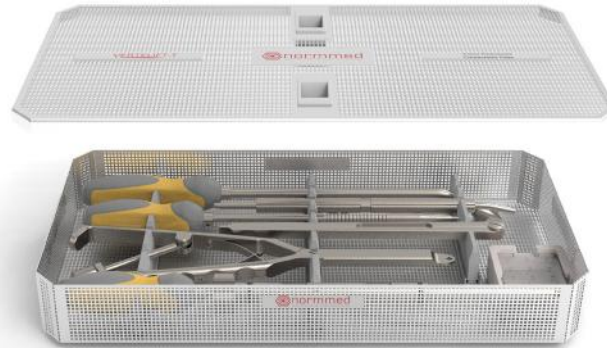


Lumbar Plate System Instrument Set

(Set Code: NM-SS-014)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

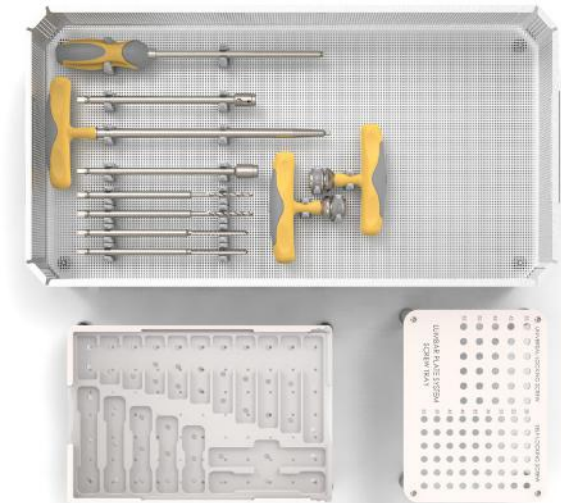
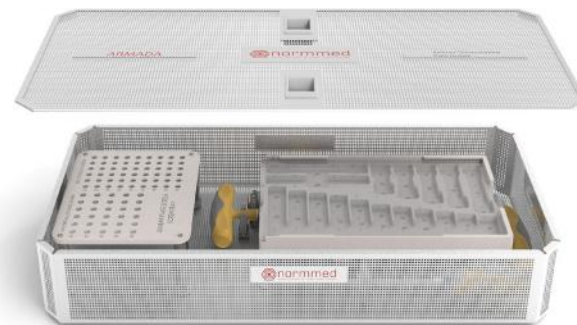


U-Device Instrument Set

(Set Code: NM-SS-018)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

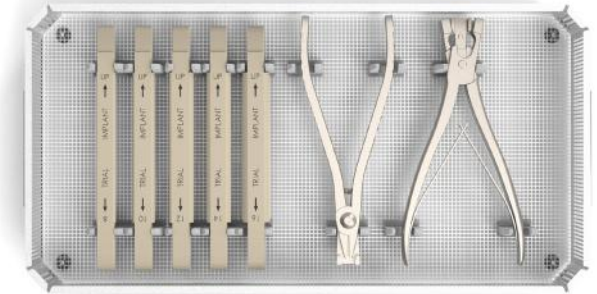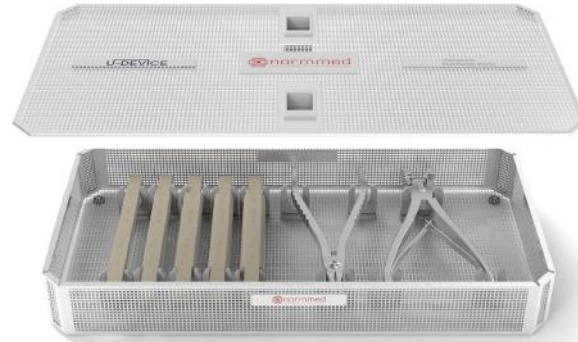


Twisty TLIF Instrument Set

(Set Code: NM-SS-016)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.


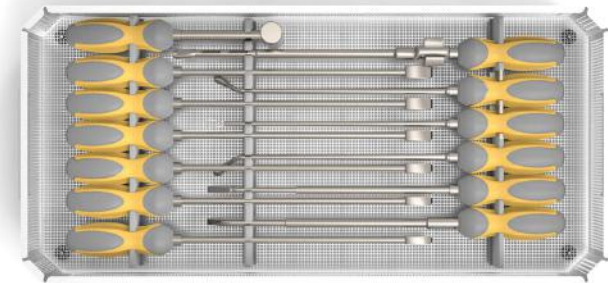


Alligator and Alligator-Exp PLIF Instrument Set

(Set Code: NM-SS-015)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

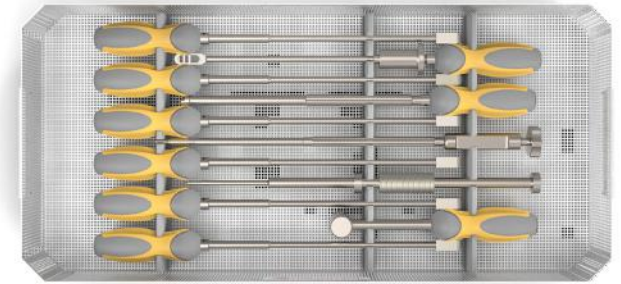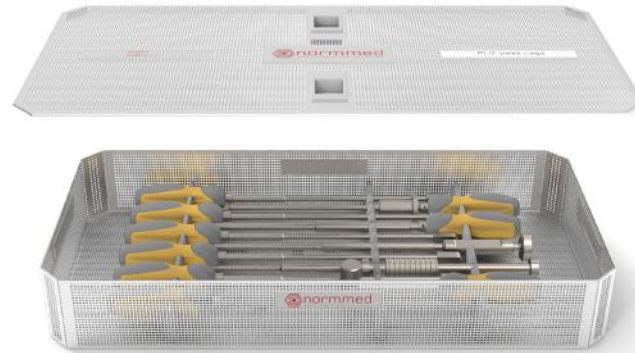


ALIF Peek Cage Instrument Set

(Set Code: NM-SS-023)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

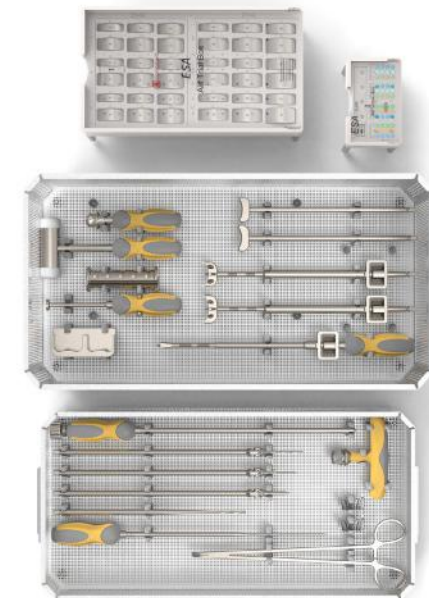


Osteotomy Instrument Set

(Set Code: NM-SS-003)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.


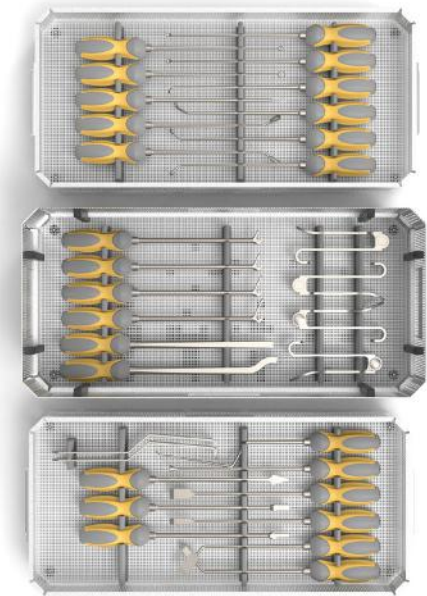


Plexus Hook System Instrument Set

(Set Code: NM-SS-022)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

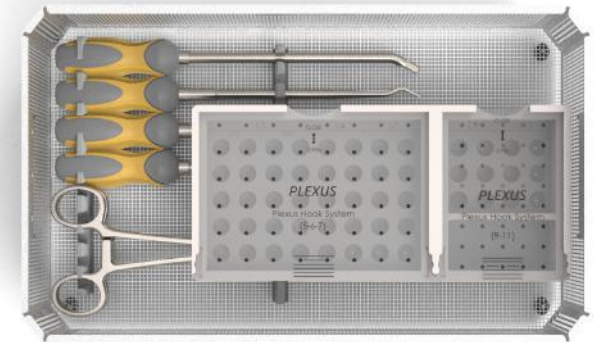
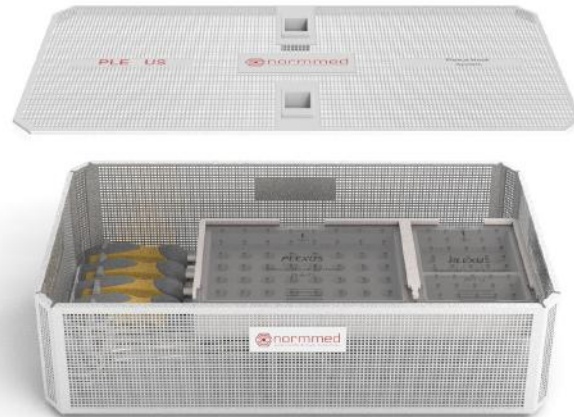


Cervical Retractor System Instrument Set

(Set Code: NM-SS-010)



This container is made of wiremesh stainless steel. It has a high stability, low weight and good sterilization feature.

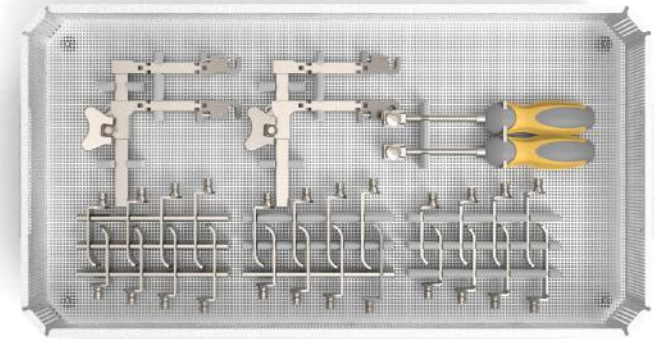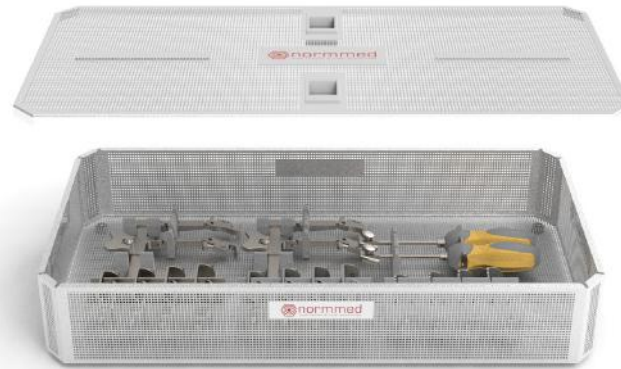



Normmed Medikal San. ve Tic. A.Ş.

İvedik OSB Mah. Havalandırmacılar Cad. No : 193
06378 Yenimahalle / ANKARA / TÜRKİYE

T: +90 312 395 61 84

F: +90 312 395 61 85

info@normmed.com.tr

www.normmed.com.tr

