


4.12.4 Fluoroscopy L.I.H. (Last Image Hold) Function

The L.I.H. function remains the fluoroscopy image on the acquisition monitor after releasing the fluoroscopy foot switch, and is set in the [Fluoroscopy] tab in the [Edit Procedure] window.

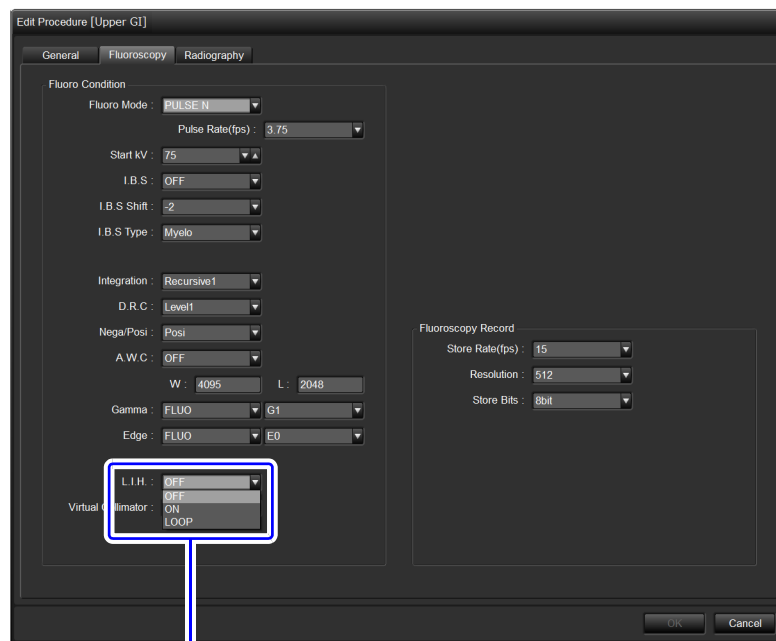

L.I.H. setting

The L.I.H. has three options below.