



TRUST
YOUR HANDS

Gastrointestinal Endoscopy Accessories

INNOVATION
FOR HEALTH

Jiangsu Vedkang Medical Science & Technology Co.,Ltd.

A Address: NO.52, Guoxiang Road, Wujin Economic Development Zone, Changzhou, Jiangsu, China
T Tel: 0086-519-69877751/61 **F** Fax: 0086-519-69877753 **E** E-mail: sales@vedkang.com



About us

Vedkang Medical is one of the leaders that develop, manufacture and market high quality endoscopic devices. Our product lists include ESD products, ERCP products and basic GI endoscopic treatment products, which have been distributed to more than 80 countries worldwide.

Founded in 2003, with more than 750 employees, our mission has always been to innovate for health: to make surgeries easier and patients safer. In 2020, Vedkang medical gained China Science and Technology Entrepreneurship Contribution and National Model Medical Device Enterprise Award.

Culturally, Vedkang is dedicated to be a reliable partner for doctors and a happy place for employees.

Mission: Innovation for easier surgery


Vision: Trusted partners for doctors; happy workplace for employees

Value Proposition: Respect life, respect regulation, innovation focus, develop together, sharing responsibility, simple and efficient, self-examination and growth

Struggle for human health is our eternal pursuit.

More information is available at www.vedkang.com.

Please contact us at: sales@vedkang.com.

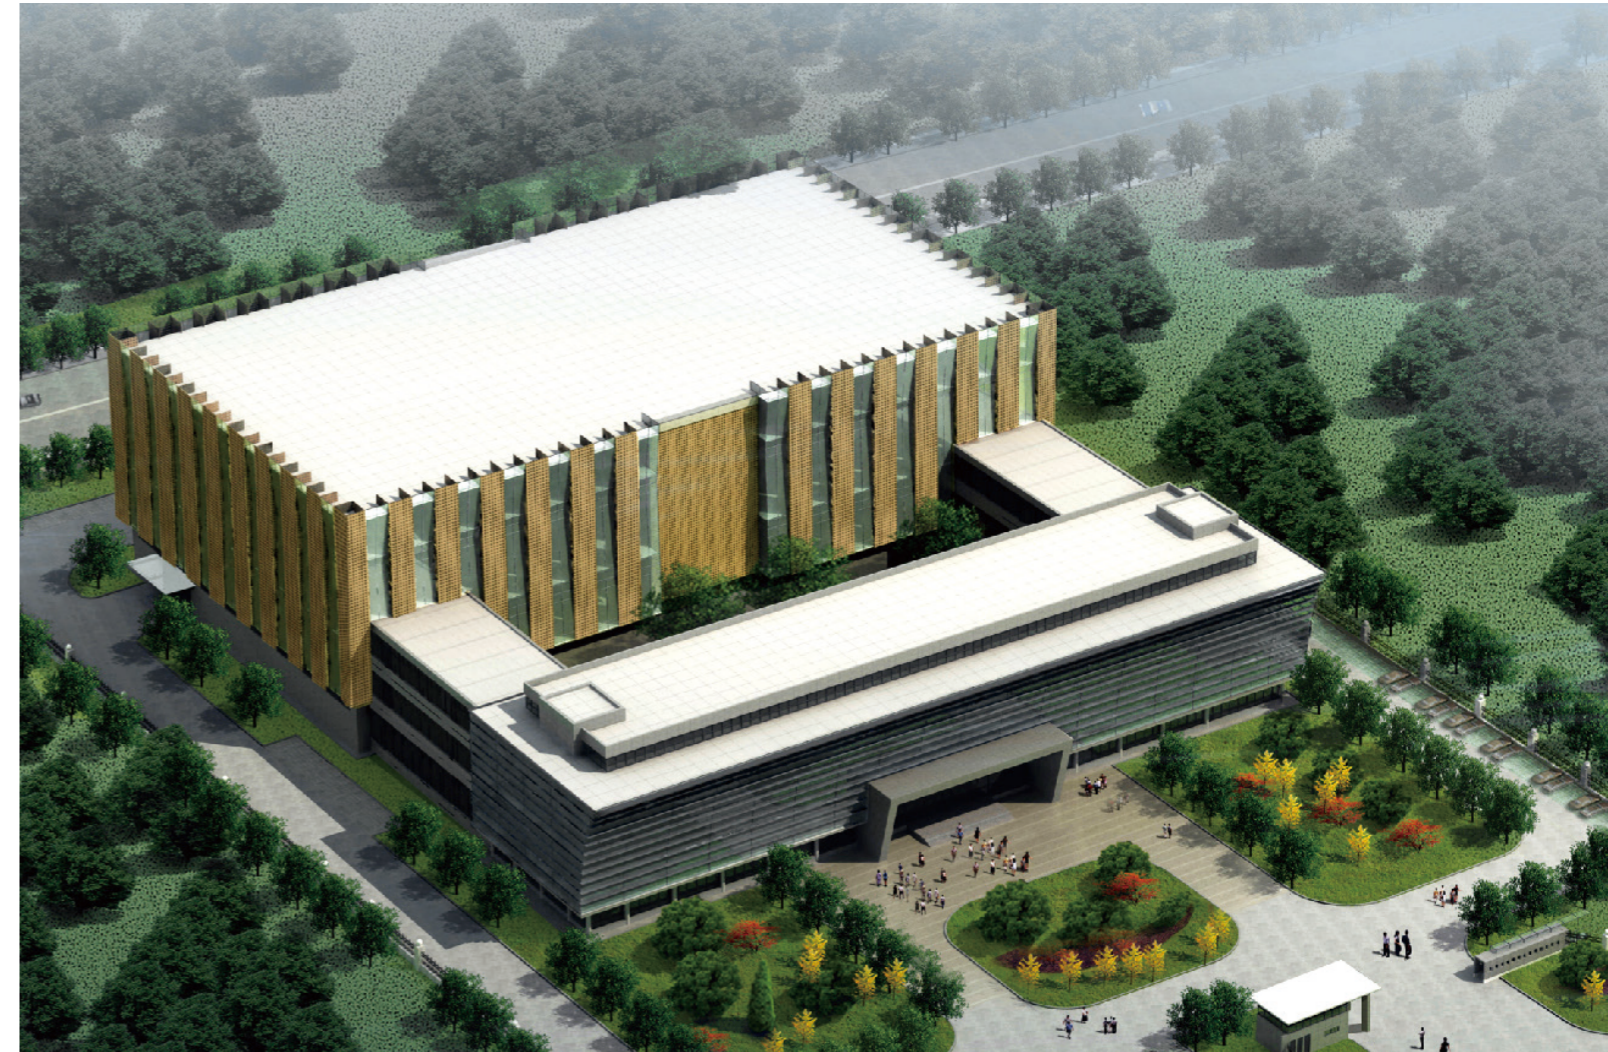

Contents



VedClip

-Disposable Endoscopic Hemoclip /P01



VedBite


-Disposable Non-electric Biopsy Forceps /P15

VedBite Mini

-1.0 Non-electric Biopsy Forceps /P17

VedBite Jumbo

-Non-electric Jumbo Biopsy Forceps /P19



VedBalloon

-Gastrointestinal and Biliary Balloon Catheter /P27



Disposable Nasal Biliary Drainage Tube /P35



VedKnife

Disposable Endoscopic Submucosal Dissection Knife

-D-Type /P04

-T-Type /P05


-L-Type /P06

-Triangle Type /P07



VedBite Hot

-Disposable Hot Biopsy Forceps /P21



VedDilator

-3-Stage Balloon Dilation Catheter /P29



VedGrasper

-Disposable Grasping Forceps /P37


-Disposable Grasping Forceps Net type /P39



VedSnare

-Disposable Polyp Snare /P09

-Disposable Cold Snare /P11



VedWire

-Non-vascular Guidewire /P23



VedExtractor

-Stone Extraction Balloon /P31



VedAccessories

-Disposable Spray Catheter /P41

-Disposable Cytology Brush /P43

-Cleaning Brush for Endoscope /P45

-Balloon Inflator /P47

-Disposable Bite Block /P49


-Polyp Trap /P50

-Disposable Bougie Dilator /P51

-Bougie Dilator Set /P52

-Biopsy Valve /P53

-Biopsy Valve Set /P54



VedNeedle

-Injection Needle /P13



VedTome

-Disposable Sphincterotome /P25




VedBasket

-Stone Extraction Basket /P33

Disposable Endoscopic Hemoclip

- ☑ ESD
- ☑ Hemostasis
- ☑ EMR
- ☑ STER

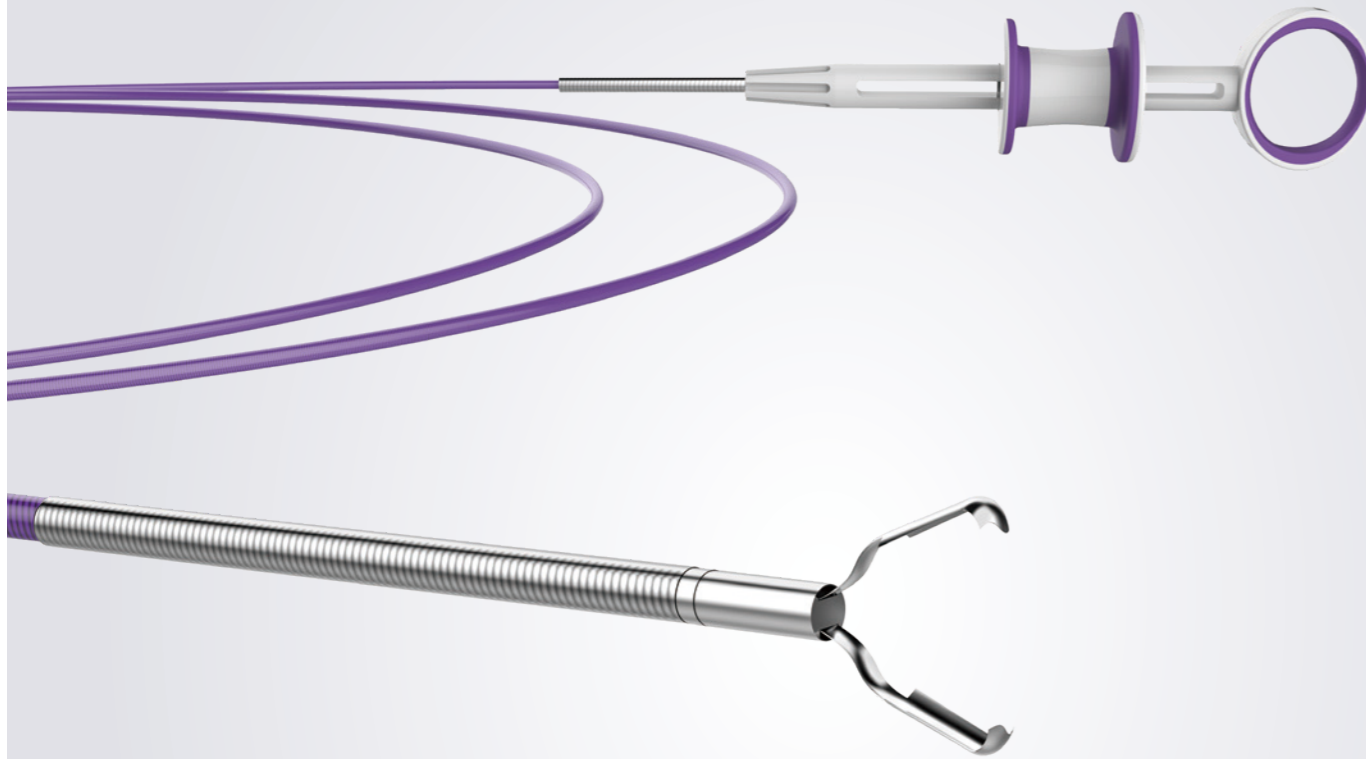

1: 1 360° ROTATION
MAKES A MORE PRECISE CLOSURE

Usage

- The instrument is designed to be used with endoscope for clipping of the soft tissue in gastrointestinal (GI) tract.

Features

- One-one rotation.
- Accurate positioning.
- Handle safety lock design.
- Repositionable clips.


Specifications

Model	Clip opening size (mm)	Working Length (mm)	Endoscope Channel (mm)	Characteristics	
VDK-CD-09-160-O	9	1600	≥ 2.8	Gastroscopy	Uncoated
★ VDK-CD-11-160-O	11	1600	≥ 2.8		
VDK-CD-13-160-O	13	1600	≥ 2.8		
VDK-CD-16-160-O	16	1600	≥ 2.8		
VDK-CD-09-230-O	9	2300	≥ 2.8	Colonoscopy	
★ VDK-CD-11-230-O	11	2300	≥ 2.8		
VDK-CD-13-230-O	13	2300	≥ 2.8		
VDK-CD-16-230-O	16	2300	≥ 2.8		
VDK-CD-09-160-P	9	1600	≥ 2.8	Gastroscopy	Coated
★ VDK-CD-11-160-P	11	1600	≥ 2.8		
VDK-CD-13-160-P	13	1600	≥ 2.8		
VDK-CD-16-160-P	16	1600	≥ 2.8		
VDK-CD-09-230-P	9	2300	≥ 2.8	Colonoscopy	
★ VDK-CD-11-230-P	11	2300	≥ 2.8		
VDK-CD-13-230-P	13	2300	≥ 2.8		
VDK-CD-16-230-P	16	2300	≥ 2.8		

★ Common specifications

Disposable Endoscopic Submucosal Dissection Knife

☑ ESD

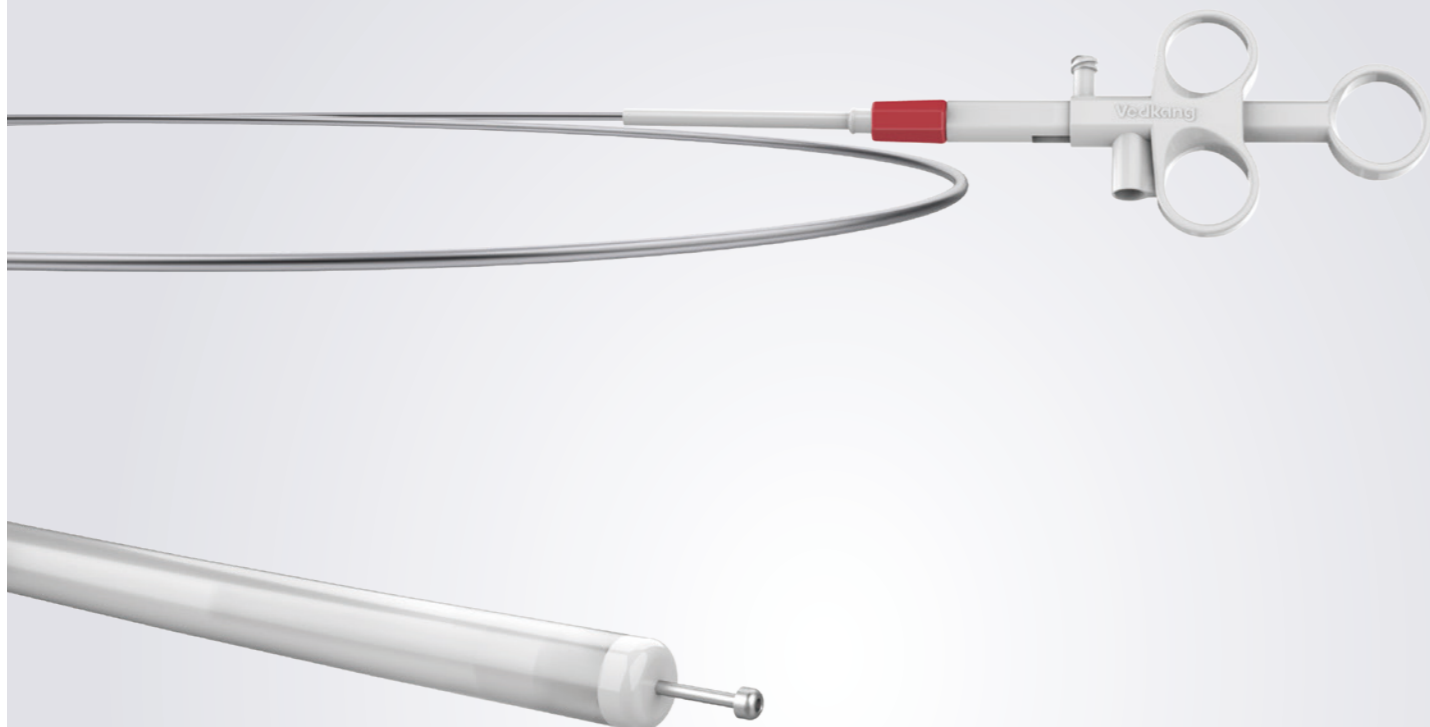


GOOD CUTTING EFFICIENCY
HIGH SAFETY

Usage

- Used with endoscope to perform marking, incision, dissection and hemostasis in gastrointestinal mucosa and submucosa.

Disposable Endoscopic Submucosal Dissection Knife

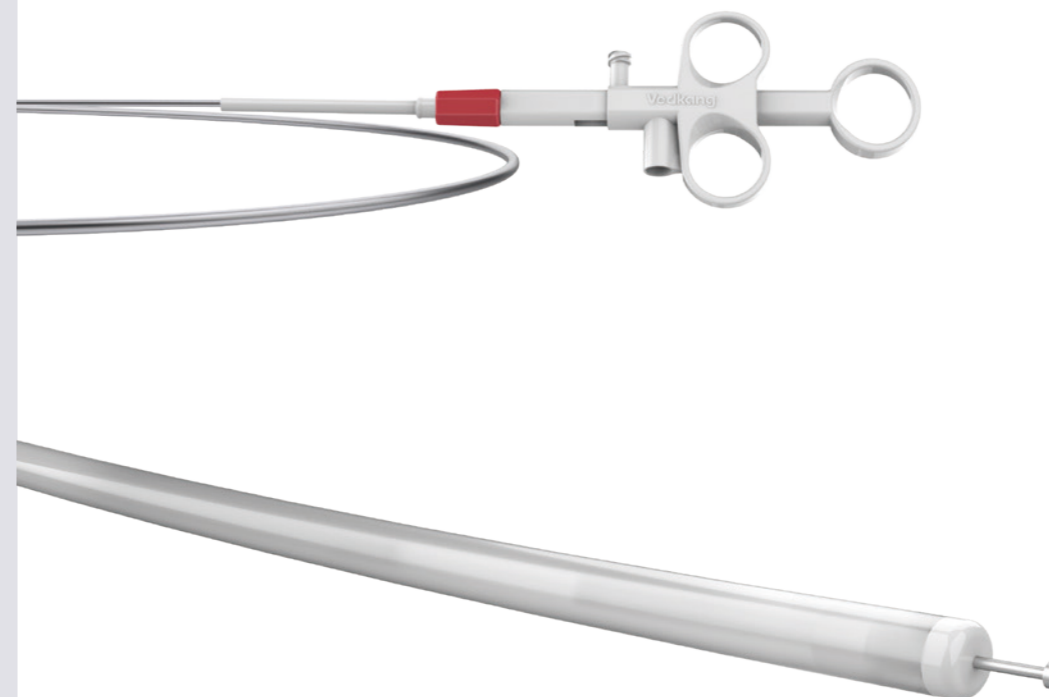


Features

D type:

- With Versatile function : Marking , Hemostasis, Dissection, the controllable knife tip can reduce the instrument exchange and save procedure time.
- The special coating on Knife tip ensures no eschar during dissection to make good endoscopic view .
- Water jet design on knife tip can replenish liquid and flush bleeding area during procedure, reducing instrument exchange.

Specifications

Model	Cutting Knife Length(mm)	Length(mm)	Working Channel (mm)	Characteristics
VDK-KM-20-160-D	2	1600	≥2.8	D type
VDK-KM-20-165-D	2	1650	≥2.8	
VDK-KM-15-195-D	1.5	1950	≥2.8	
VDK-KM-15-200-D	1.5	2000	≥2.8	
VDK-KM-15-220-D	1.5	2200	≥2.8	
VDK-KM-15-230-D	1.5	2300	≥2.8	

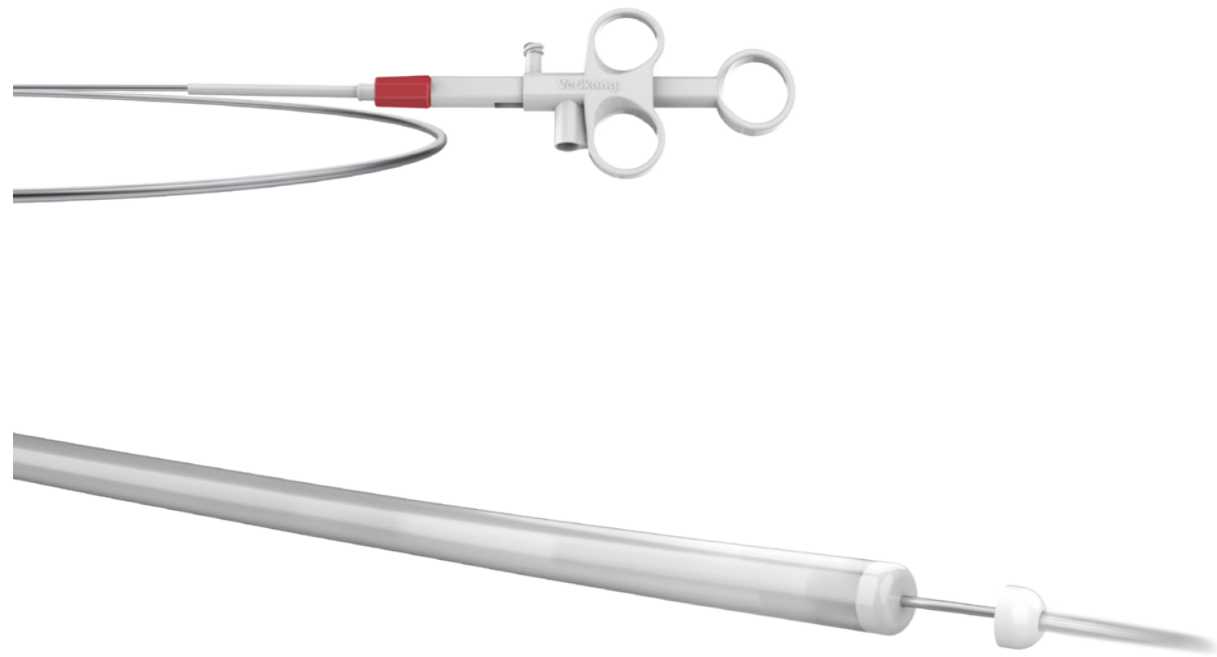


Features

T type:

- Water jet design on knife tip can replenish liquid and flush bleeding area during procedure, reducing instrument exchange.
- Groove design on ceramic tip can Insulate metal tip's contact with normal tissue ,Preventing heating damage.
- The triangle electrode can widen the cutting range ,keeping cutting efficiency .

Specifications

Model	Cutting Knife Length(mm)	Length(mm)	Working Channel (mm)	Characteristics
VDK-KM-40-160-T	4	1600	≥2.8	T type
VDK-KM-40-165-T	4	1650	≥2.8	

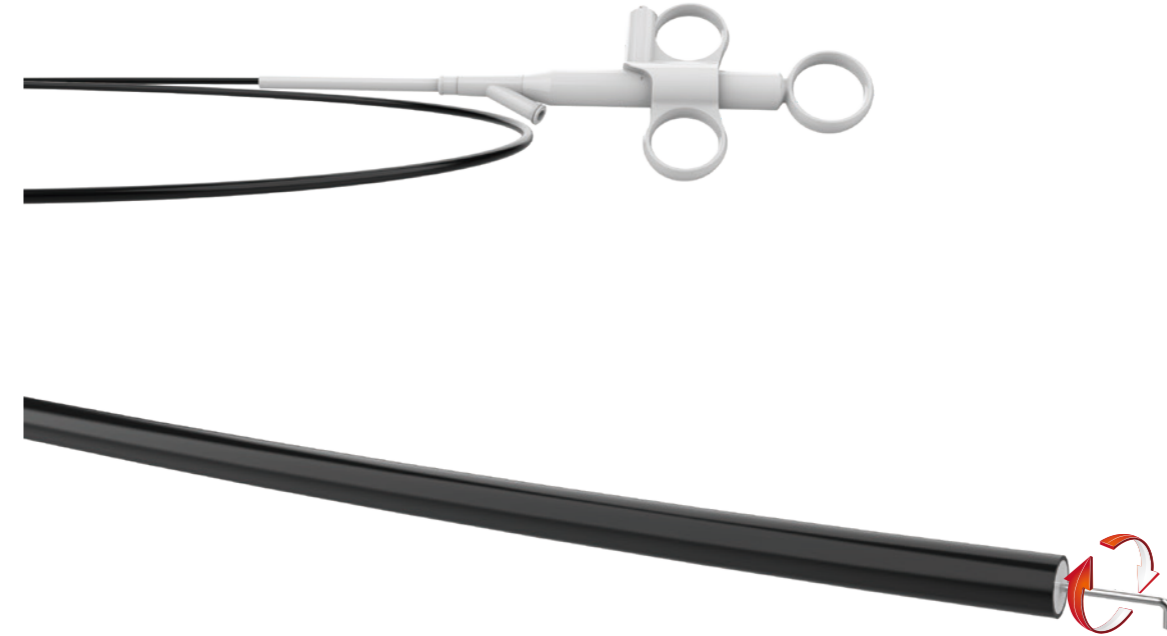

Features

L type:


- The hook shaped knife can be used to hook tissues and cut. And it is also suitable for controlling cutting depth and cutting in any direction, making it safer for incision.
- Rotatable L-shaped knife tip can make it easier to obtain the best incision direction .

Specifications

Model	Cutting Knife Length(mm)	Length(mm)	Working Channel (mm)	Characteristics
VDK-KM-45-160-H	4.5	1600	≥2.8	L type
VDK-KM-45-165-H	4.5	1650	≥2.8	
VDK-KM-45-195-H	4.5	1950	≥2.8	
VDK-KM-45-200-H	4.5	2000	≥2.8	
VDK-KM-45-230-H	4.5	2300	≥2.8	

Disposable Endoscopic Submucosal Dissection Knife


- ☑ STER
- ☑ POEM

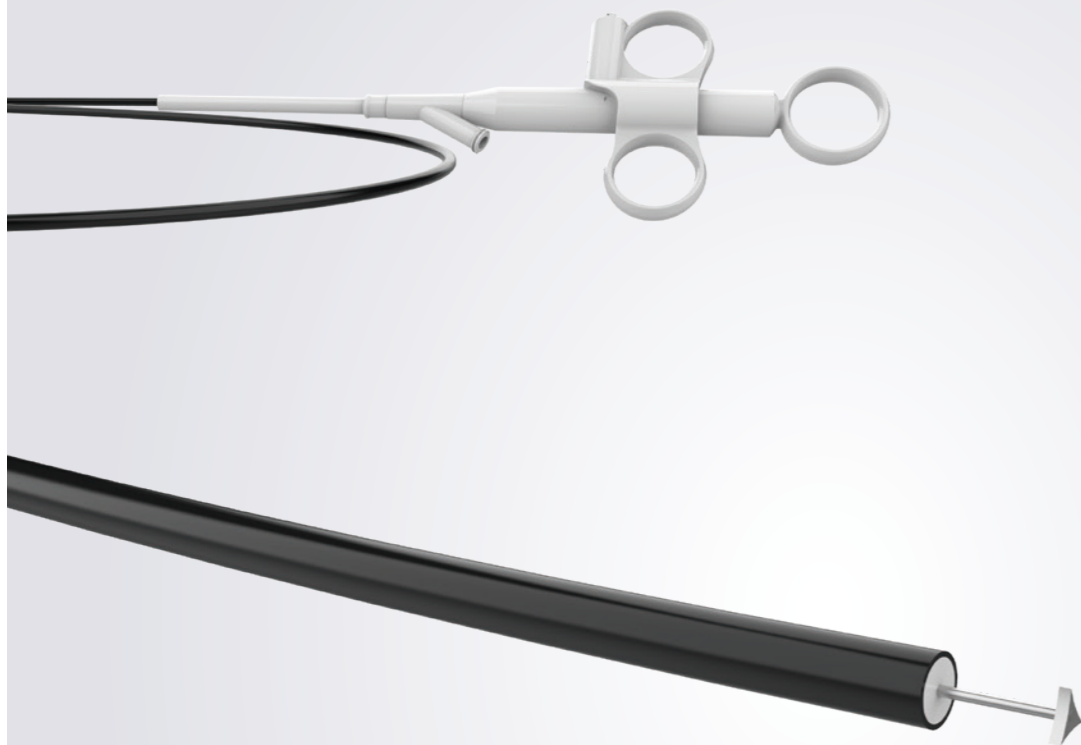

GOOD CUTTING EFFICIENCY
HIGH SAFETY

Usage

- Used with endoscope to perform marking, incision, dissection and hemostasis in gastrointestinal mucosa and submucosa.

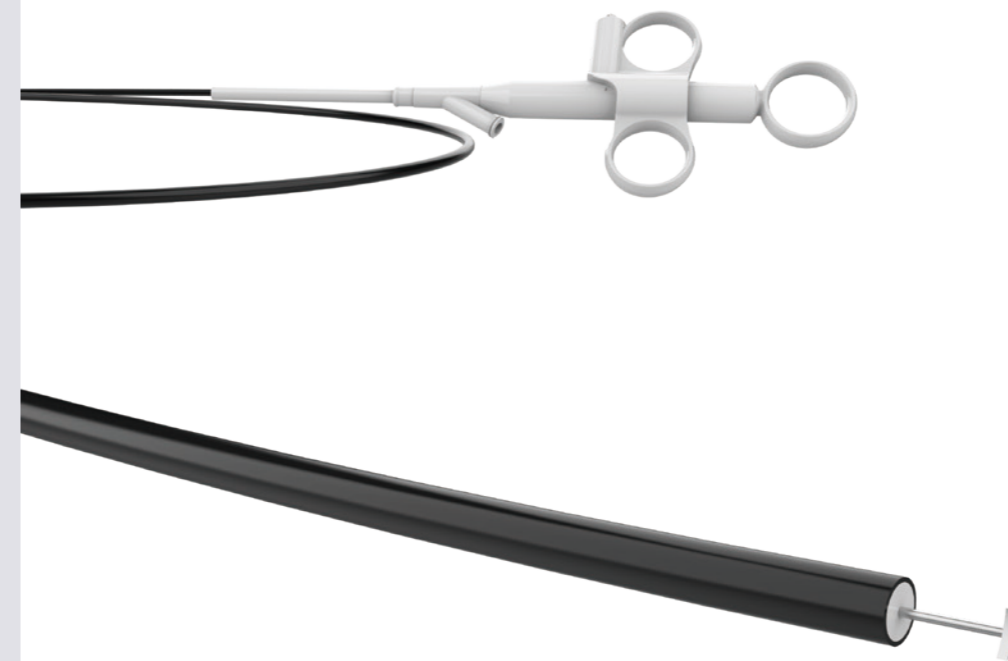

Features

Triangle type:


- Triangle knife tip performs free cutting in an arbitrary direction.
- Good Sharpness is suitable for muscular layer.

Specifications

Model	Cutting Knife Length(mm)	Length(mm)	Working Channel (mm)	Characteristics
VDK-KM-45-160-J	4.5	1600	≥2.8	Triangle type
VDK-KM-45-165-J	4.5	1650	≥2.8	

Disposable Polyp Snare

- ☑ ESD
- ☑ Polyp Retrieval
- ☑ EMR

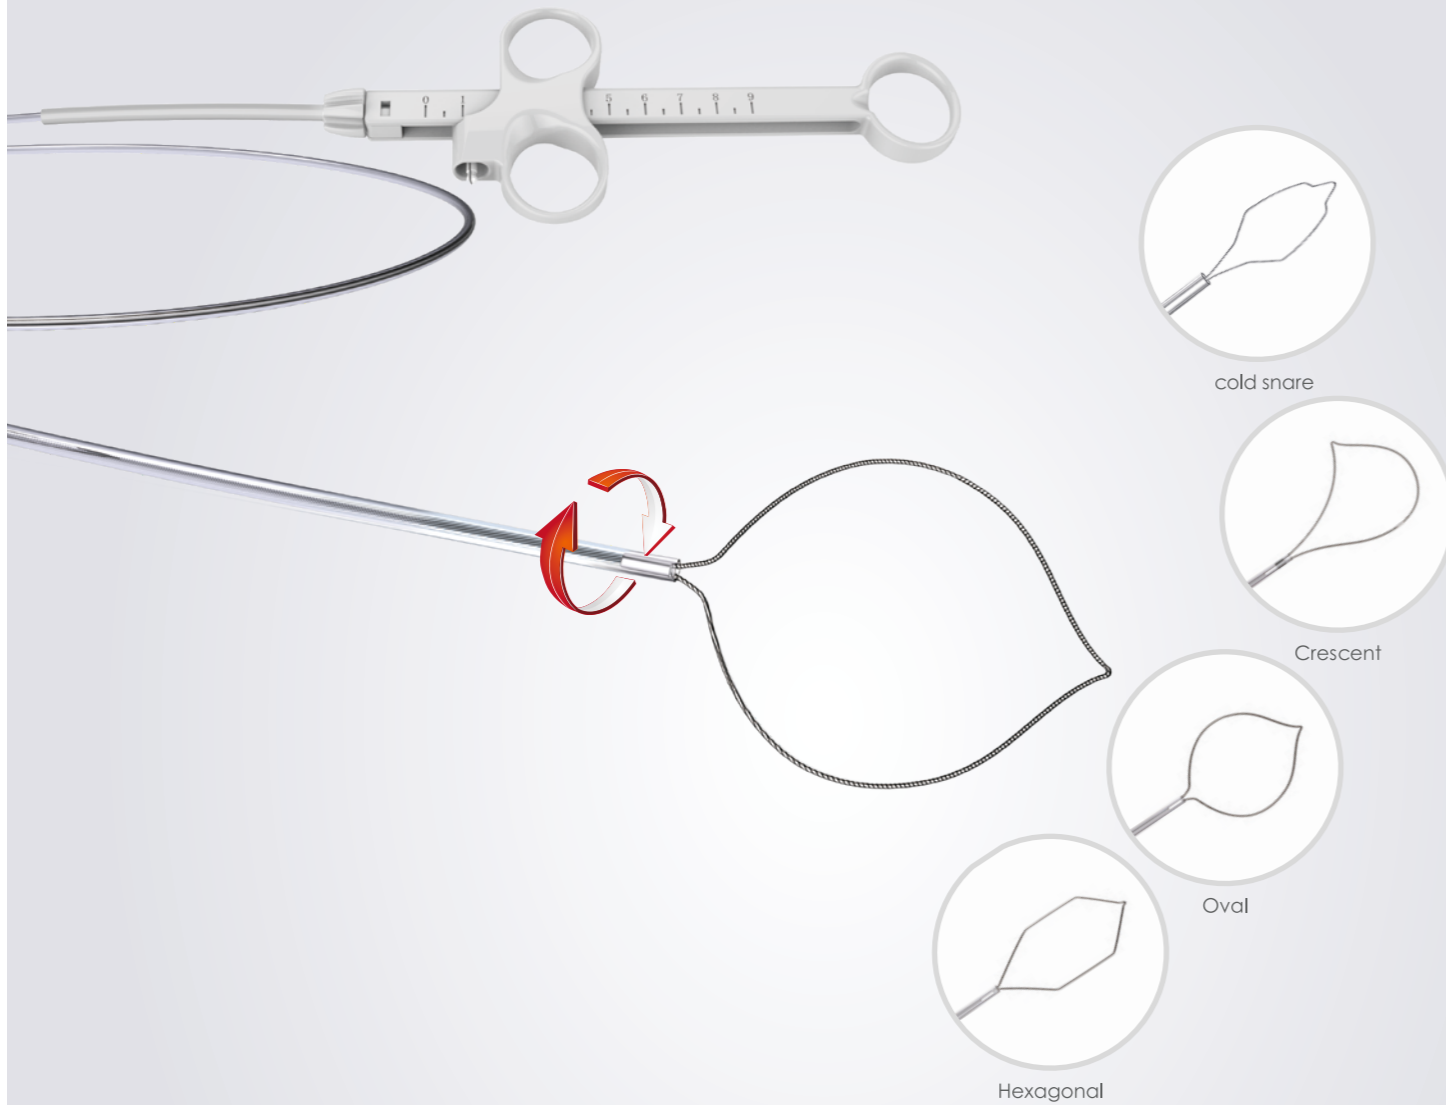

**VEDSNARE,
YOUR EMR FIRST CHOICE**

Usage

- This instrument is used in combination with endoscope for cutting polyps or other redundant tissues with high-frequency current in digestive tract.

Features

- Rotatable type optional, guaranteed one-one rotation.
- Moderated soft wire avoids slipping off.

Specifications

Oval Snare

Model	O.D.(mm)	Length(mm)	Loop Width(mm)	Characteristics
VDK-SD-18-160-20-A1	1.8	1600	20	Standard Rotation
VDK-SD-23-160-10-A1	2.3	1600	10	
★ VDK-SD-23-230-10-A1	2.3	2300	10	
VDK-SD-23-160-15-A1	2.3	1600	15	
★ VDK-SD-23-230-15-A1	2.3	2300	15	
VDK-SD-23-160-20-A1	2.3	1600	20	
★ VDK-SD-23-230-20-A1	2.3	2300	20	
VDK-SD-23-160-25-A1	2.3	1600	25	
★ VDK-SD-23-230-25-A1	2.3	2300	25	
VDK-SD-23-160-30-A1	2.3	1600	30	
★ VDK-SD-23-230-30-A1	2.3	2300	30	
VDK-SD-23-160-35-A1	2.3	1600	35	
★ VDK-SD-23-230-35-A1	2.3	2300	35	
VDK-SD-23-160-50-A1	2.3	1600	50	
★ VDK-SD-23-230-50-A1	2.3	2300	50	
★ VDK-SD-23-230-10-A1R	2.3	2300	10	Synchronous Rotation
★ VDK-SD-23-230-15-A1R	2.3	2300	15	
★ VDK-SD-23-230-20-A1R	2.3	2300	20	
★ VDK-SD-23-230-25-A1R	2.3	2300	25	
★ VDK-SD-23-230-30-A1R	2.3	2300	30	

Crescent Snare

Model	O.D.(mm)	Length(mm)	Loop Width(mm)	Characteristics
VDK-SD-18-160-20-B1	1.8	1600	20	Standard Rotation
VDK-SD-23-160-10-B1	2.3	1600	10	
VDK-SD-23-230-10-B1	2.3	2300	10	
VDK-SD-23-160-15-B1	2.3	1600	15	
VDK-SD-23-230-15-B1	2.3	2300	15	
VDK-SD-23-160-20-B1	2.3	1600	20	
VDK-SD-23-230-20-B1	2.3	2300	20	
VDK-SD-23-160-25-B1	2.3	1600	25	
VDK-SD-23-230-25-B1	2.3	2300	25	
VDK-SD-23-160-30-B1	2.3	1600	30	
VDK-SD-23-230-30-B1	2.3	2300	30	


Hexagonal Snare

Model	O.D.(mm)	Length(mm)	Loop Width(mm)	Characteristics	
★ VDK-SD-18-160-20-C1	1.8	1600	20	Standard Rotation	
VDK-SD-23-160-10-C1	2.3	1600	10		
★ VDK-SD-23-230-10-C3	2.3	2300	10		
VDK-SD-23-160-15-C1	2.3	1600	15		
★ VDK-SD-23-230-15-C3	2.3	2300	15		
VDK-SD-23-160-20-C1	2.3	1600	20		
★ VDK-SD-23-230-20-C1	2.3	2300	20		
VDK-SD-23-160-25-C1	2.3	1600	25		
VDK-SD-23-230-25-C1	2.3	2300	25		
VDK-SD-23-160-30-C1	2.3	1600	30		
VDK-SD-23-230-30-C1	2.3	2300	30		
★ VDK-SD-23-230-10-C3R	2.3	2300	10		Synchronous Rotation
★ VDK-SD-23-230-15-C3R	2.3	2300	15		

★ Common specifications

| Disposable Cold Snare

- Polyp Retrieval

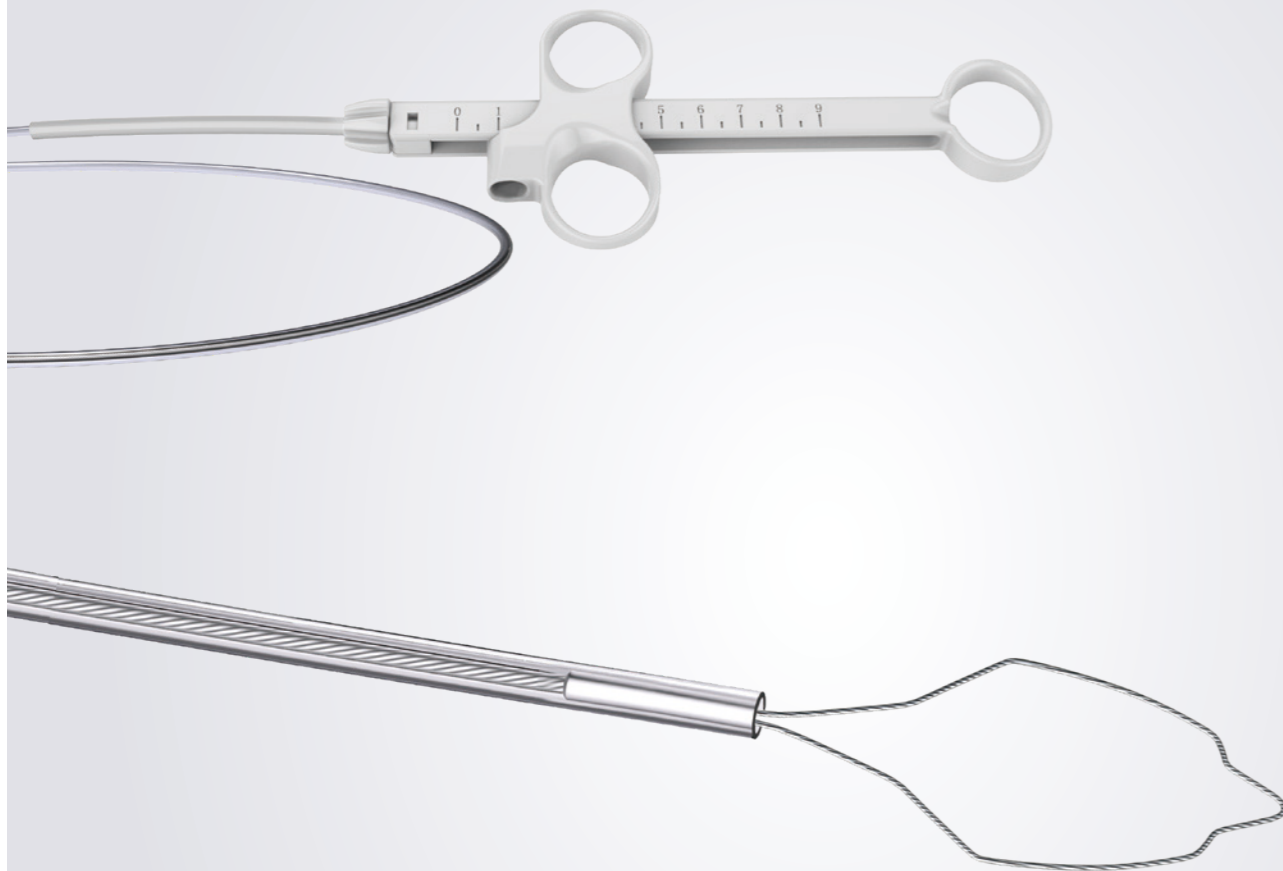

***EASY CUT,
EASY WAY***

Usage

- This instrument is used in combination with endoscope for cutting polyps or other redundant tissues in digestive tract.

Features

- Rotatable Type Optional, Guaranteed One-One Rotation.
- Easy for cutting, excellent performance.

Specifications

Model	O.D.(mm)	Length(mm)	Loop Width(mm)	Characteristics
VDK-CS-23-230-10-C3	2.3	2300	10	Standard Rotation
VDK-CS-23-230-15-C3	2.3	2300	15	Standard Rotation
VDK-CS-23-230-10-C3R	2.3	2300	10	Synchronous Rotation
VDK-CS-23-230-15-C3R	2.3	2300	15	Synchronous Rotation

Injection Needle

- ESD
- Hemostasis
- Polyp Retrieval
- EMR



**EASY PUNCTURE,
RAPID INJECTION**

Usage

- Endoscopic treatment for gastrointestinal polyps or submucosal tumors
- Endoscopic treatment for patients with gastrointestinal varicose veins.

Features

- Less friction tube material & hard outer tube support pushing power.
- Scientific 3-cut sharp needle enables easier puncturing.
- Lager tube I.D. & Super smooth material brings the rapid injection.
- Bigger cut section part provides faster flow.


Specifications

Model	O.D. (mm)	Working Length (mm)	Needle size (diameter/ length)	Endoscope Channel (mm)
★ VDK-IN-18-120-2205-A	1.8	1200	22G, 5mm	≥2.0
VDK-IN-18-180-2204-A	1.8	1800	22G, 4mm	≥2.0
VDK-IN-18-180-2205-A	1.8	1800	22G, 5mm	≥2.0
VDK-IN-18-180-2206-A	1.8	1800	22G, 6mm	≥2.0
VDK-IN-18-180-2304-A	1.8	1800	23G, 4mm	≥2.0
VDK-IN-18-180-2305-A	1.8	1800	23G, 5mm	≥2.0
VDK-IN-18-180-2306-A	1.8	1800	23G, 6mm	≥2.0
VDK-IN-18-180-2504-A	1.8	1800	25G, 4mm	≥2.0
VDK-IN-18-180-2505-A	1.8	1800	25G, 5mm	≥2.0
VDK-IN-18-180-2506-A	1.8	1800	25G, 6mm	≥2.0
VDK-IN-23-180-1904-A	2.3	1800	19G, 4mm	≥2.8
VDK-IN-23-180-1905-A	2.3	1800	19G, 5mm	≥2.8
VDK-IN-23-180-1906-A	2.3	1800	19G, 6mm	≥2.8
VDK-IN-23-180-2204-A	2.3	1800	22G, 4mm	≥2.8
VDK-IN-23-180-2205-A	2.3	1800	22G, 5mm	≥2.8
VDK-IN-23-180-2206-A	2.3	1800	22G, 6mm	≥2.8
★ VDK-IN-23-180-2304-A	2.3	1800	23G, 4mm	≥2.8
★ VDK-IN-23-180-2305-A	2.3	1800	23G, 5mm	≥2.8
VDK-IN-23-180-2306-A	2.3	1800	23G, 6mm	≥2.8
★ VDK-IN-23-180-2504-A	2.3	1800	25G, 4mm	≥2.8
VDK-IN-23-180-2505-A	2.3	1800	25G, 5mm	≥2.8
VDK-IN-23-180-2506-A	2.3	1800	25G, 6mm	≥2.8
VDK-IN-23-230-1904-A	2.3	2300	19G, 4mm	≥2.8
VDK-IN-23-230-1905-A	2.3	2300	19G, 5mm	≥2.8
VDK-IN-23-230-1906-A	2.3	2300	19G, 6mm	≥2.8
★ VDK-IN-23-230-2104-A	2.3	2300	21G, 4mm	≥2.8
★ VDK-IN-23-230-2204-A	2.3	2300	22G, 4mm	≥2.8
★ VDK-IN-23-230-2205-A	2.3	2300	22G, 5mm	≥2.8
VDK-IN-23-230-2206-A	2.3	2300	22G, 6mm	≥2.8
★ VDK-IN-23-230-2303-A	2.3	2300	23G, 3mm	≥2.8
★ VDK-IN-23-230-2304-A	2.3	2300	23G, 4mm	≥2.8
★ VDK-IN-23-230-2305-A	2.3	2300	23G, 5mm	≥2.8
VDK-IN-23-230-2306-A	2.3	2300	23G, 6mm	≥2.8
★ VDK-IN-23-230-2503-A	2.3	2300	25G, 3mm	≥2.8
★ VDK-IN-23-230-2504-A	2.3	2300	25G, 4mm	≥2.8
★ VDK-IN-23-230-2505-A	2.3	2300	25G, 5mm	≥2.8
★ VDK-IN-23-230-2506-A	2.3	2300	25G, 6mm	≥2.8

★ Common specifications

Disposable Non-electric Biopsy Forceps

- Biopsy
- Polyp Retrieval

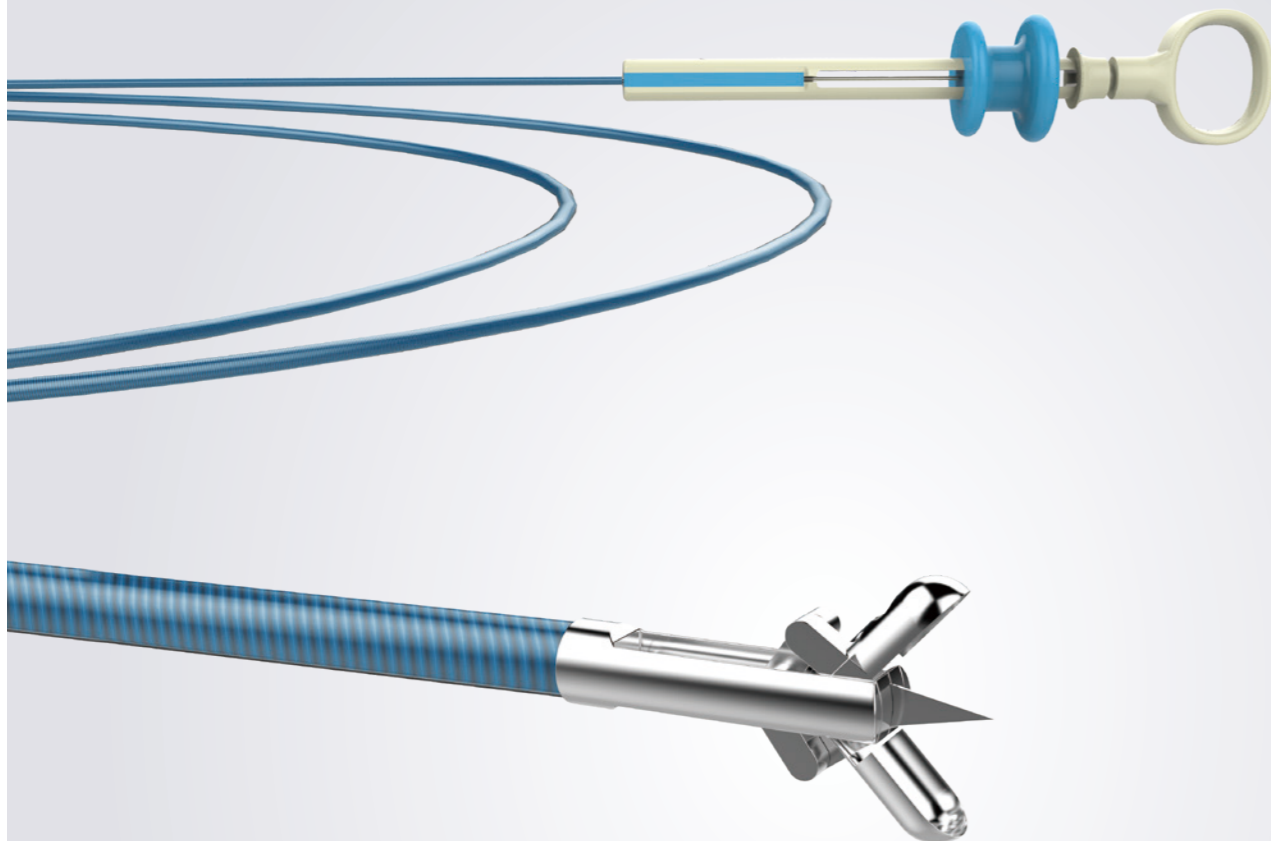

**STRONG BITE FORCE,
EASILY GRASP THE MUCOSAL TISSUE
WITH NO RISKS OF TEARING AND BLEEDING**

Usage

- It is used for tissue sampling from alimentary tract or respiratory tract in the combined use of endoscope.

Features

- Special sharpness treatment on cups, easier to sample.
- Innovational 4-bar linkage design, offering an excellent rigidity.
- Tiny interval between jaws, large occlusal force and outstanding fitness.
- Smooth jaws, effectively decrease the friction to working channel.
- Standard cups design with proper sampling capacity, small tissue harm.


Specifications

Model	O.D. (mm)	Length (mm)	Endoscope Channel (mm)	Characteristics
★ VDK-FB-18-105-O-P-B1	1.8	1050	≥ 2.0	without spike, uncoated
VDK-FB-18-105-W-O-B1	1.8	1050	≥ 2.0	with spike, uncoated
VDK-FB-18-160-O-O-B1	1.8	1600	≥ 2.0	without spike, uncoated
VDK-FB-18-160-W-O-B1	1.8	1600	≥ 2.0	with spike, uncoated
VDK-FB-23-160-O-O-B1	2.3	1600	≥ 2.8	without spike, uncoated
VDK-FB-23-180-W-O-B1	2.3	1800	≥ 2.8	with spike, uncoated
VDK-FB-23-200-O-O-B1	2.3	2000	≥ 2.8	without spike, uncoated
VDK-FB-23-200-W-O-B1	2.3	2000	≥ 2.8	with spike, uncoated
★ VDK-FB-23-230-O-O-B1	2.3	2300	≥ 2.8	without spike, uncoated
★ VDK-FB-23-180-O-O-B1	1.8	2300	≥ 2.0	with spike, uncoated
★ VDK-FB-18-160-O-P-B1	1.8	1600	≥ 2.0	without spike, coated
VDK-FB-18-160-W-P-B1	1.8	1600	≥ 2.0	with spike, coated
★ VDK-FB-23-160-O-P-B1	2.3	1600	≥ 2.8	without spike, coated
★ VDK-FB-23-160-W-P-B1	2.3	1600	≥ 2.8	with spike, coated
VDK-FB-23-180-O-P-B1	2.3	1800	≥ 2.8	without spike, coated
★ VDK-FB-23-180-W-P-B1	2.3	1800	≥ 2.8	with spike, coated
★ VDK-FB-23-230-O-P-B1	2.3	2300	≥ 2.8	without spike, coated
★ VDK-FB-23-230-W-P-B1	2.3	2300	≥ 2.8	with spike, coated
VDK-FB-18-105-O-O-A1	1.8	1050	≥ 2.0	without spike, uncoated, with alligator teeth
VDK-FB-18-105-O-P-A1	1.8	1050	≥ 2.0	without spike, coated, with alligator teeth
VDK-FB-23-160-O-O-A1	2.3	1600	≥ 2.8	without spike, uncoated, with alligator teeth
VDK-FB-23-160-O-P-A1	2.3	1600	≥ 2.8	without spike, coated, with alligator teeth
VDK-FB-23-160-W-O-A1	2.3	1600	≥ 2.8	with spike, uncoated, with alligator teeth
VDK-FB-23-180-O-O-A1	2.3	1800	≥ 2.8	without spike, uncoated, with alligator teeth
★ VDK-FB-23-180-O-P-A1	2.3	1800	≥ 2.8	without spike, coated, with alligator teeth
VDK-FB-23-180-W-P-A1	2.3	1800	≥ 2.8	with spike, coated, with alligator teeth
VDK-FB-23-200-O-O-A1	2.3	2000	≥ 2.8	without spike, uncoated, with alligator teeth
VDK-FB-23-200-O-P-A1	2.3	2000	≥ 2.8	without spike, coated, with alligator teeth
VDK-FB-23-200-W-P-A1	2.3	2000	≥ 2.8	with spike, coated, with alligator teeth
★ VDK-FB-23-230-O-P1-A1	2.3	2300	≥ 2.8	without spike, uncoated, with alligator teeth
★ VDK-FB-23-230-O-P-A1	2.3	2300	≥ 2.8	without spike, coated, with alligator teeth
★ VDK-FB-23-230-W-P-A1	2.3	2300	≥ 2.8	with spike, coated, with alligator teeth
★ VDK-FB-23-230-W-P1-A1	2.3	2300	≥ 2.8	with spike, plastic screen printing scale
★ VDK-FB-23-180-W-P1-A1	2.3	1800	≥ 2.8	with spike, plastic screen printing scale
VDK-FB-23-160-O-P1-B1	2.3	1600	≥ 2.8	without spike, plastic screen printing scale
★ VDK-FB-23-180-W-P1-B1	2.3	1800	≥ 2.8	with spike, plastic screen printing scale
★ VDK-FB-23-230-O-P1-B1	2.3	2300	≥ 2.8	without spike plastic screen printing scale
★ VDK-FB-23-230-W-P1-B1	2.3	2300	≥ 2.8	with spike ,plastic screen printing scale
★ VDK-FB-23-230-W-O-B1	2.3	2300	≥ 2.8	with spike, uncoated

★ Common specifications

| Disposable 1.0 Non-electric Biopsy Forceps

Biopsy

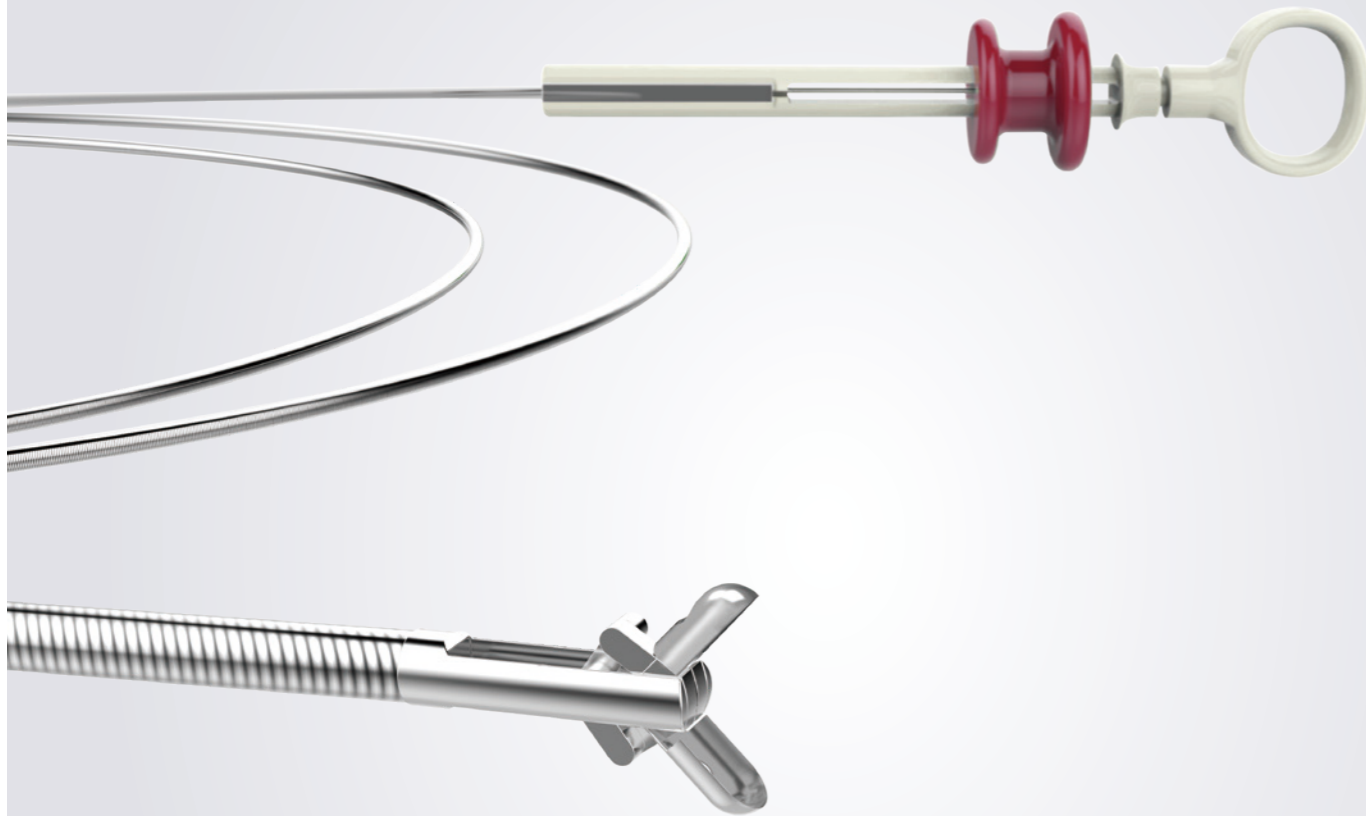

Φ1.0MM

Usage

- Tissue sampling from alimentary tract or respiratory tract in the combined use of endoscope.

Features

- Smooth insertion into working channel .
- Metal coil sheath resistant to kinking.
- Maximun 1.0mm diameter insertion portion .


Maximun 1.0mm diameter insertion portion .

Specifications

Model	O.D. (mm)	Working Length(mm)	Working Channel(mm)	Characteristics
VDK-MFB-80-B1	1.0	800	≥ 1.2	without spike, uncoated
VDK-MFB-120-B1	1.0	1200	≥ 1.2	without spike, uncoated
VDK-MFB-180-B1	1.0	1800	≥ 1.2	without spike, uncoated
VDK-MFB-230-B1	1.0	2300	≥ 1.2	without spike, uncoated
VDK-MFB-260-B1	1.0	2600	≥ 1.2	without spike, uncoated
VDK-MFB-290-B1	1.0	2900	≥ 1.2	without spike, uncoated

Disposable Non-electric Jumbo Biopsy Forceps

- Biopsy
- Polyp Retrieval

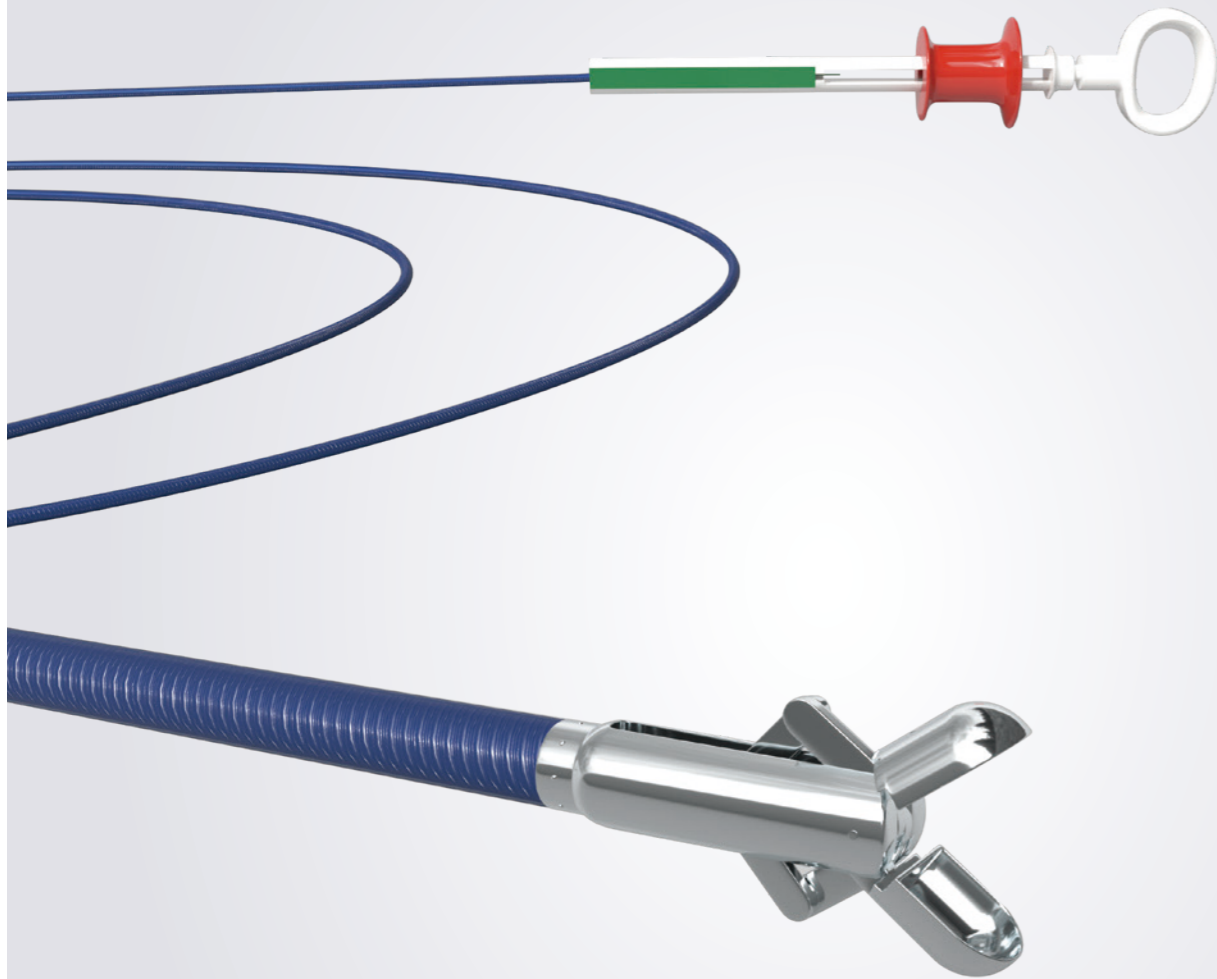

Φ3.0MM

Usage

- Tissue sampling in digestive tracts.

Features

- Obtain more adequate biopsy specimens with superior quality.
- Yield better diagnostic accuracy with less tissue acquisition.
- Remove small, sessile colorectal polyps efficiently.


Specifications

Model	O.D. (mm)	Length(mm)	Working Channel(mm)	Characteristics
VDK-FB-30-180-O-O-B1	3.0	1800	≥3.2	without spike, uncoated
VDK-FB-30-180-O-P-B1	3.0	2300	≥3.2	without spike, coated
VDK-FB-30-230-O-O-B1	3.0	2300	≥3.2	without spike, uncoated
VDK-FB-30-230-O-P-B1	3.0	2300	≥3.2	without spike, coated
VDK-FB-30-180-O-P1-B1	3.0	1800	≥3.2	without spike, coated with mark
★ VDK-FB-30-230-O-P1-B1	3.0	2300	≥3.2	without spike, coated with mark
VDK-FB-30-180-W-P1-B1	3.0	1800	≥3.2	with spike, coated with mark
★ VDK-FB-30-230-W-P1-B1	3.0	2300	≥3.2	with spike, coated with mark
VDK-FB-30-180-W-O-B1	3.0	1800	≥3.2	with spike, uncoated
VDK-FB-30-230-W-O-B1	3.0	2300	≥3.2	with spike, uncoated
VDK-FB-30-180-W-P-B1	3.0	1800	≥3.2	with spike, uncoated
VDK-FB-30-230-W-P-B1	3.0	2300	≥3.2	with spike, uncoated

★ Common specifications

| Disposable Hot Biopsy Forceps

- ☑ ESD
- ☑ Hemostasis
- ☑ Polyp Retrieval

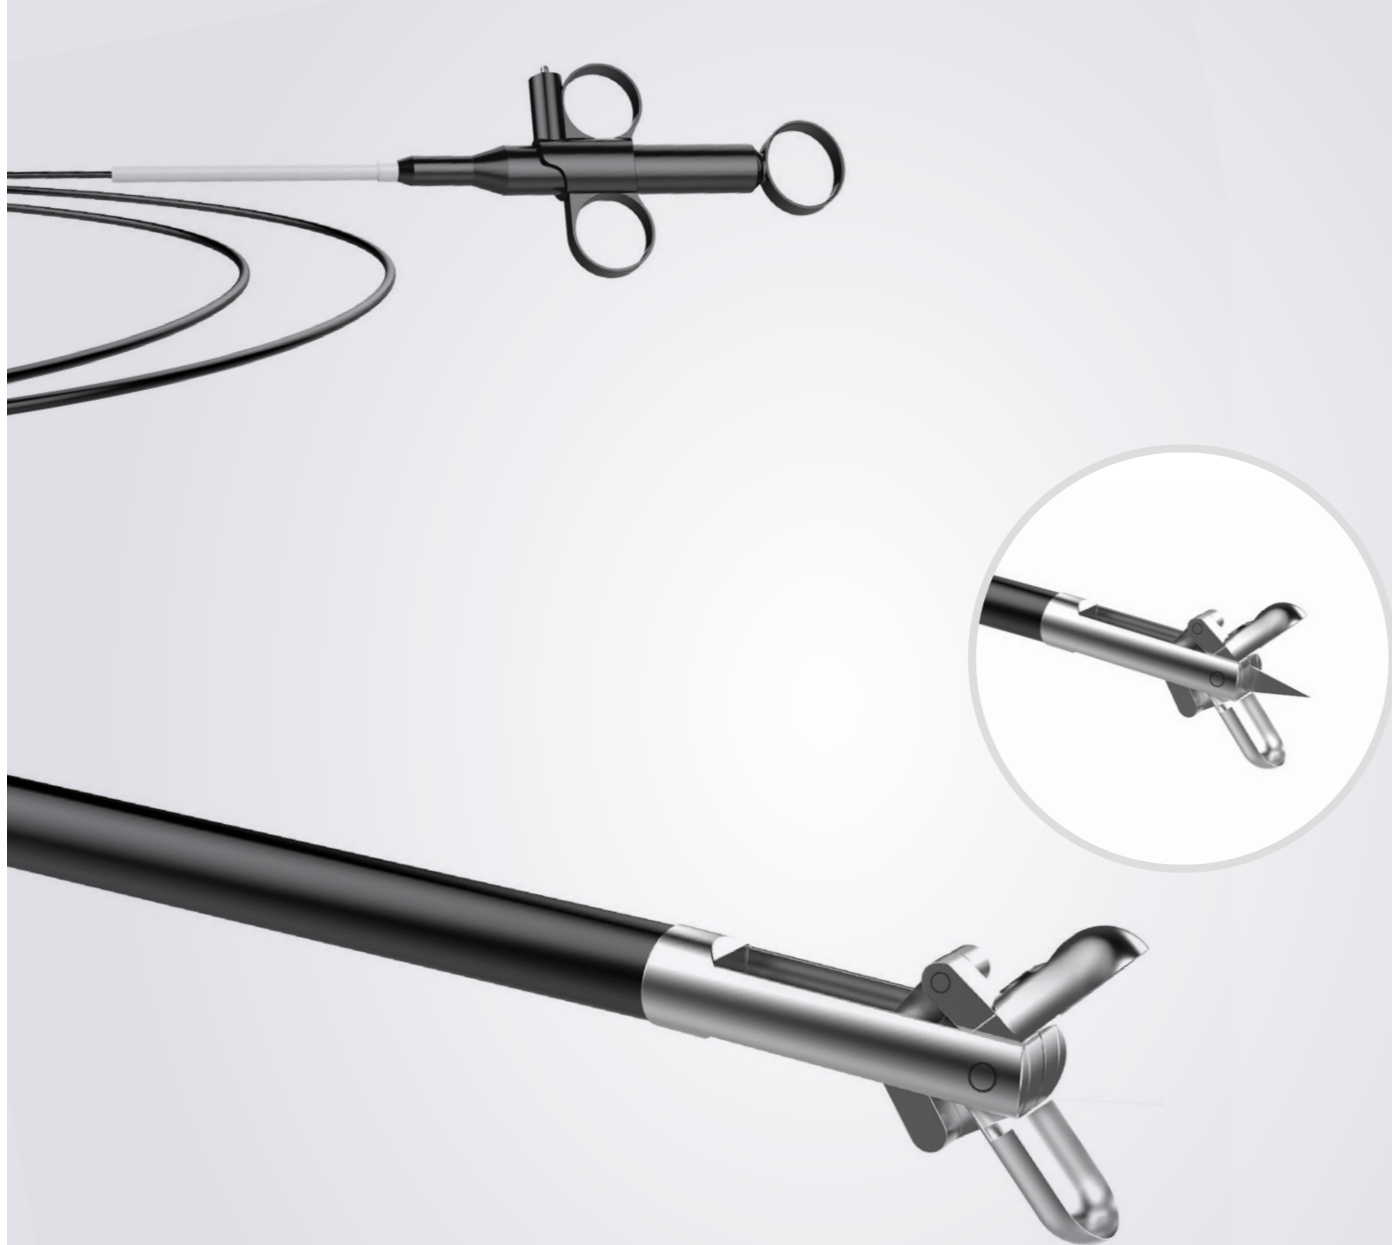

Usage

- The product should be equipped with high-frequency instrument, mainly intend to conduct electricity burning,coagulationand hemostasis.

Features

- Easy and comfortable to use.
- With smooth tube, easy to pass through the endoscope channel.
- With puncture-proof insulation, high safety.

Specifications

Model	O.D. (mm)	Length (mm)	Endoscope Channel (mm)	Characteristics
VDK-FD-23-160-A	2.3	1600	≥2.8	Without spike
VDK-FD-23-180-A	2.3	1800	≥2.8	
★ VDK-FD-23-230-A	2.3	2300	≥2.8	
VDK-FD-23-260-A	2.3	2600	≥2.8	
VDK-FD-23-160-A1	2.3	1600	≥2.8	With spike
VDK-FD-23-180-A1	2.3	1800	≥2.8	
★ VDK-FD-23-230-A1	2.3	2300	≥2.8	
VDK-FD-23-260-A1	2.3	2600	≥2.8	

★ Common specifications