



full face mask

full face mask




Silicone
Head Support



Adjustable polycarbonate
head support



Double Frame
Silicone Body

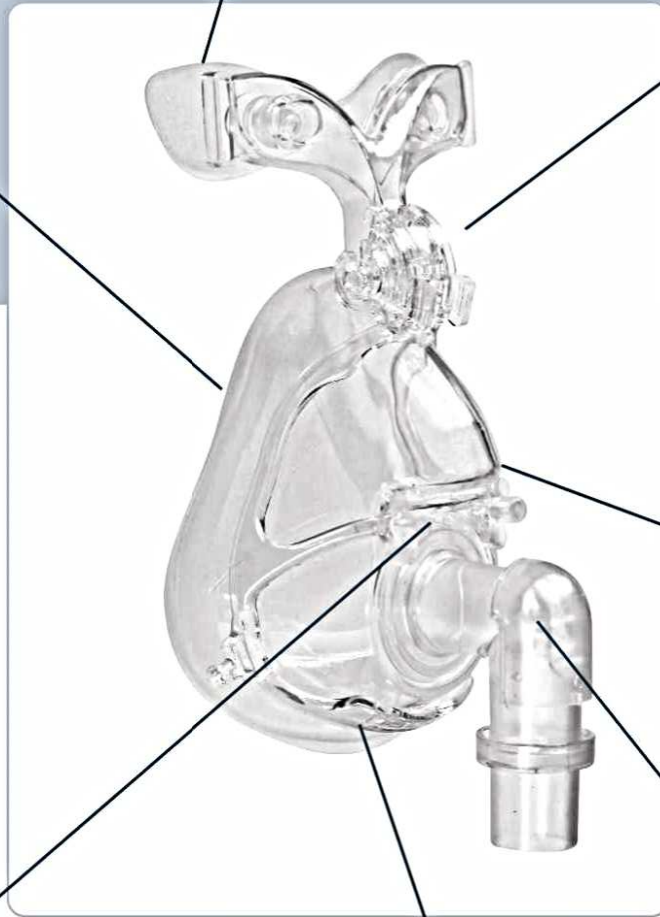

Breatheable Foam
Headgear



Reinforced
Polycarbonate Frame



Oxygen and
Pressure Port



Exhalation Port



Nonvented Elbow
Connector for noninvasive
ventilator usage

full face mask


Raw Material

Features

Design

Usage

Available Sizes

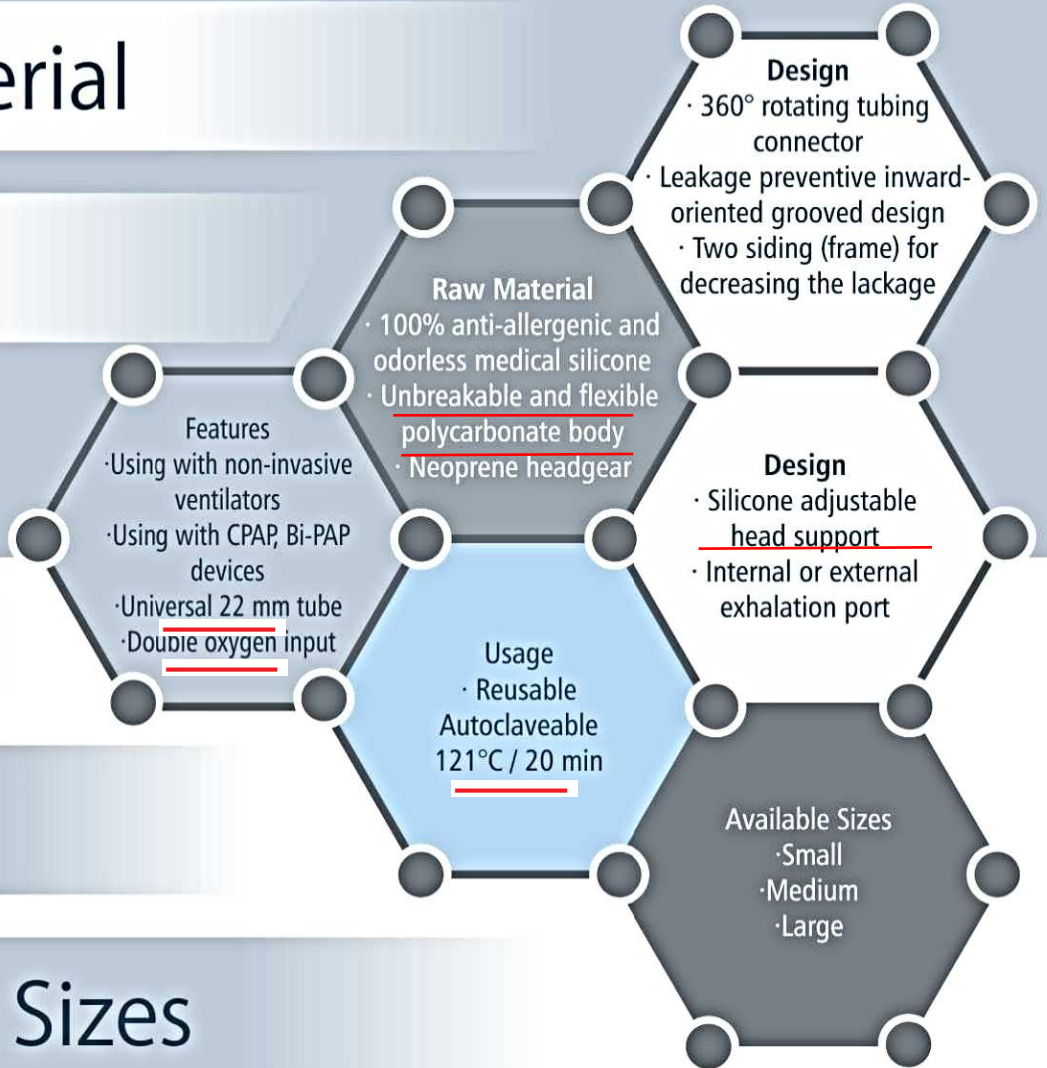

Available Sizes (Small, Medium, Large)

- | | |
|-------------------------|--|
| 1. SemiVent (item no): | #7600040-S
#7600040-M
#7600040-L |
| 2. NonVented (item no): | #7600041-S
#7600041-M
#7600041-L |
| 3. Vented (item no): | #7600042-S
#7600042-M
#7600042-L |

full face mask



Cleaning the Mask at Home:

- Clean the Silicone masks and head gears before first use and daily with a mild dishwashing detergent.
- The headgear does not need to be removed for daily cleaning of the masks.
- Hand wash in warm water with a mild dishwashing detergent.
- All components should be rinsed well with drinking quality water and allowed to air dry out of direct sunlight.
- Replace any parts of your mask that have visibly deteriorated as cracking, crazing, tears, etc.



For Multi-patient use in the Hospital:

- Use mask autoclaving (121°C and 20 min.) or disinfection liquids instructions to reprocess the mask between patients.



- If oxygen is used with device, the oxygen flow must be turned off when the device is not operating. Otherwise, Oxygen accumulated in the device enclosure will create a risk of fire.



- Discontinue using mask if you have any adverse reaction, and consult your physician or sleep therapist.
- Clean the Full mask before first use and daily.
- Inspect all parts for damage or wear and replace any parts that have visibly deteriorated as cracking, crazing, tears, etc.



- The Full face mask and headgear should fit comfortably and the Full mask should not dig into your skin. Verify that the Full mask and headgear are the correct size.
- Do not use the masks, If you are using a pill that potentially causes vomiting



Full silicone fullface mask is designed for use the patients for whom prescribed the CPAP, Bi-PAP, Auto-PAP or VPAP therapy by a health care professional or respiratory therapist. Full silicone full face mask is used with the CPAP, Bi-PAP, Auto-PAP or VPAP therapy devices for single patient use in the home or multi-patient use in the hospital or a health center.



Warnings

Shelf life: 5 (five) years.

Storage temperature: - 20 °C + 60 °C

full face mask



- At low PAP pressures the flow through the exhalation port may not be poured out completely and rebreathing may occur.



full face

KNGMED
»KNG-ilkelerin adresi«→



Tel : +90 232 833 42 62

Fax: +90 232 833 42 63

info@kngmed.com

kng.info@yahoo.com

10001 Sokak No.28 / A - 10


Çınar Sanayi Sitesi

Ulukent / Menemen / İzmir / TÜRKİYE

Technical Data Sheet of Ora-Nasal Masks

Thearpy Pressure-Exhaust Flow Rate:

Mask	REF	Exhaust Rate				
		Pressure				
		3cmH ₂ O	10cmH ₂ O	20cmH ₂ O	30cmH ₂ O	40cmH ₂ O
KNGMED	#7600040	8,2	19	32	39	48
Ora-Nasal	#7600041					
Mask	#7600042					

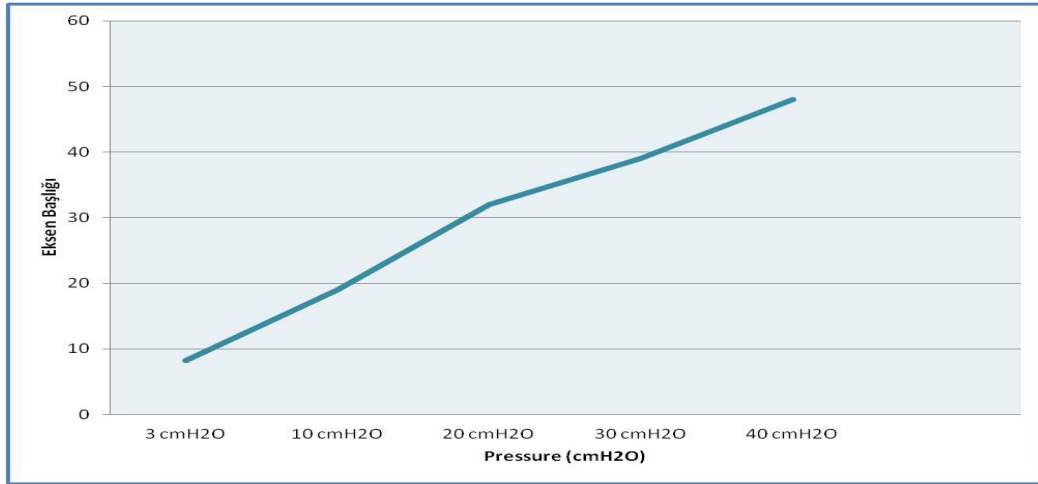


Pressure(cmH2O)

Pressure Drop:

Pressure Drop			
Mask	REF	Flow Rate	
		50L/Min	100L/Min
KNGMED Ora-Nasal Mask	#7600040	0.24	0.62
	#7600041		
	#7600042		


Pressure Drop Graphic

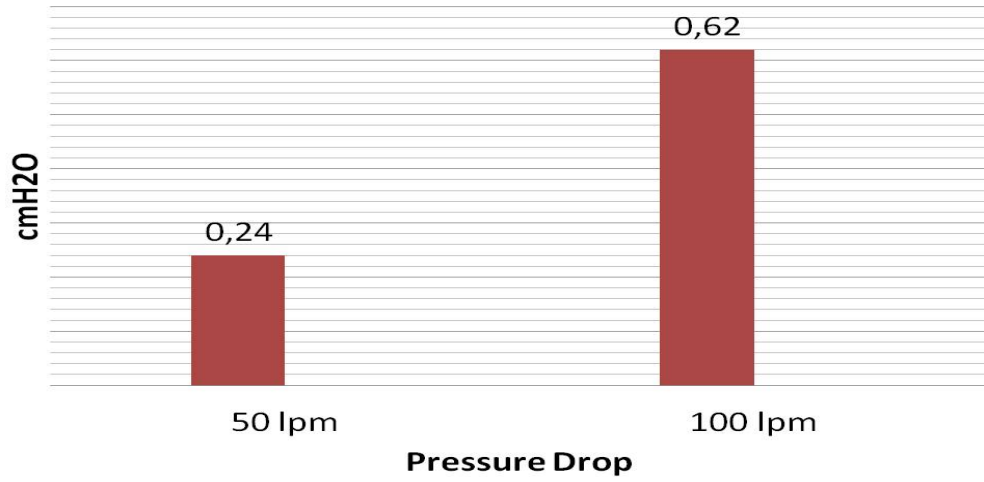

Anti Asphyxia Valve Activation/Deactivation Pressure:

AAV Pressure Activation/ Deactivation			
Mask	REF	Activation	Deactivation
Pressure*			
KNGMED	#7600040	1.73	0.88
Ora-Nasal Mask	#7600042		

*AAV Pressure Activation/ Deactivation
Graphic*

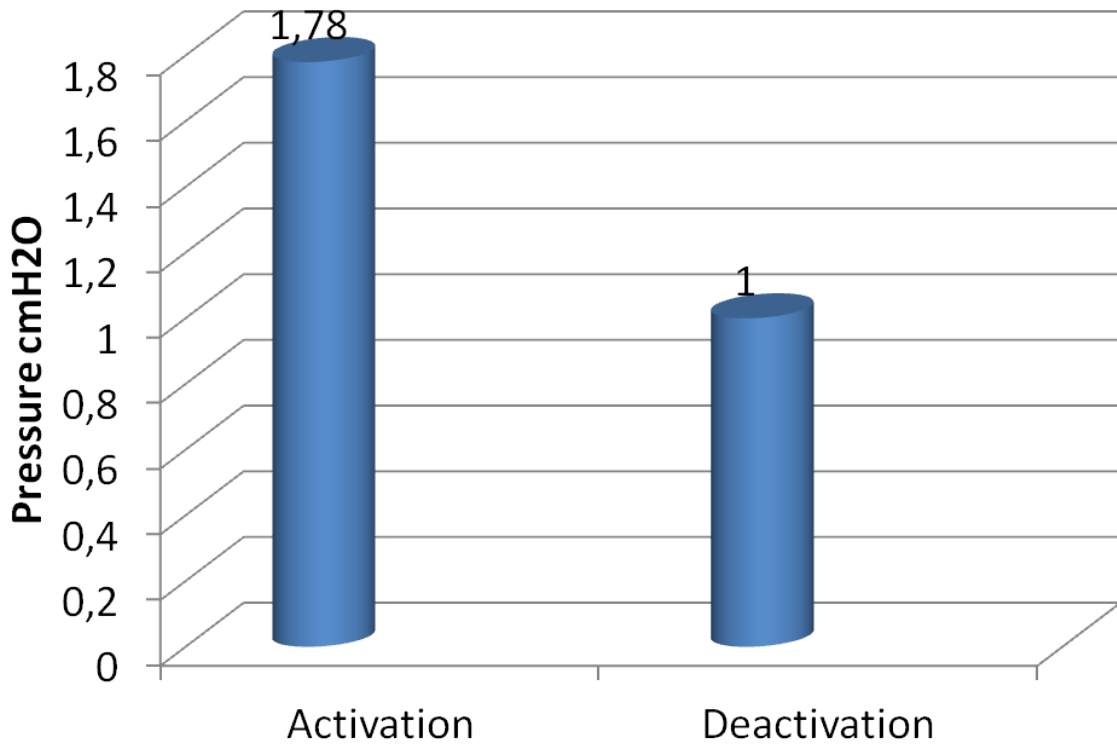

* Tested all pressures are below the minimum pressure rate of CPAP Therapy devices. (<3cmH2O).




Kngmed Medical Co Ltd.
29 Ekim Mah. 10007 Sk.
No:26/B
Menemen/Izmir/Turkey

Specification of Fullface Masks

Kngmed FullFace Masks



7600041

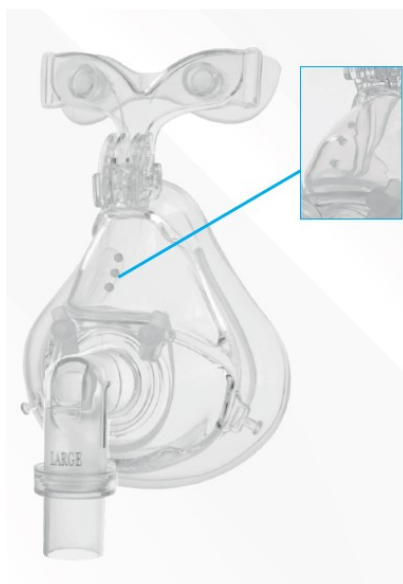

7600042



7600040

Product Number	
Mask	REF
KNGMED Fullface Mask Standard Elbow	#7600041
KNGMED Fullface Mask EE Elbow	#7600040
KNGMED Fullface Mask EE Elbow with Exhalation	#7600042

Available Sizes	Small, Medium, Large
-----------------	----------------------

Intended Use	FullFace Mask is intended to provide an interface for application of CPAP or bi-level or ventilation therapy to patients. This mask is for single patient use in the home or multi-patient use in the hospital/institutional environment. The standard elbow (SE) does not have any exhalation port. If the SE elbow is used, it is necessary a separated exhalation port.
--------------	---

Dead Space	Small: 125 ml, Medium: 151 ml, Large:169 ml,
Material List	Face plate: Polycarbonate Cushion: Medical Grade silicone Port Cap: Silicone Elbows: Polycarbonate Elbow Split: Polycarbonate Headgear Clips: Polycarbonate Headgear: UBL/Foam/Spandex
Production	LSR Injection
Manufacturer	Kngmed Medical / Made in Turkey
Instruction for Use	Labeling present on each mask
Standards	EN ISO 14971 EN ISO 17510-2 TS EN 10993-1 EN ISO 13485 Med. Dev. 93/42/EEC



Kngmed Medical Co Ltd.
29 Ekim Mah. 10007 Sk.
No:26/B
Menemen/Izmir/Turkey