





**WUHU RUIJIN MEDICAL INSTRUMENT  
& DEVICE CO.,LTD**

Address/Tel/Fax: No.33, EastWanchun Road, Wuhu Economic  
& Technology Development Zone, Wuhu Anhui China;

Tel: 86-553-2672511 Fax: 86-553-2672510

Cellphone: +86 13675533452

Website: [www.whruijin.com](http://www.whruijin.com)



***Medical electric drill -  
canulate drill RJ-PD (ND-2511) :***

***Holds K-wires or be used in  
intramedullary interlocking nail surgery  
or arthroscopic surgery.***

## » Feature

01 *Variable speed, convenient for use*

02 *Imported motor*

03 *High coaxiality, low noise*

04 *Can be autoclavable up to 135°C*



## Composition »

*One handpiece  
One charger  
Two batteries  
Two battery aseptc transfer rings  
One drill chuck key  
One instruction manual  
One Aluminum case*

» Main Technical Data

Hand Piece	Output Power	150W
	Unit rise in temperature	≤25℃
Charger	Input Voltage	AC 110-220V , 50-60Hz
Battery	Voltage	14.4V
	Battery capacity	3000mAh
	Battery feature	Lithium battery
	Charging time	Two hours
Non-loading speed	0-680/0-1000rpm	
Non-loading noise	≤65dB ( A )	
Axial run out	≤0.15mm	
Rated torque	5.5N.m/4N.m	
Impulsive torque	10.5N.m/8.5N.m	
Drill chuck clamping range	0.8-7.9mm	
Canulated diameter	≤4.2mm	

» Product details



» Accessories

Drill chuck & Key



Charger



Battery of 14. 4v




Aspetic battery transfer rings






*Aluminum case packing*

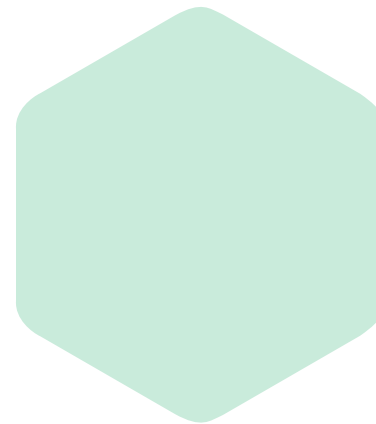

*Sterilization case is additional cost.*

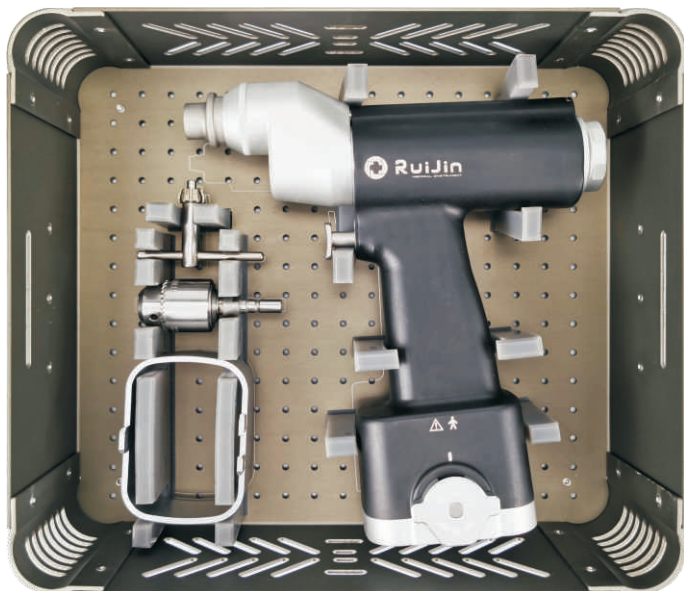

*Can connect various flexible reamer,  
k wire adapter and acetabular reamer,  
changable during the process of surgery.*

*Basic steps of sterilization, cleaning and  
maintenance of power tools.*

*1.Disaccessibly: All the consumable parts (saw blades, drill bits, etc) and battery should be  
removed before cleaning.*

*2.Cleaning: Please wash and rinse with flowing water. Note: use soft brush to clean, then  
wipe with soft dry cloth. All instruments are prohibited from soak cleaning.*

*3.Maintenance: Maintain by medical lubricant every time when cleaning and wiping instruments.  
Apply lubricant on every mobilizable part.*

*Note: Applying lubricant and rotate parts to lubricate to the full.*

*4.Assembly: Assembly and functional test. Note: After cleaning and applying lubricants,  
install all parts one by one and conduct function test and then check its intactness.*

*5.Sterilization: Forevacuum high temperature for 132 centigrade and high pressure within 20  
minutes; natural cooling time is more than 40 minutes. Expoxymethane and formaldehyde are  
prohibited. Instruments must be kept dry before sterilization*