


■ Setting AEC Radiography

You can configure the items for AEC (automatic exposure control) radiography.


Turning AEC ON/OFF and Setting Photo Pickup Field

- 1 Press the lower  icon on the touch panel.

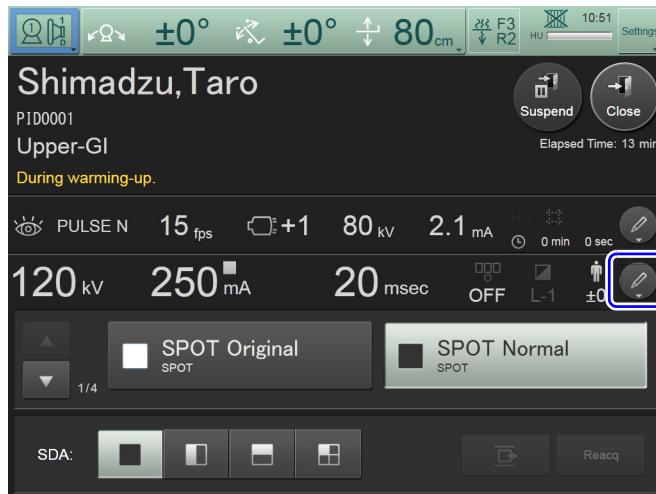


The [Radiography Condition Details] screen is displayed.

- 2 Press .

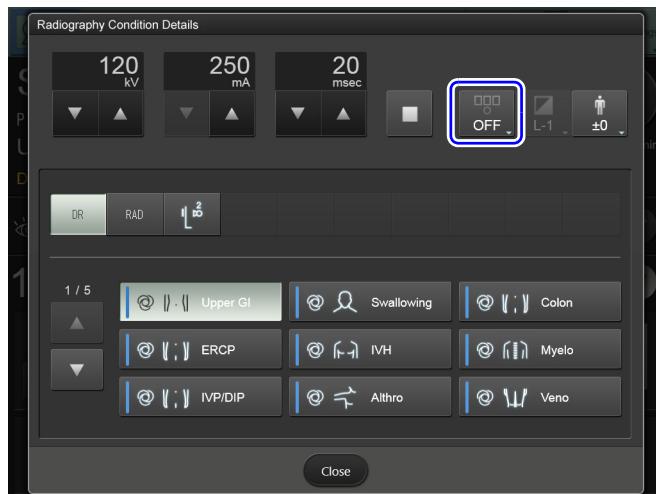

3 Select the photo pickup field you want to configure.

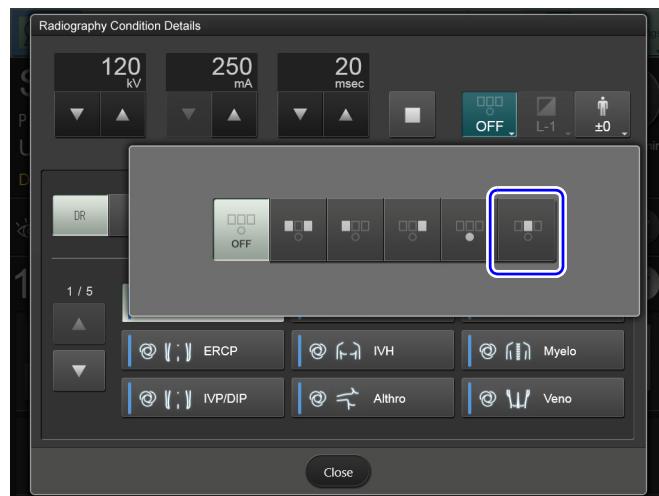

4

4 Press [Close] when the settings are completed.

The [Radiography Condition Details] screen closes.



Select the center photo pickup field of the phototimer () if the magnification size is 12" or less. X-ray may not be radiated in the upper photo pickup fields (, ,), stopping the AEC from operating normally. However, select the upper center photo pickup field () when selecting urology mode.

Reference "Operation in Urology Mode" P.4-61