





hybrid

Hydrophilic guidewire

Designed to facilitate the insertion of catheters into intracranial vascular branches for diagnostic or therapeutic use.



radiopaque coil tip available in multiple lengths

O.D. as small as

Optimized navigation

Trackability and pushability given by the stainless steel proximal part

Shape retention and suppleness thanks to the distal part in Nitinol

Smooth navigability nhanced by the hydrophilic coating

Visibility

ensured by the distal radiopaque coil tip



thanks to the double angle haped tip and broad options of "O.D. as small as .007"







HYBRIDOOZ & HYBRIDOO8D



HYBRID1214D



ordering information

Developed portfolio with unique references

	Reference	Distal O.D.	Length (cm)	Compatible with	Curve
Hybrid	HYBRID007D	.007" (0,18mm)	220	SONIC all references MAGIC all references BALTACCI all references & others*	Straight (D)
	HYBRID007J				Double Angle (J)
	HYBRID008D	.008" (0,20mm)	220	SONIC all references except 1.2F MAGIC all references except 1.2F BALTACCI all references except 1.2F & others*	Straight (D)
	HYBRID008J				Double Angle (J)
	HYBRID007D.120	.007" (0,18mm)	120	Shorter length	Straight (D)
	HYBRID1214D	.012" (0,30mm)	200	Any microcatheter compatible with .014" guidewire*	Straight (D)
	HYBRID1214DA				Double Angle (DA)
	HYBRID014D	.014" (0,35mm)	200	Any microcatheter compatible with .014" guidewire* COPERNIC RC	Straight (D)
	HYBRID10D300	.010" (0,25mm) .012" (0,30mm)	310	Exchange microguidewires	Straight (D)
	HYBRID12D300				

^{*}Check compatibility on products labelling

HYBRID are quickwires designed to bacilitate the insertion of cotheters into intracranial vascular branches for diagnostic or therapeutic use. Class III CEO277 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT Extrusion SAS. Carefully read the instructions for use before use. Not reimbursed. First E marking: 2010. SONIC are builded micro-combeters intended for selective and hyperselective vascular catheterization for diagnostic on therapeutic purposes. Class III CEO297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT Extrusion SAS. Carefully read the instructions for use before use. Not reimbursed. First E marking: 1998. MAGIC are micro-combeters intended for selective and hyperselective vascular catheterization for diagnostic and therapeutic purposes. Class III ECO297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT Extrusions for use before use. Not reimbursed. First E marking: 1998. MAGIC are micro-combeters intended for selective and hyperselective vascular catheterization for diagnostic and therapeutic purposes. Class III ECO297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT Extrusions Sc. Carefully read the instructions for use before use. Not reimbursed. First E marking: 1998. VASCO- are reinforced micro-combeters intended: for injection of diagnostic or therapeutic products; to position pushable coils: "SPRINAES" or deterbable coils especially the acuse of MDS s mechanical detachments systems » for the use first particular parts and the products of the prod

Balt

10, rue de la Croix Vigneron, 95 160 Montmorency, France

Tél.: +33 (0)1 39 89 46 41 Fax: +33 (0)1 34 17 03 46

fax : +33 (0) | 34 | / 0



Intended use

<u>Description</u>

HYBRID guidewires have a nitinol distal core & a proximal section made of stainless steel. The proximal shaft section is coated with polytetrafluoroethylene (PTFE).

HYDROSPEED treatment reduces the friction coefficient, which makes it easier to advance & withdraw the guidewire.

HYBRID guidewires are radio-opaque & sterilised with ethylene oxide.

Intended use

INTERNAL USE -CONFIDENTIAL

HYBRID guidewires are designed to facilitate the insertion of catheters into intracranial vascular branches for diagnostic or therapeutic use.

HYBRID Hydrophilic Guidewires

DNTRAINDICATIONS

III guide wise may be centre indicated depending on the physician profe
the device may decrease the patient health especially in those cases:
leocompatible vascular anatomy with the advancement of the guide wire.
This blood vessel.
Patient alargit; to Rickel
devices are correlated for reconstency, premature reconstens and infants

These devices are contransdicated for recordate, per A. POTENTIAL COMPLICATIONS
Patiental conficiations include to a law not invited to:
Vised or consumption perforation

- Vised or consumption perforation

- Hermitions at the site of entry

- Emodelies

- International at the site of entry

- Emodelies

- International at the site of entry

- International at the site of

- each procedure:

 Live fluorocopic systems to insert the guidewire and to avoid damaging blood vessels.
 Where possible, use a trequer attached to the proximal part of the guidewire to facilitate
 guidewire.

 Perfuse the cultivater through the side channel of a Y-valve connection to avoid thrombut
 Phorizor this guidewire abody once the goal that both reached.

The content of this document, in particular data, information, trademarks & logos is BALT SAS & affiliates' sole property. ©2018 BALT & affiliates, all rights reserved. Consequently, all representation &/or reproduction, whether in part or in full, is forbidden & would be considered a vidation of BALT SAS & affiliates' copyrights & other intellectual propertery rights. This document with associated pictures is non-contractual & is solely dedicated to BALT's distributors (BALT SAI shall exclusively be used in accordance with the instructions for use included in the bowes. The distribution, the sale & the use of BALT's products commercialized by BALT shall exclusively be used in accordance with the instructions for use included in the bowes. The distribution, the sale & the use of BALT's products is under distributor's liability.



Components Usage


The Hybrid guidewire packaging is including:

- · One Guidewire
- One Torquer is added in the peelable pouch with the HYBRID. This
 accessory improves the manipulation, the control & the handling of the
 device
- One needle (Introducer) is also added to enable the introduction in the Y adaptator

<u>Units per box</u>: \rightarrow 1/box

Shelf life: → 5 years



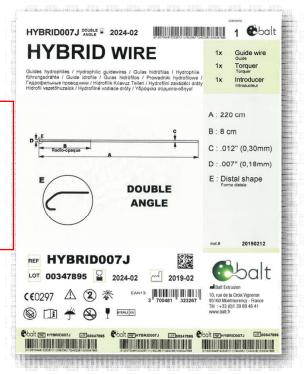

The content of this document, in particular data, information, trademarks & logos is BALT SAS & affiliates' sole property. ©2018 BALT & affiliates, all rights reserved. Consequently, all representation &/or reproduction, whether in part or in full, is forbidden & would be considered a violation of BALT SAS & affiliates' copyrights & other intellectual proprietary rights. This document with associated pictures is non-contractual & is solely dedicated to BALT's distributors (BALT's supplier's distributors), The products commercialized by BALT shall exclusively be used in accordance with the instructions for use included in the boxes. The distribution, the sale & the use of BALT's products is under distributor's ||ability.

INTERNAL USE -CONFIDENTIAL

