



HUACETONG

TEST REPORT

EN 149

**Respiratory protective devices - Filtering half masks to protect
against particles - Requirements, testing, marking**

Report Number.....: **WUX202003020438S**

Test by (name+signature).....: Sally Liu

Compiled by (+signature).....: Lucy Ni

Approved by (+signature).....: Tony Bi

Date of issue.....: Mar. 18, 2020

Total number of pages.....: 13 pages

Testing laboratory: Shenzhen Huacetong Testing and certification Co., Ltd.

Address: Building B, Xinbaosheng, No.233, Xixiang Street, Bao'an District,
Shenzhen, China

Testing location: As above

Applicant's name.....: Fujian xinjiu'an Medical Technology Co., Ltd

Address.....: Third floor, workshop 224, Jincheng Road, printing base,
Cizao Town, Jinjiang City, Quanzhou City, Fujian Province

Test specification:

Standard.....: EN 149:2001+A1:2009

Test procedure.....: N/A

Non-standard test method.....: N/A

Test Report Form No.....: EN 149

Test Report Form(s) Originator.....: Huacetong

Master TRF.....: N/A

Test item description.....: Disposable protective mask

Trade Mark.....: 倍力天

BARLETAY

Manufacturer.....: Fujian xinjiu'an Medical Technology Co., Ltd

Model/Type reference.....: Plane lug type B

| | |
|---|---|
| Summary of testing: | |
| <p>Tests performed (name of test and test clause):</p> <p>- EN 149:2001+A1:2009</p> <p>The submitted samples were found to comply with the requirements of above specification.</p> | <p>Testing location:</p> <p>Shenzhen Huacetong Testing and certification Co., Ltd.</p> <p>Building B, Xinbaosheng, No.233, Xixiang Street, Bao'an District, Shenzhen, China</p> |

| | | | | |
|---|--|----------------|------|-------------------|
| Summary of testing: | | | | |
| Tests performed (name of test and test clause): | | | | Testing location: |
| EN 149 | | | | |
| 7.2 | Nominal values and tolerances | Applicable | Pass | 1) |
| 7.3 | Visual inspection | Applicable | Pass | 1) |
| 7.4 | Packaging | Applicable | Pass | 1) |
| 7.5 | Material | Applicable | Pass | 1) |
| 7.6 | Cleaning and disinfecting | Non-Applicable | N/A | 1) |
| 7.7 | Practical performance | Applicable | Pass | 1) |
| 7.8 | Finish of parts | Applicable | Pass | 1) |
| 7.9 | Leakage | Applicable | Pass | 1) |
| 7.10 | Compatibility with skin | Applicable | Pass | 1) |
| 7.11 | Flammability | Applicable | Pass | 1) |
| 7.12 | Carbon dioxide content of the inhalation air | Applicable | Pass | 1) |
| 7.13 | Head harness | Applicable | Pass | 1) |
| 7.14 | Field of vision | Applicable | Pass | 1) |
| 7.15 | Exhalation valve(s) | Applicable | Pass | 1) |
| 7.16 | Breathing resistance | Applicable | Pass | 1) |
| 7.17 | Clogging | Non-Applicable | N/A | 1) |
| 7.18 | Demountable parts | Non-Applicable | N/A | 1) |

| | |
|---|--------------------------------|
| Test item particulars.....: | |
| Temperature.....: | 20°C |
| Relative humidity.....: | 40-50% |
| Atmospheric pressure.....: | (9.0±0.2)kPa |
| Mass of the equipment (kg).....: | See instruction |
| Possible test case verdicts: | |
| - test case does not apply to the test object.....: | N/A |
| - test object does meet the requirement.....: | P (Pass) |
| - test object does not meet the requirement.....: | F (Fail) |
| Testing.....: | |
| Date of receipt of test item.....: | Mar. 02, 2020 |
| Date (s) of performance of tests.....: | Mar. 02, 2020 to Mar. 18, 2020 |

General remarks:

The test results presented in this report relate only to the object tested.

This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.

"(See Enclosure #)" refers to additional information appended to the report.

"(See appended table)" refers to a table appended to the report.

Throughout this report a ☒ comma / ☐ point is used as the decimal separator.

Clause numbers between brackets refer to clauses in report

Attachment No. 1: 1 pages of photo.

General product information:

The product is Disposable protective mask, without valve, Non-reusable.

| EN149 | | | |
|------------------|---|---------------------------------|---------------|
| Clause(s) | Test(s) | Test Remarks | Result |
| 4 | Description | | P |
| | A particle filtering half mask covers the nose and mouth and the chin and may have inhalation and/or exhalation valve. | Without valve | P |
| 5 | Classification | | P |
| | FFP1, FFP2 and FFP3 | FFP2 | P |
| 6 | Designation | | P |
| 7 | Requirements | | N/A |
| 7.1 | General | | P |
| | In all tests all test samples shall meet the requirements. | | P |
| 7.2 | Nominal values and tolerances | 25°C | P |
| 7.4 | Packaging | | P |
| | Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use. | Closed plastic bag | P |
| 7.5 | Material | See 8.3.1, 8.3.2, 8.2 | P |
| 7.6 | Cleaning and disinfecting | | N/A |
| 7.7 | Practical performance | | P |
| | The particle filtering half mask shall undergo practical performance tests under realistic conditions. | | P |
| 7.8 | Finish of parts | No sharp edges or burrs on mask | P |
| 7.9 | Leakage | | P |
| | the particle filtering half mask can be used by the wearer to protect with high probability against the potential hazard to be expected. | | P |
| | For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than | | P |


| | | | | | | | | | | | | | | | | | |
|----------------|---|---|-------------------------------------|--|--|---|------|----|----|------|---|---|------|---|---|--|--|
| | 25 % for FFP1 11 % for FFP2 5 % for FFP3 | 9.1% | P | | | | | | | | | | | | | | |
| | at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than | | P | | | | | | | | | | | | | | |
| | 22 % for FFP1 8 % for FFP2 2 % for FFP3 | 7.3% | P | | | | | | | | | | | | | | |
| 7.9.2 | Penetration of filter material | | P | | | | | | | | | | | | | | |
| | Sodium chloride test, 95 l/min | 5.5%, Test 9 samples | P | | | | | | | | | | | | | | |
| | Paraffin oil test 95 l/min | 5.1%, Test 9 samples | P | | | | | | | | | | | | | | |
| | <table><tr><td rowspan="2">Classification</td><td colspan="2">Maximum penetration of test aerosol</td></tr><tr><td>Sodium chloride test 95 l/min % max.</td><td>Paraffin oil test 95 l/min % max.</td></tr><tr><td>FFP1</td><td>20</td><td>20</td></tr><tr><td>FFP2</td><td>6</td><td>6</td></tr><tr><td>FFP3</td><td>1</td><td>1</td></tr></table> | Classification | Maximum penetration of test aerosol | | Sodium chloride test 95 l/min % max. | Paraffin oil test 95 l/min % max. | FFP1 | 20 | 20 | FFP2 | 6 | 6 | FFP3 | 1 | 1 | | |
| Classification | Maximum penetration of test aerosol | | | | | | | | | | | | | | | | |
| | Sodium chloride test 95 l/min % max. | Paraffin oil test 95 l/min % max. | | | | | | | | | | | | | | | |
| FFP1 | 20 | 20 | | | | | | | | | | | | | | | |
| FFP2 | 6 | 6 | | | | | | | | | | | | | | | |
| FFP3 | 1 | 1 | | | | | | | | | | | | | | | |
| 7.10 | Compatibility with skin | | P | | | | | | | | | | | | | | |
| | Materials that may come into contact with the wearer's skin shall not be known to be likely to cause irritation or any other adverse effect to health. | | P | | | | | | | | | | | | | | |
| 7.11 | Flammability | | P | | | | | | | | | | | | | | |
| | The material used shall not present a danger for the wearer and shall not be of highly flammable nature. When tested, the particle filtering half mask shall not burn or not to continue to burn for more than 5 s after removal from the flame. | <4.0s | P | | | | | | | | | | | | | | |
| 7.12 | Carbon dioxide content of the inhalation air | | P | | | | | | | | | | | | | | |
| | The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume). | <0.69% | P | | | | | | | | | | | | | | |
| 7.13 | Head harness | | P | | | | | | | | | | | | | | |
| | The head harness shall be designed so that the particle filtering half mask can be donned and removed easily. | Removed easily and donned, self-adjusting. Elastic rope fixing | P | | | | | | | | | | | | | | |
| 7.14 | Field of vision | | P | | | | | | | | | | | | | | |
| | The field of vision is acceptable if determined so in practical performance tests. | Does not affect line of sight | P | | | | | | | | | | | | | | |
| 7.15 | Exhalation valve(s) | | N/A | | | | | | | | | | | | | | |
| | A particle filtering half mask may have one or more exhalation valve(s), which shall function correctly in all orientations. | No exhalation valve | N/A | | | | | | | | | | | | | | |

| | an exhalation valve is provided it shall be protected against or be resistant to dirt and mechanical damage and may be shrouded or may include any other device | >300 l/min Tensile force 10N, 10s No damaged, Function no change. | N/A | | | | | | | | | | | | | | | | | | | | | | |
|----------------|---|--|-------------------------------------|--|--|------------|--|------------|----------|----------|-----------|------|-----|-----|-----|------|-----|-----|-----|------|-----|-----|-----|--|----|
| 7.16 | Breathing resistance | | P | | | | | | | | | | | | | | | | | | | | | | |
| | The breathing resistances apply to valved and valveless particle filtering half masks and shall meet the requirements | | P | | | | | | | | | | | | | | | | | | | | | | |
| | inhalation | | P | | | | | | | | | | | | | | | | | | | | | | |
| | 30 l/min | 0,64 | P | | | | | | | | | | | | | | | | | | | | | | |
| | 95 l/min | 1.77 | P | | | | | | | | | | | | | | | | | | | | | | |
| | exhalation | | P | | | | | | | | | | | | | | | | | | | | | | |
| | 160 l/min | 2.46 | P | | | | | | | | | | | | | | | | | | | | | | |
| | <table border="1"> <thead> <tr> <th rowspan="3">Classification</th><th colspan="3">Maximum permitted resistance (mbar)</th></tr> <tr> <th colspan="2">inhalation</th><th>exhalation</th></tr> <tr> <th>30 l/min</th><th>95 l/min</th><th>160 l/min</th></tr> </thead> <tbody> <tr> <td>FFP1</td><td>0,6</td><td>2,1</td><td>3,0</td></tr> <tr> <td>FFP2</td><td>0,7</td><td>2,4</td><td>3,0</td></tr> <tr> <td>FFP3</td><td>1,0</td><td>3,0</td><td>3,0</td></tr> </tbody> </table> | Classification | Maximum permitted resistance (mbar) | | | inhalation | | exhalation | 30 l/min | 95 l/min | 160 l/min | FFP1 | 0,6 | 2,1 | 3,0 | FFP2 | 0,7 | 2,4 | 3,0 | FFP3 | 1,0 | 3,0 | 3,0 | | -- |
| Classification | Maximum permitted resistance (mbar) | | | | | | | | | | | | | | | | | | | | | | | | |
| | inhalation | | exhalation | | | | | | | | | | | | | | | | | | | | | | |
| | 30 l/min | 95 l/min | 160 l/min | | | | | | | | | | | | | | | | | | | | | | |
| FFP1 | 0,6 | 2,1 | 3,0 | | | | | | | | | | | | | | | | | | | | | | |
| FFP2 | 0,7 | 2,4 | 3,0 | | | | | | | | | | | | | | | | | | | | | | |
| FFP3 | 1,0 | 3,0 | 3,0 | | | | | | | | | | | | | | | | | | | | | | |
| 7.17 | Clogging | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| 7.17.1 | General | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | For single shift use devices, the clogging test is an optional test. For re-usable devices the test is mandatory | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | Devices designed to be resistant to clogging, shown by a slow increase of breathing resistance when loaded with dust | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | The specified breathing resistances shall not be exceeded before the required dust load of 833 mg · h/m³ is reached. | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| 7.17.2 | Breathing resistance | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| 7.17.2.1 | Valved particle filtering half masks | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | FFP1: 4 mbar | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | FFP2: 5 mbar | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | FFP3: 7 mbar | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | at 95 l/min continuous flow | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | The exhalation resistance shall not exceed 3 mbar at 160 l/min continuous flow. | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| 7.17.2.2 | Valveless particle filtering half masks | | N/A | | | | | | | | | | | | | | | | | | | | | | |
| | After clogging the inhalation and exhalation resistances shall not exceed | | N/A | | | | | | | | | | | | | | | | | | | | | | |

| | | | |
|--------|--|--|-----|
| | FFP1: 3 mbar | | N/A |
| | FFP2: 4 mbar | | N/A |
| | FFP3: 5 mbar | | N/A |
| | at 95 l/min continuous flow. | | N/A |
| 7.17.3 | Penetration of filter material | | N/A |
| | All types (valved and valveless) of particle filtering half masks claimed to meet the clogging requirement | | N/A |
| 7.18 | Demountable parts | No demountable parts | N/A |
| | All demountable parts (if fitted) shall be readily connected and secured, where possible by hand. | | N/A |
| 8 | Testing | | P |
| 8.1 | General | | P |
| 8.2 | Visual inspection | | P |
| 8.3.1 | Simulated wearing treatment | Saturated at $(37 \pm 2) ^\circ\text{C}$ | P |
| 8.3.2 | Temperature conditioning | | P |
| | Expose the particle filtering half masks to the following thermal cycle: | | P |
| | for 24 h to a dry atmosphere of $(70 \pm 3) ^\circ\text{C}$; | 70°C 24h | P |
| | for 24 h to a temperature of $(-30 \pm 3) ^\circ\text{C}$; | -30°C 3h | P |
| 8.3.3 | Mechanical strength | | P |
| 8.3.4 | Flow conditioning | | P |
| 8.4 | Practical performance | Test 2 samples | P |
| | head harness comfort | Good | P |
| | security of fastenings | Good | P |
| | field of vision | Does not affect line of sight | P |
| | any other comments reported by the wearer on request. | No other comments | P |
| 8.4.2 | Walking test | 6km/h, 10 min | P |
| 8.4.3 | Work simulation test | | P |


| | | | |
|-----|---|-----------------------------|-----|
| | <p>walking on the level with headroom of (1,3 ± 0,2) m for 5 min;</p> <p>crawling on the level with headroom of (0,70 ± 0,05) m for 5 min;</p> <p>c) filling a small basket (see Figure 1, approximate volume = 8 l) with chippings or other suitable material from a hopper which stands 1,5 m high and has an opening at the bottom to allow the contents to be shovelled out and a further opening at the top where the basket full of chippings is returned.</p> <p>The subject shall stoop or kneel as he wishes and fill the basket with chippings. He shall then lift the basket and empty the contents back into the hopper. This shall be done 20 times in 10 min.</p> | | P |
| 8.5 | Leakage | | P |
| | General test procedure | total of 10 test specimens | P |
| | The total inward leakage shall be tested using sodium chloride aerosol. | | P |
| | ten clean-shaven persons (without beards or sideburns) | 6km/h | P |
| | Test procedure | | P |
| | Method | | P |
| 8.6 | Flammability | 800°C flame height: 40mm | P |
| 8.7 | Carbon dioxide content of the inhalation air | Test 3 samples | P |
| | Air shall be supplied to it from a breathing machine adjusted to 25 cycles/min and 2,0 l/stroke and the exhaled air shall have a carbon dioxide content of 5 % by volume. | | P |
| | The total dead space of the gas path (excluding the breathing machine) of the test installation should not exceed 2000 ml. | | P |
| | The air flow from the front shall be 0,5 m/s. | | P |
| 8.8 | Strength of attachment of exhalation valve housing | 10N, 10s Test 3 samples | N/A |
| 8.9 | Breathing Resistance | Test 12pcs samples | P |



| | <p>Exhalation resistance</p> <p>Seal the particle filtering half mask on the Sheffield dummy head. Measure the exhalation resistance at the opening for mouth of the dummy head using the adapter shown in Figure 6 and a breathing machine adjusted to 25 cycles/min and 2.0 l/stroke or a continuous flow 160 l/min. Use a suitable pressure transducer.</p> <p>Measure the exhalation resistance with the dummy head successively placed in 5 defined positions:</p> <ul style="list-style-type: none"> - facing directly ahead - facing vertically upwards - facing vertically downwards - lying on the left side - lying on the right side <p>8.9.3 Inhalation resistance</p> <p>Test the inhalation resistance at 30 l/min and 95 l/min continuous flow.</p> | | P | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
|--|---|------------------------------|-------------------|------------------------|--|--|--------------------------------|------------------------------|-------------------|-----|-----|---|------|---|----|---|------|---|----|---|----|---|----|---|----|---|---|---|----|--|--|----|----|---|---|----|----|--|--|----|----|----|---|----|---|--|-----|
| 8.10 | Clogging | Test 3 samples dolomite dust | N/A | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | <p>The working area of the test chamber has a suggested square section of 650 mm × 650 mm.</p> <p>The breathing machine has a displacement of 2,0 l/stroke. The exhaled air shall pass a humidifier in the exhaled air circuit, such that the exhaled air temperature, measured at the position of the sample particle filtering half mask is (37 ± 2) °C and 95 % R.H. minimum.</p> | | N/A | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | <table border="1"> <thead> <tr> <th colspan="2">Coulter counter</th> <th colspan="2">Sedimentation analysis</th> </tr> <tr> <th>Size (equivalent spherical diameter) µm</th> <th>% Number particles oversize</th> <th>Size (Stokes diameter) µm</th> <th>% weight oversize</th> </tr> </thead> <tbody> <tr> <td>0,7</td> <td>100</td> <td>1</td> <td>99,5</td> </tr> <tr> <td>1</td> <td>80</td> <td>2</td> <td>97,5</td> </tr> <tr> <td>2</td> <td>30</td> <td>3</td> <td>95</td> </tr> <tr> <td>3</td> <td>17</td> <td>5</td> <td>85</td> </tr> <tr> <td>5</td> <td>7</td> <td>8</td> <td>70</td> </tr> <tr> <td></td> <td></td> <td>10</td> <td>50</td> </tr> <tr> <td>9</td> <td>2</td> <td>12</td> <td>26</td> </tr> <tr> <td></td> <td></td> <td>14</td> <td>10</td> </tr> <tr> <td>12</td> <td>1</td> <td>18</td> <td>1</td> </tr> </tbody> </table> | Coulter counter | | Sedimentation analysis | | Size (equivalent spherical diameter) µm | % Number particles oversize | Size (Stokes diameter) µm | % weight oversize | 0,7 | 100 | 1 | 99,5 | 1 | 80 | 2 | 97,5 | 2 | 30 | 3 | 95 | 3 | 17 | 5 | 85 | 5 | 7 | 8 | 70 | | | 10 | 50 | 9 | 2 | 12 | 26 | | | 14 | 10 | 12 | 1 | 18 | 1 | | N/A |
| Coulter counter | | Sedimentation analysis | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Size (equivalent spherical diameter) µm | % Number particles oversize | Size (Stokes diameter) µm | % weight oversize | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 0,7 | 100 | 1 | 99,5 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 1 | 80 | 2 | 97,5 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 2 | 30 | 3 | 95 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 3 | 17 | 5 | 85 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 5 | 7 | 8 | 70 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | | 10 | 50 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 9 | 2 | 12 | 26 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | | 14 | 10 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 12 | 1 | 18 | 1 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 8.11 | Penetration of filter material | | N/A | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| 9 | Marking | | P | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |


| | | | |
|-------|---|---------|-----|
| 9.1 | Packaging | | P |
| 9.1.1 | The name, trademark or other means of identification of the manufacturer or supplier. | | P |
| 9.1.2 | Type-identifying marking. | | P |
| 9.1.3 | Classification | | P |
| 9.1.3 | FFP1, FFP2 or FFP3 "NR" if the particle filtering half mask is limited to single shift use only. Example: FFP3 NR, or "R" if the particle filtering half mask is re-usable. Example: FFP2 R D." | FFP2 NR | P |
| 9.1.4 | The number and year of publication of this European Standard | | P |
| 9.1.5 | the year of end of shelf life. | | P |
| 9.1.6 | ‘see information supplied by the manufacturer’  | | P |
| 9.1.7 | The manufacturer's recommended conditions of storage | | P |
| 9.1.8 | The packaging of those particle filtering half masks passing the dolomite clogging test shall be additionally marked with the letter "D" | | N/A |
| 9.2 | Particle filtering half mask | | P |

P

Photos

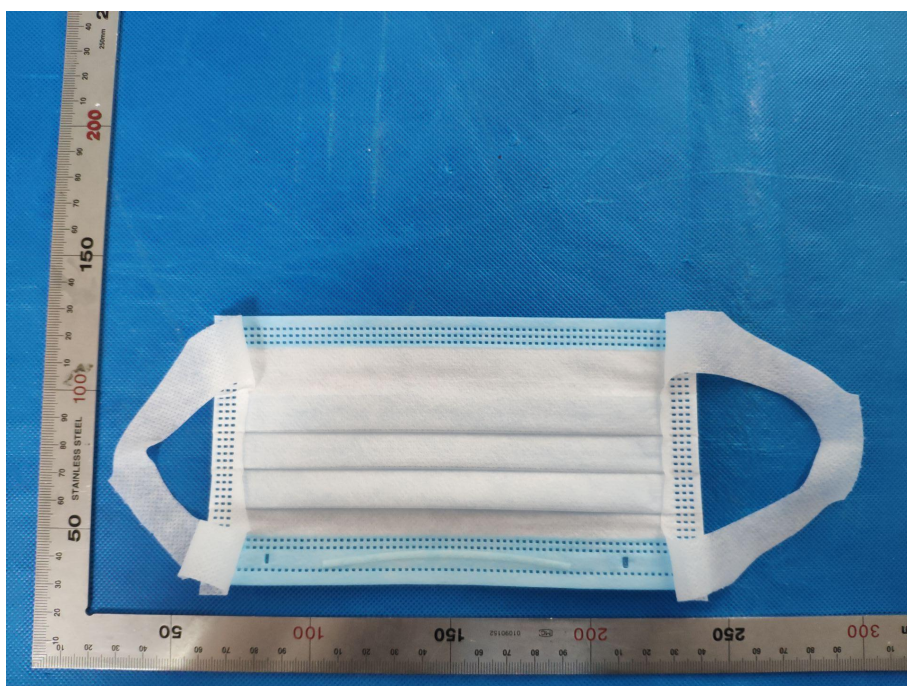

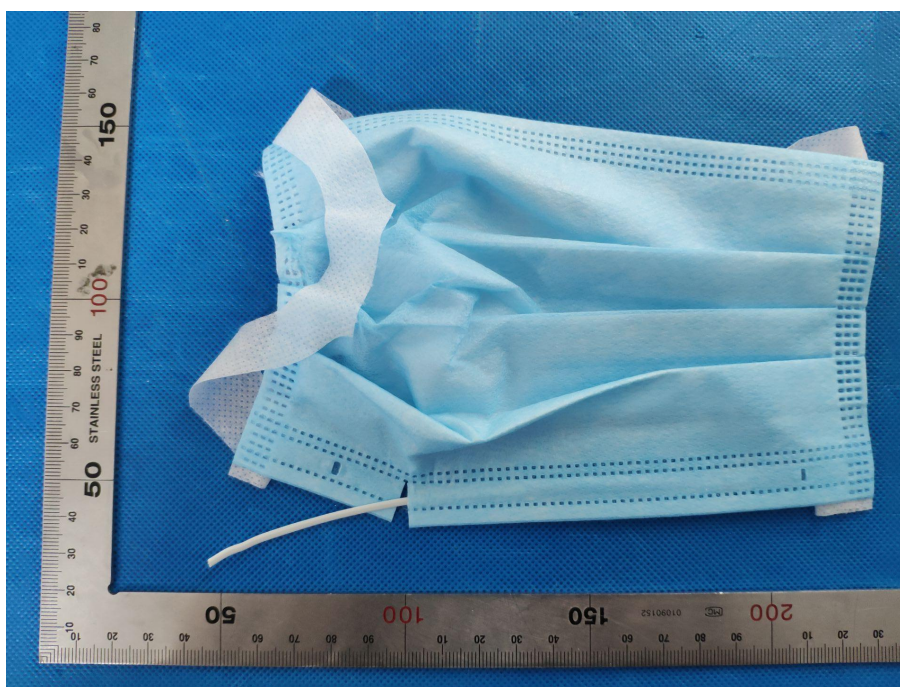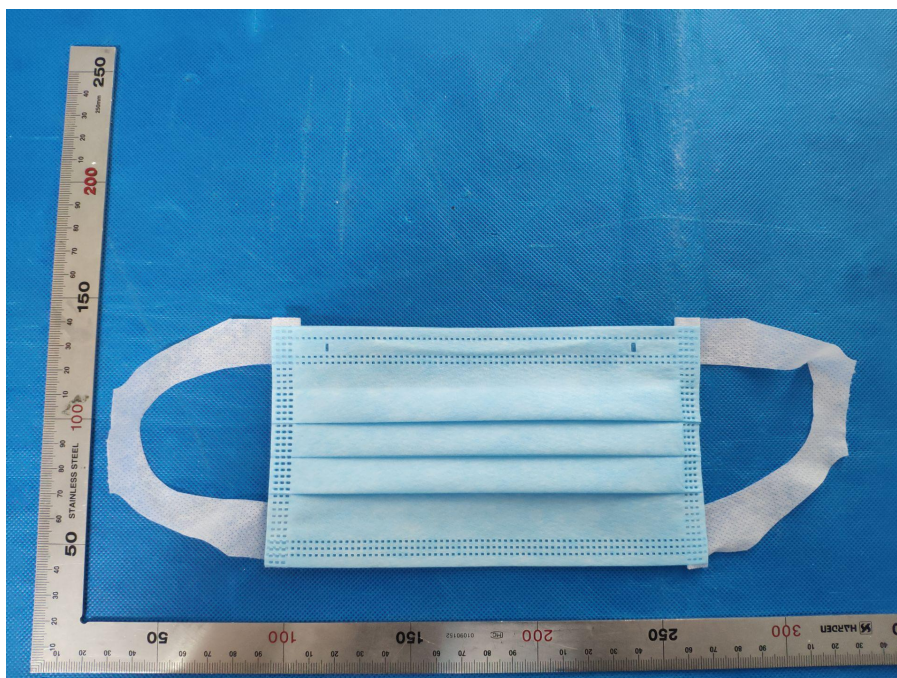

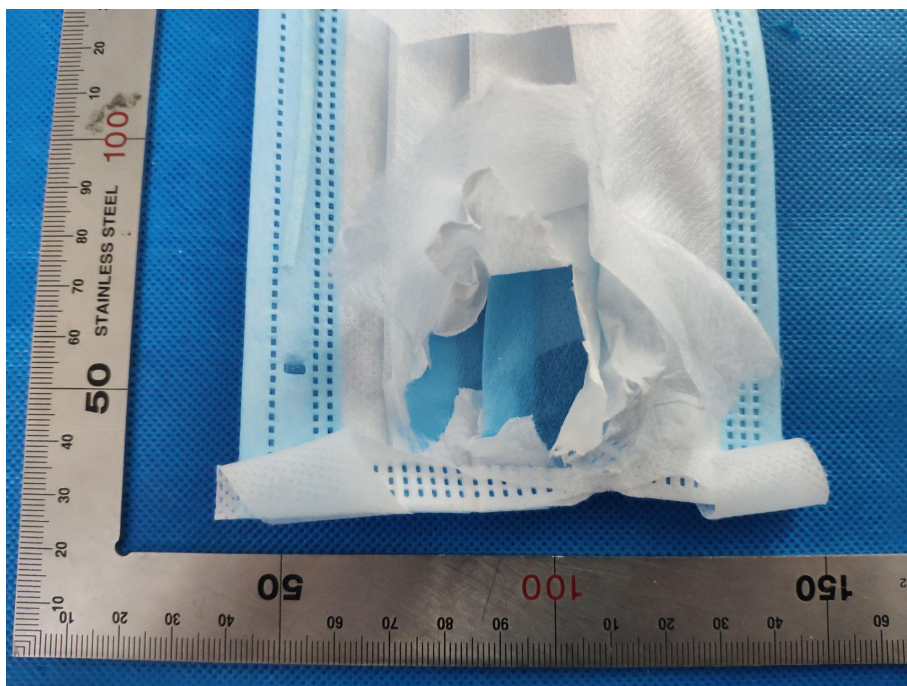

*****End of Test Report*****