

Lot 10, Sistem RT-PCR**Rotor-Gene Q MDx 5plex HRM Platform, cu soft Rotor-Gene AssayManager 2.1****Qiagen GmbH, Malaesia****DM000308110 – numar inregistrare in calitate de DM**

Parametri solicitati	Parametri oferiti
"Aplicare: Pentru analiza PCR în timp real validată IVD în aplicații clinice Sistem optic: 5 canale + HRM (Blue, Green, Yellow, Orange, Red, Crimson, HRM) Surse de excitare: diode emițătoare de lumină de înaltă energie Detector: fotomultiplicator Probe per run (debit): Tuburi 0,2 ml, 36 – 96 probe/run Tehnologie: Ciclor PCR în timp real Performanta termică: interval de temperatură, 35–99°C, acuratețea temperaturii, ± 0,5°C Software: cu soft pentru analiză și interpretare a testelor IVD și soft pentru analiza HRM Calculator (computer sau notebook) – da Seturi pentru calibrare și verificare – da Termen de garanție: ≥24 luni Instalare, darea în exploatare, instruirea de către participantul câștigător – obligatoriu Training pentru utilizatori la instalare și la solicitare - obligatoriu. Servicii de mentenanță preventivă pe perioada de garanție Documente confirmative: Manual de service si manual de utilizare in conformitate cu LEGEA Nr. 102 cu privire la dispozitivele medicale din 09.06.2017, capitolul 4 Articolul 14. P. 3. Ghid rapid al utilizatorului in limba de stat - obligatoriu. "	"Aplicare: Pentru analiza PCR în timp real validată IVD în aplicații clinice Sistem optic: 5 canale + HRM (Blue, Green, Yellow, Orange, Red, Crimson, HRM) Surse de excitare: diode emițătoare de lumină de înaltă energie Detector: fotomultiplicator Probe per run (debit): Tuburi 0,2 ml/0,1ml/0,03ml, 36 -72- 100 probe/run Tehnologie: Ciclor PCR în timp real Performanta termică: interval de temperatură, 35–99°C, acuratețea temperaturii, ± 0,5°C Software: cu soft pentru analiză și interpretare a testelor IVD și soft pentru analiza HRM Calculator (computer sau notebook) – da Seturi pentru calibrare și verificare – da Termen de garanție: 24 luni Instalare, darea în exploatare, instruirea de către participantul câștigător – obligatoriu Training pentru utilizatori la instalare și la solicitare - obligatoriu. Servicii de mentenanță preventivă pe perioada de garanție Documente confirmative: Manual de service si manual de utilizare in conformitate cu LEGEA Nr. 102 cu privire la dispozitivele medicale din 09.06.2017, capitolul 4 Articolul 14. P. 3. Ghid rapid al utilizatorului in limba de stat - obligatoriu. "

Rotor-Gene® Q — Pure Detection

Now with even more applications!



Sample & Assay Technologies



The Rotor-Gene Q — for your success

Quantitative, real-time PCR is a precision science that places high demands on the instrument, chemistry, and software. High thermal and optical uniformity, short equilibration times, and fast ramping rates are critical for precise and rapid quantitative analysis. Sensitivity, speed, and specificity are also highly dependent on the performance of the DNA polymerase and reaction components.

QIAGEN's real-time PCR cycler, the Rotor-Gene Q, combines multiple optimized design features to provide the outstanding performance and reliable results that your research demands. Together with optimized QIAGEN® kits for real-time PCR, the Rotor-Gene Q enables streamlined analysis for a wide range of applications.



Benefits of the Rotor-Gene Q:

- Outstanding thermal and optical performance due to rotary format
- An unmatched optical range spanning UV to infrared wavelengths
- Various state-of-the-art analyses supported by user-friendly software
- Low maintenance and maximum convenience due to robust design
- High performance in multiple applications with QIAGEN kits

Comprehensive application range

The Rotor-Gene Q combined with optimized QIAGEN kits addresses a wide range of real-time PCR and high-resolution melting (HRM™) applications:

- | | |
|----------------------------|---------------------|
| ■ Gene expression analysis | ■ Genotyping |
| ■ Pathogen detection | ■ Mutation analysis |
| ■ DNA methylation analysis | ■ miRNA research |

For details of applications, see page 8.

Visit www.qiagen.com/PCR-applications and navigate your way through the Rotor-Gene Q Virtual World. Experience more than 20 instrument and software animations!



Unique rotary design for outstanding performance

The unique centrifugal rotary design of the Rotor-Gene Q makes it the most precise and versatile real-time PCR cycler currently available (Figure 1). Each tube spins in a chamber of moving air, keeping all samples at precisely the same temperature during rapid thermal cycling. Detection is similarly uniform. When each tube aligns with the detection optics, the sample is illuminated and the fluorescent signal is rapidly collected from a single, short optical pathway. This thermal and optical uniformity results in sensitive, precise, and fast real-time PCR analysis (Figure 2). It also eliminates sample-to-sample variation and edge effects. These are unavoidable in traditional block-based instruments due to temperature gradients across the block and multiple, complex optical pathways.

The rotary design delivers:

- Well-to-well temperature variation below $\pm 0.02^{\circ}\text{C}$
- Uniform detection eliminating the need for ROX reference dye
- Fast ramping and negligible equilibration times for short run times
- Complete confidence in your results!

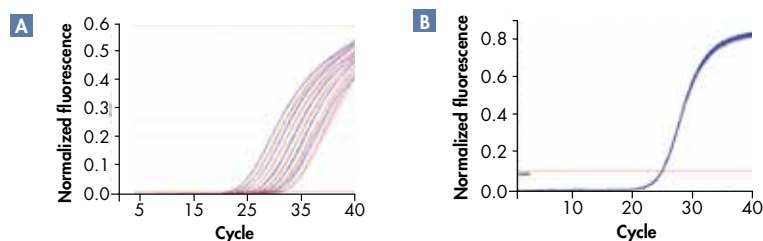


Figure 2. Precise real-time PCR analysis. **A** Twofold dilutions of human genomic DNA from 30 ng (10,000 copies) to 0.06 ng (20 copies) were used as template in real-time PCR. Five replicate reactions were run for each dilution using a self-designed TaqMan[®] assay for IL1R2 and the Rotor-Gene Probe PCR Kit on the Rotor-Gene Q. The average difference in the C_T values between all dilutions was 1.07 cycles. **B** Human genomic DNA was used as template in 72 replicate real-time PCRs using a self-designed TaqMan assay for BCL2 on the Rotor-Gene Q without ROX normalization. The average C_T value was 24.94 with a standard deviation of only 0.05, equivalent to a CV of 0.2%.

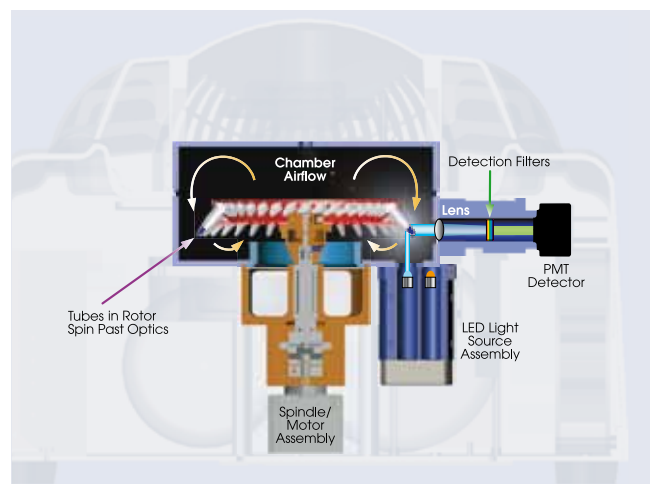


Figure 1. Cross-section of the Rotor-Gene Q. Heating/cooling is achieved by rapid airflow in the reaction chamber. Tubes spin past the excitation/detection optics every 150 milliseconds enabling high-speed data capture. Up to 6 separate LED light sources can be used in combination with 6 different detection filters and a highly sensitive photomultiplier detector.



Placing a 72-Well Rotor into the Rotor-Gene Q.



Multiple PCR tube and Rotor-Disc formats.

Unrivalled optical range enables multiple applications

Whether your assay is based on intercalating dyes such as SYBR® Green, probes such as hydrolysis (TaqMan), hybridization (FRET), or Scorpion probes, the Rotor-Gene Q meets your requirements. With up to 6 channels spanning UV to infrared wavelengths, the cyclor delivers the widest optical range currently available (Table 1), and is highly suited for all multiplex applications. In addition, the software allows you to create new excitation/detection wavelength combinations, which means that the Rotor-Gene Q is compatible with dyes you may use in the future.

Table 1. Channels for optical detection

Channel	Excitation (nm)	Detection (nm)	Examples of fluorophores detected
Blue	365±20	460±20	Marina Blue®, Edans, Bothell Blue, Alexa Fluor® 350, AMCA-X
Green	470±10	510±5	FAM™, SYBR Green I, Fluorescein, EvaGreen®, Alexa Fluor 488
Yellow	530±5	557±5	JOE™, VIC®, HEX, TET™, MAX™, CAL Fluor®, Gold 540, Yakima Yellow®
Orange	585±5	610±5	ROX™, CAL Fluor Red 610, Cy®3.5, Texas Red®, Alexa Fluor 568
Red	625±5	660±10	Cy5, Quasar® 670, LightCycler®, Red640, Alexa Fluor 633
Crimson	680±5	712 high pass	Quasar 705, LightCycler Red705, Alexa Fluor 680
HRM	460±20	510±5	SYBR Green I, SYTO®9, LC Green®, LC Green Plus+, EvaGreen

Flexible formats match your workflows

The Rotor-Gene Q supports multiple PCR tube formats to suit a range of needs. Changing the format, by simply switching the snap-fit metal rotor that holds the tubes, takes just seconds.

As well as tubes, Rotor-Disc™ rotors are available, which offer accelerated setup and higher throughput. Rotor-Discs are circular plates of vertically-oriented reaction wells. The Rotor-Disc 100 is the equivalent of a 96-well plate with an additional 4 reference wells. These extra wells can be conveniently used for more reactions or additional controls. Rotor-Discs can be quickly and easily sealed with plastic film using a Rotor-Disc Heat Sealer.

You can perform manual reaction setup, or take advantage of QIAGEN's automated solutions for reaction setup. The QIAgility® is cost-effective and delivers rapid, high-precision PCR setup, while the QIASymphony® AS is ideal for laboratories performing routine PCR tests on a day-to-day basis. Both instruments perform automated reaction setup in Rotor-Gene formats, allow direct transfer of sample lists, and are supplied with verified protocols for real-time PCR master mixes.

Minimum maintenance, maximum convenience

The Rotor-Gene Q is engineered to reduce the need for maintenance and to maximize ease of use. This saves time and costs and allows you to focus on your research, not on keeping the cyclor up and running. For example, highly stable excitation source LEDs are provided with a life-long guarantee, eliminating the need for frequent and time-consuming lamp replacement.

Features of the Rotor-Gene Q:

- Few moving parts and short, fixed optical path increase robustness
- No need for optical alignment, calibration, or lamp replacement
- Small, light instrument is easily transportable for flexibility in your lab

Easy routine verification

Laboratories may often want to verify thermal accuracy. For most cyclers, this requires interaction with a service engineer. With the Rotor-Gene Q, this is not necessary. Instead, the easy-to-use, cost-effective Rotor-Disc OTV (Optical Temperature Verification) Kit automates accuracy testing. The kit includes a specialized Rotor-Disc filled with temperature-sensitive liquid crystals and dedicated analysis software. The full procedure takes less than 30 minutes.

Reliable support for your peace of mind


In the unlikely event of any service issues with your Rotor-Gene Q, QIAGEN Instrument Service provides comprehensive support services to ensure the continued success of your PCR applications. QIAGEN Instrument Service offers a wide range of flexible Service Support products, giving you peace of mind and letting you enjoy complete coverage and cost control. Our Application Services and Training Programs give you the freedom and flexibility to adapt your system to specific or changing research needs. With ISO 9001/ISO 13485 certification and an international team of highly qualified and experienced Support Specialists, we deliver the high-quality service that you deserve and that your applications demand.

Specifications of the Rotor-Gene Q

View the outstanding technical features of the Rotor-Gene Q (Table 2).

Table 2. Rotor-Gene Q specifications


Dimensions and weight	Width 370 mm (14.6 in.) x Depth 420 mm (16.5 in.) x Height 286 mm (11.3 in.)
	Depth (door open): 538 mm (21.2 in.)
	Weight: 12.5 kg (27.6 lb)
Thermal performance	Temperature uniformity: $\pm 0.02^{\circ}\text{C}$ (Standard deviation)
	Temperature accuracy: $\pm 0.5^{\circ}\text{C}$
	Temperature resolution: $\pm 0.02^{\circ}\text{C}$
	Temperature range: 35 – 99°C
Optical system	Up to 6 separate channels (365–680 nm excitation, 460–750 nm detection)
	Fixed optical path, separate high-power excitation LEDs and emission filters per channel
	Highly sensitive photomultiplier (PMT) detector with gain setting (sensitivity control)
	Dynamic range: 10 orders of magnitude (assay dependent)
Rotor and well configurations	Rotor-Disc 100: 30 μl x 100 wells, 15–25 μl recommended reaction volume
	Rotor-Disc 72: 0.1 ml x 72 wells, 20–25 μl recommended reaction volume
	Strip Tubes 0.1 ml: 0.1 ml x 72 wells, 10–50 μl recommended reaction volume, strips of 4 tubes and caps
	PCR Tubes 0.2 ml: 0.2 ml x 36 wells, 20–50 μl recommended reaction volume, individual tubes with caps
Typical run time	40 cycles in 45–60 minutes with QIAGEN Rotor-Gene Kits (detection method dependent)
Electrical requirements	100–240 V AC, 50/60 Hz; 560 VA (peak)
Warranty	1 year on instrument; lifetime guarantee on excitation LEDs

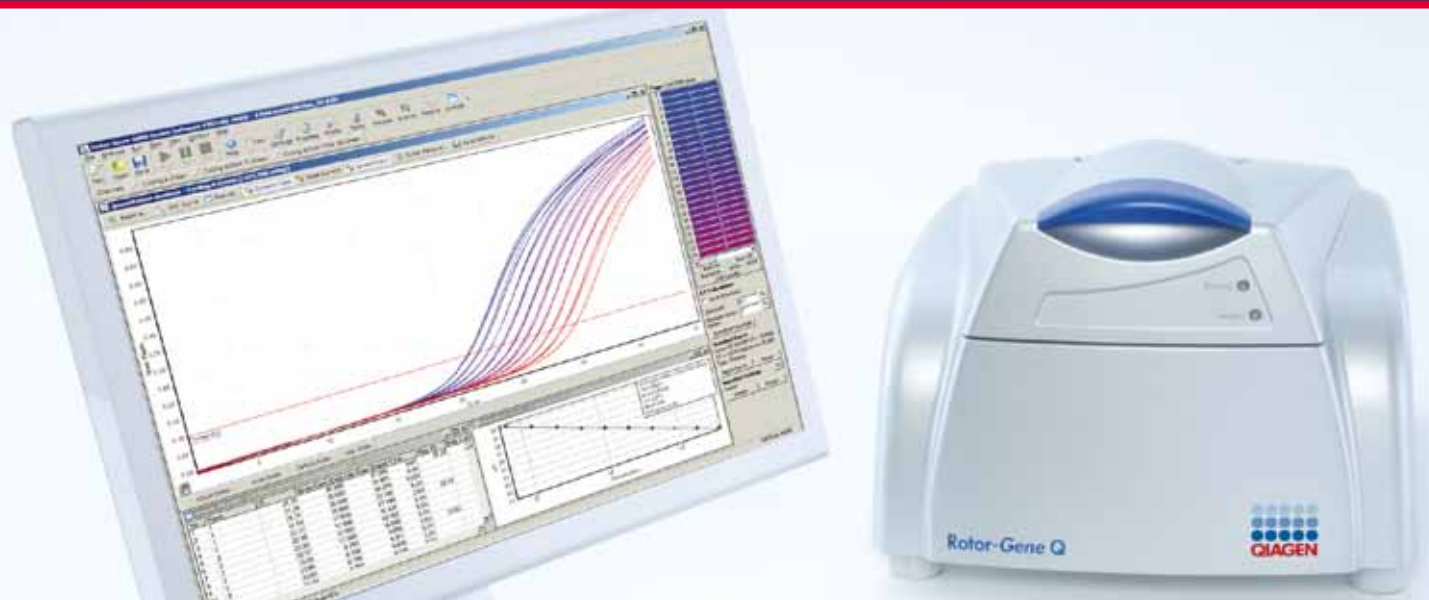

Software enables quantification and enhances data security

The comprehensive Rotor-Gene Q software package supports all current state-of-the-art real-time analysis procedures with basic to advanced algorithms. This provides complete freedom to analyze your valuable experimental data and increases the reliability of your results. Data security is assured and process steps are trackable from starting the run to exporting the results.


Analysis procedures supported by Rotor-Gene Q software

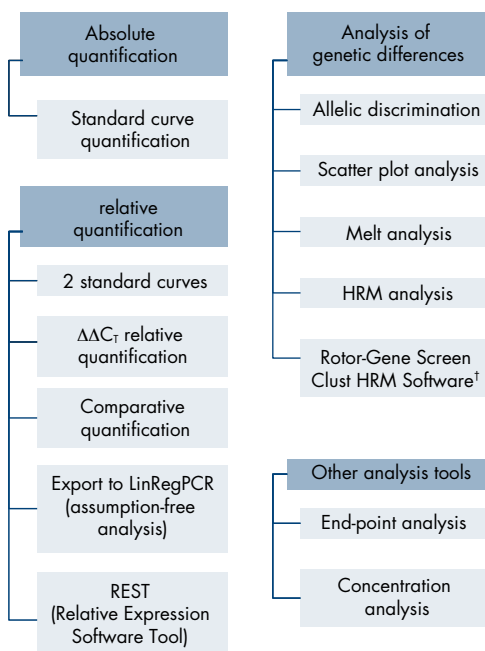

* REST employs differing PCR efficiencies and multiple reference genes for normalization, available free of charge at www.qiagen.com/rest † Software available separately

The easy-to-use software provides:

- Unlimited user licenses and individual user management
- A digital signature for every result file
- Audit trails to track changes made to experiment files
- Various result reports and export functions
- Raw data export for validation purposes

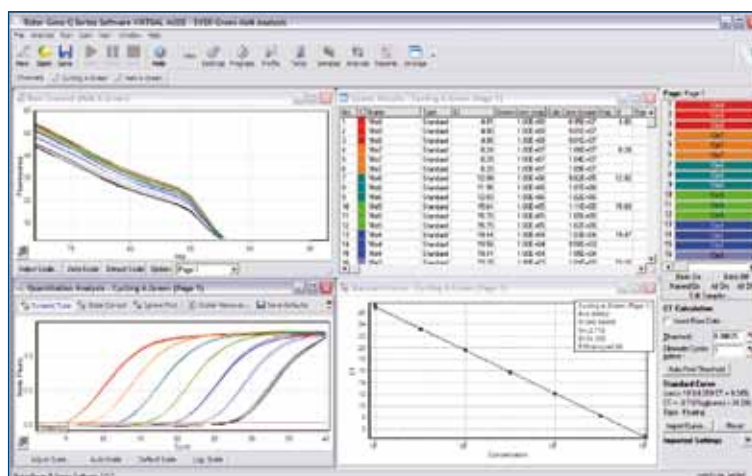

Expand your research with HRM

High-resolution melting analysis (HRM) is a closed-tube, post-PCR analysis that has raised enormous scientific interest. HRM characterizes double-stranded PCR products based on their dissociation (melting) behavior. It is similar to classical melting curve analysis, but provides far more information for a wider range of applications. PCR products can be discriminated according to sequence, length, GC content, or strand complementarity, down to single base-pair changes. Previously unknown and even complex sequence variations can be readily detected and characterized in a robust and straightforward way. The Rotor-Gene Q is ideal for HRM applications due to its outstanding temperature and fluorescence precision for every well.

The HRM option for the Rotor-Gene Q features:

- A specially tuned high-intensity optical HRM channel
- Thermal resolution down to 0.02°C
- High data acquisition rates
- Comprehensive HRM software

HRM on the Rotor-Gene Q is capable of deciphering minute genetic differences such as difficult A/T class IV SNPs with melting point differences below 0.2°C (Figure 3 and 4).

Harness the power of HRM for applications such as:

- Genotyping
- Pathogen typing
- Gene scanning
- Quantitative methylation analysis

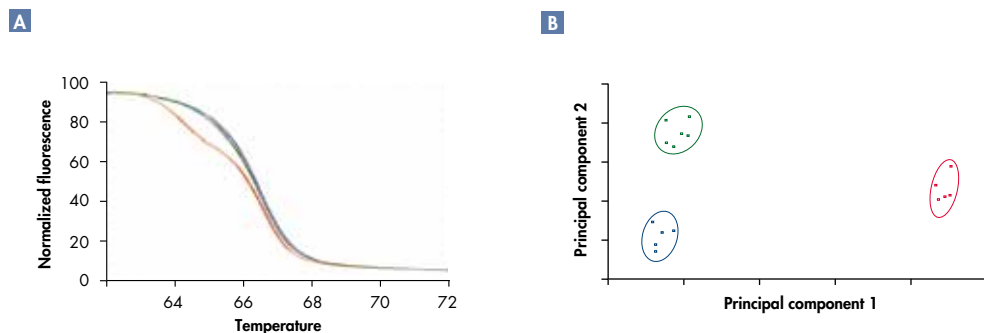


Figure 4. HRM Analysis of a class IV SNP with less than 0.1°C difference between homozygote alleles. A human A/T SNP in the AHRR gene was analyzed using genomic DNA from wild-type (blue), homozygous mutant (green), and heterozygous (red) samples. Experiments were performed using the Type-it HRM PCR Kit, Rotor-Gene Q HRM instrument, and Rotor-Gene ScreenClust HRM Software. **A** Normalized melting curves: homozygote curves are almost identical. **B** ScreenClust HRM cluster plot: all pseudo-unknowns including homozygous alleles were unambiguously clustered according to the correct genotype.

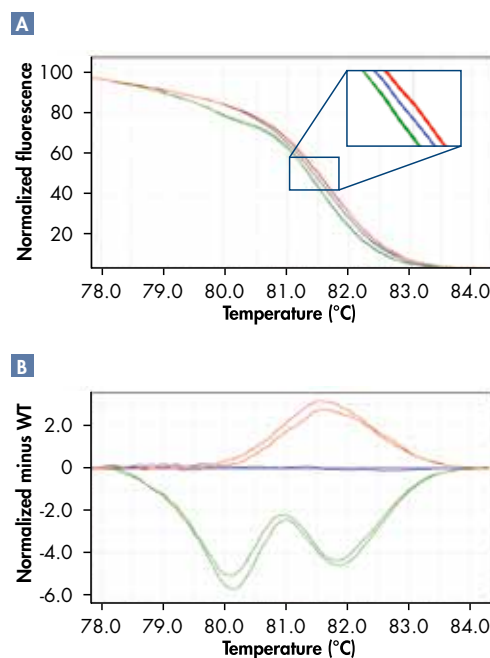


Figure 3. Successful genotyping of an A/T Class IV SNP. Typing the SNP (rs2270938) in the human GYS1 gene using the Type-it HRM PCR Kit results in highly reproducible and accurate results. The normalized melting curve and difference plot show successful and reliable discrimination of all 3 genotypes (Blue: wild-type; Green: heterozygous; Red: mutant). **A** normalized melt curve. **B** difference plot normalized to wild type samples.

Optimized reagents for all your applications

A range of QIAGEN kits for the Rotor-Gene Q enables reliable quantification in your real-time PCR applications without the need for optimization of reaction and cycling conditions (Table 3).

Features and benefits of QIAGEN's kits for real-time PCR

Highly specific amplification is assured through a balanced combination of NH₄⁺ and K⁺ ions that minimizes nonspecific primer annealing. Fast cycling without compromising performance is achieved using Q-Bond, a proprietary PCR additive that enables cycle run times of as low as 45 minutes. For multiplex PCR applications, synthetic Factor MP allows different amplicons in the same reaction to all be amplified with the same high efficiency. Factor MP, an innovative PCR additive, increases the local concentration of primers at the template and stabilizes specifically bound primers, allowing efficient primer extension by DNA polymerase.

Table 3. Pure detection for all your applications

Application	Detection method	Procedure	QIAGEN kit	Data
Gene expression analysis	SYBR Green	PCR and 2-step RT-PCR	Rotor-Gene SYBR Green PCR Kit	Table 4
	SYBR Green	1-step RT-PCR	Rotor-Gene SYBR Green RT-PCR Kit	Fig. 5
	SYBR Green	2-step RT-PCR array	Pathway-Focused RT ² Profiler PCR Arrays	Fig. 9
	Probe (singleplex)	PCR and 2-step RT-PCR	Rotor-Gene Probe PCR Kit	Fig. 2
	Probe (singleplex)	1-step RT-PCR	Rotor-Gene Probe RT-PCR Kit	
	Probe (multiplex)	PCR and 2-step RT-PCR	Rotor-Gene Multiplex PCR Kit	Fig. 7
	Probe (multiplex)	1-step RT-PCR	Rotor-Gene Multiplex RT-PCR Kit	Fig. 8
	Probe (duplex)	2-step RT-PCR and 1-step RT-PCR	QuantiFast Probe Assays and Kits	Fig. 6
miRNA detection	SYBR Green	Two-step RT-PCR	miScript SYBR Green PCR Kit	Fig. 10
Pathogen detection	Probe (multiplex)	PCR, 2-step RT-PCR, and 1-step RT-PCR	QuantiTect® Virus +ROX Vial Kit	
	Probe (duplex)	PCR or 1-step RT-PCR incl. universal internal control	QuantiFast Pathogen +IC Kits	Fig. 11
Food safety testing	Probe	Real-time PCR assays	mericon™ food testing portfolio	Fig. 12
Pathogen typing	EvaGreen	HRM	Type-it HRM PCR Kit	Fig. 13
Genotyping	Probe	PCR	Type-it Fast SNP Probe PCR Kit	Fig. 14
	EvaGreen	HRM	Type-it HRM PCR Kit	Fig. 15, 3
Methylation analysis	Probe	PCR	EpiTect® Methylight PCR Kit	Table 5
	EvaGreen	HRM	EpiTect HRM PCR Kit	Fig. 16

Gene expression analysis

The combination of Rotor-Gene SYBR Green Kits, QuantiTect Primer Assays, and the Rotor-Gene Q provides a complete, ready-to-run solution for gene expression analysis. QuantiTect Primer Assays are predesigned primer sets for any gene from human, mouse, rat, and many other species. Assays can be easily ordered online at the GeneGlobe® Web portal (www.qiagen.com/GeneGlobe). When the assays are used together with Rotor-Gene SYBR Green Kits, highly sensitive quantification of specific PCR products is achieved without the need for optimization (Figure 5 and Table 4).

Table 4. Superior performance in RT-PCR with SYBR Green

	QIAGEN		Supplier A _{II}	
	C _T	Mean deviation	C _T	Mean deviation
BAX (BCL2-associated X protein)	24.84	0.05	29.57	0.46
BCL2 (apoptosis gene)	26.96	0.05	32.83	0.29
MYC (proto-oncogene)	28.42	0.21	35.26	0.72
β-Actin (housekeeping gene)	20.24	0.03	24.39	0.12

Human leukocyte cDNA (1 ng) was used as template in SYBR Green-based real-time two-step RT-PCR. Triplicate reactions were run using QuantiTect Primer Assays for 4 different targets: BAX, BCL2, MYC, and β-Actin. The Rotor-Gene Q and Rotor-Gene SYBR Green PCR Kit provided highly sensitive detection, indicated by lower C_T values and lower mean deviations compared to an instrument and kit from Supplier A_{II}.

For gene expression analysis using probe detection, QuantiFast Probe Assays, containing a premixed primer pair and dual-labeled probe (TaqMan-based probe), can be used in combination with dedicated master mix kits on the Rotor-Gene Q for fast and sensitive quantification. QuantiFast Probe Assays are designed using a proprietary algorithm to enable amplification and detection of RNA and cDNA targets less than 100 bp in size with high efficiency and reliability. They are highly suited for use with degraded starting material such as formalin-fixed, paraffin-embedded (FFPE) analytes. (Figure 6).

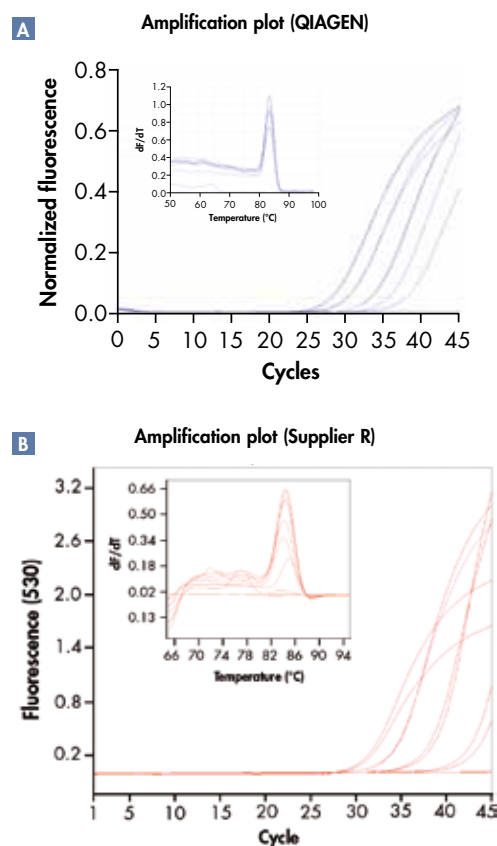
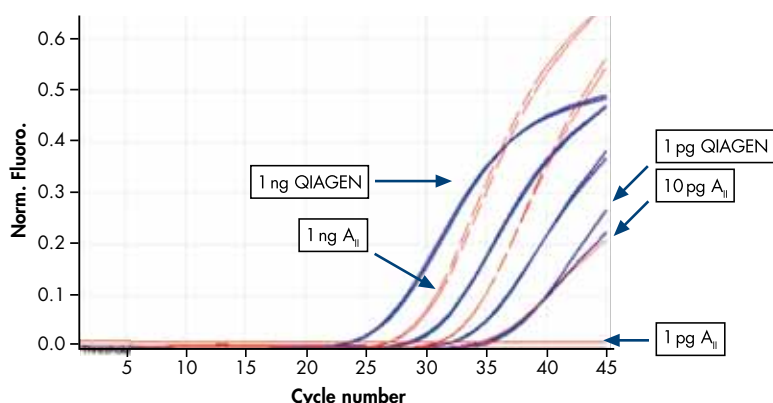


Figure 5. Specific and sensitive detection using SYBR Green. Tenfold dilutions of human leukocyte RNA (100 ng to 10 pg) were used as template in SYBR Green-based real-time one-step RT-PCR. Duplicate reactions were run using the QuantiTect Primer Assay for BCL2 (B-cell CLL/lymphoma 2). **A** The Rotor-Gene Q and Rotor-Gene SYBR Green RT-PCR Kit provided sensitive detection from 10 pg RNA and amplification of specific PCR product (melting curve shown in inset). **B** In contrast, an instrument and kit from Supplier R provided detection only after optimization of Mg²⁺ concentration. However, the limit of detection was 100 pg RNA and coamplification of nonspecific products was observed (melting curve shown in inset).

Figure 6. Highly efficient real-time RT-PCR detection using RNA from FFPE samples. Total RNA (1 ng, 100 pg, 10 pg, and 1 pg) was purified from a breast tissue FFPE sample using the RNeasy FFPE Kit. Transcripts of the human MUC1 gene were amplified and detected on the Rotor-Gene Q cyclor using the QuantiFast Probe RT-PCR Plus Kit and the QuantiFast Probe Assay (blue curves) or a predesigned assay from Supplier A_{II} (red curves). Results from the QuantiFast Probe Assay showed lower C_T values and higher sensitivity compared to results using the assay from Supplier A_{II}. As low as 1 pg template was detectable using the QuantiFast Probe Assay (1 pg was undetectable using the assay from Supplier A_{II}).

The ultimate solution for fast and reliable gene expression analysis is provided by the combination of the Rotor-Gene Multiplex PCR and RT-PCR Kits and the Rotor-Gene Q. Up to 4 cDNA targets can be simultaneously and rapidly quantified in the same tube, increasing throughput and saving precious sample material (Figures 7 and 8). Genes with different expression levels are all amplified in the same tube with the same high efficiency, enabling reliable relative quantification of gene expression.

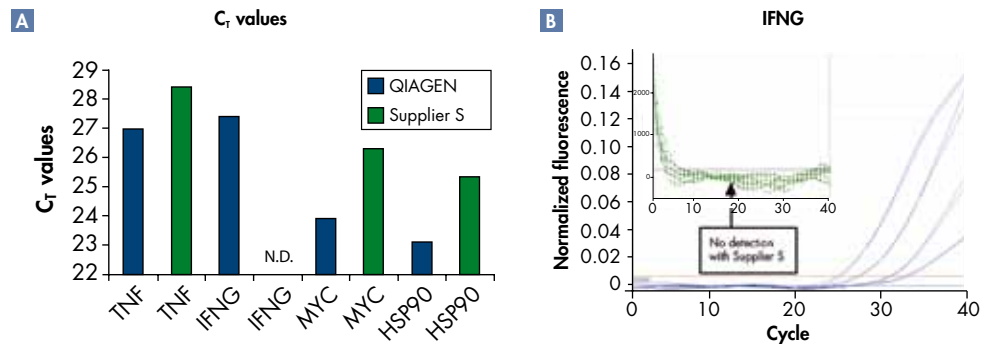


Figure 7. Reliable multiplex analysis. Tenfold dilutions of human leukocyte cDNA (10 ng to 10 pg) were used as template in 4-plex, real-time PCR. Reactions were run in triplicate using either the Rotor-Gene Q and Rotor-Gene Multiplex PCR Kit or an instrument and kit from Supplier S. Target genes: TNF (tumor necrosis factor), IFNG (interferon, gamma), MYC (v-myc myelocytomatosis viral oncogene homolog [avian]), HSP90AA1 (heat shock protein 90 kDa alpha [cytosolic], class A member 1). **A** C_t values obtained for all 4 targets (instrument and kit from Supplier S did not successfully detect IFNG; N.D.). Lower C_t values on the Rotor-Gene Q demonstrate detection with greater sensitivity. **B** Amplification plots for IFNG (plots for Supplier S in inset).

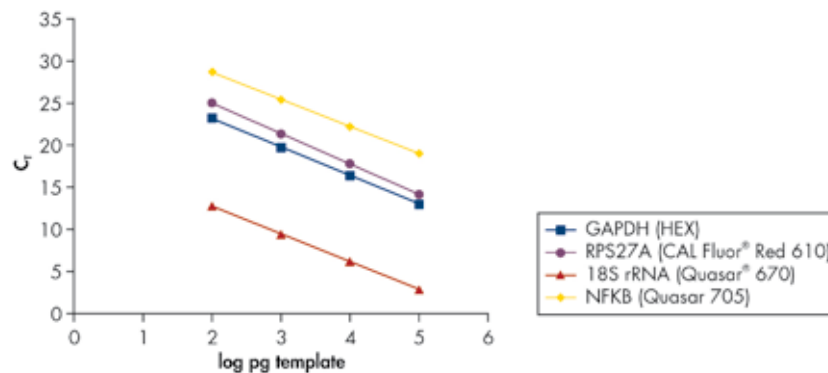


Figure 8. Highly efficient 4-plex analysis. 4-plex, real-time one-step RT-PCR was performed using the Rotor-Gene Multiplex RT-PCR Kit and self-designed TaqMan assays for the indicated targets. Reactions were run on the Rotor-Gene Q using 100, 10, 1, or 0.1 ng RNA from HeLa cells. The plots of C_t value versus log template amount were parallel, indicating all 4 targets were amplified with the same high efficiency. GAPDH: glyceraldehyde-3-phosphate dehydrogenase; RPS27A: ribosomal protein S27a; NFKB: nuclear factor of kappa light polypeptide gene enhancer in B-cells.

Pathway- and disease-focused PCR arrays

Pathway-focused RT² Profiler PCR Arrays are exceptionally reliable tools for analyzing the expression of a focused panel of genes. Each 100-well Rotor-Disc PCR Array includes SYBR Green-optimized (laboratory-tested) primer assays for a thoroughly researched panel of relevant, pathway- or disease-focused genes on the Rotor-Gene Q. RT² profiler PCR Arrays can also be customized to contain a panel of genes tailored to your specific research interests. Our high-quality primer design and master mix formulation enable the RT² profiler PCR Array to amplify 96 different gene-specific products simultaneously under uniform cycling conditions. This combination provides the RT² profiler PCR Array with the specificity and the high amplification efficiencies required for accurate real-time SYBR Green results (see Figure 9).* The simplicity of RT² profiler PCR Arrays makes them accessible for routine use in every research laboratory.

New developments in PCR array technology enable optimal performance of RT² Profiler PCR Arrays using RNA prepared from regular samples (0.1–5 µg RNA), FFPE samples, and small samples (1–100 ng RNA). See the PCR Array Protocol Guide to learn more.

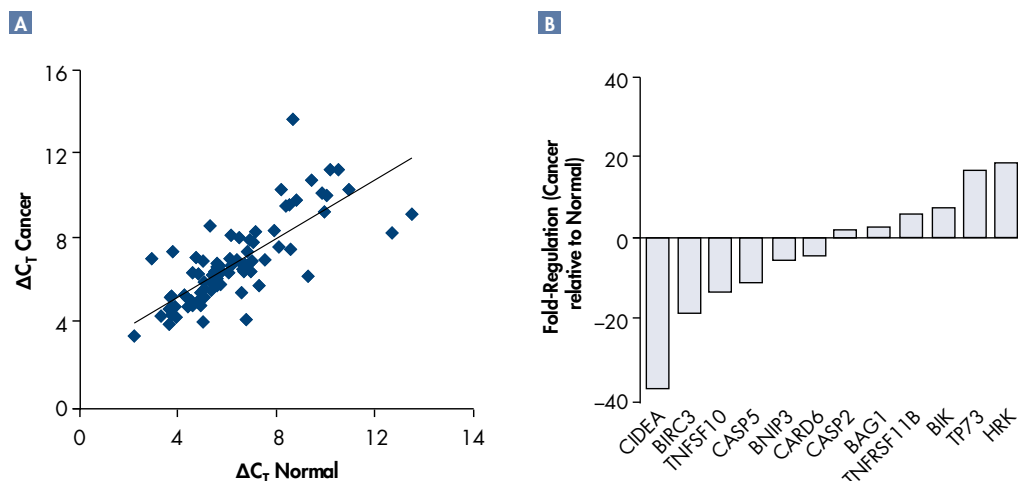


Figure 9. Gene expression profiling of normal and cancerous colon tissue. Using the Human Apoptosis RT² Profiler PCR Array, gene expression analysis of both normal (adult ascending colon) and cancer (adult colon adenocarcinoma) colon was performed using the Rotor-Gene Q. **A** ΔC_t values (data normalized to the geometric mean of 5 housekeeping genes) were plotted for both the normal and cancer tissue. **B** The fold-changes for selected targets that underwent significant (greater than 2-fold) changes in expression (cancer relative to normal) were plotted. Altogether, a total of 36 genes had a differential expression pattern in the cancer versus normal tissue, with 30 genes showing down-regulation and 6 genes showing up-regulation. Collectively, these data demonstrate the power of RT² Profiler PCR Arrays performed on the Rotor-Gene Q to profile differential gene expression patterns in cancer versus normal tissue.

* Data analysis software for pathway-focused RT² Profiler PCR Arrays is available free of charge at www.sabiosciences.com/pcarraydataanalysis.php

miRNA detection

miRNAs play an important role in many diverse biological processes. Dysregulation of miRNA expression is associated with several cancers and other diseases. For this exciting, emerging research area, QIAGEN offers the miScript PCR System, a three-component system that covers all steps of conversion of miRNA, mRNA, and other noncoding RNAs into cDNA and their subsequent detection of miRNAs by SYBR Green-based real-time PCR. Fast and easy reverse transcription using the miScript Reverse Transcription Kit is followed by sensitive and specific miRNA detection using the miScript SYBR Green PCR Kit and a miScript Primer Assay on the Rotor-Gene Q. Using appropriate assays, it is possible to detect either mature miRNA or precursor miRNA (Figure 10). For more information on the miScript PCR System, visit www.qiagen.com/miRNA.

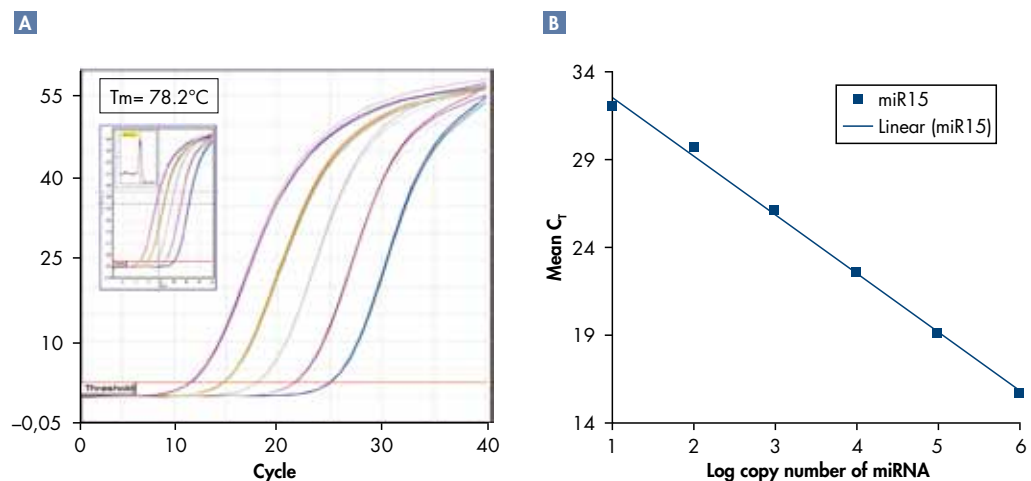


Figure 10. Quantification of miR-15 and RNU6B using the miScript PCR System on the Rotor-Gene Q. **A** Sensitive, specific quantification for a wide range of template amounts. The miScript Reverse Transcription Kit was used to generate cDNA from HeLa S3 cells. A range of cDNA amounts from 1 pg to 10 ng was used in real-time PCR with the miScript PCR System and a miScript Primer Assay for RNU6B. Real-time PCR was performed on the Rotor-Gene Q cyclor. The amplification plot shows sensitive, accurate quantification from low to high cDNA template amounts. The melting curve (inset) shows a single peak indicating specific detection. **B** Accurate detection of as low as 10 miRNA copies. Synthetic miR-15 was used to generate cDNA using the miScript Reverse Transcription Kit. A range of amounts from 10 copies to 10^6 copies of this cDNA was used in real-time PCR using the miScript PCR System. Real-time PCR was performed on the Rotor-Gene Q cyclor. The resultant C_t values decreased linearly with increasing miRNA copy number, indicating sensitive detection from a wide range of template amounts. The resultant C_t values were plotted against the log copy numbers, showing sensitive and linear detection from a wide range of template amounts.

Pathogen detection and food safety testing

Regardless of the pathogen or the material being examined, standard pathogen testing typically begins with a screening assay to simply assess presence or absence of a target. If results from the screening assay indicate presence of pathogens, further typing of the pathogen may be beneficial. Real-time PCR is the method of choice for accurate and reliable detection of pathogens and QIAGEN technologies and assays greatly facilitate this screening process. To streamline detection workflows, QIAGEN offers verified, ready-to-use assays as well as QuantiTect Virus Kits and QuantiFast Pathogen +IC RT-PCR Kits that enable multiplex qPCR for the detection of multiple targets in a single run.

Highly sensitive detection of viral RNA and/or DNA

The combination of the QuantiTect Virus +ROX Vial Kit and the Rotor-Gene Q provides highly sensitive and rapid detection of up to 4 viral DNA and RNA targets simultaneously. A concentrated master mix allows larger volumes of template to be added to assays, lowering the limit of detection. Viral nucleic acid targets can be individually detected in singleplex assays or detected together with internal controls in multiplex assays.

QuantiFast Pathogen +IC Kits show the same performance as QuantiTect Virus Kits, but are also delivered with a universal internal control to enable high process safety through correct interpretation of negative results e.g., by detecting PCR inhibition. In combination with the Rotor-Gene Q, the QuantiFast Pathogen +IC Kits enable simultaneous detection of viral RNA or DNA targets plus internal control over a wide linear range without loss of sensitivity when duplexing (Figure 11).

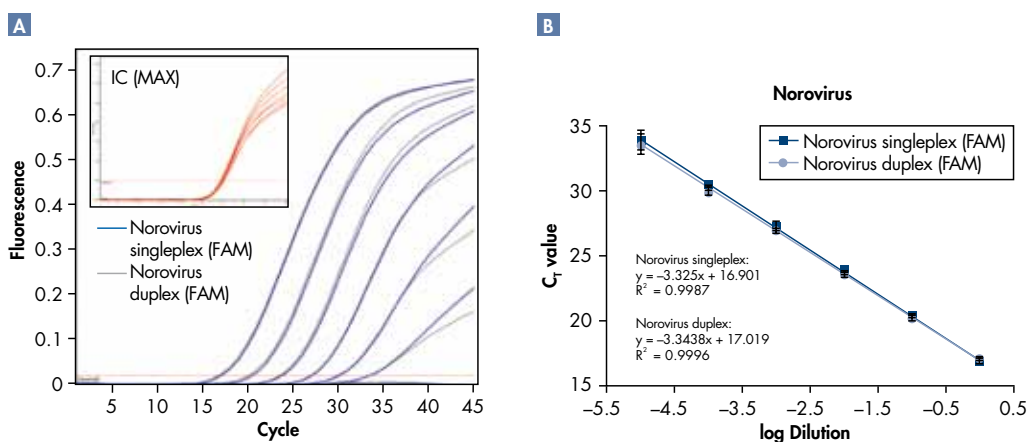


Figure 11. Sensitive and precise detection of Norovirus on the Rotor-Gene Q. **A** Norovirus transcript was serially diluted and detected by either singleplex real-time RT-PCR or by duplex real-time RT-PCR in parallel with the QIAGEN international control. Real-time RT-PCR was carried out using the QuantiFast Pathogen +IC RT-PCR Kit on the Rotor-Gene Q without any PCR optimization. The duplex reactions contained a fixed amount of IC template. Each dilution was analyzed in triplicate, one replicate per dilution is shown. **B** A 6-log range of both Norovirus RNA singleplex detection and Norovirus/IC duplex detection shows high precision and linearity. Error bars each represent ± 1 SD of 3 real-time RT-PCR replicates.

Rapid identification of animal pathogens with the Rotor-Gene Q

QIAGEN provides everything you need for pathogen identification and genotyping — reagents, enzymes, and instruments. *cador* real-time PCR reagents are developed for sensitive identification of specific animal pathogens (viral and bacterial) using PCR on the Rotor-Gene Q. For example, *cador* TKP PCR Reagent contains reagents and enzymes for simultaneous multiplex amplification of highly conserved regions of *Taylorella equigenitalis*, *Klebsiella pneumoniae*, and *Pseudomonas aeruginosa* genomes. The amplicons are detected in one tube by measuring the green, orange, and crimson fluorescence on a Rotor-Gene Q. An internal control is included in the same tube, to monitor DNA extraction and/or the presence of PCR inhibitors. QIAGEN is one of the few companies with a worldwide PCR license for animal testing, without additional licensing costs for the user.

Complete workflow solutions for food safety testing

The *mericon*[™] food testing portfolio is a complete system of sample preparation and assay kits that meet the increasing demands of food research and monitoring. The assays, with detection by real-time PCR, enable sensitive and accurate detection of a broad range of pathogens, genetically-modified organisms, and plant and animal matter in food, animal feed, or pharmaceutical products. The entire workflow for food safety testing using *mericon* sample preparation kits and *mericon* PCR Assays has been validated. *mericon* PCR Assays perform optimally on the Rotor-Gene Q (Figure 12).

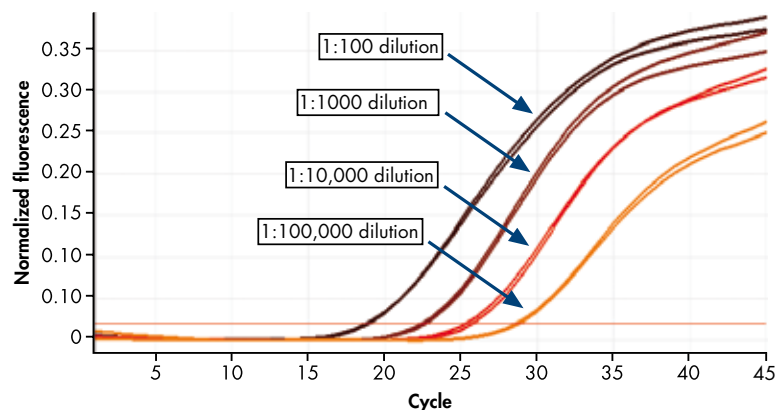


Figure 12. Highly sensitive pathogen detection, even in difficult food matrices such as peanut butter. Peanut butter was homogenized in buffered peptone water, spiked with < 5 cfu of Salmonella, and enriched for 20 h at 37°C. DNA was extracted from serially diluted samples of the enrichment culture using the *mericon* DNA Bacteria Kit and then tested with the *mericon* Salmonella Kit on the Rotor-Gene Q. Although the original inoculation was small, Salmonella was still reliably detected at a dilution factor of 1:100,000.

Beyond pathogen detection — pathogen typing using HRM technology

In pathogen research, categorization of various pathogen subtypes is often required. This pathogen typing enables identification of different strains, for instance drug-resistant mutations or highly pathogenic variants. The resolution and flexibility of HRM in combination with the Type-it HRM PCR Kit on the Rotor-Gene Q, makes it the method of choice for pathogen typing in many application areas (Figure 13).

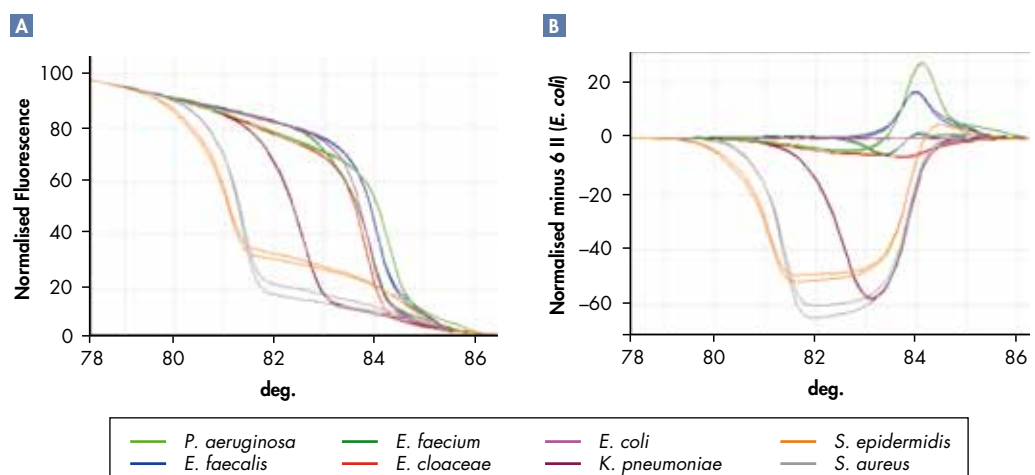


Figure 13. Pathogen typing using robust HRM detection. HRM primers were designed to recognize and differentiate the 16S ribosomal DNA of 8 different bacterial strains. Microbial DNA (10 pg) from each strain was used as template and amplified using the Type-it HRM PCR Kit. PCR products were sequenced to confirm the results and the robustness of the HRM detection method for this application.

Genotyping

The analysis of differences in DNA between individuals has become increasingly important in all areas of biological and medical research. The term “genotyping” is used as a synonym for a wide range of applications associated with human, animal, plant, microbial, or viral samples. QIAGEN has developed highly specific and accurate PCR solutions and versatile detection methods to address the requirements of genotyping studies for accuracy, speed, reliability, and standardization.

PCR-based genotyping analysis

The Type-it Fast SNP Probe PCR Kit provides accurate SNP genotyping using the Rotor-Gene Q, even for difficult templates or SNPs and low template amounts. Outstanding separation and tight allele clustering, together with the allelic discrimination or scatter plot analysis functions of the Rotor-Gene Q software, ensure high call rates and accurate, reproducible, and reliable genotyping results (Figure 14). The kit is functionally validated with commercially available SNP genotyping assays and is compatible with TaqMan MGB probes as well as custom assays consisting of TaqMan MGB, TaqMan, or other dual-labeled probes.

Accurate genotyping with the Type-it HRM PCR Kit

The optimized Type-it HRM PCR Kit ensures accurate resolution of sequence variations and is an unmatched tool for unambiguous allelic discrimination using HRM technology. Together with the Rotor-Gene Q, the Type-it HRM PCR Kit requires no optimization in the development of new HRM assays. Due to the unique master mix chemistry and optimized HRM buffer, specific amplification products and reliable results are consistently ensured, even when analyzing Class IV SNPs (Figures 3 and 4). Unlike HRM kits from other suppliers, the unique features of the Type-it HRM PCR Kit enable amplification of the most challenging subtle sequence differences, even in difficult gene mutations in cancer-related genes (Figure 15).

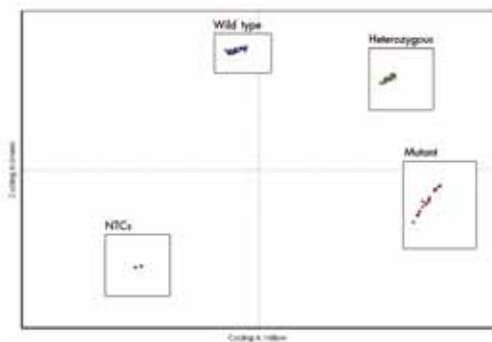


Figure 14. Reliable SNP genotyping even with low template amounts. Allelic discrimination plot analysis was performed with a panel of 70 different genomic DNAs (1 ng each) using the Type-it Fast SNP Probe PCR Kit. PCR was performed on the Rotor-Gene Q with a TaqMan SNP genotyping assay for rs 951134 and two no template controls (NTCs). **Black:** NTCs. **Green:** heterozygous samples. **Red:** homozygous for VIC fluorescence (A allele). Even using low amounts of template, tight clustering and reliable genotyping results were observed.

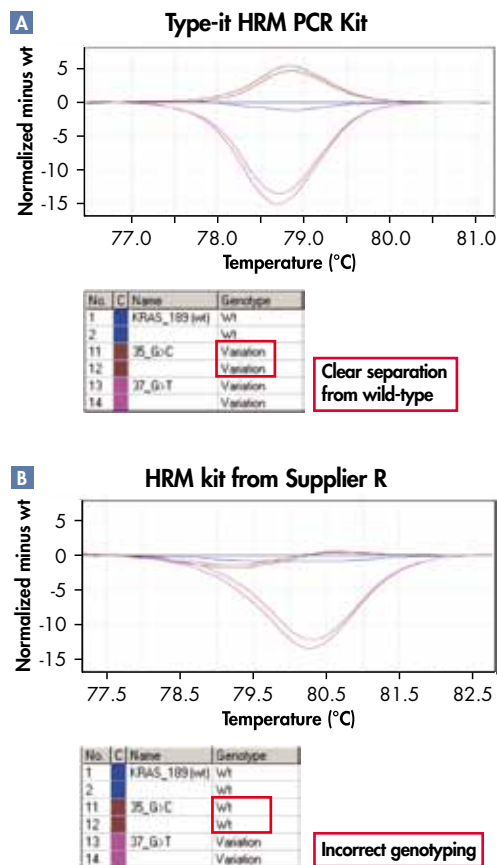


Figure 15. Successful typing of gene mutations in the human KRAS gene using the Type-it HRM PCR Kit.

A Difference plot showing reliable discrimination between the wild-type sequence (blue), the c.35 G>C mutation (brown), and the c.37 G>T mutation (pink). Reproducible discrimination with high confidence was obtained without the need for optimization. **B** The c.35 G>C mutation could not be resolved from the wild-type even after extensive optimization of Mg²⁺ concentration and cycling parameters when using the HRM master mix from Supplier R. The mutation affects the amino acid in position 12, resulting in p.G12A and in position 13, resulting in p.G13C.

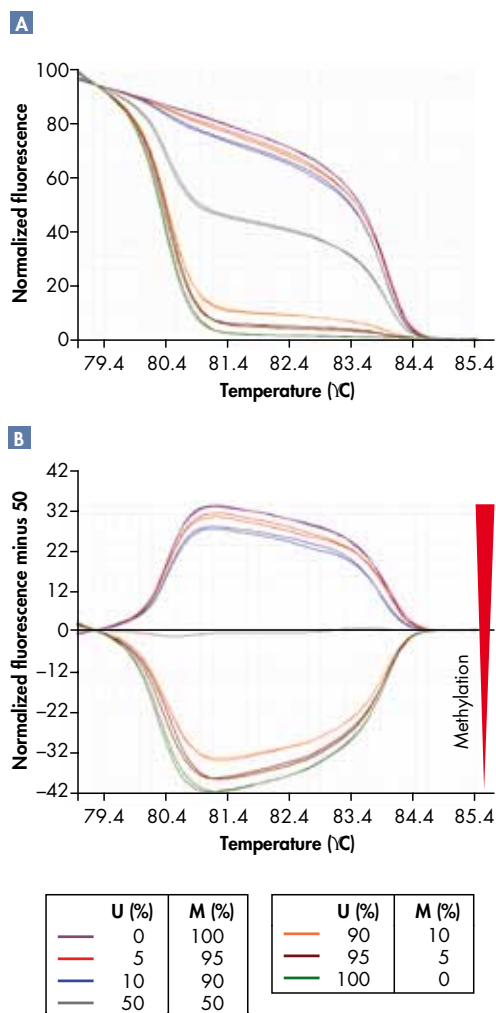


Figure 16. Highly sensitive results — detection of even low percentages of methylated DNA. Mixtures of methylated and unmethylated DNA of varying ratios were used as template. A CpG island from the promoter region of the APC gene (adenomatosis polyposis coli) was amplified and the degree of methylation was determined by HRM methylation analysis on the Rotor-Gene Q using the EpiTect HRM PCR Kit. **A** A standard normalized melt curve and **B** a difference plot normalized to the 50% methylated sample are shown.

DNA methylation analysis

EpiTect HRM PCR Kit — for reliable screening of changes in methylation status by HRM analysis

The EpiTect HRM PCR Kit uses high-resolution melting (HRM) technology for fast screening and accurate detection of changes in the CpG methylation status of bisulfite-converted DNA.

The EpiTect HRM PCR Kit offers:

- Highly specific PCR amplification without the need for optimization
- Distinct melting curves due to EvaGreen fluorescent dye
- Convenient master mix format and optimized protocol
- Fast and easy development of new HRM methylation assays

For CpG methylation analysis by HRM, the DNA has to undergo complete bisulfite conversion before the melting behavior of DNA can be measured by HRM analysis. Unknown samples can be compared to a standard control based on their melting characteristics. The sensitivity ensured by the EpiTect HRM PCR Kit together with the Rotor-Gene Q means that even low amounts of methylated DNA can be detected (Figure 16).

EpiTect MethyLight PCR Kits — for quantitative, real-time probe-based PCR analysis of methylation status

Once methylation sites have been identified using HRM, probe-based techniques can be used for sensitive quantification of CpG sites. Using the EpiTect MethyLight PCR Kit with the Rotor-Gene Q allows sensitive and reliable analysis of methylation status using TaqMan or other dual-labeled probes. Highly accurate quantitative methylation analysis is achieved when the kit is used together with probe-based Methylation assays (such as EpiTect MethyLight Assays). EpiTect MethyLight Assays consist of PCR primers and 2 probes — one methylation-specific, the other nonmethylation-specific — which can be used in a single reaction to simultaneously detect methylated and unmethylated sites (Table 5).

Table 5. Sensitive detection of small changes in methylation

Defined experimental methylation degree	Mean $C_{T(FCQ)}$ value (FAM probe)	Mean $C_{T(TG)}$ value (VIC probe)	Calculated methylation degree in % per sample
0% methylation	45	30.37	0.004
10% methylation	34.62	30.72	6.278
50% methylation	31.27	31.67	56.887
90% methylation	30.52	33.43	88.258
100% methylation	30.05	45	99.997

Ordering Information

Product	Contents	Cat. no.
Rotor-Gene Q 2plex	Real-time PCR cyclers with 2 channels (green, yellow), laptop computer, software, accessories, 1-year warranty on parts and labor, optional installation and training	Inquire
Rotor-Gene Q 2plex HRM	Real-time PCR cycler and HRM instrument with 2 channels (green, yellow) plus HRM channel, laptop computer, software, accessories, 1-year warranty on parts and labor, optional installation and training	Inquire
Rotor-Gene Q 5plex	Real-time PCR cycler with 5 channels (green, yellow, orange, red, crimson), laptop computer, software, accessories, 1-year warranty on parts and labor, optional installation and training	Inquire
Rotor-Gene Q 5plex HRM	Real-time PCR cycler and HRM instrument with 5 channels (green, yellow, orange, red, crimson) plus HRM channel, laptop computer, software, accessories, 1-year warranty on parts and labor, optional installation and training	Inquire
Rotor-Gene Q 6plex	Real-time PCR cycler with six channels (blue, green, yellow, orange, red, crimson), laptop computer, software, accessories, 1-year warranty on parts and labor, optional installation and training	Inquire
Warranty PLUS 1 Basic, Rotor-Gene Q	2-year warranty, all labor, travel, and parts 9241779	
Rotor-Disc 100 Starter Kit	Kit includes: 2 Rotor-Disc 100 packs, Rotor-Disc Heat Sealer, Rotor-Disc Heat Sealing Film, Rotor-Disc 100 Rotor and Locking Ring, Rotor-Disc 100 Loading Block, Rotor-Disc Pipetting Aid	Inquire
Rotor-Disc 100 (30)	Pack of 30 individually wrapped discs for 3000 reactions	981311
Rotor-Disc 72 Starter Kit	Kit includes: 3 Rotor-Disc 72 packs, Rotor-Disc Heat Sealer, Rotor-Disc Heat Sealing Film, Rotor-Disc 72 Rotor and Locking Ring, Rotor-Disc 72 Loading Block, Rotor-Disc Pipetting Aid	Inquire
Rotor-Gene Probe PCR Kit (400)*	For 400 x 25 µl reactions: 2x Master Mix, RNase-Free Water	204374
Rotor-Gene Probe RT-PCR Kit (400)	For 400 x 25 µl reactions: 2x Master Mix, RT Mix, RNase-Free Water	204574
QuantiFast Probe Assay (400)*	For 400 x 25 µl reactions: dual-labeled, probe-based, predesigned 20x lyophilized assays; includes master mix and reagents for real-time one-step or two-step RT-PCR	Varies
Rotor-Gene Multiplex PCR Kit (400)*	For 400 x 25 µl reactions: 2x Master Mix, RNase-Free Water	204774
Rotor-Gene Multiplex RT-PCR Kit (400)*	For 400 x 25 µl reactions: 3 x 1.7 ml 2x Rotor-Gene Multiplex RT-PCR Master Mix, 100 µl Rotor-Gene RT Mix, 2 x 2 ml RNase-Free Water	204974
QuantiTect Primer Assay (200)*	For 200 x 50 µl reactions: 10x QuantiTect Primer Assay (lyophilized)	Varies

* Various kit sizes available; please inquire.

Ordering Information

Product	Contents	Cat. no.
QuantiTect Reverse Transcription Kit (50)*	For 50 x 20 µl reactions: Buffers, Quantiscript® Reverse Transcriptase, RT Primer Mix, RNase-Free Water	205311
miScript SYBR Green PCR Kit (200)*†	For 200 x 50 µl reactions: 2x Master Mix, Universal Primer, RNase-Free Water	218073
QuantiTect Virus +ROX Vial Kit (200)*	For 200 x 50 µl reactions: 5x Master Mix, RT Mix, RNase-Free Water, Nucleic Acid Dilution Buffer	211033
QuantiFast Pathogen PCR +IC Kit (400)*	For 400 x 25 µl reactions: Master Mix, lyophilized Internal Control Assay, lyophilized Internal Control DNA, ROX Dye Solution, High-ROX Dye Solution, RNase-Free Water, Nucleic Acid Dilution Buffer, Buffer TE	211354
QuantiFast Pathogen RT-PCR +IC Kit (400)*	For 400 x 25 µl reactions: Master Mix, RT Mix, lyophilized Internal Control Assay, lyophilized Internal Control RNA, ROX Dye Solution, High-ROX Dye Solution, RNase-Free Water, Nucleic Acid Dilution Buffer, Buffer TE	211454
Type-it Fast SNP Probe PCR Kit (800)*	For 800 x 25 µl reactions: 2x Master Mix, RNase-Free Water, Q-Solution®	206045
EpiTect MethyLight PCR Kit (200)*	For 200 x 50 µl reactions: 2x Master Mix, RNase-Free Water	59436
EpiTect HRM PCR Kit (100)	For 100 x 25 µl reactions: 2x Master Mix, RNase-Free Water	59445
Type-it HRM PCR Kit (100)	For 100 x 25 µl reactions: 2x Master Mix, RNase-Free Water	206542
Pathway-Powered RT ² Profiler PCR Arrays	PCR Array includes SYBR Green-optimized primer assays for a panel of relevant pathway- or disease-focused genes	330231
Custom RT ² Profiler PCR Arrays	Custom PCR Arrays containing any set of human, mouse, rat, dog, rhesus macaque, or fruit fly genes	330131
RT ² SYBR Green ROX FAST Mastermix	For 200 x 20 µl reactions: 2x SYBR Green ROX FAST qPCR Mastermix, HotStart DNA Taq Polymerase, dNTP mix, dyes	330520

* Various kit sizes available; please inquire. † The kit is part of the miScript PCR System; for details, visit www.qiagen.com/miRNA.

For up-to-date licensing information and product-specific disclaimers, see the respective QIAGEN kit handbook or user manual. QIAGEN kit handbooks and user manuals are available at www.qiagen.com or can be requested from QIAGEN Technical Services or your local distributor.

Discover more about the Rotor-Gene Q at www.qiagen.com/pure-detection



Trademarks: QIAGEN®, QIAgility™, QIASymphony®, EpiTect®, GeneGlobe®, HotStarTaq®, HRM®, Q.Solution®, Quantiscript®, QuantiTect®, Rotor-Disc®, Rotor-Gene®, ScreenClust™, Type-it™ (QIAGEN Group); Alexa Fluor®, Marina Blue®, SYBR®, SYTO®, Texas Red® (Molecular Probes, Inc.); CAL Fluor® (Biosearch Technologies, Inc.); Cy® (GE Healthcare); EvaGreen® (Biotium, Inc.); FAM™, JOE™, ROX™, TET™, VIC® (Applied Biosystems or its subsidiaries); LC Green® (Idaho Technology, Inc.); LightCycler®, TaqMan® (Roche Group); Quasar® (Biosearch Technologies, Inc.); Yakima Yellow® (Nanogen, Inc.). MAX™ (Integrated DNA Technologies, Inc.)

For HRM versions only: Hi-Res Melting™ Mark under license from Idaho Technology, Inc. for applicable countries.

For applicable countries:

The purchase of this product includes a limited, non-transferable license to one or more of U.S. Patent Nos. 6,787,338; 7,238,321; 7,081,226; 6,174,670; 6,245,514; 6,569,627; 6,303,305; 6,503,720; 5,871,908; 6,691,041; 7,387,887; U.S. Patent Application Nos. 2003/0224434, and 2006-0019253, and all continuations and divisionals, and corresponding claims in patents and patent applications outside the United States, owned by the University of Utah Research Foundation, Idaho Technology, Inc., Evotec Biosystems GmbH, and/or Roche Diagnostics GmbH, for internal research use or for non-in vitro diagnostics applications. No right is conveyed, expressly, by implication or estoppel, for any reagent or kit, or under any other patent or patent claims owned by the University of Utah Research Foundation, Idaho Technology, Inc., and/or Roche Diagnostics GmbH, or by any other Party. For information on purchasing licenses for in-vitro diagnostics applications or reagents contact Roche Molecular Systems, 4300 Hacienda Drive, Pleasanton, CA 94588, USA.

For applicable countries:

This real-time thermal cycler is licensed under U.S. Patent No. 6,814,934 and corresponding claims in any foreign counterpart patent thereof owned by Applied Biosystems LLC, in all fields, including research and development, all applied fields, and human and animal in-vitro diagnostics. No rights are conveyed expressly, by implication or estoppel to any patents on real-time methods, including but not limited to 5' nuclease assays, or to any patent claiming a reagent or kit. For further information on purchasing additional rights, contact the Director of Licensing at Applied Biosystems, 850 Lincoln Centre Drive, Foster City, California, 94404, USA.

Purchase of this product (Rotor-Gene SYBR Green Kits and miScript SYBR Green PCR Kit) is accompanied by a limited, non-transferable immunity from suit to use it with detection by a dsDNA-binding dye as described in U.S. Patents Nos. 5,994,056 and 6,171,785 and corresponding patent claims outside the United States for the purchaser's own internal research. No real-time apparatus or system patent rights or any other patent rights, and no right to use this product for any other purpose is hereby granted expressly, by implication or by estoppel.

For all kits propagating melting curve analysis: The purchase of this product includes a limited, non-transferable license under U.S. Patent No. 5,871,908 and all continuations and divisionals, and corresponding claims in patents and patent applications outside the United States, owned by Roche Diagnostics GmbH, for internal research use or for non-in vitro diagnostics applications with authorized reagents with regard to Melting Curve Analysis. No right is conveyed, expressly, by implication or estoppel, under any other patent or patent claims owned by Roche Diagnostics GmbH, or by any other Party.

This product (Rotor-Gene Probe Kits, Rotor-Gene Multiplex PCR Kit, QuantiTect Virus +ROX Vial Kit, Type-it Fast SNP Probe PCR Kit, and EpiTect MethylLight PCR +ROX Vial Kit) is an Authorized 5' Nuclease Core Kit without Licensed Probe. Its purchase price includes a limited, non-transferable immunity from suit under certain patents owned by Roche Molecular Systems, Inc. or F. Hoffmann-La Roche Ltd, for using only this amount of the product in the practice of the 5' nuclease process solely for the purchaser's own internal research when used in conjunction with Licensed Probe. No right under any other patent claims (such as apparatus or system claims) and no right to use this product for any other purpose is hereby granted expressly, by implication or by estoppel. Further information on purchasing licenses may be obtained by contacting the Director of Licensing, Applied Biosystems, 850 Lincoln Centre Drive, Foster City, California 94404, USA.

The use of this product (miScript SYBR Green PCR Kit) is covered by at least one claim of U.S. Patent No. 7,687,247 owned by Life Technologies Corporation. The purchase of this product conveys to the buyer the non-transferable right to use the purchased amount of the product and components of the product in research conducted by the buyer (whether the buyer is an academic or for-profit entity). The buyer cannot sell or otherwise transfer (a) this product, (b) its components, or (c) materials made by the employment of this product or its components to a third party or otherwise use this product or its components or materials made by the employment of this product or its components for Commercial Purposes. Commercial Purposes means any activity for which a party receives or is due to receive consideration and may include, but is not limited to: (1) use of the product or its components in manufacturing; (2) use of the product or its components to provide a service, information, or data; (3) use of the product or its components for therapeutic, diagnostic or prophylactic purposes; or (4) resale of the product or its components, whether or not such product or its components are resold for use in research. The buyer cannot use this product or its components or materials made using this product or its components for therapeutic, diagnostic or prophylactic purposes. Further information on purchasing licenses under the above patents may be obtained by contacting the Licensing Department: Life Technologies Corporation, 5791 Van Allen Way, Carlsbad, CA 92008. Email: outlicensing@lifetech.com

Use of this product (RT² Profiler PCR Arrays) is covered by one or more of the following US patents and corresponding patent claims outside the US: 5,994,056 and 6,171,785. The purchase of this product includes a limited, non-transferable immunity from suit under the foregoing patent claims for using only this amount of product for the purchaser's own internal research. No right under any other patent claim and no right to perform commercial services of any kind, including without limitation reporting the results of purchaser's activities for a fee or other commercial consideration, is conveyed expressly, by implication, or by estoppel. This product is for research use only. Diagnostic uses under Roche patents require a separate license from Roche. Further information on purchasing licenses may be obtained by contacting the Director of Licensing, Applied Biosystems, 850 Lincoln Centre Drive, Foster City, California 94404, USA.

This product (RT² Profiler PCR Arrays) is provided under an agreement between Molecular Probes, Inc. and SABiosciences and the manufacture, use, sale, or import of this product is subject to one or more of U.S. Patent Nos. 5,436,134; 5,658,751 and corresponding international equivalents, owned by Invitrogen Corp. The purchase of this product conveys to the buyer the non-transferable right to use the purchased amount of the product and components of the product in research conducted by the buyer, where such research does not include testing, analysis or screening services for any third party in return for compensation on a per test basis. The buyer cannot sell or otherwise transfer (a) this product (b) its components or (c) materials made using this product or its components to a third party or otherwise use this product or its components or materials made using this product or its components for Commercial Purposes. Commercial Purposes means any activity by a party for consideration and may include, but is not limited to: (1) use of the product or its components in manufacturing; (2) use of the product or its components to provide a service, information, or data; (3) use of the product or its components for therapeutic, diagnostic or prophylactic purposes; or (4) resale of the product or its components, whether or not such product or its components are resold for use in research. For information on purchasing a license to this product for purposes other than research, contact Molecular Probes, Inc., Business Development, 29851 Willow Creek Road, Eugene, OR 97402 Tel: (541) 465-8300, Fax: (541) 335-0504.

The purchase of this product (RT² Profiler PCR Arrays, Rotor-Gene SYBR Green Kits, miScript SYBR Green PCR Kit) includes a limited, non-transferable license under specific claims of U.S. Patent Nos. 6,174,670, 6,569,627 and 5,871,908, owned by the University of Utah Research Foundation or Evotec Biosystems GmbH and licensed to Idaho Technology, Inc. and Roche Diagnostics GmbH, to use only the enclosed amount of product according to the specified protocols. No right is conveyed, expressly, by implication, or by estoppel, to use any instrument or system under any claim of U.S. Patent Nos. 6,174,670, 6,569,627 and 5,871,908, other than for the amount of product contained herein.

The purchase of this product (QuantiTect Virus +ROX Vial Kit, RT² SYBR Green ROX FAST Mastermix) includes a limited, non-transferable right to use the purchased amount of the product to perform Applied Biosystems' patented Passive Reference Method for the purchaser's own internal research. No right under any other patent claim and no right to perform commercial services of any kind, including without limitation reporting the results of purchaser's activities for a fee or other commercial consideration, is conveyed expressly, by implication, or by estoppel. This product is for research use only. For information on obtaining additional rights, please contact outlicensing@lifetech.com or Out Licensing, Life Technologies, 5791 Van Allen Way, Carlsbad, California 92008.

RESEARCH USE ONLY: A license under U.S. Patents 5,786,146, 6,017,704, 6,265,171 and 6,200,756 or their foreign counterparts is required to practice MSP, Methylation-Specific PCR. The purchase price of this product (EpiTect MethylLight PCR Kit) includes limited, non-transferable rights to use only this amount of the product to practice MSP solely for the internal research activities of the purchaser. To obtain rights to practice MSP in any in vitro diagnostic application or to perform or offer commercial services of any kind using MSP, contact OncoMethylome Sciences.

Certain specific embodiments of the process of multiplex PCR may be covered by patents of third parties in certain countries and may require a license.

© 2009–2010 QIAGEN, all rights reserved.

www.qiagen.com

Australia = Orders 1-800-243-800 = Fax 03-9840-9888 = Technical 1-800-243-066

Austria = Orders 0800-28-10-10 = Fax 0800-28-10-19 = Technical 0800-28-10-11

Belgium = Orders 0800-79612 = Fax 0800-79611 = Technical 0800-79556

Brazil = Orders 0800-557779 = Fax 55-11-5079-4001 = Technical 0800-557779

Canada = Orders 800-572-9613 = Fax 800-713-5951 = Technical 800-DNA-PREP (800-362-7737)

China = Orders 86-21-3865-3865 = Fax 86-21-3865-3965 = Technical 800-988-0325

Denmark = Orders 80-885945 = Fax 80-885944 = Technical 80-885942

Finland = Orders 0800-914416 = Fax 0800-914415 = Technical 0800-914413

France = Orders 01-60-920-920 = Fax 01-60-920-925 = Technical 01-60-920-930

Germany = Orders 02103-29-12000 = Fax 02103-29-22000 = Technical 02103-29-12400

Hong Kong = Orders 800 933 965 = Fax 800 930 439 = Technical 800 930 425

Ireland = Orders 1800 555 049 = Fax 1800 555 048 = Technical 1800 555 061

Italy = Orders 800-789 544 = Fax 02-334304-826 = Technical 800-787980

Japan = Telephone 03-6890-7300 = Fax 03-5547-0818 = Technical 03-6890-7300

Korea (South) = Orders 080-000-7146 = Fax 02-2626-5703 = Technical 080-000-7145

Luxembourg = Orders 8002-2076 = Fax 8002-2073 = Technical 8002-2067

Mexico = Orders 01-800-7742-639 = Fax 01-800-1122-330 = Technical 01-800-7742-436

The Netherlands = Orders 0800-0229592 = Fax 0800-0229593 = Technical 0800-0229602

Norway = Orders 800-18859 = Fax 800-18817 = Technical 800-18712

Singapore = Orders 1800-742-4362 = Fax 65-6854-8184 = Technical 1800-742-4368

Spain = Orders 91-630-7050 = Fax 91-630-5145 = Technical 91-630-7050

Sweden = Orders 020-790282 = Fax 020-790582 = Technical 020-798328

Switzerland = Orders 055-254-22-11 = Fax 055-254-22-13 = Technical 055-254-22-12






UK = Orders 01293-422-911 = Fax 01293-422-922 = Technical 01293-422-999

USA = Orders 800-426-8157 = Fax 800-718-2056 = Technical 800-DNA-PREP (800-362-7737)








Rotor-Gene® Q accessories

Accessories that can be used with the Rotor-Gene® Q are listed below.

Product	Contents	Cat. no.
36-Well Rotor 	For holding PCR Tubes, 0.2 ml; requires 36-Well Rotor Locking Ring	9018907
36-Well Rotor Locking Ring 	For locking PCR Tubes, 0.2 ml, in the 36-Well Rotor	9018906
72-Well Rotor 	For holding Strip Tubes and Caps, 0.1 ml; requires Locking Ring 72-Well Rotor	9018903
Locking Ring 72-Well Rotor 	For locking Strip Tubes and Caps, 0.1 ml in the 72-Well Rotor	9018904
Rotor-Disc® 72 Rotor 	For holding Rotor-Disc 72 discs in the Rotor-Gene Q; requires Rotor-Disc 72 Locking Ring	9018899



Rotor-Disc 72 Locking Ring	For locking a Rotor-Disc 72 in the Rotor-Disc 72 Rotor	9018900
		
Rotor-Disc 100 Rotor	For holding Rotor-Disc 100 discs in the Rotor-Gene Q; requires Rotor-Disc 100 Locking Ring	9018895
		
Rotor-Disc 100 Locking Ring	For locking a Rotor-Disc 100 in the Rotor-Disc 100 Rotor	9018896
		
Rotor-Disc Pipetting Aid	Aid for marking well during manual reaction setup on a Rotor-Disc Loading Block	9018897
		
Rotor-Disc 72 Starter Kit (115V)	3 Rotor-Disc 72 packs, Rotor-Disc Heat Sealer, Rotor-Disc Heat Sealing Film, Rotor-Disc 72 Rotor and Locking Ring, Rotor-Disc 72 Loading Block, Rotor-Disc Pipetting Aid	9001600
Rotor-Disc 72 Starter Kit (230V)	3 Rotor-Disc 72 packs, Rotor-Disc Heat Sealer, Rotor-Disc Heat Sealing Film, Rotor-Disc 72 Rotor and Locking Ring, Rotor-Disc 72 Loading Block, Rotor-Disc Pipetting Aid	9001601
Rotor-Disc 100 Starter Kit (115V)	2 Rotor-Disc 100 packs, Rotor-Disc Heat Sealer, Rotor-Disc Heat Sealing Film, Rotor-Disc 100 Rotor and Locking Ring, Rotor-Disc 100 Loading Block, Rotor-Disc Pipetting Aid	9001602
Rotor-Disc 100 Starter Kit (230V)	2 Rotor-Disc 100 packs, Rotor-Disc Heat Sealer, Rotor-Disc Heat Sealing Film, Rotor-Disc 100 Rotor and Locking Ring, Rotor-Disc 100 Loading Block, Rotor-Disc Pipetting Aid	9001603
Rotor-Disc Heat Sealer 110V	Heat sealing instrument for use with Rotor-Discs; requires Rotor-Disc 72 or 100 Loading Block	9018898
		

Rotor-Disc Heat Sealer 230V



Heat sealing instrument for use with Rotor-Discs; requires Rotor-Disc 72 or 100 Loading Block

9019725

Loading Block 72 x 0.1 ml Tubes



Aluminum block for manual reaction setup with a single-channel pipet in 72 x 0.1 ml tubes

9018901

Loading Block 72 x 0.1 ml Multi-channel



Aluminum block for reaction set-up with multichannel pipets in 72 x 0.1 ml tubes 9018902

Loading Block 96 x 0.2 ml Tubes



Aluminum block for manual reaction set-up in a standard 8 x 12 array using 96 x 0.2 ml tubes

9018905


Rotor Holder



Metal free-standing holder for assembling tubes and Rotor-Discs into rotors

9018908


Rotor-Disc 72 Loading Block



Aluminum block for manual and automated reaction setup in Rotor-Disc 72 discs

9018910

Rotor-Disc 100 Loading Block



Aluminum block for manual and automated reaction setup
in Rotor-Disc 100 discs

9018909

For up-to-date licensing information and product-specific disclaimers, see the respective QIAGEN kit handbook or user manual. QIAGEN kit handbooks and user manuals are available at www.qiagen.com or can be requested from QIAGEN Technical Services or your local distributor.

Trademarks: QIAGEN®, (QIAGEN Group); Rotor-Gene®, Rotor-Disc™ (Corbett Research Pty Ltd).

06/2009 © 2009 QIAGEN, all rights reserved.

www.qiagen.com

Canada ■ 800-572-9613

China ■ 021-3865-3865

Denmark ■ 80-885945

Finland ■ 0800-914416

France ■ 01-60-920-930

Germany ■ 02103-29-12000

Hong Kong ■ 800 933 965

Ireland ■ 1800 555 049

Italy ■ 800-787980

Japan ■ 03-6890-7300

Korea (South) ■ 1544 7145

Luxembourg ■ 8002 2076

Mexico ■ 01-800-7742-639

The Netherlands ■ 0800 0229592

Norway ■ 800-18859

Singapore ■ 65-67775366

Spain ■ 91-630-7050

Sweden ■ 020-790282

Switzerland ■ 055-254-22-11

UK ■ 01293-422-911

USA ■ 800-426-8157

Australia ■ 1-800-243-800

Austria ■ 0800/281010

Belgium ■ 0800-79612





Brazil ■ 0800-557779







Sample & Assay Technologies

Rotor-Gene® Q consumables

Consumables that can be used with the Rotor-Gene® Q are listed below.

Product	Contents	Cat. no.
PCR Tubes, 0.2 ml (1000)	1000 thin-walled tubes for 1000 reactions	981005
		
PCR Tubes, 0.2 ml (10000)	10 x 1000 thin-walled tubes for 1000 reactions	981008
		
Strip Tubes and Caps, 0.1 ml (250)	250 strips of 4 tubes and caps for 1000 reactions	981103
		
Strip Tubes and Caps, 0.1 ml (2500)	10 x 250 strips of 4 tubes and caps for 10,000 reactions	981106
		



Rotor-Disc® 72 (24)	24 individually wrapped discs for 1728 reactions	981301
		
Rotor-Disc 72 (240)	10 x 24 individually wrapped discs for 17,280 reactions	981303
		
Rotor-Disc 100 (30)	30 individually wrapped discs for 3000 reactions	981311
		
Rotor-Disc 100 (300)	10 x 30 individually wrapped discs for 30,000 reactions	981313
		
Rotor-Disc Heat Sealing Film (60)	60 films for sealing Rotor-Disc 100 or Rotor-Disc 72 discs	981601
Rotor-Disc Heat Sealing Film (600)	10 x 60 films for sealing Rotor-Disc 100 or Rotor-Disc 72 discs	981604

For up-to-date licensing information and product-specific disclaimers, see the respective QIAGEN kit handbook or user manual. QIAGEN kit handbooks and user manuals are available at www.qiagen.com or can be requested from QIAGEN Technical Services or your local distributor.

Trademarks: QIAGEN®, (QIAGEN Group); Rotor-Gene®, Rotor-Disc™ (Corbett Research Pty Ltd).

06/2009 © 2009 QIAGEN, all rights reserved.

www.qiagen.com

Canada ■ 800-572-9613

China ■ 0086-21-3865-3865

Denmark ■ 80-885945

Finland ■ 0800-914416

France ■ 01-60-920-930

Germany ■ 02103-29-12000

Hong Kong ■ 800 933 965

Ireland ■ 1800 555 049

Italy ■ 800-787980

Japan ■ 03-6890-7300

Korea (South) ■ 1544 7145

Luxembourg ■ 8002 2076

Mexico ■ 01-800-7742-639

The Netherlands ■ 0800 0229592

Norway ■ 800-18859

Singapore ■ 65-67775366

Spain ■ 91-630-7050

Sweden ■ 020-790282

Switzerland ■ 055-254-22-11

UK ■ 01293-422-911

USA ■ 800-426-8157

Australia ■ 1-800-243-800

Austria ■ 0800/281010

Belgium ■ 0800-79612

Brazil ■ 0800-557779



Sample & Assay Technologies