

PAGINA 0

**CREATA PENTRU A
PUTEA SEMNA
ELECTRONIC
DOCUMENTUL**

Medtronic



Resolute Onyx™ DES

**Different
by design**

Different by design




Best-in-class deliverability

Resolute Onyx DES is made from a single wire, which gives it a **fluid range of motion** and provides the flexibility needed for best-in-class deliverability.¹

Enhanced visibility with thinner struts

The platinum iridium core within Resolute Onyx DES **increases visibility** for accurate stent placement without compromising strut thickness.¹

Cobalt alloy shell




Platinum iridium core



Broadest diameter range

Resolute Onyx is the only DES with **diameters ranging from 2.0 mm to 5.0 mm** to treat a broad range of coronary vessel sizes.

MAXIMUM EXPANSION CAPABILITIES

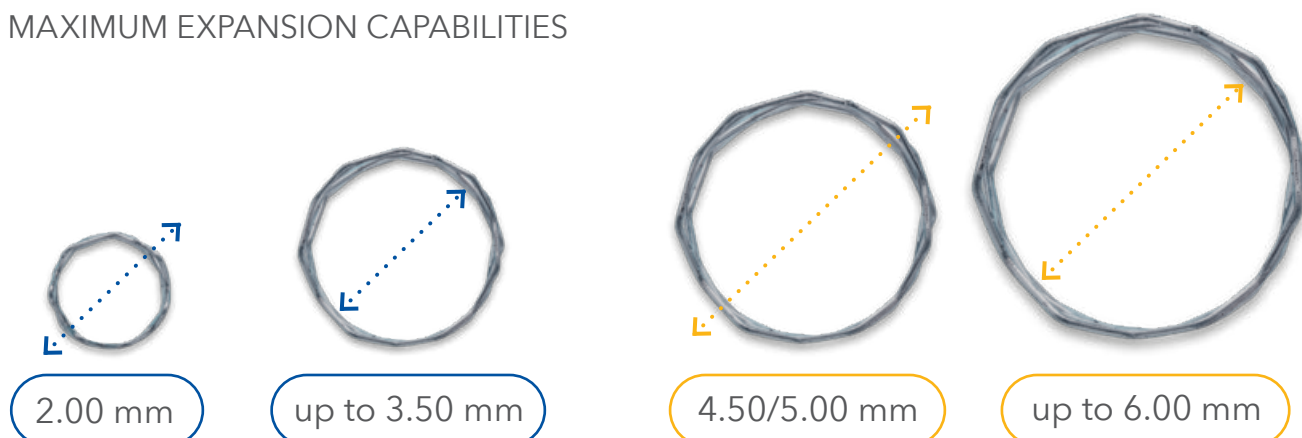

Safe and effective in real-world HBR patients on 1-month DAPT



Fast healing

- Single-wire design provides a fluid range of motion and the conformability needed for **superior strut apposition**¹
- BioLinx™ biocompatible polymer provides **superior thromboresistance**²
- When combined, **fast healing** occurs as evidenced by nearly 90% strut coverage at 30 days,³ providing the foundation for the Onyx One Global Trial

Onyx One Global Trial

- Resolute Onyx DES was safe and effective in real-world high bleeding risk (HBR) patients on 1-month DAPT⁴ with no lesion or vessel limitations
- Randomised trial comparing Resolute Onyx DES to BioFreedom™* DCS

Real-world patient population

Onyx ONE Global Trial						
Onyx ONE Clear Analysis						
1003 1506	53% 49%	33% 36%	39% 39%	80% 79%	38 mm 37 mm	46% 50%
Resolute Onyx DES patients studied	ACS patients included	AF patients included	Diabetic patients included	B2/C lesions	Average stented length	Moderate/severe calcified lesions

Onyx ONE Clear Analysis


Prospective, multicentre, single-arm analysis of ~1500 patients on 1-month DAPT that reinforced safety and efficacy results from the Onyx ONE Global Trial.

1 month DAPT

Resolute Onyx DES was the first DES CE-indicated for 1-month DAPT in HBR patients.


Optimised for complex PCI

Optimised for left main and other extra-large vessels

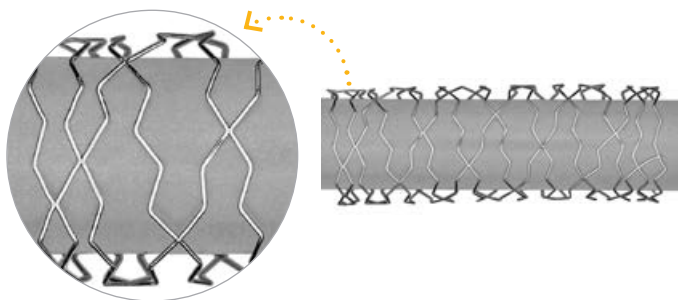

Resolute Onyx DES' 4.5 and 5.0 mm diameters:

- **Expand to 6.0 mm[†]** for optimal deployment with even scaffolding¹
- Provide the **sustained radial strength** needed to handle the left main artery's elasticity¹

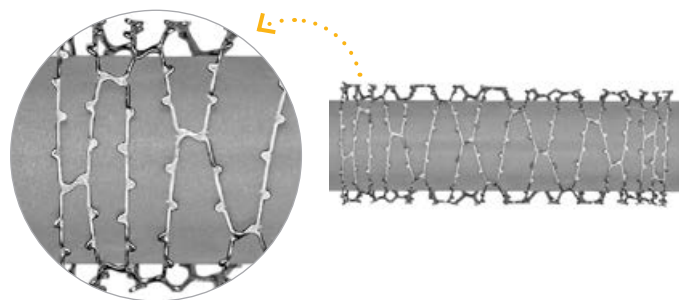

Synergy™* Megatron DES' post-dilatation to 6.0 mm diameter causes the struts to straighten as they approach their expansion limit.




Resolute Onyx is the only DES with randomised data supporting provisional and dual-stent strategies in left main bifurcation PCI (EBC Main Study).

Optimised for bifurcation PCI

- Other DES feature irregular cell shapes which may obstruct wire or catheter advancement through the cell's opening
- Resolute Onyx DES has round struts to **create a smooth passage when accessing the side branch** and lower the propensity to catch¹

CROSS-SECTION OF ACTUAL STENTS



Resolute Onyx DES



Synergy™* DES



Xience Sierra™* DES

Bifurcation education and visualisations from a totally different perspective

Bifurcation exploration website



5 step-by-step techniques using Resolute Onyx DES

View endoscopic imaging captured inside an isolated, reanimated, beating porcine heart. We created this resource with the **European Bifurcation Club** and the **Visible Heart® Lab at the University of Minnesota** to enhance bifurcation procedure skills or to help teach fellows.



Visit and bookmark today

CE mark indications

1-month DAPT in HBR patients
 Diabetes mellitus
 In-stent restenosis (ISR)
 Multivessel disease
 Chronic total occlusions (CTO)
 Acute coronary syndrome (ACS)
 Total occlusions (TO)
 Acute myocardial infarction (AMI)
 Left main (LM)
 Unstable angina (UA)
 Small vessel (SV)
 Bifurcation lesions

Ordering information

Stent diameter (mm)	Maximum expansion capabilities (MSID)	Stent length (mm)								
		8	12	15	18	22	26	30	34	38
2.00	3.50 [†]	RONYX20008X	RONYX20012X	RONYX20015X	RONYX20018X	RONYX20022X	RONYX20026X	RONYX20030X	–	–
2.25	3.50 [†]	RONYX22508X	RONYX22512X	RONYX22515X	RONYX22518X	RONYX22522X	RONYX22526X	RONYX22530X	RONYX22534X	RONYX22538X
2.50	3.50 [†]	RONYX25008X	RONYX25012X	RONYX25015X	RONYX25018X	RONYX25022X	RONYX25026X	RONYX25030X	RONYX25034X	RONYX25038X
2.75	4.00 [‡]	RONYX27508X	RONYX27512X	RONYX27515X	RONYX27518X	RONYX27522X	RONYX27526X	RONYX27530X	RONYX27534X	RONYX27538X
3.00	4.00 [‡]	RONYX30008X	RONYX30012X	RONYX30015X	RONYX30018X	RONYX30022X	RONYX30026X	RONYX30030X	RONYX30034X	RONYX30038X
3.50	5.00 [‡]	RONYX35008X	RONYX35012X	RONYX35015X	RONYX35018X	RONYX35022X	RONYX35026X	RONYX35030X	RONYX35034X	RONYX35038X
4.00	5.00 [‡]	RONYX40008X	RONYX40012X	RONYX40015X	RONYX40018X	RONYX40022X	RONYX40026X	RONYX40030X	RONYX40034X	RONYX40038X
4.50	6.00 [‡]	–	RONYX45012X	RONYX45015X	RONYX45018X	RONYX45022X	RONYX45026X	RONYX45030X	–	–
5.00	6.00 [‡]	–	RONYX50012X	RONYX50015X	RONYX50018X	RONYX50022X	RONYX50026X	RONYX50030X	–	–

* Third party brands are trademarks of their respective owners.

† Resolute Onyx DES received CE and FDA approval for increased expansion in 2020.

‡ Do not postdilute greater than listed value.

1 Based on bench test data on file at Medtronic. May not be indicative of clinical performance.

2 Jinnouchi H, Sato Y, Cheng Q, et al. Thromboresistance and endothelial healing in polymer-coated versus polymer-free drug-eluting stents: Implications for short-term dual anti-platelet therapy. *Int J Cardiol.* March 15, 2021;327:52-57.

3 Roleder T, Kedhi E, Berta B, et al. Short-term stent coverage of second-generation zotarolimus-eluting durable polymer stents: Onyx one-month optical coherence tomography study. *Adv Interv Cardiol.* 2019;15(2):143-150.

4 Windecker S, Latib A, Kedhi E, et al. Polymer-based or Polymer-free Stents in Patients at High Bleeding Risk. *N Engl J Med.* March 2020;382(13):1208-1218.

CE
2797

See the device manual for detailed information regarding the instructions for use, indications, contraindications, warnings, precautions, and potential adverse events.

For further information, contact your local Medtronic representative and/or consult the Medtronic website at medtronic.eu.

For distribution only in markets where the Resolute Onyx coronary stent and the 0.25 mm expansion has been approved. Not for distribution in the USA, Japan, France, Canada, or Australia. 01/2022.

Medtronic

Europe

Medtronic International Trading Sàrl.
 Route du Molliau 31
 Case postale
 CH-1131 Tolochenaz
 Tel. +41 (0)21 802 70 00
 Fax +41 (0)21 802 79 00

United Kingdom/Ireland

Medtronic Limited
 Building 9, Croxley Park
 Hatters Lane, Watford, Herts
 WD18 8WW
www.medtronic.co.uk
 Tel. +44 (0)1923 212213
 Fax +44 (0)1923 241004