

676843

Lot: 830307

Nitroxinil

1. General Information

Formula	C7H3IN2O3	Expiry Date	01 Feb 2030
Mol. Weight	290.01 g/mol	Store at	20°C (in the dark)
CAS-No.	1689-89-0		

2. Batch Analysis

Identity	confirmed by LC-MS		
Overall Purity	99.98 % (g/g)	Expanded Uncertainty	0.34 % (g/g)
Assay Purity (HPLC)	99.99 % (g/g)	Uncertainty	0.17 % (g/g)
Water	<0.01 % (g/g)		

Certified on 07 Feb 2025



by Jacqueline Seidel
RM Release

The overall purity is calculated by: $\text{Purity(\%)} = \frac{\text{Assay purity} \cdot (100 - \text{water content} - \text{impurities})}{100}$
For non-specified hydrates, the overall purity refers to the stated molecular formula.

The reported uncertainties are determined in accordance with ISO 17034 with a 95% confidence level ($k=2$). The Uncertainty is based on the combined uncertainties, including uncertainties of characterization and stability testing. The expiry date is based on the current knowledge and holds only for proper storage conditions in the originally closed flask. If the substance is proven to be unstable under the given storage conditions, you will be contacted immediately. The warranty of this product is limited to the purchasing price of this product and to the first point of use. The indicated long-term storage temperature can vary in a range of ± 4 °C.

Our standards are for laboratory use only and can be used as reference material for calibration of chromatographic systems or related analytical techniques. For handling instructions see the MSDS. A minimum sample of 2 mg is recommended. Deploying less material will increase the uncertainty by a factor 2 for half of sample and 4 for a quarter of sample. The material in the vial can be used multiple times, but it is strongly recommended that all external negative influences to the material are considered and ruled out (e.g. high temperatures, UV-radiation, moisture, oxygen). It is strongly recommended to open the vial at room temperature only and handle the material under inert gas if necessary. The integrity of the purity cannot be guaranteed if the substance is handled under unfavorable conditions.

The balances used are calibrated with weights traceable to the national standards (DKD).

HPC Standards GmbH produces reference materials according to ISO 17034. For further information, check:




HPLC-Method

Article 676843
 Lot-No. 830307
 Column L=250mm, ID=4.6mm; Luna-Omega C18, 100A, 5µm
 Eluent A Acetonitrile
 Eluent B 0.1 % Phosphoric acid (Water)
 Gradient

time	%A	%B
0min	0	100
22.5min	90	10
25min	90	10

Flow 1.0 ml min-1
 Detector UV-220nm
 Injection-Volume 5 µl
 Sample 0.3 mg ml-1 (Acetonitrile)

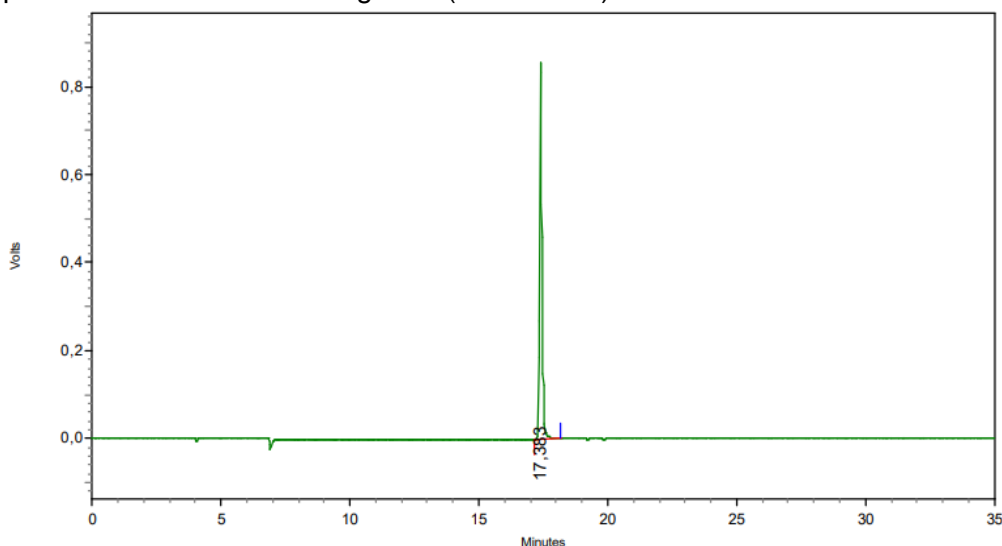

Detector A - 1 (220nm)

Retention Time	Height	Area	Area Percent
17,383	856580	6213657	100,00
Totals			
	856580	6213657	100,00

Exemplary chromatogram of given method.

Version	Article	Lot	Reason for Change	Date
1	676843	830307	Initial Version	07 Feb 2025