


CE Declaration of Conformity

We,
Atlas Medical GmbH
 Head office: Ludwig-Erhard-Ring 3
 15827 Blankenfelde-Mahlow Germany
 Tel: +49(0)33708355030
 Email: info@atlas-medical.com

Middle East Site: Sahab Industrial Zone Area, King Abdullah II Industrial City
 Amman 11512, Jordan
 Tel.: +962 6 4026468
 Fax: +962 6 4022588
 Email: info@atlas-medical.com

Declare our responsibility that the following product:

Product Code	Product Name	Class	GMDN code
8.00.18.0.0005	RPR Carbon Antigen Reagent, 5 ml/vial	General-IVD	32450
8.00.18.2.1000	RPR Carbon Antigen 1000ml/bottle	General-IVD	32450
8.00.18.0.0050	RPR Carbon Antigen Kit, 50 Tests	General-IVD	32450
8.00.18.1.0050	RPR Carbon Antigen Kit, 50 Tests, White Glass Slide.	General-IVD	32450
8.00.18.2.0500	RPR Carbon Antigen Kit, 500 Tests (2ml latex, 2x0.5 ml control) Without card.	General-IVD	32450
8.00.18.3.0500	RPR Carbon Antigen Kit, 500 Tests (10ml latex, 2x0.5 ml control) Without card, stirring sticks.	General-IVD	32450
8.00.18.0.0100	RPR Carbon Antigen Kit, 100 Tests (2ml latex, 2x0.5 ml control)	General-IVD	32450
8.00.18.2.0100	RPR Carbon Antigen Kit, 100 Tests (2ml latex, 2x0.5 ml control +White Glass slide stirring sticks)	General-IVD	32450
8.00.18.0.0025	RPR Carbon Antigen Kit, 25 Tests (0.5ml latex, 2x0.5 ml control)	General-IVD	32450
8.00.18.0.0150	RPR Carbon Antigen Kit, 150 Tests	General-IVD	32450
8.00.18.0.0200	RPR Carbon Antigen Kit, 200 Tests	General-IVD	32450
8.00.18.0.0250	RPR Carbon Antigen Kit, 250 Tests	General-IVD	32450

Atlas Medical	First issue date	Date of review	Management approval	MRXDO10F.10 08.02.2011
	September.2021	06.09.2021		

Amin Al-Habashat
 RA Manager

Declaration Ref No: DC21-0193

8.00.18.0.0500	RPR Carbon Antigen Kit,500 Tests	General-IVD	32450
8.00.18.0.1000	RPR Carbon Antigen Kit, 1000 Tests	General-IVD	32450
8.00.18.4.0500	RPR Carbon Antigen Kit,500 Tests (3x3.4ml reagent,2x1 controls)	General-IVD	32450
8.00.18.5.0500	RPR Carbon Antigen Kit, 500 Tests, (3x3.4ml reagent,2x1 controls)	General-IVD	32450
8.00.18.8.0500	RPR Carbon Antigen 500 Test (10ml reagent) without Control's.	General-IVD	32450
8.00.18.9.0050	RPR Carbon Antigen Kit, (5x10ml Reagent,2x2ml Control) , white glass Slide, Stirring Stick.	General-IVD	32450
8.33.04.0.0001	RPR Positive control	General-IVD	32450
8.33.04.1.0001	RPR Positive control ,Bulk	General-IVD	32450
8.33.04.0.0100	RPR Positive control(100ml/vial)	General-IVD	32450
8.33.04.0.0500	RPR Positive control(500ml/bottle)	General-IVD	32450
8.33.08.0.0001	RPR Negative control	General-IVD	32450

Is produced under Atlas quality system (ISO13485: 2016) supported by GMED certificate:

Certificate N^o.: 36655 rev 1

Expiry Date: October 8th.2023

and complies with the essential requirements of
In Vitro Diagnostic Medical Devices Directive 98/79/EC Annex I
And

EN ISO 18113-1, -2 :2011, EN ISO 15223:2016

EN ISO 14971:2019, EN ISO 23640 :2015 , ISO 2859 :2017,

EN 13612:2002, EN 13641:2002 , EN 13975:2003, ISO 13485:2016

And

Intended for In-Vitro Professional use only.

This Declaration includes the batches produced beyond this day according to the product Lot Log.


Manufacturer

Atlas Medical GmbH

Ludwig-Erhard-Ring 3

15827 Blankenefelde-Mahlow Germany.

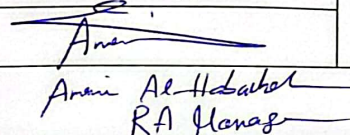

Atlas Medical	First issue date	Date of review	Management approval	MRXDO10F.10 08.02.2011
	September.2021	06.09.2021		

Amir Al-Hadad
RA Manager

Declaration Ref No: DC22-0065

CE Declaration of Conformity

According to Annex III of the IVD Directive 98/79/EC

We,

Atlas Medical GmbH

Head office: Ludwig-Erhard-Ring 3
Blankenfelde-Mahlow, Germany.

Tel: +49 - 33708 – 3550 30

Email: info@atlas-medical.com

Manufacturing Site: Sahab Free Zone Area, P. O. Box 204, Amman 11512, Jordan.

Tel.: +962 6 4026468

Fax: +962 6 4022588

Email: info@atlas-medical.com

Declare our responsibility that the following product:

See Attached list


- Comply with all essential requirements (Annex I) of the IVD Directive 98/79/EC. This compliance has been properly documented and covers the items listed in Annex I of the IVD Directive.
- This product is produced under Atlas quality system (ISO13485:2016) issued by GMED:
Certificate N°: 36655 rev 1
Expiry Date: October 8th.2023
- Comply with the essential requirements of following standards (EN 18113-1, -2,-4:2011, EN ISO 15223:2016 , EN ISO 23640:2015, EN ISO 14971:2019, ISO 2859/1:1999, EN ISO 13612:2002, EN ISO 13641:2002.

And

Intended for In-Vitro Professional use only.

Manufacturer
Atlas Medical
Ludwig-Erhard-Ring 3
Blankenfelde-Mahlow , Germany.



Atlas Medical	Issue date	Date of review	Management approval	MRXDO10F.10 08.02.2011
	May.2022	21.05.2022		

CE Declaration of Conformity

According to Annex III of the IVD Directive 98/79/EC

Item code	Product Description
8.00.01.0.0100	Atlas CRP Latex Kit with Buffer (100 Tests)
8.00.05.0.0100	Atlas RF Latex kit with Buffer(100 Tests)
8.00.11.0.0050	Atlas SLE Latex kit (50 Tests)
8.00.11.0.0100	Atlas SLE Latex kit (100 Tests)
8.00.12.0.0100	Atlas Staphylococcus Latex Kit (100 Tests)
8.00.17.0.0050	Atlas D-Dimer Latex Kit (50 Tests)
8.00.19.3.0100	Atlas TPHA Kit (100 Tests)
8.00.19.3.0200	Atlas TPHA Kit (200 Tests)
8.00.20.3.2500	Atlas VDRL Kit, 5ml+55ml buffer
8.04.38.0.0020	Atlas Fecal Occult Blood Test (FOB) Test Cassette , 20 Tests/Box
8.04.85.0.0050	Atlas Fecal Occult Blood Test (FOB) Test Strip, 50 Tests/Box
8.04.109.0.0020	Atlas Procalcitonin test (PCT) , 20 Tests/Box
8.16.78.0.0025	Atlas Calprotectin Test Cassette , 25 Tests/Box
8.04.45.0.0001	Atlas Troponin I Test Cassette, Bulk
8.04.45.0.0020	Atlas Troponin I Test Cassette , 20 Tests/Box.
8.04.45.0.0030	Atlas Troponin I Test Cassette , 30 Tests/Box.
8.04.46.0.0001	Atlas Myoglobin Test Cassette, Bulk
8.04.46.0.0020	Atlas Myoglobin Test Cassette , 20 Tests/Box.
8.04.46.0.0030	Atlas Myoglobin Test Cassette , 30 Tests/Box.
8.04.47.0.0001	Atlas CK-MB Test Cassette , Bulk.
8.04.47.0.0020	Atlas CK-MB Test Cassette , 20 Tests/Box.
8.04.47.0.0030	Atlas CK-MB Test Cassette , 30 Tests/Box.
8.04.48.0.0001	Atlas Cardiac Triple Tests Cassette (Troponin I, CK-MB, Myoglobin), Bulk.
8.04.48.0.0020	Atlas Cardiac Triple Tests Cassette (Troponin I, CK-MB, Myoglobin), 20 Tests/Box.
8.04.48.0.0030	Atlas Cardiac Triple Tests Cassette (Troponin I, CK-MB, Myoglobin), 30 Tests/Box.
8.14.19.1.0096	Helicobacter pylori Antigen ELISA, 96 Tests.
8.51.00.0.0096	25-OH VITAMIN D Elisa Kit, 96 Tests.
8.57.00.0.0096	Vitamin B12 Elisa Kit, 96 Tests

LA

GMED certifie que le système de management de la qualité développé par
GMED certifies that the quality management system developed by

ATLAS MEDICAL GmbH
Ludwig-Erhard-Ring 3
15827 Blankenfelde-Mahlow GERMANY

pour les activités
for the activities

Conception et développement, fabrication et vente de dispositifs médicaux de diagnostic in vitro .

Design and Development, Manufacturing and Sales of in vitro diagnostic medical devices.

réalisées sur le(s) site(s) de
performed on the location(s) of

Voir addendum

See addendum

est conforme aux exigences des normes internationales
complies with the requirements of the international standards

ISO 13485: 2016

Début de validité / Effective date October 9th, 2020 (included)

Valable jusqu'au / Expiry date : October 8th, 2023 (included)

Etabli le / Issued on : October 8th, 2020




**CERTIFICATION
DE SYSTEMES
DE MANAGEMENT**
Accréditation n°4-0608
Liste des sites accrédités
et portée disponible sur
www.cofrac.fr

GMED N° 36655-1

Ce certificat est délivré selon les règles de certification GMED / This certificate is issued according to the rules of GMED certification

Renouvelle le certificat 36655-0



On behalf of the President
Béatrice LYS
Technical Director

GMED • Société par Actions Simplifiée au capital de 300 000 € • Organisme Notifié/Notified Body n° 0459
Siège social : 1, rue Gaston Boissier - 75015 Paris • Tél. : 01 40 43 37 00 • gmed.fr

Ce certificat couvre les activités et les sites suivants :
This certificate covers the following activities and sites:

French version :

Conception et développement, fabrication et vente de dispositifs médicaux de diagnostic *in vitro* à usage professionnel et/ ou d'autodiagnostic, dans les domaines du groupage sanguin, de la microbiologie, de la biochimie, de la toxicologie, de l'oncologie, de la cardiologie, de l'histologie, de l'endocrinologie et des maladies infectieuses, dans les techniques d'Agglutination/ ELISA/ Tests rapides/ Colorimétrie/ Disques antibiotiques.

English version:

Design and Development, Manufacturing and Sales of in vitro diagnostic medical devices for professional use and/or for self-testing, in the field of Immunohematology, Microbiology, Biochemistry, Toxicology, Oncology, Cardiology, Histology, Endocrinology Biosensors and Infectious diseases, in techniques of Agglutination/ ELISA/ Rapid tests/ Colorimetry/Antibiotic disks.

**ATLAS MEDICAL GmbH
Ludwig-Erhard-Ring 3
15827 Blankenfelde-Mahlow
GERMANY**

French version:

Siège social, responsable de la mise sur le marché

English version:

Headquarter, legal manufacturer

**Sahab Industrial Zone Area
King Abdullah II Industrial City
Amman 11512
JORDAN**

French version:

Conception, fabrication et contrôle final

English version:

Design, manufacture and final control

**William James House
Cowley Road,
Cambridge, CB OWX
United Kingdom**

French version:


Contact réglementaire

English version:

Regulatory Administration

3 sites / 3 sites

DocuSigned by:

Beatrice Lys
EF33BDA9BAA04A3...


**On behalf of the President
Béatrice LYS
Technical Director**



Date: 05/Jan/2023

STATEMENT

We, Atlas Medical having a registered office at Ludwig-Erhard-Ring 3, 15827 Blankenfelde-Mahlow, Berlin, Germany assign SRL Sanmedico having a registered office at A. Corobceanu Street 7A, apt.9, Chisinau MD-2012, Moldova, as authorized representative in correspondence with the conditions of directive 98/79/EEC.

We declare that the company mentioned above is authorized to register, notify, renew or modify the registration of medical devices on the territory of the Republic of Moldova.

On Behalf of Manufacturer:

General Manager

Haya Amawi

Signature: _____

Date: _____

Atlas Medical GmbH
Ludwig - Erhard Ring 3
15827 Blankenfelde - Mahlow
Tel. (0049) 33708 - 355030

Atlas Medical: Ludwig-Erhard-Ring 3, 15827 Blankenfelde-Mahlow, Berlin, Germany,
Tel: +4933708355030

Regulatory Office: William James House, Cowley Rd, Cambridge, CB4 0WX, United Kingdom
Tel: +44 (0) 1223 858 910

Middle East Site: P.O Box 204, King Abdullah II Industrial Estate, Amman, 11512, Jordan
Tel: +962 6 4026468

RPR SYPHILIS CARD TEST

IVD For In-Vitro diagnostic and professional use only

2°C 8°C
Store at 2 to 8 °C

INTRODUCTION

Syphilis is a disease caused by infection with the spirochete *Treponema pallidum*. The infection is systemic and the disease is characterized by periods of latency. These features, together with the fact that *T. pallidum* cannot be isolated in culture, mean that serologic techniques play a major role in the diagnosis and follow-up of treatment for syphilis.

Syphilis is categorized by an early primary infection in which patients may have non-specific symptoms, and potentially, genital lesions. Patients tested by serology during the primary phase may be negative for antibodies, especially if testing is performed during the first 1 to 2 weeks after symptom onset. As the disease progresses into the secondary phase, antibodies to *T. pallidum* reach peak titers, and may persist indefinitely regardless of the disease state or prior therapy. Therefore, detection of antibodies to nontreponemal antigens, such as cardiolipin (a lipoidal antigen released by host cells damaged by *T. pallidum*) may help to differentiate between active and past syphilis infection. Nontreponemal antibodies are detected by the rapid plasma reagin (RPR) assay, which is typically positive during current infection and negative following treatment or during late/latent forms of syphilis.

PRINCIPLE

RPR utilises carbon particles coated with cardiolipin antigen to detect reagin antibodies present in serum or plasma of syphilitic persons.

Specimens that contain reagin cause aggregation of the carbon particles which appear as dark clumps against a white background. The aggregation can be read macroscopically. Non-reactive samples typically appear as a smooth non-aggregated pattern which may form buttons in the centre of the test area.

MATERIALS

MATERIALS PROVIDED

- **RPR carbon antigen reagent:** Contains less than 0.1% sodium azide.
- **Positive Control :** Contains less than 0.1% sodium azide.
- **Negative control:** Contains less than 0.1% sodium azide

- **RPR test cards (Optional).**
- **Plastic sticks.**
- **Package insert.**

NOTE: This package insert is also used for individually packed reagent.

MATERIALS NEEDED BUT NOT PROVIDED

- Rotator (100rpm).
- Timer.
- Pipettes.

SAMPLES

Fresh serum or plasma. The samples with presence of fibrin should be centrifuged before testing. Do not use highly hemolyzed or lipemic samples.

PRECAUTIONS

- For professional in vitro diagnostic use only. Do not use after expiration date.
- Do not eat, drink or smoke in the area where the specimens or kits are handled.
- Always use a fresh pipette tip for every test.
- Handle all negative and positive in the manner as patient specimens .
- Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are assayed.
- The used test should be discarded according to local regulations.
- Components of different human origin have been tested and found to be negative for the presence of antibodies anti- HIV 1+2 and anti-HCV, as well as for HBsAg. However, the controls should be handled cautiously as potentially infectious.

STORAGE AND STABILITY

All components of the kit are stable until the expiration date on the label when stored tightly closed at 2-8°C.

PROCEDURES

QUALITATIVE PROCEDURE

- **Mix well the RPR reagent before use.**
- 1. Bring the reagents and samples to room temperature.
- 2. Dispense **50 µL of each sample** into a separate circle on the card. Use a separate tip for each sample.
- 3. Dispense **1 drop of each of positive and negative controls** into two additional circles.
- 4. Gently shake the dispensing vial and slightly press to remove air bubbles from the needle and the drop obtained is correct.

5. Dispense **1 drop (17.5 µl) of RPR antigen** to each circle next to the sample to be tested.
6. Place the card on a mechanical rotator and rotate at 100 r.p.m. for 8 minutes.
7. Observe macroscopically for agglutination within a minute after removing the card from the rotator.

SEMI-QUANTITATIVE PROCEDURE


- **Mix well the RPR reagent before use.**
- 1. Make doubling dilutions from Undiluted to 1:16 normal saline.
- 2. Place 50 µl of each dilution in to a separate circle on the test card.
- 3. Spread each dilution evenly over the test circle.
- 4. Continue as from Qualitative procedure .
The titer of the sample is expressed as the final dilution which shows aggregation of the carbon particles.

PERFORMANCE CHARACTERISTICS


1. **Sensitivity:** 100%.
2. **Specificity:** 100%.

INTERPRETATION OF TEST RESULTS

1. **Strong Reactive:** Large clumps of carbon particles with a clear background.



2. **Reactive:** Large clumps of carbon particles somewhat more disperse than Strong Reactive pattern.



3. **Weak Reactive:** Small clumps of carbon particles with light grey background.



4. **Trace Reactive:** Slight clumping of carbon particles typically seen as a button of aggregates in the centre of the test circle or dispersed around the edge of the test circle.



5. **Non-Reactive:** Typically a smooth grey pattern or a button of non-aggregated carbon particles in the centre of the test circle.



















REFERENCES

- Falcone V.H., Stout G.W. and Moore M.B. Jr., PHR 79: 491-495, 1964.

 **ATLAS MEDICAL**
Ludwig-Erhard Ring 3
15827 Blankenfelde-Mahlow
Germany
Tel: +49 - 33708 – 3550 30
Email: Info@atlas-medical.com
Website: www.atlas-medical.com


PPI2074A01
Rev B (15.03.2021)

	Catalogue Number		Temperature limit
	<i>In Vitro</i> diagnostic medical device		Caution
	Contains sufficient for <n> tests and Relative size		Consult instructions for use (IFU)
	Batch code		Manufacturer
	Fragile, handle with care		Use-by date
	Manufacturer fax number		Do not use if package is damaged
	Manufacturer telephone number		Date of Manufacture
	Keep away from sunlight		Keep dry

Fecal Occult Blood Test Strip (Feces)

A rapid, one step test for the qualitative detection of human occult blood in feces.

IVD For In-Vitro diagnostic and professional use only



INTENDED USE

The FOB One Step Fecal Occult Blood Test Strip (Feces) is a rapid chromatographic immunoassay for the qualitative detection of human occult blood in feces.

INTRODUCTION

Most of diseases can cause hidden blood in the stool. In the early stages, gastrointestinal problems such as colon cancer, ulcers, polyps, colitis, diverticulitis, and fissures may not show any visible symptoms, only occult blood. Traditional guaiac-based method lacks sensitivity and specificity, and has diet-restriction prior to the testing.

The FOB One Step Fecal Occult Blood Test Strip (Feces) is a rapid test to qualitatively detect low levels of fecal occult blood in feces. The test uses double antibody sandwich assay to selectively detect as low as 50ng/mL of hemoglobin or 6µg hemoglobin/g feces. In addition, unlike the guaiac assays, the accuracy of the test is not affected by the diet of the patients.

PRINCIPLE

The FOB One Step Fecal Occult Blood Test Strip (Feces) is a qualitative, lateral flow immunoassay for the detection of human occult blood in feces. The membrane is pre-coated with anti-hemoglobin antibody on the test line region of the Strip. During testing, the specimen reacts with the particle coated with anti-hemoglobin antibody. The mixture migrates upward on the membrane chromatographically by capillary action to react with anti-hemoglobin antibody on the membrane and

generate a colored line. The presence of this colored line in the test region indicates a positive result, while its absence indicates a negative result. To serve as a procedural control, a colored line will always appear in the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

MATERIALS

MATERIALS PROVIDED

- Test Strip (contains anti-hemoglobin antibody particles and anti-hemoglobin antibody coated on the membrane).
- Specimen collection tube with extraction buffer.
- Package insert.

MATERIALS NEEDED BUT NOT PROVIDED

- Specimen collection container.
- Timer.
- Pipette.

PRECAUTIONS

- For professional *in vitro* diagnostic use only. Do not use after expiration date.
- Do not eat, drink or smoke in the area where the specimens or kits are handled.
- Handle all specimens as if they contain infectious agents. Observe established precautions against microbiological hazards throughout the testing and follow the standard procedures for proper disposal of specimens.
- Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are being tested.
- Humidity and temperature can adversely affect results.

STORAGE AND STABILITY

- The kit can be stored at room temperature or refrigerated (2-30°C).
- The test Strip is stable through the expiration date printed on the sealed pouch.

- The test Strip must remain in the sealed pouch until use.
- Do not freeze.
- Do not use beyond the expiration date.


PATIENT PREPARATION

- Specimen should not be collected during or within three days of a menstrual period, or if the patient suffers from bleeding hemorrhoids or blood in the urine.
- Alcohol, aspirin and other medications taken in excess may cause gastrointestinal irritation resulting in occult bleeding. Such substances should be discontinued at least 48 hours prior to testing.
- Dietary restrictions are not necessary.

PROCEDURE

1. Allow the test strips and samples to reach room temperature (15-30°C) prior to testing. Do not open the package until ready to perform the assay.
2. Using the applicator stick of the provided sample diluent vial, transfer a small portion (5mm diameter) of stool specimen into the sample diluent.
3. Shake gently in order to unstuck and facilitate the sample dispersion.
4. Hold the vial and break the tip off.
5. Dispense 10 drops (approximately 0.5 ml) of the sample extract in a test tube.
6. Immerse the test strip in the liquid prepared in step 5. Do not exceed the line shown on the strip.
7. Read the result 5 minutes after the immersion of the strip. Do not read result after 10 minutes.

INTERPRETATION OF RESULTS (Please refer to the illustration below)

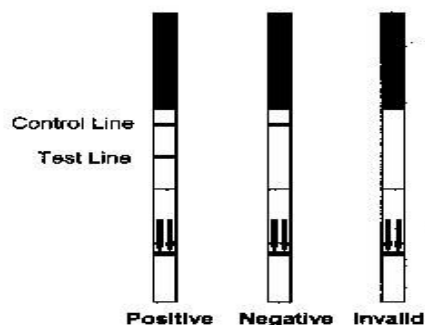

POSITIVE:*

Two distinct red lines appear. One line should be in the control region (C) and another line should be in the test region (T).

*NOTE:

The intensity of the red color in the test line region (T) will vary depending on the concentration of hemoglobin present in the specimen. Therefore, any shade in the test region indicates positive result.

NEGATIVE:

One red line appears in the control region (C). No apparent red or pink line appears in the test region (T).

INVALID:

Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test Strip. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

EXPECTED VALUES

The FOB One Step Fecal Occult Blood Test Strip (Feces) has been compared with another leading commercial rapid test. The correlation between these two systems is 98%.

QUALITY CONTROL

- A procedural control is included in the test. A red line appearing in the control region (C) is the internal procedural control. It confirms

sufficient specimen volume and correct procedural technique.

- Control standards are not supplied with this kit; however it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

LIMITATION

- The FOB One Step Fecal Occult Blood Test Strip (Feces) is for *in vitro* diagnostic use only.
- The FOB One Step Fecal Occult Blood Test Strip (Feces) will only indicate the presence of human hemoglobin in the specimen and the presence of blood in feces may be other than colorectal bleeding.
- As with all diagnostic tests, all results must be considered with other clinical information available to the physician.
- Other clinically available tests are required if questionable results are obtained.

PERFORMANCE CHARACTERISTICS

Sensitivity

The FOB One Step Fecal Occult Blood Test Strip (Feces) can detect the levels of human occult blood as low as 50 ng/mL hemoglobin or around 2µg hemoglobin/g feces.

Specificity

The FOB One Step Fecal Occult Blood Test Strip (Feces) is specific to human hemoglobin. Specimen containing the following substances at the standard concentration were tested on both positive and negative controls with no effect on test results.

Substances	Concentrations (Diluted with the extraction buffer)
Bovine hemoglobin	1 mg/mL
Chicken	1 mg/mL
Pork hemoglobin	1 mg/mL
Goat hemoglobin	1 mg/mL
Horse hemoglobin	1 mg/mL

Rabbit hemoglobin	1 mg/mL
Turkey hemoglobin	1 mg/mL

REFERENCES

- Simon J.B. *Occult Blood Screening for Colorectal Carcinoma: A Critical Review*, Gastroenterology, Vol. 1985; 88: 820.
- Blebea J. and Ncpherson RA. *False-Positive Guaiac Testing With Iodine*, Arch Pathol Lab Med, 1985;109:437-40




ATLAS MEDICAL
William James House, Cowley Rd,
Cambridge, CB4 4WX, UK
Tel: ++44 (0) 1223 858 910
Fax: ++44 (0) 1223 858 524
PPI589A01
Rev C (23.04.2015)

	Product Reference No.		For in-vitro diagnostic use.
	Caution.		Store at 2 - 30°C.
	Read product insert before use.		Number of tests in the pack.
	Lot (batch) number.		Manufacturer.
	Expiry date.		Manufacturer telephone number.
	Manufacturer fax number.		

ANTISTREPTOLYSIN-O (ASO) LATEX SLIDE TEST

For the qualitative and quantitative measurement of antibodies to Antistreptolysin-O in human serum.

IVD For in -vitro diagnostic and professional use only



Store at 2-8°C

INTENDED USE

ATLAS ANTISTREPTOLYSIN-O (ASO) latex slide Test is used for the qualitative and quantitative measurement of antibodies to Antistreptolysin-O in human serum.

INTRODUCTION

The group A β -hemolytic streptococci produces various toxins that can act as antigens. One of these exotoxins streptolysin-O, was discovered by Todd in 1932.

A person infected with group A -hemolytic streptococci produces specific antibodies against these exotoxins, one of which is antistreptolysin-O. The quantity of this antibody in a patient's serum will establish the degree of infection due to the -hemolytic streptococcal.

The usual procedure for the determination of the antistreptolysin titer is based on the inhibitory effect that the patient's serum produces on the hemolytic power of a pre-titrated and reduced streptolysin-O. However, the antigen-antibody reaction occurs independently of the hemolytic activity of streptolysin-O. This property enables the establishment of a qualitative and quantitative test for the determination of the antistreptolysin-O by agglutination of latex particles on slide.

PRINCIPLE

ASO test method is based on an immunologic reaction between streptococcal exotoxins bound to biologically inert latex particles and streptococcal antibodies in the test sample. Visible agglutination occurs when increased antibody level, are present in the test specimen.

MATERIALS

MATERIALS PROVIDED

- ASO Latex Reagent: Latex particles coated with streptolysin O, pH, 8,2. Preservative
- ASO Positive Control(Red cap): Human serum with an ASO concentration > 200 IU/mL.Preservative
- ASO Negative Control (Blue cap) Animal serum. Preservative
- Reaction Slide.
- Stirring Sticks.

MATERIALS REQUIRED BUT NOT PROVIDED

- Timer.
- Test Tubes 12x75mm.
- Test Tube Rack.
- Serological pipettes.
- High intensity light.
- Saline Solution, 0.9% NaCL.

PRECAUTIONS

- All reagents contain 0.1% (w/v) sodium azide as a preservative. Store all reagents at 2-8°C. **DO NOT FREEZE.**
- Reagents containing sodium azide may be combined with copper and lead plumbing to form highly explosive metal azides. Dispose of reagents by flushing with large amounts of water to prevent azide build-up.
- For In Vitro diagnostic use.
- Positive and negative controls prepared using human serum found negative for hepatitis B surface antigen (HBsAg) and HIV-III by FDA required test; however, handle controls as if potentially infectious.

REAGENT STORAGE AND STABILITY

- Reagents are stable until specified expiry date on bottle label when stored refrigerated (2-8°C).
- **DO NOT FREEZE.**
- The ASO Latex Reagent, once shaken must be uniform without visible clumping. When stored refrigerated, a slight sedimentation may occur and should be considered normal.
- Do not use the latex reagent or controls if they become contaminated.

SPECIMEN COLLECTION AND STORAGE

- Use fresh serum collected by centrifuging clotted blood.
- If the test cannot be carried out on the same day, store the specimen for 7 days at 2-8°C and for 3 months at -20°C.

- For longer periods the sample must be frozen.
- As in all serological tests, hemolytic or contaminated serum must not be used.
- **DO NOT USE PLASMA.**

PROCEDURE

Qualitative method

1. Allow the reagents and samples to reach room temperature. The sensitivity of the test may be reduced at low temperatures.
2. Place 50 μ L of the sample and one drop of each Positive and Negative controls into separate circles on the slide test.
3. Mix the ASO-latex reagent vigorously or on a vortex mixer before using and add one drop (50 μ L) next to the sample to be tested.
4. Mix the drops with a stirrer, spreading them over the entire surface of the circle. Use different stirrers for each sample.
5. Place the slide on a mechanical rotator at 80-100 r.p.m. for 2 minutes. False positive results could appear if the test is read later than two minutes.

Semi-quantitative method

1. Make serial two fold dilutions of the sample in 9 g/L saline solution.
2. Proceed for each dilution as in the qualitative method.

QUALITY CONTROL

Positive and Negative Controls should be included in each test batch.


Acceptable performance is indicated when a uniform milky suspension with no agglutination is observed with the ASO Negative Control and agglutination with large aggregates is observed with the ASO Positive Control.

RESULTS

A.QUALITATIVE TEST:

A negative reaction is indicated by a uniform milky suspension with no agglutination as observed with the ASO Negative Control.

A positive reaction is indicated by any observable agglutination in the reaction mixture. The specimen reaction should be compared to the ASO Negative Control (Fig. 1).

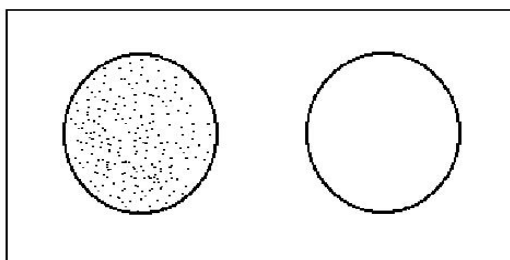

Positive Negative

Figure 1

B. QUANTITATIVE TEST

A positive reaction is indicated by any observable agglutination in the reaction mixture. Record the last dilution showing a positive reaction. Concentration of ASO can be determined by multiplying the last positive dilution factor of the sample with the concentration of the positive control (200 IU/ml).

The titer of the serum is the reciprocal of the highest dilution which exhibits a positive reaction.

IU/ml of sample = conc. of positive control (200) x specimen titer

<u>DILUTION</u>	<u>IU/ml</u>
1:1	200
1:2	400
1:4	800
1:8	1600
Etc.	

REFERENCE VALUES

Up to 200 IU/mL (adults) and 100 IU/mL (children < 5 years old)⁶. Each laboratory should establish its own reference range.

PERFORMANCE CHARACTERISTICS

Analytical sensitivity:

200 (±50) IU/ml.

PROZONE EFFECT

No prozone effect was detected up to 1500 IU/ml.

SENSITIVITY

98%.

SPECIFICITY

97%.

INTERFERENCES

NON INTERFERING SUBSTANCES:

- Hemoglobin (10g/dl)
- Bilirubin (20mg/dl)
- Lipemia (10g/dl)

Other substances may interfere

REFERENCES

1. Haffejee . Quarterly Journal of Medicine 1992. New series 84; 305: 641-658.
2. Ahmed Samir et al. Pediatric Annals 1992; 21: 835-842.
3. Spaun J et al. Bull Wld Hlth Org 1961; 24: 271-279.
4. The association of Clinical Pathologists 1961. Broadsheet 34.
5. Picard B et al. La Presse Medicale 1983; 23: 2-6.
6. Klein GC. Applied Microbiology 1971; 21: 999-1001.
7. Young DS. Effects of drugs on clinical laboratory test, 4th ed. AACC Press, 1995.



ATLAS Medical

William James House,














Cowley Road, Cambridge, CB4 4WX, UK

Tel: ++44 (0) 1223 858 910

Fax: ++44 (0) 1223 858 524

PPI003A01

Rev H (09.09.2017)

	Catalogue Number		Store at
	For In-Vitro Diagnostic use		Caution
	Number of tests in the pack		Read product insert before use
	Lot (batch) number		Manufacturer
	Fragile, handle with care		Expiry date
	Manufacturer fax number		Do not use if package is damaged
	Manufacturer telephone		

ATLAS C-REACTIVE PROTEIN (CRP) LATEX KIT

For the qualitative and semi-quantitative measurement of C-reactive protein (CRP) in human serum.

IVD For in -vitro diagnostic and professional use only

2°C  8°C
Store at 2-8°C

INTENDED USE

Atlas C-Reactive Protein (CRP) is used to measure the CRP in human serum qualitatively and semi- quantitatively.

INTRODUCTION

C-reactive protein (CRP), the classic acute-phase of human serum, is synthesized by hepatocytes. Normally, it is present only in trace amounts in serum, but it can increase as much as 1,000-fold in response to injury or infection. The clinical measurement of CRP in serum therefore appears to be a valuable screening test for organic disease and a sensitive index of disease activity in inflammatory, infective and ischemic conditions. MacLeod and Avery found that antibody produced against purified CRP provided a more sensitive test than the C-polysaccharide assay. Since that time a number of immunological assays have been devised to measure CRP such as capillary precipitation, double immunodiffusion and radical immunodiffusion.

The CRP reagent kit is based on the principle of the latex agglutination assay described by Singer and Plotz. The major advantage of this method is the rapid two (2) minute reaction time.

PRINCIPLE

The CRP reagent kit is based on an immunological reaction between CRP Antisera bound to biologically inert latex particles and CRP in the test specimen. When serum containing greater than 6 mg/L CRP is mixed with the latex reagent, visible agglutination occurs.

MATERIALS

MATERIALS PROVIDED

- CRP Latex Reagent: Latex particles coated with goat IgG anti-human CRP, pH 8.2 **MIX WELL BEFORE USE.**

- CRP Positive Control Serum: A stabilized pre-diluted human serum containing >20mg/L CRP.
- CRP Negative Control Serum: A stabilized pre-diluted animal serum.
- Glass Slides.
- Stirring Sticks.

MATERIALS REQUIRED BUT NOT PROVIDED

- Mechanical rotator with adjustable speed at 80-100 r.p.m.
- Vortex mixer.
- Pipettes 50 µL.
- Glycine Buffer (20x): add one part to nineteen parts of distilled water before use.

PRECAUTIONS

- Reagents containing sodium azide may be combined with copper and lead plumbing to form highly explosive metal azides. Dispose of reagents by flushing with large amounts of water to prevent azide buildup.
- For In Vitro diagnostic use.
- Positive and negative controls prepared using human serum found negative for hepatitis B surface antigen (HBsAg) by FDA required test; however, handle controls as if potentially infectious.
- Accuracy of the test depends on the drop size of the latex reagent (40µl). Use only the dropper provided with the latex and hold perpendicularly when dispensing.
- Glass slides should be thoroughly rinsed with water and wiped with lint-free tissue after each use.

STORAGE AND STABILITY

- Reagents are stable until specified expiry date on bottle label when stored refrigerated (2 - 8°C). **DO NOT FREEZE.**
- The CRP latex reagent, once shaken must be uniform without visible clumping. When stored refrigerated, a slight sedimentation may occur and should be considered normal.
- Do not use the latex reagent or controls if they become contaminated.

SPECIMEN COLLECTION AND STORAGE

- Use fresh serum collected by centrifuging clotted blood.

- If the test cannot be carried out on the same day, store the specimen for 7 days at 2-8 °C and for 3 months at -20°C.
- For longer periods the sample must be frozen.
- As in all serological tests, hemolytic or contaminated serum must not be used.
- Do not use plasma.

PROCEDURE

A.QUALITATIVE TEST:

- Allow the reagents and samples to reach room temperature. The sensitivity of the test may be reduced at low temperatures.
- Place 40 µL of the sample and one drop of each Positive and Negative controls into separate circles on the slide test.
- Mix the CRP-latex reagent vigorously or on a vortex mixer before using and add one drop (40 µL) next to the samples to be tested.
- Mix the drops with a stirrer, spreading them over the entire surface of the circle. Use different stirrers for each sample.
- Place the slide on a mechanical rotator at 80-100 r.p.m. for 2 minutes. False positive results could appear if the test is read later than two minutes.

B.SEMI-QUANTITATIVE TEST:

- Make serial two fold dilutions of the sample in 9 g/L saline solution.
- Proceed for each dilution as in the qualitative method.

QUALITY CONTROL

Positive and Negative controls are recommended to monitor the performance of the procedure, as well as a comparative pattern for a better result interpretation.


All result different from the negative control result, will be considered as a positive.

INTERPRETATION OF RESULTS

A.QUALITATIVE TEST:

A **negative** reaction is indicated by a uniform milky suspension with no agglutination as observed with the CRP Negative Control.

A **positive** reaction is indicated by any observable agglutination in the reaction mixture. The specimen reaction should be compared to the CRP Negative Control (Fig. 1).

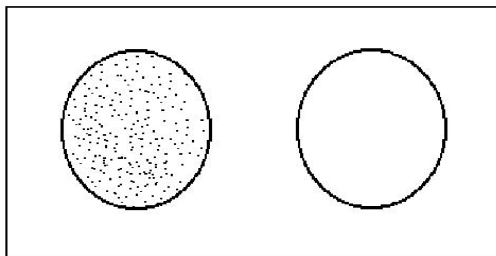

Positive Negative

Figure 1

B. Semi-QUANTITATIVE TEST:

The approximate CRP concentration in the patient sample is calculated as follow:

6×CRP titer = ---- mg/L

INTERFERENCES

NONE INTERFERING SUBSTANCES:

- Hemoglobin (10g/dl)
- Bilirubin(20mg/dl)
- Lipemia(10g/dl)
- Other substances interfere, such as RF (100IU/ml).

NOTE

- High CRP concentration samples may give negative results .Retest the sample again using a drop of 20µl.
- The strength of agglutination is not indicative of the CRP concentration in the samples tested.
- Clinical diagnosis should not be made on findings of a single test result, but should integrate both clinical and laboratory data.

LIMITATIONS

1. Reaction time is critical. If reaction time exceeds two (2) minutes, drying of the reaction mixture may cause false positive results.
2. Freezing the CRP Latex Reagent will result in spontaneous agglutination.
3. Intensity of agglutination is not necessarily indicative of relative CRP concentration; therefore, screening reactions should not be graded.
4. A false negative can be attributed to a prozone phenomenon (antigen excess). It is recommended, therefore, to check all negative sera by retesting at a 1:10 dilution with glycine buffer.

REFERENCE VALUES

Up to 6 mg/L. Each laboratory should establish its own reference range.

PERFORMANCE CHARACTERISTICS

- **Sensitivity:** 6(5-10) mg/L
- **Prozone effect:** No prozone effect was detected up to 1600 mg/L
- **Diagnostic sensitivity:** 95.6 %.
- **Diagnostic specificity:** 96.2 %.

REFERENCES

1. Pepys, M.B.. Lancet 1:653 (1981).
2. Werner, M.. Clin.Chem. Acta 25:299 (1969).
3. MacLeod, C.M., et. al.. J. Exp. Med 73:191 (1941).
4. Wood, HF., et. al.. J. Clin. Invest. 30: 616 (1951).
5. Mancini, G., et. al. Immunochemistry 2:235 (1965).
6. Singer, J.M., et. al.. Am. J. Med 21: 888 (1956).
7. Fischer, C.L., Gill, C.W.. In Serum Protein Abnormalities. Boston, Little, Brown and Co., (1975).



ATLAS MEDICAL














William James House,
Cowley Road, Cambridge,
CB4 0WX, UK

Tel: +44 (0) 1223 858 910

Fax: +44 (0) 1223 858 524

PPI005A01

Rev H (06.06.2017)

	Catalogue Number		Store at
	For In-Vitro Diagnostic use		Caution
	Number of tests in the pack		Read product insert before use
	Lot (batch) number		Manufacturer
	Fragile, handle with care		Expiry date
	Manufacturer fax number		Do not use if package is damaged
	Manufacturer telephone number		

ATLAS RHEUMATOID FACTOR (RF) LATEX KIT

latex slide test for the qualitative and semi-quantitative measurement of RF in human serum.

IVD For In-Vitro diagnostic and professional use only



Store at 2-8°C

INTENDED USE

A latex slide test for the qualitative and semi-quantitative measurement of RF in human serum.

INTRODUCTION

Rheumatoid factors (RF) are antibodies directed against antigenic sites in the Fc fragment of human and animal IgG. Their frequent occurrence in rheumatoid arthritis makes them useful for diagnosis and monitoring of the disease.

One method used for rheumatoid factor detection is based on the ability of rheumatoid arthritis sera to agglutinate sensitized sheep red cells, as observed by Waaler and Rose. A more sensitive reagent consisting of biologically inert latex beads coated with human gamma globulin was later described by Singer and Plotz. The RF kit is based on the principle of the latex agglutination assay of Singer and Plotz. The major advantage of this method is rapid performance (2 minute reaction time) and lack of heterophile antibody interference.

PRINCIPLE

The RF reagent is based on an immunological reaction between human IgG bound to biologically inert latex particles and rheumatoid factors in the test specimen. When serum containing rheumatoid factors is mixed with the latex reagent, visible agglutination occurs.

MATERIALS

MATERIALS PROVIDED

- RF Latex Reagent: Latex particles coated with human gamma-globulin, pH, 8.2. Preservative. Contains N, N-dimethylformamide.
- RF Positive Control Serum: Human serum with a RF concentration > 30 IU/mL. Preservative.

- RF Negative Control Serum: Animal serum. Preservative.
- Reaction Slide
- Stirring sticks

MATERIALS REQUIRED BUT NOT PROVIDED

- Timer
- Test Tubes (for dilution)
- Serological pipettes (for sample addition and for dilution)
- Rotator (optional)
- Glycine Buffer (20x): add one part to nineteen parts of distilled water before use.

PRECAUTIONS

- All reagents contain 0.1 % (w/v) sodium azide as a preservative.
- Reagents containing sodium azide may be combined with copper and lead plumbing to form highly explosive metal azides. Dispose of reagents by flushing with large amounts of water to prevent azide buildup.
- For In Vitro diagnostic use.
- Positive and negative controls prepared using human serum found negative for hepatitis B surface antigen (HBsAg) by FDA required test; however, handle controls as if potentially infectious.
- Accuracy of the test depends on the drop size of the latex reagent (40 µL). Use only the dropper supplied with latex and hold it perpendicularly when dispensing.
- Use a clean pipette tip and stirring stick for each specimen, and glass slides should be thoroughly rinsed with water and wiped with lint-free tissue after each use.
- Check reactivity of the reagent using the controls provided.

STORAGE AND STABILITY

- Reagents are stable until specified expiry date on bottle label when stored refrigerated (2-8°C).
- Do not freeze.
- The RF latex reagent, once shaken must be uniform without visible clumping. When stored refrigerated, a slight sedimentation may occur and should be considered normal.
- Do not use the latex reagent or controls if they become contaminated.

SPECIMEN COLLECTION AND STORAGE

- Use fresh serum collected by centrifuging clotted blood.
- If the test cannot be carried out on the same day, store the specimen for 7 days at 2-8°C and for 3 months at -20°C.
- As in all serological tests, hemolytic or contaminated serum must not be used.
- Do not use PLASMA.

PROCEDURE

Qualitative method

- Allow the reagents and samples to reach room temperature. The sensitivity of the test may be reduced at low temperatures.
- Place 50 µL of the sample and one drop of each Positive and Negative controls into separate circles on the slide test.
- Mix the RF-latex reagent rigorously or on a vortex mixer before using and add one drop (50 µL) next to the sample to be tested.
- Mix the drops with a stirrer, spreading them over the entire surface of the circle. Use different stirrers for each sample.
- Place the slide on a mechanical rotator at 80-100 r.p.m. for 2 minutes. False positive results could appear if the test is read later than two minutes.

Semi-quantitative method

- Make serial two fold dilutions of the sample in 9 g/L saline solution.
- Proceed for each dilution as in the qualitative method.

READING AND INTERPRETATION

Examine macroscopically the presence or absence of visible agglutination immediately after removing the slide from the rotator. The presence of agglutination indicates a RF concentration equal or greater than 8 IU/mL (Note 1). The titer, in the semi-quantitative method, is defined as the highest dilution showing a positive result.

CALCULATIONS

The approximate RF concentration in the patient sample is calculated as follows:

$$8 \times \text{RF Titer} = \text{IU/mL}$$

INTERFERENCES

NON INTERFERING SUBSTANCES:

- Hemoglobin (10g/dl)
- Bilirubin(20mg/dl)
- Lipemia(10g/dl)

Other substances may interfere.

QUALITY CONTROL

1. RF Positive and Negative Control should be included in each test batch.
2. Acceptable performance is indicated when a uniform milky suspension with no agglutination is observed with the RF Negative Control and agglutination with large aggregates is observed with the RF Positive Control.

PERFORMANCE CHARACTERISTICS

Analytical sensitivity

8(6-16) IU/ml, under the described assay conditions.

PROZONE EFFECT

No prozone effect was detected up to 1500 IU/ml.

DIAGNOSTIC SENSITIVITY

100%.

DIAGNOSTIC SPECIFICITY

100%.

The diagnostic sensitivity and specificity have been obtained using 118 samples compared with the same method of a computer.

LIMITATIONS

- Reaction time is critical. If reaction time exceeds 2 minutes, drying of the reaction mixture may cause false positive result.
- Freezing the RF Latex Reagent will result in spontaneous agglutination.
- Intensity of agglutination is not necessarily indicative of relative RF concentration; therefore, screening reactions should not be graded.
- Increased levels of RF may be found in some diseases other than rheumatoid arthritis such as infectious mononucleosis, sarcoidosis, lupus erythematosus, Sjogren's syndrome.
- Certain patients with rheumatoid arthritis will not have the RF present in their serum.

- The incidence of false positive results is about 3-5 %.Individuals suffering from infectious mononucleosis, hepatitis, syphilis as well as elderly people may give positive results.
- Diagnosis should not be solely based on the results of latex method but also should be complemented with a Waaler Rose test along with the clinical examination.

REFERENCE VALUES

Up to 8 IU/mL. Each laboratory should establish its own reference range.

NOTES

1. Results obtained with a latex method do not compare with those obtained with Waaler Rose test. Differences in the results between methods do not reflect differences in the ability to detect rheumatoid factors.

REFERENCES

1. Robert W Dorner et al. Clinica Chimica Acta 1987; 167: 1 – 21.
2. Frederick Wolfe et al. Arthritis and Rheumatism 1991; 34: 951- 960.
3. Robert H Shmerling et al. The American Journal of Medicine 1991; 91: 528 –534.
4. Adalbert F. Schubart et al. The New England Journal of Medicine 1959; 261: 363 – 368.
5. Charles M. Plotz 1956; American Journal of Medicine; 21:893 – 896.
6. Young DS. Effects of drugs on clinical laboratory test, 4th ed. AACC Press, 1995.



William James Hous Cowley Road,
Cambridge, CB4 0WX, UK.

Tel: +44 (0) 1223 858 910

Fax: +44 (0) 1223 858 524

PPI008A01, Rev H (17.06.2017)

	Catalogue Number		Store at
	For In-Vitro Diagnostic use		Caution
	Number of tests in the pack		Read product insert before use
	Lot (batch) number		Manufacturer
	Fragile, handle with care		Expiry date
	Manufacturer fax number		Do not use if package is damaged
	Manufacturer telephone number		