

## WOUND DRAINAGE

# SILICONE WOUND DRAIN


## T-KEHR

### DESCRIPTION

Redax T-Kehr drain is a T-shape postoperative drain. It is made of medical grade silicone and provided with an x-ray line and depth marks.

### CLINICAL INDICATIONS

T-Kehr wound drain is use for removal of common bile duct stone, postoperatively. It is recommended for long term biliary drainage, sclerosing cholangitis and biliary strictures. It can be used with any controlled suction system and/or by gravity.

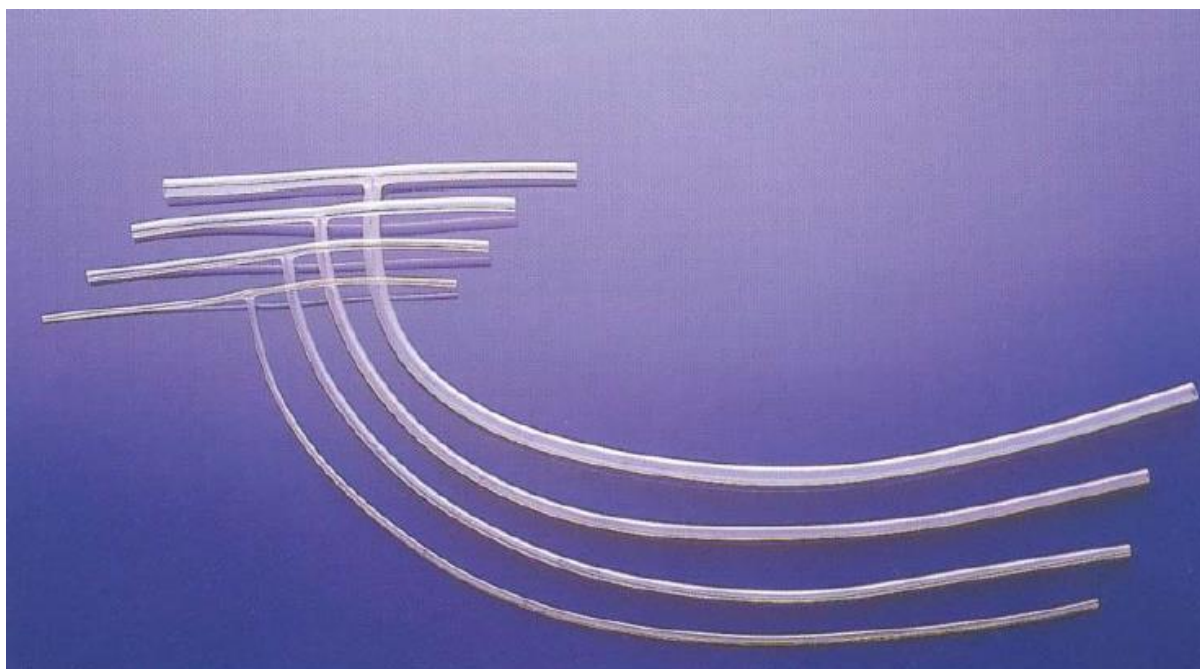

**Figure 1: Silicone wound drain – T-Kehr**

### TECHNICAL CHARACTERISTICS

- Medical grade, biocompatible silicone drains. Soft, kink-resistant conforms easily to anatomical contour for superior patient comfort and improved drainage performance
- Perfect seaming the horizontal tubes with the vertical part by the high techniques. The lengths are: 180 mm for the horizontal arm and 450 mm for the vertical tube
- T-Tube is made of a translucent color material with blue X-ray opaque line
- Smooth drainage functions through the soft horizontal tubes and the rigid vertical tubes, which is resistant to being crushed or kinked
- Sizes: 6 different sizes from 9 to 24 CH

- Inside every single package, there is a conical connector for connecting the drainage to the suction system
- We recommend the use of the drainages no longer than 29 days, based on the classification according to Annex IX Directive 93/42/EEC
- Single-use, Sterile

## CONFIGURATIONS

Code	Description	Size [CH]	Outer Diameter [mm]
24409	Silicone T-Kehr wound drain CH 9	9	3
24412	Silicone T-Kehr wound drain CH 12	12	4
24415	Silicone T-Kehr wound drain CH 15	15	5
24418	Silicone T-Kehr wound drain CH 18	18	6
24421	Silicone T-Kehr wound drain CH 21	21	7
24424	Silicone T-Kehr wound drain CH 24	24	8

## TECHNICAL DATA

<b>PRODUCTION SITE</b>	<b>REDAX S.p.A. - Via Galileo Galilei, 46025 Poggio Rusco [Mantova, Italy]</b>
<b>MATERIALS</b>	Tubing: Silicone medical grade [Latex and phtalate free]  Biocompatibility and haemocompatibility according to the International Standard UNI EN ISO 10993-1 and UNI EN ISO 10993-4
<b>STERILIZATION</b>	Ethylene Oxide Gas
<b>PACKAGING</b>	Sterile single package: double sterile wrapping constituted by an internal blister OPA/PE and PP/PE and an external pouch in medical paper PET/PP.  Shipping box: 10 pieces/box
<b>TECHNICAL STANDARDS</b>	UNI EN ISO 20697:2018 and UNI EN 1618:1997
<b>STERILIZATION</b>	Ethylene Oxide Gas  Single-use - do not sterilize and/or reuse the product For a single patient
<b>EXPIRATION DATE</b>	5 Years
<b>CERTIFICATIONS</b>	Redax Quality System is compliant with standard ISO 13485. Redax devices are certified with EC Mark 0123, released by TÜV SÜD Product Service GmbH (Germany)
<b>CLASSIFICATION</b>	Class IIa/Rule 7 - MDD 93/42 CEE
<b>STORAGE, CONSERVATION AND TRANSPORT</b>	Temperature range: 0° ÷ 60°C Recommended storage at room temperature.

# TECHNICAL DATA SHEET



<b>MARKET INTRODUCTION YEAR</b>	1999
-------------------------------------	------

**Technical Director**

Andrea Gibertoni

A handwritten signature in blue ink, appearing to read 'Andrea Gibertoni', written over the printed name.