




Nuova Aptaca Srl Regione Monforte, 30 - 14053 Canelli (Asti) Italy Tel. (+39) 0141/83.50.75 – Fax (+39) 0141/83.52.92 E-Mail: info@aptaca.com – Website: www.aptaca.com

CERTIFIED COMPANY UNI EN ISO 9001 & UNI CEI EN ISO 13485

SCHEDA TECNICA PRODOTTO TECHNICAL DATA SHEET

0.5 ml Trisodium Citrate (3.8%) in polypropylene test tubes with pressure cap, for 4.5 ml of blood.

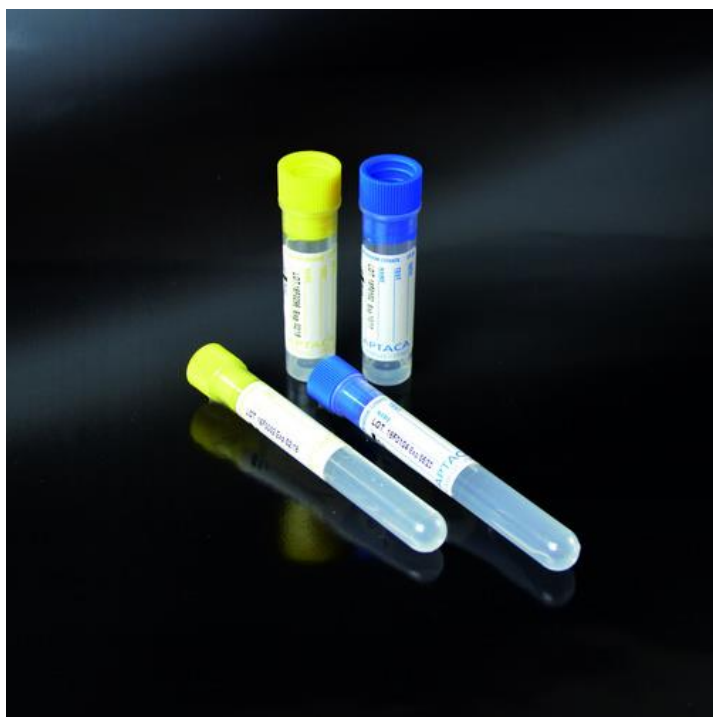

Cod.	Cap Colour	Test Tubes	Ratio	Filling Line
2511	Yellow	Ø 16x60 mm	1:9	5 ml
2512	Yellow	Ø 12x86 mm	1:9	5 ml
2511/B	Blue	Ø 16x60 mm	1:9	5 ml
2512/B	Blue	Ø 12x86 mm	1:9	5 ml