


## Standard Sterile Surgical Set Specifications

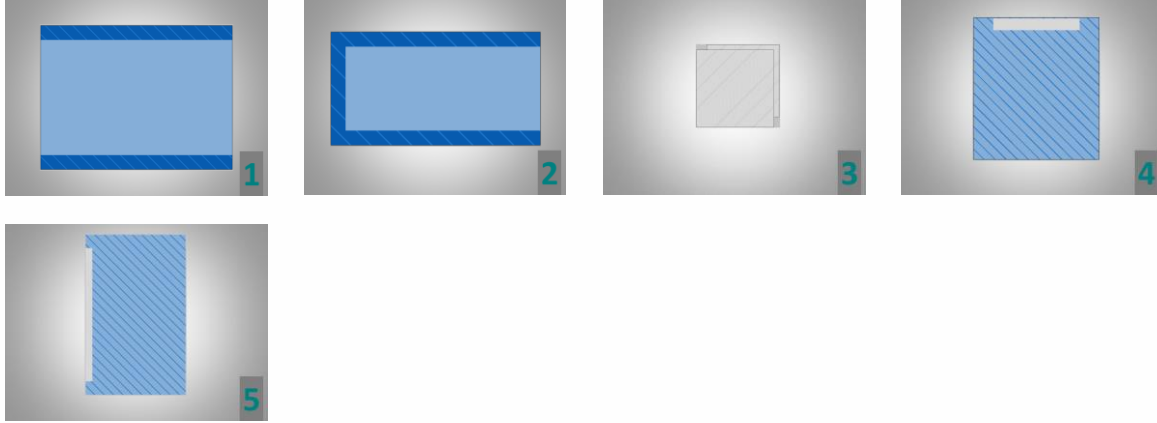

OPS ADVANCED	STANDARD STERILE SURGICAL SET
Reference(s)	Z10-001-01
Description	<ol style="list-style-type: none"> <li>Field For Instrument Table With Reinforced Zone From SMS 150x190 – 1 pc.</li> <li>Field For Mayo Table With SMS Reinforcement 80x40 - 1 pcs.</li> <li>Napkin For Absorption – Not to leave lint – 40x40 2 pcs.</li> <li>Lower Part Field 190x195 - 1 pcs. <ul style="list-style-type: none"> <li>Positioning tape – on the entire surface of the incision area, impregnated in the fabric, 5cm wide</li> <li>Absorbent area – on the entire incision surface; liquid penetration resistance of min. 150cm of H2O/cm2</li> <li>SMS material on the entire surface of the field with liquid resistance 50cm H2O/cm2</li> </ul> </li> <li>Upper Part Field 150x270 - 1 pcs. <ul style="list-style-type: none"> <li>Positioning tape – on the entire surface of the incision area, impregnated in the fabric, width of 5cm</li> <li>Absorbent area – on the entire incision surface; resistance to liquid penetration of min. 150cm of H2O/cm2</li> <li>SMMS material on the entire surface of the field with liquid resistance min. 50cm H2O/cm2 . OP-Tape 10x50 - 1 pcs.</li> </ul> </li> </ol>
Main Materials	SMS (40 GR, %100 PP), BIFLEX SPUNBOND (56 GR, SB+PE FILM)
Packaging	Sterilization Pack 42x60
Manufacturer	ZENMED TIBBİ CİHAZLAR VE SAĞLIK ÜRÜNLERİ SAN. VE TİC. LTD. ŞTİ. ISO 13485:2016
Regulation	In compliance with Medical Devices Directive 93/42/EEC HP: High performance according to EN 13795 standard MDD class: I sterile

ZENMED TIBBİ CİHAZLAR  
VE SAĞLIK ÜRÜNLERİ SAN. VE TİC. LTD.ŞTİ.  
Mahmutbey Mah. 2567. Sk. No:1 İş Yeri No:11,21  
Bağcılar / İSTANBUL / TÜRKİYE  
Tel: 0212 445 45 25 Tic.Sic.No: 794704  
Güneşli M.D.: 897 067 1942

Latex Free

CE 1984



STERILE EO

### Manufacturing Company:

ZENMED TIBBİ CİHAZLAR VE SAĞLIK ÜRÜNLERİ SAN. VE TİC. LTD. ŞTİ

Mahmutbey Mahallesi 2567. Sk. No: 1/11 Bağcılar-İstanbul/TURKEY

+90 212 445 45 25

+90 212 445 45 40

www.zenmed.com.tr

