

**BeneVision™**  
See more With ease

**BeneVision™ N22/N19**  
**Patient Monitor**  
Change your perspective, again.  
Maximize your confidence.  
Built for a paperless future.



[www.mindray.com](http://www.mindray.com)  
P/N: ENG-BeneVision N22/N19-210285x14Px20190129  
©2018 Shenzhen Mindray Bio-Medical Electronics Co., Ltd. All rights reserved.

**mindray**  
healthcare within reach

**mindray**

**BeneVision N22/N19**  
Patient monitor  
Always in sight, always in mind





# BeneVision.

## Change your perspective, again.

### BeneVision N22/N19

At Mindray, we believe the best way to predict the future is to create it today. We're thinking how to help you save your time in order to treat more patients effectively. We also focus on clinical safety, and efficiency. Now for the first time in the world, the BeneVision patient monitor ROTATES between landscape and portrait. You have both higher and wider clinical views when patient care demands them.





Design.  
Excellence for visionaries.



Original technology innovations have been combined with thoughtful considerations to improve patient monitoring experience.

During the design process, we strove to make the details “and” instead of “or”, such as the ingenious portrait and landscape display, as well as the single-level menu user interface.



Modular design brings so many options.

- Parameter modularity allows you flexibility in patient care and makes the most of your equipment investment.
- iView module combines a powerful, embedded PC and the patient monitor in the same unit. The innovative design optimizes cooling without the need for a fan.
- Ultra-compact main unit and big screen can be used as a combined unit or separated to make use of the rotating screen feature.



Auto



Built-in



No fan



Seamless






# Innovative.

## Maximize your confidence.

Everyday, Mindray delivers accurate, real-time, physiological measurement data from millions of patients worldwide, which clinicians have come to rely on when making decisions. BeneVision provides the worlds best monitoring technologies for you and promotes new ones continuously.


### Cardiology

ΔST monitoring and ST segment templates.  
Real-time QT/QTc measurement.  
Glasgow 12-lead resting interpretation.




### Hemodynamics and volumetric

Less-invasive PiCCO and ScvO<sub>2</sub> monitoring.  
Non-invasive cardiac output with ICG module.




### Airway gas and lung mechanics

One-slot CO<sub>2</sub>+O<sub>2</sub> module  
Volumetric CO<sub>2</sub> and metabolic measurements  
AION Multi-Gas +SPIRIT respiratory mechanics




### Tissue perfusion


INVOS rSO<sub>2</sub> provides a noninvasive and continuous reading of changes in regional oxygen saturation of blood in tissue microvascular circulation.




### Neurology

EEG, and BIS/BISx4 monitoring.  
Advanced NMT monitoring technology can detect movement in all directions accurately.




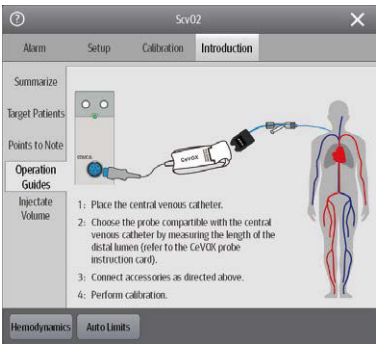


Online Guide

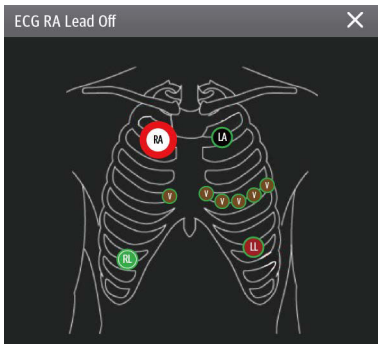

Infographic alarm

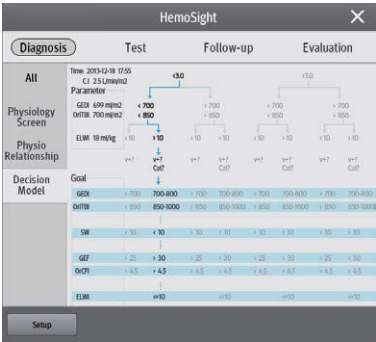

HemoSight™  
Help clinicians to make decisions through sets of hemodynamic assistance applications.

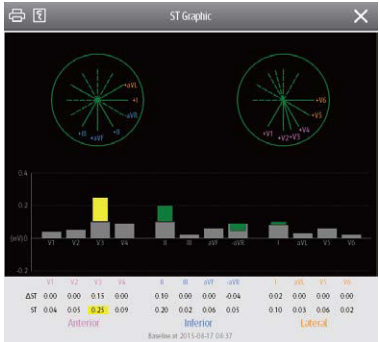

ST Graphic™  
Quickly and accurately detect changes in ST values for analysis.



Comparison review  
Events summary and details ease contextual evaluation.





# Mobility. Streamlined.

Since the introduction of the world's first portable cardiac monitor in 1964, Mindray has committed itself to being the pioneer in early patient mobilization for better recovery. BeneVision extends the typical mobile monitoring solution with more wireless roaming, data continuity, and streamlined workflow in every situation. Combined with its patient-worn telemetry monitor, which is also a cableless measurement module, BeneVision ensures a supreme level of mobility and offers more freedom to both patient and caregiver.



BeneVision N22/N19 wirelessly pairs with its TM80 and BP10 patient-worn modules for cableless measurement at the bedside and beyond.



Ambulatory patients monitored around the bedside and beyond.



The Mindray classical transport monitoring solution with BeneVision N1 also works seamlessly with BeneVision for unmatched patient safety.





## Connected. Built for a paperless future.


As a pioneer in clinical informatics with patient monitoring, Mindray integrated the embedded PC (iView) in 2007, which enables a patient monitor to run user APPs for the first time in the world. BeneVision enhances the iView open platform with a more intuitive display, modular design, and powerful performance. Patient monitoring and healthcare applications are combined into one workstation at the point of care.

Mindray provides a flexible solution for monitoring your patient's status anywhere, anytime, even when you are away from the clinical environment. . .Based on layer 3 network structure, the Mindray patient monitoring system has a high network adaptability to integrate seamlessly with your hospital's current network.

With Mindray's central station and eGateway further connecting BeneVision with your clinical world, bedside device data and other clinical system data is shared to enhance your diagnosis and clinical decision making.



### BeneVision EMR(Electronic Medical Record)

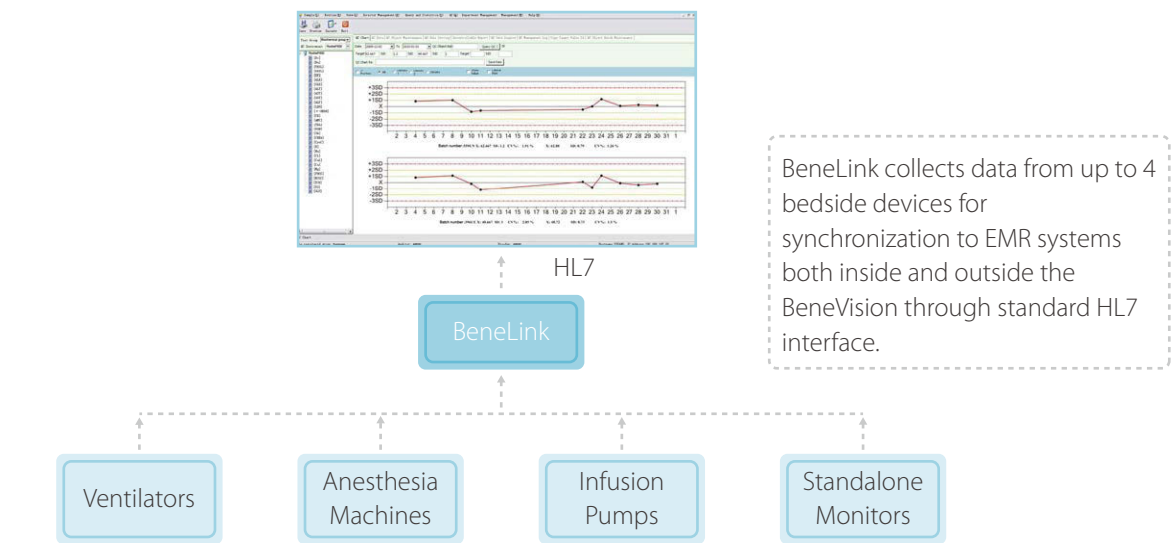

iView can run your own clinical Apps (such as PACS, LIS, HIS/CIS, and EMR) on one intuitive view and connects with your hospital network infrastructure directly without any additional server or gateway.

With its 1680 x 1050 pixels 22-inch screen, BeneVision N22 has a perfect split layout in portrait display. No need to worry that the waveforms will be obstructed by the iView application window as you browse the patient's information.



# BeneVision N22/N19

## Patient monitor

### Physical Specifications

<b>Weight</b>	Including main unit with a battery, screen with handle & navigation knob, iView module, and Wi-Fi module.
N22:	11.5 kg (25.4 lbs)
N19:	10.3 kg (22.7 lbs)
<b>Size</b>	Including main unit, screen with handle.
N22:	641 x 383 x 115 mm (portrait) 566 x 458 x 115 mm (landscape)
N19:	584 x 348 x 115 mm (portrait) 509 x 423 x 115 mm (landscape)
Main unit:	268 x 268 x 68 mm
<b>Display</b>	
Type	Medical-grade color TFT LCD, capacitive touch screen, support multi-touch operation. Rotatable screen (Landscape and portrait)
Resolution	1680 x 1050 pixels
Screen	
N22:	22-inch, 178° viewing angle
N19:	19-inch, 170° viewing angle
Waveforms	Up to 16 waveforms (portrait) Up to 13 waveforms (landscape)

### ECG

Meet standards of IEC 60601-2-27 and IEC 60601-2-25.	
<b>Lead Sets</b>	Automatic 3/5/6/12 - lead recognition
3-lead:	I, II, III
5-lead:	I, II, III, aVR, aVL, aVF, V
6-lead:	I, II, III, aVR, aVL, aVF, Va, Vb
12-lead:	I, II, III, aVR, aVL, aVF, V1 to V6
Sweep Speed	6.25 mm/s, 12.5 mm/s, 25 mm/s, 50 mm/s
Gain Selection	x 0.125, x 0.25, x 0.5, x 1, x 2, x 4, auto
Waveform format	Standard, Cabrera
Input Signal Range	± 8 mV (p-p)
Electrode Offset Potential Tolerance	± 500 mV
<b>Bandwidth</b>	
Diagnostic Mode:	0.05 to 150 Hz
Monitor Mode:	0.5 to 40 Hz
Surgical Mode:	1 to 20 Hz
ST Mode:	0.05 to 40 Hz
High Freq Cut-off (for 12-lead ECG analysis):	350 Hz, 150 Hz, 35 Hz, 20 Hz selectable
<b>CMRR</b>	
Diagnostic:	> 90 dB
Monitor, Surgical, ST mode:	> 105 dB (with notch filter on)
<b>Pace detection</b>	
Amplitude:	± 2 mV to ± 700 mV
Width:	0.1 to 2 ms
Rise time:	10 to 100 µs (without overshoot)
<b>Defibrillator Protection</b>	Withstand 5000VAC (360J) defibrillation
Defib. Recovery Time	≤ 5 seconds
ESU recovery time	≤ 10 s
Provides Glasgow resting 12-lead ECG algorithm.	
Provides Mindray Multi(4)-lead ECG monitoring analysis algorithm.	
(* These ECG specifications are from MPM Platinum module.)	

### Heart Rate

<b>Measurement Range</b>	
Adult:	15 to 300 bpm
Pediatric/Neonate:	15 to 350 bpm
<b>Accuracy</b>	± 1 bpm or ± 1%, whichever is greater.
<b>Resolution</b>	1 bpm

### Arrhythmia Analysis

<b>Patient</b>	Adult/Pediatric/Neonate.
<b>Monitored Arrhythmias</b>	Asystole, VFib/VTac, VTac, Vent. Brady, Extreme Tachy, Extreme Brady, Vrrhythm, PVCs/min, Pauses/min, Couplet, Bigeminy, Trigeminy, R on T, Run PVCs, PVC, Tachy, Brady, Missed Beats, PNP, PNC, Multif. PVC, Nonsus. VTac, Pause, Irr. Rhythm, AFib. SVT, SVTs/min

### ST Segment Analysis

<b>Patient</b>	Adult/Pediatric.
<b>Range</b>	- 2.0 to + 2.0 mV (RTI)
<b>Accuracy</b>	± 0.02 mV or ± 10%, whichever is greater (- 0.8 to + 0.8 mV)
<b>Resolution</b>	0.01 mV

### QT Analysis

<b>Patient</b>	Adult/Pediatric/Neonate.
<b>Parameters</b>	QT, QTc, ΔQTc
<b>QTc Formula</b>	Bazett, Fridericia, Framingham, or Hodges
<b>Range</b>	
QT/QTc:	200 to 800 ms
QT-HR:	Adult: 15 to 150 bpm Pediatric/Neonate: 15 to 180 bpm
<b>QT Accuracy</b>	± 30 ms
<b>Resolution</b>	QT 4 ms; QTc 1 ms

### Respiration

<b>Range</b>	0 to 200 bpm
<b>Resolution</b>	1 rpm
<b>Apnea Alarm Time</b>	10, 15, 20, 25, 30, 35, 40 sec
<b>Accuracy</b>	
0 - 120 rpm:	± 1 rpm
121 - 200 rpm:	± 2 rpm
<b>Lead</b>	I, II, or auto (default: lead II)

### Pulse Oximetry

Meet standards of ISO 80601-2-61.	
<b>Module</b>	Mindray, Masimo, Nellcor
<b>Range</b>	0 to 100 %
<b>Resolution</b>	1%
<b>Accuracy</b>	
Mindray/Nellcor:	± 2 % (70 to 100%, Adult/Pediatric); ± 3 % (70 to 100%, Neonate) Unspecified (0 to 69%)
Masimo:	± 2 % (70 to 100%, Adult/Pediatric, non-motion) ± 3 % (70 to 100%, Neonate, non-motion) ± 3 % (70 to 100%, motion) Unspecified (0 to 69%)
<b>Perfusion indicator (PI)</b>	Yes, for Mindray/Masimo SpO <sub>2</sub>
<b>Pitch Tone</b>	Yes
<b>Dual-SpO<sub>2</sub></b>	Yes, SpO <sub>2</sub> , SpO <sub>2</sub> b, ΔSpO <sub>2</sub>
<b>Pulse Rate Range</b>	
Mindray/Nellcor:	20 to 300 bpm
Masimo:	25 to 240 bpm
<b>Pulse Rate Accuracy</b>	
Mindray:	± 3 bpm (20 - 300 bpm)
Nellcor:	± 3 bpm (20 - 250 bpm)
Masimo:	± 3 bpm (non-motion) ± 5 bpm (motion)

### PR Refresh Rate

### Temperature

Meet standard of ISO 80601-2-56.	
<b>Method</b>	Thermal resistance
<b>Channels</b>	Up to 8 channels
<b>Units of Measure</b>	Selectable °C or °F
<b>Range</b>	0 to 50 °C / 32 to 122 °F
<b>Resolution</b>	0.1 °C, 0.1 °F
<b>Accuracy</b>	± 0.1 °C or ± 0.2 °F (without probe)
<b>Refresh Rate</b>	1 sec
<b>Genius™ Tympanic Thermometer</b>	
<b>Measurement Range</b>	33 to 42 °C / 91.4 to 107.6 °F
<b>Calibrated Accuracy</b>	± 0.1 °C (environment temperature 25 °C, target temperature 36.7 to 38.9 °C) ± 0.2 °C (environment temperature 16 °C, target temperature 33 to 42 °C)

### Resolution

### Response Time

### Non-Invasive Blood Pressure

Meet standards of ISO 80601-2-30.	
<b>Method</b>	Oscillometry
<b>Modes</b>	Manual, Auto, STAT, Sequence
<b>Units of Measure</b>	mmHg, kPa (user-selectable)
<b>Resolution</b>	1 mmHg
<b>Systolic range</b>	
Adult:	25 to 290 mmHg
Pediatric:	25 to 240 mmHg
Neonate:	25 to 140 mmHg
<b>Diastolic range</b>	
Adult:	10 to 250 mmHg
Pediatric:	10 to 200 mmHg
Neonate:	10 to 115 mmHg
<b>Mean range</b>	





Adult:	15 to 260 mmHg
Pediatric:	15 to 215 mmHg
Neonate:	15 to 125 mmHg
<b>Accuracy</b>	
Max Mean Error:	± 5 mmHg
Max Standard Deviation:	8 mmHg
<b>Cuff Deflation Technique Step bleed</b>	
<b>Initial Cuff Inflation</b>	
Adult:	80 to 280 mmHg (default: 160 mmHg)
Pediatric:	80 to 210 mmHg (default: 140 mmHg)
Neonate:	60 to 140 mmHg (default: 90 mmHg)
<b>Over Pressure Protection</b>	
Adult/ Pediatric:	297 ± 3 mmHg
Neonate:	147 ± 3 mmHg
<b>Max Measurement time</b>	
Adult/Pediatric:	180 sec
Neonate:	90 sec
Assisting Venous Puncture	Yes
Pulse Rate Range	30 to 300 bpm
Pulse Rate Accuracy	± 3 bpm or ± 3 %, whichever is greater

#### IBP

Meet standard of IEC 60601-2-34.	
Number	Up to 8 channels
Measurement Range	-50 to 360 mmHg
Resolution	1 mmHg
Accuracy	± 1 mmHg or ± 2 %, whichever is greater (excluding sensor error)
Sensitivity	5 µV/V/mmHg
Impedance Range	300 to 3000 Ω
PPV Range	0 to 50 %
PAWP	Yes
ICP measurement	Support
Support waveforms overlapping.	
Pulse Rate Range	25 to 350 bpm
Pulse Rate Accuracy	± 1 bpm or ± 1 %, whichever is greater

#### Cardiac Output

Method	Thermodilution
Measurement Range	0.1 - 20 L/min
Resolution	0.1 L/min
Accuracy	± 0.1 L/min or ± 5%, whichever is greater
TB Range	23 to 43 °C / 73.4 to 109.4 °F
TB, TI Accuracy	± 0.1 °C (without sensor)
TB, TI Resolution	0.1 °C

#### PiCCO

Parameters	Measurement Range	Coefficient of Variation
CCO	0.25 to 25.0 L/min	≤ 2%
C.O.	0.25 to 25.0 L/min	≤ 2%
GEDV	40 to 4800 ml	≤ 3%
SV	1 to 250 ml	≤ 2%
EVLW	10 to 5000 ml	≤ 6%
ITBV	50 to 6000 ml	≤ 3%

(Coefficient of variation is measured using synthetic and/or database wave forms (laboratory testing.) Coefficient of variation= SD/mean error.)

TB Range	23 to 43 °C / 73.4 to 109.4 °F
TB, TI Accuracy	± 0.1 °C (without sensor)
TB, TI Resolution	0.1 °C
pArt/pCVP Range	-50 to 300 mmHg
pArt/pCVP Accuracy	± 1 mmHg or ± 2 %, whichever is greater

#### ScvO<sub>2</sub>

Range	0 to 99 %
Accuracy	± 3% (50 to 80 %)

#### ICG

Method	Thoracic electrical bioimpedance (TEB)
HR Range	40 to 200 bpm (ICG), accuracy ± 2 bpm
C.O. Range	1.0 to 15 L/min
SV Range	5 to 250 ml
Provides Monitoring Parameters ACI, VI, PEP, LVET, TFI, TFC, HR, C.O., C.I., SV, SVI, SVR, SVRI, PVR, PVRI, LCW, LCWI, LVSW, LVSWI, STR, VEPT	

#### Continuous Cardiac Output Interface

Measured Parameter	Consistent with CCO-related parameters outputted by Vigilance II®, Vigileo™, EV1000 or HemoSphere
--------------------	---

#### Artema Sidestream CO<sub>2</sub>

Meet standard of ISO 80601-2-55.

<b>Measurement Range</b>	
etCO <sub>2</sub> :	0 to 150 mmHg
O <sub>2</sub> (optional):	0 to 100 %
<b>CO<sub>2</sub> Accuracy</b>	
0 to 40 mmHg:	± 2mmHg
41 to 76 mmHg:	± 5% of reading
77 to 99 mmHg:	± 10% of reading
100 to 150 mmHg:	± (3 mmHg+8% of reading)
<b>O<sub>2</sub> Accuracy</b>	
0 to 25 %:	± 1 %

25.1 to 80 %:	± 2 %
80.1 to 100 %:	± 3 %

#### Resolution

etCO <sub>2</sub> :	1 mmHg
O <sub>2</sub> (optional):	1 %

#### Sample Flow Rate

Adult/Pediatric:	120 ml/min (with or without O <sub>2</sub> monitoring)
Neonate:	70 ml/min or 90 ml/min, selectable
	90 ml/min (with O <sub>2</sub> monitoring)

#### Sample Flow Rate Tolerance

± 15 ml/min or ± 15 %, whichever is greater.

#### Warm-up Time

90 sec (maximum), 20 sec (typically)

Measured with a neonatal watertrap and 2.5-meter neonatal sampling line, or an adult watertrap and a 2.5-meter adult sampling line:

#### Rise Time

etCO <sub>2</sub> :	≤ 250 ms @ 70 ml/min (Neonate watertrap)
	≤ 250 ms @ 90 ml/min (Neonate watertrap)
	≤ 300 ms @ 120 ml/min (Adult watertrap)
O <sub>2</sub> (optional):	≤ 800 ms @ 90 ml/min (Neonate watertrap)
	≤ 750 ms @ 120 ml/min (Adult watertrap)

#### Sampling Delay Time

etCO <sub>2</sub> :	≤ 5.0 sec @ 70 ml/min (Neonate watertrap)
	≤ 4.5 sec @ 90 ml/min (Neonate watertrap)
	≤ 5.0 sec @ 120 ml/min (Adult watertrap)
O <sub>2</sub> (optional):	≤ 4.5 sec @ 90 ml/min (Neonate watertrap)
	≤ 5.0 sec @ 120 ml/min (Adult watertrap)
awRR Range	0 to 150 rpm

#### awRR Accuracy

0 to 300 rpm:	± 1 rpm
61 to 150 rpm:	± 2 rpm

#### Apnea Time

10, 15, 20, 25, 30, 35, 40 sec

Provide VCO<sub>2</sub>, VO<sub>2</sub>, MVCO<sub>2</sub>, MVO<sub>2</sub>, EE, RQ parameters, when monitoring with RM module.

#### Oridion Microstream CO<sub>2</sub>

Measurement Range	0 to 99 mmHg
Resolution	1 mmHg
<b>Accuracy</b>	
0 to 38 mmHg:	± 2 mmHg
39 to 99 mmHg:	± 5 % + 0.08 % of the reading – 38 mmHg
Sample Flow Rate	50 <sup>-7.5</sup> <sub>+15</sub> ml/min
Start-up Time	30 sec (typical)
Response Time	2.9 s (typical)
awRR Range	0 to 150 rpm
<b>awRR Accuracy</b>	
0 to 70 rpm:	± 1 rpm
71 to 120 rpm:	± 2 rpm
121 to 150 rpm:	± 3 rpm

#### Apnea time

10, 15, 20, 25, 30, 35, 40 sec

#### Capnostat Mainstream CO<sub>2</sub>

Measurement Range	0 to 150 mmHg
Resolution	1 mmHg
<b>Accuracy</b>	
0 to 40 mmHg:	± 2mmHg
41 to 70 mmHg:	± 5% of reading
71 to 100 mmHg:	± 8% of reading
101 to 150 mmHg:	± 10% of reading
Rise time	< 60 msec
awRR Range	0 to 150 rpm
awRR Accuracy	± 1 rpm
Provide VCO <sub>2</sub> , MVCO <sub>2</sub> , FeCO <sub>2</sub> , SlopeCO <sub>2</sub> , Vtalv, MValv, Vdaw, Vdaw/Vt, Vdalv, Vdalv/Vt, Vdphy, Vd/Vt, when monitoring with RM module.	

#### Anesthesia Gases

Meet standard of ISO 80601-2-55.

#### Sampling Rate

Adult/pediatric:	200 ml/min
Neonate:	120 ml/min

Sampling Rate Tolerance ± 10 ml/min or ± 10%, whichever is greater.

#### Sampling Delay Time

< 4 sec

#### Refresh Rate

1 sec

#### Warm-up Time

45 sec to warm-up status  
10 min to ready-to-measure status

#### Measurement Range

CO <sub>2</sub> :	0 to 30 %
N <sub>2</sub> O:	0 to 100 %
Des/Sev/Enf/Iso/Hal:	0 to 30 %
O <sub>2</sub> :	0 to 100 %
awRR:	2 to 100 rpm

#### Resolution

CO <sub>2</sub> :	0.1 %
N <sub>2</sub> O:	1 %
Des/Sev/Enf/Iso/Hal:	0.1 %
O <sub>2</sub> :	1 %



awRR:	1 rpm	
Full Accuracy		
Gases	Range (%REL)	Accuracy (%ABS)
CO <sub>2</sub> :	0 to 1 %	± 0.1 %
	1 to 5 %	± 0.2 %
	5 to 7 %	± 0.3 %
	7 to 10 %	± 0.5 %
	> 10 %	Not specified
N <sub>2</sub> O:	0 to 20 %	± 2 %
	20 to 100 %	± 3 %
Des:	0 to 1 %	± 0.15 %
	1 to 5 %	± 0.2 %
	5 to 10 %	± 0.4 %
	10 to 15 %	± 0.6 %
	15 to 18 %	± 1 %
Sev:	> 18 %	Not specified
	0 to 1 %	± 0.15 %
	1 to 5 %	± 0.2 %
	5 to 8 %	± 0.4 %
Enf/Iso/Hal:	> 8 %	Not specified
	0 to 1 %	± 0.15 %
	1 to 5 %	± 0.2 %
O <sub>2</sub> :	> 5 %	Not specified
	0 to 25 %	± 1 %
	25 to 80 %	± 2 %
awRR:	80 to 100 %	± 3 %
	2 to 60 rpm	± 1 rpm
	> 60 rpm	Not specified
Rise Time		
Sampling flow 120 ml/min, using the DRYLINE II™ watertrap and a neonatal 2.5m sampling line,		
CO <sub>2</sub> / N <sub>2</sub> O:	≤ 250 ms	
Iso/Hal/Sev/Des:	≤ 300 ms	
Enf:	≤ 350 ms	
O <sub>2</sub> :	≤ 600 ms	
Sampling flow 200ml/min, using DRYLINE II™ watertrap and an adult 2.5m sampling line:		
CO <sub>2</sub> / N <sub>2</sub> O:	≤ 250 ms	
Iso/Hal/Sev/Des:	≤ 300 ms	
Enf:	≤ 350 ms	
O <sub>2</sub> :	≤ 500 ms	
Sampling Delay Time		
Sampling flow 120 ml/min, using the DRYLINE II™ watertrap and a neonatal 2.5m sampling line,		
CO <sub>2</sub> :	≤ 4 sec	
N <sub>2</sub> O:	≤ 4.2 sec	
O <sub>2</sub> :	≤ 4 sec	
Enf /Iso/Hal/Sev/Des:	≤ 4.4 sec	
Sampling flow 200ml/min, using DRYLINE II™ watertrap and an adult 2.5m sampling line:		
CO <sub>2</sub> :	≤ 4.2 sec	
N <sub>2</sub> O:	≤ 4.3 sec	
O <sub>2</sub> :	≤ 4 sec	
Enf/Iso/Hal/Sev/Des:	≤ 4.5 sec	
Apnea time	10,15,20,25,30,35,40 sec	
Provide MAC value (support calibrated by age).		
Support two mixed gas identify and monitoring.		
RM		
Method	Diff-Pressure flow	
Measurement Range		
Flow	Adult/Pediatric: ± (2 to 120) L/min	
	Neonate: ± (0.5 to 30) L/min	
Paw	-20 to 120 cmH <sub>2</sub> O	
MVe/MVi	Adult/Pediatric: 2 to 60 L/min	
	Infant: 0.5 to 15 L/min	
TVe/TVi	Adult/Pediatric: 100 to 1500 ml	
	Infant: 20 to 500 ml	
awRR range	4 to 120 rpm	
Resolution		
Flow	0.1 L/min	
Paw	0.1 cmH <sub>2</sub> O	
MVe/MVi	0.01 L/min (MVe/MVi < 10 L/min)	
	0.1 L/min (MVe/MVi ≥ 10 L/min)	
TVe/TVi	1 ml	
awRR:	1 rpm	
Accuracy		
Flow	Adult/Pediatric: ± 1.2 L/min or ± 10% of the reading, whichever is greater.	
	Neonate: ± 0.5 L/min or ± 10%, whichever is greater.	
Paw	± 3% of reading	
MVe/MVi	± 10% of reading	
TVe/TVi	Adult/Pediatric: ±10% or ±15 ml, whichever is greater.	

awRR:	Infant: ±10% or ±6 ml, whichever is greater. ±1 rpm (4 to 99 rpm) ±2 rpm (100 to 120 rpm)
Provide loops display.	
Monitoring parameters include PEEP, Pmean, PIP, Pplat, PEF, PIF, MVe, MVi, TVe, TVi, RR, I:E, FEV1.0, Compl, RSBI, NIF, WOB, RAW.	
<b>rSO<sub>2</sub></b>	
Patient	Adult/Pediatric/Neonate.
Method	INVOS, NIRS (Near Infrared Spectroscopy)
Number	Up to 4 channels
Measurement Range	15 to 95 %
<b>NMT</b>	
Meet the standard of IEC 60601-2-10	
Sensor Type	Acceleromyography sensor
Stimulation Modes	ST, TOF, PTC, DBS3.2, DBS3.3
Stimulation Current Range	0 to 60 mA
Stimulation Current Accuracy	± 5% or ± 2 mA, whichever is greater.
Stimulation Pulse Width	100,200 or 300µs, monophasic rectangle pulse
Stimulation Pulse Width Accuracy	± 10 %
Max. Output Voltage	300 V
<b>BISx/BISx4</b>	
Meet standard of IEC 60601-2-26.	
Method	Bispectral Index
Impedance Range	0 to 999 kΩ
EEG Bandwidth	0.25 to 100 Hz
BIS Range	0 to 100 (BIS, BIS L, BIS R)
SQI Range	0 to 100 % (SQI, SQI L, SQI R)
ASYM	0 to 100%
DSA Trend	Yes
<b>EEG/aEEG</b>	
Meet standard of IEC 60601-2-26.	
EEG Channels	Up to 4 channels
Montage Mode	Biopolar mode, referential mode
Input Signal Range	- 2 mVp-p to + 2mVp-p
Max. Input DC Offset	± 500 mV
CMRR	≥ 100 dB @51 kΩ imbalance and 60 Hz
Noise Level	≤ 0.5 µV rms (0.5 Hz to 70 Hz)
Differential Input Impedance	> 15 MΩ @10 Hz
Electrode Impedance	
Range	1 to 90 kΩ
Accuracy	± 1 kΩ or ± 10%, whichever is greater
Sampling Frequency	EBN EEG: 1024 Hz Mindray EEG: 256Hz
Analog bandwidth	EBN EEG: 0.5 to 110 Hz Mindray EEG/aEEG: 0.1 to 110 Hz
Spectrum analysis	SEF, MF, PPF, TP, SR, EMG, Delta, Theta, Alpha, Beta
Trend	DSA, CSA
<b>ANI</b>	
Patient	Adult, Pediatric (over 12 years old)
Measurement Range	ANLi: 12 to100 ANIm: 12 to 100 Energy: 0.00 to 65.54
<b>tcGas</b>	
Interfaces with TCM CombiM, TCM TOSCA or SenTec SDM monitor.	
Measurement Range	
tcpCO <sub>2</sub>	5 to 200 mmHg
tcpO <sub>2</sub>	0 to 800 mmHg
SpO <sub>2</sub>	0 to 100 %
PR	25 to 240 bpm
Power	0 to 1000 mW
Accuracy	
tcpCO <sub>2</sub>	TOSCA Sensor 92, tc Sensor 54: Better than 1 mmHg (1 % or 10 % CO <sub>2</sub> ) Better than 3 mmHg (33 % CO <sub>2</sub> ) tc Sensor 84: Better than 1 mmHg (1 % or 10 % CO <sub>2</sub> ) Better than 5 mmHg (33 % CO <sub>2</sub> )
tcpO <sub>2</sub>	tc Sensor 84: Better than 1 mmHg (0 % O <sub>2</sub> ) Better than 3 mmHg (21 % O <sub>2</sub> ) Better than 5 mmHg (50 % O <sub>2</sub> ) Better than 25 mmHg (90 % O <sub>2</sub> )
SpO <sub>2</sub>	± 3 % (70 to 100 %)
PR	±3 bpm
Power	±20 % of reading
<b>iView</b>	
CPU	Intel Pentium N4200 2.5GHz
Memory	8 GB
Hard-disk	mSATA SSD 128GB
OS	Windows 10



## Recorder

Type	Thermal array
Speed	25 mm/sec, 50 mm/sec
Trace	Up to 3 (paper 50 mm width, 20 m length)
Supports two-slots recorder module.	

## Alarms

Audible indicator	Yes, 4 different alarm tones, and prompt tone
Visible indicator	Red/yellow/cyan LED, and alarm message
Provide AlarmSight infographic alarm indicator.	
Support iAlarm features (alarm limits recommendations, etc.)	
Support iStatus combined alarms	

## Data Storage

Trends Data	> 120 hrs @ 1 min, 4 hrs @ 5 sec.
Events	1000 events, including parameter alarms, arrhythmia events, technical alarms, and so on.
NIBP	1000 sets
Interpretation of resting	12-lead ECG results
	20 sets
Full disclosure	48 hours for all parameters and waveforms (8G storage card)
	48 hours at maximum. The specific storage time depends on the waveforms stored and the number of stored waveforms. (2G storage card)
OxyCRG	48 hrs
ST review	120 hrs @ 1 min
Minirend	Yes

## Special Functions

Clinical Assistive Application (CAA):	
	HemoSight™, ST Graphic™, SepsisSight™, BoA Dashboard™, EWS, GCS, ECG 24h Summary, Pace View, AF Summary, NeuroSight
Support calculations (drug, hemodynamic, Oxygenation, Ventilation, Renal), and Titration table.	
Support wireless connection with BeneVision TM80 and BP10.	
Support nView remote display tool	

## Wi-Fi Communications

Protocol	IEEE 802.11a/b/g/n
Modulation Mode	DSSS and OFDM
Operating Frequency	
	IEEE 802.11b/g/n (2.4G):
ETSI/FCC/KC:	2.4 to 2.483 GHz
MIC:	2.4 to 2.495 GHz
	IEEE 802.11a/n (5G):
ETSI:	5.15 to 5.35 GHz, 5.47 to 5.725 GHz
FCC:	5.15 to 5.35 GHz, 5.725 to 5.82 GHz
MIC:	5.15 to 5.35 GHz
KC:	5.15 to 5.35 GHz, 5.47 to 5.725 GHz, 5.725 to 5.82 GHz
Channel Spacing	5 MHz @ 2.4 GHz (802.11 b/g/n)
	20 MHz @ 5 GHz (802.11 a/n)
Wireless Baud Rate	IEEE 802.11a: 6 to 54 Mbps
	IEEE 802.11b: 1 to 11 Mbps
	IEEE 802.11g: 6 to 54 Mbps
	IEEE 802.11n: 6.5 to 72.2 Mbps
Output Power	< 20dBm (CE requirement: detection mode- RMS)
	< 30dBm (FCC requirement, detection mode- peak power)
Operating Mode	Infrastructure
Data Security	WPA-PSK, WPA2-PSK, WPA-Enterprise, WPA2-Enterprise (EAP-FAST, EAP-TLS, EAP-TTLS, PEAP-GTC, PEAP-MSCHAPv2, PEAP-TLS, LEAP)
	Encryption: TKIP and AES

## Output

Auxiliary Output	
Standard	Meets the requirements of ANSI/AAMI/IEC 60601-1 for short-circuit protection and leakage current

## ECG Analog Output

Bandwidth (- 3 dB; reference frequency: 10 Hz)	
Diagnostic Mode:	0.05 to 150 Hz
Monitor Mode:	0.5 to 40 Hz
Surgical Mode:	1 to 20 Hz
ST Mode:	0.05 to 40 Hz
QRS Delay	≤ 25 ms (in diagnostic mode, and non-paced)
Sensitivity	1 V/mV, ± 5 %
Pace Enhancement	
Signal Amplitude:	Voh ≥ 2.5 V
Pulse Width:	10 ms ± 5 %
Signal Rising and Falling Time:	≤ 100 μs

## IBP Analog Output

Bandwidth (- 3 dB; reference frequency: 10 Hz)	
	0 to 40 Hz
Max. Transmission Delay	30 ms
Sensitivity	1 V/100 mmHg, ± 5 %

## Interfacing

Main Unit	
	1 AC Power Connector
	2 RJ45 Network Connector, 100 Base-TX, IEEE 802.3
	6 USB 2.0 Connector
	3 Nonstandard USB SMR Connector
	1 VP Connector, VP1 for the secondary display
	1 BNC Connector
	1 Equipotential Grounding Terminal
Modular iView	
	1 VP Connector, VP2
	4 USB 2.0 Connector
	1 RJ45 Network Connector, 100 Base-TX, IEEE 802.3
Multifunction Connector for Defib Sync and Analog Output	
	1 on multi-parameter module
Barcode Scanner	Support 1D and 2D barcode
Keyboard & Mouse	Support wire and wireless type
Remote Control	Support
Network Printer	Support

## Battery

Type	Rechargeable lithium-ion
Number of Battery	1
Capacity	5600mAh
Run Time	> 1 hrs
	when powered by a new fully-charged battery at 25 °C±5 °C with 12-lead ECG, Resp, SpO2, 4-ch IBP, 2-ch Temp, CO2, C.O. and NIBP measurements every 15 min, WiFi enabled, and screen brightness set to default 5, 5 hrs to 90% when the monitor is off.
Recharge Time	

## Power Requirements

AC Voltage	100 to 240 VAC (±10 %)
Current	2.8 to 1.6 A
Frequency	50 Hz/60 Hz (±3 Hz)

## Environmental

Temperature	Operating: 0 to 40 °C (32 to 104 °F)
	Storage: -20 to 60 °C (-4 to 140 °F)
Humidity	Operating: 15 to 95 % (non condensing)
	Storage: 10 to 95 % (non condensing)
Barometric	Operating: 427.5 to 805.5 mmHg (57.0 to 107.4 kPa)
	Storage: 120 to 805.5 mmHg (16.0 to 107.4 kPa)

## Safety

Type of Protection	Class I
Degree of Protection	MPM/IBP/C.O./NMT/(a)EEG/PiCCO/ANI module: CF
	ScvO2/CO2/AG/ICG/BIS/RM/rSO2 module: BF
Protection Against Ingress of Fluids	
	IPX1

Some of functions marked with an asterisk may not be available. Please contact your local Mindray sales representative for the most current information.

[www.mindray.com](http://www.mindray.com)

P/N:ENG- BeneVision N22/N19 Datasheet-210285x4P-20211225

©2021 Shenzhen Mindray Bio-Medical Electronics Co.,Ltd. All rights reserved.

**mindray**  
healthcare within reach



# **BeneVision seria N**

Monitor de pacient

## **Manualul operatorului**

### **Volum I**

(BeneVision N22/BeneVision N19/BeneVision N17/  
BeneVision N15/BeneVision N12/BeneVision N12C)



© Copyright 2016-2022 Shenzhen Mindray Bio-Medical Electronics Co., Ltd. Toate drepturile rezervate.

Data publicării: Martie 2022

Revizuire: 3.0

Acest manual conține două volume. Volumul I conține informații legate de siguranță și introducerea despre echipament. Vă informează despre cum să efectuați alte sarcini decât măsurarea parametrilor și cum să îngrijiți și să întrețineți echipamentul. Volumul II vă arată cum să efectuați măsurători asociate parametrilor. De asemenea, menționează specificațiile pentru măsurarea parametrilor, alarmele și setările implicite.



Problemă	Acțiuni corective
Traietorii ECG cu perturbații	<ol style="list-style-type: none"> <li>1. Verificați dacă electrozii sunt detașați sau uscați. Înlocuiți cu alți electrozi umezi, dacă este necesar.</li> <li>2. Verificați astfel încât conductoarele să nu fie defecte. Înlocuiți conductoarele, dacă este necesar.</li> <li>3. Verificați astfel încât cablul pacientului sau conductoarele să nu fie direcționate prea aproape de alte dispozitive electrice. Mutați cablul pacientului sau conductoarele la distanță de dispozitivele electrice.</li> </ol>
Interferență excesivă la nivelul cauterelor	Utilizați cablurile ECG rezistente la ESU. Pentru mai multe informații, consultați 42.1 <i>Accesorii pentru ECG</i> .
Perturbație cauzată de mușchi	<p>Pregătire inadecvată a pielii, tremur, subiect încordat și/sau poziționare precară a electrozilor.</p> <ol style="list-style-type: none"> <li>1. Pregătiți pielea din nou și înlocuiți electrozii din nou. Pentru informații suplimentare, consultați 20.4.1 <i>Pregătirea pielii pacientului</i> și 20.4.2 <i>Aplicarea electrozilor</i>.</li> <li>2. Aplicați alți electrozi umezi. Evitați zonele musculare.</li> </ol>
Semnal intermitent	<ol style="list-style-type: none"> <li>1. Verificați astfel încât cablurile să fie conectate corespunzător.</li> <li>2. Verificați dacă electrozii sunt detașați sau uscați. Pregătiți pielea din nou conform descrierii din 20.4.1 <i>Pregătirea pielii pacientului</i> și aplicați alți electrozi umezi.</li> <li>3. Verificați astfel încât cablul pacientului și conductoarele să nu fie deteriorate. Modificați-le, dacă este cazul.</li> </ol>
Alarmer excesive: ritm cardiac, defecțiune derivație	<ol style="list-style-type: none"> <li>1. Verificați dacă electrozii sunt uscați. Pregătiți pielea din nou și înlocuiți electrozii din nou. Pentru informații suplimentare, consultați 20.4.1 <i>Pregătirea pielii pacientului</i> și 20.4.2 <i>Aplicarea electrozilor</i>.</li> <li>2. Verificați în privința mișcării excesive a pacientului sau a tremurului muscular. Repozitionați electrozii. Înlocuiți cu alți electrozi umezi, dacă este necesar.</li> </ol>
Semnal ECG cu amplitudine scăzută	<ol style="list-style-type: none"> <li>1. Verificați dacă amplificarea ECG nu este setată la un nivel prea scăzut. Reglați amplificarea, după caz. Pentru mai multe informații, consultați 20.6 <i>Modificarea setărilor ECG</i>.</li> <li>2. Pregătiți pielea din nou și înlocuiți electrozii din nou. Pentru informații suplimentare, consultați 20.4.1 <i>Pregătirea pielii pacientului</i> și 20.4.2 <i>Aplicarea electrozilor</i>.</li> <li>3. Evitați locurile de aplicare a electrozilor. Evitați zona osoasă sau musculară.</li> <li>4. Verificați dacă electrozii sunt uscați sau dacă au fost utilizați pentru o perioadă îndelungată. Înlocuiți cu alți electrozi umezi, dacă este necesar.</li> </ol>
Formă de undă ECG lipsă	<ol style="list-style-type: none"> <li>1. Verificați dacă amplificarea ECG nu este setată la un nivel prea scăzut. Reglați amplificarea, după caz. Pentru mai multe informații, consultați 20.6.3 <i>Setarea modului de analiză</i>.</li> <li>2. Verificați astfel încât conductoarele și cablurile pacientului să nu fie conectate necorespunzător.</li> <li>3. Schimbați cablul și conductoarele.</li> <li>4. Verificați astfel încât cablul pacientului și conductoarele să nu fie deteriorate. Modificați-le, dacă este cazul.</li> </ol>
Devierea liniei de bază	<ol style="list-style-type: none"> <li>1. Verificați în privința mișcării excesive a pacientului sau a tremurului muscular. Fixați conductoarele și cablul.</li> <li>2. Verificați dacă electrozii sunt detașați sau uscați și înlocuiți cu alți electrozi umezi, dacă este necesar. Pentru informații suplimentare, consultați 20.4.1 <i>Pregătirea pielii pacientului</i> și 20.4.2 <i>Aplicarea electrozilor</i>.</li> <li>3. Verificați setarea filtrului ECG. Setati modul Filtru ECG la <b>Monitor</b> pentru a reduce devierea liniei de bază pe afișaj.</li> </ol>



---

## Accessories and Consumables

CATALOGUE

2022.07

---

[www.mindray.com](http://www.mindray.com)

P/N:ENG-Accessories and Consumables Catalogue-210210X142P-20220728  
©2022 Shenzhen Mindray Bio-Medical Electronics Co., Ltd. All rights reserved.







## Welcome to the Mindray Accessories Catalogue

This catalogue will provide you with the parts and accessories that connect to your Mindray Patient Monitor, Electrocardiograph, Defibrillator. Each Mindray product is the product of a special brand of patient focused, clinician-friendly design. For this reason, you can expect the same service, focus and quality with our parts and accessories.

## Finding the Right Part

This catalog has been designed to make finding the right part easy. Chapters are organized by specific parameter categories. Simply locate the type of part you are looking for under the appropriate category.

## Note:

This catalog is not an Operating Instructions Manual. This catalog will assist you in identifying the correct parts and accessories to connect to your Mindray product, please refer to the Operating Instructions Manual.

Warnings, Precautions and Notes can also be found in the Operating Instructions.

01

## Patient Monitor Accessories

ECG	2
SpO <sub>2</sub>	22
NIBP	36
TEMP	52
CO <sub>2</sub>	61
AG	74
IBP	78
ICP	83
RM	84
C.O.	86
ICG	89
BIS	90
PiCCO <sub>2</sub>	91
CCO/ScvO <sub>2</sub>	95
EEG	96
ANI	101
NMT	102
rSO <sub>2</sub>	105
Mounting	106
Rolling stands	116
Others	118

02

## Defibrillator Accessories

122




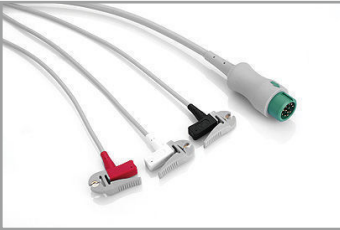
03

## Electrocardiograph Accessories

136

Integrated ECG Cables - AHA

For BeneVision, BeneView, ePM, iPM, uMEC, iMEC series monitors, BeneHeart defibrillator, uMED 20

Picture	Model	Part No.	No. Description	Purchasing Unit
	EA6251B	040-000961-00	ECG cable and wires (integrative): Adu/Ped, 12 Pin 5-Lead, Defib-Proof, AHA, Snap, 3.6 m	Each
	EA6231B	040-000965-00	ECG cable and wires (integrative): Adu/Ped, 12 Pin 3-Lead, Defib-Proof, AHA, Snap, 3.6 m	Each
	EA6251A	040-000960-00	ECG cable and wires (integrative): Adu/Ped, 12 Pin 5-Lead, Defib-Proof, AHA, Clip, 3.6 m	Each
	EA6231A	040-000964-00	ECG cable and wires (integrative): Adu/Ped, 12 Pin 3-Lead, Defib-Proof, AHA, Clip, 3.6 m	Each

Trunk Cables

- Easy to replace leadwires
- Meeting the requirements of EC53
- Outstanding shielding property and anti-interference performance, protecting ECG signal from being interfered
- Excellent defibrillation-proof performance, well protecting the equipment
- ESU-proof, ensuring ECG signals not interfered during operation Flexible and durable cables
- Outstanding cable material, enduring repeated cleaning and disinfection
- Latex free

For BeneVision, BeneView, ePM, iPM, uMEC, iMEC series monitors, BeneHeart defibrillator, uMED 20




Picture	Model	Part No.	No. Description	Purchasing Unit
	EV6201	0010-30-42719 (009-004728-00)	ECG trunk cable: 3/5-lead, Adu/Ped, 12 Pin, Defib-Proof, AHA/IEC, 3 m	Each
	EV6211	0010-30-42723	ECG trunk cable: 3/5-lead, Adu/Ped, 12 Pin, ESU-Proof, AHA/IEC, 3 m	Each
	EV6202	0010-30-42720	ECG trunk cable: 3-lead, Ped/Neo, 12 Pin, Defib-Proof, AHA/IEC, 3 m	Each



ECG Leadwires – IEC


- Easy to replace trunk cables
- Meeting the requirements of EC53
- Outstanding shielding property and anti-interference performance, protecting ECG signal from being interfered
- Flexible and durable cables
- Outstanding cable material, enduring repeated cleaning and disinfection
- Latex free

Match with 3/5-lead cables (0010-30-42719, 0010-30-42723)

Picture	Model	Part No.	No. Description	Purchasing Unit
	EL6502A	0010-30-42728	5-Lead ECG wires, Clip, Adu, TPU, IEC, 0.6 m/1m	Each
	EL6504A	0010-30-42730	5-Lead ECG wires, Clip, Adu/Ped, TPU, IEC, long, 1m/1.4 m	Each
	EL6502B	0010-30-42736 (009-004730-00)	5-Lead ECG wires, Snap, Adu, TPU, IEC, 1m/1.4 m	Each

Picture	Model	Part No.	No. Description	Purchasing Unit
	EL6308B	0010-30-42733	3-Lead ECG wires, Snap, Adu/Ped, TPU, IEC, 1m	Each
	EL6304A	0010-30-42732	3-Lead ECG wires, Clip, Adu/Ped, TPU, IEC, 1m	Each


Match with 3-lead cables (0010-30-42720, 0010-30-42724)

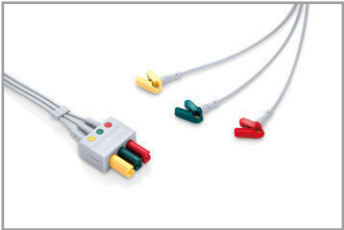Picture	Model	Part No.	No. Description	Purchasing Unit
	EL6306A	0010-30-42897	3-Lead ECG wires, Clip, Neo, TPU, IEC, 1m	Each

Electrode

- Latex free
- DEHP free
- Good biocompatibility, avoiding allergic reactions to patient

Picture	Model	Part No.	No. Description	Purchasing Unit
	31499224	0010-10-12304	Adult ECG Electrode (Kendall, Medi Trace 210)	10 pcs/pouch
	H124SG	900E-10-04880	Neonatal ECG Electrode (Kendall, H124SG)	50pcs/pouch
		040-002711-00	Adult ECG electrode (INTCO)	5 pcs/pouch

Picture	Model	Part No.	No. Description	Purchasing Unit
		040-002833-00	Pediatric/Neonatal ECG electrode (INTCO)	30 pcs/pouch

Match with 3-lead Neonatal cables (040-000754-00)

Picture	Model	Part No.	No. Description	Purchasing Unit
	0406062	040-003254-00	Disposable neonatal 3-lead pre-wired electrode, radio translucent, AHA, 60 cm	50 pouch/box (3 pcs/pouch)



# SpO<sub>2</sub> Accessories

## Mindray SpO<sub>2</sub> Accessories



## Integrated SpO<sub>2</sub> Cable

For BeneVision, BeneView, ePM, iPM, uMEC, iMEC, VS series monitors, BeneHeart defibrillator

Picture	Model	Part No.	No. Description	Purchasing Unit
	512FLH	115-012807-00	Integrative reusable SpO <sub>2</sub> sensor, Adult, Finger, >30 kg, 3 m	Each
	518BLH	115-020887-00	Integrative reusable SpO <sub>2</sub> sensor, Neo, Foot (adult/pediatric, finger), <5 kg, 3 m	Each

## Mindray SpO<sub>2</sub> Cable

For BeneVision, BeneView, ePM, iPM, uMEC, iMEC, VS series monitors, BeneHeart defibrillator

- Ergonomic design, precise engineering and clinical testing guaranteeing reliable measurement
- Well anti-electromagnetic interference, suitable for complex electrical environment
- Flexible and durable cables
- Outstanding cable jacket, enduring repeated cleaning and disinfection
- Easy to change sensor, meeting clinical requirements for patient use
- Latex free

Picture	Model	Part No.	No. Description	Purchasing Unit
	562A	0010-20-42710 (009-004600-00)	Mindray SpO <sub>2</sub> extension cable, 7 Pin, 2.5 m	Each
	562B	040-001443-00	Mindray SpO <sub>2</sub> extension cable, 7 Pin, 1.2 m	Each

## For Telemetry

Picture	Model	Part No.	No. Description	Purchasing Unit
	SAT 10	115-029488-00	Mindray SpO <sub>2</sub> module for BeneVision TM80, 6 Pin, 0.5 m	Each

Mindray SpO<sub>2</sub> Sensor

Finger-Clip Sensor (Reusable)

- Ergonomic design, precise engineering and clinical testing guaranteeing reliable measurement
- High quality photoelectric element, ensuring precise measurement
- Well anti-electromagnetic interference, suitable for complex electrical environment
- Perfect performance against light interference, can be used in environment of strong light
- ESU-proof, ensuring SpO<sub>2</sub> signals not interfered during operation
- Strict electric safety specification, guaranteeing safety for use
- Few pit structure, not easily staining, convenient for cleaning
- Outstanding cable jacket, enduring repeated cleaning and disinfection
- Latex free
- Good biocompatibility, avoiding allergic reactions to patient

For all Mindray SpO<sub>2</sub> Cables and PM-50/60 pulse oximeter

Picture	Model	Part No.	No. Description	Purchasing Unit
A white reusable finger-clip sensor with a blue connector cable, designed for adult use.	512F	512F-30-28263	Reusable sensor, adult, finger-clip, 1.1 m, >30 kg	Each
A white reusable finger-clip sensor with a blue connector cable, designed for pediatric use.	512H	512H-30-79061	Reusable sensor, pediatric, finger-clip, 1.1 m, 10-30 kg	Each

Finger-Tip Sensor (Reusable)


- Ergonomic design, precise engineering and clinical testing guaranteeing reliable measurement
- High quality photoelectric element, ensuring precise measurement
- Well anti-electromagnetic interference, suitable for complex electrical environment
- Perfect performance against light interference, can be used in environment of strong light
- ESU-proof, ensuring SpO<sub>2</sub> signals not interfered during operation
- Strict electric safety specification, guaranteeing safety for use
- Silicone rubber sheath, not likely to break in case of drop, hardly sensor off
- Few pit structure, not likely staining, convenient for cleaning
- Outstanding cable jacket, enduring repeated cleaning and disinfection
- Latex free
- Good biocompatibility, avoiding allergic reactions to patient

For all Mindray SpO<sub>2</sub> Cables and PM-50/60 pulse oximeter

Picture	Model	Part No.	No. Description	Purchasing Unit
A white reusable finger-tip sensor with a blue connector cable, designed for adult use.	512E	512E-30-90390	Reusable sensor, adult, finger-tip, 1.1 m, >30 kg	Each
A white reusable finger-tip sensor with a blue connector cable, designed for pediatric use.	512G	512G-30-90607	Reusable sensor, pediatric, finger-tip, 1.2 m, 10-30 kg	Each





Adapted with the tubing (6200-30-09688, 115-012522-00, 040-002712-00)


Picture	Model	Part No.	No. Description	Purchasing Unit
	CM1905	040-000688-00	NIBP Cuff Tubing Adapter (Adult tubing to Neonate cuff)	Each

CM1200 Series


- Soft and comfortable. Low hazard to skin even if a long-term use
- Easy to clean. The cuff wrap can not be damped or stained by liquid if duly cleaned
- Pilling-proof. Not deform even if for long-term use
- TPU bladder ensures good air tightness and long life
- Latex free, PVC free
- Good biocompatibility, free from biological hazard to skin

Connected with the tubing 6200-30-09688, 115-012522-00 and 040-002712-00

Picture	Model	Part No.	No. Description	Purchasing Unit
	CM1200	115-002480-00	Reusable cuff, Small Inf, 7-13 cm	Each
	CM1201	0010-30-12157	Reusable cuff, Inf, 10-19 cm, with connector	Each

Picture	Model	Part No.	No. Description	Purchasing Unit
	CM1202	0010-30-12158	Reusable cuff, Child, 18-26 cm, with connector	Each
	CM1203	0010-30-12159	Reusable cuff, Adu, 25-35 cm, with connector	Each
	CM1204	0010-30-12160	Reusable cuff, Large Adu, 33-47 cm, with connector	Each
	CM1205	0010-30-12161	Reusable cuff, Thigh, 46-66 cm, with connector	Each



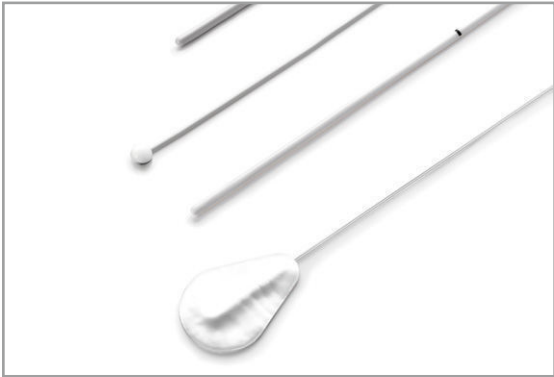

Temperature Accessories



Reusable Temperature Probes



- Available in Rectal/Esophageal and Skin Surface Styles
- Flexible and durable cables
- Outstanding cable material, enduring repeated cleaning and disinfection
- Latex free
- Good biocompatibility, avoiding allergic reactions to patient

For BeneVision, BeneView, ePM, iPM, uMEC, iMEC series monitors, BeneHeart defibrillator





Picture	Model	Part No.	No. Description	Purchasing Unit
	MR401B	0011-30-37392	Reusable Temp Probe, Adu, Esophageal/Rectal, 2 Pin, 3 m	Each
	MR402B	0011-30-37394	Reusable Temp Probe, Ped/Neo, Esophageal/Rectal, 2 Pin, 3 m	Each
	MR403B	0011-30-37393	Reusable Temp Probe, Adu, Skin, 2 Pin, 3.6 m	Each
	MR404B	0011-30-37395	Reusable Temp Probe, Ped/Neo, Skin, 2 Pin, 3.6 m	Each



For BeneVision, BeneView, ePM, uMEC series monitors, BeneHeart defibrillator

Picture	Model	Part No.	No. Description	Purchasing Unit
	EA6231B	115-043024-00 (100-000080-00)	M02C DRYLINE II water trap Adu/Ped for single-slot module	10 pcs/box
	EA6232B	115-043025-00 (100-000081-00)	M02C DRYLINE II water trap Neo for single-slot module	10 pcs/box

For BeneVision, BeneView, ePM, iPM, uMEC, iMEC series monitors, BeneHeart defibrillator

Picture	Model	Part No.	No. Description	Purchasing Unit
	60-15200-00	115-043017-00 (9200-10-10533)	Sampling line, Adu/Ped, 2.5 m	25 pcs/box
	60-15300-00	115-043018-00 (9200-10-10555)	Sampling line, Neo, 2.5 m	25 pcs/box
	60-14100-00	115-043020-00 (9000-10-07486)	Dryline airway adapter, straight	10 pcs/box
	60-14200-00	115-043021-00 (9000-10-07487)	Dryline airway adapter, elbow	10 pcs/box



# Invasive Blood Pressure (IBP) Accessories

## Invasive Blood Pressure Cables


- Compatible solution with major monitor IBP module interface and disposable pressure transducer brands in the market
- Flexible and durable cables
- Outstanding cable material, enduring repeated cleaning and disinfection
- Latex free

For BeneVision, BeneView, ePM, iPM, uMEC, iMEC series monitors, BeneHeart defibrillator

Picture	Model	Part No.	No. Description	Purchasing Unit
	IM2201	001C-30-70759	12 Pin IBP Cable (for ICU Medical), 4 m	Each
	IM2202	001C-30-70757	12 Pin IBP Cable (for BD), 4 m	Each
	IM2207	0010-21-43082	12 Pin IBP Cable (for Memscap, SP844 82031 transducer), 4 m	Each




Picture	Model	Part No.	No. Description	Purchasing Unit
	IM2211	0010-21-12179	12 Pin IBP Cable (for Edwards), 4 m	Each
	IM2206	115-017849-00	12 Pin IBP cable (for Utah), 4 m	Each





Y-type IBP cable: For BeneView, iPM series patient monitor

Picture	Model	Part No.	No. Description	Purchasing Unit
	IM2204	040-001029-00	Y-type IBP cable (switch one connector to two connectors)	Each






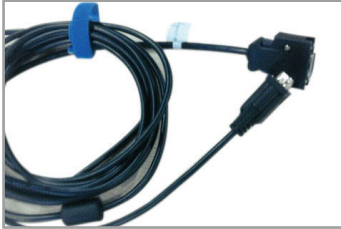

Rolling stands

Picture	Model	Part No.	No. Description	Purchasing Unit
		045-003133-00	Roll Stand A (≤ 23kg, fixed-angle) (for N22/N19)	Each
		045-000915-00	Roll Stand B (≤15kg, fixed-angle, with two baskets) + Adapter (for N17/N15/ePM15/ePM15M)	Each
		045-003255-00	Roll Stand C (≤6kg, fixed-angle, with two brakets and barrel fix mounting) + Quick lock (for N12, ePM under 12" inch screen)	Each
		045-000924-00	Roll stand (for N12, ePM and uMEC under 12" inch screen)	Each

Picture	Model	Part No.	No. Description	Purchasing Unit
		045-003053-00	Basic rolling stand (for ePM under 12" inch screen and uMEC series in ROW market)	Each
		045-003052-00	VS series basic rolling stand (ONLY for ROW market)	Each
		045-004267-00	Rolling Stand (Standard) + commen Quick lock (compact with all existing models under 12" inch screen and VS)	Each
		045-004268-00	VS 8/9 Rolling Stand (Advanced) + commen Quick lock	Each
		045-004269-00	VS 8/9 Rolling Stand (Advanced, with extended battery capacity) + commen Quick lock (the extended battery 115-034132-00 need to be purchased separately)	Each

Others

Picture	Model	Part No.	No. Description	Purchasing Unit
		009-003116-00	Nurse call cable (for ePM, VS series)	Each
		8000-21-10361	Nurse call cable (for N series)	Each
		009-005391-00	Output cable for ECG, IBP analog signal and Defib. Sync, MPM with MP1 port (for N series)	Each

Picture	Model	Part No.	No. Description	Purchasing Unit
		009-003117-00	Analog output cable (for ePM, iPM, uMEC, iMEC series)	Each
		009-003118-00	Defib Sync cable (for ePM, iPM, uMEC, iMEC series)	Each
		A30-000001---	Thermal Paper (50 mmX20 m)	Each

**REFERENCE: IBP-UT**

compatible Disposable IBP transducer  
with Utah/Biosensors connector, to  
work with Utah/Biosensor compatible

Manufacture date: 2022-10

expiry date: 2025-10

Lot number: 2210

Origin: China



Shunmei Medical Co. Ltd  
No.8 Jinlong Street, Baolong  
Industrial Zone, Longgang  
District, Shenzhen, China  
Tel: 0086-18344359973







NMT Accessory Kit  
For BeneVision series monitors

Part No.	NO. Description	Purchasing Unit
115-040403-00	NMT accessory kit Including: 040-001462-00 NMT main cable 040-001463-00 NMT transducer cable 040-001464-00 NMT stimulation cable 040-002711-00 Adult ECG electrode (INTCO), 5 pcs 040-002258-00 Bandage for NMT transducer, disposable, 20 pcs	Set
115-057396-00	NMT accessory kit Including: 040-001462-00 NMT main cable 040-001463-00 NMT transducer cable 040-001464-00 NMT stimulation cable 040-002711-00 Adult ECG electrode (INTCO), 5 pcs 115-058073-00 Reusable NMT handadapter for adult/pediatric A30-000010---- Shipping label printing paper 100X150 mm	Set

INVOS rSO<sub>2</sub> Accessories  
For BeneVision series monitors

Picture	Part No.	Description
	115-033947-00	INVOS rSO <sub>2</sub> accessory kit, Adu Including: INVOS 5100C cable, channel 1&2, with Pre-ampliter A 1pcs INVOS 5100C reusable sensor, channel 1 (blue) 1pcs INVOS 5100C reusable sensor, channel 2 (brown) 1pcs INVOS SomaSensor disposable sensor, Adu>40kg, 2 pcs
	115-033948-00	INVOS rSO <sub>2</sub> accessory kit, Ped Including: INVOS 5100C cable, channel 1&2, with Pre-ampliter A 1pcs INVOS 5100C reusable sensor, channel 1 (blue) 1pcs INVOS 5100C reusable sensor, channel 2 (brown) 1pcs INVOS SomaSensor disposable sensor, Ped<40kg, 2 pcs
	115-033949-00	INVOS rSO <sub>2</sub> accessory kit, Neo Including: INVOS 5100C cable, channel 1&2, with Pre-ampliter A 1pcs INVOS cable + disposable sensor, Neo<5kg, brain/body, 2 pcs