



BC "MOLDINDCONBANK" S.A. Filiala "Invest"

Republica Moldova, MD-2068
mun. Chişinău, bd. Moscovei, 14/1
Tel. : (373-22) 43-44-81, 43-46-24
Fax : (373-22) 43-44-22
cod: MOLDM2X329

Data 14. IAN. 2016
Nr. 03/2 - 19/23

Республика Молдова, MD-2068
мун. Кишинэу, бул. Московей, 14/1
Тел. : (373-22) 43-44-81, 43-46-24
Факс : (373-22) 43-44-22
код: MOLDM2X329

Filiala „Invest” BC „Moldindconbank” SA confirmă existența contului curent
in moneda nationala al **“BIOSISTEM MLD” S.R.L. (c/f 1010600028048)**, cu
IBAN MD95ML000000002251429243.

Codul băncii MOLDM2X329.

Director

Nina Turcan

Director financiar



Nina Balmuş

Ex. Diana Brinza
Tel. 43-45-96

REPUBLICA



MOLDOVA

CERTIFICAT DE ÎNREGISTRARE

Societatea cu Răspundere Limitată "BIOSISTEM MLD"
— ESTE ÎNREGISTRATĂ LA CAMERA ÎNREGISTRĂRII DE STAT —

Numărul de identificare de stat - codul fiscal
1010600028048

Data înregistrării

12.08.2010

Data eliberării

12.08.2010

Svirepova Ludmila, registrator

*Funcția, numele, prenumele persoanei
care a eliberat certificatul*

L. Svirepova
semnătura

MD 0101250





AGENȚIA SERVICII PUBLICE

Departamentul înregistrare și licențiere a unităților de drept

EXTRAS

din Registrul de stat al persoanelor juridice

Nr. 531522 data 15.09.2023

Denumirea completă: **Societatea cu Răspundere Limitată "BIOSISTEM MLD"**

Denumirea prescurtată: **"BIOSISTEM MLD" S.R.L.**

Forma juridică de organizare: **Societate cu răspundere limitată,**

Numărul de identificare de stat și codul fiscal (IDNO): **1010600028048**

Data înregistrării de stat: **12.08.2010**

Sediul: **MD-2001, str. Albișoara, 16/1, ap. 7, mun. Chișinău, Republica Moldova.**

Obiectul principal de activitate:

- 1. Activitatea farmaceutică; importul și (sau) producerea articolelor de parfumerie și cosmetică**
- 2. Fabricarea, comercializarea, asistența tehnică, repararea și verificarea articolelor de tehnică și optică medicală**
- 3. Acordarea asistenței medicale de către instituțiile medico-sanitare private**
- 4. Comerțul cu ridicata al calculatoarelor, echipamentelor periferice și software-ului**
- 5. Întreținerea și repararea mașinilor de birou și a tehnicii de calcul**
- 6. Consultații în domeniul sistemelor de calcul**

Capitalul social: **5400 lei.**

Administrator: **POIATA VITALIE, IDNP 0983103892591,**

Asociații:

1. **POIATA VITALIE, IDNP 0983103892591, cota 1803,60 lei, ce constituie 33,4%**

Beneficiar efectiv:

1.1. **POIATA VITALIE, IDNP 0983103892591,**

2. **NASEDCHIN ALEXANDR, IDNP 2002001070747, cota 1798,20 lei, ce constituie 33,3%**

Beneficiar efectiv:

2.1. **NASEDCHIN ALEXANDR, IDNP 2002001070747,**

3. **KOJEVNIKOV DMITRII, IDNP 0972305012362, cota 1798,20 lei, ce constituie 33,3%**

Beneficiar efectiv:

3.1. **KOJEVNIKOV DMITRII, IDNP 0972305012362**

Prezentul extras este eliberat în temeiul art.34 al Legii nr.220-XVI din 19 octombrie 2007 privind înregistrarea de stat a persoanelor juridice și a întreprinzătorilor individuali și confirmă datele din Registrul de stat la data de: **15.09.2023.**

**Registrator în domeniul
înregistrării de stat**

Digitally signed by Rusu Diana
Date: 2023.09.15 16:44:17 EEST
Reason: MoldSign Signature
Location: Moldova



Rusu Diana



EB 0461494

Lista fondatorilor Biosistem-mld SRL

Nr.	Nume, Prenume	IDNP
1.	Vitalie Poiata	0983103892591
2.	Alexandr Nasedchin	2002001070747
3.	Dmitrii Kojevnikov	0972305012362

Liga²®
Titanium Ligating Clips



TITANIUM

Reliable Ligation

Ligating Clips

LigaV[®]


LigaV[®] Ligating clips are implantable medical devices. They are widely used in surgery for marking and ligating purposes. Medical practitioners value the product for its hemostatic features.

LigaV[®] manufactured by Grena Ltd., comes with inner and outer serration which enhances its function. The outer serration helps to grip the clip in the applicator's jaws; the inner serration enables its proper nourishment.

The product is offered in 4 standard sizes ensuring every user will be able to find appropriate clip for the given tissue. The LigaV[®] clips are delivered in colour coded cartridges to ensure easy and intuitive identification. A cartridge includes 4 or 6 clips that ensure economical and comfortable use. The product is disposable, sterilised with EO.

Clip applicators with proper sized jaws depending on the clip should be used. Clip applicators are made of highest quality surgical grade steel. Handle rings are color coded matching cartridge hue.

Low density
High strength
Full biocompatibility
Safe for MRI

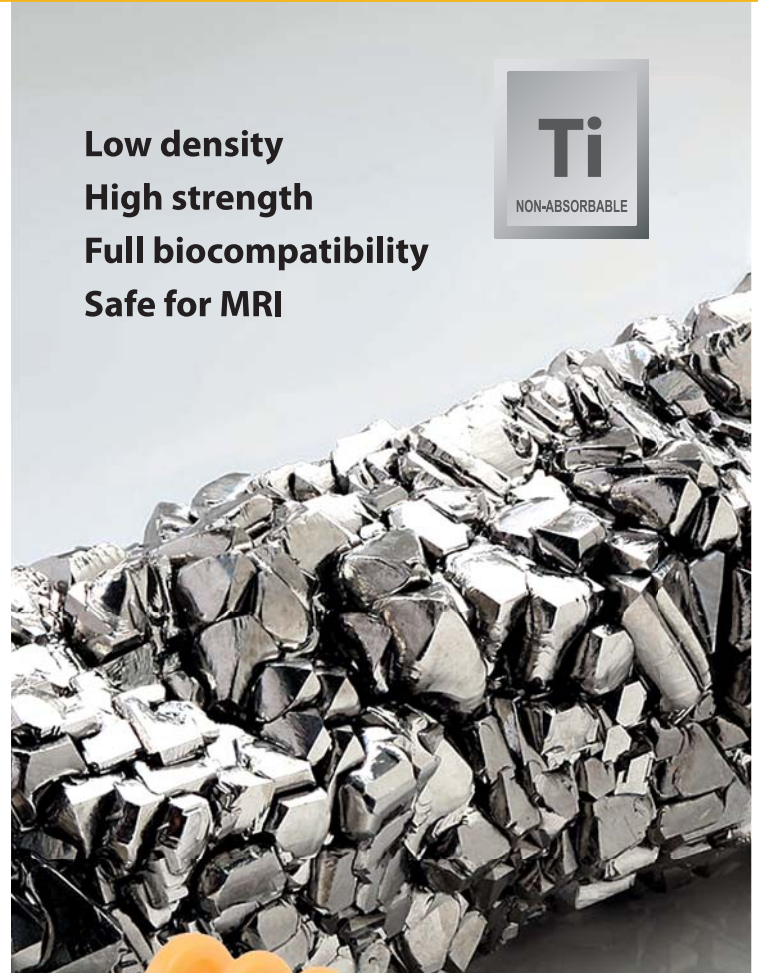

Ligating Clips

LigaV[®]

The LigaV[®] ligating clips are manufactured of a medical grade titanium which ensures proper level of biocompatibility. The applied technology guarantees the product meets the requirements of even the most demanding clinical institutes.



TITANIUM

Ligating Clips

Ligating Clips

**Cost-effective alternative
for simple procedures**








4 clips per cartridge





Key features

- 4 sizes to ligate tissue structures,
- made of apyrogenic titanium,
- easy loading system,
- clips delivered in color-coded cartridges for easy identification,
- 4 or 6 clips per cartridge to ensure economical and comfortable use of the product,
- V-shaped,
- color-coded applicator rings for easy identification



REF	Clip size	Compatible with applicators (jaws grip) (mm)	Product specification	Colour	Pcs per cartridge	Pcs cartridges per box
0301-01S	Small	0,59-0,75	V-shaped titanium ligating clips		6	50
0301-01M	Medium	0,84-1,00			6	50
0301-01ML	Medium-Large	1,16-1,32			6	20
0301-01ML04	Medium-Large	1,16-1,32			4	20
0301-01L	Large	1,26-1,42			6	20

Open Surgery Clip Appliers

-  S
-  M
-  ML
-  L



Open Surgery Clip Appliers

**Ergonomic and effective approach
in endoscopic procedures**

Open Surgery Clip Appliers

Open Surgery Clip Appliers

Key features

- available for Small, Medium, Medium-Large and Large non-absorbable LigaV® clips to be used on large spectrum of tissue sizes,
- 15cm, 20cm and 28cm clip,
- non-detachable design for easier maintenance and durability, appliers with proper sized jaws made of high quality stainless steel,
- colour-coded rings matching cartridge hue,
- compatible with corresponding sizes of LigaV® titanium non-absorbable clips.



REF	Clip size	Applier length	Pcs per box
0301-02S15*	Small	15	1
0301-02S20	Small	20	1
0301-02S28*	Small	28	1
0301-02M15*	Medium	15	1
0301-02M20	Medium	20	1
0301-02M28*	Medium	28	1
0301-02ML20	Medium-Large	20	1
0301-02ML28	Medium-Large	28	1
0301-02L20	Large	20	1
0301-02L28	Large	28	1



* Manufactured on request.

Endoscopic Clip Appliers

Endoscopic Clip Appliers

Key features

- available for Medium, Medium-Large and Large non-absorbable LigaV® clips to be used on large spectrum of tissue sizes,
- jaws activated by front handle for better stability,
- 360° shaft rotation by index finger allows one-hand operation,
- flushing port facilitates easy cleaning, thus eliminating potential contamination,
- made of high quality stainless steel,
- colour coded size matching cartridge hue,
- compatible with corresponding sizes of LigaV® titanium non-absorbable clips.

REF 0301-02ME

Size	M
Colour	○
Shaft diameter (mm)	5
Trocar diameter (mm)	5
Working length (cm)	33
Loading	front - loaded
Box quantity (pcs)	1



REF 0301-02MLE

Size	ML
Colour	●
Shaft diameter (mm)	10
Trocar diameter (mm)	10
Working length (cm)	33
Loading	front - loaded
Box quantity (pcs)	1





REF 0301-02LE

Size	L
Colour	●
Shaft diameter (mm)	10
Trocar diameter (mm)	10
Working length (cm)	33
Loading	front - loaded
Box quantity (pcs)	1



Endoscopic Clip Appliers

-  M
-  ML
-  L



Endoscopic Clip Appliers

**Ergonomic and effective approach
in endoscopic procedures**



Endoscopic Clip Appliers



Bariatric Endoscopic Clip Appliers - 45 cm

Extra length for bariatric surgery

Endoscopic Clip Appliers

Bariatric Endoscopic Clip Appliers

Key features

- 45 cm long shaft,
- available for Medium, Medium-Large and Large non-absorbable LigaV[®] clips to be used on large spectrum of tissue sizes,
- jaws activated by front handle for better stability,
- 360° shaft rotation by index finger allows one-hand operation,
- flushing port facilitates easy cleaning, thus eliminating potential contamination,
- made of high quality stainless steel,
- colour coded size matching cartridge hue,
- compatible with corresponding sizes of LigaV[®] titanium non-absorbable clips.

REF 0301-02MEB

Size	M
Colour	○
Shaft diameter (mm)	5
Trocar diameter (mm)	5
Working length (cm)	45
Box quantity (pcs)	1



REF 0301-02MLEB

Size	ML
Colour	●
Shaft diameter (mm)	10
Trocar diameter (mm)	10
Working length (cm)	45
Box quantity (pcs)	1



REF 0301-02LEB

Size	L
Colour	●
Shaft diameter (mm)	10
Trocar diameter (mm)	10
Working length (cm)	45
Box quantity (pcs)	1



Accessories

Accessories

REF	Product	Clip size	Pcs per box
0301-05CB	Cartridge base	S, M, ML, L	1



New International Initiative

GRENA[®] DG
Think Medical

Grena forges Talents!



Who's next?

Visit us

<http://talents.grena.co.uk>

Brentford 23.04.2012

TECHNICAL PARAMETERS OF GRENA TITANIUM AND POLYMER LIGATING CLIPS

LigaV

REF	S	M	ML	L
Clip shape in the cartridge	V shaped	V shaped	V shaped	V shaped
Opened clip length (outer) after loading into applier	3,20 mm	4,70 mm	8,00 mm	11,90 mm
Opened clip width (internal) after loading into applier	2,10 mm	2,90 mm	5,20 mm	5,40 mm
Closed clip length	3,70 mm	5,40 mm	9,00 mm	12,30 mm
Recommended tissue thickness	0,30-1,50 mm	1,00-2,50 mm	2,50-4,00 mm	3,50-7,50 mm

Vclip

REF	XS	S	M	ML	L
Clip shape in the cartridge	Chevron shaped	Chevron shaped	Chevron shaped	Chevron shaped	Chevron shaped
Opened clip length (outer) after loading into applier	2,25 mm	3,20 mm	5,30 mm	8,10 mm	11,00 mm
Opened clip width (internal) after loading into applier	1,80 mm	2,00 mm	3,30 mm	5,30 mm	7,70 mm
Closed clip length	2,65 mm	3,70 mm	6,00 mm	9,10 mm	12,50 mm
Recommended tissue thickness	0,15-0,30 mm	0,30-1,50 mm	1,00-2,50 mm	2,50-4,00 mm	3,50-7,50 mm

Click'aV

REF	M	ML	L	XL
Clip shape in the cartridge	Divergent curved	Divergent curved	Divergent curved	Divergent curved
Outer leg length	7,00 mm	9,50 mm	13,00 mm	17,80 mm
Clip leg thickness	0,83 mm	0,83 mm	1,29 mm	1,29 mm
Retention bosses diameter	1,00 mm	1,10 mm	1,20 mm	1,30 mm
Recommended tissue thickness	2 - 7 mm	3 - 10 mm	5 - 13 mm	7 - 16 mm
Hinge type	Living hinge	Living hinge	Living hinge	Living hinge
Retention bosses distance in the applier	5,50 mm	7,50 mm	10,20 mm	14,00 mm

DECLARATION OF CONFORMITY

Manufacturer Grena Limited
1000 Great West Road
Brentford, Middlesex, TW8 9HH
United Kingdom

Product(s)

Disposable circular staplers with related surgical instruments (class IIb, rule 8)
Disposable linear staplers and cartridges for linear staplers (class IIb, rule 8)
Disposable bone marrow aspiration needles (class IIa, rule 6)
Disposable bone marrow biopsy needles (class IIa, rule 6)
Disposable staples cartridges for reusable linear staplers (class IIb, rule 8)
Disposable staples cartridges for reusable circular staplers (class IIb, rule 8)
Disposable endoscopic linear cutting staplers (class IIa, rule 6)
Cartridges for disposable endoscopic linear cutting staplers (class IIb, rule 8)
Surgical meshes (class IIb, rule 8)
Disposable automatic clip appliers with clips (class IIb, rule 8)
LigaV® – Titanium ligating clips (class IIb, rule 8)
VClip® – Titanium ligating clips (class IIb, rule 8)
Click'a-V® – Polymer ligating clips (class IIb, rule 8)
Disposable endoscopic instruments:
Disposable grasper with ratchet atraumatic fenestrated (class IIb, rule 9)
Disposable grasper with ratchet-Allis (class IIb, rule 9)
Disposable grasper with ratchet-Maxi Grip (class IIb, rule 9)
Disposable toothed grasper with ratchet (class IIb, rule 9)
Disposable grasper with ratchet –Babcock (class IIb, rule 9)
Disposable Metzenbaum scissors-curved (class IIb, rule 9)
Disposable scissors-straight (class IIb, rule 9)
Disposable scissors-hook (class IIb, rule 9)
Disposable dissector-Maryland (class IIb, rule 9)
Disposable dissector with ratchet- Maryland (class IIb, rule 9)
Disposable endoscopic dissector 3mm – Maryland, non-ratcheted
Disposable endoscopic dissector 3mm – Maryland, ratcheted
Disposable endoscopic grasper 3mm – atraumatic fenestrated
Disposable endoscopic scissors 3mm – curved
Limited use endoscopic instruments:
Limited use dissector- Maryland (class IIb, rule 9)
Limited use dissector with ratchet- Maryland (class IIb, rule 9)
Limited use Metzenbaum scissors- curved (class IIb, rule 9)
Limited use scissors-straight (class IIb, rule 9)
Limited use scissors-hook (class IIb, rule 9)
Limited use grasper with ratchet atraumatic fenestrated (class IIb, rule 9)
Limited use disposable grasper with ratchet-Allis (class IIb, rule 9)
Limited use grasper with ratchet-Maxi Grip (class IIb, rule 9)
Limited use toothed grasper with ratchet (class IIb, rule 9)
Limited use grasper with ratchet –Babcock (class IIb, rule 9)
Reusable endoscopic surgical instruments (class IIb, rule 9)
Disposable linear cutting staplers and cartridges for cutting staplers (class IIb, rule 8)
Disposable trocars with accessories (class IIa, rule 7)
Sterile disposable skin staplers (class IIa, rule 7)
Thoracentesis/paracentesis sets (class IIa, rule 6)
Suction cannulas and suction sets (class IIa, rule 7)
Suction-irrigation sets (class IIa, rule 6)
Disposable skin staples removers (class I sterile, rule 1)
Chest drainage systems (class I sterile, rule 1)
Connecting tubes (class I sterile, rule 1)
Retrieval bags (class IIa, rule 6)
Veress needles (class IIa, rule 6)
Silicone slings (class IIa, rule 6)
Arida® absorbing pads (class I, rule 1)
Arida® absorbing pads – sterile (class I sterile, rule 1)
Solidifying agent (class I, rule 1)
Open surgery and endoscopic clip appliers (class I, rule 6)
Vomit bags (class I, rule 1)

Classification According to Annex IX of Directive 93/42/EEC

We herewith declare under our sole responsibility that the above mentioned products meet the provisions of the directive 93/42/EEC concerning medical devices which apply to them. All supporting documentation is retained under the premises of the manufacturer.

Standards Applied

All applicable harmonized standards required by the Directive 93/42/EEC. The detailed list in the Technical Files.

Notified Body

CE 0197

TÜV Rheinland LGA Products GmbH
Lillystrasse 2
90431 Nürnberg
Germany

EC Certificate(s)

HD 60040590 0001
DD 60040589 0001

Brentford, 09.05.2014

Wiesław Brodaczewski
Director

