

## **STREPTOMYCIN ELISA**

*5111STREP[18]02.24*

A competitive enzyme immunoassay for the  
screening and quantitative analysis of  
Streptomycin and Dihydrostreptomycin in  
various matrices

# EUROPROXIMA STREPTOMYCIN ELISA

**A competitive enzyme immunoassay for the screening and quantitative analysis of Streptomycin and Dihydrostreptomycin in various matrices**

## TABLE OF CONTENTS

	PAGE:
Brief Information .....	2
1. Introduction .....	2
2. Principle of the Streptomycin-ELISA .....	3
3. Specificity and Sensitivity .....	4
4. Handling and Storage .....	5
5. Kit contents .....	6
6. Equipment and materials required but not provided .....	7
7. Safety precautions .....	7
8. Sample preparations .....	8
9. Preparations of reagents .....	10
10. Assay Procedure .....	12
11. Interpretation of results .....	14
12. Literature .....	15
13. Ordering information .....	15
14. Revision history .....	15

The quality management system of R-Biopharm Nederland B.V. is  
ISO 9001:2015 certified

5111STREP[18]02.24



**Table I:** Provisional Maximum Residue Limits (mg/kg) for aminoglycosides.

<b>Aminoglycoside</b>	<b>Kidney</b>	<b>Liver</b>	<b>Muscle</b>	<b>Milk</b>	<b>Fat</b>	<b>Eggs</b>
<b>Streptomycin</b>	1.0	0.5	0.5	0.2	0.5	-
<b>Dihydrostreptomycin</b>	1.0	0.5	0.5	0.2	0.5	-
<b>Gentamicin</b>	0.75	0.2	0.05	0.1	0.05	-
<b>Neomycin</b>	5.0	0.5	0.5	1.5	0.5	0.5

EuroProxima has also available a Neomycin- and a Gentamicin-ELISA.

## 2. PRINCIPLE OF THE STREPTOMYCIN-ELISA

The microtiter based ELISA kit consists of 12 strips, each 8 wells, precoated with sheep antibodies to rabbit IgG. A specific antibody (rabbit anti-Streptomycin), horseradish peroxidase labelled Streptomycin (enzyme conjugate) as well as Streptomycin standards or samples are pipetted into the precoated wells followed by a single incubation step. The specific antibodies are bound by the immobilised antibodies and simultaneously free Streptomycin (present in the standard solution or sample) and enzyme labelled Streptomycin compete for the Streptomycin antibody binding sites (competitive enzyme immunoassay). After an incubation time of 1 hour, the non-bound (enzyme labelled) reagents are removed in a washing step.

The amount of Streptomycin enzyme conjugate bound to the specific antibody is visualised by the addition of chromogen / substrate (tetramethylbenzidine, TMB). During the incubation the colourless chromogen is converted by the enzyme into a blue coloured reaction product. This blue colour is inversely proportional to the amount of bound Streptomycin. The more Streptomycin is present in the standard solution or sample, the less colour is developed. The substrate reaction is stopped by the addition of sulphuric acid. In the acetic environment the blue colour changes into a yellow colour. The colour intensity is measured photometrically at 450 nm.

### 3. SPECIFICITY AND SENSITIVITY

The Streptomycin-ELISA utilizes a polyclonal antiserum raised in rabbits against protein conjugated Streptomycin.

Cross- reactivity:	Streptomycin	100	%
	Dihydrostreptomycin	100	%
	Neomycin	< 0.1	%
	Kanamycin	< 0.1	%
	Tobramycin	< 0.1	%
	Amikacin	< 0.1	%
	Gentamicin	< 0.1	%
	Sisomycin	< 0.1	%

The cross-reactivities are determined in a buffer system. The reported values may be different in samples due to matrix effects.

The test cannot discriminate between analytes and cross-reactive substances

The Limit of detection (LOD) is determined under optimal conditions. Cut-off criteria need critical consideration.

<b>Matrix</b>	<b>Procedure</b>	<b>LOD (ppb)</b>
Milk	8.1	4
Tissue	8.2	10
Serum	8.4	2
Urine	8.7	4
Honey	8.5.1	6
Honey	8.5.2	5
Royal Jelly	8.5.2	5
Egg	8.6	2

If the sample is found to be non-compliant, the results shall be verified by re-analysis of the sample using a confirmatory method.

#### 4. HANDLING AND STORAGE

- Kit and kit components should be stored at 2°C to 8°C in a dark place. For repeated use store kit components as specified under chapter 9.
- After the expiry date of the kit and/or components has passed, no further quality guarantee is valid.
- Bring all kit components including the microtiter plate to ambient (room) temperature before use.
- Dilute the kit components immediately before use, but after the components are brought to ambient temperature.
- Avoid condensation in the wells of the plate. Bring the sealed plate to ambient temperature before opening the plate sealing.
- The substrate chromogen solution can be stored in a refrigerator (2°C to 8°C) until the expiry date stated on the label.
- Exposure of the chromogen solution to light should be avoided.

Degeneration of the reagents may have occurred when the following phenomena are observed:


- A blue colouring of the chromogen solution before transferring it into the wells.
- A weak or no colour reaction in the zero standard wells ( $E_{450nm} < 0.8$ ).

## 5. KIT CONTENTS

Manual

1 sealed microtiter plate (12 strips, 8 wells each), coated with antibodies to rabbit IgG. Ready-to-use.

Position of the reagents in the kit. For preparation of the reagents see Chapter 9.

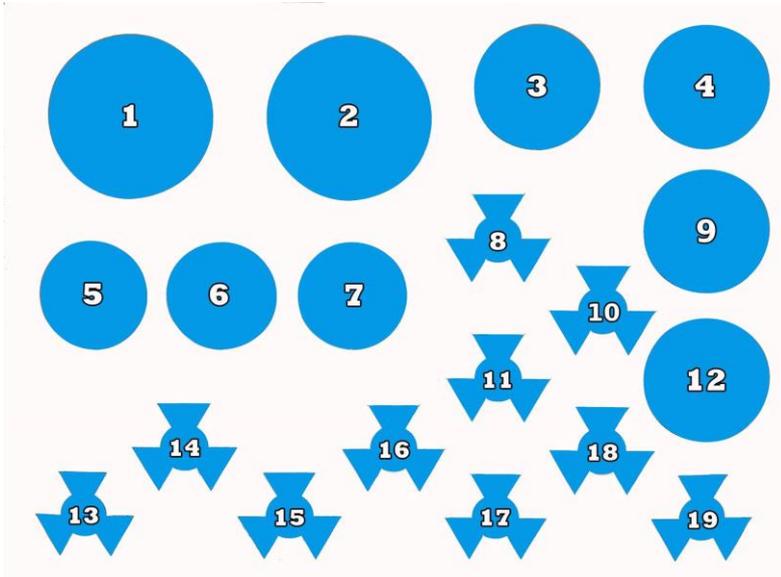

1. **Dilution buffer** (20 ml, Ready-to-use)
2. **Rinsing buffer** (30 ml, 20x concentrated)
3. **Substrate solution** (12 ml, Ready-to-use)
4. **Stop solution** (15 ml, Ready-to-use)
5. **Conjugate** (lyophilised, blue cap)
6. **Antibody** (lyophilised, yellow cap)
7. not in use
8. **Standard solution 100 ng/ml** (1ml, Ready-to-use))
9. not in use
10. not in use
11. not in use
12. not in use
13. **Zero Standard solution** (2ml, Ready-to-use)
14. **Standard solution 1** (1ml, Ready-to-use) **0.25 ng/ml**
15. **Standard solution 2** (1ml, Ready-to-use) **0.5 ng/ml**
16. **Standard solution 3** (1ml, Ready-to-use) **1 ng/ml**
17. **Standard solution 4** (1ml, Ready-to-use) **2 ng/ml**
18. **Standard solution 5** (1ml, Ready-to-use) **10 ng/ml**
19. **Standard solution 6** (1ml, Ready-to-use) **20 ng/ml**

## 6. EQUIPMENT AND MATERIALS REQUIRED BUT NOT PROVIDED

- Scales and weighing vessels
- Gloves
- Fume hood
- Homogeniser (blender, Ultra Turrax, mixer)
- Centrifuge (for 10 – 15 ml test tubes, with cooling, 2000xg)
- Vortex
- Automated microplate washer or 8 channel micropipette 100-300  $\mu$ l
- Magnetic stirrer
- Microtiter plate shaker
- Siliconised glass test tubes or plastic tubes
- Micropipettes 20-200  $\mu$ l, 100-1000  $\mu$ l
- Multipipette with 2.5 ml combitips
- Aluminum foil or parafilm
- 0.8  $\mu$ m Filter
- SPE Column
- Disodium hydrogen phosphate
- Potassium dihydrogen phosphate
- Potassium chloride
- Sodium chloride
- Distilled water
- Tween 80
- Methanol 100%

## 7. PRECAUTIONS

- This kit may contain hazardous substances. For hazard notes please refer to the appropriate safety data sheets (SDS).
- Avoid contact of all biological materials with skin and mucous membranes.
- Do not pipette by mouth.
- Do not eat, drink, smoke, store or prepare foods, or apply cosmetics within the designated work area.
- Do not use components past expiration date and do not use components from different lots.
- Each well is ultimately used as an optical cuvette. Therefore, do not touch the under surface of the wells, prevent damage and dirt.
- All components should be completely dissolved before use. Take special attention to the substrate and rinsing buffer, which crystallize at +4°C.
- Optimal results will be obtained by strict adherence to this protocol. Careful pipetting and washing throughout this procedure are necessary to maintain good precision and accuracy.

R-Biopharm Nederland makes no warranty of any kind, either expressed or implied, except that the materials from which its products are made are of standard quality. There is no warranty of merchantability of this product, or of the fitness of the product for any purpose. R-Biopharm Nederland shall not be liable for any damages, including special or consequential damage, or expense arising directly or indirectly from the use of this product.

## 8. SAMPLE TREATMENT

### 8.1 Milk samples

- Defat milk by centrifugation for 10 min. at 4°C and 2000 x g.
- Eliminate the upper fat layer.
- Dilute and homogenize the defatted milk sample 10 times in sample dilution buffer (see chapter 9)
- Check pH  $7.4 \pm 0.4$ .
- Pipette 50  $\mu$ l of this solution into the microtiter plate.

### 8.2 Tissue samples

- Weigh 5 gram finely cut subsequently homogenized tissue in a plastic tube
- Add 20 ml sample dilution buffer (see chapter 9)
- Homogenise (for instance using an Ultra Turrax or head over head mixer) for 30 minutes
- Centrifuge a part of the mixture 10 minutes at 4000 x g at 4°C
- Remove the upper fat layer
- Pipette 50  $\mu$ l supernatant into a plastic tube, add 450  $\mu$ l SDB, vortex
- Use 50  $\mu$ l of this solution in the microtiter plate.

### 8.3 Fat samples

- Weigh 1 g of homogenized (melted) fat in a plastic tube.
- Add 10 ml of sample dilution buffer (see chapter 9) and heat in a water bath at 70°C for 30 min.
- Centrifuge 15 min., 2000 x g, at 4°C.
- Remove the upper fat layer and pipette 1 ml of sample extract in a plastic tube.
- Add 4 ml of sample dilution buffer, mix well.
- Pipette 50  $\mu$ l of this solution into the microtiter plate.

### 8.4 Serum samples

- Dilute serum samples 10 times in sample dilution buffer (see chapter 9) .
- E.g. pipette 50  $\mu$ l of serum sample into a clean siliconised glass tube or plastic vial.
- Add 450  $\mu$ l of sample dilution buffer.
- Mix well using a vortex
- Use 50  $\mu$ l of this solution in the microtiter plate.

## 8.5 Honey and Royal Jelly samples

### 8.5.1. Honey diluted

- Weigh 1 g of homogenized honey in a plastic tube
- Add 4 ml of sample dilution buffer (see chapter 9) and mix well using a vortex
- When no clear solution is obtained filtrate the solution through a 0.8 µm filter
- Pipette 1 ml of the mixture into a clean tube and add 4 ml of sample dilution buffer
- Mix well using a vortex
- Use 50 µl of this solution in the ELISA.

The dilution procedure is not applicable for all honey samples nor Royal Jelly. The composition of the honey sample may give background in the ELISA. For these samples we advise the SPE procedure.

A homogenous sample has to be obtained from a representative part of the honey and Royal Jelly.

### 8.5.2. SPE procedure

- Weigh 1 g of homogenized honey or Royal Jelly into a plastic tube
- Add 9 ml of distilled water, vortex
- Mix head over head, 30 minutes (Rotor)

Activate the column

- Add 1 ml Methanol 100%
- Add 1 ml Distilled water

Note: It is important that the cartridge is not allowed to dry completely during activation and prior to sample addition.

Filtrate the royal jelly mixture through an 0,8 µm filter

Carefully transfer 2 ml diluted honey or 2 ml royal jelly filtrate onto the activated column (flow 1 ml/min.)

Washing procedure

- Wash the column with 2 ml Methanol 100%
- Let the column dry for two minutes

Elution of the Streptomycin

- Pipette 2 ml sample dilution buffer (see chapter 9) onto the column
- Collect eluent
- Let the column dry for two minutes
- Diluted the eluate 1:1 with sample dilution buffer
- Pipette 50 µl of this solution in the microtiter plate

### 8.6 Egg samples

- Homogenise an egg, both egg-protein and yolk
- Pipette 1 ml of the homogenised sample into a clean tube
- Add 4 ml of sample dilution buffer (see chapter 9)
- Mix well using a vortex
- Use 50 µl of this solution in the microtiter plate

### 8.7 Urine samples

- Dilute urine samples 10 x in sample dilution buffer (see chapter 9)
- E.g. pipette 1 ml of urine sample into a clean siliconised glass tube or plastic vial.
- Add 9 ml of sample dilution buffer
- Check pH  $7.4 \pm 0.4$ .
- Use 50 µl of this solution in the ELISA.

## 9. PREPARATION OF REAGENTS

Before starting the test, the reagents should be brought up to ambient temperature.

### Microtiter plate

Return unused strips into zip lock bag with desiccant and store at +2°C to +8°C for use in subsequent assays. Retain also the strip holder.

### Rinsing buffer

The rinsing buffer is delivered 20 times concentrated. Prepare dilutions freshly before use. Per strip 20 ml of diluted rinsing buffer is used (1 ml concentrated rinsing buffer + 19 ml distilled water).

### Substrate solution

The substrate solution (ready-to-use) precipitates at 4°C. Take care that this vial is at room temperature (keep in the dark) and mix the content before pipetting into the wells.

### Standard solutions 100 ng/ml

To prepare standards in the appropriate matrix or to prepare spikes use the standard solution containing 100 ng Streptomycin per ml. Dilute the standard solution in the appropriate matrix to make a dilution range of 20, 10, 2, 1, 0.5, 0.25 ng/ml. Also the zero standard should be of the same matrix.

### Conjugate solution

Reconstitute the vial of lyophilised conjugate (Streptomycin-HRP) with 4 ml of dilution buffer, mix thoroughly and keep in the dark until use.

### Antibody solution

Reconstitute the vial of lyophilised antibodies with 4 ml of dilution buffer, mix thoroughly and keep in the dark until use.

Sample dilution buffer

Sample dilution buffer is not provided in the kit. Prepare this buffer as follows:

Dissolve in 1 litre distilled water:

Na <sub>2</sub> HPO <sub>4</sub>	1.15 g
KH <sub>2</sub> PO <sub>4</sub>	0.2 g
KCl	0.2 g
NaCl	30 g
Tween 80	0.5 ml
pH	7.4 (7.3-7.5)

## 10. ASSAY PROCEDURE

### Rinsing protocol

In ELISA's, between each immunological incubation step, un-bound components have to be removed efficiently. This is reached by appropriate rinsing. It should be clear that each rinsing procedure must be carried out with care to guarantee good inter- and intra-assay results. Basically, manual rinsing or rinsing with automatic plate wash equipment can be done as follows:

### Manual rinsing

1. Empty the contents of each well by turning the microtiter plate upside down followed by a firm short vertical movement.
2. Fill all the wells to the rims (300  $\mu$ l) with rinsing solution.
3. This rinsing cycle (1 and 2) should be carried out 3 times.
4. Turn the plate upside down and empty the wells by a firm short vertical movement.
5. Place the inverted plate on absorbent paper towels and tap the plate firmly to remove residual washing solution in the wells.
6. Take care that none of the wells dry out before the next reagent is dispensed.

### Rinsing with automatic microtiter plate wash equipment

When using automatic plate wash equipment, check that all wells can be aspirated completely, that the rinsing solution is nicely dispensed reaching the rim of each well during each rinsing cycle. The washer should be programmed to execute three rinsing cycles.

### Assay Protocol

1. Prepare samples according to Chapter 8 and prepare reagents according to Chapter 9.
2. Pipette 100  $\mu$ l of zero standard in duplicate (wells H1, H2).  
Pipette 50  $\mu$ l of zero standard in duplicate (wells A1, A2).  
Pipette 50  $\mu$ l of each of the standard dilutions in duplicate (wells B1, B2 to G1, G2 i.e. 20, 10, 2, 1, 0.5 and 0.25 ng Streptomycin/ml).  
Pipette 50  $\mu$ l of each sample solution in duplicate into the remaining wells of the microtiter plate.
3. Add 25  $\mu$ l of conjugate (Streptomycin-HRP) to all wells, except wells H1 and H2.
4. Add 25  $\mu$ l of antibody solution to all wells, except wells H1 and H2.
5. Seal the microtiter plate and shake the plate for a few seconds.
6. Incubate for 1 hour in the dark in a refrigerator (2°C to 8°C).

7. Discard the solution from the microtiter plate and wash 3 times with rinsing buffer.
8. Pipette 100  $\mu\text{l}$  of substrate solution into each well.
9. Incubate 30 min. in a dark place at room temperature (20°C to 25°C).
10. Add 100  $\mu\text{l}$  of stop solution to each well.
11. Read the absorbance values immediately at 450 nm.

## 11. INTERPRETATION OF RESULTS

In general, the O.D. values of the samples, that are measured in this ELISA test, are converted into corresponding concentrations in the following way:

The mean optical density (O.D.) value of the blank wells is subtracted from the individual O.D. of the wells containing the standards and the samples. Then these O.D. values of the standards and the samples (mean values of the duplicates) are divided by the mean O.D. value of the zero standard and multiplied by 100. The zero standard is thus made equal to 100% (maximal absorbance) and the other O.D. values are quoted in percentages of the maximal absorbance.

The values calculated for the standards are entered in a semi-logarithmic plot against the concentration of the analyte.

### Alternative for calibration curve:

The values of absorption (logit) calculation of the standards are plotted on Y-axis versus the analyte equivalent concentration on a logarithmic X-axis.

As customer-friendly options R-Biopharm offers 2 software programs that can be used for the interpretation of the ELISA test:

- RIDASOFT@Win.NET Food & Feed (art. nr. Z9996FF). This software program comes with a driver for your reader (if applicable) and all R-Biopharm ELISA tests (including EuroProxima) are preprogrammed in the database.
- Simplefit. This Excel based program is developed to calculate the results of all EuroProxima tests.

### Milk samples

The amount of Streptomycin and Dihydrostreptomycin in the milk samples is expressed as Streptomycin equivalents (ng/ml). The Streptomycin equivalents in the milk (ng/ml) corresponding to the percentage maximal absorbance of each sample can be read from the calibration curve. These calculated Streptomycin equivalents have to be multiplied by 10 to obtain the Streptomycin equivalents (ng/ml) in the undiluted milk sample.

### Tissue samples

The Streptomycin equivalents in the tissue extract corresponding to the percentage maximal absorbance of each sample can be read from the calibration curve. These equivalents have to be multiplied by 50 to obtain the Streptomycin equivalents (ng/g) in the tissue samples.

### Fat samples

Multiply the calculated Streptomycin equivalents by 50 to obtain the Streptomycin equivalents (ng/g) in fat samples.

### Serum samples

Multiply the calculated Streptomycin equivalents by 10 to obtain the Streptomycin equivalents (ng/ml) in undiluted serum samples.

Honey samples (dilution in buffer)

Multiply the calculated Streptomycin equivalents by 25 to obtain the Streptomycin equivalents (ng/g) in honey samples.

Honey samples (SPE solid phase extraction)

Multiply the calculated Streptomycin equivalents by 20 to obtain the Streptomycin equivalents in ng/g honey and royal jelly samples.

Egg samples

Multiply the calculated Streptomycin equivalents by 5 to obtain the Streptomycin equivalents (ng/ml) in egg samples.

Urine samples:

Multiply the calculated Streptomycin equivalents by 10 to obtain the Streptomycin equivalents (ng/ml) in undiluted urine samples.

**12. LITERATURE**

Berdy J., Aszalos A., Bostian M and McNitt K.L. Handbook of Antibiotic Compounds, Vol. 1, CRC Press Inc. Boca Raton, Florida U.S.A., 1980.

Standefor J.C. and Saunderson G.C. Enzymeimmunoassay for Gentamicin, Clin. Chem. (1978), 24, 903, 1987.

Analysis of Antibiotic Drug Residues in Food Products of Animal Origin., Ed. Vipin K. Agarwal U.S.A. 1992.

Haasnoot W., Stouten P., Cazemier G., Lommen A., Nouws J.F.M. and Keukens H.J. Immunochemical detection of Aminoglycosides in milk, and kidney. The Analyst, 1999, 124, 301-305.

**13. ORDERING INFORMATION**

For ordering the Streptomycin ELISA kit, please use cat. code 5111STREP.

**14. REVISION HISTORY**

Chapter 11 has been updated.