



Enzyme immunoassay for the detection of sulphonamides (code SM390)

I'screen SULFA is an enzyme immunoassay which allows the quantitative determination of sulphonamides. The kit contains the procedure and the materials sufficient for 96 determinations (**code SM390**) standards included. A microtiter plate or a strip photometer is required.

Samples: Muscle, egg, milk, honey. feed.

Sample preparation

- **Muscle, egg, milk (METHOD I):** homogenization, (skimming for milk), solvent extraction, centrifugation, evaporation, reconstitution.
- **Muscle, egg, honey (METHOD II)** homogenization, (acid hydrolysis for honey) buffer extraction, centrifugation and filtration.
- **Milk(METHOD II):** centrifugation and dilution.
- **Honey (METHOD III):** acidic hydrolysis, purification on SPE column, elution, evaporation, resuspension.
- **Feed:** extraction with solvent, dilution.

Assay time: 75 minutes (sample preparation not included).

Detection limit

Milk (method I) : 0,25 ppb

Muscle, egg, (method I) and honey (method III): 0.5 ppb.

Muscle, egg, honey, milk (method II): 5 ppb.

Feed: 66,6 ppb.

Compound	Specificity	Cross-reactivity (%)
Sulfamerazine		>100
Sulfamonomethoxine		>100
Sulfadiazine		>100
Sulfachloropyridazine		>100
Sulfaclozine (sulfachloropyrazine)		>100
Sulfamethoxydiazine (sulfamethoxine, sulfameter)		>100
Sulfamethoxypyridazine (sulfapyridazine)		>100
Sulfadimethoxine		>100
Sulfaquinoxaline		>100
Sulfathiazole		>100
Sulfamethizole		>100
Sulfamethazine		100
Sulfamethoxazole		90
Sulfisoxazole		50
Sulfapyridine		36
Sulfadoxine		24
Sulfacetamide		2,5
Sulfaphenazole		< 2
Sulfabenzamide		< 2
Sulfaguanidine		<0,1
Sulfanilamide		<0,1

1 TEST PRINCIPLE

The assay is performed in a polystyrene microtiter plate coated with the antigen, which constitutes the solid phase. Standards, samples and antibody are added in sequence in the microtiter plate.

During the first incubation, free sulphonamides molecules in the standards or samples and the antigen coated on the solid phase compete for the anti-sulphonamide antibody binding sites. After the first incubation, any unbound molecule is removed in a washing step.

The enzyme conjugate is then added; during the second incubation it will bind to the anti-sulphonamides antibodies bound on the solid phase. After a washing step, the enzyme conjugate-antibody bound on the solid phase is detected by the addition of a colourless substrate/chromogen solution, which during the third incubation is converted by the enzyme into a blue coloured reaction product.

After addition of the stop solution, the absorbance is measured at 450 nm with a microtiter plate photometer. The absorbance is inversely proportional to the sulphonamides concentration in the sample.

2 PROVIDED REAGENTS

Microtiter plate: 96 wells (12 strips x 8 wells), coated with the antigen.

As the strips are breakable, the wells can be used individually. For this purpose, it is sufficient to break the joint.

Sulfamethazine Standard: 6 amber plastic vials containing 1.5 ml of sulfamethazine in the following concentrations: 0 ng/ml; 0.5 ng/ml; 1 ng/ml; 10 ng/ml; 50 ng/ml, 250 ng/ml.

Anti-sulphonamides Antibody: 1 glass vial containing 8 ml of anti-sulphonamides antibody. Blue solution.

Enzyme conjugate: 1 amber plastic vial containing 0.2 ml of enzyme conjugate.

Enzyme conjugate diluent: 1 amber plastic vial containing 17 ml of the enzyme conjugate diluent. Red solution.

Washing-buffer 20X: 1 plastic bottle containing 50 ml of washing buffer.

Developing solution: 1 amber plastic bottle containing 14 ml of developing solution.

Dilution buffer 20X: 1 plastic bottle containing 30 ml of dilution buffer.

Stop solution: 1 glass bottle containing 8 ml of stop solution. White cap.

3 MATERIALS REQUIRED BUT NOT PROVIDED

For sample preparation:

- Balance (muscle, egg, honey)
- Homogenizer (muscle)
- Grinder (feed)
- NaOH, HCl, pH indicator strips (honey)
- Distilled water

METHOD I

- Shaker
- Vortex
- Refrigerated centrifuge
- System to evaporate solvent
- Ethylacetate
- n-hexane (muscle,egg)

METHOD II

- Shaker (muscle,egg)
- Vortex (honey)
- 20°C Freezer (muscle,egg)
- Refrigerated centrifuge (muscle, egg, honey)
- Incubator or water bath incubator (muscle, egg, honey)
- Filter paper (Whatman n.1) (muscle, egg, honey)

METHOD III

- Vortex
- Shaker
- Centrifuge
- System to evaporate solvent
- NH₃
- Methanol HPLC grade
- SPE Column "Strata X-C" 200 mg/6ml (cod: 8B-S029-FCH) or 100 mg/6 ml (cod.8B-S029-ECH) Fenomenex.

FEED

- Shaker
- Vortex
- Centrifuge
- Acetonitrile
- 0.45 µm filter

For assay implementation:

- Micropipette 20-200 µl and 200-1000 µl with suitable tips.
- Multichannel variable pipette (20-200 µl) with suitable tips.
- ELISA plate reader or strip photometer equipped with a 450 nm filter.

4 WARNING AND PRECAUTIONS FOR THE USERS

- For *in vitro* diagnostic use only.
- Some reagents contain solutions that may be identified as dangerous substance by the Regulation (EC) No 1272/2008. Please refer to Safety Data Sheet available on Tecna web site.
- Handle the reagents with caution, avoiding contact with skin, eyes and mucous membranes.

5 HANDLING AND STORAGE INSTRUCTIONS

- Store the kit at +2/+8 °C and never freeze any component.
- Reseal the unused strips of the microtiter plate in the bag together with the desiccant bag provided.
- Do not use components after the expiration date.
- Do not intermix components between different kit lots.
- Do not use photocopies of the instruction booklet. Keep always to the instruction booklet which is included inside the kit.

6 SAMPLE PREPARATION

6.1 Muscle

METHOD I

- Homogenize about 100 g of defatted sample without fibrous parts.
- Weight 1 g of homogenized sample.
- Add 5 ml of ethylacetate and vortex for 10 seconds.
- Shake for 15 minutes (400 rpm).
- Centrifuge at 3000g for 10 minutes at 15°C.
- Collect 3 ml of supernatant and evaporate to dryness at +50°C under a stream of nitrogen or air.
- Dissolve the residue with 0.6 ml of dilution buffer 1x.
- Add 1 ml of n-hexane, vortex for 30 seconds.

- Centrifuge at 3000g for 5 minutes.
- Collect the lower aqueous phase. The extract is ready for the assay. The dilution factor is 1.
- It is suggested to test the samples immediately after preparation.

METHOD II (alternative)

- Homogenize about 100 g of defatted sample without fibrous parts.
- Weight 1 g of homogenized sample.
- Add 10 ml of dilution buffer 1x.
- Shake for 10 minutes (400 rpm).
- Incubate at 80°C for 45 minutes.
- Refrigerate at -20°C for 20 minutes.
- Centrifuge at 4500g for 5 minutes at +2/+8°C
- Collect the supernatant and filtrate with Whatman n.1 filter paper. The extract is ready for the assay. The dilution factor is 10.
- It is suggested to test the samples immediately after preparation.

6.2 Egg

METHOD I

- Mix well the yolk and the egg white to obtain an homogeneous sample.
- Weight 1 g of sample.
- Add 5 ml of ethylacetate and vortex for 10 seconds.
- Shake for 15 minutes (400 rpm).
- Centrifuge at 3000g for 10 minutes at 15°C.
- Collect 3 ml of supernatant and evaporate to dryness at +50°C under a stream of nitrogen or air.
- Dissolve the residue with 0.6 ml of dilution buffer 1x.
- Add 1 ml of n-hexane, vortex for 30 seconds.
- Centrifuge at 3000g for 5 minutes.
- Collect the lower aqueous phase. The extract is ready for the assay. The dilution factor is 1.
- It is suggested to test the samples immediately after preparation.

METHOD II

- Mix well the yolk and the egg white to obtain an homogeneous sample.
- Weight 1 g of sample.
- Add 10 ml of Dilution buffer 1x.
- Shake for 10 minutes (400 rpm).
- Incubate at 80°C for 45 minutes.
- Refrigerate at -20°C for 20 minutes.
- Centrifuge at 4500g for 10 minutes at +2/+8°C.
- Collect the supernatant and filtrate with Whatman n.1 filter paper. The extract is ready for the assay. The dilution factor is 10.
- It is suggested to test the samples immediately after preparation.

6.3 Milk

METHOD I

- Cool the sample at 4°C.
- Centrifuge a 5 ml sample in a 50 ml Falcon tube for 15 minutes, 4000 rpm at 4°C.
- Eliminate the top fat.
- Transfer 2.5 ml of skimmed milk in a 50 ml Falcon tube.
- Add 5 ml of ethylacetate and mix upsidedown for 1 minute.
- Let separate the two phases for 5-10 minutes at room temperature.
- Take 4 ml of supernatant and evaporate it under air or N₂ stream at 50°C.
- Reconstitute with 1 ml of dilution buffer 1x.
- The dilution factor is 0.5.

METHOD II

- Refrigerate the sample at +2/+8°C and centrifuge at +2/+8°C for 10 minutes at 3000g.
- Separate the fat from the skimmed milk.

- Add to 0.1 ml of skimmed milk 0.9 ml of washing buffer 0.5x (see chapter 7). The sample is ready for the assay. The dilution factor is 10.
- It is suggested to test the samples immediately after preparation.

6.4 Honey

METHOD II

- Weigh 1 g of honey and add 1 ml of 0.5 M HCl.
- Homogenize with vortex.
- Incubate at 37°C for 30 minutes.
- Add 0.5 ml of 1M NaOH and 7.5 ml of dilution buffer 1x.
- Adjust the pH at 7.5 with NaOH 0,5M/HCl 0.5M, if necessary, using a pH indicator.
- Filter with Whatman N°1. The extract is ready for the assay. The dilution factor is 10.
- It is suggested to test the samples immediately after preparation.

METHOD III

- Weigh 3.0 g of honey.
- Add 3 ml of 2M HCl.
- Shake with vortex.
- Shake on shaker (400 rpm) for 30 minutes.
- Dilute with 17 ml of distilled water.
- Centrifuge at 4500 rpm for 10 minutes
- Purification with SPE 200 mg (100 mg) columns
- Prime the column with 5 ml of methanol and with 5 ml of 0.5 M HCl.
- Apply the diluted sample in the column.
- Wash the column sequentially with: 5 ml (3 ml) of 0,5 M HCl, 5 ml (3 ml) of n-hexane and 5 ml (3 ml) of methanol.
- Elute with 6 ml (4 ml) of methanol/30%NH3 solution in water (90/10, v/v).
- Evaporate under N2 or air stream at temperature of 50°C
- Resuspend with 1 ml of dilution buffer.
- Dilute 3 more times (for example 100 µl + 200µl of dilution buffer 1x.
- The dilution factor is 1.

6.5 Feed

- Weigh 3.0 g of grinded feed.
- Add 20 ml of a 95/5 acetonitrile/water mixture.
- Vortex for approximately 30 seconds.
- Shake on shaker for 10 minutes (400 rpm)
- Centrifuge at 4000 rpm for 10 minutes
- Dilute 20x with dilution buffer 1x(for example: 100 µl of supernatant + 1900 µl of dilution buffer 1x)
- If necessary, filter with a 0.45 µm filter. The dilution factor is 133.

7 WORKING SOLUTIONS PREPARATION

Sulfamethazine Standard: ready to use.

Anti-sulphonamides Antibody: ready to use.

Enzyme conjugate: **PAY ATTENTION**, in order to recover the total conjugate amount, centrifuge the vial briefly at low speed (spin-down) before use. Calculate and prepare the quantity necessary for the experiment. Dilute the conjugate **1/100** with the enzyme diluent (for example, 20 µl of enzyme conjugate concentrated + 1980 µl of enzyme conjugate diluent).

To draw a minimal volume of 20ul of the enzyme conjugate concentrate is recommended.

Gently mix head over head. DO NOT VORTEX.

Enzyme conjugate diluent: ready to use.

Washing buffer: **for microtiter plate washing (buffer 1x)**: dilute the concentrated washing buffer 1:20 (1+19) with distilled water; **for milk sample dilution (buffer 0.5x)**: dilute the concentrated washing buffer 1:40 (1+39) with distilled water.

ATTENTION: in presence of crystals, bring the solution at room temperature and stir in order to solve them completely.

The diluted washing buffer is stable at room temperature for 24 hours and at +2/+8°C for two weeks.

Developing solution: ready to use; the developing solution is light sensitive: keep away from direct light.

Stop solution: ready to use.

Dilution buffer: dilute the concentrated dilution buffer 1:20 (1+19) with distilled water. ATTENTION: in presence of crystals, bring the solution at room temperature and stir in order to solve them completely.

8 ASSAY PROCEDURE

8.1 Preliminary comments

- Before use, bring all reagents at room temperature.
- Return all reagents at +2/+8 °C immediately after use.
- Do not change the assay procedure, particularly:
- do not prolong or shorten the first and incubation time;
- do not incubate the plate at a temperature > 25°C or < 18°C;
- do not shake the plate during the incubations.
- Use always accurate and precise micropipettes with suitable tips;
- Once started, complete all the steps without interruption.
- The reproducibility of ELISA results largely depends upon the efficiency and uniformity of microwells washing; always keep to the described procedure.
- Use a single disposable tip for each standard and sample to avoid cross-contamination.
- Do not allow tips to contact the liquid already present in the microwells or the internal microwells surface.
- Avoid direct sunlight during all incubations. Do not use sealing tapes to cover the microtiter plate.
- ATTENTION: we warn to handle the reagents and the sample extracts with care in order to avoid cross-contaminations, particularly in case of spiking experiments.

8.2 Assay procedure

1. Predispose an assay layout, recording standards and samples positions, taking into account that all have to be run in duplicate.
2. Add 50 µl of standard /sample into the wells.
3. Using a multichannel pipet, add 50 µl of anti-sulphonamide antibody to each well and shake the plate gently with rotatory motion for few seconds.
4. Incubate 30 minutes at room temperature.

Do not prolong the first incubation time and do not use shaker.

5. Washing sequence:

- Pour the liquid out from the wells.
- Fill completely all the wells with working wash solution using a squeeze bottle. Pour the liquid out from the wells.
- Repeat the washing sequence four (4) times. Remove the remaining droplets by tapping the microplate upside down vigorously against absorbent paper.

Do not allow the wells to dry out.

6. Using a multichannel pipet, add 100 µl of enzyme conjugate to each well; shake the plate gently with rotatory motion for few seconds.
7. Incubate for 30 minutes at room temperature. *Do not prolong the incubation time and do not use shaker.*
8. Repeat the washing sequence as above.
9. Developing:

- using the multichannel micropipette, add 100 µl of developing solution to each well;
 - shake the plate gently with rotatory motion for few seconds.
10. Incubate for 15 minutes at room temperature. Protect from light.
 11. Using a multichannel pipet, add 50 µl of stop solution to each well and shake the plate gently.
 12. Measure the absorbance at 450 nm. Read within 60 minutes.

9 RESULTS INTERPRETATION

- Calculate the mean absorbance of the standards and samples.
- Divide the mean absorbance value of each standard and of the samples by the mean absorbance of the Standard 0 and multiply by 100; the Maximum Binding (Bo) is thus made equal to 100% and the absorbance values are indicated in percentage:

$$\frac{\text{absorbance standard (or sample)}}{\text{absorbance Standard 0 (B}_0\text{)}} \times 100 = \frac{B}{B_0} (\%)$$


- Enter the B/B₀ values calculated for each standard in a semi-logarithmic system of coordinates and draw the standard curve.
- Take the B/B₀ (%) value for each sample and interpolate the corresponding concentration from the calibration curve. The concentration read on the calibration curve must be further multiplied by the corresponding dilution factor, as reported in chapter 6 for each kind of matrix.

WARNING: sample preparation according to method II and milk preparation method can cause high background levels. In this case it is necessary to establish an appropriate decision limit (CC_α) for each matrix.

WARNING: By use of preparative methods I and III, the kit is more sensible than the confirmation method HPLC-DAD. Therefore supposed false positives could actually be real positives with concentrations that just LCMS/MS method is able to confirm.

Please note: For results calculation, Excel spreadsheets are available on Tecna website www.tecnalab.com and can be downloaded directly from the bottom of the product page.

10 STANDARD CURVE EXAMPLE

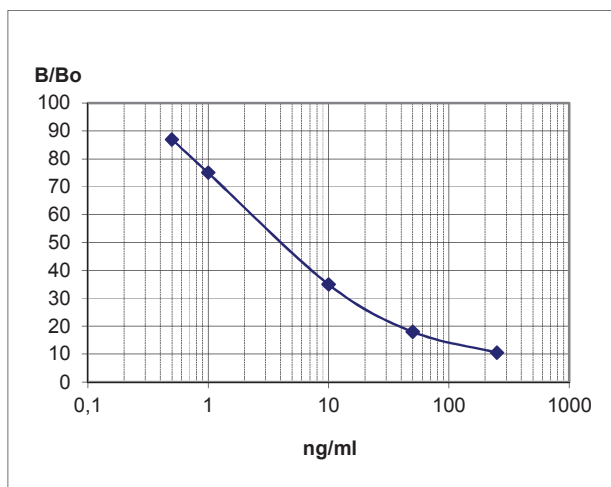

11 RESULTS EVALUATION

After results elaboration it is necessary to verify the assay performance. The verification is performed by comparison of obtained data with those given in kit specifications (see chapter 12). If the values are out from the specifications given, it is advised to control the expiry date of the kit, the wavelength of absorbance recording, as well as the procedure employed. If operation errors do not emerge, contact our technical assistance.

WARNING: substitution will be possible just in case of rendered kit. The kit must be stored in its integral version and at the temperature indicated in this booklet.

12 KIT SPECIFICATIONS

12.1 Assay specification

Mean Bo absorbance	≥ 0.7 OD _{450nm}
B/Bo 50%	2.5 – 11 ng/ml
Std duplicates mean C.V. (%)	≤ 6

12.2 Assay performance

The kit performances hereby presented have been established in a collaborative validation study. Detection Capability (CC_β) was calculated as requested by of EU Decision 657/2002. A Performance Data Sheet (PDS) with more detailed information is available upon request.

Sample	Detection capability	
	CC _β	
Muscle (METHOD I)	10 ppb of sulfamethazine	
	10 ppb of sulfaquinoxaline	
Muscle (METHOD II)	50 ppb of sulfamethazine	
Egg, milk (METHOD I)	10 ppb of sulfamethazine	
	25 ppb of sulfamethazine	
Milk (METHOD II)	1 ppm of sulfamethazine	
	25 ppb of sulfamethazine	
Honey (METHOD II)	8 ppb of sulfathiazole	
	2 ppb of sulfamerazine	
Honey (METHOD III)	5 ppb of sulfamethazine	

13 BIBLIOGRAPHY

R. Galarini, R. Buratti, B. Bertini, L. Persic. Validation of a high sensitivity ELISA kit for a broad range sulfonamides detection in food and feed. Poster presentation at RAFA. November 1st-4th, 2011. Prague, Czech Republic.
R. Galarini, F. Diana, S. Moretti, B. Puppini, G. Saluti, L. Persic. Development and validation of a new qualitative ELISA screening for multiresidue detection of sulfonamides in food and feed. Food control. 35. 2014. 300 – 310.

14 LIABILITY

Samples evaluated as positive using the kit have to be re-tested with a confirmation method.
Tecna shall not be liable for any damages to the customer caused by the improper use of the kit and for any action undertaken as a consequence of results.
Tecna shall not be liable for the unsafe use of the kit out of the current European safety regulations.