

### Certified Reference Material

This certificate is designed in accordance with ISO 17034 and ISO Guide 31. This certified reference material (CRM) was designed, produced and verified in accordance with ISO/IEC 17025, ISO 17034 and a registered quality management system ISO 9001.

**Product Name**  
Nitroxynil

**Product Code**  
DRE-C15617000

**CAS No.**  
1689-89-0

**Mol. Weight**  
290.01


**Mol. Formula**  
C<sub>7</sub>H<sub>3</sub>IN<sub>2</sub>O<sub>3</sub>

**Lot Number**  
H1596226

**Format**  
Neat

**Expiry Date**  
30 Oct 2031

**Storage Temp**  
20°C ± 4°C




<p><b>CERTIFIED</b></p> <p>Purity 99.20% (g/g)</p>	<p><b>CERTIFIED</b></p> <p>Expanded Uncertainty (U) 0.50% (g/g)</p>
--	---


**Uncertainty**

The certified value(s) and uncertainty(ies) are determined in accordance with ISO 17034 with an 95% confidence level (k=2). Uncertainty is based on the Total Combined Uncertainty, including uncertainties of characterisation, homogeneity and stability testing. Stability values are based on real evidence opposed to simulation.

The producer certifies that this certified reference material meets the specification stated in this certificate until the expiry date, provided it is stored unopened at the recommended temperature herein. Product warranties for this certified reference material are set out in the terms and conditions of purchase.

CERTIFIED BY	CERTIFIED ON		
F. Maunz	30 Oct 2025		RM Release

CHROMATOGRAM

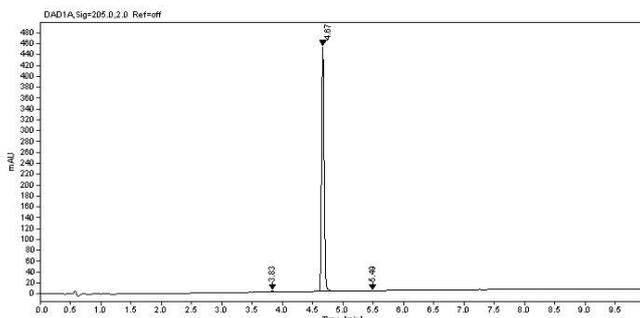

Nr.	RT [min]	Area	Height	Area%
1	3.83	8.28282	2.76	0.62
2	4.67	1324.16389	450.15	99.32
3	5.49	0.73677	0.27	0.06

**Instrument**  
UHPLC/DAD

**Detection**  
DAD

**Column**  
LUNA Omega C18 1.6 µm 100 x 2.1 mm

**Method Details**  
see Batch Information

**Inj.-Vol.**  
2.0 µL

**Flow**  
0.5 mL/min

**Method of Characterisation**

Purity = 100% - Assay impurities – Residual Solvents (NMR)

**Method of Identification**

EA, NMR, RT, IR, MS, UV

**Batch Information**

Water content below LOQ (< 0.08%).

**Method Details:**

Eluent A: 100% Acetonitrile

Eluent B: 100% Water + H3PO4

Time [min]	Eluent A [%]	Eluent B [%]
0	10	90
0.3	10	90
8	98	2
9.5	98	2

**Intended Use**

This CRM is intended for use in a laboratory as a calibration and quality control standard or in method development for analytical techniques.

**Safety**

Proper precautions should be observed while handling. See Safety Data Sheet.

**Homogeneity**

Random replicate samples of the final packaged CRM have been analysed to prove homogeneity compliant with ISO 17034.

**Traceability**

The balances used for gravimetric measurements are calibrated with weights traceable to the national standards (DKD). The calibration of the balances is verified daily internally and annually by an external accredited calibration service. Characterisation methods accredited to ISO 17025 are traceable through an unbroken chain of comparisons with national and international standards to the International System of Units (SI).

**Storage**

The CRM should be stored in the original sealed container at the indicated temperature.

**Instructions for use**

It is recommended to use 1 mg as the minimum sample size and if less material is used, to increase the certified uncertainty by a factor of two for half sample and four for a quarter of sample. If storage after opening is necessary, the CRM should be tightly closed and kept from light and moisture. If the CRM was in a sealed ampoule, it should be transferred to a vial with minimum head space. Visit the support section of our website [lgcstandards.com](http://lgcstandards.com) for a series of Dr. Ehrenstorfer Tech Tip videos and frequently asked questions.

LGC Labor GmbH  
Bgm.-Schlosser-Straße 6A  
86199 Augsburg, Germany  
T | +49 821 906080  
F | +49 821 9060888  
E | [dr.ehrenstorfer@lgcgroup.com](mailto:dr.ehrenstorfer@lgcgroup.com)

LGC Labor GmbH is accredited by DAkkS as reference material producer on ISO 17034 (D-RM-19883-01-00).

All characterisation measurements at LGC Labor GmbH are accredited methods to ISO/IEC 17025.

