



KONFORMITÄTSERKLÄRUNG DECLARATION OF CONFORMITY

Doc#200/08-2022

Hersteller / Manufacturer: **TECO Medical Instruments
Production + Trading GmbH**
 Adresse / Address: **Dieselstrasse 1, 84088 Neufahrn, Germany**
 Marktakteur / Actor ID SRN: **DE-MF-000022642 <https://ec.europa.eu>**

Wir erklären hier für die im Anhang A (Seite 2 – 23 IVD Produkte) spezifizierten Produkte dass sie gemäß der Richtlinie für In-vitro-Diagnostika Medizinprodukte 98/79/EC klassifiziert sind als allgemeine IVD.

Diese Konformitätserklärung wird unter der alleinigen Verantwortung des Herstellers i.V.m. Artikel 110 Abs.3 und Abs.4 der Verordnung (EU) 2017/746 und des § 8 Abs.1 des Medizinprodukte-Durchführungsgesetzes, in der jeweils geltenden Fassung, ausgestellt.

Im Falle eigenmächtiger Veränderungen am Produkt oder der nicht bestimmungsgemäßen Verwendung verliert diese Erklärung ihre Gültigkeit.

We declare herewith for the products specified in Annex A (page 2 - 23 IVD products) that they are classified as general IVD according to the In Vitro Diagnostic Medical Devices Directive 98/79/EC.

This declaration of conformity is issued under the sole responsibility of the manufacturer in according to article 110 para.3 and para.4 of Regulation (EU) 217/746 and section 8 para.1 of the Medical Device Law Implementing Act.

In case of unauthorised modifications to the products or un-intended use, this declaration loses its validity.

Sie entsprechen den anwendbaren Anforderungen der Richtlinie:	They meet applicable requirements of:
Richtlinie 98/79/EG über In-vitro-Diagnostika klassifiziert gemäß Artikel 9 als "alle anderen Produkte"	Directive 98/79/EC on in-vitro-diagnostic medical devices classified according to article 9 as „all other products“
Die Qualitätssicherung entspricht den Anforderungen der Richtlinie 98/79/EG über In-vitro-Diagnostika für diese Art von Produkten.	The Quality Assurance is in accordance with the requirements of Directive 98/79/EC on in-vitro-diagnostic medical devices for those kind of products.
Der implementierte QM-Prozess entspricht der EN ISO 13485:2021	The implemented QM Process complies with EN ISO 13485:2021
Die vorstehende Konformitätserklärung ist gültig für alle Chargen dieser Produkte, die nach dem Datum der Unterzeichnung in Verkehr gebracht wurden.	The above mentioned declaration of conformity is valid for all lots of this product, which are distributed after the date of signature.
Das Konformitätsbewertungsverfahren entspricht Anhang III der Richtlinie 98/79/EG über In-vitro-Diagnostika für diese Art von Produkten.	The conformity assessment procedure complies with Annex III of Directive 98/79/EC on in-vitro-diagnostic medical devices for those kind of products.

Ort und Datum der Unterzeichnung: **Neufahrn, 2022-08-31**
Place and date of issue:



Christian Hötzl
Verantwortliche Person / PRRC

Doc#200/08-2022

KONFORMITÄTSERKLÄRUNG – DECLARATION OF CONFORMITY

Directive 98/79/EC Annex A

Übrige Produkte – Reagenzien für In-vitro-Diagnostika

Other products – Reagents for in vitro diagnostic – general IVD

Pos.	Article No	Tradename	Unit	Generic Device Term	EMDN / GMDN Code EUDAMED DI
1	A0230-040	TEClot PT-S (Quick)	10x4ml PT-S	Prothrombin time (quick test)	W0103020101 / 30539 B-PTS-A0230-040X7
2	A0230-100	TEClot PT-S (Quick)	10x10ml PT-S	Prothrombin time (quick test)	W0103020101 / 30539 B-PTS-A0230-100WY
3	A0260-050	TEClot PT-B (Owren)	5x10ml PT-B	Prothrombin time (quick test)	W0103020199 / 55986 B-PTB-A0260-050G2
4	A0320-050	TEClot APTT-S	10x5ml APTT-S	Activated partial thromboplastin time	W0103020102 / 55982 B-APTT-A0320-050AM
5	A0401-020	TEClot TT	10x2ml TT	Thrombin time / reptilase / batroxbin time	W0103020103 / 55988 B-TT-A0401-0207P
6	A0511-020	TEClot FIB	10x2ml FIB	Fibrinogen assays (factor i)	W0103020201 / 55997 B-FIB-A0511-020N2
7	A0511-050	TEClot FIB	10x5ml FIB	Fibrinogen assays (factor i)	W0103020201 / 55997 B-FIB-A0511-050NB
8	C1010-020	TEChrom AT	6x6ml reagent FXa 3x3 ml substrate	Antithrombin	W0103020602 / 56156 B-AT-C1010-020HL
9	D2010-012	Red D-Dimer	3x4ml latex 3x7ml reaction buffer	D-Dimer	W0103020503 / 47349 B-DD-D2010-0126W
10	D2020-005	Blue D-Dimer LC	1x5ml latex LC 1x7ml reaction buffer	D-Dimer	W0103020503 / 47349 B-DD-D2020-0057E
11	P8001-010	TECal N	10x1ml	Calibration plasma for haemostasis	W0103020701 / 45786 B-CAL-P8001-005X8
12	P8200-005	TECal DD	5x1ml	Calibration plasma for haemostasis	W0103020701 / 47348 B-CAL-P8200-005XX
13	P6001-010	TEControl N	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6001-010H7
14	P6101-010	TEControl A	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6101-010HQ
15	P6201-010	TEControl A Plus	10x1ml	Control plasma for haemostasis	W0103020702 / 30590 B-CTRL-P6201-010J9
16	P5001-010	TEClot Factor II	10x1ml	Coagulation factor ii (prothrombin)	W0103020202 / 30542 B-FAC-II-P5001-010ML
17	P5101-010	TEClot Factor V	10x1ml	Coagulation factor v	W0103020204 / 30544 B-FAC-V-P5101-010AN
18	P5201-010	TEClot Factor VII	10x1ml	Coagulation factor vii	W0103020205 / 30545 B-FAC-VII-P5201-0107B
19	P5301-010	TEClot Factor VIII	10x1ml	Coagulation factor viii	W0103020207 / 30547 B-FAC-VIII-P5301-01097
20	P5401-010	TEClot Factor IX	10x1ml	Coagulation factor ix	W0103020208 / 30548 B-FAC-IX-P5401-0106C
21	P5501-010	TEClot Factor X	10x1ml	Coagulation factor x	W0103020209 / 30549 B-FAC-X-P5501-010EQ
22	P5601-010	TEClot Factor XI	10x1ml	Coagulation factor xi	W0103020210 / 30551 B-FAC-XI-P5601-010A8
23	P5701-010	TEClot Factor XII	10x1ml	Coagulation factor xii	W0103020211 / 30552 B-FAC-XII-P5701-010CJ

(Recital 23 of Directive 98/79/EC on In Vitro Diagnostics Medical Devices) - Annex A - general IVD



KONFORMITÄTSERKLÄRUNG

DECLARATION OF CONFORMITY

Doc#007/11-2021

Wir / We **TECO Medical Instruments Production and Trading GmbH**

Name des Herstellers / Manufacturer's *name*
Dieselstrasse 1, 84088 Neufahrn, Germany
Anschrift / *Address*

erklären in alleiniger Verantwortung, dass die Produkte – IVD-Blutgerinnungsmessgeräte,
declare under our own responsibility, that the products – IVD Coagulation analyzers

Coatron A4

Bezeichnung, Typ oder Modellname / *name, type or model*

Alle anwendbaren Anforderungen der folgenden Richtlinien entsprechen:

1. Richtlinie 98/79/EG über In-vitro Diagnostika klassifiziert gemäß Artikel 9 –"alle anderen Produkte"
2. Richtlinie 2014/30/EU über Elektromagnetische Verträglichkeit
3. Richtlinie 2011/65/EU RoHS III

Weitere angewandte Normen:

4. Sicherheit: EN 61010-2-101:2002
5. Risikomanagement: DIN EN ISO 14971:2019
6. Informationen: EN ISO 18113-3:2011
7. Medizingeräte-Software
- Lebenszyklus-Prozesse: DIN EN 62304:2016

Standards and regulations applied:

1. Directive 98/79/EC on In-vitro diagnostic medical devices classified according to article 9 as: "all other products"
2. Directive 2014/30/EU on electromagnetic Compatibility
3. Directive 2011/65/EU RoHS III

Further related standards:

4. Safety: EN 61010-2-101:2002
5. Riskmanagement: DIN EN ISO 14971:2019
6. Information: EN ISO 18113-3:2011
7. Medical device software
- life-cycle processes: DIN EN 62304:2016

Das QM-System des Herstellers ist zertifiziert nach:

EN ISO 13485:2016

The QM-system of the manufacturer is certified for:

EN ISO 13485:2016

Konformitätsbewertungsverfahren:

Gemäß Anhang III der Richtlinie 98/79/EG

Conformity assessment procedure:

According to Annex III of Directive 98/79/EC

Ort und Datum der Unterzeichnung:
Place and date of issue:

Neufahrn, 11.11.2021
Neufahrn, November 11, 2021

Matthias Dieckmann
General Manager





KONFORMITÄTSERKLÄRUNG

DECLARATION OF CONFORMITY

Doc#100/07-2021

Wir / We

TECO Medical Instruments Production and Trading GmbH

Name des Herstellers / Manufacturer's name
Dieselstrasse 1, 84088 Neufahrn, Germany
Anschrift / Address

erklären in alleiniger Verantwortung, dass die unten gelisteten IVD Zubehör Produkte:
declare under our own responsibility, that the IVD accessories products, listed below:

Doppelküvette / <i>Double cuvette</i>	Ref. 19 000 02
Einzelküvette / <i>Single cuvette</i>	Ref. 20 000 02, 24 100 00
4-fach Küvette / <i>Cuvette 4 pos/ea</i>	Ref. 80 521 10
6-fach Küvette / <i>Cuvette 6 pos/ea</i>	Ref. 80 560 00
6-fach Küvette (micro) / <i>Cuvette 6 pos/ea (micro)</i>	Ref. 80 570 00

allen anwendbaren Anforderungen folgender Richtlinien entsprechen: *meet all applicable requirements of:*

1. Richtlinie 98/79/EG über In-vitro Diagnostika und ihrem Zubehör, klassifiziert gemäß Artikel 9 als: "alle anderen Produkte"- im Sinne von Zubehör zu In vitro Diagnostika gemäß Artikel 1.

1. Directive 98/79/EC on In-vitro diagnostic medical devices and their accessories, classified according to article 9 as: "all other products" – and in term of accessories for in vitro diagnostics according to article 1.

2. Richtlinie 2011/65/EU (RoHS III)

2. Directive 2011/65/EU (RoHS III)

Das QM-System des Herstellers ist zertifiziert nach:

The QM-system of the manufacturer is certified for:

EN ISO 13485:2016

EN ISO 13485:2016

Konformitätsbewertungsverfahren gemäß:

Conformity assessment procedure according to:

Gemäß Anhang III der Richtlinie 98/79/EG

According to Annex III of Directive 98/79/EC

Ort und Datum der Unterzeichnung:
Place and date of issue:

Neufahrn, 27.07.2021
Neufahrn, July 27, 2021

Matthias Dieckmann
General Manager



TO WHOM IT MAY CONCERN

To any governmental departments,
registration and/or trade offices in MOLDOVA

Distribution Authorisation Letter

This letter confirms that **Sanmedico**
Mun. Chisinau
Str. Petricani 88/1 of. 10
Republica MOLDOVA

is the **legal, exclusive and sole** representative of **TECO Medical Instruments Production + Trading GmbH, Dieselstr. 1, 84088 Neufahrn NB, Germany**, for the territory of **MOLDOVA** only for all TECO products listed below. **Sanmedico** may participate in public and private tenders, providing sales to all TECO customers in the territory. We as manufacturer certify that our warranty is duly passed to the purchaser through **Sanmedico** for the price, delivery schedules and the specifications of the published literature, catalogues and fully covering the commodities offered.

Sanmedico will provide the following information to TECO GmbH when so required in relation to its market surveillance activities:

Reporting of incidents to TECO must take place within 3 working days
Serial number of the device, exact location of the device and the user.

Validity: January 1st, 2023 to December 31st, 2024


Termination: Confirmation ends automatically on Dec. 31st of 2024
and must be then renewed.

Products:

- Coatron M1 Semi-automated 1-channel Coagulometer (out of production)
 - Coatron M2 Semi-automated 2-channel Coagulometer (out of production)
 - Coatron X Eco Semi-automated 1-channel Coagulometer
 - Coatron X Pro Semi-automated 2-channel Coagulometer
 - Coatron X Top Semi-automated 4-channel Coagulometer
 - Coatron A4 Fully automated Coagulometer, 4 optic channels
 - Coatron A6 Fully automated Coagulometer, 6 optic channels
 - Coatron A6 plus Fully automated Coagulometer, 6 optic channels
 - Hemostasis Reagents Complete product line
- all instruments with complete accessory, consumables and spare parts

This document is signed in Neufahrn, Germany, on January 18th, 2023

TECO Medical Instruments Production+Trading GmbH


Christian Hoetzl






Quality Management

We are certified

Voluntary participation in regular monitoring according to ISO 9001:2008

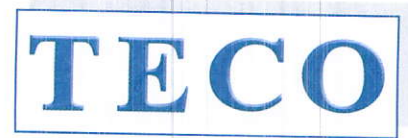

MEDICAL INSTRUMENTS
PRODUCTION+TRADING GMBH

Dieselstraße 1

D-84088 Neufahrn N.B.

fon: +49-8773/707 80-0

fax: +49-8773/707 80-29

CERTIFICATE

for: **Mr. Vitalie Goreacii**

Company: **Sanmedico SRL**
Str. Petricani 88/1, oficiul 10
Chisinau - Rep. Moldava MD-2059
MOLDOVA

have participated with success at the intensive training session:

Application and technical training for following instruments:

- **Coatron X series**
 - **Installation**
 - **Application**
 - **General use, also in combination with TECAM Software**
 - **Technical and After Sales Service**

Supervisors: **Mr. Chr. Hoetzi and Mrs. Wendy Guo**

Place of Training: **TECO – Germany**

Date: **November 18th, 2019**



Christian Hoetzi
General Manager



**Medical Instruments
Production+Trading GmbH**
web: www.teco-gmbh.com
mail: info@teco-gmbh.com

**Dieselstrasse 1
D-84088 Neufahrn/NB**
fon: +49 8773 70780 00
fax: +49 8773 70780 29

CERTIFICATE OF TRAINING

Vitalie Goreacii

General manager of
Sanmedico
Chisinau
Republic of Moldava

have participated with success at the training session supervised
by TECO GmbH, Germany for following instruments:

Coatron A series

- **Installation**
- **Application**
- **General use, also in combination with TECAM**
- **Maintenance**
- **Troubleshooting**
- **After Sales Service**

Training details:

Supervisor: Chr. Baumgartner, Director RD of TECO
Device: Coatron A4 + A6, Inhouse Master Device
Place: Laboratories of TECO
Date: May 5th 2023



Dipl.-Ing. Univ. (TUM)
Christian Baumgartner
Director R&D



Quality Management

We are certified

Voluntary participation in regular monitoring according to ISO 9001:2008



MEDICAL INSTRUMENTS
PRODUCTION+TRADING GMBH

Dieselstraße 1

D-84088 Neufahrn N.B.

fon: +49-8773/707 80-0

fax: +49-8773/707 80-29

TO WHOM IT MAY CONCERN

To any governmental departments,
registration and/or trade offices
in Moldova

Distribution / Service Authorisation for the years 2019 - 2023

This letter confirms that company

SANMEDICO SRL

Str. Petricani 88/1, oficiul 10

Chisinau - Rep. Moldava MD-2059

MOLDOVA

Phone: 00373-22-623032

Email: sanmedico.office@gmail.com

is the **authorized, exclusive and sole** representative of **TECO Medical Instruments, Production + Trading GmbH, Dieselstrasse 1, 84088 Neufahrn i.NB, Germany**, for the territory of **Moldova**, only for all TECO products listed below. **Sanmedico** may participate in public and privat tenders, providing sales to all TECO customers in the territory. We as manufacturer, certify that our **warranty and service** is duly passed to the purchaser through **Sanmedico** for the price, delivery schedules, and the specifications of the published literature, catalogues and fully covering the commodities offered.

Validity:

August 20th, 2019 to December 31st, 2023

Termination:

Confirmation ends automatically on Dec. 31st of 2023
and must be then renewed.

TECO products:

- Coatron X (Eco, Pro, Top) new manual Coagulometers (1, 2 and 4 channel)
- Coatron A4, A6, A6 Plus Fully automated Coagulometers (4 and 6 channel)
- Complete line of Hemostasis Reagents, Consumables and Spareparts

This document is signed in Neufahrn, Germany, on August 20th, 2019.

TECO Medical Instruments, Production + Trading GmbH



MEDICAL INSTRUMENTS
PRODUCTION+TRADING GMBH
Dieselstraße 1
D-84088 Neufahrn N.B.
fon: +49-8773/70780-0

Christian Hoetzl
General Manager

Zertifikat

Hiermit wird bescheinigt, dass das Managementsystem von:

TECO Medical Instruments, Production + Trading GmbH

Dieselstr. 1, 84088 Neufahrn, Deutschland

durch LRQA geprüft und bewertet wurde und den folgenden Normen entspricht:

ISO 13485:2016

Gültigkeits-Nr.: ISO 13485 – 00038268

Das Managementsystem ist anwendbar für:

Konstruktion, Entwicklung, Herstellung, Lagerung und Vertrieb von Gerinnungsmessgeräten und in-vitro Diagnostik Reagenzien aus den Bereichen der Hämostaseologie und Koagulation.



Paul Graaf

Area Operations Manager, Europe

Ausgestellt von: LRQA Limited



0001

Coatron® A4

Fully automated Hemostasis Analyzer

Made in Germany
REF: 80 900 00



- ▶ Easy operation
- ▶ Multi languages
- ▶ Highly reliable
- ▶ Four channels
- ▶ Fully optical detection
- ▶ Clotting, chromogenic and immunturbidimetric methods
- ▶ Autosense optics to reduce interferences of Bilirubin and Hemoglobin
- ▶ Approved clotting algorithm with biphasic waveform analysis
- ▶ Batch and Random Access
- ▶ High throughput
- ▶ Emergency (STAT) mode
- ▶ Laser Barcode reader for samples and reagents
- ▶ Liquid Level sense
- ▶ Cap piercing
- ▶ Compact construction
- ▶ Operation as open or closed system

TECO

Innovation in Coagulation

Coatron® A4

Fully automated Hemostasis Analyzer



1 Keyboard

Numerical and function keys for easy controlling of the instrument, as well quick setup of all individual tests.

2 Grafic display

128 x 128 dot matrix
Blue backlight

3 Cuvette waste drawer

Removable waste drawer for fast removing of used cuvettes

4 Cuvette tower

For load of 45 cuvettes: enough for 180 tests, continuous loadable

5 Printer (back side)

Thermal printer for quick printout of results, system analysis, test setups etc.

6 Liquid handling

x-y-z robotic system with special Cap Piercing probe, Level sense. Autoskip function for empty reagent vials. Special clean solution and software program to avoid carry over from sample to sample, sample to reagent and reagent to reagent to.


TECAM PROLIS

For Microsoft Windows™ XP/Vista

Software for TECO Coatron® A4 Analyzer

- ▶ New features for Coatron® A4
- ▶ Intuitive and easy one click operation
- ▶ Database up to 1 Mio results
- ▶ Worklist management
- ▶ Bidirectional ASTM interface to LIMS
- ▶ Multi-lingual (Chinese+ Russian included)
- ▶ Reaction curve display
- ▶ Powerful filter and patient report engine
- ▶ QC with Levey-Jennings and Westgard rules


TECAM PROLIS is a perfect and user friendly tool to combine laboratory data management, quality control and research purpose in one. The Worklist management allows defining orders much faster and flexible then on the instrument itself. Powerful filter functions will help to create any report. Levey-Jennings graph and Westgard analysis are used for quality control monitoring. An ASTM interface is included, which allows to link over LAN network with the laboratory information system.

Coagulation Data-Report
 Thrombosis & Haemostasis Research Center
 Dieselstr.1, D-84088 Neufahrn, Germany
 tel: +49 8773 910010
 email: info@teco-medical.de

Test	Warning	Result	Range
APTT	08.05.2007 14:31:39 A	38,4s	[26-38s]
PT	08.05.2007 14:30:31 A	* 27,7s 11,6% 2,22 INR	[10-15s] [70-120%] [0,8-1,2INR]
TCT	08.05.2007 14:33:19 A	26,5s	[16-24s]


Create reports with a click. Powerful filter functions will help to select just specific results. (e.g. day report, report the last 30 days of patient xyz, report all D-Dimer results of last year which are positive)

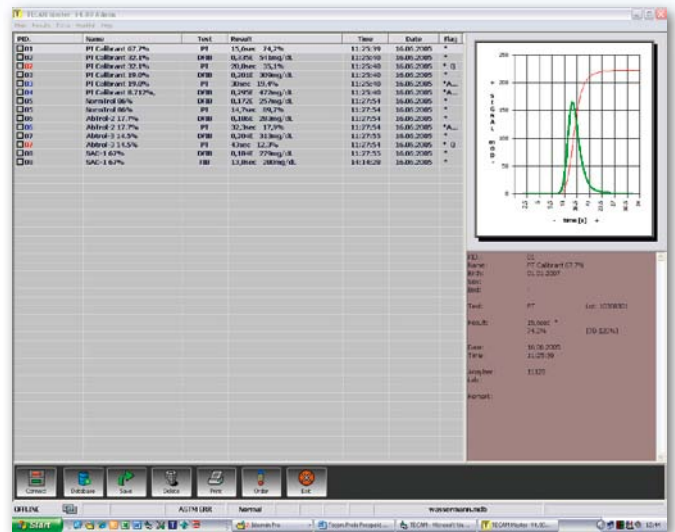

Receive results from instrument including the reaction curve which will help to validate before saving them into the database.

POS.	PID.	Name	PT	DFIB	APTT	FIB	AT	TT11	VT	DD	HEP
<input type="checkbox"/>	35	QC									
<input checked="" type="checkbox"/>	01	0002 Control-2	PT		APTT	FIB					
<input checked="" type="checkbox"/>	02	00602004 Akratou,John	PT		APTT						
<input checked="" type="checkbox"/>	03	00702004 Terzides	PT		APTT	FIB					
<input checked="" type="checkbox"/>	04	00732004 Triadafiou	PT		APTT	FIB					DD
<input checked="" type="checkbox"/>	05	00742004 Mourtzou	PT		APTT	FIB					
<input checked="" type="checkbox"/>	06	00752004 Xanthous	PT		APTT	FIB	AT				HEP
<input type="checkbox"/>	07										
<input type="checkbox"/>	08										
<input type="checkbox"/>	09										
<input type="checkbox"/>	10										
<input type="checkbox"/>	11										
<input type="checkbox"/>	12										
<input type="checkbox"/>	13										
<input type="checkbox"/>	14										
<input type="checkbox"/>	15										
<input type="checkbox"/>	16										
<input type="checkbox"/>	17										
<input type="checkbox"/>	18										
<input type="checkbox"/>	19										
<input type="checkbox"/>	20										
<input type="checkbox"/>	21										

Create or receive orders from LIMS and send them to instrument.

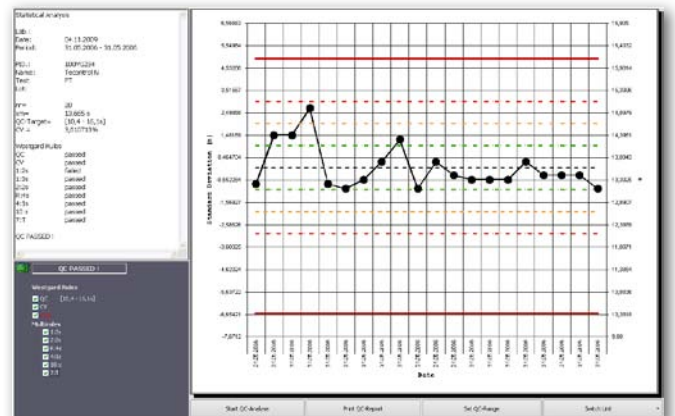

Results can be displayed in a Levey-Jennings graph and analysed with Westgard rules. This tool can be used for QC but also for powerful patient monitoring (e.g. last 30 PT of patient)

TECAM PROLIS

For Microsoft Windows™ XP/Vista

▶ Recommended system requirements:

Microsoft XP, CPU 1.5 GHZ, 1GB RAM, Graphic 1280x1024

▶ Support instruments

Coatron® A4 and OEM's

▶ Instrument Interface

Serial RS232, 115000 Baud, 8,1,N

Bidirectional for results, including reaction curve and orders.

▶ ASTM Interface

Protocol: ASTM E1381-94; E1394-97

Communication: TCP/IP (network, LAN)

Bidirectional for results, including reaction curve and orders.

▶ Intuitive handling

One click principle for data collection, filtering, reporting or QC

▶ Multi lingual

English, Spanish, Italian, Portuguese, Russian, Greek, Chinese, further languages possible.

▶ Database

Manage over 1 Mio results and patient information in one database.

▶ Data fields for:

Date, patient (Id, name, sex, birth, bed, station), test, results (s, %, INR), reaction curve, Flags, error, comment, reagent-LOT, patient-memo, analyser SN., ranges (QC + normal)

▶ Database functions:

Create, Switch, Backup, Compress, Import, Export, Replace or fill data

▶ Complete Traceability by one click

Review for Date, PID, Test, and QC by one click

▶ Reporting

Make reports by one click. Use multi-filter or presets to generate specific reports (e.g. show results of specific patient of all PT within the last 30 days)

▶ Worklist management

Create, load, save, repeat, receive and send. Positive patient identification by barcode validation. USB barcode scanner supported. Up to 3 different profiles. Max 8 tests per profile. Preset for up to 6 different QC samples.

▶ Flexible multi filter

Combine every data field:

PID=1234+ Date=today + Test=FIB + Result< 200mg/gL + Reagent LOT = 1234 + etc)

▶ Filter Presets:

Today; last 7, 15, 30, 180, 360 days; morning, afternoon; only QC etc.

▶ Statistical analyse for QC or patients

Filter any data (e.g. Patient XYZ, only PT, last 30days), and visualize them with Levey Jenning diagram with one click.

Analyse data with Westgard Multirules. Define QC or Patient ranges.

▶ Research

Curve analysis, Tecmoni transmission, Export data, grids, charts, curves to PDF, XLS, TXT or HTML file

▶ Tecmoni transmission

This tools allows to visualize all optic channels in real-time. It is perfect for enhanced curve analysis and used in many research laboratories. With Tecmoni the reaction curves can also sent back to instrument. Especially for developing new test application and instrument firmware, this will save a lot of reagent and time.

▶ Security

Operator can login as Administrator or user in order to control and manage the database with different access rights

▶ Online update



Innovation in Coagulation

Coatron® A4

Fully automated Hemostasis Analyzer

7 Pump/syringe

Maximum volume: 1000 µl
Minimum volume: 3 µL
Long life syringe
Easy to replace and maintain

8 Rinse container (back side)

Containing 1,25 Liter high quality rinse solution for flushing the probe after each pipette circle.

9 Reagent block

4 positions heated at 37°C
2 positions at room temp.
6 positions cooled
3 positions for prewarm

10 System block

5 positions heated at 37°C for Buffers, Clean solution and Flush position for the probe, inside and outside
Separate STAT position for immediate Emergency

11 Sample racks

2 racks with 12 positions each, suitable for most common primary tubes.
Every position have individual bar code for positive sample identification

12 Barcode

Laser Barcode Scanner for quick and accurate identification of all Common Barcodes

13 Liquid waste drawer

Contain container for collection liquid waste
Volume: 1,25 Liter max.

14 Trolley (Option)

For mobile usage and enlarged waste management (big box for used cuvettes and large container for liquid waste)
Lift-up plate for sample preparation (more work area)
Moveable plate for easy replacement of box and container
Additional drawer for accessories and spare parts

Special features of the Coatron® A4:

System

- ▶ Ultraviolet light (400 nm). The measurement amplification is adapted Photometric measurement principle with high-resolution 4-channel optics, automatically to the methods used. Extraneous and scattered light energy is absorbed.
- ▶ High-precision XYZ pipetting system with liquid level sensor
- ▶ Long living and flexible Cap Piercing needle for primary tubes such as BD Vacutainer® or Sarstedt Monovette®.
- ▶ Integrated ID-barcode reader
- ▶ Bi-directional Interface for PC-Link to LIS.
- ▶ Optional trolley to enlarge the waste management
- ▶ Integrated graphical thermal printer
- ▶ Heated and cooled positions for reagents
- ▶ Integrated drawers for consumables

Software

- ▶ Approved and highly accurate detection algorithm based on optical density. The clotting time is defined at the turning point of reaction.
- ▶ An intuitive TECO familiar graphical user interface with „Plug and Go“ feeling.
- ▶ Multi language dialogue. (English, German and other)
- ▶ Random access scheduler. Profiles can be performed as batch or selective.
- ▶ Positive sample identification (ID and rack position) either manual or with barcode scanner
- ▶ Fast and easy processing of STAT samples

- ▶ Free programmable test protocols to change or adapt new tests
- ▶ Calculation of activity %, INR, Ratio, g/L, mg/dL and more.
- ▶ Calibration curve can be identified with up to 6 points per test. The results can be calculated with regression line analysis or linear interpolation.
- ▶ Single or double determinations
- ▶ Simple firmware update

Special Functions

- ▶ Automatic plasma dilutions up to 1:100
- ▶ Automatic cleaning cycles
- ▶ Automatic test calibration routines
- ▶ Automatic quality control
- ▶ Automatic or manual printout
- ▶ Automatic test skip, if reagent run out.
- ▶ Quality control according to Westgard rules *
- ▶ Result traceability *
- ▶ Patient monitoring for long time periods *
- ▶ Reaction curve monitoring *

Economic

- ▶ Half volume procedures resulting in 50% cost savings.
- ▶ Reagent dead volume is below 300 µL
- ▶ Very economic consumption of rinse and cleaning solution.
- ▶ Cuvette with no mixing bars, etc.
- ▶ All critical system parameters are monitored and make the instrument nearly free of service.

Coatron® A4

Fully automated Hemostasis Analyzer



Tests on board:

PT
APTT
TT
Fibrinogen Clauss
Fibrinogen derived
Factor II
Factor V
Factor VII
Factor VIII
Factor IX
Factor X
Factor XI
Factor XII
Protein C
Protein S
LA Screen (DRVVT)
LA Confirm (DRVVT)
Activated Protein C resistance
Heparin
Antithrombin
D-Dimer

Calculated units

% , R, INR, mg/dl, µg/L

Technical specification

Dimension
85 x 60 x 70 cm

Weight
50 kg

Power input
90-240 Vac / 50-60 Hz

Ambient conditions
18°C – 30°C
20 to 80% RH.
no direct sunlight



Optional available

- ▶ Trolley (for enlarged waste management)
- ▶ Complete Cover protection
- ▶ TECAM PRO – Research, QC, and Patient management software
- ▶ TECAM PRO LIS - Research, QC and Patient management software with LIS Module

Delivery package

- 1 Coatron® A4
- 1 Power cord
- 100 Cuvettes, 4 pos/ea
- 10 Reagent container Ø 22,5
- 10 Reagent tubes Ø 13
- 10 Plasma tubes Ø 16
- 4 Magnetic stirrer
- 1 Rinse Solution, 1,25 L
- 1 Clean solution, 50 mL
- 1 Thermal paper roll
- 1 Waste container
- 1 Reagent adapter Ø 22,5
- 2 Plasma adapter Ø 16
- 1 Operation manual
- 1 CE Conformity declaration
- 1 Service CD
- 1 Download cable
- 1 Screw driver, small
- 1 Flat wrench, size 8



Innovation in Coagulation


TECO Medical Instruments,
Production + Trading GmbH

Dieselstr. 1
D-84088 Neufahrn NB.
Germany

Fon: +49-(0)87 73 - 91 00 10
Fax: +49-(0)87 73 - 91 00 11
Email: info@teco-gmbh.com
Web: www.teco-gmbh.com

Coatron A4

Operator's Manual

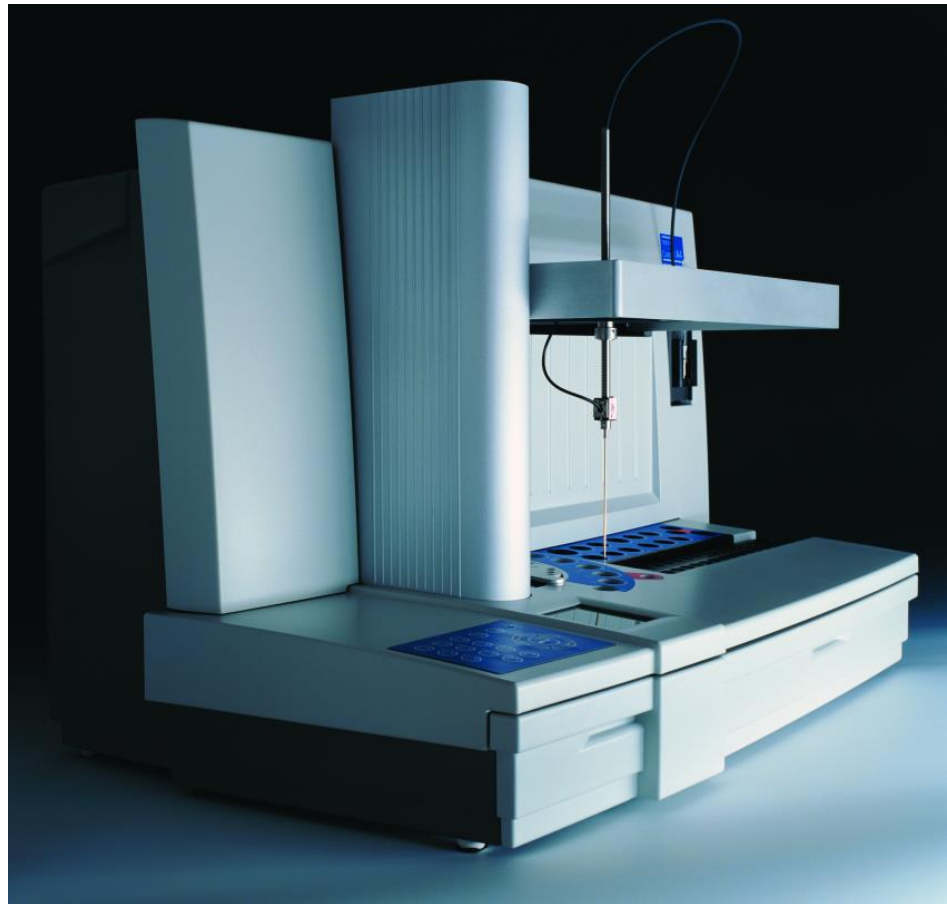

Instrumentation and Reagents for *In-Vitro* Diagnostic use

Revision 22

Issue Oct-2015

Document No:21 440 01

Updates

Operator's Manual Version	Software Version	Date
10	1.03.30	05/2006
11	1.05.00	02/2009
12	1.05.02	05/2009
14	1.06.01	10/2010
15	1.06.02	05/2011
16	1.06.04	10/2011
17	1.06.04 SW3	3/2012
18	1.06.06	2/2013
19	1.06.08SW2	12/2013
20	1.07.01SW3	6/2014
21	1.07.01SW4	12/2014
22	1.07.02	10/2015

Copyright

Copyright © 2015 by Teco GmbH. Neither the Operator's Manual nor any part thereof may be copied, digitally processed or otherwise transferred without written permission from Teco GmbH.

The software for Teco GmbH products is the intellectual property of Teco GmbH, which company retains all rights to usage of the software. The purchaser of a COATRON A4 acquires rights of use for this software

Trademarks

COATRON A4 is a trademark of Teco GmbH. Other product names used in this Operator's Manual are trademarks of the respective companies.

Manufacturer

Instrument is produced by

TECO GmbH
 Dieselstrasse. 1
 D-84088 Neufahrn
 Germany

Phone: +49 (0)8773 70780-0
 Fax: +49 (0)8773 70780-29
 Internet: <http://www.teco-gmbh.com>

1.	Introduction.....	7
1.1	Symbols.....	7
1.2	Safety information.....	8
1.2.1	Intended use.....	8
1.2.2	Safety information for operation.....	8
1.2.3	Safety information for MATERIALS.....	9
1.2.4	Safety information regarding risk of health.....	9
1.2.5	Safety information for cleaning, maintenance and servicing.....	10
1.2.6	Electrical safety.....	11
2.	Installation of the COATRON A4.....	12
2.1	Scope of delivery.....	12
2.2	Laboratory Requirement.....	13
2.3	Unpacking the COATRON A4.....	13
2.4	Removal of the transport retainer elements.....	13
2.5	Switching ON and off the COATRON A4.....	14
2.6	Installation of Components.....	16
2.7	Installation of TECAM software.....	17
3.	Description of the COATRON A4.....	18
3.1	Short introduction.....	18
3.2	Views of the device.....	20
3.2.1	Front view.....	20
3.2.2	Rear view.....	21
3.2.3	Side view.....	22
3.2.4	Sample rack.....	22
3.2.5	Working Positions.....	23
3.2.6	Keypad.....	24
3.2.7	Screen segments.....	24
3.3	Measurement principle.....	25
3.3.1	Mathematical principles.....	25
3.3.2	Units.....	25
3.3.3	Clotting method.....	26
3.3.4	Derived fibrinogen.....	26
3.3.5	Chromogenic, endpoint and immunoturbidimetric method.....	27
3.4	Test overview.....	28
4.	Routine measurement (Typical use case).....	29
4.1	Preparation.....	29
4.2	New list input.....	30

4.3	Interrupt or exit measurement	32
4.4	Out of liquid or cuvette during measurement	32
4.5	Continuous loading of samples	33
4.6	Measuring the emergency samples	34
4.7	Quality control measurement	35
5.	Software description	36
5.1	Main menu Analysis	37
5.1.1	Submenu New List	37
5.1.2	Submenu Continue	43
5.1.3	Submenu Repeat	43
5.1.4	Submenu Stat	43
5.1.5	Submenu Overview	44
5.1.6	Submenu Print Option	46
5.1.7	Submenu System Activation	46
5.1.8	Submenu Cuvette Activation	47
5.1.9	Submenu Reagent Activation	47
5.1.10	Reflex testing	48
5.1.11	Display during measurement	49
5.1.12	Result warning messages	49
5.1.13	Printout of results	50
5.1.14	Host communication	50
5.2	Main menu Test Setup	51
5.2.1	Using of reagent barcode	51
5.2.2	Test Selection	51
5.2.3	Submenu "Set Data"	52
5.2.4	Test Calibration	53
5.2.5	Submenu Normal Range	56
5.2.6	Submenu QC Range	56
5.2.7	Storing of test data	57
5.2.8	Submenu Test Printout	57
5.2.9	Submenu Test Overview	58
5.2.10	Setup of test protocol	58
5.3	Main menu System Setup	61
5.3.1	Language	61
5.3.2	Date	61
5.3.3	Time	61
5.3.4	Signal	61
5.3.5	Contrast	61
5.3.6	Mixer	62
5.3.7	Simulator	62
5.4	Main Menu SERVICE	63
5.4.1	System report	64

5.4.2	Adjust XYZ.....	65
5.4.3	Check Temperature	66
5.4.4	Check Optics	67
5.4.5	Check Robot.....	68
5.4.6	Move Cuvettes.....	68
5.4.7	Clean Needle.....	68
5.4.8	Replace Rinse tank.....	68
5.4.9	Replace Needle	69
5.4.10	Replace Syringe.....	70
5.4.11	Adjust Motor.....	70
5.4.12	Cap Piercing	71
5.5	Main menu PIPET STATION	72
6.	Replacement of consumables	73
6.1	Disposal.....	73
6.2	Refill cuvettes	73
6.3	Replace Rinse tank.....	73
6.4	Replenishing the printer paper	74
7.	Cleaning and maintenance	75
7.1	General cleaning information.....	75
7.2	Cleaning	75
7.3	Decontamination	75
7.4	Daily activities.....	75
7.5	Weekly activities.....	76
7.6	Yearly activities.....	76
7.7	Regular Replacements.....	76
7.8	Reset Service Interval	76
7.9	Error messages	77
8.	Elimination of malfunctions	78
8.1	Device malfunctions	78
8.2	Measurement malfunctions	79
8.3	Packing the COATRON A4 for shipment	80
9.	Appendix.....	81
9.1	Interface to LIS.....	81
9.1.1	Bidirectional communication with TECAM software	81
9.1.2	Unidirectional communication	82
9.2	Technical data.....	83

9.3	Declaration of Conformity	86
9.4	Disposal and recycling	87
9.5	Barcode Guideline	88
	Index	89







Figure 1: COATRON A4, front view	20
Figure 2: COATRON A4, rear view	21
Figure 3: Side view	22
Figure 4: Sample rack	22
Figure 5: Working Positions	23
Figure 6: Keypad	24
Figure 7: Screen segments	24
Figure 8: Determination of turning point in clotting method	26
Figure 9: Determination of rise in the kinetic test method	27
Figure 10: Replace Needle	69
Figure 11: Installation of syringe	70
Figure 10: Refill cuvettes	73
Figure 13: Printer cover	74
Figure 14: Replenishing the printer paper	74

1. Introduction

This device left the factory in fault-free condition regarding its safety and engineering functionality. To maintain this condition and ensure risk-free operation, the operator must comply with the safety warnings and information in this Operator's Manual.

1.1 Symbols

The following standard symbols are used in this manual:

Symbol	Meaning	Explanation
Courier	Info	Key on keypad.
CAPS	Info	Screen message.
	Read	Indicates important information and tips.
	Info	Describes reaction of COATRON A4 to operator input.
	Warning	Risk of possible health damage or considerable damage to equipment if warning is not heeded.
	Danger	Potential risk to operating personnel or equipment due to electric shock.
	Biohazard	Equipment can be potentially infectious due to the samples and reagents used .
	Laser Radiation	Avoid direct eye exposure

1.2 Safety information

1.2.1 Intended use

IVD

The **COATRON A4** is designed to carry out coagulometric tests such as PT, PTT, TT, fibrinogen, single factor tests, chromogenic and immunoturbidimetric tests (for instance Antithrombin, D-dimer etc.). The instrument has to be used for the expected purposes and in perfect technical conditions, by qualified personnel, in working conditions and maintenance operations as described in this manual, according to the SAFETY WARNINGS. This manual contains instructions for professional qualified operators.



Do not use plasma with more than 25mg/dL Bilirubin (428µmol/l)
Do not use plasma with more than 1000mg/L Hemoglobin
Do not use plasma with more than 25 g/l Triglyceride (28.5 mmol/l)



Use only citrated plasma for sample analysis. Mix 9 parts of venous blood with 1 part 3.2% (0.105M) sodium citrate and centrifuge the mixture at 1500g x 15min. Use plasma within 4 hours.

1.2.2 Safety information for operation



Use only the cleaning and rinsing liquids approved by the manufacturer. Failure to do so could result in faulty measurements or malfunctions of the COATRON A4. Prevent reagents from leaking into the Analyzer. Failure to do so may make expensive maintenance work necessary!



Never touch moving parts such as the measurement rotor or pipetting arm during device operation. Never try to pull a cuvette block out of the measurement rotor during test processing operation. Carry out control measurement runs at regular intervals to ensure that the Analyzer continues to function faultlessly.



If instrument is used in a manner not specified by the manufacturer, the protection impairment could be affected!

1.2.3 Safety information for MATERIALS

**Important!**

Use only organic solvents where specified. The cuvettes are intended as single-use items only. Repeated use may result in false results due to contamination. Follow the instructions in the reagent package circulars. Incorrect handling may result in falsified results.

1.2.4 Safety information regarding risk of health

**Infectious Material**

Avoid direct contact with samples and sample residues in the used cuvettes.

Infectious material such as cuvette waste and liquid waste must be disposed in compliance with local regulations governing for infectious materials.

Wear medical infection grade protective gloves for all cleaning and maintenance works involving potential contact with infectious liquids and use each pair of gloves once only. Use a hand disinfectant product, e.g. Sterilium[®], to disinfect your hands after completion of the work.

NOTICE

Analytical instruments for in vitro diagnostic application involve the handling of human samples and controls which should be considered at least potentially infectious. Therefore every part and accessory of the respective

instrument which may have come into contact with such samples must equally be considered as potentially infectious. The

„BIOHAZARD“ warning label must be affixed to instrument prior to first use with biological material!

**Laser Radiation**

The internal barcode scanner is assigned to laserclass 2 – EN60825-1:2007.

Avoid direct eye exposure

max. power = 1.7 mW pulse period = 420 µs wavelength = 655 nm

1.2.5 Safety information for cleaning, maintenance and servicing

**About authorized service !**

Carry out only the maintenance, repair and replacement measures listed in this Operator's Manual. Improper manipulation of the device will void the manufacturer's liability obligations and may make service calls necessary, payment of which is not covered by warranty. Only the authorized Customer Service may carry out servicing. Only original replacement parts may be used. Before doing any servicing on the instrument it is very important to thoroughly disinfect all possibly contaminated parts

**About cleaning and decontamination !**

Before the instrument is removed from the laboratory for disposal or servicing, it must be decontaminated. The procedure is described in chapter "7 Cleaning and maintenance" and should be performed by authorised well-trained personnel only, observing all necessary safety precautions

**Cleaning certificate required !**

Instruments to be returned have to be accompanied by a decontamination certificate completed by the responsible laboratory manager. If a decontamination certificate is not supplied, the returning laboratory will be responsible for charges resulting from non-acceptance of the instrument by the servicing centre, or from authority's interventions.






Regard all surfaces and materials which might be in contact with plasma or other biological liquid as potentially contaminated with infectious material.



Avoid any direct contact with decontaminants or disinfections.

1.2.6 Electrical safety

	<p>Precautions:</p> <ul style="list-style-type: none"> ▪ Avoid spilled liquids into system. But in case disconnect system from power and clean and dry all contaminated parts. ▪ Remove power cord before open the instrument ▪ Do not touch any electronic parts during operation. ▪ Do not operate system without proper connection to grounding ▪ Never intentionally interrupt protective ground contacts. ▪ Never remove housing elements, protective covers or secured structural elements, since so doing could expose parts carrying electric current. ▪ Make sure surfaces such as the floor and workbench are not moist while work is being done on the device. ▪ Check electrical equipment regularly. Defective leads or socket must be replaced without delay.
	<p>Connect to power:</p> <p>Instrument is classified to Class-1 (IEC) and must therefore be reliably earthed and professionally installed in accordance with the prevailing electrical wiring regulations and the safety standards covered herein.</p> <ul style="list-style-type: none"> ▪ Use only three wire power cord. ▪ Make sure the operating voltage setting is correct before connecting the device to the power mains. ▪ Ensure at least 20cm space to power socket and instrument power ON/OFF switch for easy and quick access to power cord during operation.
	<p>Disconnect from power:</p> <ul style="list-style-type: none"> ▪ Unplug power cord from wall socket/UPS or from instrument power-in

2. Installation of the COATRON A4



Initial startup of the COATRON A4 is carried out by the authorized Customer Service of the dealer. A protocol is kept of the first installation which is then sent in to the manufacturer as a basis for processing guarantee claims.

Procedures of first installation:

- Unbox and place instrument in conformity with the laboratory requirements (see below)
- Remove transport retainer
- Switch on
- Install Rinse tank + Rinse waste container
- Install print paper
- Install cuvette + cuvette waste drawer

2.1 Scope of delivery

The scope of delivery can be different from customer to customer and must be read in the document "List of accessories", which is separately included to the operation manual on the first page.

2.2 Laboratory Requirement

- Power Input: 85 – 264VAC; 45-60Hz ; Class-1 socket (connected to earth)
- Ambient temperature must be 15-30°C
- Rel. humidity < 70%
- Altitude 0 - 3000m
- A stable, flat surface free of vibrations. Recommended workspace 80x150cm. On rearside a minimum space of 20cm is required.
- No direct sunlight
- Avoid ionizing air conditioner or circulating air
- Surroundings free of moisture and dust

2.3 Unpacking the COATRON A4

Following receipt of the shipment, please inspect the packaging of the COATRON A4 for any visible external damage. If the packaging is damaged, contact the transport company so that any damage to the device or accessories can be assessed. Inspect the COATRON A4 and accessories for any damage. Report any damage found to the dealer without delay. Even if the packaging appears undamaged, check the analyzer and accessories for any transport damage, caused for example by impact, dropping, etc. during transport.



Keep the original packaging material for purposes of later transport


2.4 Removal of the transport retainer elements

1. Remove the tape strips on the printer shaft.
2. Remove the 3 cable binders on the pipetting arm.
3. Remove the foam element between the pipetting arm and protective bar

2.5 Switching ON and off the COATRON A4

Switching the COATRON A4 on

1. Make sure the COATRON A4 is connected to the power mains.
2. Check for sufficient rinsing and cleaning fluid levels.
3. Set main switch to on. See rear side, location #18
4. Set standby switch to on. See right side, location #22

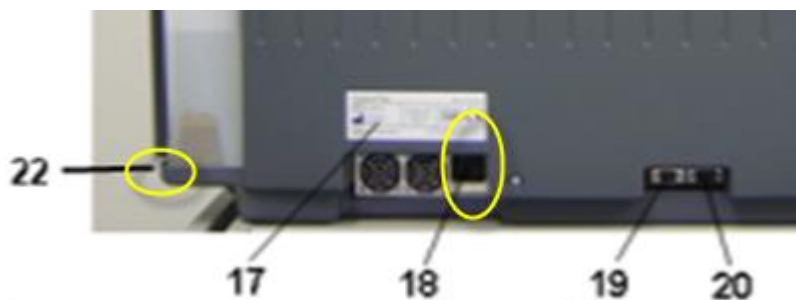

Location of power and standby switch Main screen


The following screen appear in this order after the COATRON A4 is switched on.

Coatron A4	Name of instrument
V6.07.02	Version of firmware
SN-12345	Serialnumber
Service: 100000	Tests until next service
CUVETTES:1	Activated cuvettes
RINSE: 0	Activated rinse tank
REAGENT: CLOSE	Reagent system is closed



There is no information about cuvette or Rinse or reagent , if system is configured as "OPEN DEVICE". Please contact local distributor for more information about open or closed system.

At the end of the initialization phase, the main screen appears:

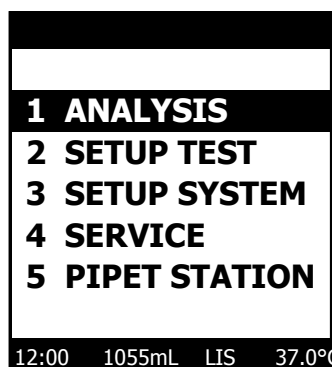

Main screen

Time= 12:00
Rinse installed = 1055mL
LIS = online
Temperature at cuvette= 37°C

After about 15 min. of warm-up time (depending on the ambient temperature), the lighting up of the LED (Temp.) on the keypad indicates the system is ready to make measurements.

Switching the COATRON A4 off:


For normal shutdown at the end of the day and for changing the pipetting needle, rinsing solution tank and syringe, switch off the COATRON A4 with the standby switch on the right side of the housing. This will shut off all power-consuming components of the COATRON A4 except the ventilator. For longer interruptions in operation such as weekends, holiday periods and service activities such as cleaning and maintenance, switch off the mains power switch as well.



Switching off the device deletes all measurement data. Backup the data as required by means of manual printout or manual transmission to the host

Never switch off the system while processing a worklist to avoid clogging the needle tip with coagulation residues.


2.6 Installation of Components




1. Remove a strip of cuvettes from the package.
2. Shift the cuvettes as shown from above in the guide groove back into the cuvette tower.
3. Remove the tape off the cuvettes.



4. Place a new Rinse tank as shown
5. Insert the tube completely
6. Fill a reagent container (15 ml) with cleaning solution and place it into position CLEAN



7. Open the print cover
8. Feed paper. Device has autofeed function.
9. Set printer to online by shift on arresting lever in the direction of the front of the housing.



10. Plug download cable into left port (19)
11. Plug in power cord (18)
12. Connect download cable with PC computer
13. Move power switch to ON. (right of 18)
14. Move standby switch to ON (22).
15. After Bootup start TECAM software

2.7 Installation of TECAM software

TECAM software is a powerful enhancement of the Coatron A4 and allows very easy and flexible to generate orders (including sample continuous loading). Results can be reported including the reaction curve and administrate in a database. For further information read the online manual of TECAM software

System requirement


- Operating system: Microsoft Windows XP or 7 32Bit
- 100 MB free hard-disk space
- Grafik: 1280x1024 Pixel
- Interface: RS232 Sub-D9 (if not supported, use USB convertor, comport must be set between com1 - com15)
- Cable: 2x Female Sub D9, crosslink. Pin 2 to 3; Pin 3 to 2 and Pin 5 to 5. All other wires should be disconnected.

Install:

1. Link instrument left RS232 port to
2. Check PC comport number (it must be between 1 to 15)
3. Start "SETUP.EXE" from the CD. The Setup will install Smart ,PRO or PROLIS and all required driver for database access.
4. Enter fingerprint and activation code

Run TECAM:

1. Switch on and bootup instrument
2. Start TECAM and enter administrator password (default = blank) or enter "Blank" to login as a restricted user
3. Tecam search automatically for any available system and connects.

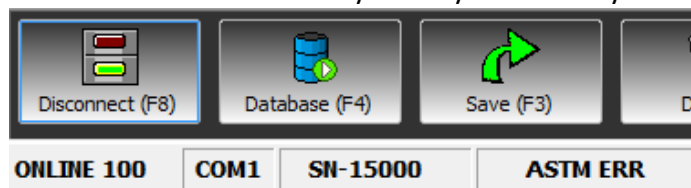

TECAM is linked to system "15000" over com port 1. No ASTM is active

4. Enter administrator password (default = blank) or enter "Blank" to login as a restricted user



TECAM license can be installed on any PC, but is locked to the serial number of instrument

3. Description of the COATRON A4

3.1 Short introduction

The Coatron A4 is a fully automated, stand alone “State of Art” analyzer for the fast and flexible coagulation diagnostic. It is equipped with four optical channels and offers clotting, chromogenic and immunological testing in random access mode as well as fast processing of STAT samples. All sample dilutions and assay calibration are performed automatically. ID-barcode scanner is on board. CAP Piercing is supported for any primary tube system. The analyzer is also focused on a minimum consumption of consumables and reagents, which makes the analyzer very cost effective. The nearly zero service requirements will ensure a long living device by a minimum of service costs.

Optional the analyser can be linked to powerful LIMS software to give exceptional features like unlimited result traceability by an one click report engine or a unique quality control system with Levey Jennings chart and Westgard rules



Use only citrate plasma for sample analysis. Mix 9 parts of venous blood with 1 part 3.2% (0.105M) sodium citrate and centrifuge the mixture at 1500g x 15min. Use plasma within 4 hours.



Do not use plasma with more than 25mg/dL Bilirubin concentration.
Do not use plasma with more than 1000mg/L Hemoglobin concentration.

Based on the optical measurement principle used by this device (transmitted light turbidimetry) with ultraviolet light, a number of coagulation and fibrinolysis parameters can be determined, for example

- Prothrombin time (Quick or Owrens)
- Activated partial thromboplastin time (APTT)
- Fibrinogen (FIB) (Clauss) & derived PT (DFIB)
- Thrombin time (TT)
- Single factor measurements
- Protein C (PC)
- Protein S (PS)
- Lupus Anticoagulant (LA)
- Activated protein C resistance (APCR)
- Heparin (chromogenic)
- ATIII (chromogenic)
- D-dimers (immunoturbidimetric)

Special features:

System

- Ultraviolet light (400 nm). The measurement amplification is adapted to photometric measurement principle with high-resolution 4-channel optics and automatic amplification to any method. Extraneous and scattered light energy is absorbed.
- High-precision XYZ pipetting system with liquid level sensor
- Long living and flexible Cap Piercing needle for primary tubes such as BD Vacutainer® or Sarstedt Monovette®.
- Integrated ID-barcode reader
- Bi-directional ASTM Interface for PC-Link to LIS.*
- Optional trolley to enlarge the waste management
- Integrated graphical thermal printer
- Heated and cooled positions for reagents
- Integrated drawers for consumables

Software

- Approved and highly accurate detection algorithm based on optical density. The clotting time is defined at the turning point of reaction.
- An intuitive TECO GMBH familiar graphical user interface with “Plug And Go” feeling.
- Multi language dialogue. (english , german, spanish, italian)
- Random access scheduler. Profiles can be performed as batch or selective.
- Positive sample identification (ID and rack position) either manual or with barcode scanner
- Fast and easy processing of STAT samples
- Free programmable test protocols to change or adapt new tests
- Calculation of activity %, INR, ratio, g/L , mg/dL , and more.
- Calibration curve can be identified with up to 6 points per test. The results can be calculated with regression line analysis or linear interpolation.
- Single or double determinations
- Simple firmware update
- ASTM interface to link to any LIS *

Special Functions

- Automatic plasma dilutions upto 1:100
- Automatic cleaning cycles
- Automatic test calibration routines
- Automatic quality control
- Automatic or manual printout
- Automatic test skip, if reagent run out.
- Automatic reflex testing for “+++2 results
- Unlimited result management including also reaction curve *
- Quality control according to Westgard rules *
- Result traceability *
- Patient monitoring for long time periods *

Economic

- Half volume procedures resulting in 50% cost savings.
- Reagent dead volume is below 300 µL
- Very economic consumption of Rinse and cleaning solution.
(1L Rinse ~ 1000 det. ; 15mL cleaner is enough for a day work)
- Cuvette with no mixing bars, etc.
- All critical system parameters are monitored and make the instrument nearly free of service.

* only the TECAM PRO software

3.2 Views of the device

3.2.1 Front view

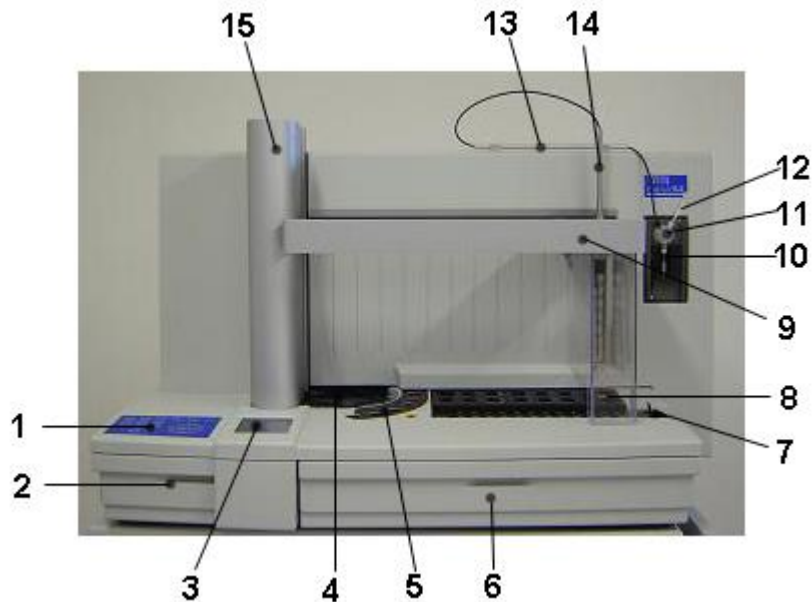


Figure 1: COATRON A4, front view

- | | |
|----|--------------------------------------|
| 1 | Keyboard |
| 2 | Cuvette waste drawer |
| 3 | Screen |
| 4 | Cuvette rotor |
| 5 | System block |
| 6 | Rinse solution waste drawer |
| 7 | Sample racks |
| 8 | Reagent block |
| 9 | Protective bar |
| 10 | Syringe |
| 11 | Pump unit |
| 12 | Tube to Rinsing solution tank |
| 13 | Tube guide for Pipetting needle tube |
| 14 | Pipetting arm |
| 15 | Cuvette tower |

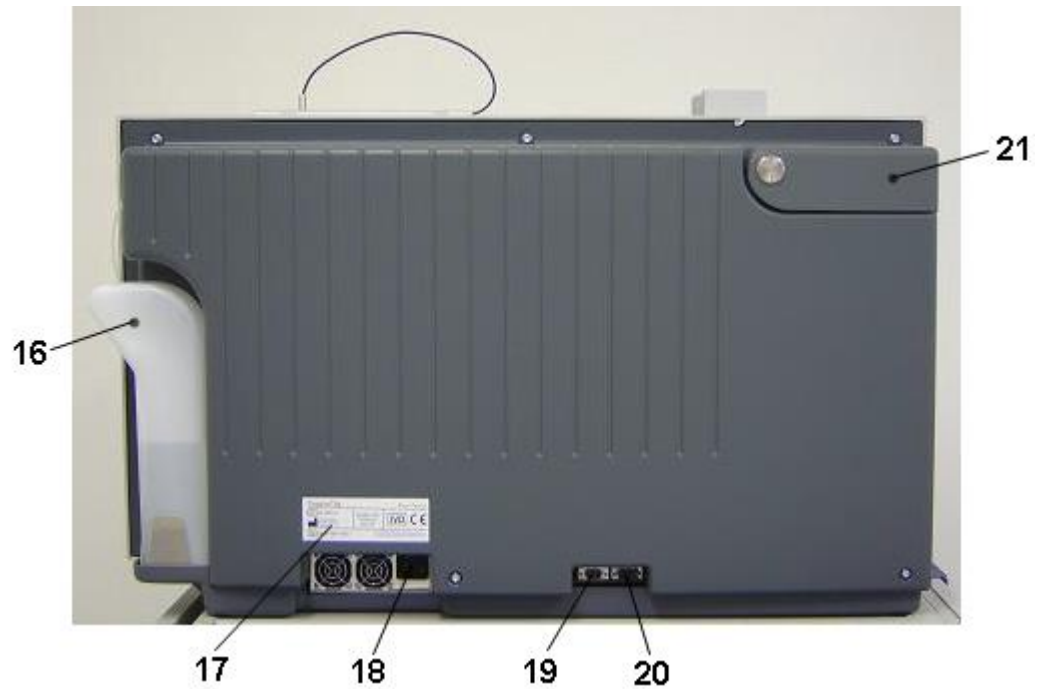
3.2.2 Rear view

Figure 2: COATRON A4, rear view

- 16 Rinsing solution tank
- 17 Type plate
- 18 Mains switch and power input
- 19 RS232 service interface for updating and data transmission (115K, 8,1,N)
- 20 RS232 debug interface for error analysis (reserved for manufacturer)
- 21 Printer cover

3.2.3 Side view

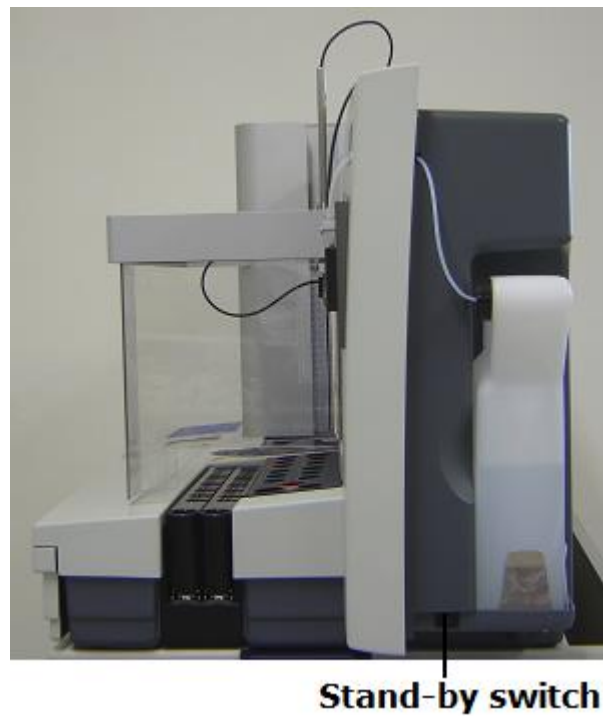


Figure 3: Side view

3.2.4 Sample rack

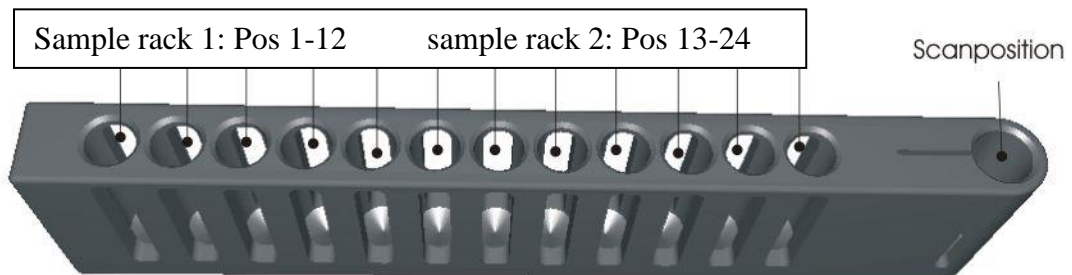


Figure 4: Sample rack

All commercially available sampling systems with a diameter of 11-13 mm can be used as sample tubes (eg. Sarstedt Monovette® or BD Vacutainer®).

3.2.5 Working Positions

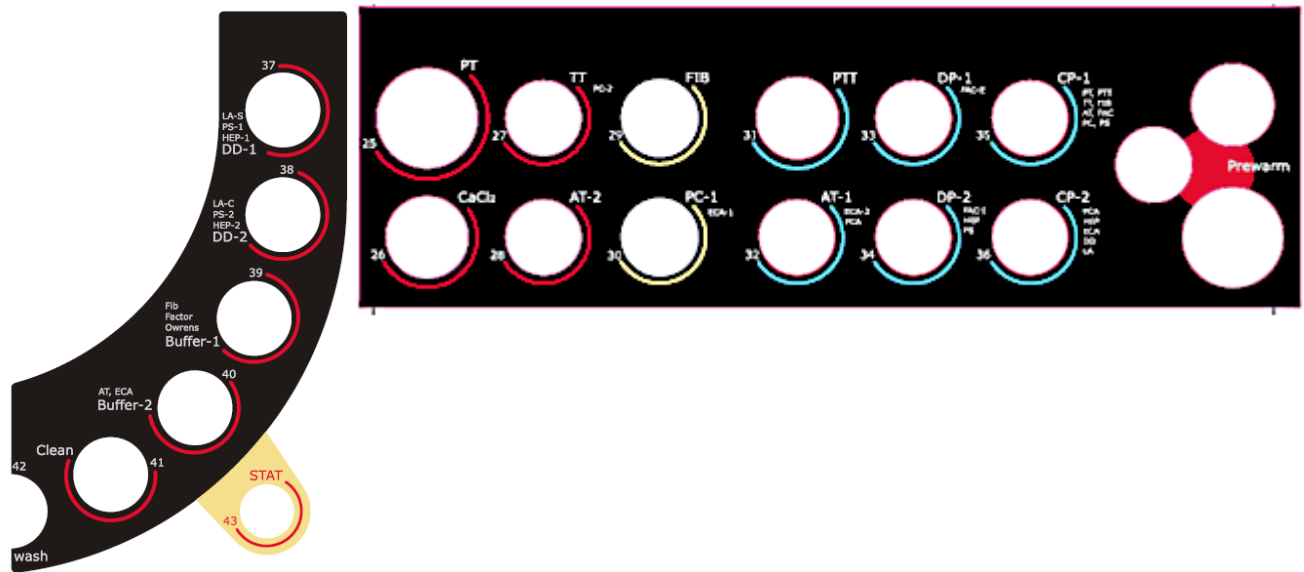


Figure 5: Working Positions

Pos. 1 - 24		Sample positions	Room temperature
Pos. 25	PT	Reagent position for PT, magnetic stirring function	37.0 °C
Pos. 26	CaCl ₂	Reagent position for CaCl ₂	37.0 °C
Pos. 27	TCT	Reagent position for TCT and PC-2 , APC	37.0 °C
Pos. 28	AT-2	Reagent position for AT-2 (substrate)	37.0 °C
Pos. 29	FIB	Reagent position for FIB	Room temperature
Pos. 30	PC-1	Reagent position for PC-1 (activator)	Room temperature
Pos. 31	PTT	Reagent position for PTT	15.0 °C
Pos. 32	AT-1	Reagent position for AT-1 (thrombin/factor Xa reagent)	15.0 °C
Pos. 33	DP-1	Deficient Plasma 1: for FII,FV ,FIIIV, FX ,	15.0 °C
Pos. 34	DP-2	Deficient Plasma 2 : for FVIII, FIX, FXI,FXII,PS,APCR, PK,HMWK	15.0 °C
Pos. 35	CP-1	Control plasma 1: for PT, PTT, TCT, FIB, Factors, PC, AT	15.0 °C
Pos. 36	CP-2	Control plasma 2 : for DD, HEP, APCR, LA	15.0 °C
Pos. 37	DD-1	used for DD-1, HEP-1, LA Screen	37.0 °C
Pos. 38	DD-2	used for DD-2, HEP-2, LA Confirm	37.0 °C
Pos. 39	Buffer-1	Owren's Buffer for plasma dilution (FIB , factors)	37.0 °C
Pos. 40	Buffer-2	Working Buffer for chromogenic tests (AT)	37.0 °C
Pos. 41	Clean	Position for cleaning solution	37.0 °C
Pos. 42	Wash	Wash and waste position	37.0 °C
Pos. 43	STAT	Emergency sample position	Room temperature
Pre-heat	Prewarm	3 prewarm positions	~37.0 °C

Reagent adapters are found in the right-hand device drawer for various reagent container or vials.



The above test reagent allocations are only valid for the factory default protocols.

3.2.6 Keypad

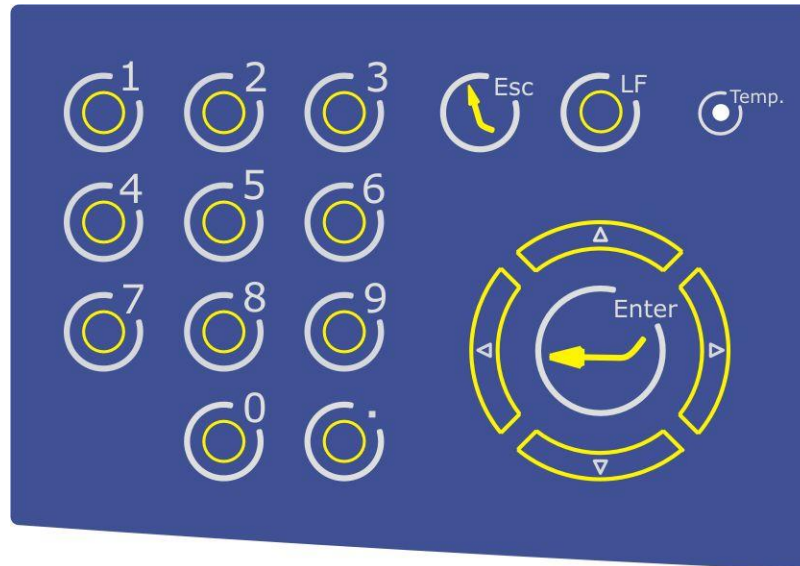


Figure 6: Keypad

0-9	Numeric value input	ARROW ↑	Navigation key
Esc	Leave screen	ARROW ↓	Navigation key
LF	Line up, printer paper	ARROW ←	Navigation key
Temp	Display of standby to measure status	ARROW →	Navigation key
Enter	Input / selection confirmation		

Use the arrow keys to change to the screens up, down, right or left. See chap. 5 for an accurate description of software operations.

3.2.7 Screen segments

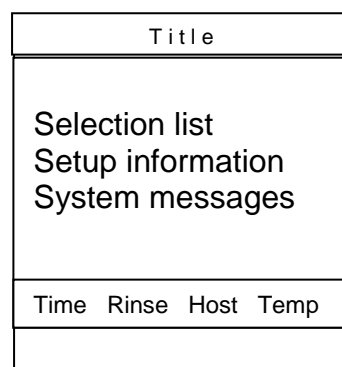


Figure 7: Screen segments

There are 3 screen segments:

- The current menu item appears in the title line.
- The main segment displays the selection lists, information and system messages.
- The bottom line contains the current time, volume of Rinse solution, status of host connection and the temperature in the Optic block.

3.3 Measurement principle

The COATRON A4 is equipped with highly sensitive 4-channel LED optics at a wavelength of 400 nm, making precise and reliable measurements possible even with icteric or lipaemic plasmas.

Once a reaction charge has been prepared, the optimum transillumination settings are found using an amplifier that facilitates measurement of both clear and cloudy samples.

Recording of measurement process data is started automatically when the start reagent is added. When coagulation begins, transmission is reduced, which changes the form of the measurement curve. The time from measurement start to this change (turning point) in seconds [s] is the result. The software then converts this datum into other units.

3.3.1 Mathematical principles

The conversion of coagulation time into a specific test unit is one using a linear, hyperbolic, semi-logarithmic or double-logarithmic interpolation of the stored calibration points. The current mathematical model is printed out in "TEST SETUP." Values outside the calibration range are calculated by extrapolation and flagged as " * ".

3.3.2 Units

Unit	Decimal places	Maximum value
s	1	-
%	1	180
U	0	999
INR	2	12
Ratio	2	9
INR+	2	12
mg/dl	0	900
g/l	2	9
U/ml	2	1
mg/l	2	5
µg/ml	1	999
ng/ml	0	5,000
µg/l	0	5,000

Ratio = clotting time / normal time

INR = Ratio^{ISI} (International Normal Ratio)

ISI = International Sensitivity Index (sensitivity of the PT reagent).
(The ISI value is listed on the reagent information sheet)

INR+ = Like INR, except the ISI value is determined for a specific device. This is done using a calibration curve with INR standards.

3.3.3 Clotting method

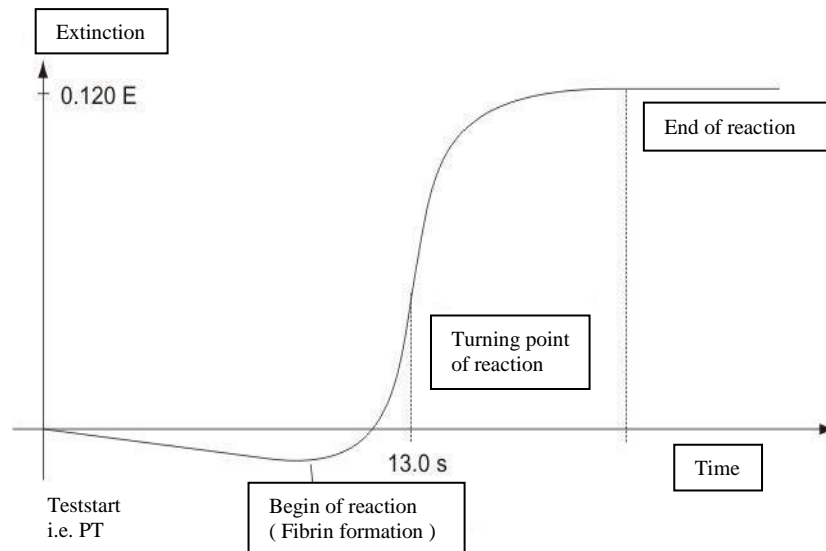


Figure 8: Determination of turning point in clotting method

The final reaction in the coagulation cascade is the transformation of fibrinogen into fibrin catalyzed by thrombin. Fibrin formation results in clouding (higher turbidimetric level) in the sample, which is measured by the photometer and stored as the extinction. The result in seconds is the time from the start of the reaction to the time of greatest extinction increase (reaction turning point).

3.3.4 Derived fibrinogen

The photometric measurement method facilitates measurement of the prothrombin time (PT) as well as, at the same time, derivation of the relevant fibrinogen concentration.

The optical reaction rise (see figure above) between the start and end of the fibrinogen transformation reaction is linearly proportional to the fibrinogen concentration.



The DFIB method should only be used to select samples. Samples with a fibrinogen concentration outside the normal range must be confirmed using the FIB Claus method.

3.3.5 Chromogenic, endpoint and immunoturbidimetric method

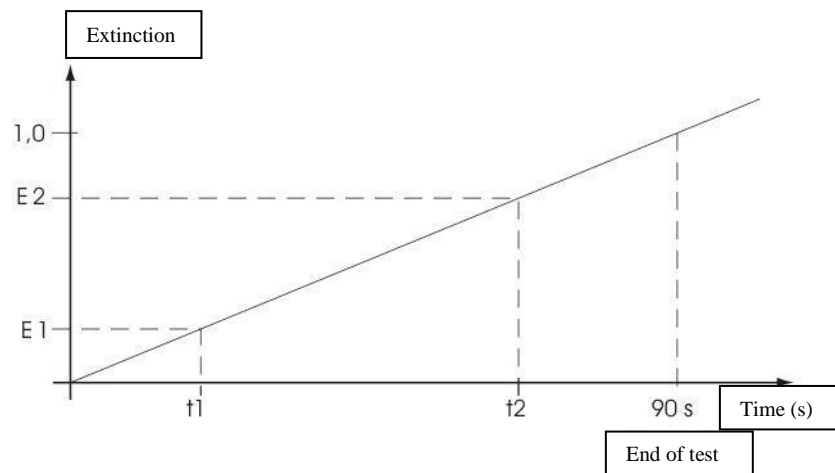


Figure 9: Determination of rise in the kinetic test method

t1 = deadtime in s

t2 = endtime in s

Delta signal $dE = E2 - E1$

Delta time $dT = t2 - t1$

Result of method „CHROM“ = $60 * (dE/dT)$ [dE/min]

Result of method „IMMUN“ = dE/dT

Result of method „POINT“ = dE

3.4 Test overview

Test	Name
PT	Prothrombin Time
DFIB	Fibrinogen, derived
aPTT	Activated Partial Clotting Time
FIB	Fibrinogen, Clauss
AT	Antithrombin
TT	Thrombin Time
DD	D-Dimer
HEP	Heparin
PC	Protein-C
PS	Protein-S
F2	Factor II
F5	Factor V
F7	Factor VII
F8	Factor VIII
F9	Factor IX
F10	Factor X
F11	Factor XI
F12	Factor XII
PLG	Plasminogen
-APC	Activated PC resistance Step1
APCR	Activated PC resistance Step2
LA-S	Lupus Anticoagulants Screen
La-C	Lupus Anticoagulants Confirm
PSF	free Protein S
FDP	Fibrin Degradation Product



Setup off test protocol is described in 5.2.10




Ask local distributor for more information about specific test protocol setup

4. Routine measurement (Typical use case)

- Run 24 patients with PT + aPTT + FIB
- Scan the barcode of the samples
- Instrument should carry out all measurements in single
- Instrument should skip test, if system is out of reagent
- Instrument should not repeat results automatically
- Instrument should report first samples as soon as possible

4.1 Preparation

1. Wait until the COATRON A4 has reached operating temperature.
2. Make sure sufficient cuvettes, rinsing liquid and cleaning liquid are available for the testing procedure.
3. Supply the reagent positions with the required reagents and buffer solutions.
4. Re-enter the calibration curve for the planned tests when new reagents with new lot numbers are used.
See chap. 5.2.2 Submenu Data input for input of a calibration curve
5. Wait about 15 min. after supplying the reagent positions before test processing until the reagents have reached the right temperature (37°C in positions 25 – 28 and room temperature in positions 29 and 30).
6. Change to menu ANALYSIS

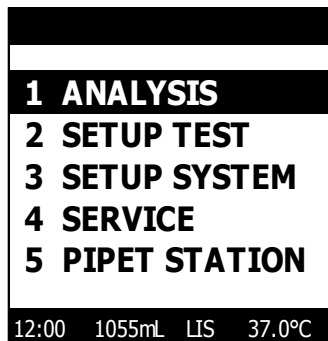

Select ANALYSIS and confirm with ENTER.

4.2 New list input

1. Fill the sample racks with the sample test tubes.
2. Remove the sample test tube cover
3. Make sure barcode labels are visible in the barcode window of the sample rack.
4. In the menu ANALYSIS, go to NEW LIST

CONTINUE:		YES
TEST:	PRFL	
BARCODE:	YES	
RELFEY:	NO	
DOUBLE:	NO	
QC-ACTIVE:	NO	
AUTOSKIP:	NO	
HCT-L:	00 mm	
CLEAN:	MIN	
SHIELD:	YES	
MODE:	CUV	

Select YES and press ENTER to continue

- Select PRFL. Later define profile as PT+aPTT+FIB
- The samples identifications input by barcode
- No automatic test repeat
- Single determination
- No quality control
- Skip test, if out of reagent
- Search for plasma until bottom of tube
- Standard cleaning procedure
- Activate shield protection
- Run worklist in cuvette

CONTINUE:		YES
TEST1: PT	TEST5: -	
TEST2: APTT	TEST6: -	
TEST3: FIB	TEST7: -	
TEST4: -	TEST8: -	

Select YES and press ENTER to continue

Set profile to PT + APTT + FIB

5. Input patient-ID by barcode reader:

BARCODE ENTRY	
RACK1	RACK2
01	13
02	14
03	15
04	16
05	17
06	18
07	19
08	20
09	21
10	22
11	23
12	24

Shift the racks separately at an even and moderate speed in front of the barcode scanner. A signal tone is heard for each recognized barcode

In case of reading errors, check correct position of barcode, shift out rack and repeat scanning..

Press ENTER to continue

6. Start measurement

By select START and press ENTER

PREPARE SYSTEM	
P25	800uL
P26	500uL
P29	500uL
P31	500uL
P39	740uL
CUVETTES 5	
CONTINUE >> KEY ENTER	

Check, if all required reagents are on board and in correct position.

Press ENTER to start measurement
Star
measurement

7. After completion of the measurement, the results and other information on the test are printed out and send to LIS automatically.

4.3 Interrupt or exit measurement

Automatic interrupt of worklist:

Instrument will interrupt worklist automatically, if it runs out of reagent or cuvette during measurement.

Manual interrupt worklist: Press key ESC:

Robotic will finish current command and moves to home and set measurement to pause and an alarm will be activated. Following actions can be performed during interrupt:

Exit worklist: Press key ESC again:

Measurement and worklist will be aborted.

Move robotic: Press key LEFT/RIGHT:


Moves robotic to left or right home position.

Continue worklist: Press key ENTER:

Continuous measurement

4.4 Out of liquid or cuvette during measurement

System will interrupt worklist automatically, if

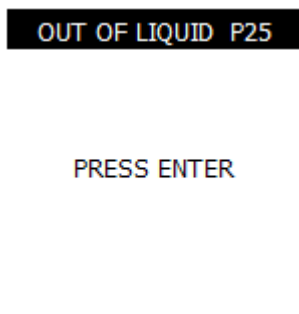

Out of liquid:

Replace vial at indicated position within 30sec after alarm and press ENTER to continue worklist. After 30sec system will exit worklist or skip order according to setup of autoskip function.

Out of cuvette:

Reload cuvettes and press ENTER to continue worklist

4.5 Continuous loading of samples

This feature requires the host software TECAM PRO. The system must be set to "HC", which means host communication is online.

Samples can be loaded during measurement.

(1) Samples without patient barcode

- Define new orders with TECAM software and send to instrument
- Goto instruments and press ESC and wait until robotic is idle
- Place patient samples into rack according to TECAM order sequence

(2) Samples with patient barcode

- Scan patient barcode. System will display rack position and barcode number and interrupt current worklist.
- Wait until measurement is interrupted. Then place the tube into the required rack position.
- Scan and place further samples
- press ENTER to continue worklist
- New PID are now visible at TECAM software. Add methods and send order to instrument.



Do not access or move patient racks during operation of robotic. Always interrupt measurement before loading reagent, cuvette or samples during measurement. Otherwise system can be damaged !

4.6 Measuring the emergency samples

The emergency sample position (STAT position) makes it possible to interrupt regular test processing without losing the worklist settings or the measurement results up to that point. All current tests are terminated and the current worklist is saved so that the worklist can be continued after the emergency measurement. The STAT position is only designed for individual samples. If several emergency samples are to be measured, either repeat the following steps or start with a new list.

STAT ENTRY	
PID:	
TEST:	PT
	INFO
MODE:	MANUAL
CONTINUE:	YES

1. Interrupt the current worklist with Esc (*see chap. 4.4*).
2. Go to the submenu STAT in the main menu ANALYSIS.
3. Either input the PID manually via the numeric keypad or with the barcode scanner as described in chap. 5.1.4.
4. Place the emergency sample in the STAT position (position 43).
5. Select the test.
6. Under INFO you can print out the test SETUP.
7. Set the mode. If it is set to Manual, the interrupted worklist must be continued manually after the emergency sample has been measured. In Auto mode this is done automatically.
8. Leave the screen with Enter.
9. Check the reagents according to the information in the following screen, SYSTEM PREPARATION.
10. Start the emergency measurement with Enter.
11. After the measurement is completed, the test results are printed out analogously to normal test processing.
12. With CONTINUE in the main menu ANALYSIS, processing of the interrupted worklist recommences.



The software "TECAM PRO" features STAT orders, which can be run in regular patient rack and loaded during during operation.



4.7 Quality control measurement

The analyser allows to run one control plasma for each test. The specific control range must be entered in the menu "TEST SETUP". No warning flag "Q" is generated, if the control range is defined equal to zero.

There are two internal position for control plasma (CP-1 , CP-2). But also rack positions can be used for control plasma. The internal positions CP1/CP2 for each test can be found in the printout of the test setup

The analyser identifies a sample as a control if its position is CP1/CP2 or if its PID is equal to one of the two entered lot-numbers A control result is always marked with flag "C" and in case that it is out of range also with flag "Q". All further results will be flagged with "Q" until a new control result is successfully or the instrument is rebooted.

QC with positions CP-1 and CP-2:

- Define control range in the menu SETUP TEST
- Activate QC-ACTIVE within worklist menu
- Optional: Enter lot-number of control plasma within the worklist menu
- Place control plasma to position CP-1 or CP-2. The corresponding control position is printed with the test setup.

QC with rack position P01 and P02:


- Define control range in the menu SETUP TEST
- Set QC-ACTIVE=NO within worklist menu
- Set BARCODE=YES within worklist menu
- Enter the lot-number of control plasma within the worklist menu
- Place control plasma to position P01 and/or P02 and then all samples
- Enter the PID of the samples manually or by barcode. It is important that the PID number of sample P01 is equal to lot-number.



The terminal program "TECAM PRO" features quality control processing according to Levey-Jennings graphics and Westgard rules.

5. Software description

Following menu is displayed after start of instrument

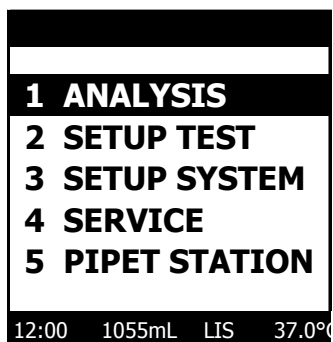

- **ANALYSIS**
Menu to define orders and run patient samples
- **SETUP TEST**
Menu to calibrate methods
- **SETUP SYSTEM**
Menu to change system parameters
- **SERVICE**
Menu to service system
- **PIPET STATION**
Menu to reconstitute reagent and controls

The statusbar shows current information about time, installed RINSE solution, LIS connection and onboard temperature.

5.1 Main menu Analysis

WORKLIST	
1 NEW LIST	
2	CONTINUE
3	REPEAT
4	STAT
5	VIEW
6	PRINT OPTION
7	SYSTEM ACTIVATION
8	REAGENT ACTIVATION
12:00	1055mL LIS 37.0°C

5.1.1 Submenu New List

Creation and processing of a new list is achieved in 3 consecutive screens, each reached from the previous screen by way of Enter on CONTINUE: YES.

ARROW ↑ / ARROW ↓ selects the desired menu item, ARROW ← / ARROW → pages through the options.

With ESC one returns to the previous screen.

Select *CONTINUE = YES* to come to the next screen.

Screen: worklist settings

CONTINUE:	YES
TEST:	PRFL
BARCODE:	NO
RELFEY:	NO
DOUBLE:	NO
QC-ACTIVE:	NO
AUTOSKIP:	NO
HCT-L:	00 mm
CLEAN:	MIN
SHIELD:	YES
MODE:	CUV

Possible settings:

- **Test:**
With ARROW → one proceeds to the list of all available tests in which one navigates with the arrow keys, Enter selects the test from the worklist. With Enter on the field INFO an overview of the test settings is printed out (identical with *chap. 5.2.5, Test printout*).
- **Barcode YES / NO:**
Primary tubes are provided with barcode label, which is used to input the patient identification number (PID)
- **Reflex YES / NO:**
Activates reflex testing. The instrument can repeat automatically suspected results like +++ (no clot detected).
- **Double: YES / NO**
Activates the double test. The mean value is automatically used in the results report. If the two individual results differ by 15%, the result is labelled Flag "%."
- **QC Active: YES / NO**
Carries out control measurements with control plasma before each worklist is started; for this purpose, positions P35 (CP-1) or P36 (CP-2) must be filled with control plasma. The control positions for each test is defined in the Test Setup printout. If the control measurement results are outside the QC range (*see chap. 5.2.4, Submenu QC range*), the results printouts for the worklist will bear the remark "Q."
- **Autoskip YES / NO:**
The instrument will skip current job or test, if plasma or reagent run out and continue with the next order. Skipped jobs are printed as "SKP". Select "CONTINUE" in the analysis menu to re-run only skipped jobs.
- **HCT-L: 0 – 63 mm**
Determines the height of the coagulum (haematocrit level) measured from bottom of tube. The needle will search for plasma only upto this level. HCT-L must be set to 0 ,if only plasma is used

- **CLEAN:** Min - Max
Defines how to clean needle after pipetting samples
 - MIN: Don't perform a clean cycle from sample to sample. The risk of sample to sample carryover was evaluated with extreme high levels of Heparin and concerned low.
 - MAX: Always perform a clean cycle from sample to sample. It required much more Rinse solution and time to carry out a worklis

- **SHIELD:** Yes - No
This setting is only display, if a protection shield is installed.
 - YES: System stop immediately operation, if protection shield is opened during worklist.
 - No: Deactivate shield detection

**Important:**

Deactivated shield function may lead to injury and infections cause by piercing needle.

- **Mode:** BAT / SEL / CUV / EV1 / QC
Determines the mode of test processing:
 - Test Batch (BAT): Processes all similar tests in sequence (eg. all PT , than all APTT, ..) Well-suited to time-optimized test processing in routine operation, but complete patient reports are available after end of worklist.
 - Patient selective (SEL): Processes patients in sequence (eg. Patient 1, PT+APTT then next patient). Important: Complete patient reports are available during run, but worklist need more time and Rinse.
 - Cuvette Batch (CUV): This is a combination of BAT and SEL and combines the best of both. (eg. First cuvette PT, second cuvette aPTT,...).
 - Evaluation 1 (EV1): Regardless of how many samples were entered, plasma is only taken from sample position 1. Well-suited for determination of precision, consumption and throughput volume.
 - QC (QC): This mode is used for quality issues during production of service.



EV1, QC are not suitable for routine processing and should used only for research issues.

Screen: Test Profil, Control plasma and Autoseries input:

CONTINUE:	YES
SAMPLES:	24
1.PID:	1000
CP-1:	N12345678
CP-2:	P23456789
TEST 1:PT	5: AT
	2:APTT 6: -
	3:FIB 7: -
	4:TT 8: -

Possible settings:

- **Samples:**
(only visible of barcode is set to no)
Manual input of number of samples.
- **1. ID**
(only visible of barcode is set to no)
Manual input of Identification Number for first sample. The other samples were automatically incremented by 1 (1000, 1001, 1002,.....)
- **CP-1 , CP-2:**
Input of lot.-numbers for two control plasma manually or by barcode. If the analyser identify a PID number as a control lot. , the result will flagged with "C" and checked if within control range.
- **Test 1 – 8:**
When a profile is to be measured, you can define the individual tests here once again.



-DFIB requires also PT
-ACPR requires also –APC and reverse
-LA requires also LA-C and reverse



Ensure yourself that all reagents for profile can be placed on board.
Otherwise the profile will not operate correctly and lead to erratic results.

Input of PID by barcode or manual entry:

(set BARCODE=YES , see screen 1 above)

In this screen you can enter the patient ident numbers by 3 ways:

BARCODE ENTRY	
RACK 1	RACK 2
01	13
02	14
03	15
04	16
05	17
06	18
07	19
08	20
09	21
10	22
11	23
12	24

- Shift the racks separately at an even and moderate speed in front of the barcode scanner. A signal tone is heard for each recognized barcode

- Use cursor keys to mark the current sample position and scan the sample. Place the sample into current rack position.

- Use cursor keys to mark the current sample position and enter manually the ID number and place the sample into the rack.



If a barcode was not recognized, check alignment and rescan. Read detailed information in chapter "Barcode Guideline"

Press *ENTER* to come into the next screen.

SYNCHRONIZE TO HOST


If PID: 1000

All patient identification numbers will be send to host.

the instrument is linked to host, it will receive corresponding job orders.

In the next screen you can still revise the PID numbers and active tests, which are counted upwards from the PID number of the first sample

POS	PID	1	2	3	4	5	6	7	8
P01	1001	X	X	X	X	X	X	X	X
P02	1001	X	X	X	X	X	X	X	X
P03	1002	X	X	X	X	X	X	X	X
P04	1003	X	X	X	X	X	X	X	X
P05	1004	X	X	X	X	X	X	X	X
P06	1005	X	X	X	X	X	X	X	X
1=PT	2=APTT	3=FIB							
4=TT	5=AT	6=DD							
7=F5	8=F5								



POS	PID	1	2	3	4	5	6	7	8
P01	1000	X	X	X	X	X	X	X	X
P02	1001	X	X	X	X	X	X	X	X
P03	1002	X	X	X	X	X	X	X	X
P04	1003	X	X	X	X	X	X	X	X
P05	1004	X	X	X	X	X	X	X	X
P06	1005	X	X	X	X	X	X	X	X
1=PT	2=APTT	3=FIB							
4=TT	5=AT	6=DD							
7=F5	8=F5								

- Select the order record with cursor keys UP/DOWN.
- Select the order items PID or TESTS with cursor keys RIGHT.
- If a PID is highlighted , use numeric keys to change the number and confirm with Enter.
- If a TEST is highlighted , use Enter to (de)activate. Use dot key "." to (de)activate the tests in all orders.
- To come to the next screen , use key RIGHT until the current order is completely highlighted and press Enter.

When worklist input is complete a further input overview appears.

WORKLIST	
<-	START
TEST:	PRFL
SAMPLES:	06
DOUBLE:	NO
QC-ACTIVE:	NO
AUTOSKIP:	NO
12:00 1055mL H0 37.0°C	

The COATRON A4 requires the following to process the active worklist:

PREPARE SYSTEM	
P25	800uL
P26	500uL
P29	500uL
P31	500uL
P39	740uL
CUVETTES	5
CONTINUE >> KEY ENTER	

- 800µl reagent in position 25=PT
- 500µl reagent in position 26=CACL
- 500µl reagent in position 29=Fibrinogen
- 500µl reagent in position 31=APTT
- 740µl reagent in position 38=FIB buffer
- 5 cuvette trays

Check once again to make sure all reagents and cuvettes on the device are filled. The worklist is started with Enter.

5.1.2 Submenu Continue

Following a test interruption (e.g. due to a STAT task or discontinuation due to a lack of liquid), routine measurement can be continued here.

5.1.3 Submenu Repeat

Repeats the last worklist.

5.1.4 Submenu Stat

Interrupts the regular processing of the list and selects the emergency sample at position 43 in the system block.

STAT ENTRY	
PID:	
TEST:	PT INFO
MODE:	MANUAL
CONTINUE:	YES

- **Input of PID:**

Enter the Patient Identification Number (PID) manually or just scan it with the barcode scanner. Enter terminates input of the PID. Then place the emergency sample in the STAT position.
- **Selection of the test:**

With ARROW ↓ one gets to test selection, ARROW → opens the list of available tests; then use the navigation keys to select the test and return to STAT INPUT with Enter.
- **Information on the test:**

Confirming the INFO field with Enter prints out the test setup just as in normal measurement.
- **Setting the mode:**

If the mode is set to manual, the interrupted worklist must be continued manually after the emergency sample has been measured. In the Auto mode this is done automatically.
- **Activation of emergency measurement:**

Go to the field CONTINUE and confirm with YES.
The next screen SYSTEM PREPARATION displays the required position in the reagent block, the required amount of reagent and the number of cuvettes required.
After checking the reagent position, the measurement procedure can be initiated with Enter.

5.1.5 Submenu Overview

Displays and prints lists according to given sorting criteria.

WORKLIST	
P01	1000
PT	70,1%
APTT	36,1s
FIB	398 mg/dL
P02	1001
PT	100,0%
APTT	33,5s
FIB	250 mg/dL
OPTIONS >> KEY ENTER	


Enter calls up options, ARROW ↑ / ARROW ↓ pages through the options, Enter executes the operation:

WORKLIST	
P01	1000
PRINT REPORT SEND TO HOST STAT	
PC	
OPTIONS >> KEY ENTER	

The following options can be selected:

- Prints report
- Sends to host. Transmit the results from the processed worklist to a PC for further processing. For this function you require the optional software package "TECAM" or similar.
- Displays either the emergency list or the worklist.

5.1.6 Submenu Print Option

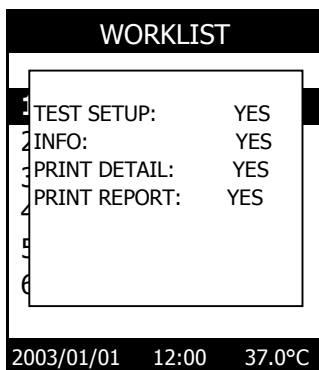


Determines what information is to be printed automatically:

- Test Setup: YES / NO
The Test Setups are printed at the beginning
- Info: YES / NO
Information on worklist is printed at the beginning
- Print details: YES / NO
Detailed results are printed during the measurements
- Print report: YES / NO
A report is printed after the worklist is processed.

5.1.7 Submenu System Activation

This menu is only visible, if instrument is configured as closed system

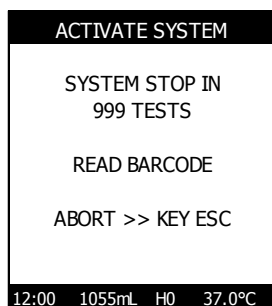

System will stop operating after 999 determinations.

- Skip message with key ESC.
- Scan "Test Activation Key" to activate system.


Barcode will be rejected in case of invalid syntax or if barcode was already scanned before.



Contact your local distributor, if you require a valid barcode.

5.1.8 Submenu Cuvette Activation


This menu is only shown, if instrument is configured as “Closed to cuvette”.
Read the barcode, which is provided with the cuvette package.

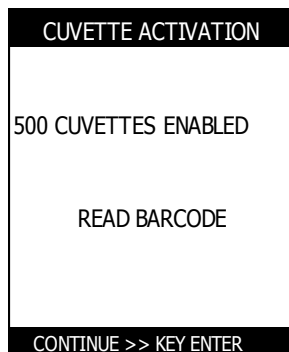

Activation barcode can be read only one time and is be checked by serialnumber of instrument.

5.1.9 Submenu Reagent Activation

A test must be activated by barcode , if the instrument is configured as closed to specific reagent. The barcode is normally printed on the label of the vial. The activation can be done in this separate menu or short before starting the worklist.

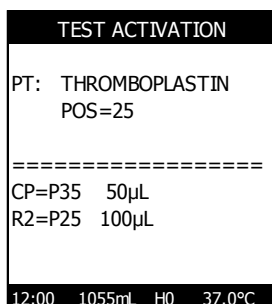

Activate reagent by scanning the barcodes of certain reagents. The activation is valid until next system reboot.

Reagent and test name is displayed as well as the test protocol (e.g. control plasma at P35 with 50µL and R2=Thromboplastin at P25 with 100µL)

Barcodes will be rejected in case of

- invalid syntax of barcode
- date expired
- barcode differs to data stored in the SETUP test



A new LOT must be first calibrated before it can be used within the Worklist. Refer to chapter 5.2 “TEST SETUP”

5.1.10 Reflex testing

This feature is always enabled. After worklist run, then instrument will validate results and repeat test under following circumstances:

- For clotting tests like PT,aPTT,Factors: If result is “+++”, then test is repeated 1x with 60s prolonged maximum reading time.
- For chromogenic tests like AT: If result is “0.000E, then test is repeated 1x.

Repeated results are flagged with “R”

5.1.11 Display during measurement

WORKLIST IN PROCESS		
ID1:	1000	
PT		70,1%
ID2:	1001	
PT		x178
ID3:	1002	
PT		x026
ID4:	1003	
PT		x003
		- HC -
		PROGRESS
		5%

A PT result for sample ID 1000 has already been found in measurement channel 1. On channel 2-4 is a measurement ongoing.

Progress in the worklist is displayed in %. 100% means the worklist has been completely processed.

"HC" indicates that the analyser is linked to HOST.

The above screen appears during measurement.

A rotating bar at the right edge of the screen indicates an incubation (e.g. PTT) in the next cuvette.

A rotating bar in front of a number indicates an ongoing measurement. The number is the current light absorbance in mOD (milli optical density). A pronounced increase in light absorption indicates a coagulation event!

5.1.12 Result warning messages

Results may also be displayed with various additional warning symbols:

- * Result outside calibrated range
- A Result outside normal range
- T Temperature outside 36 – 38°C range
- Q Quality control outside control range
- C Result is identified as a quality control
- E Reagent is expired
- F Low Fibrinogen level found
- R Result repeated (reflex testing)
- ! Result not trustful and should be repeated.
- X Double values deviate by more than 15%
- K Measurement skipped, because out of reagent
- SKP Job was skipped due to missing reagent or plasma
- XXX No result was found
- SSS Signal transmission too low.
- +++ No coagulation determined within measurement time
- ??? Result based on strange optical signals (e.g. air bubble, peaks)

5.1.13 Printout of results

Depending on how the print options are set (see chap. 5.1.6, Submenu *Print Options*), the results are automatically printed out as follows. Each report can be identified with a unique worklist-id number.

TASKLIST 18.04.2003 00:34 TEST: PRFL SAMPLES: 06 BARCODE: NO DOUBLE: NO QC ACTIVE: NO P01 1000 PT 16.1 s 70.1 % P02 1001 PT 16.1 s 70.1 % P03 1002 PT 16.1 s 70.1 % P04 1003 PT 16.1 s 70.1 % P05 1004 PT 16.1 s 70.1 % P05 1004 FIB 8.1 s 398 mg/dl P06 1005 FIB 8.1 s 398 mg/dl	REPORT OF RESULTS Worklist-ID: 1000 TIME: 18.04.2003 00:36 P01 1000 PT 70.1% 16.1s PTT 36.1s FIB 398 mg/dl 8.1s P02 1001 PT 70.1% 16.1s PTT 36.1s FIB 398 mg/dl 8.1s P03 1002 PT 70.1% 16.1s PTT 36.1s FIB 398 mg/dl 8.1s P04 1003 PT 70.1% 16.1s PTT 36.1s FIB 398 mg/dl 8.1s P05 1004 PT 70.1% 16.1s PTT 36.1s FIB 398 mg/dl 8.1s P06 1005 PT 70.1% 16.1s PTT 36.1s FIB 398 mg/dl 8.1s
---	---

Individual results

Report

5.1.14 Host communication

The COATRON A4 has a serial bi-directional interface for data transmission. The terminal program "TECAM PRO" allows to define jobs on the PC surface and send them to the analyser. Once the program has started, all results are automatically sent to the HOST, where they can be graphically presented, including the coagulation curves, and managed in a database. A demo version of TECAM can be downloaded from the distributor's homepage. An active host connection is indicated with "H1" in the screen statusbar and with "HC" in the measurement screen

5.2 Main menu Test Setup

WORKLIST			
1 CHANGE TEST			
2 SET DATA			
3 NORMAL RANGE			
4 CONTROL RANGE			
5 PRINT TEST			
6 PRINT OVERVIEW			
12:00	1055mL	H0	37.0°C

CHANGE TEST			
PT	DFIB	APTT	FIB
AT	TT	DD	HEP
PC	PS	F2	F5
F7	F8	F9	F10
F11	F12	PLG	-APC
APCR	LA-S	LA-C	PSF

1=INFO

5.2.1 Using of reagent barcode

The internal barcode scanner will be activated by entering the submenu SET DATA. After every barcode event, the Coatron A4 will enter the LOT number and expiry date of the barcode.

SETUP F8	
TEST:	F8
LOT:	123456789
EXP.:	01/2004
UNIT:	%
INCUB.:	180s
RUNTIME:	180s
ENTRY:	MANUAL
12:00	1055mL H0 37.0°C

5.2.2 Test Selection

All of the available tests are listed in a table. Navigation within the table is realized with ARROW \uparrow / ARROW \downarrow / ARROW \leftarrow / ARROW \rightarrow . Enter selects a test and returns to the main menu Test Setup. The selected test is displayed in the headline. The following menu items always refer to the current test setting. To carry out several tests on each sample, select the last item, PRFL (profile). In this case, the next menu item DATA INPUT differs from data input in single tests.

5.2.3 Submenu "Set Data"

SETUP F8	
TEST:	F8
LOT:	123456789
EXP.:	01/2004
UNIT:	%
INCUB.:	180s
RUNTIME:	180s
ENTRY:	MANUAL
12:00 1055mL H0 37.0°C	

Single tests:

After replacing the reagents, the lot number (LOT) and expiry date (EXP.) must be re-entered. With ARROW ↑ / ARROW ↓ one selects the value to be changed.

➤ **New lot number (LOT):**

If the LOT number is inverted, ARROW → is used to get to selection of individual digits, numbers and letters and ARROW ↑ / ARROW ↓ are used to page through them; numbers can also be entered directly using the numeric keypad.

➤ **Input of expiry date (EXP.):**

With ARROW ← / ARROW → the month can be changed, with ARROW ↓ the year is changed analogously to the month.



Expired dates will not be accepted by the COATRON A4

➤ **Selection of unit:**

With ARROW ← / ARROW → the units are changed in which the results are displayed with the exception of the basic unit (which depends on the measurement principle). The available units are %, INR, Ratio, INR+ and no further unit (-). Calibration curves can only be entered when a unit has been selected. See *chapter 3.3.2, Units* on the significance and calculation of the units.

➤ **Incubation time setting**

Define the delay time before start reagent (R2) is added.

With ARROW ← / ARROW → the incubation time is changed in 30-second increments from 60 to 450 seconds.

➤ **Runtime setting**

Define the maximum reading time.

➤ **Mode of calibration**

Select between Manual = manual input
 Auto = automatical test calibration

5.2.4 Test Calibration

The analyser gives the operator the option to calibrate a test manually or automatically.

- **Manual Calibration:**
The operator must prepare the standards and run them like normal samples. He must also enter the results manually
- **Auto Calibration with dilutions:**
The operator must place the reference plasma into rack position P01 and additionally empty vials in P02 – P06. The analyser will prepare all required plasma dilutions, run the standards and transfer the results into the calibration curve automatically.
- **Auto Calibration with fix standards:**
The operator can place up to 6 plasma standards into rack. The analyser will run the standards and transfer the results into the calibration curve automatically.
- **Manual calibration**

The operator must prepare the standards and run them like normal samples. He must also enter the results manually

SETUP PT	
TEST:	PT
LOT:	123456789
EXP.:	01/2004
UNIT:	%
INCUB.:	0s
RUNTIME:	120s
ENTRY:	MANUAL
12:00 1055mL H0 37.0°	

SET DATA: PT	
%	s
100	12,1
50	16,2
25	25,7
12,5	36,9
0	0
0	0
R ² =0.962	

Select test and unit, set *ENTRY* to *MANUAL* and press ENTER.

The calibration curve can be entered or changed now manually. At least 2 value pairs are required up to a maximum of 6 value pairs. List navigation is with the arrow keys and the values are confirmed with Enter. A value pair can be added, deleted or changed at any position. Subsequent data saving automatically sorts the calibration data.

INR Calibration:

The operator can select the unit between

- INR = Ratio^{ISI} (International Normal Ratio)
- INR+= INR calculated from a INR/sec reference curve

For UNIT=INR the operator must enter a normal value and the reagent ISI value manually. If a PT % calibration is entered, the instrument will calculate and display the 100% value. This value can be used as normal value if there is no laboratory inhouse normal value.

Linearity of calibration:

The curve linearity is indicated with the regression factor R^2 .

*$R^2 > 0.998$: the curve is linear. Two points are enough.
 $R^2 < 0.950$: the curve is inlinear. Use more than 2 points.
 $R^2 < 0.900$: change math. model and use more than 5 points.
Results outside of calibration are not trustful.*

Invalid calibration data

The calibration data are checked for plausibility when they are saved.


The following rules must be complied with:

- *At least 2 value pairs must be entered*
- *None of the value pairs may be entered double*
- *The values must be $\neq 0$.*
- *The expiry date must be valid*

An invalid "TEST SETUP" will be indicated with a long beep and rejected.

➤ Auto calibration

The COATRON A4 prepares and measures all of the required standard dilutions by itself and enters the mean values in the calibration curve.

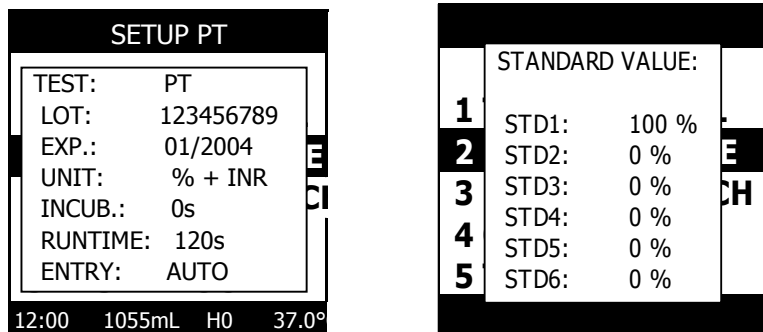


Select test and unit, set *ENTRY* to *Auto* and press ENTER.

• Autocalibration with serial dilutions

The dilutions are always prepared in following way:

1	2	3	4	5	6
1:1	1:2	1:4	1:8	1:16	1:96

1. Enter the calibrator target value in the field "STD1," e.g. 100% for PT calibration, and confirm with Enter.
2. Enter the calibrator in position 1 of the sample rack.

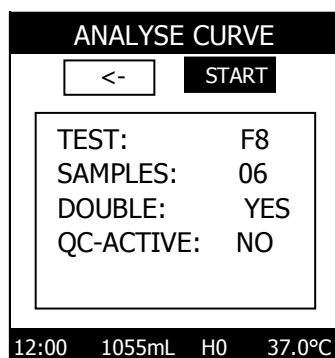

6 standards are measured for factor VIII calibration. Therefore the calibrator must be placed in rack position 1 and 5 other empty sample test tubes are required in rack positions 2-6, in which the COATRON A4 then prepares the necessary dilutions.


3. Additional empty sample test tubes are required in rack positions 2-6. The number of samples corresponds to the

number of sample test tubes and depends on the particular test.

4. Select START, check the reagents and numbers of cuvettes required in the screen SYSTEM PREPARATION and initiate the measurement procedure with Enter.

- **Autocalibration with fixed levels**

Enter more than one standard value in the fields STD1 – STD6. Enter a reference value. Confirm with ENTER. Select next standard field with key DOWN or press ENTER again to proceed with calibration.

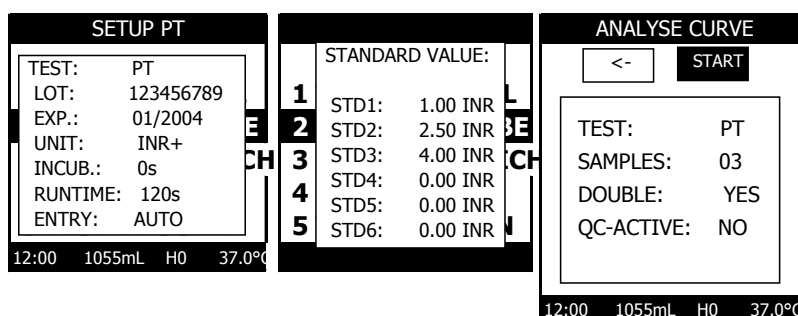

3 fixed standard levels are measured for PT INR calibration. Place INR calibration plasma STD1,2,3 into rack position P01,02 and 03.

5.2.5 Submenu Normal Range

During a routine, a measurement result is flagged "A" (abnormal) if it is outside the normal range. If the normal range is min=max=0, the results are not checked.

Selection of the upper and lower limits of the normal range for the selected tests is with ARROW ↑ / ARROW ↓. If the value is inverted, use the numeric keypad to enter the new limit directly.

Leave the screen with Esc after all of the parameters to be changed have been entered.

In response to the query SAVE DATA? use ARROW ← / ARROW → to select either YES or NO and confirm with Enter.

5.2.6 Submenu QC Range

Indicates the measurement result range expected in a control measurement. The range depends on the particular control plasma and test. See the reagent sheet for the control range. If the measurement result for a control is outside the QC range it will be flagged "Q." If the QC range is min=max=0, the results are not checked.

5.2.7 Storing of test data

Press ESC to return to the main menu "TEST SETUP". If any data was changed, the COATRON A4 will ask for confirmation before storing.

The test data are checked for plausibility when they are saved.

The following rules must be complied with:

- ***The calibration curve must be valid***
- ***The LOT-Number must be in conformity with TECO GMBH***
- ***The expiry date must be valid***

5.2.8 Submenu Test Printout

Prints out the selected parameters for this test

SETUP FIB	
LOT: 302501299	
EXP: 1/2004	- expiry date
LAST CHANGE: 03.04.2003	- date of input
<hr/>	
1: 80 mg/dl - 27.0 s	
2: 120 mg/dl - 18.0 s	
3: 240 mg/dl - 12.0 s	
4: 480 mg/dl - 7.0 s	- calibration values
<hr/>	
R ² = 0,992	- Linearity of the calibration curve (1.000 for a straight line) (R ² should be 0.850 – 1.000)
NORMAL RANGE: 0 - 0 mg/dl	ranges
QC RANGE : 0 - 0 mg/dl	
S-CORR: 0%	signal correction
T-CORR: 0% 0s	time correction
START: 4s	deadtime
INCUB.: 60s	incubation time
RUNTIME: 120s	max. runtime
METHOD: COAG	test method
CT-MECH: NO	clottingtime mechanical
SENS: 0	test sensitivity
MIX: 0	reagent mixing
CLEAN: 0	high cleaning cycle
DIL.: 1:10	plasma dilution
PAT: VOL= 10uL	- Sample volume in µl
CP : VOL= 10uL POS=35	- Control plasma, amount and position
BUF: VOL= 90uL	- Buffer, amount and position
R2 : VOL= 50uL POS=29	- Start reagent, amount and position (here 10 µl sample + 90 Owren's buffer + 50 µl fibrinogen reagent)

5.2.9 Submenu Test Overview

Prints out the current protocols of all tests.

TEST	PAT	BUF	CLR	DEF	R1	R2
PT uL	50	0	0	0	0	100
POS	P35	P38	P00	P00	P00	P25
DFIB uL	50	0	0	0	0	100
POS	P35	P38	P00	P00	P00	P25
APTT uL	50	0	0	0	50	50
POS	P35	P38	P00	P00	P31	P26
...
...

example test protocol APTT:

- add 50µL sample (the control plasma position is P35)
- add 50µL aPTT reagent from P31
- add 50µL CaCl from P26

5.2.10 Setup of test protocol

This feature allows you to change or adapt new reagents or tests.

The test protocols are protected. They can be activated or modified by trained and authorized personel only.

Important:

Improper changing can lead to false results.

Please contact your local authorized distributor/agent, if there is a need to change the parameters.

TEST:	F8
UNIT:	3
METHOD:	COAG
MATH:	logXY
CT-MECH:	NO
START:	15s
POINTS:	6
SENS:	1
MIX:	0
CLEAN:	0
VALIDATE:	YES
S-CORR:	0%
T-CORR:	0%
	0s
MULTI	NO

Screen 1 : test protocols

PAT:	10uL
	P35
BUF:	40uL
	P38
CLR:	0uL
DP:	50uL
	P34
R0:	0uL
	P00
R1:	50uL
	P31
R2:	50uL
	P26

Screen 2 : test protocols

- NAME 4 Characters for test
- UNITS selectable units, decimal code of every bit.
(i.e. units=11-> s,%,INR
 - Bit 0 = always (sec or E)
 - Bit 1 = %
 - Bit 2 = U
 - Bit 3 = INR
 - Bit 4 = RATIO
 - Bit 5 = INR+
 - Bit 6 = INR+%
 - Bit 7 = -
 - Bit 8 = mg/dL
 - Bit 9 = g/L
 - Bit 10 = IE/mL
 - Bit 11 = mg/L
 - Bit 12 = ug/mL
 - Bit 13 = ng/mL
 - Bit 14 = ug/L
 - Bit 15 = IU/mL
- METHODE COAG,FIB,CHROM,IMMUN
- MATH XY-calibration relationship (lin,1/X,logY,logXY)
- CT-MECH Clotting Time Mechanical. Define clot point at 50% of endpoint
 - YES: Clot at 50% signal
 - NO: Clot at turnpoint of reaction (default)
- START Time when measurements start (deadtime)
- POINTS data points for auto calibration
- SENS sensitivity of clotting test (Max=3 -> very sensitive)
- MIX After adding of start reagent the robot will mix in the cuvette
- CLEAN needle will be flushed with double Rinse solution
- VALIDATE reagent must will be validated by barcode (eg. lot, expiry).
- S-CORR signal correction (eg. Calculate FIB signal 10% higher)
- T-CORR % time correction (eg. Calculate PT 10% shorter)
- T-CORR s time correction (eg. Calculate PT 2s shorter)
- Multi allow sample multi dispensing to increase throughput.
- Vol Pat Volume of patient in μL
- Pos CP Position of Control plasma
- Vol Buffer Volume of buffer
- Pos Buffer Position of buffer
- Vol Clr Clear Volume
- Vol DP Volume of deficient plasma in μL
- Pos DP Position of deficient plasma
- Vol R0 Volume of reagent 0
- Pos R0 Position of reagent 0
- Vol R1 Volume of reagent 1
- Pos R1 Position of reagent 1
- Vol R2 Volume of reagent 2 = Start reagent
- Pos R2 Position of reagent 2

Set volume and position to "0" if not required

Set volume and position to "0" if not required

Regard the impression of dispenser:



- Below 4 μ L: >15%
- At 5 μ L: 5%
- Above 10 μ L: <1%

Concern the clear volume:



A minimum of 75 μ L must be left in the cuvette. Example instrument pipet 5 μ L sample and 195 μ L buffer into cuvette. Then a maximum of 125 μ L plasmadilution can be cleared.

5.3 Main menu System Setup

System Setup is used to for basic device settings that are normally only rarely changed.

SYSTEM SETUP	
LANGUAGE:	ENGLISH
DATE:	2003/01/01
TIME:	14:59:05
SIGNAL:	ON
CONTRAST:	225
MIXER:	200
SIMULATOR:	0

General operation:

ARROW ↑/↓ left column Change item

ARROW → change to right column

ARROW ↑/↓ right column: Change value

Enter to confirm the value.

ESC exit menu

5.3.1 Language

Select between: English - Italian - Spanish - German

5.3.2 Date

The date format is changed in change mode with ARROW ↑ / ARROW ↓:

- European date format (DD.MM.YYYY)
- American date format (YYYY/MM/DD)

Use Enter to get into change mode for day, month and year, use ARROW ↑ / ARROW ↓ to change the date elements (day, month, year).

5.3.3 Time

Use Enter to get into change mode for hours, minutes and seconds, use ARROW ↑ / ARROW ↓ to change the time elements (hours, minutes and seconds).

5.3.4 Signal

Switches the acoustic signal on or off.

Possible settings:

- Signal on
- Signal off

5.3.5 Contrast

Changes screen image contrast.

Continuous settings from 214 to 255; the result can be checked on the screen without delay.

5.3.6 Mixer

Changes the magnetic stirrer speed at position 25 in the reagent block. Continuous settings from 0 to 255, standard setting 200.

5.3.7 Simulator

Facilitates simulation of measurement operation without moving the pipetting arm.

- Simulator = 0:
Normal operation; simulator is not active
- Simulator = 1:
Maintenance operation; commands issued to the XYZ robot are not executed. System functions as usual otherwise. This mode is very helpful for maintenance work or while familiarizing oneself with the system.
- Simulator = 2:
Demonstration operation; remove the syringe from the pump. Fill all required test and plasma positions with water-filled vessels. Cuvettes are not required. Now start a worklist. This mode is intended for system demonstration.

5.4 Main Menu SERVICE

SERVICE	
1	PRINT REPORT
2	ADJUST XYZ
3	ADJUST TEMPERATURE
4	CHECK OPTIC
5	CHECK ROBOTICS
6	MOVE CUVETTES
7	CLEAN NEEDLE
8	REPLACE RINSE TANK
9	REPLACE NEEDLE
10	REPLACE SYRINGE
11	ADJUST MOTOR
12	CAP PIERCING

ARROW ↑/↓
Enter
1-9

the desired menu item is selected
initiates the operation directly.
select item directly

5.4.1 System report

Printout of important system data

SYSTEM - REPORT			
DATE: 2010/25/10 13:59			
SYSTEM: COATRON A4			
SERIAL NO.: 1234567			
SOFTWARE: 01.06.01			
OPTIC 1:	80	30005	(162)
OPTIC 2:	62	29984	(169)
OPTIC 3:	85	29766	(153)
OPTIC 4:	50	29793	(155)
TEMPERATURE CV:	39.2 °C	(39.0)	
	34968	(34970)	
TEMPERATURE PT:	37.1 °C	(37.0)	
	34395	(34398)	
CONTRAST:	225		
MIXER:	200		
-----WASH	REAG	CUV	PAT
OFFSET X: 1	-2	0	0
OFFSET Y: 3	1	0	-5
OFFSET Z: 0	13	0	850
OFFSET M: 4			
OFFSET P: 0			
RINSE INSTALLED:	108 ml		
NEEDLE TIMER:	2300		
SYRINGE TIMER:	32023		
STOP-STOP IN:	905 TESTS		
SERVICE IN:	58001 TESTS		
PT COUNTER:	10000		
PTT COUNTER:	10000		
FIB COUNTER:	5000		
TT COUNTER:	1000		
DD COUNTER:	1000		
ANALYSIS COUNTER:	27000		
---- SYSTEM STATUS ---			
SYSTEM =	OPEN		
SERVICE =	CLOSE		
REAGENT =	OPEN		
OPTICS :	80	30005	(162)
	80	= Digital value when LED is off	
	30005	= Digital value when LED is on	
	162	= Amplification factor	
Temperature cuvette:	current celsius	(target)	
	Current digits	(target)	
Temperature reagent PT:	current celsius	(target)	
	Current digits	(target)	
Display contrast			
Reagent mixing speed			
Needle Position for Wash , Reagent,Cuvette & Patient			
X-Offset =	left/right		
Y-Offset =	forward/backward		
Z-Offset =	up/down		
Motor Adjustment:	Offset=4		
CAP PIERCING height			
Remaining system liquid			
Age of needle:	number of performed tests		
Age of syringe:	number of up/down cycles		
Remaining determination before system stop operation.			
Number of carried out tests for counted PT,PTT,FIB or all tests			
System do not require a barcode to run tests			
System requires a barcode to reset service interval			
System do not require a barcode before use of reagent			


5.4.2 Adjust XYZ

Key 4/6	move needle left/right (X-offset)
Key 2/8	move needle backward/forward (Y-offset)
ARROW ↑/↓	move needle up/down (Z-offset)
ENTER	goto next position
ESC	exit adjustment

Ensure yourself, that the needle is straight and correct mounted 115mm in length. Place an empty reagent container to position P27, two empty cuvettes in the tower, an empty plasma tube to position P01 and an unused Sarstedt Monovette® or BD Vacutainer® in position P02. (only if CAP PIERCING option is required)

Five position must be adjusted

- Wash position
- Reagent position
- Cuvette position
- Patient position
- Cap piercing height

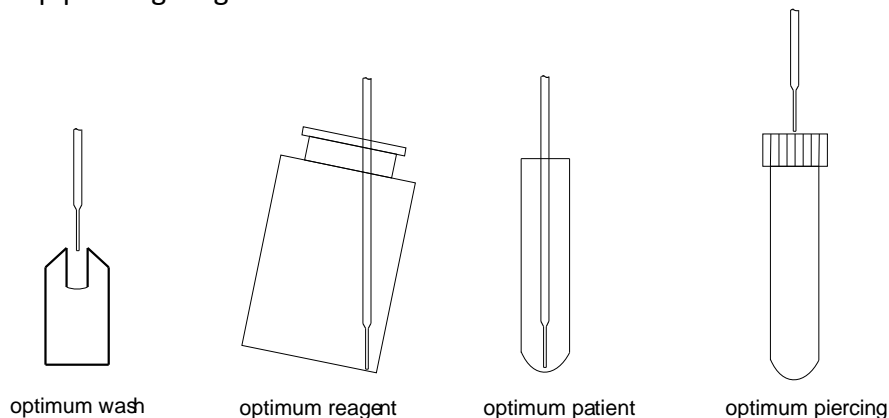

1. First the needle will go to wash position. Center the needle exactly. The needle tip must be at same level with top of wash position. Press "ENTER" to come to next position or press "ESC" to quit.
2. Second the needle will go to P27 position. Center the needle. The needle tip should be short before touching the vial bottom. Lift vial to determine the distance. Press "ENTER" to come to next position or press "ESC" to quit.
3. Third the needle will go to cuvette position. Center the needle and afterwards lower the needle until it is short before touching the cuvette. Lift the cuvette to determine the distance. Press "ENTER" to come to next position or press "ESC" to quit.

4. Forth the needle will go to P01 position. Center the needle. The needle tip should be short before touching the vial bottom. Lift vial to determine the distance. Press "ENTER" to come to next position or press "ESC" to quit.
5. Fifth the needle will go to P02 position. Center the needle. The needle tip should be short before touching the cap membrane. Press "ENTER" to test cap piercing or press "ESC" to quit.




skip cap piercing if not required. The value P-OFFSET must be 0 to deactivate cap piercing.



Important:

To avoid needle crash the z-offset is set to default, before the needle drives to this position. So even if you didn't change the offset, the z-position must be re-adjusted anytime

5.4.3 Check Temperature

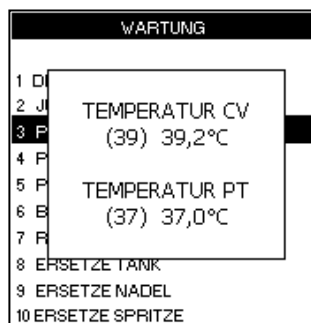

Temperature CV	Temperature around measurement cuvette.
Temperature PT	Temperature at reagent position PT (P25)
(xx)	Target temperature in degrees Celsius
xx,x	Current temperature

Setting the temperature:

With ARROW ↓ / ↑ the current temperature is changed in 0.1°C increments. Enter selects the temperature ESC returns to the service menu.

1. Place an empty cuvette in the measuring cell and fill 300 µl water into all of the 4 measurement positions. Place a standard commercial fever thermometer in one of the cuvette wells. Make sure the cuvette is standing upright.

2. Place also an empty reagent container in position "PT" (P25) and fill with 6 - 7 ml water. Place a standard commercial digital fever thermometer in the water.
3. On the keyboard the green Temp. LED should light up.
4. Wait for at least 15 minutes. Now read off the temperature on the Thermometer.
5. In the cuvette position the temperature should be in the range of $\pm 0.5^{\circ}\text{C}$ from target value. Temperature can be increased or decrease by pressing ARROW \downarrow / \uparrow .
6. Adjust temperature so often until the temperature shown on display matches the temperature in the cuvette or PT position.
7. For "PT" also the target temperature can be adjusted. Lower storage temperature of reagents will significantly increase stability, while results will be nearly unchanged.



Please ask local distributor about change of reagent target temperature.

5.4.4 Check Optics

Remove the cuvette in the measurement optics.

CHECK OPTIK			
	OFF	ON	AMP
1=	78	29851	185
2=	105	29624	192
3=	56	29799	171
4=	78	29851	185
T1=	34302		
T2=	34429		
CV-STATUS:	0		
SHIELD:	0		

X=	Measurement channel 1-4	
OFF	Digital value when LED is off. Target range <500	
ON	Digital value when LED is on. Target range 28000 - 32000	
AMP	Signal amplification, Target range 150 - 300	
T1	Digital value temperature CV, Target range 33000 - 36000	
T2	Digital value temperature PT, Target range 33500 - 36000	
CV-STAT	0=no cuvette	1=if cuvette is detected.
Shield	0=closed	1 = open



Please contact customer service if the values deviated from the target values.

5.4.5 Check Robot

To check, if XYZ, pump and level sensor is working. Press ESC to abort this test. It is used for service and quality issues. Remove all vials and tubes before continue. Print "FALSE LEVEL" indicates that level detector stops false in air. In this case the insulation block must be replaced.

5.4.6 Move Cuvettes


Turns cuvette rotor for transport of cuvettes until Enter is pressed. It is used to empty the cuvette tower.

5.4.7 Clean Needle

Carries out an intensive needle cleaning cycle. It is used after needle is complete and partial clogged during measurement.

5.4.8 Replace Rinse tank

Barcode activation is only shown if instrument is closed to Rinse solution. Read the barcode, which is provided with the cuvette package.

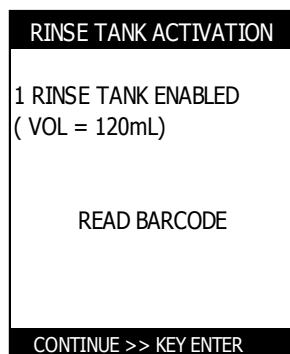

The current numbers of remaining Rinse tanks and installed volume of Rinse solution is displayed.

1. Remove the waste tank and dispose it according to regulations for infectious material
2. Replace the empty rinsing tank with a full one. Ensure that the tube is insert completely into the tank.
3. Use the empty Rinse tank as new waste tank !
4. Run menu "SERVICE\REPLACE RINSE TANK"to reset the Rinse counter
5. If zero tanks are enabled, scan the barcode of the certificate, which is included to each new box of Rinse tanks.



Make sure a full tank is really installed, since otherwise the COATRON A4 will calculate the consumption incorrectly.



The full liquid waste tank may contain infectious substances and must be handled and disposed of as infectious waste. Always wear gloves for infection protection when replacing the liquid waste tank! After this procedure, disinfect your hands with a hand disinfectant, e.g. Sterilium®.

5.4.9 Replace Needle

Resets the operating time counter of the pipetting needle to zero. This operation must be carried out when the needle is replaced.

1. Switch off instrument
2. Drive needle manually into wash position and open the tube fitting on valve.
3. Wait until needle is complete empty from Rinse solution. Clean and dry needle outside, to avoid any liquid contamination with the insulation block.
4. Loosen the screw (see figure below)and remove the needle
5. Insert new needle until 115mm is visible and tighten the screw
6. Screw the tube fittings to the left valve channel and tighten only by finger
7. Switch on instrument and run menu "SERVICE\REPLACE NEEDLE"

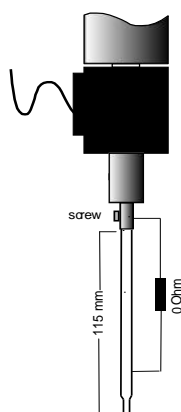


Figure 10: Replace Needle



Any liquid contamination of the insulation block with the needle may malfunction the level sensing.



The used pipetting needle may contain infectious substances and must be handled and disposed of as infectious waste.

5.4.10 Replace Syringe

Resets the operating time counter of the syringe to zero. This operation must be carried out when the COATRON A4 is when the syringe is replaced.

1. Switch off instrument
2. Lower the plunger drive manually by pushing down on the carriage assembly until it reaches the bottom of travel.
3. Now open the syringe and remove it.
4. Insert the new syringe and tighten just with your fingers
5. Switch on instrument and run menu "SERVICE\REPLACE SYRINGE"

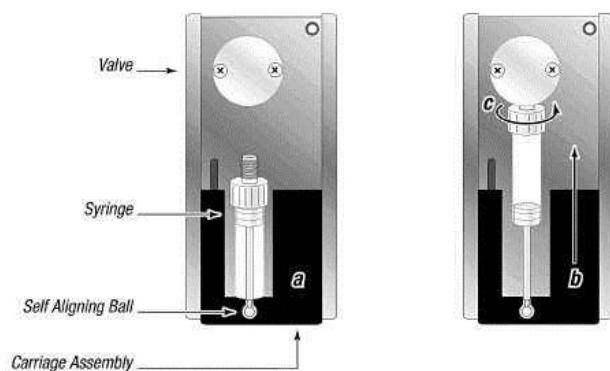


Figure 11: Installation of syringe

5.4.11 Adjust Motor

Changes the assignment of the cuvette to the measuring position. The cuvette must be positioned exactly centered to the optic, to ensure accurate results. Fill some water into a container and color the water with a green lightning pen. Remove all cuvettes onboard. Add 150 μ L green colored water into every cuvette position and place it into position prewarm. Run menu "ADJUST MOTOR". The system moves now cuvette into optics. If the light beams are not centered, change the offset value, move cuvette back and repeat the procedure until correct adjustment of the cuvette position. The factory default value is „4“ . An increase of the offset will shift the cuvette to the left.




Important:

False adjustment will reduce the measuring precision.

5.4.12 Cap Piercing

Fill a Sarstedt Monovette® or BD Vacutainer® or a similar system with 2mL water. Close the cap and place it into rack position P02. Lower the needle until it is just before touching the cap. Then center the needle to the cap.



optimum piercing

- ⇒ use keys 4/6 or 2/8 or Up/Down to move needle
- ⇒ confirm with Enter to check cap piercing
- ⇒ confirm with ESC to exit adjustment



Cap piercing function is deactivated , if height P-Offset is set to 0



Activated cap piercing function allows to operate with open or closed tubes. The throughput gets a little lower.



Warning!

The system may be damaged, if no needle protection is mounted.

Cap piercing requires also a special needle, which is designed for it. Ask your local distributor for further information.

5.5 Main menu PIPET STATION

Menu to reconstitute reagent and controls

PIPET STATION	
IN:	P26
OUT:	P25
TOTAL:	0 ul
VOL (uL):	1000
PIPET >> KEY ENTER	
ABORT >> KEY ESC	

Fill enough diluent into container and place it to position P26. Open reagent vial and place it to position P25. Change volume with keys UP/DOWN and press ENTER to dispense diluent into reagent vial. Press ENTER again if more diluent is required. The total volume will be updated with each pipeting step. Press ESC to reset total counter and press ESC again to exit menu.

6. Replacement of consumables

6.1 Disposal




Warning!

The full liquid waste tank and used cuvette may contain infectious substances and must be handled and disposed of as infectious waste. Always wear gloves for infection protection when replacing the liquid waste tank! After this procedure, disinfect your hands with a hand disinfectant, e.g. Sterilium®.

6.2 Refill cuvettes



Cuvette trays are disposable articles, reuse is not permissible for reasons related to hygiene and measurement technology!

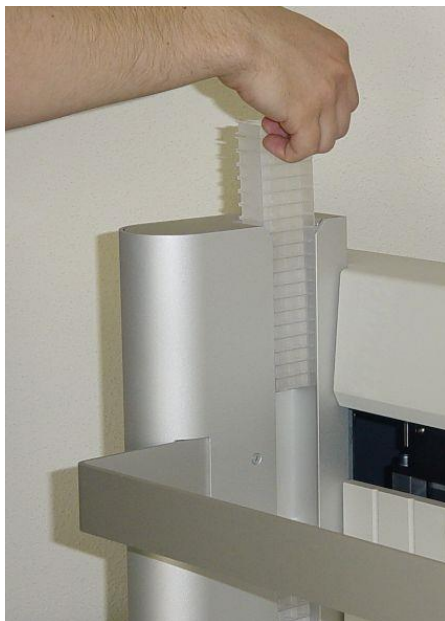

1. Remove a row of cuvettes from the package
2. Hold the row by the tape and insert the cuvettes as shown, from above and with the guide groove to the rear, into the cuvette tower.
3. Pull the tape off the cuvettes

Figure 12: Refill cuvettes

6.3 Replace Rinse tank

Follow instruction from chapter 5.4.8

6.4 Replenishing the printer paper



Figure 13: Printer cover

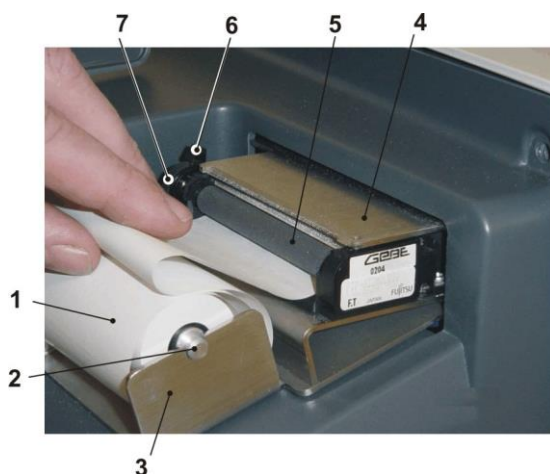


Figure 14: Replenishing the printer paper

1. Open the printer cover as shown at the back of the housing.
2. Remove the printer shaft from the mount (3).
3. Pull the empty printer paper roll off the printer shaft
4. Insert the printer shaft 2) through the new printing paper roll (1) and place the printer shaft on the mounts as shown (3), so that the paper is pulled into the rubber roller (5) from below.
5. Move the arresting lever (6) in the direction of the back wall of the housing to release it.
6. As shown, insert the printer paper under the rubber roller and turn the transport wheel (7) to the left until the printer paper sticks out of the gap between the rubber roller and the metal cover (6) by about 5 cm.
7. Secure the arresting lever 6) by moving it towards the front of the housing.
8. Hold the printer paper towards the front of the housing and close the cover.

7. Cleaning and maintenance

Maintenance must be performed on a regular basis in order to maintain accuracy and precision. The schedule below outlines the proper intervals to check or replace components of the instrument.

7.1 General cleaning information

- Use detergent and water and 10% diluted bleach or commercial decontaminant for daily cleaning
- Use 30% diluted bleach and commercial disinfectant (e.g. Bacillol®AF) for weekly decontamination
- Clean with a lint free cotton cloth or stick
- Never pour any liquid into optic or working area
- Keep the device free of dust and moisture.
- If the device is soiled with liquids, remove the soiling with an absorbent cloth.
- If a liquid has accidentally been spilt or pipetted into a measurement channel, remove it immediately with a pipette and clean the measurement channel with a lint-free cloth. Check the function of the optics in the menu SERVICE



Regard all surfaces and materials which might be in contact with plasma or other biological liquid as potentially contaminated with infectious material.



Avoid any direct contact with decontaminants or disinfections.

7.2 Cleaning

- Use detergent and water and 10% diluted bleach or commercial decontaminant
- Clean and wipe up all spills around the working area or needle pump system with detergent and water.

7.3 Decontamination

- Use 30% diluted bleach and commercial disinfectant (e.g. Bacillol®AF)
- Decontaminate working area, needle area, patient racks, keyboard, LCD screen, front casings, printer and waste drawers

7.4 Daily activities

- Clean and wipe up all spills around the working area or needle pump system

with a 10% diluted bleach.

- Inspect level of Rinse and waste container
- Empty cuvette drawer and fill tower
- Inspect tube system for any leaks and correct immediately

7.5 Weekly activities

- Decontaminate system with bleach and ethanol as described above

7.6 Yearly activities

- Clean and decontaminate equipment
- A yearly service check according to TECO test specification QMV-07-10 must be carried out by the authorized and qualified technician
-

7.7 Regular Replacements

Every 100.000 tests following parts must be replaced

1. Replace needle
2. Replace syringe seal
3. Replace tubing
4. Replace insulation block
5. Replace cleaning position
6. After 5 year replace battery of the mainboard (Li-Mn CR 2430)

7.8 Reset Service Interval

- After 100.000 tests the message "SERVICE" will be shown. The reset of the service interval is protected by barcode. Contact local distributor for more information.

7.9 Error messages

Error message	Possible cause	Action
Service	Service interval is expired after 100.000 tests	Service instrument and reset interval with barcode certificate.
Replace Rinse tank	Rinsing solution tank empty	Replace rinsing solution tank (<i>chap. 6.1</i>)
Error pump	Needle clogged	Check needle and tube system
Error robot (system error 2-28)	No connection to pipetting arm	Consult the customer service of your dealer
	Needle crash	Reboot the system
Activate System	System interval is expired	Scan barcode "Test Activation Key"
Activate Reagent	Reagent must be validated	Refill cuvettes (<i>chap. 6.3</i>)
Adjust XYZ	Replacement of needle	XYZ adjustment of pipetting arm (<i>chap. 5.4.2</i>)
Adjust Motor	Replacement of main-board or software update	adjustment of cuvette (<i>chap. 5.4.11</i>)
No liquid	No liquid in current position of pipetting needle	Refill liquid at current needle position.
	Z-offset false	XYZ adjustment of pipetting arm (<i>chap. 5.4.2</i>)
Check printer	No printer paper	Replenish printer paper (<i>chap. 6.7</i>)
	Arresting lever in offline position	Change arresting lever position (<i>chap. 6.7</i>)
	No printer connected	Consult customer service
Check temperature	Temperature in system block too high or too low	Check temperature and adjust (<i>chap. 5.4.2</i>)
Clean needle	Pipetting needle was replaced	Carry out needle cleaning cycle (<i>chap. 5.4.7</i>)
Check waste	Every 80 cuvette or every new Rinse tank the instrument do a reminder to check also the waste.	Check cuvette waste drawer and also Rinse waste tank. Then just confirm message.

8. Elimination of malfunctions

8.1 Device malfunctions

Malfunction / Error	Possible cause	Measures
No print on printout	Paper installed in wrong position	Turn paper roll around (<i>chap. 6.7</i>)
Needle does not pipette	Tube system leaky	Replace the tube system
	Needle clogged	Place the needle in COATRON A4 Cleaner for 30 min, then run the wash cycle.
Poor reproducibility	Needle-tube system	Replace the needle, tube system and syringe.
	Motor is not adjusted	Check the adjustment of the cuvette to the optic (<i>chap. 5.4.11</i>)
Cuvette assumes false position	Wrong cuvette	Use only original COATRON A4 cuvettes
	Motor is not adjusted	Check the adjustment of the cuvette to the optic (<i>chap. 5.4.11</i>)
	Defective cuvette motor or microswitch for cuvette recognition	Consult customer service of your dealer
Optics not within target value range	Cuvette is in measurement position during optics check	Remove the cuvette and repeat the optics check
	Soiling or liquid in measurement channel	Optics must be cleaned. Consult customer service
	LED does not light up.	Customer service will replace optics

8.2 Measurement malfunctions

Malfunction / Error	Possible cause	Measures
Control measurements do not supply expected results	False calibration data	Consult customer service of your dealer
	Motor is not adjusted	Check the adjustment of the cuvette to the optic (<i>chap. 5.4.11</i>)
False measurement results	Reagent	Check TEST SETUP
	Temperature	Check temperature (<i>chap. 5.4.3</i>)
	Optics	Check optics (<i>chap. 5.4.4.</i>)
	Motor is not adjusted	Check the adjustment of the cuvette to the optic (<i>chap. 5.4.11</i>)
Results flagged "*"	Result outside calibration range	
Flagged "A"	Result outside normal range	
Flagged "T"	Temperature outside 36 – 38°C range	
Flagged "E"	Reagent is expired	
Flagged "Q"	Quality control outside control range	
Flagged "S"	Environment light too bright (low >750digits)	Avoid direct sunlight or other UV sources
Flagged "F" (only test PT)	Low fibrinogen.	Run test FIB to confirm.
Flagged "R"	Result repeated. Max. Runtime too short or problems with level sensor	
Flagged "!" (only test DD)	Result not trustful.	Dilute sample and repeat.
Flagged "X"	Double values deviate by more than 15%	
Flagged "+++"	No coagulation seen with measurement time	
Flagged "???"	Coagulation time indeterminate; course of reaction does not correspond to the criteria of the evaluation algorithm (e.g. turbidity due to air bubbles or coagulation begins before dead time)	
Flagged "SSS"	Low signal. Light transmission is not enough.	Check optics (<i>chap. 5.4.4</i>)
Flagged "K"	Sample, Test is skipped because out of reagent.	

8.3 Packing the COATRON A4 for shipment

If the COATRON A4 is to be shipped, e.g. to the Technical Service, please include the following information in an accompanying letter:

- Complete address of owner.
- Name of dealer from whom the Analyzer was purchased.
- Exact designation of the Analyzer and serial number (on type plate).
- A useful description of the reason why the equipment is being sent in (error / malfunction description).

You should use the original packaging material to avoid transport damage. If the original packaging is no longer available, contact your dealer.


Preparation of the Analyzer for transport:

1. Remove the power cord from the socket and from the Analyzer.
2. Immobilize all moving parts such as sample racks printer shaft, etc. with tape.
3. Remove the needles place them in the drawer for the waste tank.
4. Fix the robot in the resting position (seen from the front—right, rear) with tape or cable binders to the protective bar.
5. Push the Analyzer to the edge of the table; then two persons must lift it by the short sides.
6. Life the Analyzer carefully into the packaging.

9. Appendix

9.1 Interface to LIS

The instrument support two serial RS232 ports to connect with laboratory information system (LIS) .

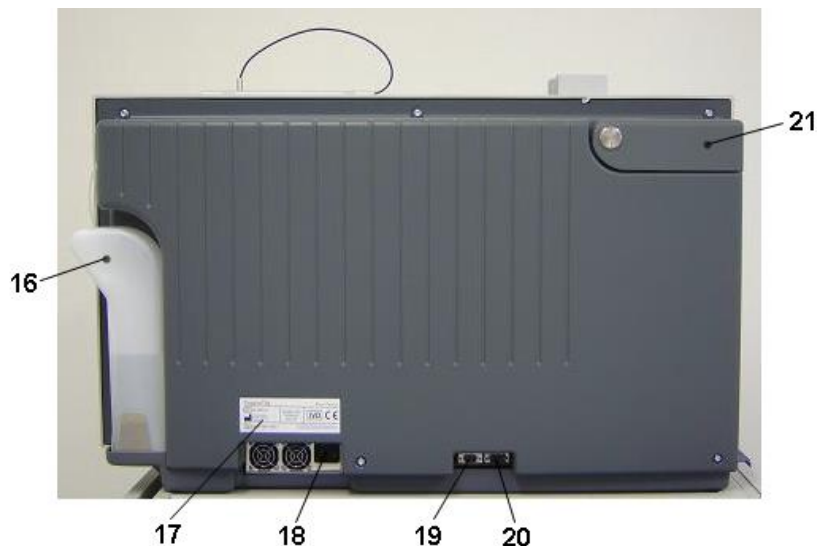

9.1.1 Bidirectional communication with TECAM software

TECAM software is a perfect and user friendly tool to combine laboratory data management, quality control and research purpose in one. The worklist management allows defining orders much faster and flexible then on the instrument itself. Powerful filter functions will help to create any report. Levey-Jennings graph and Westgard analysis are used for quality control monitoring. An ASTM interface is included, which allows to link with the laboratory information system (LIMS) over LAN network or RS232. The TECAM database can be saved central on a server and accessed simultaneously. This will allow to unify different Coatron analyser into one database.

Interface: 115200 Baud , no parity , 8 bit . 1 stop bit

Instrument port: location "19" – see picture above

Cable: 2x Female Sub D9, crosslink. Pin 2 to 3 ; Pin 3 to 2 and Pin 5 to 5. All other wires should be disconnected



Contact your local distributor for further information about TECAM software.

9.1.2 Unidirectional communication

Interface: 115200 Baud , no parity , 8 bit . 1 stop bit
 Instrument port: location "20" – see page 7
 Cable: 2x Female Sub D9, crosslink. Pin 2 to 3 ; Pin 3 to 2 and Pin 5 to 5. All other wires should be disconnected
 Handshake: No
 Establishing: Not required. The instrument sends results information automatically

Protocol & syntax: TECAM V5.30

STX	start of transmission	asc(2)	ETX	end of transmission	asc(3)
TAB	vertical tabulator	asc(9)	LF	line feed	asc(10)
CR	carriage return	asc(13)			

STX+TYPE | RID | STYP | SN | Kanal | Position | PID | LOT | Test-ID | Test-Name | Date | Time | status | result1 | scale1 | flag | result2 | scale2 | result3 | scale3 | progress|worklist-id|ETX

All fields are separated with vertical tabulator. No TAB is placed after STX or ETX !

STX: Start of Transmission
 Type: Always "R" = Result Record
 RID: Record ID. Unique record number
 SID: Analyser ID . Here always "1800"
 SN: Serial number of the analyzer
 Channel: optic channel 1-4. Here always "0".
 Position : Rack position of the sample tube (1 – 24). Here always "0".
 PID: Patient ID (max 13 characters)
 LOT: Lotnumber of the Reagent
 TEST-ID : ID Number of the Test (for ex. Test PT = 0 -> look at analyser's manual)
 TEST-Name: Name of the test, for example „PT“
 Date: Date of result. Always in format "yyyy/mm/dd".
 Date Time: Time of result. Always in format "hh:mm:ss"
 Status: Status of measuring „T“ = temperature error , „Q“ = Quality Control out of range, „%“ = big difference by double-measuring ; „A“ = abnormal ; „C“ = Control plasma; example: „TAQ%“ is possible
 Result1: Result of the standard scale (mostly sec);always in format „12.5“ ;
 Scale1: Scale of result1 ;ie. „s“ for second
 Flag: Information about the result2;
 „>“ „<“ Value smaller, bigger than ...
 „*“ result out of calibration
 „+“ no clotting detected
 „-“ clotting before dead time
 Result2: Result in the second scale ; f ex: in % : „100“
 Scale2: Scale of Result2 , ie. „%“
 Result3: Result in the third scale ; ie. INR : „1.23“
 Scale3: Scale of Result3 , ie. „INR“
 Progress: Progress of worklist. 0% = Start, 100%=End
 Worklist-ID Unique ID-number of current worklist
 ETX: End of Transmission
 CRLF: Carriage Return , LineFeed

9.2 Technical data

Analyzer	
Measurement system	4 independent measurement channels wavelength of LED 400 nm
Measurement timer	Max. 600 s, error < 0.1 s
Cuvette	4 channel cuvette for optical detection capacity: 150 – 1000 µl
Calibration	Automatic calibration or manual input of up to a max. of 6 calibration curve points for each test method
Positions	4 reagent positions at 36.5 – 37.5 °C 2 reagent positions at RT (~25°C) 6 reagent positions at 12.0 – 16.0°C 3 park positions, preheating (33-38°C) 2x12 sampe primary tubes 1 emergency STAT positions
Reaction volumes	Minimum total volume is 150 µl
Approvals	CE
XYZ Robotics	
Movement	X = 383mm, 1714 steps, v = 894mm/s Y = 150mm, 1054 steps, v = 569mm/s Z = 167mm, 3400 steps, v = 181mm/s
Level Sensor	Yes , capacity change detection with Aldium sensor
Neddle	-Capacity for 4880 µL -Inner hydrophob cermamic coating -Lifetime for 50000 determination
pump	1000 µl syringe with 1000 step resolution Lifetime of syringe is 250.000 cycles
imprecision	15% at 3µL 5% at 5µL 1% > 10µl

Barcode scanner

Laserclass 2 – EN60825-1:2007

max. power = 1.7 mW

pulse period = 420 µs

wavelength = 655 nm

Accepted codec

Code 39, Codabar, Interleaved 2 of 5,
Code 128 , EAN 128 and Code 93**Power supply**

Power input

85 – 264 VAC , Class-1 socket
at 45 – 60 Hz

Power consumption

Max. 250 VA

Approvals

EN 60950-1

UL 60950-1

IEC 60950-1

CSA 22.2 No. 60950-1

Dimensions

Size (W x D x H)

650 x 102 x 630 mm

Weight

approx. 55 kg (incl. packaging)

Size (W X D x H) on palette

650 x 1065 x 765 mm

Weight (with palette)

approx. 62 kg

Ambient conditions

Operating Temperature

15 – 30 °C, no direct sunlight

Storage and transport temperature

-20 to 60 °C

Humidity

Max. <70% rel. humidity, not
condensing

Elevation above NN sea level

0 – 3,000 m

Impact resistance

according to IEC/EN 61010-1, 8.2.2

Noise output

Operating noise

max. 65 dBA

Graphic user interface / software

Interface

RS 232 (serial interface) for commu-
nication with PC for software updates,
service functions, PC evaluation

LCD display

128 x 128 items, 70 x 70 mm

backlit, adjustable contrast

Language

German,English,Italian,Spanish

Specimen Collection

analyte	Fresh or frozen human plasma; Use within 4 hours
centrifugation	1500g x 10-15 min
anticoagulant	Sodium citrate 3.2% (0.105M)
	Mix 1 part citrate with 9 part venous blood
max. bilirubin concentration	25 mg/dL
max. hemoglobin concentration	1000 mg/L
max. triglyceride concentration	25 g/L

Typical performance data at system speed = high

Test	CV.	Range	Throughput
PT	<3%	0-30INR	108/h
APTT	<3%	15 – 420s	59/h
FIB	<7%	50-999mg/dL	65/h



Contact local distributor or manufacturer for detailed performance data (throughput, consumption, precision and accuracy).

9.3 Declaration of Conformity

 <p>Quality Management ISO 9001:2008 ▶ Voluntary participation in regular monitoring</p>			 <p>Quality Management EN ISO 13485:2003 + AC:2009 ▶ Voluntary participation in regular monitoring</p>
KONFORMITÄTSERKLÄRUNG DECLARATION OF CONFORMITY			
<p>Wir / We</p> <p style="text-align: center;">TECO Medical Instruments Production and Trading GmbH Name des Anbieters / Supplier's name Dieselstrasse 1, D-84088 Neufahrn NB Anschrift / Address</p>			
<p>erklären in alleiniger Verantwortung, dass das Produkt, <i>declare under our own responsibility, that the product,</i></p> <p style="text-align: center;">Coatron A4</p> <hr/> <p style="text-align: center;">Bezeichnung, Typ oder Modellname / name, type or model</p>			
<p>den Anforderungen der folgenden Richtlinien entspricht:</p> <p>1. Richtlinie 98/79/EG über In-vitro Diagnostika klassifiziert gemäß Artikel 9 als: "alle anderen Produkte" 2. Richtlinie 2004/108/EG über Elektromagnetische Verträglichkeit</p>		<p><i>corresponds to the requirements of:</i></p> <p>1. Directive 98/79/EC on In-vitro diagnostic medical devices classified according to article 9 as: "all other products" 2. Directive 2004/108/EC on electromagnetic Compatibility</p>	
<p>Zur Beurteilung der Konformität wurden u.a. folgende harmonisierte Normen herangezogen:</p> <p>1. Sicherheit: EN 61010-2-101:2002 Sicherheitsbestimmungen für elektrische Mess-, Steuer-, Regel- und Laborgeräte: Besondere Anforderungen an In-vitro-Diagnostik (IVD) Medizingeräte</p> <p>2. EMV: EN 61326-2-6:2006 Elektromagnetische Verträglichkeit – Anforderungen</p> <p>3. Risikomanagement: DIN EN ISO 14971:2012: Medizinprodukte – Anwendung des Risikomanagement auf Medizinprodukte</p> <p>4. Informationen: EN ISO 18113-3:2011: Bereitstellung von Informationen durch den Hersteller – Teil 3: Geräte für in-vitro-diagnostische Untersuchungen zum Gebrauch durch Fachpersonal</p>		<p>The following harmonized standards have been used amongst others:</p> <p>1. Safety: EN 61010-2-101:2002 Safety requirements for electrical equipment for measurement, control and laboratory use: Particular requirements for in-vitro diagnostic (IVD)</p> <p>2. EMC: EN 61326-2-6:2006 Electromagnetic compatibility – Requirements</p> <p>3. Risk management: DIN EN ISO 14971:2012: Medical devices – Application of risk management to medical devices</p> <p>4. Information: EN ISO 18113-3:2011: In vitro diagnostic medical devices – Information supplied by the manufacturer (labelling) – Part 3: In vitro diagnostic instruments for professional use</p>	
<p>Das QM-System des Herstellers ist zertifiziert durch DEKRA Certification, Stuttgart, nach: EN ISO 9001:2008 EN ISO 13485:2003+AC:2009</p>		<p>The QM-system of the manufacturer is certified from DEKRA Certification, Stuttgart, for: EN ISO 9001:2008 EN ISO 13485:2003+AC:2009</p>	
<p>Diese Erklärung bescheinigt die Übereinstimmung mit den genannten Harmonisierungsrechtsvorschriften, beinhaltet jedoch keine Zusicherung von Eigenschaften.</p>		<p><i>This declaration attests the accordance with the mentioned harmonization rule but does not include a warranty of quality.</i></p>	
<p>Ort und Datum der Unterzeichnung: Place and date of issue:</p>		<p>Gültig bis 01.04.2015 Valid until April 1st, 2015</p>	
<p>Neufahrn, 25.03.2014 Neufahrn, March 25th, 2014</p>  <p>Christian Högl General Manager</p>			

9.4 Disposal and recycling

Please comply with the following points when disposing of the COATRON A4:


- The housing is made of polystyrene.
- The mechanical parts are mainly aluminium.
- Electronic parts must be disposed of in accordance with currently valid regulations for their disposal.



Important!

You must disinfect the COATRON A4 prior to disposal to prevent cases of infection at the disposal company!

9.5 Barcode Guideline

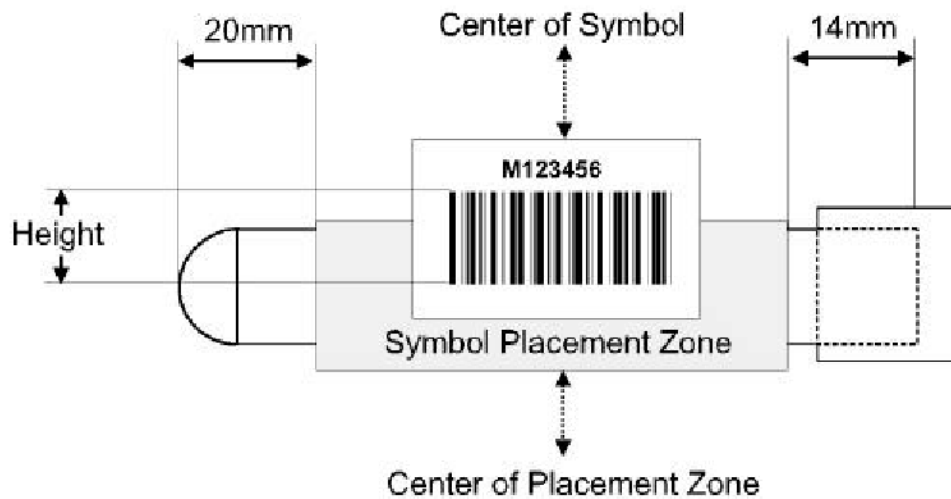

Specification of label:

- Label length: 50 – 70 mm
- Label height: 20 - 30 mm
- Barcode length: 40 – 60 mm
- Barcode height: 10 - 20 mm
- Quiet zone: >5mm
- Resolution/module: 8 -20mils (0.2 – 0.5mm)
- Ratio: min. 1:2,5 to 1:3 (two dimensional codes)
- Quality: Level A or B according to ANSI X3.192 -1990

Accepted codes:

- Code 128: 3 – 13 characters , use checksum without show
- EAN 128: 3 – 13 characters, use checksum without show
- Code 39: 4 – 13 characters, no checksum
- Code 93: 4 – 13 characters, no checksum
- 2/5 interleaved: 8 - 12 characters, no checksum

Index

+	
+++	50
A	
Activity	19
Adjust Motor.....	71, 78, 79, 80
Adjust XYZ.....	66
Administrator.....	70
Ambient conditions.....	85
Anticoagulant.....	86
Approvals	84
Arresting lever.....	75
Autoskip	33, 39
B	
Barcode.....	32, 39, 42, 52
Barcode scanner.....	85
BAT	40
Bilirubin	8, 18, 86
C	
Calibration	53, 84
Calibration,auto	56
Calibration,INR	55
Calibration,manual.....	54
Cap piercing.....	72
Centrifugation.....	86
Clean.....	40
Rinse Tank.....	69
CLEANING.....	76
Closed System	47, 48
Clotting	27
Conformity declaration	87
Contrast.....	62
Control measurement.....	8
CP-1.....	36, 41
CP-2.....	36, 41
Customer service	67, 68
CUV.....	40
Cuvette.....	69, 74, 84
Cuvette Activation	48
Cuvette rotor.....	20
Cuvette tower.....	20, 74
D	
Date	62
Decontamination.....	10, 76
DFIB	27
E	
Error messages.....	78
EVI.....	40
Expiry date.....	53
F	
Fibrinogen.....	18
Flag , summary	50
Flag ‘!’	50, 80
Flag ‘*’	50, 80
Flag ‘???’	80
Flag ‘+++’	80
Flag ‘A’	50, 57, 80
Flag ‘C’	36, 41, 50
Flag ‘E’	50, 80
Flag ‘F’	50, 80
Flag ‘K’	39, 50, 80
Flag ‘Q’	36, 50, 80
flag ‘R’	49
Flag ‘R’	50, 80
Flag ‘S’	80
Flag ‘SSS’	80
Flag ‘T’	50, 80
Flag ‘X’	50, 80
Front view	20
H	
Haematocrit.....	39
HC50, 51	
HCT-L.....	39
Hemoglobin	8, 18, 86
Host.....	25, 42, 51
I	
Immunoturbidimetric.....	28
Imprecision.....	84
Incubation time.....	53
Infection	9
Infectious Material	9
INR.....	19, 27
INR+	27
Intended Use	8
Interrupt worklist.....	33
Interruption.....	34
ISI 27	
K	
Keypad	7, 15, 24
Kinetic.....	28
L	
Language.....	62
Laser.....	9
Laserclass	85
Liquid waste tank	74
Lot No.	53
M	
Mains switch	21
Maintenance	76
Mean	39
Measurement principle.....	26
measurement screen	50
Measurement start	44
Mixer.....	63
mOD.....	50
N	
Needle	69
Normal range.....	57
O	
Optic.....	26, 68
ORDER.....	42
Out of cuvette.....	33
Out of liquid	33

P	
PID.....	39, 41, 42
PIPET STATION.....	73
Pipetting arm.....	8, 20
Pipetting needle.....	70
P-Offset.....	72
Precision.....	40
PRFL.....	41
Print out.....	51, 58, 59, 65
Protective bar.....	20
Pump.....	20
Q	
QC 40.....	
QC-Active.....	36
Quality control.....	19, 36, 39
Quality control range.....	57, 58
R	
Ratio.....	19
Reagent activation.....	48
Reagent block.....	20
Reagent position.....	66
Rear view.....	21
reflex testing.....	49
Reflex Testing.....	39
Report of all tests.....	59
Report of result.....	51
Report of system.....	65
Report of test.....	58
reproducibility.....	79
Robot.....	69
RS232.....	21
Rubber roll.....	75
Runtime.....	53
S	
Safety information.....	8, 9, 10
Sample rack.....	20, 22, 31
Sample test tubes.....	31
Scope of delivery.....	12
Screen.....	20, 25
SEL.....	40
Serial-No.....	81
Setup System.....	62
Shield.....	40
Side view.....	22
Signal.....	62
Simulator.....	63
Single factor measurements.....	18
SKP.....	39, 50, 80
Software.....	26
Software Update.....	21
SSS.....	50
Standby-switch.....	16
STAT.....	35, 44
Switching off.....	14, 15
Symbols.....	7
SYNCHRONIZE.....	42
Syringe.....	20, 71
System Activation.....	47
System block.....	20
System status.....	25
T	
Tank.....	69
Tecam.....	21, 36, 51
TECAM.....	17
Test overview.....	29
test procedure.....	59
test protocols.....	59
Thermal printer paper.....	75
Thrombin.....	27
Thrombin Time.....	18
Throughput.....	40, 72
Time.....	62
Transmission.....	26
Transport.....	81
<i>Triglyceride</i>	8
Tube system.....	20
Type plate.....	21, 81
U	
Units.....	26
W	
Warm-up time.....	15
Wavelength.....	84
Work list.....	39
Working Positions.....	23
Worklist-ID.....	51
X	
XXX.....	50

**Utilizare**

Acest produs este utilizat pentru determinarea timpului de protrombină (PT) în plasmă, conform Quick^{1,2}. Testul este sensibil la activitatea factorilor de coagulare implicați pe calea “extrinsecă”, și anume: II, V, VII, X și fibrinogen și prin urmare este utilizat pentru terapie anticoagulantă orală cu inhibitori ai Vitaminei-K precum Warfarin sau Marcumar. De asemenea, se utilizează și pentru determinarea cantitativă a factorilor de coagulare implicați pe calea “extrinsecă”. PT-ul măsoară timpul de coagulare extrinsecă (activarea factorului VII) a plazmei de testare după adăugarea reagentului PT.

Continut și Determinări

Product	TECLOT PT-S	TECLOT PT-S	TECLOT PT-S
Cat.No.	A0230-010	A0230-040	A0230-100
PT-S Reagent*	5x2 mL	10x4 mL	10x10 mL

Determinări

Coatron M**	200 Det.	800 Det.	2000 Det.
Coatron A4	100 Det.	400 Det.	1000 Det.
Coatron A6	200 Det.	800 Det.	2000 Det.

*conține un extract din creier de iepure cu Buffer, stabilizatori și Clorură de Calciu.

**Metoda micro (75μl în total)

Preparare

Reconstituiți cu apă de înaltă puritate cu volumul indicat pe eticheta flaconului

A0230-010	A0230-040	A0230-100
2 mL	4 mL	10 mL

Lăsați la temperatura camerei pentru cel puțin 15 minute cu învârtiri/rotiri ocazionale. Plasați reagentul în aparat și lăsați să se incubeze pentru încă 15 minute. Reactivul sedimentează și trebuie învârtit/rotit înainte de fiecare testare. La aparatele Coatron puteți utiliza o bară de amestecare pentru asta.

Păstrare și Stabilitate

Reagenții nedesfăcuți și păstrați între 2^o-8^oC, sunt stabili pînă la data expirării indicate pe ambalaj. Reagenții deschiși deja, sunt stabili :

	2 ^o -8 ^o C	20-25 ^o C	37 ^o C
PT reagent	5 zile	36 ore	8 ore

Măsuri de precauție

Evitați contactul cu pielea și ochii. Purtați haine de protecție adecvate. Eliminați componentele în conformitate cu reglementările locale pentru materialele infecțioase. Toate componentele sunt verificate pentru HIV, VHB, VHC. Cu toate acestea, produsele din sângele uman ar trebui considerate potențial infecțioase.

Colectarea și depozitarea probei ⁴

1. Obțineți sângele venos prin puncție curată a venei.
2. Amestecați imediat 9 părți de sânge cu 1 parte de 3,2% de Citrat de Na (0.105M) și amestecați bine.
3. Centrifugați specimenul la 1500g pentru 10 min (trombocite < 10000/ μ L).
4. Separați plazma după centrifugare și depozitați în tuburi de sticlă siliconizată.
5. Utilizați plazma în timp de 4 ore sau înghețați și dezghețați doar înainte de utilizare.

Stabilitatea plazmei: 4 ore la 18-26°C, 8 ore la 2-8°, 30 zile la -20°C, 6 luni la -70°C

Procedura

A. Metoda automată: Coatron A

Prothrombin Time		A4		A6			A4	A6		A4	A6
PAT	Patient	50 μ l	CP1	25 μ l	CP1	Incubation	0s		SENS	2	
BUF	IBS Buffer	0 μ l	P39	0 μ l	P79	Maxtime	120s		POINTS	4	
CLR	-	0 μ l	-	0 μ l	-	Unit	251		MIX	No	
DP	-	0 μ l	P00	0 μ l	P00	Method	Coag		Clean	0	0
R0	-	0 μ l	P00	0 μ l	P00	Math	log XY		Multi	1	3
R1	-	0 μ l	P00	0 μ l	P00	CT-Mech	No		S-Corr	0%	
R2	PT Reagent	100 μ l	P25	50 μ l	P46	Deadtime	7s		T-Corr	30% - 4s	

B. Metoda manuală:

1. Incubați reagentul PT la 37°C pentru cel puțin 10 minute
2. Pipetați **25 μ l** din specimen în cuveta pentru testare. Incubați la 37°C pentru 1-2 min
3. Adăugați **50 μ l** de reagent PT (37°C) și începeți simultan testul.
4. Înregistrați/măsurați în secunde timpul de coagulare.

Rezultate așteptate

Secunde tipice : 11-18 sec

Intervalul normal: 70 - 130% 0.85 – 1.15 INR

Oricum, rezultatele sunt influențate de aparate, tehnică, calibrare etc. Se recomandă ca fiecare laborator să-și stabilească propriul interval, specific aparatelor utilizate.

Standardizare și Calibrare

Rezultatul PT este exprimat în secunde sau activitate (% Quick) sau INR (International Normalised Ratio).

Rezultatele INR:

-au fost calculate din timpul normal și valoarea ISI (international sensitivity index/ indicele internațional de sensibilitate). Primul este obținut prin testarea plazmei proaspete a unui grup de indivizi sănătoși. Valoarea ISI este stabilită în certificatul de analiză specific fiecărui lot.

$$INR = \left(\frac{\text{Patient PT}}{\text{Normal PT}} \right)^{ISI}$$

Rezultatele % activității (Quick):

-au fost calculate dintr-o curbă de calibrare, care a fost pregătită după plasma de referință (e.g. **TECAL N**) și diluări în soluții saline ca 0.9% de NaCl2 sau TECLOT IBS buffer. Sunt recomandate cel puțin 3 sau mai multe puncte de calibrare . Curba de calibrare trebuie confirmată cu plasma de control cu interval normal și patologic.

% din normal diluat în soluție salină	100%*	50%	25%	12,5%**
	Fără diluție	1+1	1+3	1+7

*media de la cel puțin 21 de indivizi sănătoși este definită ca 100%⁵

**diluția de 12.5% poate cauza rezultate “+++” în unele cazuri, pentru că nivelul de diluție al fibrinogenului este prea mare pentru detecție optică.

Controlul Calității

TEControl sau altă plasmă de control comercială trebuie utilizată pentru controlul calității performanței la o frecvență în conformitate cu practicile bune de laborator (GLP). TEControl poate fi înghețat o singură dată după reconstituire. 120-150 μl păstrat închis în tuburi de polipropilen la -20°C , este stabil timp de 30 zile.

Restricții/ Limitări

O mare grijă și atenție trebuie de avut la factorii care pot părea ne semnificativi.

A. Colectarea probei. Evitați:

1. Folosiți doar tuburi de plastic sau sticlă siliconizată.
2. Amestecarea întârziată a sîngelui cu anticoagulant.
3. Contaminarea cu tromboplastină tisulară.
4. Raportul greșit de sînge cu anticoagulant.
5. Probele hemolizate, icterice sau lipemice pot interfera sistemele optice.

B. Tehnici de Laborator:

1. Efectuați testul la 37°C.
2. Utilizați doar apă cu puritate înaltă.
3. pH-ul optim este 7.0-7.5.
4. Valoarea ISI nu e constantă în primile 30 min după reconstituire.
5. Reagentul face sedimente , de aceea trebuie de agitat înainte de fiecare testare.

Caracteristici de performanță

Performanțe tipice pe aparatul Coatron M4:

Precision:	CV% (în timpul testării)	CV% (între testări)
Normal control	< 3,0	< 5,0
Abnormal control	< 3,0	< 5,0













Garantie

Acest produs este garantat doar dacă se utilizează în conformitate cu informațiile de pe eticheta proprie și din instrucțiune. TECO nu acordă garanție dacă produsul este utilizat în alt scop și în niciun caz TECO nu va fi răspunzător pentru daunele care rezultă din garanția expresă menționată mai sus.

Referințe:

1. Quick, A.J., The Hemorrhagic Diseases and the Physiology of Hemostasis. Charles C. Thomas: Springfield, IL. 1942.
2. Quick, A.J., Hemorrhagic Diseases. Lea and Febiger: Philadelphia. 1957.
3. Miale, J.B., Laboratory Medicine-Hematology, 4th Edition. C.V. Mosby: St. Louis. 1972.
4. National Committee for Clinical Laboratory Standards: Guidelines for the Standardized Collection, Transport and Preparation of Blood Specimens for Coagulation Testing and Performance of Coagulation Assays.
5. Besselaar A M H P van den, Lewis SM, Mannucci P n Poller L. 1993. Status of present and candidate International Reference Preparations (IRP) of thromboplastin for prothrombin time. Thromb Hemostas 69; 85
6. Besselaar A M H P van den. 1991. The significance of the International Normalized Ratio (INR) for oral anticoagulant therapy. H17CC 3; 146153.

Symbol keys

 Expiry date	 In Vitro Diagnostica	 Biological hazard	 Catalogue Number	 Reconstitute with dest. water	 Consult accompanying documents
 Store at 2-8°C	 EU conformity	 Manufacturer	 Lot. Number	 Ready to use	 Authorized Representative



IVD

REF

A0501-010, A0501-025, A0511-020, A0511-050

Utilizare

TECLOT FIB este utilizat pentru determinarea cantitativă a fibrinogenului în plasma umană, conform tehnicii dezvoltată de Clauss¹. Nivelul de fibrinogen poate crește ca rezultat al inflamației, sarcinii sau utilizarea contraceptivelor orale². Nivelul scăzut de fibrinogen poate fi identificat în situații concrete precum boli de ficat sau DIC (Coagulare intravasculară diseminată). Deficiențele congenitale includ afibrinogenaemia (nici un fibrinogen detectabil), hypofibrinogenaemia (<1 mg/ml) și dysfibrinogenaemia (molecula anormală de fibrinogen).

Continut și preparare

Product	TECLOT FIB Kit-10	TECLOT FIB Kit-25	TECLOT FIB	TECLOT FIB
Cat.No.	A0501-010	A0501-025	A0511-020	A0511-050
Reactivul de trombină	5x2 mL	5x5 mL	10x2 mL	10x5 mL
IBS Buffer	1x125 mL	1x125 mL	-	-
TECal Normal	1x1 mL	1x1 mL	-	-
TEControl A	1x1 mL	1x1 mL	-	-

Determinări

Coatron M*	400 Det.	1000 Det.	800 Det.	2000 Det.
Coatron A4	200 Det.	500 Det.	400 Det.	1000 Det.
Coatron A6	200 Det.	500 Det.	400 Det.	1000

*Metoda micro (75μL în total)

1. Reactivul de trombină:
Conține trombină de bovină (~80NIH) cu stabilizatori.
REF: A0501-010/A0511-020: reconstituiți cu 2 ml de apă purificată.
REF: A0501-025/A0511-050: reconstituiți cu 5 ml de apă purificată.
2. IBS Buffer: Gata de utilizare. Conține soluție salină tamponată Imidazol.
3. TECal Normal: reconstituiți cu 1 ml de apă purificată. Conține plasma umană citrată.
4. TEControl A: reconstituiți cu 1 ml de apă purificată. Conține plasma umană citrată.



Rotiți ușor după reconstituire și lăsați timp de 15 minute la temperatura camerei. Amestecați bine înainte de utilizare. Nu agitați/ scuturați.

Păstrare și stabilitate

Reagenții care nu au fost deschiși sunt stabili pînă la data expirării indicate pe ambalaj, păstrați la temperatura de 2°-8°C. Reagenții deschiși deja se păstrează:

Reactivul de trombină*	2-8 °C	15-25 °C	37 °C
	12 zile	5 zile	24 ore
TEControl sau Plasma	2-8 °C	15-25 °C	-20 °C
	8 ore	4 ore	30 zile

*Reactivul trebuie de protejat razele ultraviolete și evaporare.

Măsuri de precauție

Evitați contactul cu pielea și ochii. Purtați haine de protecție adecvate. Eliminați componentele în conformitate cu reglementările locale pentru materialele infecțioase. Toate componentele sunt verificate pentru HIV, HBV, HCV. Cu toate acestea, produsele din sângele uman ar trebui considerate potențial infecțioase.

Colectarea și păstrarea probelor³

1. Obțineți sânge venos printr-o puncție curată a venei.
2. Amestecați imediat 9 părți de sânge cu 1 parte de 3.2% sodium citrate (0.105M) și amestecați bine.
3. Centrifugați proba la 1500g timp de 10 minute (trombocite < 10000/μL).
4. Separați plasma după centrifugare și păstrați în plastic sau tuburi de sticlă siliconată.
5. Folosiți plasma în timp de 4 ore sau depozitați/păstrați înghețat și dezghețați numai înainte de folosire.

Procedura

A. Metoda automată Coatron A

Fibrinogen		A4		A6			A4	A6		A4	A6
PAT	Patient	10μl	CP1	10μl	CP1	Incubation	0s		SENS	0	
BUF	IBS Buffer	90μl	P39	90μl	P79	Maxtime	120s		POINTS	4	
CLR	-	0μl	-	0μl	-	Unit	769		MIX	No	
DP	-	0μl	P00	0μl	P00	Method	Coag		Clean	1	3
R0	-	0μl	P00	0μl	P00	Math	log XY		Multi	1	1
R1	-	0μl	P00	0μl	P00	CT-Mech	Yes		S-Corr	0%	
R2	Fibrinogen	50μl	P29	50μl	P49	Deadtime	3s		T-Corr	0%	

B. Metoda manuală Coatron M

1. Prepararea diluțiilor pentru Standard, Control și Pacient.

Diluția Standard	Plazma	IBS Buffer
1:5	200μL Standard	800μL
1:10	500μL 1:5 STD	500μL
1:20	500μL 1:10 STD	500μL
1:40	500μL 1:20 STD	500μL
Pacient sau Control	100μL Plasma	900μL

2. Pipetați 50 μl de standard diluat sau plasma pacientului (1:10) într-o cuvetă pentru testare. Preîncălziți la 37°C timp de 1-2 minute.
3. Adăugați 25 μl de reactiv de trombină și simultan începeți testul.
Pentru alte aparate, consultați manualul cu instrucțiuni specifice mai detaliate.

Calibrare

Ca referință trebuie de utilizat TECal Normal sau altă Plasma standard comercială preparată în care fibrinogenul a fost determinat. (200-300mg/dL). Reprezintă grafic timpul de coagulare obținut cu fiecare din diluțiile standard ale fibrinogenului pe axa-y , opus concentrației de fibrinogen (mg/dL) pe axa-x utilizând hîrtia grafică log-log. Linia cea mai potrivită trebuie de determinat prin analiza regresiei liniare. Fibrinogenul din probele de plasmă poate fi determinat prin interpolare din curba de calibrare.

Rezultate asteptate

Rezultatele normale tipice sunt 180-450 mg/dL^{4,5}. Oricum , rezultatele sunt influențate de metoda de detecție a coagulării și poate varia de la laborator la laborator. Este recomandat ca fiecare laborator să-și stabilească propriul interval normal specific aparatului utilizat.

Controlul Calității

Pentru un control de încredere al calității performanței , trebuie utilizată TEControl sau altă plasmă de control comercială la o frecvență în conformitate cu practicile bune de laborator (GLP). TEControl poate fi înghețat o singură dată după reconstituire. 120-150 μl păstrat închis în tuburi de polipropilen la -20°C , este stabil timp de 30 zile.

Limitări / Restricții

A. Colectarea probei.EVITAȚI:

1. Folosiți doar tuburi de plastic sau sticlă siliconizată.
2. Întîrzierea amestecării sîngelui cu anticoagulant.
3. Contaminarea cu tromboplastină tisulară.
4. Raportul greșit dintre sînge și anticoagulant.
5. Probele hemolizate, icterice sau lipemice pot interfera sistemele optice.

B . Tehnici de Laborator:

1. Efectuați testul la 37°C.
2. Utilizați doar apă cu puritate înaltă.
3. pH-ul optim este 7.0-7.5.

Caracteristici de performanță:

Precizia	CV%(în timpul testării)	CV%(între testări)
Normal control	< 5.0	< 5.0
Abnormal control	< 5.0	< 10.0

(Performanțe tipice pentru aparatul Coatron M4)

Garantie

Acest produs este garantat doar dacă se utilizează în conformitate cu informațiile de pe eticheta proprie și din instrucțiune. TECO nu acordă garanție dacă produsul este utilizat în alt scop și în niciun caz TECO nu va fi răspunzător pentru daunele care rezultă din garanția expresă menționată mai sus.

Referinte

1. Clauss, A., Gerinnungsphysiologische Schnellmethode zur bestimmung des Fibrinogens. Acta Haematol., 1957, 17: 237-246.
2. Shaw, T.S., Assays for Fibrinogen and its Derivatives, CRC Crit. Rev. Clin. Lab. Sci., 1977, 8: 145-192.
3. National Committee for the National Laboratory (NCCLS) Standards: Collection transport and preparation of blood specimens for coagulation testing and performance of coagulation assays. Document H21-A2, vol. 11, No. 23, 1991.
4. Scully, R.E. et al., Normal Reference Laboratory Values, N. Eng. J. Med., 1980, 302(37) : 37-48.
5. Okuno, T. and Selenko, V., Amer. J. Med. Tech., 1972, 38(6) : 196-201.

Symbols key:

 Expiry date	 In Vitro Diagnostica	 Biological hazard	 Catalogue Number	 Consult accompanying documents
 Store at 2-8°C	 EU conformity	 Manufacturer	 Lot. Number	 Authorized Representative



IVD

REF

A0590-125

Intended Use

The IBS Buffer solution is optimally formulated for use on Coagulation Analyzers. Use in accordance with the recommended Operators Manuals for installing and replacing Owrens Veronal Buffer (OVB). The IBS can be used as the diluent for preparing plasma dilutions in the performance of Fibrinogen determinations and Coagulation Factor Assays with all manual, mechanical, or photo-optical means of clot detection. Follow Reagent manufacturer's recommended procedures for preparation of plasma dilutions using Imidazole Buffered Saline.

Contents & Determinations

Product	IBS Buffer
Cat.No.	A0590-125
IBS Buffer	1x125 mL

Preparation

IBS: pH 7.3 - 7.4, liquid
Ready to use.

Storage and Stability

Unopened reagents are stable until the expiration date shown on the label stored at 2-8°C.

Precautions

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material.

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative



A0590-125

Verwendungszweck

Die IBS Pufferlösung (Imidazole Buffered Saline) wird für die Verdünnung von Plasma verwendet werden, wie es z.B. bei der koagulometrischen Bestimmung von Fibrinogen, Einzelfaktoren oder auch Verdünnungsreihen für die Methoden Kalibrierung notwendig ist.

Inhalte und Bestimmungen

Produkt	IBS Puffer
Kat.Nr.	A0590-125
IBS Buffer	1x125 mL

Vorbereitung

IBS: pH 7.3 - 7.4, flüssig
Gebrauchsfertig

Lagerung und Stabilität

Ungeöffnete Reagenzien sind bei Lagerung zwischen 2-8°C bis zum auf dem Etikett angegebenen Verfallsdatum haltbar.

Vorsichtsmaßnahmen

Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Bestandteile gemäß lokaler Vorschriften für infektiöse Materialien entsorgen.

Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produktes den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Verkäuflichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter

21 500 01 / 21 500 00 / 21 500 09

Rinse Solution / Clean B

TECO

Information of Use

This solution is a general laboratory article for a wide range of uses in laboratories. It is also suitable for use in in vitro diagnostic tests.

The Solution is ready for use.

It can be applied with fully automated Coagulation analyser systems to operate the pump system.

The Solution in unopened tanks should not be applied to Coagulation Analysers beyond the expiry date indicated on the label. Avoid freezing, optimal storage temperature is (18 to 25°C). Opened tanks should be consumed within max. 3 years.

Units / consumption

Cat.No.	21 500 01	21 500 00	21 500 09
Content	1 x 1,25 L	3 x 1,25 L	9 x 1,25 L

Precautions and Waste information

The Solution should be used once only.

Ingredients: Laboratory water pH 7.0 ($\pm 1,0$ at 37 °C ± 1 °C)

Collected used solution should be disposed as prescribed in local regulations. No further precautions.

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Packaging Material, Dim.

Carton (3): (mm) L310 x W250 x H140

Carton (9): (mm) L310 x W250 x H330

PP (Tank): (mm) L110 x W300 x H80


Tank with Screwcap (PP) with inner PE Foil.

Tank additionally sealed with aluminium Foil.



Product picture (exemplary)



Placement of Label

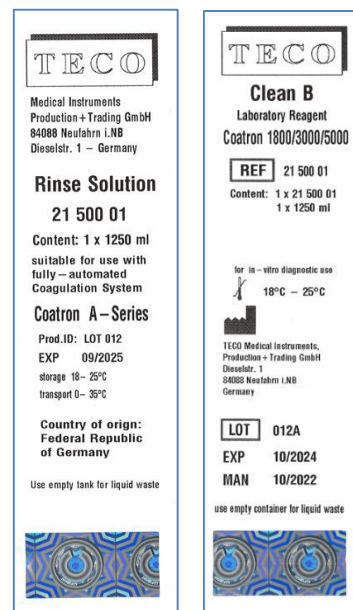

Label Artwork (with Hologram)

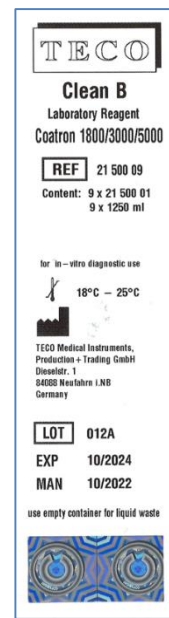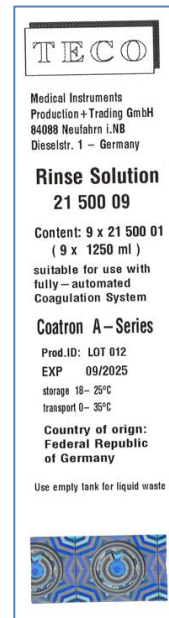

outer Packaging:



21 500 01 / 21 500 00 / 21 500 09

Rinse Solution / Clean B

TECO

Gebrauchsinformation

Die Lösung als allgemeiner Laborartikel für ein breites Spektrum von Anwendungen in Laboratorien eignet sich auch für den Einsatz bei in-vitro-diagnostischen Tests.

Die Lösung ist gebrauchsfertig. Sie kann mit voll-automatischen Gerinnungsanalysesystemen zum Betrieb des Pumpensystems verwendet werden.

Spüllösung in ungeöffneten Behältern sollte nach Ablauf des auf dem Etikett angegebenen Verfalls-datum nicht mehr in Gerinnungsanalysegeräten verwendet werden. Die Lagertemperatur sollte (-18-25°C) betragen. Geöffnete Tanks sollten innerhalb von max. 3 Jahren verwendet werden.

Verkaufeinheiten

Kat.No.	21 500 01	21 500 00	21 500 09
Inhalt	1 x 1,25 L	3 x 1,25 L	9 x 1,25 L

Vorsichtsmassnahmen und Entsorgungshinweise

Die Lösung sollte nur einmal verwendet werden.
Bestandteile: Laborwasser pH 7,0 (± 1,0 bei 37 °C ± 1 °C)
Aufgefangene gebrauchte Lösung sollte gemäß den örtlichen Vorschriften entsorgt werden. Keine weiteren Vorsichtsmaßnahmen.



Gewährleistung

Für dieses Produkt wird garantiert, dass es in Übereinstimmung mit den Angaben auf dem Etikett und in der Literatur funktioniert. TECO lehnt jede stillschweigende Garantie für die Marktgängigkeit oder die Eignung für einen anderen Zweck ab, und TECO haftet in keinem Fall für Folgeschäden, die sich aus der oben genannten ausdrücklichen Garantie ergeben.

Verpackung



Karton (3): (mm) L310 x W250 x H140
Karton (9): (mm) L310 x W250 x H330
Tank (PP): (mm) L110 x W300 x H80
Tank mit Schraubdeckel PP Schaumfolie innen PE.
Tank zusätzlich versiegelt mit Aluminiumfolie

Produktbilder (exemplarisch)

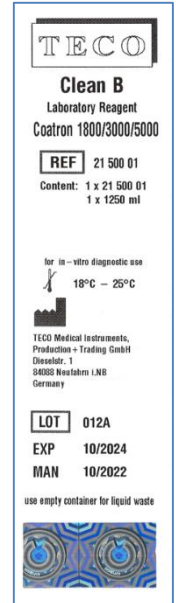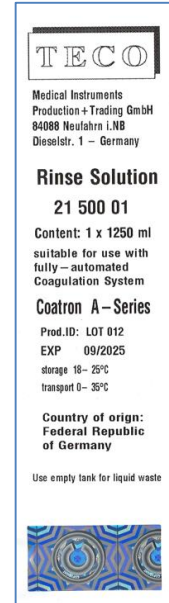

Platzierung

Label Layout (mit Hologramm)

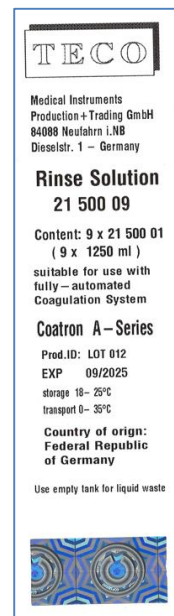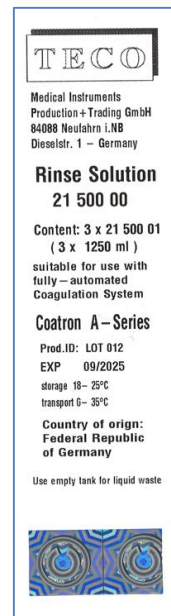

Umverpackung



21 510 00

Clean Solution / Clean A

TECO

Information of Use

The Clean Solution (Clean A) is intended as a general laboratory article for a wide range of uses in laboratories. It is also suitable for use in automatically coagulation analysers which are used for in vitro diagnostics tests.

TECO recommend it to remove any residues from needle probe on following TECO instruments: **Coatron A4, Coatron A6, Coatron A6 Plus: Coatron 1800 / 3000 / 5000.**

Contents & Composition

Product	Clean Solution (Clean A)
Cat.No.	21 510 00
Content	1 x 500 ml

Ingredients: 99,6% acidic solution (pH 1.1±0.5) with detergent (slight foaming); generally no hazardous to water.

Preparation and waste information

Ready to use. The solution should be used once only.

Storage and

Avoid freezing, best storage temperature (~18 – 25°C)

Stability

See individual Expiry date on each box.

Precautions

General laboratory safety measures for use of chemical solutions. Avoid direct contact with eyes and skin.

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Product picture (example)



Clean Solution
(both with Hologram)



Clean A

Outer Package

no specific outer package of single unit
Shipping within total packaging

Safety data sheet: sds-id.com/100202-6

Symbols key (if applicable):

 Temperature	 Manufacturer	LOT LOT Number	REF Catalogue Number
---	--	-----------------------	-----------------------------



IVD

REF

P6001-010

Intended Use

Use as a normal control for following coagulation tests:

**PT, APTT, Thrombin time, Fibrinogen,
Anti-thrombin and D-Dimer**

Contents

10 x 1mL freeze dried citrate-anticoagulated human plasma

Preparation

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

Storage & Stability

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C
1 month	8 hours	4 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

Precautions

This product contains substance from human origin!
Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

Expected Results

Refer to "Certificate of Analysis".

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative





P6001-010

Verwendungszweck

Als normale Kontrolle für folgende Gerinnungstests verwenden:

**PT, APTT, Thrombinzeit, Fibrinogen,
Antiithrombin und D-Dimer**

Inhalt

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

Vorbereitung

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TEClot PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

Lagerung und Stabilität

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C
1 Monat	8 Stunden	4 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

Vorsichtsmaßnahmen

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.

Erwartete Ergebnisse

Lesen Sie das Analysenzertifikat

Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Verkäuflichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter





IVD

REF

P6101-010

Intended Use

Use as an abnormal control for following coagulation tests:

**PT, APTT, Thrombin time, Fibrinogen,
Antithrombin and D-Dimer**

Contents

10 x 1mL freeze dried citrate-anticoagulated human plasma

Preparation

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

Storage & Stability

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C
1 month	8 hours	4 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

Precautions

This product contains substance from human origin!
Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

Expected Results

Refer to "Certificate of Analysis".

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative





P6101-010

Verwendungszweck

Als abnormale Kontrolle für folgende Gerinnungstests verwenden:

**PT, APTT, Thrombinzeit, Fibrinogen,
Antithrombin und D-Dimer**

Inhalt

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

Vorbereitung

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TEClot PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

Lagerung und Stabilität

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C
1 Monat	8 Stunden	4 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

Vorsichtsmaßnahmen

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.

Erwartete Ergebnisse

Lesen Sie das Analysenzertifikat

Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Verkäuflichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter

