

VIEWWORKS

VIVIX-S 3643VW Specifications



CE 2460

© Vieworks. 2020 All rights reserved.

The specifications and related information in this manual may be changed without notice. Refer to Vieworks Download System (VDS) for the latest version of manuals.

Under copyright laws, this manual should not be reproduced, in whole or in part, without the written permission of Vieworks.

Contents

1. Instruction	3
1.1 Document Guide	3
1.1.1 Target.....	3
1.1.2 Symbols.....	3
1.1.3 Notations.....	3
1.2 Revision History	3
1.3 Contact Us	3
2. Products	4
2.1 Detector	4
2.1.1 Specifications.....	4
2.1.2 Drawing Sheet.....	5
2.1.3 Functions	6
2.1.4 Use Environment.....	8
2.2 Battery Pack	8
2.2.1 Specifications.....	8
3. Performance	9
3.1 FXRD-3643VAW	9
3.2 FXRD-3643VAW PLUS	10
4. Defect	11
4.1 Defect Type	11
4.2 Defect Allowance	11
5. Regulatory Information	12
5.1 Medical Equipment Classification	12
5.2 Product Safety Standard	12

1. Instruction

1.1 Document Guide

1.1.1 Target

This document is intended for customers who use the **VIVIX-S 3643VW** detector.

1.1.2 Symbols

This product should be operated under the safety instructions with the warning or caution symbol in this manual. It is important for you to read and understand the contents to operate the products safely.

Caution and Warning



- This symbol is used to indicate a potentially hazardous situation that may cause death, personal injury or substantial property damage if the instructions are ignored. Users should be well acquainted with this symbol and the related contents.

Information



- This symbol is used for indicating product related references and supplementary information. Users are recommended to read the sentences with this notice carefully.

1.1.3 Notations

Bold Types

Words in bold indicate products terms, or the sentences which are needed to transmit clear meaning to the customers.

1.2 Revision History

Ver.	Date	Descriptions
1.0	2020-03-06	Initial Release

1.3 Contact Us

For any comments or inquiries regarding this document and relevant products, contact via email below.

Item	Contents
Department	Customer Support Team at Vieworks
E-mail	CustomerSupport@vieworks.com

2. Products

2.1 Detector


2.1.1 Specifications

Item	Specifications
Model	<ul style="list-style-type: none"> FXRD-3643VAW / FXRD-3643VAW PLUS
Image Sensor	<ul style="list-style-type: none"> TFT: a-Si (Amorphous Silicon)
X-ray Scintillator type	<ul style="list-style-type: none"> FXRD-3643VAW: CsI type A FXRD-3643VAW PLUS: CsI type B
Pixel Pitch	<ul style="list-style-type: none"> 0.14mm (140μm)
Field of View	<ul style="list-style-type: none"> 36cm x 43cm (14" x 17")
Active Area (H x V)	<ul style="list-style-type: none"> 358.4mm x 430.08mm
Active Array	<ul style="list-style-type: none"> 2560 x 3072 pixels
Effective Area	<ul style="list-style-type: none"> 355.04mm x 426.72mm
Effective Array	<ul style="list-style-type: none"> 2536 x 3048 pixels
Grayscale	<ul style="list-style-type: none"> 16 bit
Spatial Resolution	<ul style="list-style-type: none"> Min. 3.5 lp/mm
Image Acquisition Time (Wired)	<ul style="list-style-type: none"> Max. 3 sec. (Exposure time is set to 500ms, Excluding exposure time)
Image Acquisition Time (Wireless)	<ul style="list-style-type: none"> Max. 3 sec. (IEEE802.11ac, MiMO 3x3, 5GHz, 80MHz) (Exposure time is set to 500ms, Excluding exposure time)
Capacity for Image Backup	<ul style="list-style-type: none"> Max. 200 images
Cycle Time	<ul style="list-style-type: none"> Min. 4 sec. (Optimal wired/wireless environment, Exposure time is set to 500ms, Image processing time of software is not included)
X-ray Synchronization Control	<ul style="list-style-type: none"> AED (Auto Exposure Detection) DR Trigger (External line trigger)
Rated Power Supply	<ul style="list-style-type: none"> DC 24V, Max. 1A powered by SCU with a tether interface cable. DC 18V, Max. 4.44A powered by AC-DC Adaptor DC 9~13.2V, Max. 78.54Wh powered by two battery packs
Power Consumption	<ul style="list-style-type: none"> Max. 24W (without battery charged) Max. 80W (when charging battery)
Operating Time (Early life of battery)	<ul style="list-style-type: none"> One battery pack <ul style="list-style-type: none"> 7.5 hours (image acquired every 100 seconds) 8 hours (standby) Two battery packs <ul style="list-style-type: none"> 15 hours (image acquired every 100 seconds) 16 hours (standby)
Dimensions (H x W x D)	<ul style="list-style-type: none"> 384mm x 460mm x 15.0mm

Weight	<ul style="list-style-type: none"> • FXRD-3643VAW <ul style="list-style-type: none"> ▫ With a battery pack : 2.95kg ▫ With two battery packs : 3.15kg • FXRD-3643VAW PLUS <ul style="list-style-type: none"> ▫ With a battery pack : 3.1kg ▫ With two battery packs : 3.3kg
	<ul style="list-style-type: none"> • Wired: Gigabit Ethernet(1000BASE-T) via PoE(Power over Ethernet) • Wireless: IEEE802.11n/ac (2.4GHz/5GHz), 3 antennas
	<ul style="list-style-type: none"> • Max. 1Gbps
	<ul style="list-style-type: none"> • Max. 300Mbps (IEEE802.11n, MIMO 2x2, 5GHz, 40MHz) • Max. 1300Mbps (IEEE802.11ac, MIMO 3x3, 5GHz, 80MHz)

2.1.2 Drawing Sheet

FXRD-3643VAW / FXRD-3643VAW PLUS

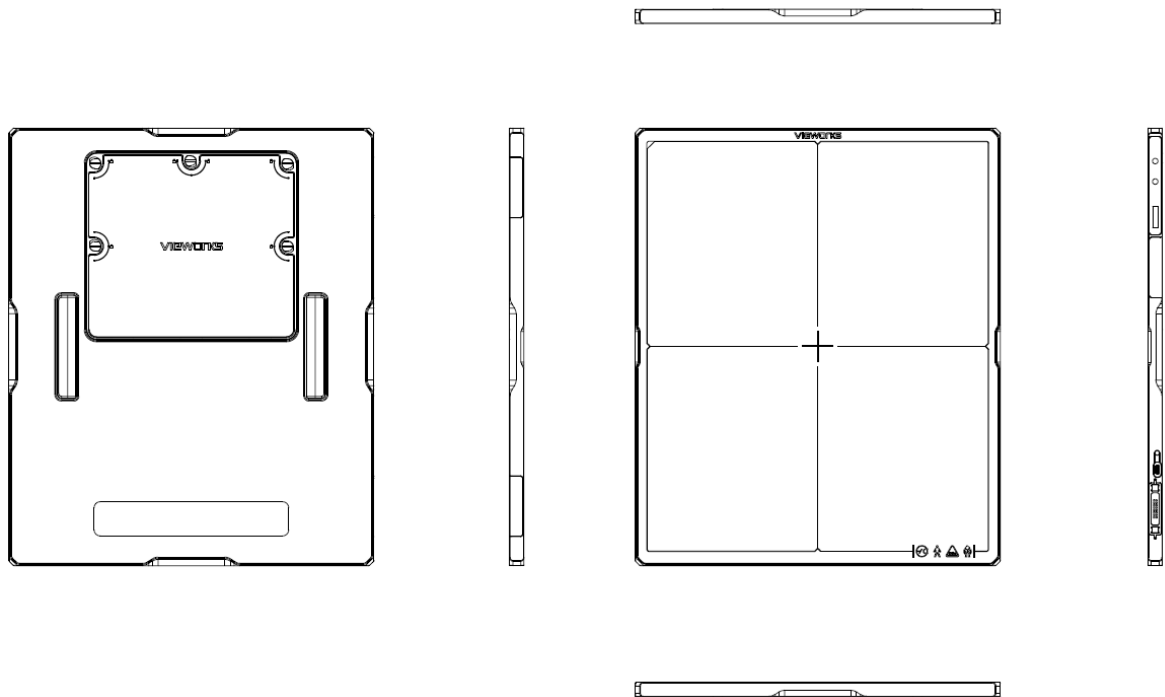

Item	Description
Dimensions (H × W × D)	384.0mm × 460.0mm × 15.0mm
Curvature of Edges	R15.0




• The allowed tolerance of a thickness of detector is from **-2.0mm ~ +1.0mm**. (Under the **ISO4090** regulation).

2.1.3 Functions


FXRD-3643VAW / FXRD-3643VAW PLUS

Side

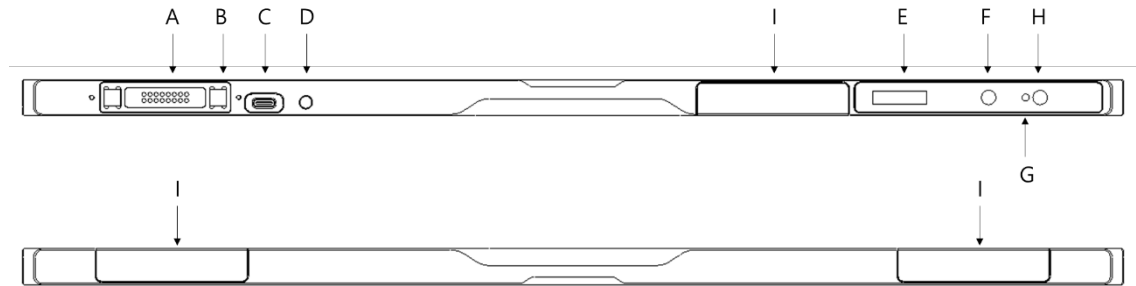

Name	Description
A Tether Interface Connector	Tether interface cable connector. <ul style="list-style-type: none"> Used for wired connection between a detector and SCU.
B Magnet for fixing the tether interface	Used for fixing a tether interface cable
C AC-DC Adapter Connector	<ul style="list-style-type: none"> Connector for fastening the AC-DC adapter Used for fast battery charging
D Charge Status LED	<ul style="list-style-type: none"> Displays the charge status of the battery
E OLED Display	<ul style="list-style-type: none"> Displays battery status Displays wired / wireless connection status Displays sleep mode status
F AP Button	<ul style="list-style-type: none"> Button for changing AP setting in wireless communication (Detector AP/STATION switching or Preset changing when detector is in STATION mode) Changes OLED screen
G Power Indicator LED	<ul style="list-style-type: none"> Displays system power status Displays system boot status
H Power Button	<ul style="list-style-type: none"> System power on/off Changes OLED screen
I Antenna for Wireless LAN	Antennas for wireless communication (3ea)

Rear

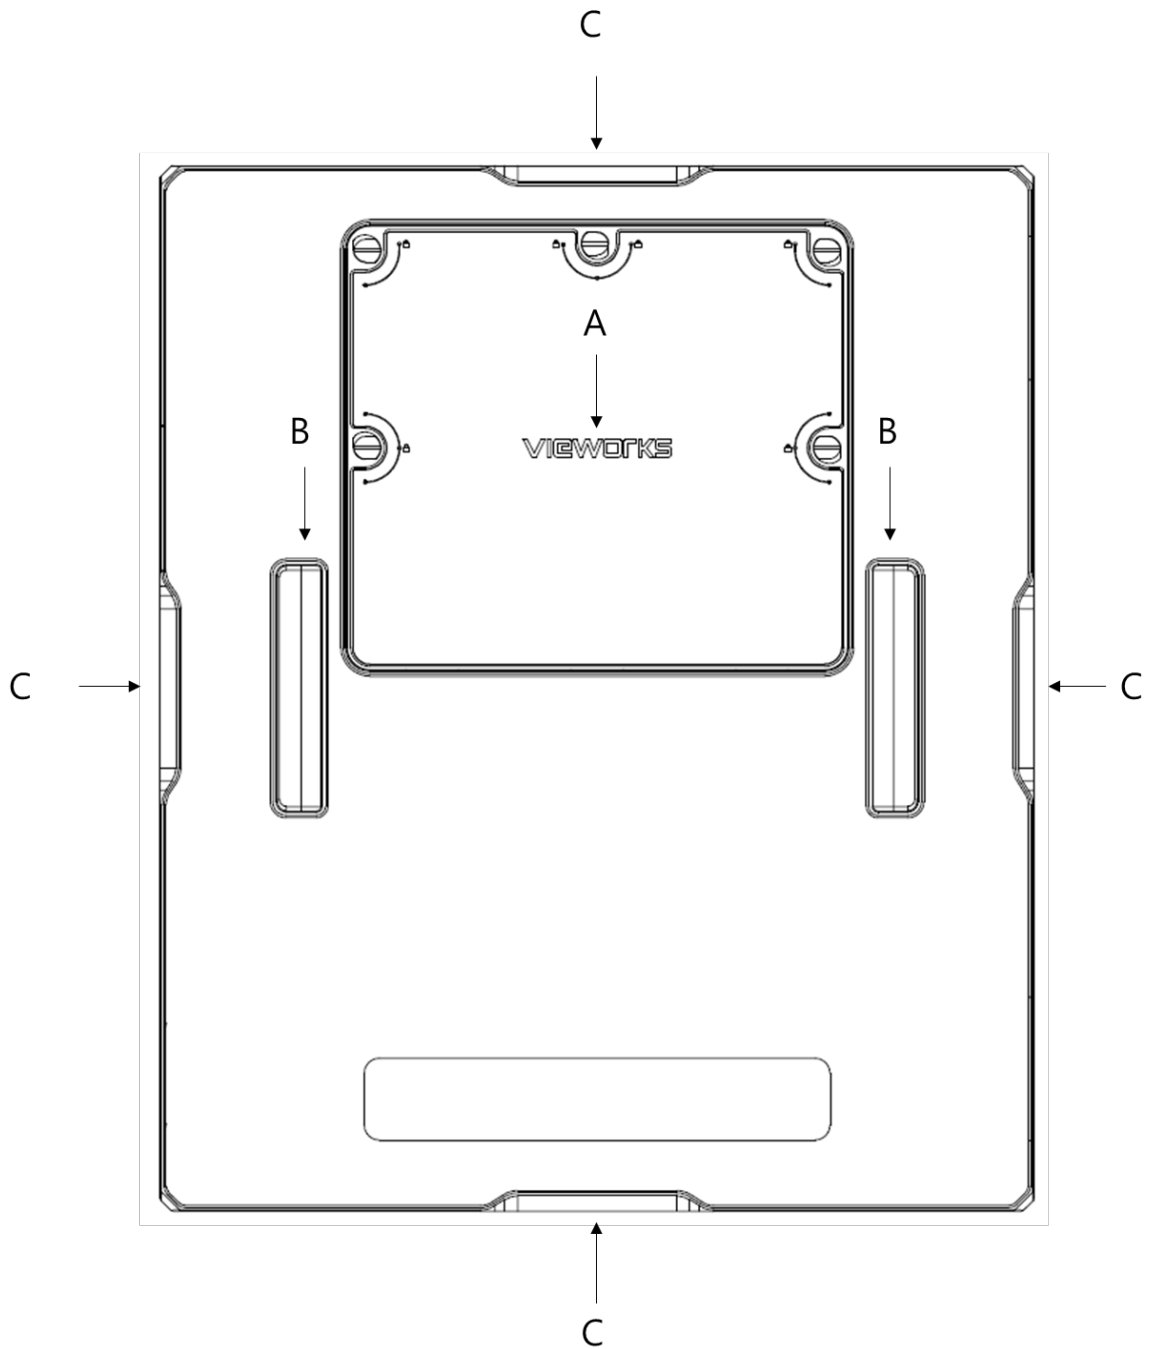

Name	Description
A Battery Pack Cover	The cover needs to be opened and closed when replacing the battery pack.
B Handle	A handle for carrying a detector
C Lift Structure	Used when the detector is placed on flay surface

2.1.4 Use Environment

Item	Operation	Storage & Transportation
Temperature	0 ~ +40°C	-15 ~ +55°C
Humidity	5 ~ 90% (Non-condensing)	5 ~ 90% (Non-condensing)
Atmospheric pressure	700 ~ 1060hPa	500 ~ 1060hPa
Shock	20G	30G
Vibration	2G	5G
Drop limit	1,000mm	1,000mm
Load limit (Local load)	200kg	200kg
Load limit (Uniform load)	400kg	400kg

2.2 Battery Pack

2.2.1 Specifications

Item	Specifications
Model	FXRB-04A
Type	Lithium Ion Polymer
Normal voltage	DC +11.55V
Normal Capacity	3,400mAh
Number of Cell	3S1P (3 Series 1 Parallel)
Life	Approx. 800 times (Fully charged/Discharged completely, 1 cycle)
Dimension (H × W × D)	Max. 189.0mm × 89.0mm × 6.65mm
Weight	Max. 185g



- The battery operation time increases under the sleep mode depending on the operational condition and environment.

3. Performance

3.1 FXRD-3643VAW

- Test Condition: RQA5, 2.5uGy, IEC 62220-1 Standard, Gain type = 1
- The typical values are for reference only.

Parameters	Unit	Minimum	Typical	Maximum
Dark Noise	cts	-	4	5
Offset (Black Image)	cts	500	-	3500
Sensitivity at G=1	cts/uGy	540	600	660
Quantum Limited Dose	uGy	-	-	0.1
Signal to Noise Ratio	dB	16	-	-
Max. Exposure Level	uGy	90	-	-
Dynamic Range	a.u	900	-	-
MTF	0.5 lp/mm	87	90	-
	1 lp/mm	70	75	-
	2 lp/mm	40	45	-
	3 lp/mm	20	24	-
DQE	0.5 lp/mm	39	46	-
	1 lp/mm	35	43	-
	2 lp/mm	27	35	-
	3 lp/mm	18	25	-



- The formula of dynamic range is as follows;
 - $Dynamic\ Range = \frac{Max.Exposure\ Level}{Quantum\ Limited\ Dose}$

3.2 FXRD-3643VAW PLUS

- Test Condition: RQA5, 2.5uGy, IEC 62220-1 Standard, Gain type = 1
- The typical values are for reference only.

Parameters	Unit	Minimum	Typical	Maximum
Dark Noise	cts	-	4	5
Offset (Black Image)	cts	500	-	3500
Sensitivity at G=1	cts/uGy	675	750	825
Quantum Limited Dose	uGy	-	-	0.07
Signal to Noise Ratio	dB	18	-	-
Max. Exposure Level	uGy	72	-	-
Dynamic Range	a.u	1028	-	-
MTF	0.5 lp/mm	81	87	-
	1 lp/mm	58	65	-
	2 lp/mm	27	33	-
	3 lp/mm	12	17	-
DQE	0.5 lp/mm	61	67	-
	1 lp/mm	52	58	-
	2 lp/mm	38	44	-
	3 lp/mm	24	27	-




- The formula of dynamic range is as follows;

$$\square \text{ Dynamic Range} = \frac{\text{Max.Exposure Level}}{\text{Quantum Limited Dose}}$$

4. Defect

4.1 Defect Type

Type	Description
Single Defect	Isolated defects, adjacent pixels are normal. (Class 0)
Cluster Defect	More than consecutive 2 pixels are defected. (Class 1~Class 8)
Line Defect	Defect occur horizontal direction from left to right, or vertical direction from top to bottom.

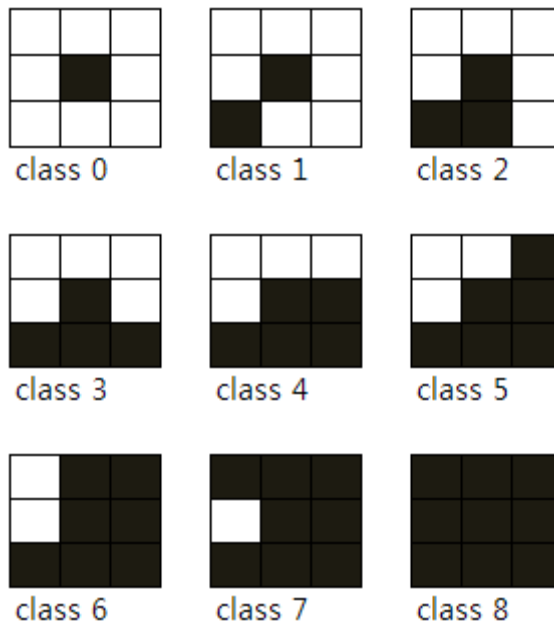

- No cluster defects are allowed over 3x3 pixels.

4.2 Defect Allowance

Item	Unit	Value
Total number of pixel defects	cts	Max. 20,000 pixels
Number of line defects	cts	Max. 5 lines
Number of normal lines between two bad lines	cts	Min. 3 lines

5. Regulatory Information

5.1 Medical Equipment Classification

Item	
Type of protection against electrical shock	Class I or Internally Powered
Degree of protection against electrical shock	Type B applied parts
Degree of protection against ingress of water and dust	IP67 (Degrees of protection against ingress of water and dust provided by enclosure.)
Operation mode	Continuous operation
Flammable anesthetics	NOT suitable for use in the presence of a flammable anesthetic mixture with air or oxygen or nitrous oxide.

5.2 Product Safety Standard

South Korea

Electrical and mechanical safety tests shall be in accordance with IEC 60601-1.

Test for electromagnetic interference prevention shall be in accordance with IEC 60601-1-2.

U.S.A / Canada

Item	
IEC 60601-1:2012 (ed.3.1)	Medical electrical equipment – Part1: General requirements for basic safety and essential performance
ANSI/AAMI ES60601-1(2005) + AMD1(2012)	Medical electrical equipment – Part1: General requirements for basic safety and essential performance
CAN/CSA-C22.2 No. 60601-1:14	Medical electrical equipment – Part 1: General requirements for basic safety and essential performance (adopted IEC 60601-1:2005, including Amendment 1:2012, with Canadian deviations)
IEC 60601-1-2: 2014(ed.4)	Medical electrical equipment-Part 1-2: Collateral Standard: Electromagnetic compatibility
IEC 62304:2006	Medical device software-software life cycle processes
ISO 14971:2012	Medical Device- Application of risk management to medical devices


European Union

Item	
MDD (Medical Device Directive)	(93/42/EEC as amended by 2007/47/EC) Medical Device Directive
EN ISO 13485:2016	Medical devices – Quality Management systems – Requirements for regulatory purposes
IEC 60601-1:2012 (ed.3.1)	Medical electrical equipment- Part1: General requirements for basic safety and essential performance
IEC 60601-1-2: 2014(ed.4)	Medical electrical equipment-Part 1-2: Collateral Standard: Electromagnetic compatibility - Requirements and tests
IEC 62304:2006	Medical device software-Software life cycle processes
ISO 14971: 2012	Medical device – Application of risk management to medical devices.

VIEWWORKS

**Vieworks.Co., Ltd**

41-3, Burim-ro 170beon-gil, Dongan-gu, Anyang-si,
Gyeonggi-do, 14055 Republic of Korea
Telephone: +82-70-7011-6161
Fax: +82-31-386-8631
Homepage: <http://www.vieworks.com>

**European representative: Obelis s.a**

Bd. Général Wahis 53
1030 Brussels, BELGIUM
Tel: +(32) 2.732.59.54
Fax: +(32) 2.732.60.03
E-mail: mail@obelis.net
