

ORDIN DE PLATA NR.: 79

TIP.DOC. 1

DATA EMITERII:9 noiembrie 2021

PLATITI: 3500-00

LEI: Trei Mii Cinci Sute lei 00 ban

i

PLATITOR: (R) S.C. "OXIVI
T-MED" S.R.L.

CONTUL DE PLATI/CODUL IBAN
MD44ML000000002251729503
CODUL FISCAL :1007600044280 /

PRESTATORUL PLATITOR
BC"Moldindconbank"S.A. fil."Invest" Chisinau

CODUL BANCII:
:MOLDMD2X329:

BENEFICIAR (R) IMSP Spitalu
l Clinic Republican "Timofei
Mosnea

CONTUL DE PLATI/CODUL IBAN
MD32ML000000002251502448
CODUL FISCAL :1003600150783 /

PRESTATORUL BENEFICIAR
BC"Moldindconbank"S.A.

CODUL BANCII:
:MOLDMD2X

DESTINATIA PLATII: Pentru garantia pentru:
oferta la procedura de achizitie public:
a nr. ocds-b3wdp1-MD-1634709502119 din 1:
0.11.2021

TIPUL TRANSFERULUI
NORMAL/URGENT :N:

L.S.

CODUL TRANZACTIEI:001:

DATA PRIMIRII:09/11/2021

: SEMNATURILE

DATA EXECUTARII:09/11/2021 0:00:00

: EMITENTULUI

CONDUCTOR:Web Kojevnikov Dmitrii

MIIGfAYJKoZIhvcNAQcCoIIGbTCCBmkCAQExCzAJBgUrDgMCGGUAMAsGCSqGSIB3:
DQEHAaCCBIUwggSBMIIDaaADAgECAhNHAACEjCA/4xcrKCbFAAAAAISMMA0GCSqG:
SIB3DQEBcWUAMCIXIDAeBgNVBAMTF0NFULQxLUNBLU1vbGRpbmRjb25iYW5rMB4X:
DTIwMDMxNjA4NDUwM1oXDTEzMDMxNjA4NTUwM1owgbGxCzAJBgNVBAYTAK1EMRow:
YDVQOIEExFSZXB1YmXpY2EgTW9sZG92YTERMA8GA1UEBxMIQ2hpc2luYXUxZmZAVV

(semnatura electronica)

CONTABIL-SEF:Web Kojevnikov Dmitrii

MIIGfAYJKoZIhvcNAQcCoIIGbTCCBmkCAQExCzAJBgUrDgMCGGUAMAsGCSqGSIB3:
DQEHAaCCBIUwggSBMIIDaaADAgECAhNHAACEjCA/4xcrKCbFAAAAAISMMA0GCSqG:
SIB3DQEBcWUAMCIXIDAeBgNVBAMTF0NFULQxLUNBLU1vbGRpbmRjb25iYW5rMB4X:
DTIwMDMxNjA4NDUwM1oXDTEzMDMxNjA4NTUwM1owgbGxCzAJBgNVBAYTAK1EMRow:
YDVQOIEExFSZXB1YmXpY2EgTW9sZG92YTERMA8GA1UEBxMIQ2hpc2luYXUxZmZAVV

L.S.

(semnatura electronica)

CONDUCTOR:

(semnatura manuala)

CONTABIL-SEF:

(semnatura manuala)

SEMNATURA PRESTATORUL

L.S.

MOTIVUL REFUZULUI

L.S.

SEMNATURA BANCII :

Zbul2TC8Vk0YEZb5ldvA4zoyKNGsIdPNcwMszZcn80vf/6PAxb6BmxkNV4/oNxk+3
MJZ1nRlJxYmfCJ/ZW10KrC0x7IV4ssYfMU4/xAA6pIZqDQLKLF+y0NmOYwQJLuFOV
giZ/csNRws6hdV/o5eFhf+R0Yg3ksSsmHzqCzs+UfcLtLBFVVe1RAQRfvZFk3m7HH
utVizdSQunZMuvvpqNUIEHu4lQrWsFY9LiLHA9UYxmbtHiVL2q8gCuPdY8WkHyPq/
I+

Nr. 12101-504

18.03.2016

**CERTIFICAT
PRIVIND EXISTENTA CONTURILOR CURENTE**

Prin prezentul, BC „Mobiasbancă – Groupe Societe Generale” S.A., codul băncii (BIC): MOBBMD22, confirmă că compania OXIVIT-MED SRL, cod fiscal (IDNO) 1007600044280, deține următoarele conturi curente la BC "Mobiasbancă-Groupe Societe Generale" S.A., Filiala, 1 Stejaur :

1. MDL - 2224710SV23488147100; IBAN- MD09MO2224ASV23488147100
2. EUR - 2224710SV22227957100; IBAN- MD17MO2224ASV22227957100
3. USD - 2224710SV22214937100; IBAN- MD86MO2224ASV22214937100

Certificatul este emis în baza cererii întreprinderii: Oxivit-Med SRL.


Dumitru Popa
Director filială „Stejaur”



Executor : Mariana Guzun
Tel: 022 812 614

Filiala Nr. 1 „Stejaur”
Bd. Ștefan cel Mare și Sfânt 196
MD-2004, Chișinău, Moldova
Cod MOBBMD22
Cont de corespondență 35213892
la Centrul de Decontări al BNM

Tel. +373 22 81 26 15
Fax. +373 22 81 26 15
www.mobiasbanca.md

BC „Mobiasbancă – Groupe Société Générale” SA
Capital Social: 100 000 000 MDL
Număr de înregistrare de stat - 1002600006089
Sediul Central:
bd. Ștefan cel Mare și Sfânt 81a
MD-2012, Chișinău, Moldova

REPUBLICA



MOLDOVA

CERTIFICAT DE ÎNREGISTRARE

Societatea Comercială "OXIVIT-MED" S.R.L.
ESTE ÎNREGISTRATĂ LA CAMERA ÎNREGISTRĂRII DE STAT

Numărul de identificare de stat - codul fiscal
1007600044280

Data înregistrării

30.07.2007

Data eliberării

30.07.2007

Bordeianu Tatiana, registrator de stat

*Funcția, numele, prenumele persoanei
care a eliberat certificatul*

semnătura

MD 0067985





I.P. "AGENȚIA SERVICII PUBLICE"

Departamentul înregistrare și licențiere a unităților de drept

EXTRAS
din Registrul de stat al persoanelor juridice

nr. 8871 din 05.05.2021

Denumirea completă: **Societatea Comercială «OXIVIT-MED» S.R.L.**

Denumirea prescurtată: **S.C. «OXIVIT-MED» S.R.L.**

Forma juridică de organizare: **Societate cu Răspundere Limitată.**

Numărul de identificare de stat și codul fiscal: **1007600044280.**

Data înregistrării de stat: **30.07.2007.**

Sediul: **MD-2032, bd. Decebal, 82, ap.(of.) 90, mun. Chișinău, Republica Moldova.**

Modul de constituire: **nou creată.**

Obiectul principal de activitate:

- 1 Importul, fabricarea, comercializarea, asistența tehnică și (sau) reparația dispozitivelor medicale și (sau) a opticii;**
- 2 Comerțul cu ridicata al parfumurilor și produselor cosmetice;**
- 3 Comerțul cu amănuntul al produselor cosmetice și de parfumerie, articolelor de toaletă;**
- 4 Intermedieri pentru vânzarea unui asortiment larg de mărfuri;**
- 5 Alte tipuri de comerț cu amănuntul în magazine nespecializate;**
- 6 Alte tipuri de comerț cu ridicata;**
- 7 Închirierea altor mașini și echipamente.**

Capitalul social: **5400 lei.**

Administrator: KOJEVNIKOV DMITRII, IDNP 0972305012362,

Asociați:

1. KOJEVNIKOV DMITRII , IDNP 0972305012362

cota 5400.00 lei, ce constituie 100 %.

Prezentul extras este eliberat în temeiul art. 34 al Legii nr. 220-XVI din 19 octombrie 2007 privind înregistrarea de stat a persoanelor juridice și a întreprinzătorilor individuali și confirmă datele din Registrul de stat la data de: 05.05.2021.

Specialist coordonator
tel. 022-207-840

Lazari Aliona



EEI 0354094

OXIVIT MED

c/f: 1007600044280; adresa: str. Decebal 82-90, or. Chişinău, Republica Moldova

telefon: + 373 22 808002; fax: + 373 22 808003

web: www.oxivit-med.com; e-mail: info@oxivit-med.com

Lista fondatorilor companiei SRL „Oxivit-Med”

Nr.	Numele, Prenumele	Codul Personal
1	Kojevnikov Dmitrii	0972305012362



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-244.10.08



Product Service

EC Certificate

Full Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex II excluding (4)

(Devices in Class IIa, IIb or III)

No. G1 039709 1263 Rev. 00

Manufacturer:

Medtronic, Inc.

710 Medtronic Parkway
Minneapolis MN 55432
USA

Product Category(ies):

- **Autotransfusion Systems and Associated Disposables**
- **Centrifugal Blood Pumps**
- **Bio-Console Drive Units**
- **Flow Monitoring Systems**
- **Bio-Cal Blood Temperature Controller**
- **Temperature Monitoring Systems and Associated Disposables**
- **Blood Monitoring Systems**
- **Cardioplegia Delivery Systems**
- **Disposable Blood Handling Devices used for Open Heart Surgery**
- **Arterial Filters**
- **Oxygenators including Heat Exchangers, with and without Cardiotomy Reservoirs**
- **Cardiotomy Venous Reservoirs**
- **Venous Reservoir Bags**
- **Perfusion Equipment and Disposable Perfusion Devices**
- **Disposable Medical Devices for Drainage Systems**
- **Disposable Medical Devices for use in Cardiopulmonary Surgery: Cardioplegia, Cannulae, Venting, Suction**
- **Pressure Display System & related accessories of class IIa**
- **Tissue Positioning/Stabilizing Devices**
- **Surgical Site Clearing Devices**
- **Intravascular Shunts**
- **Surgical Retractors**

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for design, manufacture and final

Page 1 of 3

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

TÜV SÜD Product Service GmbH • Certification Body • Ridlerstraße 65 • 80339 Munich • Germany



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-244.10.08



Product Service

EC Certificate

Full Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex II excluding (4)

(Devices in Class IIa, IIb or III)

No. G1 039709 1263 Rev. 00

inspection of the respective devices / device categories in accordance with MDD Annex II. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class III devices an additional Annex II (4) certificate is mandatory. See also notes overleaf.

Report No.: 72150396

Valid from: 2020-02-12

Valid until: 2024-05-26

Date, 2020-02-12

Christoph Dicks
Head of Certification/Notified Body



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-244.10.08



Product Service

EC Certificate

Full Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex II excluding (4)

(Devices in Class IIa, IIb or III)

No. G1 039709 1263 Rev. 00

Facility(ies):

Medtronic Mexico S.de R.L.de CV
Av. Paseo Cucapah, 10510 El Lago, C.P. 22210 Tijuana, Baja
California, MEXICO

Medtronic Perfusion Systems
7611 Northland Drive, Minneapolis, MN 55428, USA

Medtronic, Inc.
710 Medtronic Parkway, Minneapolis MN 55432, USA

ACT PLUS[®] SYSTEM

Automated Coagulation Timer



Precise, reliable – the trusted standard

ACT Plus® Sys

The ACT Plus® Automated Coagulation Timer is recognized worldwide as the trusted standard for activated clotting time testing, delivering the accurate, precise and timely results you need.

The ACT Plus® System is used with point-of-care testing during critical procedures, when accurate ACT results are necessary.

- Cardiovascular and vascular surgery
- Cardiac catheterization lab
- Critical care units
- Hemodialysis units
- Pediatric care
- ECMO
- Interventional radiology

Medtronic is the global leader in medical technology — alleviating pain, restoring health, and extending life for millions of people around the world.

As an acknowledged expert in the area of blood management and clot detection technology for more than 20 years, Medtronic leads the way in delivering reliable, cost-effective solutions.

Precise, Reliable Clot Detection Technology

The ACT Plus® System combines the trusted standard in precise clot detection technology with data management and connectivity-ready capabilities. Unlike algorithm-based test measurement, the ACT Plus® System provides real-time clot detection, ensuring accurate and precise clotting time results.

SYSTEM HIGHLIGHTS

- Dual well testing verifies your results are accurate
- Real-time clot detection ensures precise results
- Connects to industry standard point-of-care LIS interfaces, including MAS RALS®-Plus, TELCOR Quick-Linc®, AegisPOC®, and others.*
- Enhanced data management meets all POC testing requirements
 - Stores up to 1000 patient and QC records
 - Holds up to 600 operator IDs
 - Downloads data to a USB or floppy storage device
 - Enables QC and user lockout
 - Bar code scanner available for quick, accurate entry of cartridge and control information, and patient and user IDs



* Check with your local Medtronic representative for country-specific information.

stem



Cartridges, Controls and Accessories

Our unique dual channel cartridge design allows you to instantly verify your results, eliminating the need to retest.

- **Real-time clot detection** reflects patient's ability to form a clot (rather than mathematically calculated results)
- **Liquid suspended Kaolin activator** for uniform mixing with blood sample
- **Room temperature storage** saves refrigerator space

MULTIPLE TESTING APPLICATIONS

- **High Range Activated Clotting Time (HR-ACT)** for use with fresh whole blood samples in cardiovascular surgery, vascular surgery and percutaneous transluminal coronary angioplasty (PTCA)
- **Low Range Activated Clotting Time (LR-ACT)** for use with fresh whole blood samples in dialysis, ECMO and therapeutic heparin monitoring
- **Recalcified Activated Clotting Time (RACT)** for use with citrated whole blood samples in dialysis and therapeutic heparin monitoring

High Range ACT Precision				
	Baseline ACT (sec) (0 units/ml heparin)		Heparinized ACT (sec) (4 units/ml heparin)*	
	Within lot	Between lot	Within lot	Between lot
Mean	130	130	582	582
SD	3.3	6.6	19.0	27.1
%CV	2.6%	5.1%	3.3%	4.7%
N	63	63	162	162


* Internal Medtronic data

- **Heparinase Test Cartridge (HTC)** for use with fresh whole blood samples to identify the presence of presurgical and postsurgical heparin in various clinical settings, allowing you to:
 - Determine baseline clotting time in the presence of heparin
 - Determine the appropriate time to pull sheath
 - Confirm heparin reversal
 - Identify heparin rebound

The HR Heparinase Cartridge is a two channel activated clotting time test: Channel 1 with heparinase and Channel 2 without. The clotting time results for the two channels are compared.

Example for Interpreting HR Heparinase Results

CHANNEL 1 (with heparin)	CHANNEL 2 (without heparin)	INTERPRETATION
120	120	Patient at baseline. No heparin in sample.
120	260	Sample contains heparin. Extension due to effect of heparin only.
260	260	May be an underlying coagulopathy unrelated to heparin.
260	360	Heparin in the blood sample and patient may have an underlying coagulopathy.

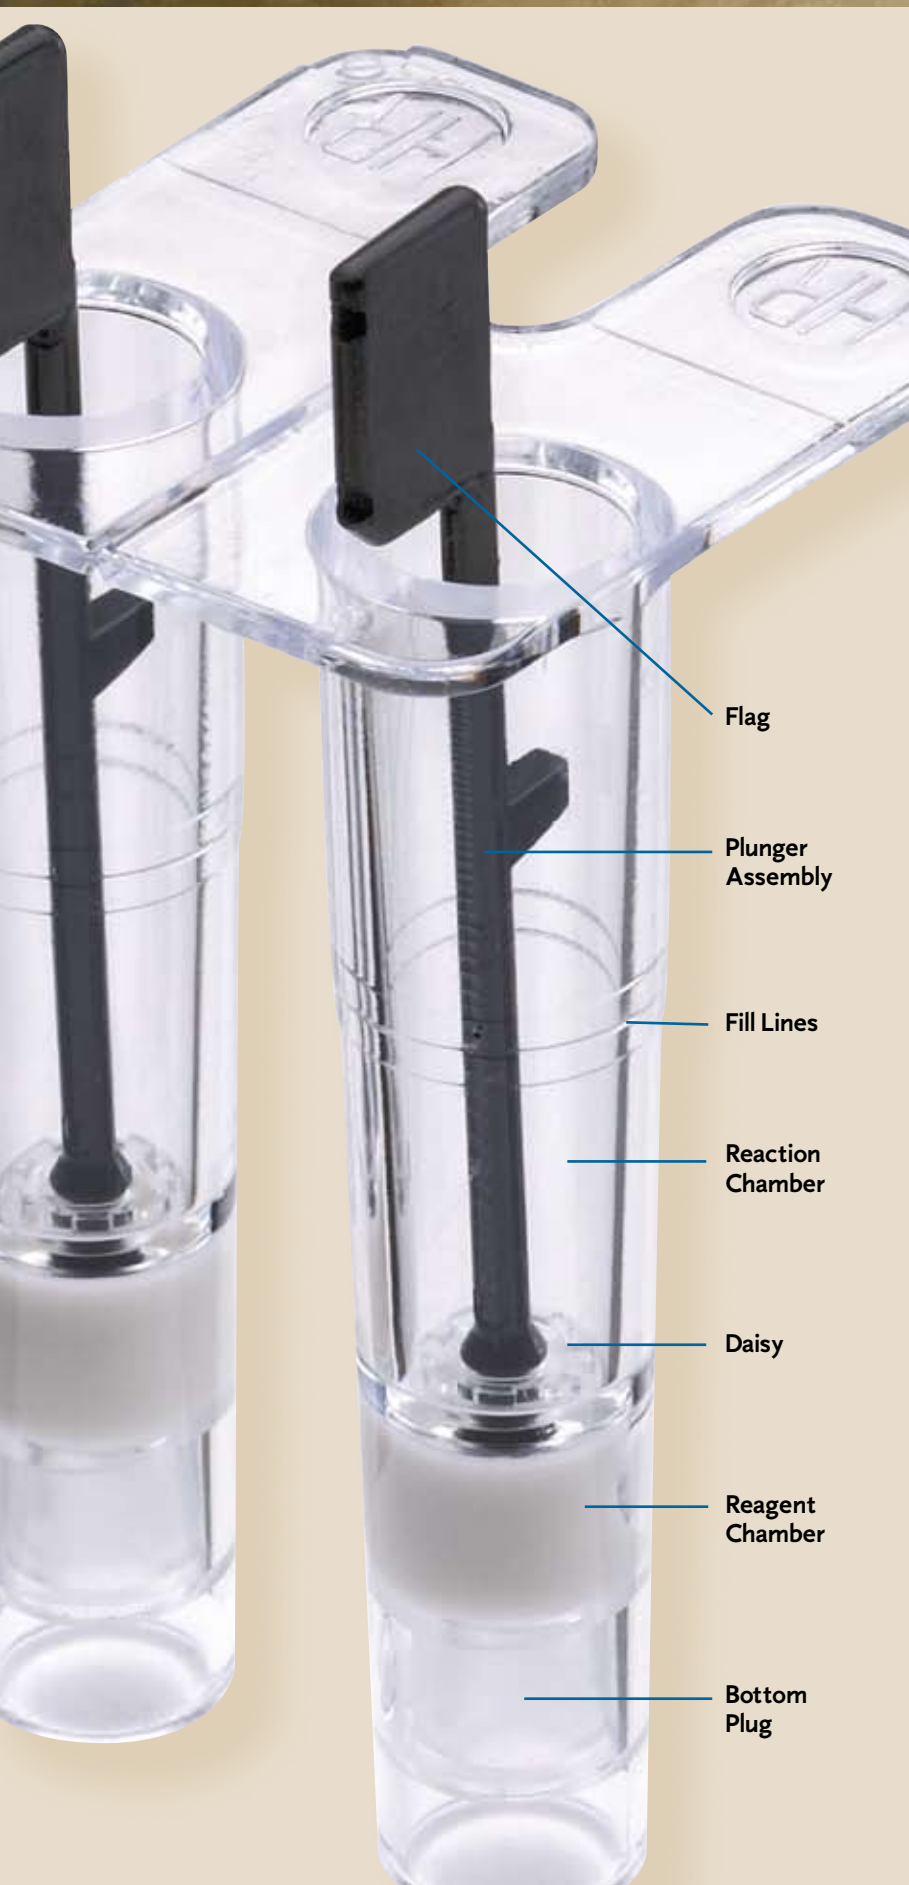

Flag

Plunger Assembly

Fill Lines

Reaction Chamber

Daisy

Reagent Chamber

Bottom Plug

QUALITY CONTROL

A full range of controls are available to verify instrument, cartridge and operator performance and meet regulatory guidelines for testing.

CLOTtrac® Coagulation Controls

Lyophilized controls provide sufficient volume for testing with multiple instruments



ACTtrac® Electronic Control

Provides a multi-level quality check to make quality control easier and faster to perform



ACT® Easy Fill Accessory

- Fill lines are easily visible, even in low light settings
- Needleless system
- Available for high range and low range cartridges



ACT Plus[®] EDM External Data Man

Manage your ACT Plus[®] System data efficiently and effectively.

Get instant access to the charts, reports and spreadsheets you need when you combine the ACT Plus[®] EDM External Data Manager with the ACT Plus[®] System. This versatile Microsoft Access-based software solution helps you to analyze test results and make informed decisions more effectively — allowing you to stay focused on improving patient outcomes.

- Manages patient, QC, instrument and user ID data efficiently
- Provides powerful PC-based software to manage data, without an LIS interface
- Delivers 13 preformatted patient and quality control reports

FEATURES AND BENEFITS

Easy-to-Use Interface

- Intuitive features allow users to be up and running with minimal training
- Prompts lead EDM users through the data import function, eliminating all guesswork

Time-Saving Reports

- Preformatted reports increase efficiency
- Provides visual assessment of QC data and ability to trend QC results
- Ability to track all results for a specific patient

Custom Reporting

- Flexibility in report design and data management
- Data can be exported to Microsoft Excel for graphical and statistical analysis

Reports Menu

Reports Menu

Reports:

- Test Records by Instrument
- Test Records by ACT Plus User ID
- Test Records by Patient
- Cartridge/Control Lot Summary
- Error Codes Summary
- Patient Data Plot
- QC Summary (Levey-Jennings)
- QC Audit
- Block Temperature Log

Administrator Reports

- Instrument Listing
- ACT Plus User Lists Report
- ACT Plus User Report
- EDM User Report

Report Options:

Test Date From: [] to []

Serial Number: []

Report Header: []

Report Footer: []

[Review/Print] [Cancel]

Users can select from a list of all preformatted reports to view the desired information and associated options

Simplified Administrative Management

- View the location of all ACT Plus® Systems at your site
- Group ACT Plus® System users into lists to upload into the ACT Plus® System
- Manage your list of all ACT Plus® System users and their certification

Secure System

- Password protection ensures that only authorized EDM users access the information
- Can be backed up onto your network server to ensure safety of and access to information anytime

The ACT Plus® EDM External Data Manager is not available in all countries.



Display Detail Option

Test Record Detail

Serial Number: 0000001	Control Range Min: <input type="text"/>	<input type="button" value="Save"/>
ACT Plus User ID: 12	Control Range Max: <input type="text"/>	<input type="button" value="Cancel"/>
Patient ID: 1	Clotting Time Ch1: 845	
Test Date: 08/09/2007	Clotting Time Ch2: 797	
Test Time: 11:48	% Difference: 5.8	
Test Type: BACT	Average: 621	
Location: CVOR	Last Updated: <input type="text"/>	
Cartridge Lot: 000000120	Last Updated By: <input type="text"/>	
Cartridge Exp Date: 12/30/2007		
Control Lot: <input type="text"/>		
Control Exp Date: <input type="text"/>		
Control Pass/Fail: <input type="text"/>		
Instrument Status: OK		<input type="button" value="Print"/>
Corrective Action: <input type="text"/>		<input type="button" value="Close"/>

Users can view a complete listing for a single record and note corrective action taken

QC Summary (Levey-Jennings)

**Test Instrument
QC Summary**
Sorted By: Test Type, Test Date/Time
Selected Date Range: 09/01/2007 to 11/20/2007
Selected Serial Number: All
Select Cartridge Lot / Control Lot: All / All

Test Type: BK-AB		-2sd	-1sd	Mean	+1sd	+2sd	Result	Test Date/Time	Serial#	Cart. Lot	Ctrl Lot	Status
		432.8		521.8		629.7						
	x						442	11/04/2007 12:12	0000010	0309000119	0309000090	PASS
	x						460	11/04/2007 12:49	0000010	0309000119	0309000090	PASS
			x				509	11/04/2007 13:20	0000010	0309000119	0309000090	PASS
				x			569	11/04/2007 14:38	0000010	0309000119	0309000090	PASS
					x		519	11/04/2007 15:05	0000010	0309000119	0309000090	PASS
						x	535	11/04/2007 18:57	0000010	0309000119	0309000090	PASS
							694	11/05/2007 12:15	0000010	0309000119	0309000090	PASS
							514	11/05/2007 12:39	0000010	0309000119	0309000090	PASS
							614	11/05/2007 15:04	0000010	0309000119	0309000090	PASS
							499	11/05/2007 18:22	0000010	0309000119	0309000090	PASS
			x				557	11/06/2007 10:56	0000010	0309000119	0309000090	PASS
					x		562	11/06/2007 18:27	0000010	0309000119	0309000090	PASS
	x						479	11/06/2007 18:52	0000010	0309000119	0309000090	PASS
Passed Test Record	12	Mean:	521.75	sd:	19.454	cv:	3.74%					
Total Test Records	13	Mean:	535.00	sd:	17.262	cv:	12.57%					

ORDERING INFORMATION

ACT PLUS® SYSTEM COMPONENTS

Catalog Number	Description
ACT100	ACT Plus® Instrument
ACT200	ACT Plus® Instrument Outside US Version
ACTSC	ACT Plus® Bar Code Scanner
31363	ACTtrac® Electronic Control for ACT Plus®
ACTEDM	ACT Plus® External Data Manager Software

CARTRIDGES AND CONTROLS

Catalog Number	Description	Packaging
----------------	-------------	-----------

ACT® DISPOSABLE TEST CARTRIDGES

402-03	High Range Activated Clotting Time (HR ACT™)	50 cartridges per box
402-01	Low Range Activated Clotting Time (LR ACT™)	50 cartridges per box
402-07	Heparinase Test Cartridge (HTC)	20 per box
402-02	Recalcified Activated Clotting Time (RACT™)	50 cartridges per box

ACT® CLOTtrac® COAGULATION CONTROLS

550-07	CLOTtrac® HR Coagulation Control	15 vials of control and deionized water per box
550-08	CLOTtrac® HR Abnormal Coagulation Control	15 vials of control and deionized water per box
550-13	CLOTtrac® HR Control Pack	1 box of HR 550-07 and 1 box of 550-08
550-01	CLOTtrac® CWB Control (normal) – for Low Range ACT® and RACT cartridges	15 vials of control and deionized water per box
550-09	CLOTtrac® LR Abnormal Coagulation Control	15 vials of control and deionized water per box
550-10	CLOTtrac® RACT Abnormal Coagulation Control	15 vials of control and deionized water per box
550-11	Calcium Chloride – for use with the Low Range ACT controls	1 vial per box
550-12	CLOTtrac® HTC Coagulation Control	15 vials of control and deionized water per box

ACT® ACCESSORIES

313-11	Temperature Verification Cartridge for ACT Plus®	1 per box
313-50	HEPline Kit	Each
303-58	Actuator Cleaning Kit	Each
ACTFILHR	High Range ACT® Easy Fill Accessory	100 per box
ACTFILLR	Low Range ACT® Easy Fill Accessory	100 per box

World Headquarters

Medtronic, Inc.
710 Medtronic Parkway
Minneapolis, MN 55432-5604
USA
Tel: (763) 514-4000
Fax: (763) 514-4879
www.medtronic.com

Medtronic USA, Inc.
Toll-free: 1 (800) 328-2518
(24-hour technical support for physicians and medical professionals)

Revascularization & Surgical Therapies

7611 Northland Drive
Minneapolis, MN 55428-1088
Internet: www.perfusionsystems.com
FAX: (763) 391-9100

Customer Service and Product Orders
Toll-free at 1-800-854-3570

Europe

Medtronic International Trading Sàrl
Route du Molliou 31
Case postale
CH-1131 Tolochenaz
Switzerland
Tel: 41.21.802.7000
Fax: 41.21.802.7900
www.medtronic.com

Canada

Medtronic of Canada Ltd.
6733 Kitimat Road
Mississauga, Ontario L5N 1W3
Canada
Tel: (905) 826-6020
Fax: (905) 826-6620
Toll-free: 1 (800) 268-5346
www.medtronic.com

ACT PLUS® SYSTEM SPECIFICATIONS

DIMENSIONS

Height: 11.9 in (30.2 cm)
Width: 9.0 in (22.9 cm)
Depth: 13.6 in (34.5 cm)
Weight: 11.5 lb (5.22 kg)

DATA PORTS

- Serial Data Port: 19200 baud, 8 data bits, 1 stop bit, no parity
- Bar Code Scanner Port:
used with the optional ACT Plus® Bar Code Scanner
- Floppy Drive: PC compatible, 1-44 MB, 3.5 inch floppy disk
- USB: used with Medtronic approved USB storage device

POWER

Voltage: 100-240 V ~ Single Phase
Frequency: 50-60 Hz
Maximum current: 1.0 A (100-240)

OPERATING LIMITS

Temperature: 14°C to 32°C (57°F to 90°F)
Humidity: 10% to 90%, noncondensing

STORAGE LIMITS

Temperature: 0°C to 49°C (32°F to 120°F)
Humidity: 5% to 90%, noncondensing

Access and Excel are either registered trademarks or trademarks of Microsoft Corporation.

AegisPOC is a registered trademark of Laboratory Data Systems, Inc.

ACT, ACT Plus, ACTtrac, and CLOTtrac are registered trademarks of Medtronic, Inc.

MAS RALS-Plus is a registered trademark of Medical Automation Systems, Inc. (MAS)

Quick-Linc is a registered trademark of TELCOR, Inc.

Asia Pacific

Medtronic International, Ltd.
16/F Manulife Plaza
The Lee Gardens, 33 Hysan Avenue
Causeway Bay
Hong Kong
Tel: (852) 2891 4456
Fax: (852) 2891 6830
enquiryap@medtronic.com
www.medtronic.com

Latin America

Medtronic USA, Inc.
Doral Corporate Center II
3750 NW 87th Avenue Suite 700
Miami, FL 33178
USA
Tel: (305) 500-9328
Fax: (786) 709-4244
www.medtronic.com

UC200802006 EN
© Medtronic, Inc. 2007
All Rights Reserved
Printed in USA



Medtronic
Alleviating Pain · Restoring Health · Extending Life