




PRODUCT SIZES


One unit per box.

Fully Open Implant Diameter	Product Code	*Working Length (mm) / Total Length (mm) at Target Vessel Diameters (mm)			Crimped Length Inside Microcatheter (mm)	% Foreshortening At Fully Open Implant Diameter
		2.0	2.5	3.0		
2.5	FREDJR2508	11 / 15	8 / 13		18	27
2.5	FREDJR2513	17 / 21	13 / 18		26	33
2.5	FREDJR2520	28 / 32	20 / 25		40	38
2.5	FREDJR2526	35 / 38	26 / 30		49	39
3.0	FREDJR3009		12 / 16	9 / 13	20	32
3.0	FREDJR3014		19 / 23	14 / 19	30	38
3.0	FREDJR3021		29 / 34	21 / 27	46	42
3.0	FREDJR3027		37 / 41	27 / 32	56	44

* Outer device total length (including flared ends) and inner device working length (marked by helical strands), constrained in vessel.

DELIVERED THROUGH:
Headway[®] 21
 Microcatheter

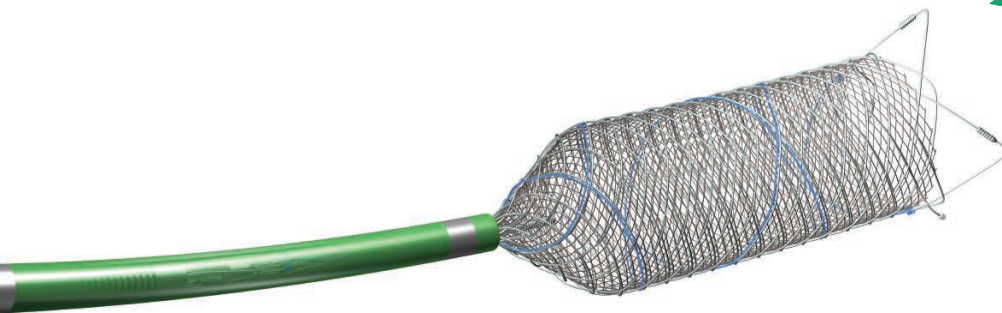

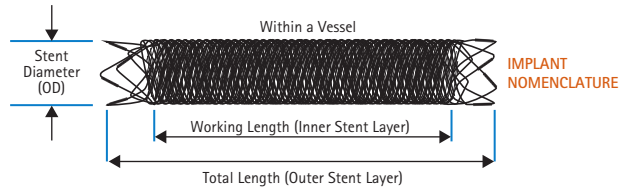

EFFECTIVE METAL SURFACE AREA One unit per box.

Fully Open Implant Diameter	Product Code	*Effective Metal Surface Area (%) at Target Vessel Diameters (mm)		
		2.0	2.5	3.0
2.5	FREDJR2508	29	31	
2.5	FREDJR2513	30	31	
2.5	FREDJR2520	29	33	
2.5	FREDJR2526	30	32	
3.0	FREDJR3009		25	28
3.0	FREDJR3014		25	28
3.0	FREDJR3021		25	28
3.0	FREDJR3027		26	29

* Effective Metal Surface Area (%) measured for the inner stent, which provides flow diversion.

The FRED® and FRED® Jr. systems are CE Marked. The FRED Jr. system is not approved in the United States. The FRED system is limited by United States law to investigational use only.

INDICATIONS FOR USE:

The system is intended for endovascular embolization of intracranial neurovascular aneurysms. The FRED and FRED Jr. system may also be used with embolic coils for the treatment of intracranial neurovascular lesions.



MicroVention, Inc.
Worldwide Headquarters
 1311 Valencia Avenue
 Tustin, CA 92780, USA
 MicroVention UK Limited
 MicroVention Europe, S.A.R.L.
 MicroVention Deutschland GmbH
Web

PH +1.714.247.8000

PH +44 (0) 191 258 6777
 PH + 33 (1) 39 21 77 46
 PH +49 211 210 798-0
microvention.com



MICROVENTION, FRED and Headway are registered trademarks of MicroVention, Inc. Refer to Instructions for Use, contraindications and warnings for additional information. © 2016 MicroVention, Inc. MM501(i) EMEA 4/16



Flow Re-Direction Endoluminal Device


PRODUCT SIZES

One unit per box.

Fully Open Implant Diameter	Product Code	*Working Length (mm) / Total Length (mm) at Target Vessel Diameters (mm)						Crimped Length Inside Microcatheter (mm)	% Foreshortening At Fully Open Implant Diameter
		3.0	3.5	4.0	4.5	5.0	5.5		
3.5	FRED3507	10 / 16	7 / 13					21	39
3.5	FRED3511	17 / 22	11 / 17					32	47
3.5	FRED3516	24 / 30	16 / 22					44	49
3.5	FRED3524	34 / 40	24 / 31					61	48
3.5	FRED3536	49 / 54	36 / 40					83	52
4.0	FRED4007		10 / 16	7 / 13				24	42
4.0	FRED4012		18 / 24	12 / 18				36	49
4.0	FRED4017		26 / 31	17 / 23				49	53
4.0	FRED4026		37 / 43	26 / 32				69	53
4.0	FRED4038		53 / 58	38 / 44				94	55
4.5	FRED4508			11 / 18	8 / 15			27	43
4.5	FRED4513			19 / 26	13 / 20			41	51
4.5	FRED4518			27 / 34	18 / 25			55	55
4.5	FRED4528			39 / 45	28 / 34			77	56
4.5	FRED4539			56 / 62	39 / 45			105	57
5.0	FRED5009				12 / 18	9 / 15		28	44
5.0	FRED5014				20 / 26	14 / 21		44	53
5.0	FRED5019				28 / 35	19 / 26		60	56
5.0	FRED5029				41 / 48	29 / 36		84	57
5.5	FRED5514					22 / 28	14 / 22	48	54
5.5	FRED5526					38 / 46	26 / 32	83	59


* Outer device total length (including flared ends) and inner device working length (marked by helical strands), constrained in vessel.

DELIVERED THROUGH:

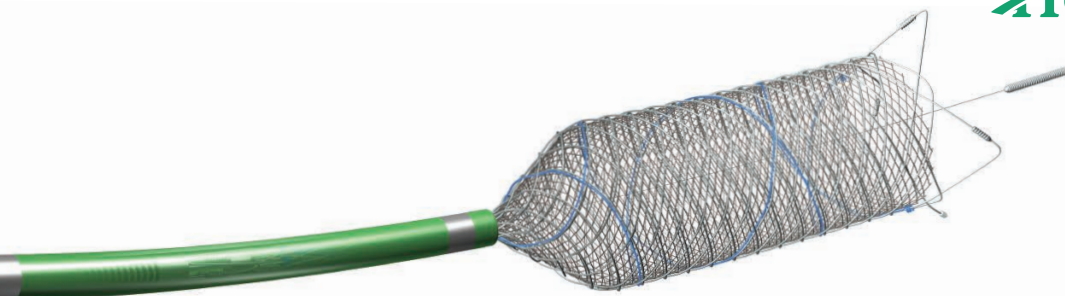



Flow Re-Direction Endoluminal Device

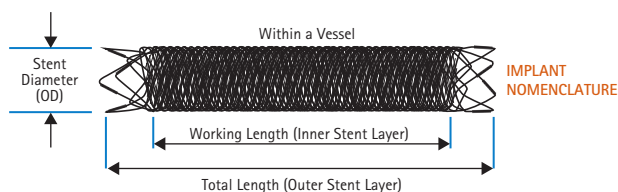

EFFECTIVE METAL SURFACE AREA One unit per box.

Fully Open Implant Diameter	Product Code	*Effective Metal Surface Area (%) at Target Vessel Diameters (mm)					
		3.0	3.5	4.0	4.5	5.0	5.5
3.5	FRED3507	35	42				
3.5	FRED3511	34	43				
3.5	FRED3516	34	44				
3.5	FRED3524	30	38				
3.5	FRED3536	31	36				
4.0	FRED4007		32	39			
4.0	FRED4012		31	40			
4.0	FRED4017		32	42			
4.0	FRED4026		28	37			
4.0	FRED4038		28	34			
4.5	FRED4508			30	37		
4.5	FRED4513			30	40		
4.5	FRED4518			29	39		
4.5	FRED4528			26	36		
4.5	FRED4539			26	33		
5.0	FRED5009				28	33	
5.0	FRED5014				28	36	
5.0	FRED5019				28	36	
5.0	FRED5029				25	33	
5.5	FRED5514					25	34
5.5	FRED5526					25	36

* Effective Metal Surface Area (%) measured for the inner stent, which provides flow diversion.

The FRED® and FRED® Jr. systems are CE Marked. The FRED Jr. system is not approved in the United States. The FRED system is limited by United States law to investigational use only.

INDICATIONS FOR USE:

The system is intended for endovascular embolization of intracranial neurovascular aneurysms. The FRED and FRED Jr. system may also be used with embolic coils for the treatment of intracranial neurovascular lesions.




MICROVENTION, FRED and Headway are registered trademarks of MicroVention, Inc. Refer to Instructions for Use, contraindications and warnings for additional information. © 2016 MicroVention, Inc. MM502(i) EMEA 4/16



MicroVention, Inc.
Worldwide Headquarters
 1311 Valencia Avenue
 Tustin, CA 92780, USA
 MicroVention UK Limited
 MicroVention Europe, S.A.R.L.
 MicroVention Deutschland GmbH
Web

PH +1.714.247.8000

PH +44 (0) 191 258 6777
 PH + 33 (1) 39 21 77 46
 PH +49 211 210 798-0
microvention.com

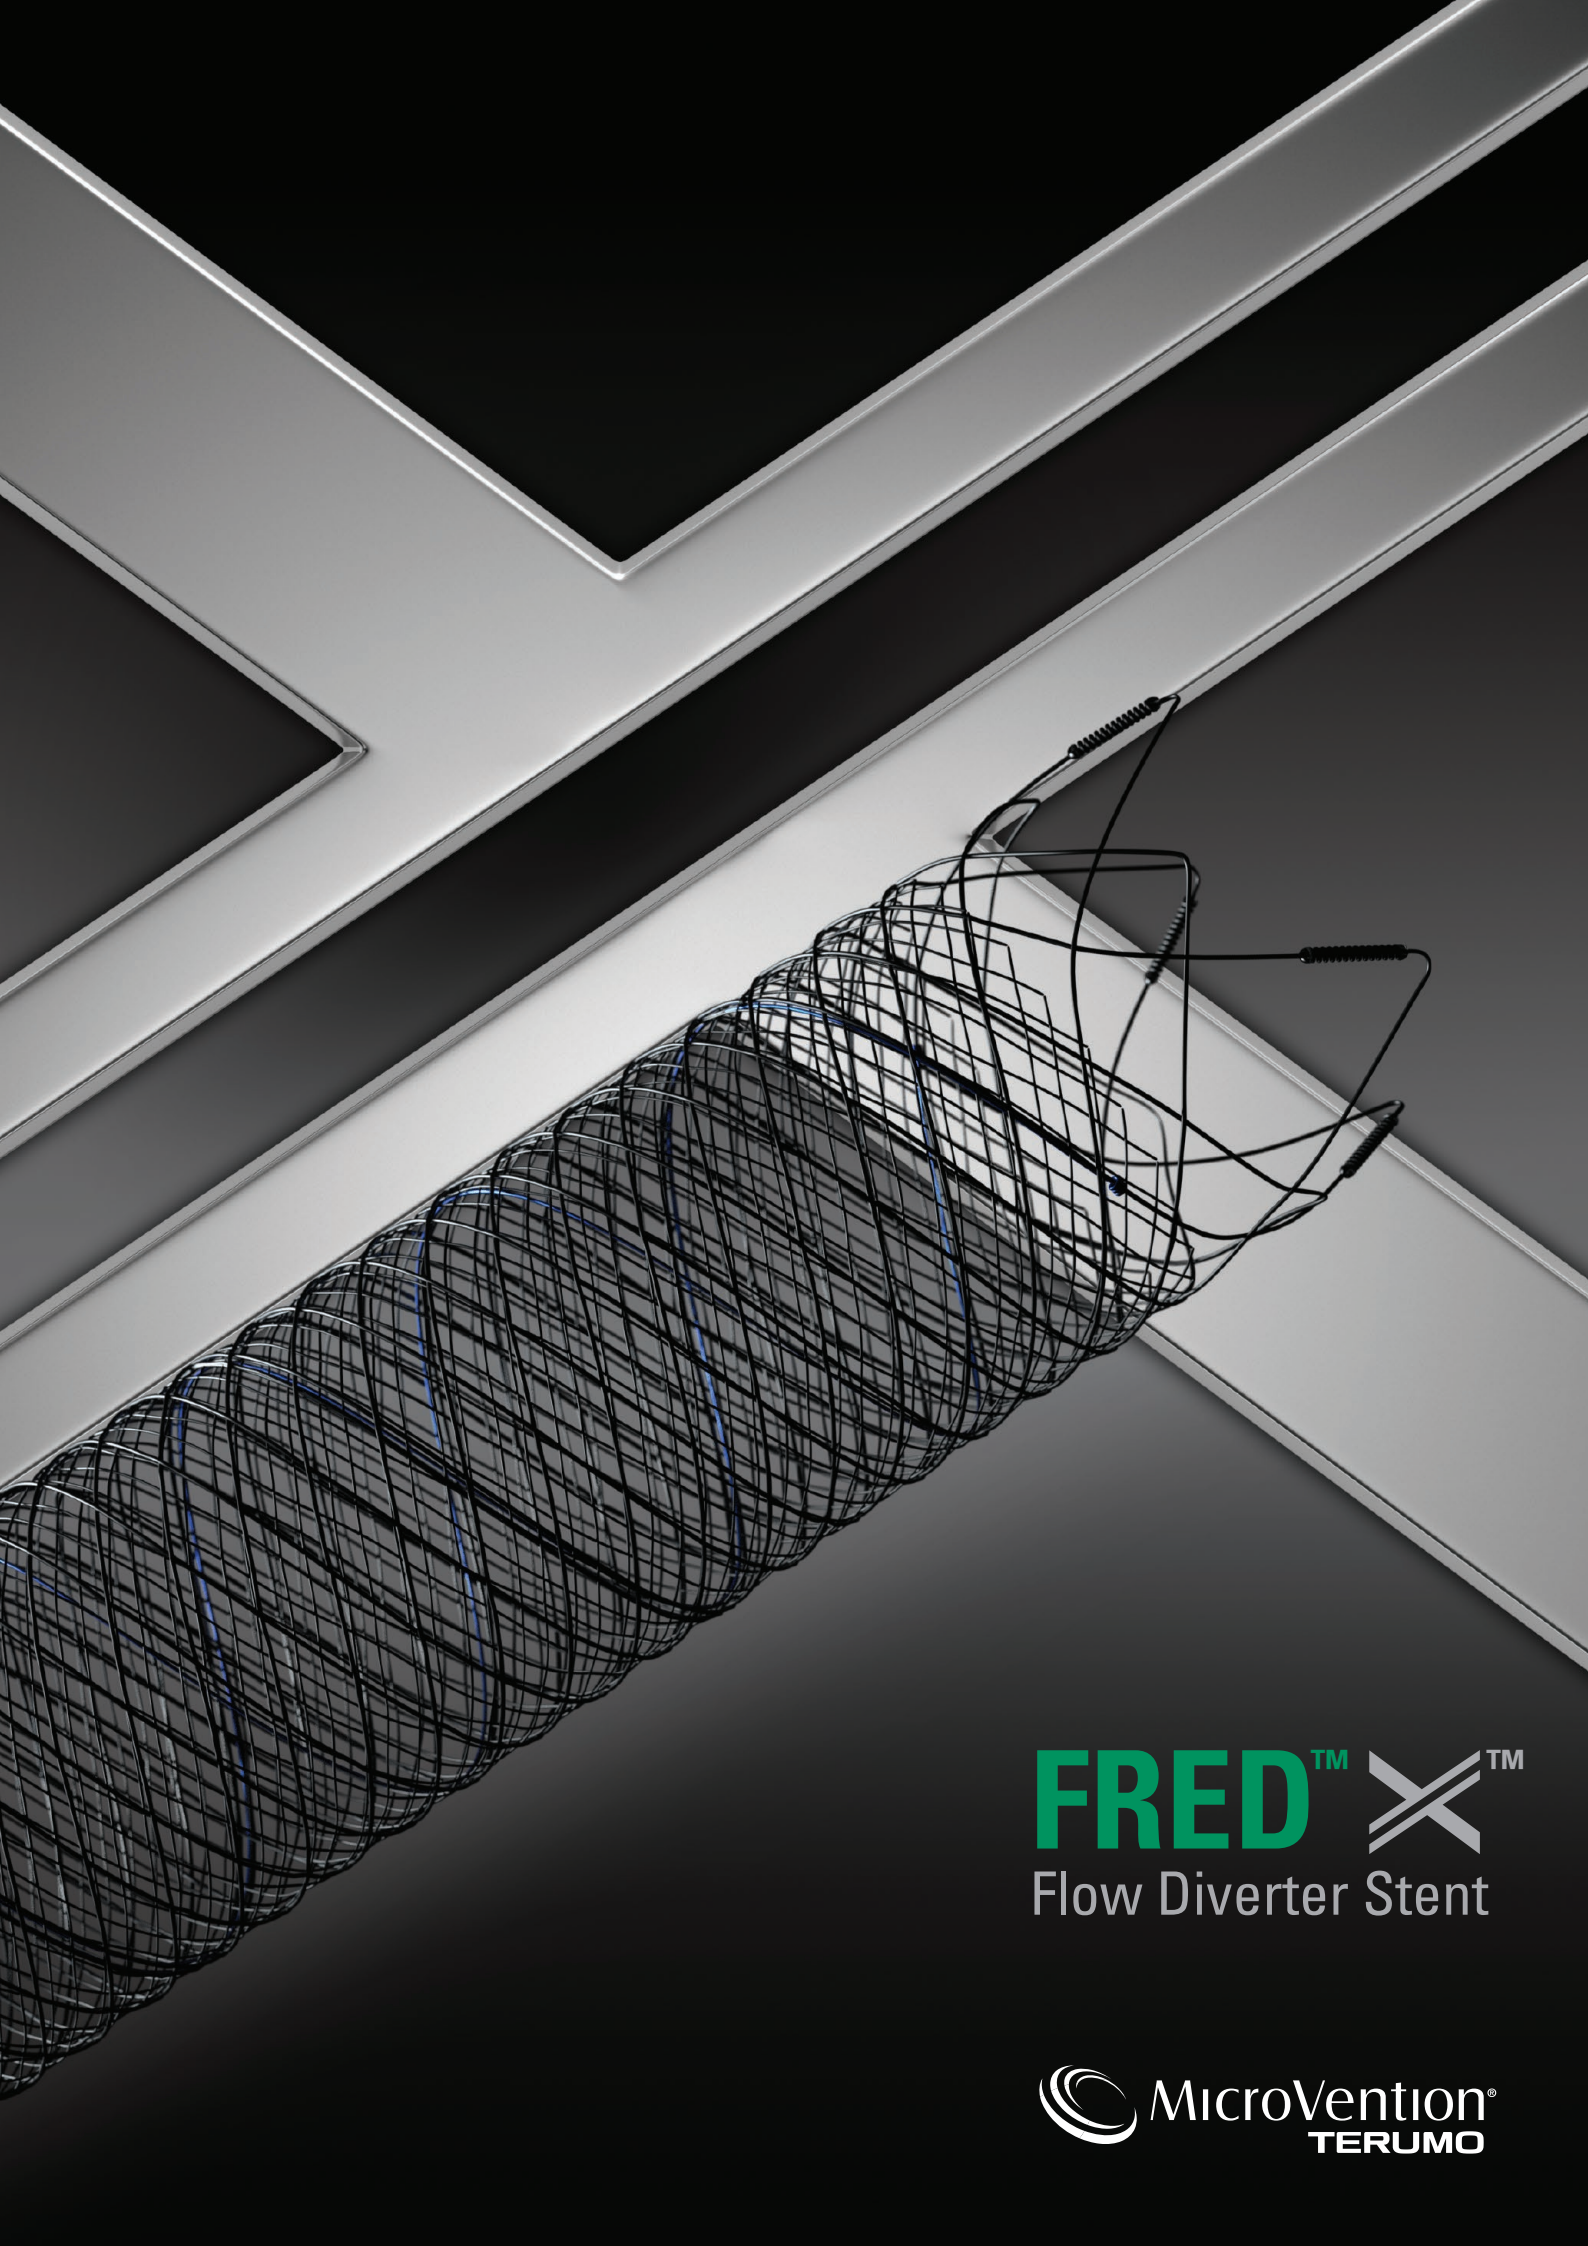


FREDTM TM
Flow Diverter Stent

 **MicroVention**[®]
TERUMO

FRED™ X™

Flow Diverter Stent

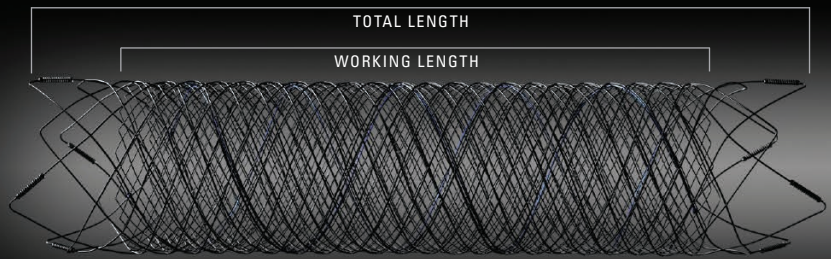

DEVICE	PRODUCT CODE	DEVICE SIZE (mm)		WORKING LENGTH / TOTAL LENGTH IN DIFFERENT VESSEL DIAMETERS (mm)							
		Unconstrained Diameter	x Total Length	2.0mm	2.5mm	3.0mm	3.5mm	4.0mm	4.5mm	5.0mm	5.5mm
FRED X 21	XFRED2508	2.5	X 13	11 / 15	8 / 13						
	XFRED2513	2.5	X 18	17 / 21	13 / 18						
	XFRED2520	2.5	X 25	28 / 32	20 / 25						
	XFRED2526	2.5	X 30	35 / 38	26 / 30						
	XFRED3009	3.0	X 13		12 / 16	9 / 13					
	XFRED3014	3.0	X 19		19 / 23	14 / 19					
	XFRED3021	3.0	X 27		29 / 34	21 / 27					
	XFRED3027	3.0	X 32		37 / 41	27 / 32					
FRED X 27	XFRED3507	3.5	X 13			10 / 16	7 / 13				
	XFRED3511	3.5	X 17			17 / 22	11 / 17				
	XFRED3516	3.5	X 22			24 / 30	16 / 22				
	XFRED3524	3.5	X 31			34 / 40	24 / 31				
	XFRED3536	3.5	X 40			49 / 54	36 / 40				
	XFRED4007	4.0	X 13				10 / 16	7 / 13			
	XFRED4012	4.0	X 18				18 / 24	12 / 18			
	XFRED4017	4.0	X 23				26 / 31	17 / 23			
	XFRED4026	4.0	X 32				37 / 43	26 / 32			
	XFRED4038	4.0	X 44				53 / 58	38 / 44			
	XFRED4508	4.5	X 15					11 / 18	8 / 15		
	XFRED4513	4.5	X 20					19 / 26	13 / 20		
	XFRED4518	4.5	X 25					27 / 34	18 / 25		
	XFRED4528	4.5	X 34					39 / 45	28 / 34		
	XFRED4539	4.5	X 45					56 / 62	39 / 45		
	XFRED5009	5.0	X 15						12 / 18	9 / 15	
	XFRED5014	5.0	X 21						20 / 26	14 / 21	
	XFRED5019	5.0	X 26						28 / 35	19 / 26	
	XFRED5029	5.0	X 36						41 / 48	29 / 36	
	XFRED5514	5.5	X 22							22 / 28	14 / 22
XFRED5526	5.5	X 32							38 / 46	26 / 32	

DEVICE	PRODUCT CODE	DISTAL ID (in)	PROXIMAL ID (in)	DISTAL OD (Fr/in)	PROXIMAL OD (Fr/in)	LENGTH (cm)
HEADWAY™ 21 and 27 Microcatheters	MC212156S	0.021	0.021	2.1 / 0.026	2.5 / 0.033	156
	MC272156S	0.027	0.027	2.6 / 0.034	3.1 / 0.041	156
SOPIA™ EX Intracranial Support Catheter	ISC5105ST	0.058	0.058	5.2 / 0.068	5.4 / 0.071	105
	ISC5115ST	0.058	0.058	5.2 / 0.068	5.4 / 0.071	115
SOPIA™ Distal Access Catheter	DA5115ST	0.055	0.055	5.1 / 0.067	5.2 / 0.068	115
	DA5125ST	0.055	0.055	5.1 / 0.067	5.2 / 0.068	125
	DA6115ST	0.070	0.070	6.2 / 0.0815	6.3 / 0.0825	115

FRED X Indications for Use: The FRED X System is intended for endovascular embolization of intracranial neurovascular aneurysms. The FRED X System may also be used with embolic coils for the treatment of intracranial neurovascular lesions.

HEADWAY Microcatheter Indications for Use: The HEADWAY Microcatheter is intended for general intravascular use, including the peripheral, coronary and neuro vasculature for the infusion of diagnostic agents, such as contrast media, and therapeutic agents, such as occlusion coils.

SOPIA EX Catheter Indications for Use: The SOPIA EX Catheter is indicated for general intravascular use, including the neuro and peripheral vasculature. The SOPIA EX Catheter can be used to facilitate introduction of diagnostic agents or therapeutic devices. The SOPIA EX Catheter is not intended for use in coronary arteries.

SOPIA Catheter Indications for Use: The SOPIA Catheter is indicated for general intravascular use, including the neuro and peripheral vasculature. The SOPIA Catheter can be used to facilitate introduction of diagnostic or therapeutic agents. The SOPIA Catheter is not intended for use in coronary arteries. Moreover, the SOPIA Catheter is intended for use in removal/aspiration of emboli and thrombi from selected blood vessels in the arterial system, including the peripheral and neuro vasculatures.

For Healthcare professional use only.