



CT Brain Perfusion

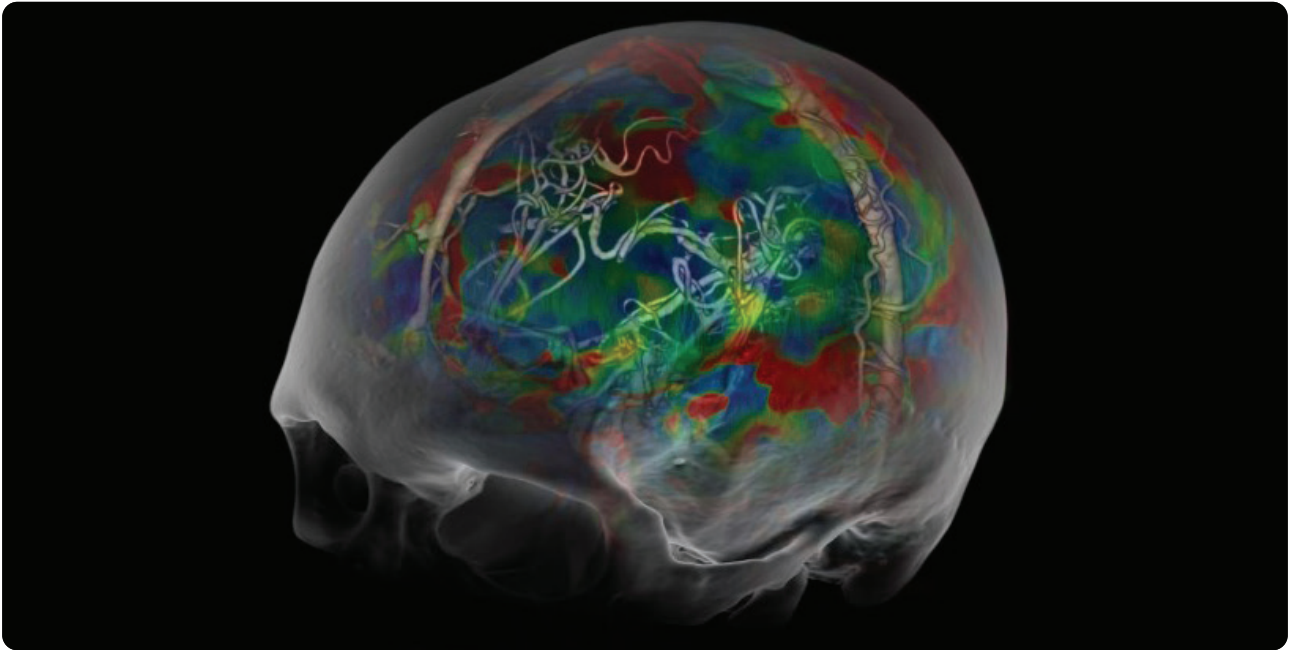

CT Brain Perfusion harnesses the power of Vitrea Advanced Visualization and is a convenient method of assessing perfusion abnormalities within the brain. Concurrent display of the perfusion maps aid in the assessment of the type and extent of abnormal cerebral blood flow. Automated tools help to efficiently visualize anatomy and pathology.

Canon Medical has expanded its CT Brain Perfusion offering from 2D perfusion to the development of delay insensitive methods, semi-automated processing, full 4D scanning, and workflow enhancements to deliver impactful images.

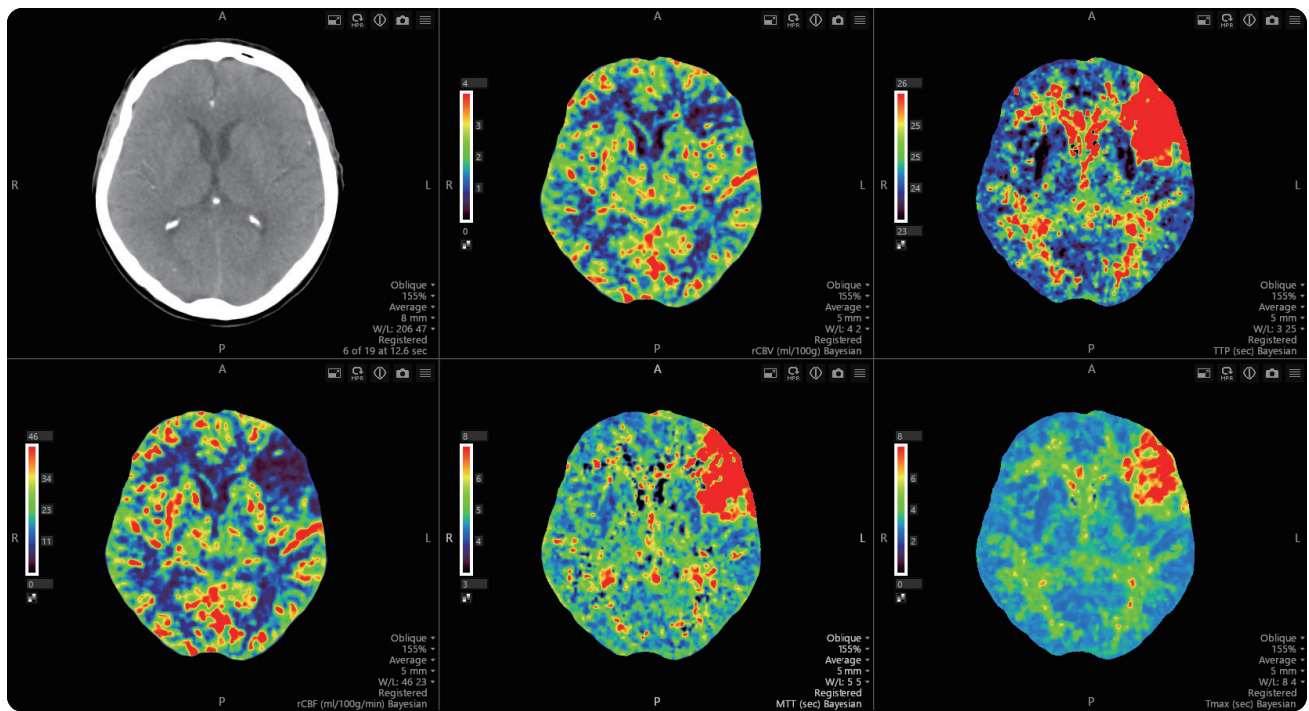

Key Benefits

- Streamlined workflow with automatic curve-fitting, midline correction, motion correction and region of interest templating
- Vitrea software identifies the artery and vein, then computes five parametric maps with quantitative results: time-to-maximum (Tmax*), mean transit time (MTT), regional cerebral blood flow (rCBF), regional cerebral blood volume (rCBV) and time to peak (TTP)
- Summary maps communicate results of a CT perfusion exam and provide tissue classification
- Bayesian processing is available in CT Brain Perfusion in addition to our SVD*² and SVD+ options. The Bayesian method excels at processing low signal-to-noise ratio (SNR) images that help provide clarity on parametric images used to compute summary maps.^{1, 2}

Key Features

- Support for 2D, 4D and thick-slice CT scan data, as well as jog, shuttle, and wide coverage acquisition
- Three processing algorithm methods:
 - Singular value decomposition (SVD)
 - Delay-insensitive singular value decomposition (SVD+)
 - Bayesian method
- Simplified image collage creation and export
- Time density graph plots display the range of image density, transit time for the artery location, image density over time for the artery and vein and corresponding time values

CT Brain Perfusion Packages

Feature	2D	4D
Algorithms		
SVD	✓	
SVD+	✓	✓
Bayesian	✓	✓
Maps		
Angio Map		✓
Automatic arterial and venous phase separation 4D views of the arteriogram and venogram (generated CTA-V view)		✓
Fusion of perfusion maps and anatomical CT view		✓
Summary Map	✓	✓

*1 Tmax mapping is not available in 2D Brain Perfusion cases.

*2 SVD is available in 2D only.

- 1 Timothe Boutelier, Koshuke Kudo, Fabrice Pautot, and Makoto Sasaki. "Bayesian Hemodynamic Parameter Estimation by Bolus Tracking Perfusion Weighted Imaging. Part I: Theory and Preliminary Results". 06 March 2012.
- 2 Anke Wouters, Søren Christensen, Matus Straka, Michael Mlynash, John Liggins, Roland Bammer, Vincent Thijs, Robin Lemmens, Gregory W. Albers and Maarten G. Lansberg. "A Comparison of Relative Time to Peak and Tmax for Mismatch-Based Patient Selection". 13 October 2007.

CANON MEDICAL SYSTEMS CORPORATION

<https://global.medical.canon>

©Canon Medical Systems Corporation 2016-2021. All rights reserved.

Design and specifications are subject to change without notice.

MCAHI0035EAE 2021-10 CMSC/Produced in Japan

Canon Medical Systems Corporation meets internationally recognized standards for Quality Management System ISO 9001, ISO 13485. Canon Medical Systems Corporation meets the Environmental Management System standard ISO 14001.

Made for Life is a trademark of Canon Medical Systems Corporation.

This document may include trademarks or registered trademarks of their respective owners.

Disclaimer: Some features presented in this brochure may not be commercially available on all systems shown or may require the purchase of additional options. Please verify the availability of this application with your local/regional representative from Canon Medical Systems.

Made For life