

使用期限 说明书
其他内容详见说明书。

980-588/003

ABL90 Series

Voltage range
100-240 V
50/60 Hz
Max. power 90W
Input fuses (2) - 2.5A HRC (T) 250 VAC

WARNING: Fire hazard. Replace fuse as marked.
AVERTISSEMENT : Risque d'incendie. Remplacer
les fusibles comme indiqué.

 Radiometer Medical ApS
Akandevvej 21
2700 Brønshøj
Denmark
www.radiometer.com

RADIOMETER 




LISTED
(LABORATORY EQUIPMENT)
36JX



980-075/005

S35

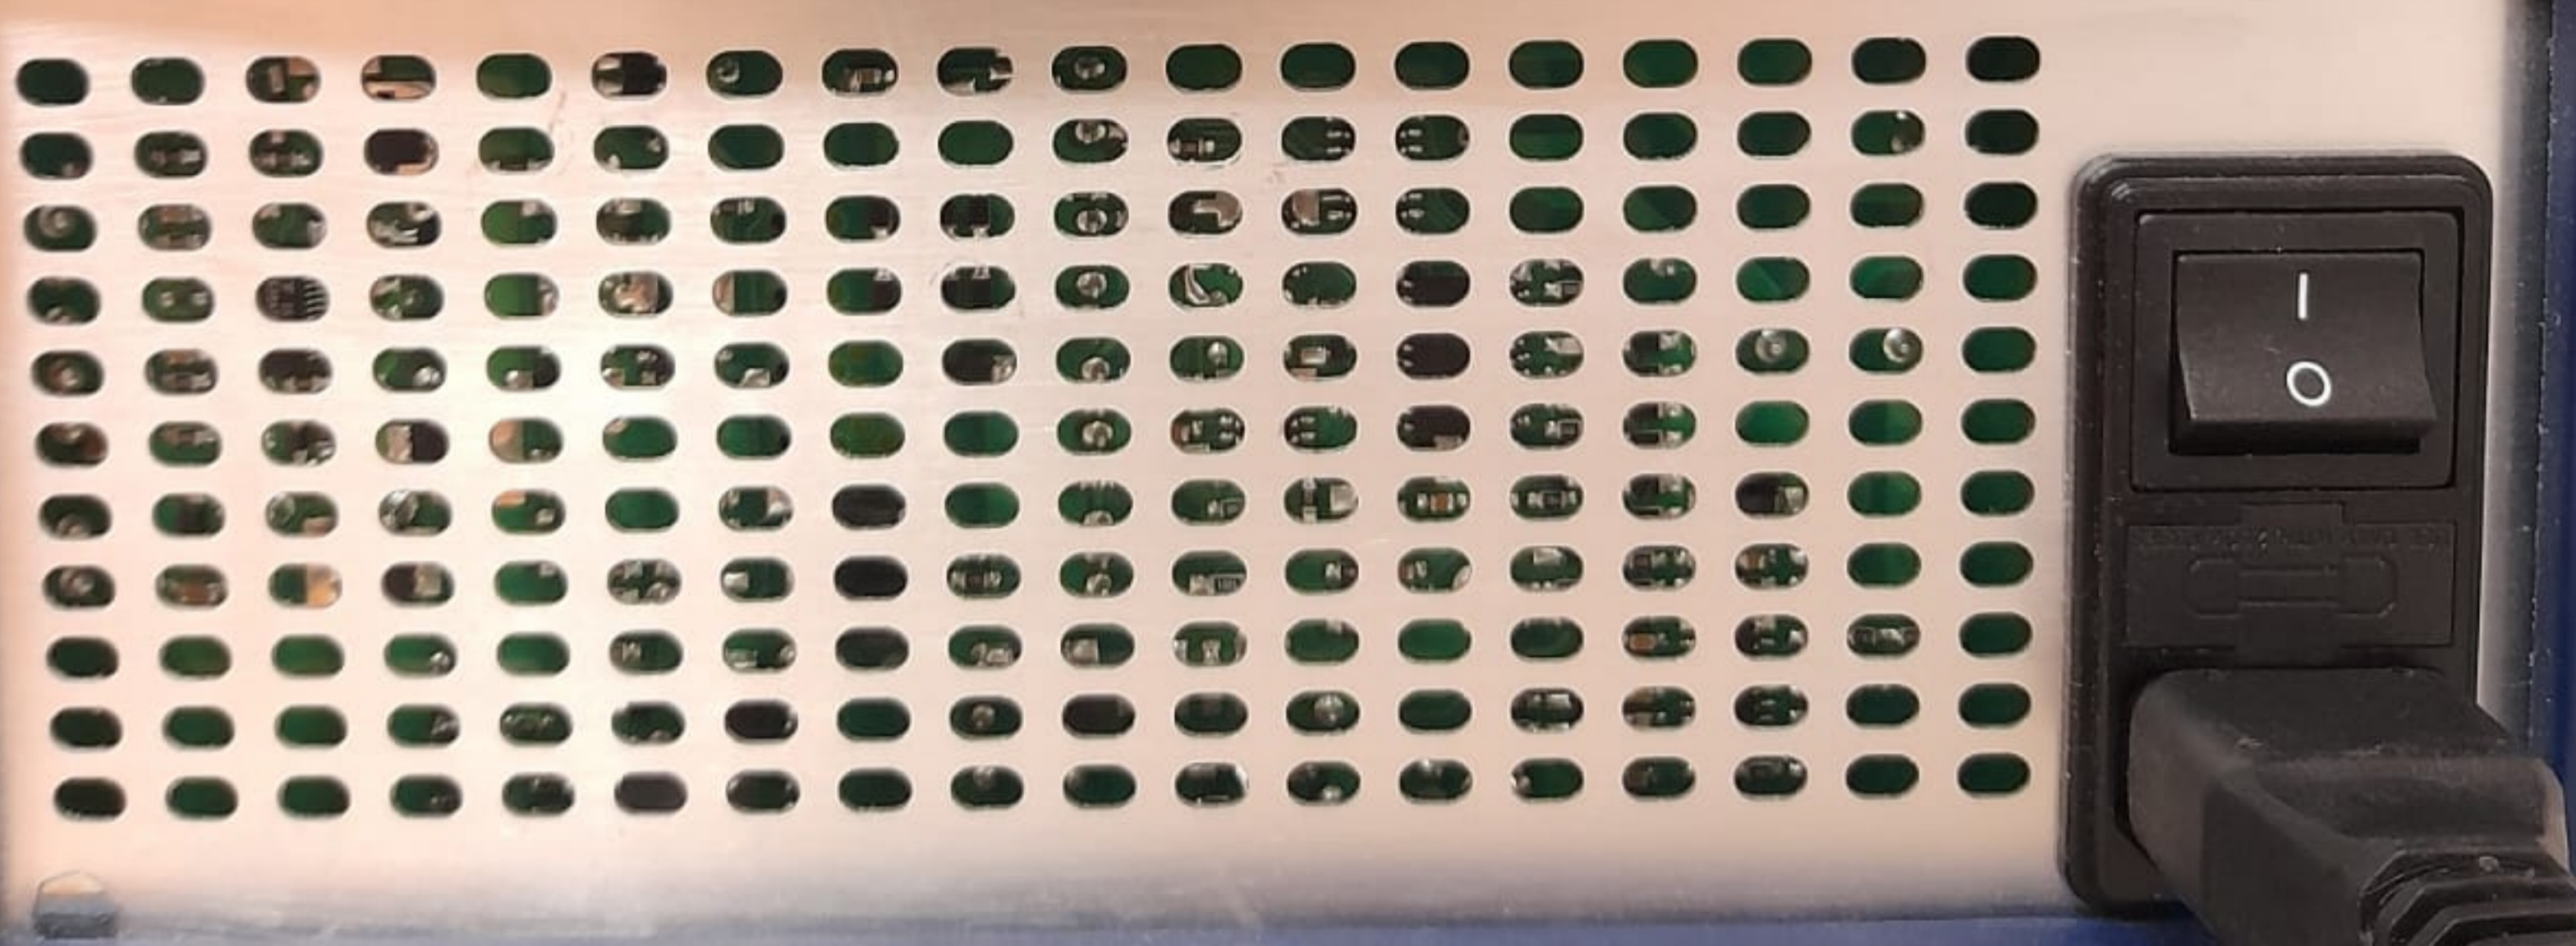

UDI - ABL90 FLEX  2020-11-24
LOT R1050N055

(01)05700693830909(10)R1050N055


ABL90 FLEX I393-090R1050N0055
A4-37447 uag 002