

	AE001-1	Adult ear clip sensor , DB9 Male, L=1M	sales@greatmade.com			
	AE001-3D	Adult ear clip sensor , DB9 Male, L=3M				
	AT001-1	Animal tongue clip sensor , DB9 Male, L=1M				
	AT001-3D	Animal tongue clip sensor , DB9 Male, L=3M				
	NW001-3D- Y	Multi-site Y cable with separate wrap , L=3m , DB9 , Wrap Detachable				
	NW 001-3D- F	Adult/ Neonate multi-site spo2 sensor ,with FOAM wrap tape, DB9 , L=3m				

Compatibilities: Compatible with BCI 3300, 3301, 3302,3303, 3304, 3401



Biosys (Korea) compatible spo2 sensor

Compatible Brand	OEM P/N	Greatmade P/N	Description(Connector, Length)	1-5 pcs	6-19 pcs	above 20 PCS
Biosys		AF002	Adult finger clip sensor , MD6M , L=3m			
		PF002	Pediatric finger clip sensor , MD6M , L=3m			
		AS002	Adult silicone soft tip sensor , MD6M , L=3m			
		PS002	Pediatric silicone soft tip sensor , MD6M , L=3m			
		NW002	Neonate silicone wrap sensor , MD6M , L=3m ,Non-detachable			
		AE002	Adult ear clip sensor , MD6M , L=3m			
		AT002	Animal tongue clip sensor , MD6M , L=3m			
		NW 002 Y	Multi-site Y cable with separate wrap ,MD6M, Wrap Detachable, L=3M			
		NW 002 F	Adult multi-site spo2 sensor ,with FOAM wrap tape,MD6M, L=3m			
			compatible with Biosys BPM-300			



Datex-Ohmeda Compatible reusable spo2 sensor

Compatible Brand	OEM P/N	Greatmade P/N	Description(Connector, Length)	1-5 pcs	6-19 pcs	above 20 PCS
Datex-Ohmeda See below compatibilities	OXY-F-UN	AF051	Adult finger clip sensor , 8pin Male , L=1M			
		PF051	pediatric finger clip sensor , 8pin Male , L=1M.			
		AS051	Adult silicone soft tip sensor , 8pin , Male , L=1M			
		PS051	Pediatric silicone soft tip sensor , 8pin Male , L=1M			
	OXY-W-UN	NW051	neonate silicone wrap sensor , 8pin Male , L=1M , Non-detachable			
	OXY-E-UN	AE051	Adult ear clip sensor , 8pin Male , L=1M			
		AT051	Animal tongue clip sensor , 8 pin Male , L=1M			
		NW051-Y	Multi-site Y cable with separate wrap,8pin male, Wrap Detachable			
		NW051- F	Adult/ Neonate multi-site spo2 sensor,8pin male,with FOAM wrap			
	Compatibilities :					


Use with Handheld pulse oximeters (Tuffsat, 3775)

Stand Alone pulse oximeter (37** series, 3800, 3900,3900P),respiratory gas monitors (4700, 5259RGM)

M-OSAT module , N-XOSAT option for Cardiocap.5 ; OEM patterning monitors ;


All S/5 monitors, all AS/3,CS/3 Monitors , Cardiocap , Capnomac Ultima and Satlite

Require Adapter EX043 or EX044 or EX042

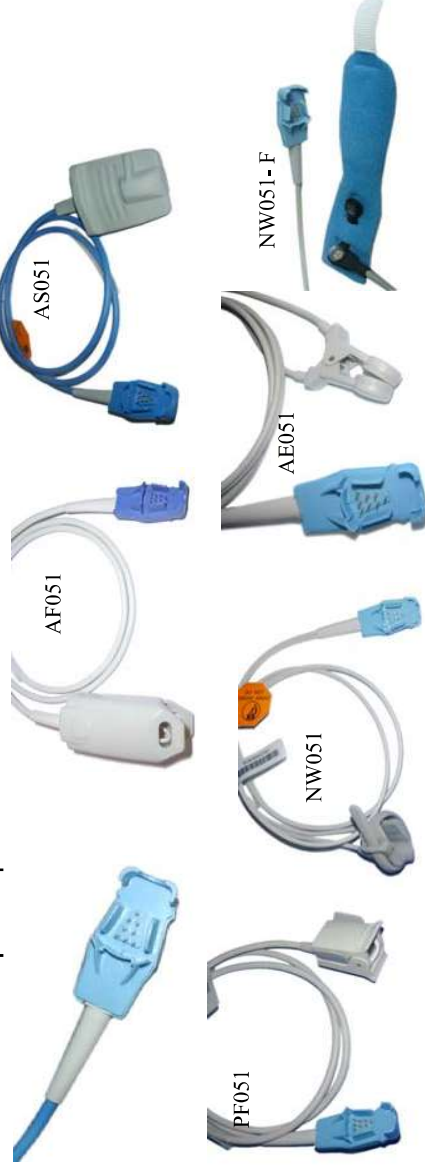


Datex-Ohmeda Compatible reusable spo2 sensor

Compatible Brand	OEM P/N	Greatmade P/N	Description(Connector, Length)	1-5 pcs	6-19 pcs	above 20 PCS
Datex-Ohmeda Trusat Pulse Oximeter	OXY-F4-MC	AF063	Adult finger clip sensor , DB9 Male , L=3M			
		PF063	pediatric finger clip sensor , DB9 Male , L=3M			
		AS063	Adult silicone soft tip sensor , DB9 Male , L=3M			
		PS063	Pediatric silicone soft tip sensor , DB9 Male , L=3M			
	OXY-W4-MC	NW063	neonate silicone wrap sensor , DB9 Male , L=3M , Non-detachable			
	OXY-E4-MC	AE063	Adult ear clip sensor DB9 Male L=3M			
		AT063	Animal tongue clip sensor , DB9 Male , L=3M			
		NW063-Y	Multi-site Y cable with separate wrap,DB9 male, Wrap Detachable			
		NW063- F	Adult/ Neonate multi-site spo2 sensor,DB9 male,with FOAM wrap			
	Compatibilities :					

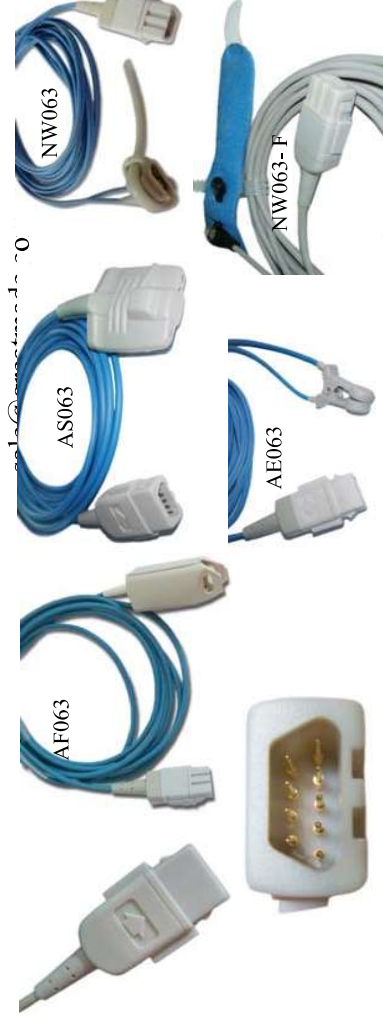

GE-Marquette Compatible reusable spo2 sensor

Compatible Brand	OEM P/N	Greatmade P/N	Description(Connector, Length)	1-5 pcs	6-19 pcs	above 20 PCS
GE Dash ,Solar eagle , Tram Cardiolab/Med-lab Nellcor Non-Oximax tech		AF039	Adult finger clip sensor, 11PIN Male blue flat ,L=3m			
		PF039	Pediatric finger clip sensor, 11PIN Male blue flat ,L=3m			
		AS039	Adult silicone soft tip sensor, 11PIN Male blue flat ,L=3m			
		PS039	Pediatric silicone soft tip sensor, 11PIN Male blue flat ,L=3m			
		NW039	Neonate silicone wrap sensor, 11PIN Male blue flat ,L=3m, Non-detachable			
		AE039	Adult ear clip sensor, 11PIN Male blue flat ,L=3m			
		AT039	Animal tongue clip sensor, 11PIN Male blue flat ,L=3m			
		NW039-Y	Multi-site Y cable with separate wrap, 11pin flat, Wrap Detachable			
		NW039- F	Adult/ Neonate multi-site spo2 sensor, 11pin flat, with FOAM wrap			

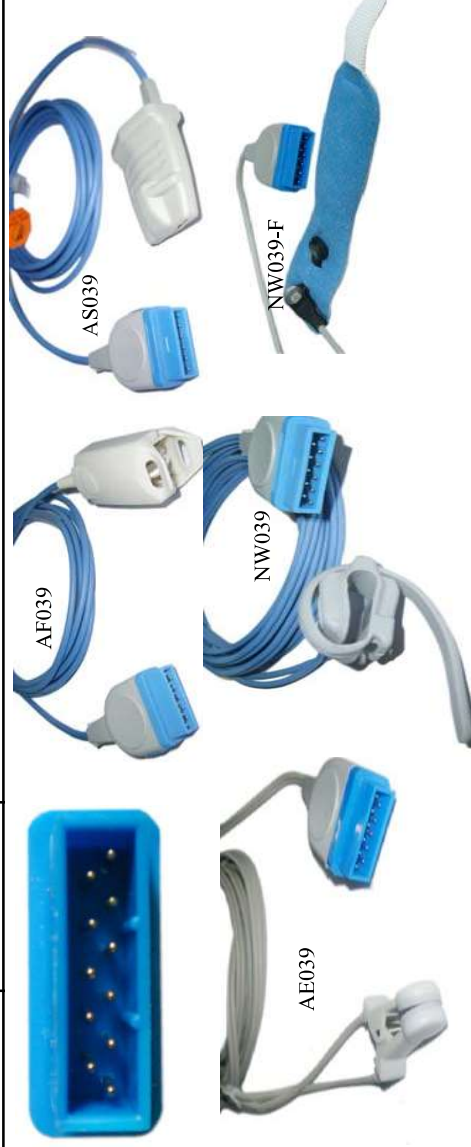

Compatible Brand	OEM P/N	Greatmade P/N	Description(Connector, Length)	1-5 pcs	6-19 pcs	above 20 PCS
GE Dash ,Solar eagle , Tram Cardiolab/Med-lab	LNC5-DCH-LNC-10-GE	AF011M	Adult finger clip sensor, 11PIN Male blue flat ,L=3m			
		PF011M	Pediatric finger clip sensor, 11PIN Male blue flat ,L=3m			
		AS11M	Adult silicone soft tip sensor, 11PIN Male blue flat ,L=3m			



Limb Electrode

OEM P/N	Greatmade No.		1-5 sets	6-19 sets	Above 20sets
	EC012	Limb Electrode (4pcs/set) Perfect for 3.0 plug , IEC, (RED ,Yellow , Green , Black)			
	EC012B	Limb Electrode (4pcs/set) Perfect for 4.0 Banana , IEC, (RED ,Yellow , Green , Black)			
	EC012C	Multi-use Limb Electrode for all types of ECG electrode, Metal plating AgCl (Dark), IEC			
	EC012C-S	Multi-use Limb Electrode for all types of ECG electrode, Metal plating Nickel (Shine), IEC			
	EC012-A	Limb Electrode (4pcs/set) Perfect for 3.0 DIN , AHA, (RED, Green, White, Black)			
	EC012B/A	Limb Electrode (4pcs/set) Perfect for 4.0 Banana , AHA, (RED, Green, White, Black)			
	EC012C/A	Multi-use Limb Electrode for all types of ECG electrode , Metal plating AgCl (Dark), AHA			
	EC012C-SA	Multi-use Limb Electrode for all types of ECG electrode , Metal plating Nickel (Shine) , AHA			



EC012A Suitable for all 3.0 Din Plug of EKG Cable

EC012B Suitable for All 4.0 Banana Plug of EKG Cable .

EC012C Suitable for All 4.0 Banana , 3.0DIN, Snap, Grabber electrode


Limb Electrode

OEM P/N	Greatmade No.	Description (Cable and connector)	1-5 pcs	6-19pcs	Above 20pcs
	EC012A-HP	Limb Electrode (4pcs/set) Perfect for 3.0 DIN , IEC, (Red, Green, Yellow, Black)			
	EC012B-HP	Limb Electrode (4pcs/set) Perfect for 4.0 Banana , IEC, (Red, Green, Yellow, Black)			
	EC012C-HP	Multi-use Limb Electrode for all types of ECG electrode, Metal plating AgCl (Dark), IEC			
	EC012D-HP	Multi-use Limb Electrode for all types of ECG electrode, Metal plating Nickel (Shine), IEC			

Suction Electrode

OEM P/N	Greatmade No.	Description (Cable and connector)	1-5pcs	6-19pcs	Above 20pcs
	EC013A	Adult Suction Electrodes (6 pcs/Set), perfect for 3.0 DIN , Silicone			
	EC013B	Adult Suction Electrodes (6 pcs/ Set), perfect for 4.0 Banana ,silicone			
	EC013A/B	Adult Suction electrodes (6 pcs/ set) , for both 3.0 and 4.0, silicone			
	EC013C	Adult Multi use electrode , 3.0, 4.0 ,Snap , grabber ,Metal PLATING AgCl (Dark)			
	EC013C-S	Adult multi use electrode,3.0,4.0,Snap,grabber,Metal PLATING Nickel(Shine)			
	EC013D	Pediatric Suction Electrode (6pcs/set) , suitable for 3.0 DIN plug			
	EC013E	Pediatric Suction Electrode (6pcs/set) , suitable for 4.0 banana			
	EC013F	Pediatric Multi-use Electrode(6 pcs/set),for 3.0 , 4.0 , Snap , Grabber . Plating AgCl(Dark)			
	EC013F-S	Pediatric Multi-use Electrode(6 pcs/set),for 3.0,4.0,Snap,Grabber,plating Nickel(Shine)			
	EC013G	Pediatric suction Electrodes (6pcs/set) , suitable for both 3.0 and 4.0			

EC013C



EC013A Suitable for all 3.0mm DIN plug for EKG cable

EC013B Suitable for All 4.0 Banana Plug of EKG Cable .

EC013C For Multi-use , Suitable for all 3.0DIN , 4.0 Banana , Snap and Grabber

EC013A/B is suitable forboth 3.0 and 4.0 banana plug

EC013A/B: Metal diameter : 21mm ,Ball diameter :26mm

C013C Metal diameter : 24mm , Ball diameter : 32mm

C013D/E Metal diameter :17mm, Ball diameter :23mm

EC013D



EC013A/B



EC013F



EC013G



EKG Cable Electrode Adapter

OEM P/N	Greatmade No.	Description (Cable and connector)	1-5pcs	6-19pcs	Above 20pcs
	EC018A	Electrode Adapter , 3.0DIN-> Snap , L=10CM			
	EC018B	Electrode Adapter , 4.0 Banana -> Snap , L=10CM			
	EC018C	Electrode Adapter , 3.0DIN->Grabber, L=10CM			
	EC018D	Electrode Adapter , 4.0 Banana-> Grabber , L=10CM			
	EC018E	Electrode Adapter , 4.0 Banana socket ->3.0 DIN Plug, L=10CM			
	EC018F	Electrode Adapter , 3.0DIN socket->4.0 Banana plug, L=10CM			

HK GREATMADE TECH LTD

Keep pace with your need

Contact: Shirley Wang
 E-mail : info@greatmade.com , sales@greatmade.com
 Website : <http://www.greatmade.com> , www.greatmade.diytrade.com
 Tel : [86-0755-28144774](tel:86-0755-28144774) , *Fax* : [86-0755-27185453](tel:86-0755-27185453)
 Hotmail : greatmade@hotmail.com
 Skype : Greatmade01

**Reusable/Disposable NIBP Cuff and Air Hose
 (Updated on April ,2012)**

NIBP CUFF

Greatmade P/N	Description (Cable , Connector)	Unit Price
CF001A	Neonate Single tube NIBP cuff , 6-11cm Arm Circumference	
CF002A	Infant single tube NIBP cuff , 10-19cm Arm Circumference	
CF003A	Child single tube NIBP cuff , 18-26cm Arm Circumference	
CF004A	Adult single tube NIBP cuff , 25-35cm Arm Circumference	
CF004LA	Large Adult Single Tube Nibp Cuff , 33-47cm Arm Circumference	
CF004TA	THIGH Single Tube Nibp Cuff , 46-66cm Arm Circumference	

**NIBP Cuff**

Greatmade P/N	Description (Cable , Connector)	Unit Price
CF001B	Neonate Dual tube NIBP cuff , 6-11cm Arm Circumference	
CF002B	Infant dual tube NIBP cuff , 10-19cm Arm Circumference	
CF003B	Child dual tube NIBP cuff , 18-26cm Arm Circumference	
CF004B	Adult dual tube NIBP cuff , 25-35cm Arm Circumference	
CF004LB	Large Adult Dual Tube Nibp Cuff , 33-47cm Arm Circumference	
CF004TB	THIGH Dual tube NIBP Cuff, 46-66cm Arm Circumference	



Adult Longer Type

CF004XL-A	Adult Long Single tube Nibp Cuff , 33-47cm Arm circumference ,L 690mm*W 145mm	
CF004XL-B	Adult Long Dual tube Nibp Cuff , 33-47cm Arm Circumference .	



EC Certificate

Full Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex II excluding (4)
(Devices in Class IIa, IIb or III)

No. G1 17 12 02231 002

Manufacturer: Shenzhen Greatmade Tech limited

3rd Floor, Building B
Baifuli Industrial Zone, Shanghenglang
Huahui Road, Dalang Street
Longhua New District
518109 Shenzhen, Guangdong Province
PEOPLE'S REPUBLIC OF CHINA



EC-Representative: Prolinx GmbH

Brehmstr. 56
40239 Duesseldorf
GERMANY

Product Category(ies): Spo2 sensor

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for design, manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex II. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class III devices an additional Annex II (4) certificate is mandatory. See also notes overleaf.

Report No.: GZ1728501

Valid from: 2018-04-11
Valid until: 2023-04-10

Date, 2018-04-11

I. Preiß
Stefan Preiß



TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 2

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



A1 / 07-09



Product Service

EC Certificate

Full Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex II excluding (4)
(Devices in Class IIa, IIb or III)

No. G1 17 12 02231 002

Facility(ies):

Shenzhen Greatmade Tech limited
3rd Floor, Building B, Baifuli Industrial Zone, Shanghenglang,
Huahui Road, Dalang Street, Longhua New District, 518109
Shenzhen, Guangdong Province, PEOPLE'S REPUBLIC OF
CHINA

Page 2 of 2

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



DANKE CERT / 18-13



Product Service

CERTIFICATE

No. Q1N 17 12 02231 001

Holder of Certificate: Shenzhen Greatmade Tech limited

3rd Floor, Building B
Baifuli Industrial Zone, Shanghenglang
Huahui Road, Dalang Street
Longhua New District
518109 Shenzhen, Guangdong Province
PEOPLE'S REPUBLIC OF CHINA

Facility(ies):

Shenzhen Greatmade Tech limited
3rd Floor, Building B, Baifuli Industrial Zone,
Shanghenglang, Huahui Road, Dalang Street,
Longhua New District, 518109 Shenzhen,
Guangdong Province, PEOPLE'S REPUBLIC OF
CHINA



Certification Mark:



Scope of Certificate: Design and Development, Production
and Distribution of Spo2 sensor,
Patient cable and leadwire, Blood pressure cuff

Applied Standard(s):

EN ISO 13485:2012 + AC:2012
Medical devices - Quality management systems -
Requirements for regulatory purposes
(ISO 13485:2003 + Cor. 1:2009)
DIN EN ISO 13485:2012
Upgrade required until 2019-03-31

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). See also notes overleaf.

Report No.: GZ1728501

Valid from: 2018-04-11
Valid until: 2021-04-10

Date, 2018-04-11

I. Preiß
Stefan Preiß



Page 1 of 1

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany

