

Allure™ RF

Cardiac Resynchronisation Therapy Pacemaker

Merlin@home™
Transmitter
Compatible

Product Highlights

- Angled header and physiologic tear drop shape provide better lead wrap
- CorVue™ Congestion Monitoring feature monitors the intrathoracic impedance and provides the option for both patient and physician alerts
- The DirectTrend™ Report provides a summary of three month daily, one year weekly or one year daily diagnostic trends
- Better patient utilization from Day 1 when paired with the Merlin@home™ transmitter at point of care
- AT/AF Alerts can be programmed to notify patients and their clinics when a programmed AT/AF threshold or continuous episode duration has been exceeded, or when a high ventricular rate accompanies the AT/AF episode
- Exclusive AF Suppression™ algorithm is clinically proven to suppress episodes of paroxysmal and persistent AF
- AT/AF burden trend provides a graphical representation of the percentage of time in AT/AF and the number of AT/AF episodes in the previous 52 weeks
- Up to 14 minutes of stored electrograms help identify key intrinsic and pacemaker-related events and simplify the diagnosis of complex ECG rhythms associated with heart failure
- Industry-leading longevity offers 8.2 years of service life supported by a 6 year warranty*

Ordering Information

Contents: Cardiac pulse generator

Model Number	Dimensions (H x W x T, mm)	Weight (g)	Volume (cc)	Connector
PM3222	55 x 59 x 6	24	14	IS-1

*Longevity calculated based on the following settings: 2.5 V, 500 Ohm, 60 BPM, 100% DDD-BiV Pacing, 0.4ms, Cap Confirm Off, and Stored EGM On

Indications: Implantation of Allure and Allure RF devices is indicated for: maintaining synchrony of the left and right ventricles in patients who have undergone an AV nodal ablation for chronic atrial fibrillation and have NYHA Class II or III heart failure, the reduction of the symptoms of moderate to severe heart failure (NYHA Class III or IV) in those patients who remain symptomatic despite stable, optimal medical therapy, and have a left ventricular ejection fraction \leq 35% and a prolonged QRS duration, implantation of Assurity, Endurity and Allure family of devices is indicated in one or more of the following permanent conditions: syncope, presyncope, fatigue, disorientation, or any combination of those symptoms. **Rate-Modulated Pacing** is indicated for patients with chronotropic incompetence, and for those who would benefit from increased stimulation rates concurrent with physical activity. **Dual-Chamber Pacing** is indicated for those patients exhibiting: sick sinus syndrome, chronic, symptomatic second- and third-degree AV block, recurrent Adams-Stokes syndrome, symptomatic bilateral bundle branch block when tachyarrhythmia and other causes have been ruled out. **Atrial Pacing** is indicated for patients with sinus node dysfunction and normal AV and intraventricular conduction systems. **Ventricular Pacing** is indicated for patients with significant bradycardia and normal sinus rhythm with only rare episodes of A-V block or sinus arrest, chronic atrial fibrillation, severe physical disability. **AF Suppression** algorithm is indicated for suppression of paroxysmal or persistent atrial fibrillation episodes in patients with one or more of the above pacing indications.

Contraindications: Implanted Cardioverter-Defibrillator (ICD). Devices are contraindicated in patients with an implanted cardioverter-defibrillator. Rate-Adaptive Pacing may be inappropriate for patients who experience angina or other symptoms of myocardial dysfunction at higher sensor-driven rates. An appropriate Maximum Sensor Rate should be selected based on assessment of the highest stimulation rate tolerated by the patient. AF Suppression stimulation is not recommended in patients who cannot tolerate high atrial-rate stimulation. **Dual-Chamber Pacing**, though not contraindicated for patients with chronic atrial flutter, chronic atrial fibrillation, or silent atria, may provide no benefit beyond that of single-chamber pacing in such

patients. **Single-Chamber Ventricular Demand Pacing** is relatively contraindicated in patients who have demonstrated pacemaker syndrome, have retrograde VA conduction, or suffer a drop in arterial blood pressure with the onset of ventricular pacing. **Single-Chamber Atrial Pacing** is relatively contraindicated in patients who have demonstrated compromise of AV conduction. **Atrial Fibrillation**. Anthem devices are contraindicated in patients having chronic atrial fibrillation or intermittent atrial fibrillation that does not terminate. For specific contraindications associated with individual modes, refer to the programmer's on-screen help.

Potential Adverse Events: The following are potential complications associated with the use of any pacing system: air embolism, body rejection phenomena, cardiac tamponade or perforation, hematoma, bleeding, hematoma, seroma, formation of fibrotic tissue, local tissue reaction, inability to interrogate or program due to programmer or device malfunction, infection/erosion, interruption of desired pulse generator function due to electrical interference, either electromyogenic or electromagnetic, lead malfunction due to conductor fracture or insulation degradation, loss of capture or sensing due to lead dislodgement or reaction at the electrode/tissue interface, loss of desired pacing and/or sensing due to lead displacement, body reaction at electrode interface, or lead malfunction (fracture or damage to insulation), loss of normal device function due to battery failure or component malfunction, pacemaker migration or pocket erosion, pectoral muscle or diaphragmatic stimulation, phrenic nerve stimulation, pneumothorax/hemothorax, endocarditis, excessive bleeding, induced atrial or ventricular arrhythmias, myocardial irritability, pericardial effusion, pericardial rub, pulmonary edema, rise in threshold and exit block, valve damage, cardiac/coronary sinus dissection, cardiac/coronary sinus perforation, coronary sinus or cardiac vein thrombosis.

Refer to the User's Manual for detailed indications, contraindications, warnings, precautions and potential adverse events.

Customer Support: 46-8-474-4756

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country. Unless otherwise noted, ™ indicates that the name is a trademark of, or licensed to, St. Jude Medical or one of its subsidiaries. ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK. are registered and unregistered trademarks and service marks of St. Jude Medical, Inc. and its related companies. ©2013 St. Jude Medical, Inc. All rights reserved.

Allure™ RF

Cardiac Resynchronisation Therapy Pacemaker

Product Specifications

PHYSICAL SPECIFICATIONS

Model	PM3222
Telemetry	RF
Dimensions (mm)	55 x 59 x 6
Weight (g)	24
Volume (cc) ¹	14
Connector	IS-1

PARAMETER SETTINGS

Resynchronisation Therapy

QuickOpt™ Timing Cycle Optimisation	Sensed/Paced AV Delay; Interventricular Paced Delay
RV and LV Pulse Width (ms)	0.05; 0.1–1.5 in steps of 0.1
RV and LV Pulse Amplitude (V)	0.25–4.0 in steps of 0.25; 4.5–7.5 in steps of 0.5
RV Pulse Configuration	Unipolar; Bipolar
LV Pulse Configuration	Unipolar; Bipolar; LV Tip–RV Ring; LV Ring–RV Ring
Ventricular Sense Configuration	BV Unipolar Tip; BV Bipolar; RV Unipolar Tip; RV Bipolar; LV Unipolar Tip; LV Bipolar; RV Unipolar Ring; LV Tip–RV Tip
Ventricular Pacing Chamber	BV; RV only; LV only (temporary mode)
First Chamber Paced	Simultaneous ² ; RV; LV
Interventricular Pace Delay (ms)	10–80 in steps of 5

Output/Sensing

Negative AV Hysteresis Search (ms)	Off; -10 to -120 in steps of 10
Shortest AV/PV Delay (ms)	25–50 in steps of 5; 60–120 in steps of 10
Atrial ACap™ Confirm	On; Off; Monitor
Primary Pulse Confirmation	Bipolar
Backup Pulse Confirmation	Bipolar
Backup Pulse Amplitude (V)	5.0
Searchable Intervals (hrs)	8; 24
Atrial Pulse Configuration	Unipolar (tip–case); Bipolar (tip–ring)
Atrial Sense Configuration	Unipolar Tip (tip–case); Bipolar (tip–ring); Unipolar Ring (ring–case)
Atrial Sensitivity ^{3,4} (Fixed) (mV)	0.1–0.5 in steps of 0.1; 0.75–2.0 in steps of 0.25; 2.5–5.0 in steps of 0.5
Atrial Pulse Amplitude (V)	0.25–4.0 in steps of 0.25; 4.5–7.5 in steps of 0.5
Atrial Pulse Width (ms)	0.05; 0.1–1.5 in steps of 0.1
RVCap™ Confirm	On; Off; Monitor
Searchable Interval (hrs)	8; 24
LVCap™ Confirm	On; Off; Monitor
Searchable Interval (hrs)	8; 24
SenseAbility™ Technology	Off; On (Automatic Sensitivity Control adjustment for atrial and ventricular events)
A Max Sensitivity (mV)	0.2–1.0 in steps of 0.1
V Max Sensitivity (mV)	0.2–2.0 in steps of 0.1
Threshold Start	(Atrial and Ventricular Post-Sense) 50; 62.5; 75; 100% (Atrial Post-Pace) 0.2–3.0 in steps of 0.1 mV (Ventricular Post-Pace) Auto; 0.2–3.0 in steps of 0.1 mV (Atrial and Ventricular Post-Sense) 0; 30; 60; 95; 125; 160; 190; 220 (Atrial Post-Pace) 0; 30; 60; 95; 125; 160; 190; 220 (Ventricular Post-Pace) Auto; 0; 30; 60; 95; 125; 160; 190; 220
Decay Delay (ms)	0.5–12.5 in steps of 0.5 ^{5,6}
Ventricular Sensitivity (fixed) (mV)	0.5–12.5 in steps of 0.5 ^{5,6}

Rate/Timing

Mode	A00(R); AAI(R); AAT(R); V00(R); VVI(R); VVT(R); D00(R); DVI(R); DD(R); DDT(R); DDD(R); VDD(R); Pacing Off
DDT Trigger ⁵	R wave
DDT Timing ⁵	DDI
Base Rate (min ⁻¹)	30–130 in steps of 5; 140–170 in steps of 10
Hysteresis Rate (min ⁻¹)	Off; 30–150 in steps of 5 ⁶
Search Interval (min)	Off; 1; 5; 10; 15; 30
Cycle Count	1–16
Intervention Rate (min ⁻¹)	Off; Same Base Rate; 80–120 in steps of 10 (Intrinsic +0; Intrinsic +10; Intrinsic +20; Intrinsic +30)
Intervention Duration (min ⁻¹)	1–10
Recovery Time	Fast; Medium; Slow; Very Slow
Rest Rate (min ⁻¹)	Off; 30–150 in steps of 5
Maximum Tracking Rate (min ⁻¹)	90–130 in steps of 5; 140–180 in steps of 10
Sensed AV Delay (ms)	25; 30–200 in steps of 10; 225–325 in steps of 25
Paced AV Delay (ms)	25; 30–200 in steps of 10; 225–300 in steps of 25; 350
Ventricular Pace/Sense Refractory ⁷ (Fixed) (ms)	125; 160–400 in steps of 30; 440; 470 ⁸
Atrial Pace Refractory	190–400 in steps of 30; 440; 470 ⁸
Atrial Sense Refractory	93; 125; 157; 190–400 in steps of 30; 440; 470 ⁸
PVARP (ms)	125–500 in steps of 25
Atrial Protection Interval (ms) ⁵	125
Far-Field Protection Interval (ms) ⁵	16

1 ± 0.5 cc
 2 LV first with 10 ms interventricular delay.
 3 Sensitivity is with respect to a 20 ms haversine test signal.
 4 Values 0.1–0.4 not available in a Unipolar Sense Configuration.
 5 This parameter is not programmable.
 6 The highest available setting for hysteresis rate is 5 min⁻¹ below the programmed base rate.
 7 In dual-chamber modes, the maximum Ventricular Refractory Period is 325 ms.
 8 Programming options dependent on pacing mode.
 9 During atrial NIPS in dual-chamber modes, the shortest Coupling Interval will be limited by the programmed AV/PV Delay.
 10 S1 Burst Cycle is applied at the preprogrammed S1 cycle length.

Customer Support: 46-8-474-4756

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country. Unless otherwise noted, ™ indicates that the name is a trademark of, or licensed to, St. Jude Medical or one of its subsidiaries. ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK. are registered and unregistered trademarks and service marks of St. Jude Medical, Inc. and its related companies. ©2013 St. Jude Medical, Inc. All rights reserved.

Item GMCRM1094EN

Rate-Modulated

Rate Responsive AV/PV Delay	Off; Low; Medium; High
Rate Responsive PVARP/VREF	Off; Low; Medium; High
Shortest PVARP/VREF	125–475 in steps of 25
Sensor	On; Off; Passive
Max Sensor Rate (min ⁻¹)	80–150 in steps of 5; 160–180 in steps of 10
Threshold	Auto (-0.5); Auto (+0.0); Auto (+0.5); Auto (+1.0); Auto (+1.5); Auto (+2.0); 1–7 in steps of 0.5
Slope	Auto (-1); Auto (+0); Auto (+1); Auto (+2); Auto (+3); 1–16
Reaction Time	Very Fast; Fast; Medium; Slow
Recovery Time	Fast; Medium; Slow; Very Slow

AF Management

AF Suppression™ Algorithm	Off; On
Lower Rate Overdrive (min ⁻¹) ⁵	10
Upper Rate Overdrive (min ⁻¹) ⁵	5
No. of Overdrive Pacing Cycles	15–40 in steps of 5
Rate Recovery (ms)	8; 12
Auto Mode Switch	Off; DDD(R) to DDI(R); DDD(R) to DDT(R); DDD(R) to VVI(R); DDD(R) to VVT(R); VDD(R) to VVI(R); VDD(R) to VVTR(R)
AMS Base Rate (min ⁻¹)	40–170 in steps of 5

Stored Electrograms

Options	
Priority Options	Off; Low; High
Channel	1; 2; 3
Triggers	
Advanced Hysteresis	Off; Low; High
AMS Entry/AMS Exit	Off; Low; High
AT/AF Detection	Off; Low; High
Magnet Response	Off; Low; High
High Atrial Rate Rate (min ⁻¹)	125–300 in steps of 25
No. of Consecutive Cycles	2; 3; 4; 5; 10; 15; 20
High Ventricular Rate Rate (min ⁻¹)	125–300 in steps of 25
No. of Consecutive Cycles	2; 3; 4; 5; 10; 15; 20
PMT Termination	Off; Low; High
Consecutive PVCs	Off; Low; High
No. of Consecutive PVCs	2; 3; 4; 5
Noise Reversion	Off; Low; High

Other

Magnet Response	Off; Battery Test
Ventricular Intrinsic Preference, VIP™ (ms)	Off; 50–150 in steps of 25; 160–200 in steps of 10
VIP Search Interval	30 sec.; 1; 3; 5; 10; 30 min.
VIP Search Cycles of the Atrial Tachycardia Detection Rate (min ⁻¹)	1; 2; 3
Post Vent. Atrial Blanking (PVAB) (ms)	110–200 in steps of 10; 225–300 in steps of 25
Ventricular Safety Standby (PVC Response)	60–200 in steps of 10; 225; 250
PVC Response	Off; On
PMT Options	Off; Atrial Pace ⁸
PMT Detection Rate (min ⁻¹)	Off; Passive; Atrial Pace ⁸
Lead Type	90–180 in steps of 5
NIPS Options	Uncoded; Unipolar; Bipolar
Stimulation Chamber Coupling Interval ⁹ (ms)	Atrial; Right Ventricular
S1 Count	200–800 in steps of 10
S1 ¹⁰ ; S2; S3 and S4 Cycle (ms)	2–25 in steps of 1
Right Ventricular Support Rate (min ⁻¹)	Off; 100–800 in steps of 10 (Fixed or Adaptive)
Sinus Node Recovery Delay (s)	Off; 30–95 in steps of 5
Diagnostic Trends	1–5 in steps of 1
CorVue™ Congestion Monitoring	AT/AF Activity; Exercise; Lead Impedance; P and R Wave; A and V threshold; CorVue™ Congestion Monitoring
CorVue Congestion Trigger	Off; On
	8–18 days

Patient Notifiers

Programmable Notifiers (On; Off)	Device at ERI; Atrial Lead Impedance Out of Range; Ventricular Lead Impedance Out of Range; LV Lead Impedance Out of Range; AT/AF Burden; AT/AF Episode Duration; High V Rate During AT/AF; High V Rate; Percent BIV/RV Pacing Alert; CorVue Alert
Device Reset	On
Entry into Backup VVI Mode	On
Audible Duration (sec)	2; 4; 6; 8; 10; 12; 14; 16
Number of Audible Alerts per Notification	2
Number of Notifications	1–16
Time Between Notifications (hours)	10; 22

Tendril™ STS

Pacing Lead

Product Highlights - Pacing Lead

- The Tendril STS lead allows patients to undergo MRI scans when used in conjunction with a MRI Ready pacemaker from St. Jude Medical
 - Allows MRI scans (See Parameter Settings for scan exclusion zone)
 - Permits a maximum whole body averaged specific absorption rate (SAR) of 2 watts per kilogram (W/kg)
- Soft silicone tip offers more compliance and less tip pressure at the lead tip-endocardium interface
- Small diameter lead offers improved ease of venous passage, reduced risk of venous thrombosis or rib-clavicle crush and ability to accommodate additional leads more easily
- Optim™ lead insulation—a chemical co-polymer that blends the best features of polyurethane and silicone for improved handling and increased durability
- Titanium nitride (TiN) fractal coating on the tip and ring electrodes is designed to promote precise sensing and to provide improved contact with the myocardium
- Lubricious Fast-Pass™ coating facilitates lead insertion through the introducer and veins to ease implantation
- Fits through a 6 F introducer



Ordering Information - MRI-Ready Pacing System

Model Number	Description	Insulation	Fixation	Min. Introducer (F)	Connector	Length (cm)
2088TC	Tendril™ STS Pacing Lead	Optim™	Ext/Ret helix	6	IS-1 bipolar	46*; 52*; 58*; 65; 100

* Indicates lead lengths that are MRI conditional with a scan exclusion zone.

Model Number	Description	Dimensions (H x W x T, mm)	Weight (g)	Volume (cc)	Connector
PM1140	Endurity™ Core Pacemaker	41 x 50 x 6	19	9,7 (± 0,5)	IS-1
PM2140	Endurity Core Pacemaker	46 x 50 x 6	19	10,4 (± 0,5)	IS-1
PM1152	Endurity Core Pacemaker	41 x 50 x 6	19	9,7 (± 0,5)	IS-1
PM2152	Endurity Core Pacemaker	46 x 50 x 6	19	10,4 (± 0,5)	IS-1
PM1162	Endurity Pacemaker	41 x 50 x 6	19	9,7 (± 0,5)	IS-1
PM2162	Endurity Pacemaker	46 x 50 x 6	19	10,4 (± 0,5)	IS-1
PM1172	Endurity MRI™ Pacemaker	41 x 50 x 6	19	9,7 (± 0,5)	IS-1
PM2172	Endurity MRI Pacemaker	46 x 50 x 6	19	10,4 (± 0,5)	IS-1
PM1272	Assurity MRI™ Pacemaker	47 x 50 x 6	20	10,4 (± 0,5)	IS-1
PM2272	Assurity MRI Pacemaker	47 x 50 x 6	20	10,4 (± 0,5)	IS-1

Indications: Tendril™ STS lead is designed for permanent sensing and pacing in either the right atrium or the right ventricle, in combination with a compatible device. Active leads such as the Tendril STS lead may be indicated for patients where permanent fixation of passive leads is suspected to be unstable.

In atrial applications, the use of screw-in leads such as Tendril STS lead may be indicated in the presence of an abnormal, surgically altered or excised atrial appendage.

Contraindications: Tendril STS lead is contraindicated: in the presence of tricuspid atresia, for patients with mechanical tricuspid valves, in patients who are expected to be hypersensitive to a single dose of one milligram of dexamethasone sodium phosphate.

Adverse Events: Potential complications associated with the use of Tendril STS lead are the same as with the use of other active fixation leads and include: cardiac tamponade, diaphragmatic stimulation, embolism, excessive bleeding, induced ventricular ectopy, infection, loss of pacing and/or sensing due to dislodgment or mechanical malfunction of the pacing lead, phrenic nerve stimulation, thrombosis. Complications reported with direct subclavian venipuncture include pneumothorax, hemothorax, laceration of the subclavian artery, arteriovenous fistula, neural damage, thoracic duct injury, cannulation of other vessels, massive hemorrhage and, rarely, death.

Refer to the User's Manual for detailed indications, contraindications, warnings, precautions and potential adverse events.

Tendril™ STS

Pacing Lead

Product Specifications - Pacing Leads

PHYSICAL SPECIFICATIONS

Model	2088TC
Minimum Introducer Size	6 F
Type of Lead	Active-fixation, bipolar, steroid-eluting, endocardial, pacing lead
Lead Connector	IS-1 bipolar
Lead Lengths	46; 52; 58; 65; 100 cm
Fixation Mechanism	Extendable/Retractable helix
Typical Number of Rotations for Helix Extension	6-11 (straight stylet)
Lead Body Diameter	1.9 mm (max)
Tip-to-Ring Spacing	10 mm
Lead Tip Electrode (Cathode)	Active titanium-nitride-coated Pt/Ir helix (2,0 mm extension)
Tip Electrode Surface Area	6.9 mm ²
Ring Electrode (Anode)	Titanium-nitride-coated Pt/Ir
Ring Electrode Surface Area	16 mm ²
Mapping	Capable with titanium-nitride-coated Pt/Ir helix
Steroid	< 1 mg dexamethasone sodium phosphate
Inner Conductor/Outer Conductor	MP35N™* coil
Inner Insulation	Silicone rubber
Outer Insulation	Optim™ lead insulation
Lead Body Coating	Fast-Pass™ coating

In Pack

Straight stylets	1 x-soft in lead; 1 x-soft; 1 soft
J-curved stylets	2 soft
Helix extension/retraction clip-on tools	2 clip-on tools

Accessory Kits

Available Separately	Model Number	Compatible Lengths	Description
Stylet Kit	DS06002 with appropriate length designation	46; 52; 58; 65; 100 cm	1 fixation tool; 1 clip-on tool; 1 J-shaped soft; 1 x-soft; 1 soft; 1 firm; 1 x-firm
	DS06003 with appropriate length designation	46; 52; 58; 65; 100 cm	1 clip-on tool; 1 J-shaped soft; 1 x-soft; 1 soft; 1 firm; 1 x-firm
Locator™ Plus Deflectable Stylet	1281 with appropriate length designation	46; 52; 58; 65 cm	Disposable implant tool to facilitate precise lead positioning and manipulation with one hand
	1292 with appropriate length designation	46; 52; 58; 65 cm	

MRI Conditional Parameters

Magnet strength: 1.5 Tesla

SAR: ≤ 2 W/kg

Scan region: Isocenter must be inferior to L4 or 10 cm superior to C1



*MP35N is a trademark of SPS Technologies, Inc.

Customer Support: 46-8-474-4756

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country.

Unless otherwise noted, ™ indicates that the name is a trademark of, or licensed to, St. Jude Medical or one of its subsidiaries. ST. JUDE MEDICAL and the nine-squares symbol are trademarks and service marks of St. Jude Medical, Inc. and its related companies. © 2015 St. Jude Medical, Inc. All Rights Reserved.

SJM-TND-1214-0003 | This document is for International use only.

QuickFlex™ μ

4F Bipolar, Optim™ Insulation-Insulated, Left Ventricular Pacing Lead

MODEL 1258T



SPECIFICATIONS

St. Jude Medical's innovative QuickFlex™ μ lead—the latest in lead technology—is designed to provide predictable outcomes through superb access, delivery and fixation.

Based on the QuickFlex™ lead family, this 4 F bipolar lead features a narrow ring electrode for lead tip flexibility, and a steerable tip for control and deliverability. The large S-curve provides superior fixation for this small diameter lead. The 4.3 F lead body diameter allows Direct-to-Target™ placement through a sub 5 F inner catheter to deliver leads to small, acute venous anatomies that may have been unreachable in the past.

The addition of the QuickFlex μ lead to the QuickFlex CRT family of leads provides implanters with even more lead options to enable predictable placement and stability for varied patient needs.

DESIGNED TO DELIVER

- Optim™ Lead Insulation
 - Optim insulation is a hybrid insulation material—the first of its kind developed specifically for cardiac lead use. It blends the biostability and flexibility of high-performance silicone rubber with the strength, tear resistance and abrasion resistance of polyurethane. This insulation allows for an abrasion resistant, thin diameter lead.
- Low Profile
 - Entire lead body: 4,3 F
 - Lead tip: 4,0 F
- Flexible Lead Body
 - Tip-to-ring electrode spacing of 20 mm and reduced lengths of rigid portions (tip and ring) create superb flexibility.
- Steerable Tip
 - Distal tip angle can be controlled to maneuver the lead through venous anatomy.
- Over-the-Wire or Stylet-Approach Compatibility
 - Specially designed leads give the implanting physician the option of using either approach during the same procedure.
- Fast-Pass™ Lubricious Coating
 - Enables multiple leads to easily slide against one another, possibly reducing inadvertent dislodgement.

EXCEPTIONAL STABILITY AND PERFORMANCE

- S-Shaped for Stability
 - The S-curve shape is designed to provide enhanced lead stability in a wide variety of vein sizes.
- Options for Any Anatomy
 - The complete family of QuickFlex leads, including QuickFlex μ, QuickFlex and QuickFlex XL is a comprehensive suite of CRT leads with varying diameters and S-Shape sizes, providing options to enable predictable procedures — regardless of the patient's venous anatomy.
- Suture Sleeve
 - The new suture sleeve has been designed with silicone ridges to secure a thinner lead body.
- Titanium Nitride Coating (TiN)
 - TiN coating on the tip and ring electrodes has been shown to improve stimulation efficiency and lower polarisation.
- Steroid Elution
 - Steroid elution minimizes inflammatory reaction at the electrode-tissue interface and provides lower acute and chronic thresholds than non-steroid-eluting leads.



ST. JUDE MEDICAL™
MORE CONTROL. LESS RISK.

QuickFlex™ μ 4F Bipolar, Optim™ Insulation-Insulated, Left Ventricular Pacing Lead

MODEL 1258T

SPECIFICATIONS

Parameter	Description
Connector	IS-1 Bipolar
Lead Length	75 cm, 86 cm, 92 cm
Lead Body Size	4,3 F (1,42 mm/0.056")
Tip Electrode Size	4,0 F (1,33 mm/0.052")
LV Lead Delivery System Introducer Size	Minimum 5 F ID
Minimum S-Curve Height	16 mm
Tip Electrode	Pt/Ir, TiN coated, ring-shaped, two grooves
Steroid	Dexamethasone sodium phosphate
Tip Electrode Surface Area	5,0 mm ²
Ring Electrode Surface Area	7,4 mm ²
Tip-to-Ring Electrode Spacing	20 mm
Lead Body Insulation	Optim™ insulation
Lead Body Coating	Fast-Pass™ coating
Conductors	
Distal (coil)	MP35N™
Proximal (cables)	MP35N™
Suture Sleeve	Attached

Indications and Usage

The QuickFlex lead has application as part of a St. Jude Medical™ biventricular system.

Contraindications

The use of QuickFlex leads is contraindicated in patients who:

- Are expected to be hypersensitive to a single dose of 1,0 mg of dexamethasone sodium phosphate.
- Are unable to undergo an emergency thoracotomy procedure.
- Have coronary venous vasculature that is inadequate for lead placement, as indicated by venogram.

Global Headquarters

One Lillehei Plaza
St. Paul, Minnesota 55117
USA
+1 651 483 2000
+1 651 490 4310 Fax

Cardiac Rhythm

Management Division
15900 Valley View Court
Sylmar, California 91342
USA
+1 818 362 6822
+1 818 364 5814 Fax

St. Jude Medical AB

Veddestavägen 19
175 84 Järfälla
Sweden
+46 8 474 4000
+46 8 760 9542 Fax

St. Jude Medical Europe, Inc.

The Corporate Village
Figueras Building
Avenue Da Vinci laan, 11 Box F1
B-1935 Zaventem
Belgium
+32 2 774 68 11
+32 2 772 83 84 Fax

St. Jude Medical Brasil Ltda.

Rua Frei Caneca, 1380
7º ao 9º andares
01307-002 - São Paulo (SP)
Brazil
+55 11 5080 5400
+55 11 5080 5423 Fax

St. Jude Medical (Hong Kong) Ltd.

Unit 2701-07 27/F, COSCO Tower
Grand Millennium Plaza
183 Queen's Road
Central, Hong Kong
+852 2996 7688
+852 2956 0622 Fax

St. Jude Medical Japan Co., Ltd.

3-1-30, Minami-Aoyama
Minato-ku
Tokyo 107 0062
Japan
+81 3 3423 6450
+81 3 3402 5586 Fax



ST. JUDE MEDICAL™
MORE CONTROL. LESS RISK.

www.sjm.com

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country.

Unless otherwise noted, TM indicates that the name is a trademark of, or licensed to, St. Jude Medical, Inc., and its related companies. MP35N™ is a trademark of SPS Technologies, Inc.
©2009. St. Jude Medical, Inc. All Rights Reserved.
Item No. GMCRM391

CPS Direct™ PL

Peelable Outer Guide Catheter

Product Highlights

- Unique SiteMark™ tungsten marker stripes provide superior fluoroscopic visibility to verify torque transfer
- Compatible with CPS Aim™ inner catheter and CPS Luminary™ bideflectable catheter with lumen to modify shape and extend reach if necessary
- EvenPeel™ stripes provide more smooth and reliable peeling for worry-free sheath removal



Ordering Information

Included: sheath with hemostasis valve attached, dilator and 2 valve bypass tools

Model Number	Curve Shape	Available Length (cm)	Overall Length (cm)	Inner Diameter (F/mm)	Outer Diameter (F/mm)
410210	Straight (OC-STR)	47	50,7	7/2,44	9/3,00
410211	Multipurpose (OC-MP)	47	50,7	7/2,44	9/3,00
410212	115° (OC-115)	47	50,7	7/2,44	9/3,00
410213	135° (OC-135)	47	50,7	7/2,44	9/3,00
410214	Wide (OC-W)	47	50,7	7/2,44	9/3,00
410215	Extra Wide (OC-XW)	47	50,7	7/2,44	9/3,00
410216	Right Sided (OC-R)	47	50,7	7/2,44	9/3,00
410224	145° (OC-145)	47	50,7	7/2,44	9/3,00
410217	Straight (OC-STR)	54	57,7	7/2,44	9/3,00
410218	Multipurpose (OC-MP)	54	57,7	7/2,44	9/3,00
410219	115° (OC-115)	54	57,7	7/2,44	9/3,00
410220	135° (OC-135)	54	57,7	7/2,44	9/3,00
410221	Wide (OC-W)	54	57,7	7/2,44	9/3,00
410222	Extra Wide (OC-XW)	54	57,7	7/2,44	9/3,00
410223	Right Sided (OC-R)	54	57,7	7/2,44	9/3,00
410225	145° (OC-145)	54	57,7	7/2,44	9/3,00



Separately Available Accessories

Model Number	Name	Type
410194	CPS Direct™ PL Valve Bypass Tool (Pack of 2)	Valve bypass tool
410195	CPS Direct™ PL Inner Catheter SafeSheath™ Sealing Adapter	Self-sealing valve
410190	CPS™ Implant Kit (Includes Needle, Syringe and 0,035" Guidewire)	Implant Kit

Customer Support: 46-8-474-4756

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country. Unless otherwise noted, ™ indicates that the name is a trademark of, or licensed to, St. Jude Medical or one of its subsidiaries. ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK are registered and unregistered trademarks and service marks of St. Jude Medical, Inc. and its related companies. ©2011 St. Jude Medical, Inc. All rights reserved.

CPS Direct™ SL II Slittable Outer Guide Catheter




Product Highlights

- Integrated hub and hemostasis valve
- Increased curve retention and optimized catheter body structure for improved kink resistance
- Soft tip to lessen risk of traumatic insertion

Ordering Information

Included: dilator and 2 valve bypass tools

Model Number	Curve Shape	Available Length (cm)	Overall Length (cm)	Inner Diameter (F/mm)	Outer Diameter (F/mm)
DS2C001	Straight	47	50,7	7/2,44	9/3,00
DS2C002	115°	47	50,7	7/2,44	9/3,00
DS2C003	135°	47	50,7	7/2,44	9/3,00
DS2C004	Wide	47	50,7	7/2,44	9/3,00
DS2C005	X-Wide	47	50,7	7/2,44	9/3,00
DS2C006	Right Side	47	50,7	7/2,44	9/3,00
DS2C011	Straight	54	57,7	7/2,44	9/3,00
DS2C012	115°	54	57,7	7/2,44	9/3,00
DS2C013	135°	54	57,7	7/2,44	9/3,00
DS2C014	Wide	54	57,7	7/2,44	9/3,00
DS2C015	X-Wide	54	57,7	7/2,44	9/3,00

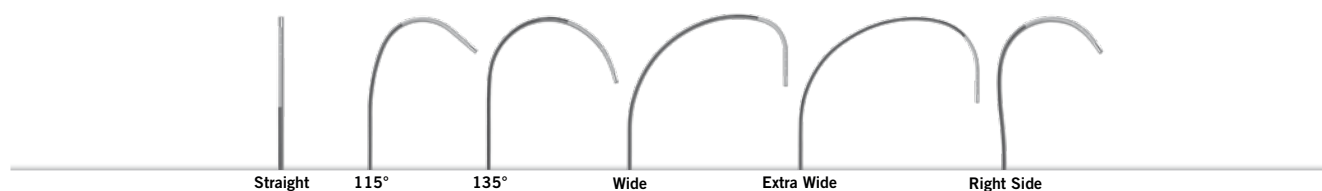

Separately Available Accessories

Model Number	Name	Type
DS2A003	CPS™ Universal Slitter	Slitter
DS2A004	CPS Direct™ SL Valve Bypass Tool	Valve bypass tool

Customer Support: 46-8-474-4756

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country. Unless otherwise noted, ™ indicates that the name is a trademark of, or licensed to, St. Jude Medical or one of its subsidiaries. ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK. are registered and unregistered trademarks and service marks of St. Jude Medical, Inc. and its related companies. ©2011 St. Jude Medical, Inc. All rights reserved.

CPS Aim™ Universal

Slittable Inner Catheter with Integrated Valve

MODELS DS2N026, DS2N027, DS2N028, DS2N029, DS2N030



SPECIFICATIONS

- The CPS Aim™ Universal family of inner catheters with integrated valve is designed to assist with coronary sinus cannulation, branch vein subselection and left ventricular lead delivery. The catheters are compatible with other products in the St. Jude Medical™ Cardiac Positioning System (CPS™) family—an inter-compatible system of tools designed to give you more control to deliver the left-heart lead—efficiently and predictably—to your vein of first choice.
- Three CPS Aim Universal inner catheters enable atraumatic subselection.
 - CPS Aim Universal inner catheters enable access to the vein of first choice through Direct-To-Target™ placement. The CPS Aim Universal inner catheter provides a tunnel to acute and tortuous venous anatomies for 5 F leads (including the Quartet™ lead) and guidewire.
 - The CPS Aim Universal inner catheters are easy to remove with a low slit force after Direct-To-Target™ placement.
 - Three curve shapes (acute, 90°, obtuse) with fluoroscopic visibility facilitate first-choice target vein access, even when encountering difficult angulations and tortuous anatomy.
 - The soft tip enables atraumatic subselection.
- Two CPS Aim™ cannulators assist with coronary sinus access
 - When used in conjunction with CPS Direct™ Universal outer guide catheters, CPS Aim™ Universal cannulators facilitate coronary sinus cannulation.
 - CPS Aim Universal cannulators help extend the reach and modify the shape of CPS Direct Universal outer guide catheters, helping overcome challenging anatomies.
- A combination of PEBAX™ material that becomes softer from the proximal to the distal end and increased braid wire at the distal end provide for a torqueable, kink resistant and soft-tipped subselector. The catheter has been designed to access acute and tortuous anatomies.
- The catheter body and tip are clearly seen under fluoroscopy. Fluoroscopic material in the catheter profile illuminates the catheter body. A platinum band at the tip provides a landmark to access venous anatomy.
- The CPS Aim Universal inner catheter has a low slit force to reduce the risk of lead movement when slitting the catheter. To assist in this effort, the CPS Aim Universal inner catheter has a slittable hub with a smooth hub-to-shaft transition. In addition, the braidwire and PEBAX material construction has been optimized for smooth slitting. The CPS Aim Universal slittable inner catheter has been designed to remove easily after Direct-To-Target™ placement.



ST. JUDE MEDICAL™

PHYSICAL SPECIFICATIONS

Model	DS2N026	DS2N027	DS2N028	DS2N029	DS2N030
Model Name	SUB-ACU	SUB-90	SUB-OBT	CN-CSL	CN-ALII
Curve Shape	Acute	90°	Obtuse	CSL	ALII
Available Lengths - cm (working)	59, 65	59, 65	59, 65	65	65
Overall Length - cm (respectively)	63, 69	63, 69	63, 69	69	69
Valve	Integrated				
Inner Diameter	5.87 F (1.96 mm)				
Outer Diameter	7.62 F (2.6 mm)				
Material	Multi-durometer PEBAX™ material reinforced with stainless steel braid wire for a kink-resistant catheter shaft and soft distal tip. Lubricious inner liner/outer coating.				
Marker	Platinum tip				
Accessories (available separately)					
Accessory Name	CPS™ Universal Slitter (DS2A003)	CPS Direct™ Valve Bypass Tool (DS2A004)			
Accessory Type	Slitter	Valve Bypass Tool			

*PEBAX is a trademark of Arkema, Inc.

Global Headquarters
 One St. Jude Medical Drive
 St. Paul, Minnesota 55117
 USA
 +1 651 756 2000
 +1 651 756 3301 Fax

St. Jude Medical Cardiovascular & Ablation Technologies
 5050 Nathan Lane North
 Plymouth, Minnesota 55442
 USA
 +1 651 756 5400
 +1 651 756 5470 Fax

St. Jude Medical Implantable Electronic Systems
 15900 Valley View Court
 Sylmar, California 91342
 USA
 +1 818 362 6822
 +1 818 364 5814 Fax

U.S. Division
 6300 Bee Cave Road
 Bldg. Two, Suite 100
 Austin, TX 78746
 USA
 +1 512 286 4000
 +1 512 732 2418 Fax

SJM Coordination Center BVBA
 The Corporate Village
 Da Vincilaan 11 Box F1
 1935 Zaventem, Belgium
 +32 2 774 68 11
 +32 2 772 83 84 Fax

St. Jude Medical Brasil Ltda.
 Rua Itapeva, 538
 5º ao 8º andar
 01332-000 – São Paulo – SP
 Brazil
 +55 11 5080 5400
 +55 11 5080 5423 Fax

St. Jude Medical (Hong Kong) Ltd.
 Suite 1608, 16/F Exchange Tower
 33 Wang Chiu Road
 Kowloon Bay, Kowloon
 Hong Kong SAR
 +852 2996 7688
 +852 2956 0622 Fax

St. Jude Medical Australia Pty, Ltd.
 17 Orion Road
 Lane Cove, NSW 2066
 Australia
 +61 2 9936 1200
 +61 2 9936 1222 Fax

SJMprofessional.com



Rx Only

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use.

Unless otherwise noted, ™ indicates that the name is a trademark of, or licensed to, St. Jude Medical or one of its subsidiaries. ST. JUDE MEDICAL and the nine-squares symbol are trademarks and service marks of St. Jude Medical, Inc. and its related companies. © 2013 St. Jude Medical, Inc. All Rights Reserved.



ARROW BALLOON WEDGE-PRESSURE CATHETERS



AT A GLANCE

- trusted catheters in use for over 30 years
- wide variety of catheter options, lengths and sizes
- enlarged distal lumen for clear visualization of waveforms
- most sizes matched to introducer size*
- easy handling:
 - good torque control
 - catheter length markings to confirm insertion depth
 - flotation control for secure positioning
 - easy determination of catheter tip position

SMOOTH FLEXIBLE CATHETER BODY FACILITATES INSERTION

- ARROW catheters are designed to provide a greater degree of torque control
- flotation control allows blood flow to carry the inflated balloon naturally through the ventricle and into the pulmonary artery
- catheter tip position may be determined by continuous pressure monitoring

CATHETER LENGTH MARKINGS

Each catheter has clear, easy to identify increment markings every 10 cm along the catheter body to confirm insertion depth.

WIDE RANGE OF SIZES AND LENGTHS ALLOW FOR MORE ACCURATE MATCHING OF PATIENT NEEDS TO CATHETER SIZES

ARROW balloon wedge-pressure catheters are available in French sizes 4, 5, 6, 7 and 8 for a more complete selection.

CONVENIENT PACKAGING

Each catheter is packaged in a sterile peel-pack tray with a control stroke syringe.

SIMULTANEOUS PRESSURE MONITORING

Double pressure lumen balloon wedge-pressure catheters are available in French sizes 5, 6 and 7, allowing determination of pressure gradients between adjacent parts of the heart as well as identifying a variety of congenital heart defects and obstructions.

WEDGE-PRESSURE CATHETERS

ARROW

SINGLE PRESSURE LUMEN BALLOON WEDGE-PRESSURE CATHETERS

REF.	FRENCH SIZE	INTRODUCER SIZE RECOMMENDED	USEFUL LENGTH	MAX. INFLATION* CAPACITY	INFLATED BALLOON DIAMETER	MAX. WIRE RECOMMENDED
AI-07121	4 Fr.	5 Fr.	60cm	0.60cc	6.5mm	0.021"
AI-07122	4 Fr.	5 Fr.	110cm	0.60cc	6.5mm	0.021"
AI-07123	5 Fr.	5 Fr.	60cm	0.75cc	8.0mm	0.025"
AI-07124	5 Fr.	5 Fr.	110cm	0.75cc	8.0mm	0.025"
AI-07125	6 Fr.	6 Fr.	60cm	1.00cc	10.0mm	0.035"
AI-07126	6 Fr.	6 Fr.	110cm	1.00cc	10.0mm	0.035"
AI-07126-J	6 Fr.	6 Fr.	90cm	1.00cc	10.0mm	0.035"
AI-07127	7 Fr.	7 Fr.	110cm	1.25cc	11.0mm	0.038"
AI-07127-STC ¹⁰	7 Fr.	7 Fr.	110cm	1.25cc	11.0mm	0.038"
AI-07128	8 Fr.	8 Fr.	110cm	1.25cc	11.0mm	0.038"

DOUBLE PRESSURE LUMEN BALLOON WEDGE-PRESSURE CATHETERS

REF.	FRENCH SIZE	INTRODUCER SIZE RECOMMENDED	USEFUL LENGTH	MAX. INFLATION* CAPACITY	INFLATED BALLOON DIAMETER	MAX. WIRE RECOMMENDED	EXIT PORT SPACING
AI-07025	5 Fr.	5 Fr.	80cm	1.00cc	8.0mm	0.018"	proximal port exits 3 cm from tip
AI-07026	6 Fr.	6 Fr.	110cm	1.00cc	10.0mm	0.021"	proximal port exits 3 cm from tip
AI-07141	6 Fr.	6 Fr.	110cm	1.00cc	10.0mm	0.021"	proximal port exits 20 cm from tip
AI-07027	7 Fr.	7 Fr.	110cm	1.50cc	12.0mm	0.025"	proximal port exits 3 cm from tip
AI-07143	7 Fr.	7 Fr.	110cm	1.50cc	12.0mm	0.025"	proximal port exits 30 cm from tip



SPECIAL DOUBLE PRESSURE LUMEN BALLOON WEDGE-PRESSURE CATHETER

REF.	FRENCH SIZE	INTRODUCER SIZE RECOMMENDED	USEFUL LENGTH	MAX. INFLATION* CAPACITY	INFLATED BALLOON DIAMETER	MAX. WIRE RECOMMENDED	EXIT PORT SPACING
AI-07142	8 Fr.	8 Fr.	100cm	1.50cc	11.0mm	both to 0.038"	proximal port exits 6 cm from tip

NOTE: 1. Contact Customer Service for available sizes. | 2. Except 4 Fr. where balloon is 4-1/2 Fr. | 3. Cardella, JF, Smith, TP, Darcy, MD, Hunter, DW, Castaneda-Zunigo, W, Amplatz, K. Balloon occlusion femoral angiography prior to in situ saphenous vein bypass. *Cardiovascular and Interventional Radiology*. (1987) 10: 181 – 187. | 5. Zeevi B, et al. A newly-Designed Double Pressure Balloon Catheter: Clinical Use in Congenital Heart Disease. *Journal of Invasive Cardiology*. 1989;1:3. | 6. Kelly DT, Krovetz II, Rowe RD. Double-Lumen Flotation Catheter for use in Complex Cardiac Anomalies. *Circulation*. 1971;44:910-913. | 7. Black IFS. Floating a Catheter into the Pulmonary Artery in Transportation of Great Arteries. *Am Heart J*. 1972;84:761-763. | 8. Radiopaque marker just in front of proximal port provides convenient point for catheter port location. | 9. CO₂ is the recommended inflation media. See instructions for use prior to using air. Do not use any liquid to inflate balloon. | 10. STC = Super Torque Control

FEATURES

- unique tapered construction of the balloon allows the catheter to be matched to the introducer size*



* except 4 Fr.

DISTRIBUTED BY:

TELEFLEX MEDICAL HEADQUARTER INTERNATIONAL, IRELAND

IDA Business & Technology Park · Dublin Road · Athlone · Co Westmeath
Tel. +353 (0)9 06 46 08 00 · Fax +353 (0)14 37 07 73 · orders.intl@teflex.com

UNITED KINGDOM Tel. +44 (0)14 94 53 27 61 · info.uk@teflex.com

SOUTH AFRICA Tel. +27 (0)11 807 4887 · assist.africa@teflex.com

WWW.TELEFLEX.COM

94 10 99 - 00 00 01 · REV A · 03 13 02 · All data current at time of printing. Subject to technical changes without further notice.

teflex

CPS Courier™

Guidewires

Product Highlights

- Helps physicians more easily subselect the target coronary branch vein and deliver the LV lead to its preferred destination



Ordering Information


Model Number	Distal Support	Length (cm)	Units per box	Diameter (in)
DS2G001	Soft	195	5	0,014
DS2G002	Medium	195	5	0,014
DS2G003	Firm	195	5	0,014
DS2G004	Extra Firm	195	5	0,014

CPS Duo™

Stylet Guidewire System

Product Highlights

- Enables optimal subselection of the branch vein and offers greater maneuverability and control of the LV lead

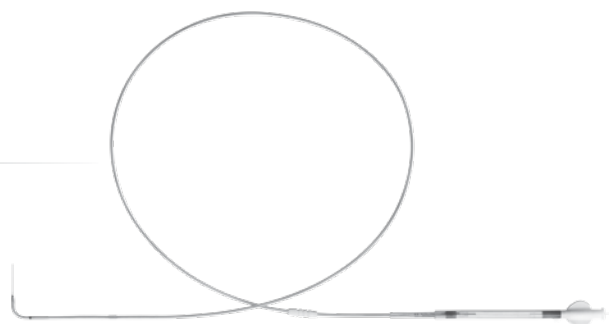

Ordering Information

Model Number	Type	Lengths (cm)	Diameter
DS2M001	CPS Duo™ Stylet	75; 86	OD: 0,014" LV lead lumen compatible ID: 0,012" compatible
DS2M006	CPS Duo™ Guidewire	195	0,012"

Customer Support: 46-8-474-4756

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use. Devices depicted may not be available in all countries. Check with your St. Jude Medical representative for product availability in your country. Unless otherwise noted, ™ indicates that the name is a trademark of, or licensed to, St. Jude Medical or one of its subsidiaries. ST. JUDE MEDICAL, the nine-squares symbol and MORE CONTROL. LESS RISK. are registered and unregistered trademarks and service marks of St. Jude Medical, Inc. and its related companies. ©2011 St. Jude Medical, Inc. All rights reserved.



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-200.14.03



Product Service

EC Certificate

EC Design-Examination Certificate

Directive 90/385/EEC on Active Implantable Medical Devices (AIMDD), Annex 2 (4)
(Other devices than custom made or intended for clinical investigation)

No. I7 014607 0234 Rev. 00

Manufacturer: **St. Jude Medical**
Cardiac Rhythm Management
Division
15900 Valley View Court
Sylmar CA 91342
USA

EC-Representative: St. Jude Medical Coordination Center BVBA
The Corporate Village, Da Vincilaan 11 Box F1, 1935 Zaventem,
BELGIUM

Product: **Implantable Pacemakers**

The Certification Body of TÜV SÜD Product Service GmbH declares that a design examination has been carried out on the respective devices in accordance with AIMDD Annex 2 (4). This design of the devices conforms to the requirements of this Directive. For marketing of these devices an additional Annex 2 certificate is mandatory. See also notes overleaf.

Report no.: 713149860

Valid from: 2019-06-15

Valid until: 2024-05-26

Date, 2019-06-14

Stefan Preiß



Benannt durch/Designated by
 Zentralstelle der Länder
 für Gesundheitsschutz
 bei Arzneimitteln und
 Medizinprodukten
 www.zlg.de
 ZLG-BS-200.14.03



Product Service

EC Certificate

EC Design-Examination Certificate

Directive 90/385/EEC on Active Implantable Medical Devices (AIMDD), Annex 2 (4)
 (Other devices than custom made or intended for clinical investigation)

No. I7 014607 0234 Rev. 00

Model(s): see below

Facility(ies): St. Jude Medical Cardiac Rhythm Management Division
 15900 Valley View Court, Sylmar CA 91342, USA

St. Jude Medical Puerto Rico LLC
 Lot A Interior - #2 Rd Km. 67.5, Santana Industrial Park, Arecibo
 PR 00612, USA

St. Jude Medical Operations (M) Sdn.Bhd.
 Plot 102, Lebuhraya Kampung Jawa, Bayan Lepas Industrial Zone,
 11900 Penang, MALAYSIA

Parameters ./.

Design Facility(ies): St. Jude Medical Cardiac Rhythm Management Division
 15900 Valley View Court, Sylmar, CA 91342, USA

Product: Implantable Pacemakers

Test Report No.: 70069297

Model:	Model No.:	Variant:
Microny™ II SR+	2525T	

Test Report No.: 70110810

Model:	Model No.:	Variant:
Zephyr™ SR	5620	
Zephyr™ DR	5820	
Zephyr™ XL DR	5826	

TÜV SÜD
 CERTIFICATE ◆ CERTIFICADO ◆ CERTIFIKAT ◆ 認證書 ◆ CERTIFICATE ◆ ZERTIFIKAT ◆ CERTIFICADO ◆ CERTIFIKAT ◆ 認證書 ◆ CERTIFICATE ◆ ZERTIFIKAT



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-200.14.03



Product Service

EC Certificate

EC Design-Examination Certificate
Directive 90/385/EEC on Active Implantable Medical Devices (AIMDD), Annex 2 (4)
(Other devices than custom made or intended for clinical investigation)

No. I7 014607 0234 Rev. 00

Test Report No.: 71321436

Model:	Model No.:	Variant:
Zephyr™ XL SR	5626	

Test Report No.: 713017309_1

Model:	Model No.:	Variant:
Assurity™	PM1240	
Assurity™	PM2240	
Endurity™	PM1160	
Endurity™	PM2160	
Allure™	PM3120	
Allure™ RF	PM3222	
Allure Quadra™ RF	PM3242	

Test Report No.: 713028360

Model:	Model No.:	Variant
Quadra Allure MP™RF	PM3262	

Test Report No.: 713043621

Model:	Model No.:	Variant:
Assurity MRI™	PM1272	MR Conditional
Assurity MRI™	PM2272	MR Conditional
Endurity MRI™	PM1172	MR Conditional
Endurity MRI™	PM2172	MR Conditional
Endurity™	PM1162	MR Conditional
Endurity™	PM2162	MR Conditional

TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD
 ZERTIFIKAT ◆ CERTIFICATE ◆ 認證書 ◆ CERTIFICADO ◆ CERTIFICAT



Benannt durch/Designated by
Zentralstelle der Länder
für Gesundheitsschutz
bei Arzneimitteln und
Medizinprodukten
www.zlg.de
ZLG-BS-200.14.03



Product Service

EC Certificate

EC Design-Examination Certificate

Directive 90/385/EEC on Active Implantable Medical Devices (AIMDD), Annex 2 (4)
(Other devices than custom made or intended for clinical investigation)

No. I7 014607 0234 Rev. 00

Test Report No.: 713057320

Model:	Model No.:	Variant:
Endurity™ Core	PM1140	MR Conditional
Endurity™ Core	PM2140	MR Conditional
Endurity™ Core	PM1152	MR Conditional
Endurity™ Core	PM2152	MR Conditional

Test Report No.: 713084189

Model:	Model No.:	Variant:
Quadra Allure™	PM3542	MR Conditional
Quadra Allure MP™	PM3562	MR Conditional

Test Report No.: 713130819

Model:	Model No.:	Variant:
Zenex™	PM1250	
Zenex™	PM2250	
Zenus™	PM1170	
Zenus™	PM2170	
Zenex MRI™	PM1282	MR Conditional
Zenex MRI™	PM2282	MR Conditional
Zenus MRI™	PM1182	MR Conditional
Zenus MRI™	PM2182	MR Conditional

TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD TÜV SÜD
 ZERTIFIKAT ◆ CERTIFICATE ◆ 認證書 ◆ CERTIFICADO ◆ CERTIFICAT



**SJM Declaration of Conformity
Implantable Pacemakers
ATTACHMENT TO DECLARATION OF CONFORMITY**

St. Jude Medical (SJM) hereby declares that the following SJM facilities and products conform to the applicable provisions of Annex 2 the European Union’s Active Implantable Medical Devices Directive, AIMDD, 90/385/EEC. All supporting documentation is retained under the premises of SJM. We declare no application has been lodged with any other notified body for the same products. This declaration is issued under the sole responsibility of the manufacturer. This declaration supersedes any declaration issued previously for the same product(s).

Manufacturer Address: *St. Jude Medical Cardiac Rhythm Management Division
15900 Valley View Court
Sylmar, CA 91342*

European Representative: *St. Jude Medical Coordination Center BVBA
The Corporate Village
Da Vincilaan 11 Box F1
1935 Zaventem, Belgium*

Product Type: *Implantable Pacemakers*

Product Name(s): *See Attachment*

Model Number(s): *See Attachment*

Classification: *AIMD*

GMDN Code(s): *See Attachment*

Original CE Mark Date: *See Attachment*

(FQA or EC as appropriate) Certificate No and expiration date: *EC
Certification No: I7 014607 0234 Rev. 00
Expiration Date: 2024-05-26*

*FQA
Certificate No: I1 16 12 14607 211
Expiration Date: 2021-07-25*

*ISO13485
Certificate No: Q1N 17 09 14607 217
Expiration Date: 2020-10-31*

Signature:

Kathy Berg

Kathy Berg
Manager Regulatory Affairs

14 Jun 2019

Issue Date



**SJM Declaration of Conformity
Implantable Pacemakers
ATTACHMENT TO DECLARATION OF CONFORMITY**

Applicable Quality System Standards:

Fulfills the requirements of Annex 2 of the European Union's Active Implantable Medical Devices Directive, AIMDD, 90/385/EEC and corresponding national legislation.

Fulfills applicable requirements including CE marking and the Essential Requirements of the AIMDD, 90/385/EEC and corresponding national legislation.

Notified Body:

TÜV SÜD Product Service GmbH Zertifizierstelle
Ridlerstraße 65, 80339, München, Germany

Notified Body Number:

0123


Manufacturing Facilities:

*St. Jude Medical Cardiac Rhythm Management Division
15900 Valley View Court Sylmar, CA 91342 USA*

*St. Jude Medical Puerto Rico LLC
Lot A Interior - #2 Rd Km. 67.5, Santana Industrial Park,
Arecibo PR 00612, USA*

*St. Jude Medical Operations (M) Sdn. Bhd
Plot 102, Lebuhraya Kampung Jawa, Bayan Lepas
Industrial Zone, 11900 Penang, MALAYSIA*

Signature:



Kathy Berg
Manager Regulatory Affairs



Issue Date

SJM Declaration of Conformity
Implantable Pacemakers
ATTACHMENT TO DECLARATION OF CONFORMITY

The following product(s) is/are approved under EC-certificate number **I7 014607 0230 Rev. 00:**

Product Name	Model No.	GMDN Codes	First Date of CE Marking
Microny™ II SR+	2525T	47267	1999-9-17
Zephyr™ XL DR	5826	47265	2006-5-9
Zephyr™ DR	5820	47265	2006-5-9
Zephyr™ SR	5620	47267	2006-5-9
Zephyr™ XL SR	5626	47267	2007-6-13
Assurity™	PM1240	47267	2013-3-7
Assurity™	PM2240	47265	2013-3-7
Endurity™	PM1160	47267	2013-3-7
Endurity™	PM2160	47265	2013-3-7
Allure™	PM3120	47263	2013-3-7
Allure™ RF	PM3222	47263	2013-3-7
Allure Quadra™ RF	PM3242	47263	2013-3-7
Quadra Allure MP™ RF	PM3262	47263	2014-7-31
Assurity MRI™	PM1272 (MR Conditional)	47267	2014-12-18
Assurity MRI™	PM2272 (MR Conditional)	47265	2014-12-18
Endurity MRI™	PM1172 (MR Conditional)	47267	2014-12-18
Endurity MRI™	PM2172 (MR Conditional)	47265	2014-12-18
Endurity™	PM1162 (MR Conditional)	47267	2014-12-18
Endurity™	PM2162 (MR Conditional)	47265	2014-12-18
Endurity™ Core	PM1140 (MR Conditional)	47267	2015-7-24
Endurity™ Core	PM2140 (MR Conditional)	47265	2015-7-24
Endurity™ Core	PM1152 (MR Conditional)	47267	2015-7-24
Endurity™ Core	PM2152 (MR Conditional)	47265	2015-7-24
Quadra Allure™	PM3542 (MR Conditional)	47263	2016-10-21
Quadra Allure MP™	PM3562 (MR Conditional)	47263	2016-10-21
Zenex™	PM1250	47267	2018-10-12
Zenex™	PM2250	47265	2018-10-12
Zenus™	PM1170	47267	2018-10-12
Zenus™	PM2170	47265	2018-10-12
Zenex MRI™	PM1282 (MR Conditional)	47267	2018-10-12

Signature:


 Kathy Berg
 Manager Regulatory Affairs


 Issue Date



**SJM Declaration of Conformity
Implantable Pacemakers
ATTACHMENT TO DECLARATION OF CONFORMITY**

Product Name	Model No.	GMDN Codes	First Date of CE Marking
Zenex MRI™	PM2282 (MR Conditional)	47265	2018-10-12
Zenus MRI™	PM1182 (MR Conditional)	47267	2018-10-12
Zenus MRI™	PM2182 (MR Conditional)	47265	2018-10-12

Signature:

Kathy Berg

Kathy Berg
Manager Regulatory Affairs

14 Jun 2019

Issue Date