

Turkey
Discover
the potential

Broche[®]
medical

PRODUCT CATALOGUE

Broche[®]
Medical

BROCHE

nonwovens



Address and Contact Details :

Factory Address: Veliköy Beldesi Sanayi Mah.9.Cad. No.35/A Çerkezköy /Tekirdağ/TURKEY

Headquarter Address: Oruç Reis Mah. Tekstilkent Sitesi,B-Blok Kat:3 No:12 Esenler/İstanbul-TURKEY

Web Site for Medical : www.brochemedikal.com/en/

Web Site for Nonwovens: www.brochenonwovens.com.tr/en

Phone: +90 (212) 438 02 42 (Pbx)

E-Mail: info@brochemedikal.com

ABOUT US

Nurteks Tekstil ve Medikal San. Dış Tic. A.Ş. has started production and sale of disposable surgical gowns and surgical drape sets with **Broche**® brand in its own facilities in the beginning of 2006 to convey its experiment, in non-woven sector since 1995, to medical sector.

Nurteks Tekstil, having a well earned place in all over Turkey with **Broche**® brand by quick delivering all kinds of consumable goods, mostly gloves, which have been produced and, as well, imported since its establishment, 2006, has hold a prominent place and been an important brand, especially, in the markets of Europe, Africa and Middle East with its export activities.

Nurteks Tekstil, making use of ever developing technologies since the beginning of 2012, improved its all machine lines and sterilization devices, and extended its production and stock areas to a total 7.000 SM closed area.

Nurteks Tekstil is steadily carrying on its activities to hold the prominence to be one of the leading brands in the medical sector with high quality and fair price it has been offering in the market with **Broche**® brand.

Quality Policy;

- To make production in the medical sector with the latest technology and provide persistence in production quality and a quality management system.
- To enhance the customer satisfaction by taking any suggestions and complaints into consideration.
- To offer products and services in compliance with current laws and regulations by giving due importance to human health.

Certificates;

CE2195, ISO 13485, ISO 9001,

All drapes and gowns are

TS EN 13795 + A1 certified by TURKISH STANDARDS INSTITUTE.



EN 13795 + A1



INDEX

TEST REPORT

| | |
|--------------------|--------|
| Fabric Test Report | 7 - 12 |
|--------------------|--------|

STERILE SURGICAL PACKS

| | |
|---|----|
| General Surgery Pack - Standard | 13 |
| General Surgery Pack - Large | 14 |
| General Surgery Pack - Extra Large | 15 |
| Laparoscopy Pack | 16 |
| Angiography Pack - Standard | 17 |
| Angiography Pack - Large | 18 |
| Angiography Pack W / Transparent Panel Standard | 19 |
| Angiography Pack W / Transparent Panel Large | 20 |
| Cardiovascular Pack W / Pouch - Standard | 21 |
| Cardiovascular Pack W / Pouch - Large | 22 |
| Tur Pack W \ Pouch (Urology Set) | 23 |
| Lithotomic Gynaecology Pack W / Pouch | 24 |
| Gynaecology / Cystoscopy Pack | 25 |
| Caesarean Section Pack W / Pouch - Standard | 26 |
| Caesarean Section Pack W / Pouch - Large | 27 |
| Caesarean Section Pack W / Pouch - Extra Large | 28 |
| Delivery Pack | 29 |
| Delivery Pack W / Pouch | 30 |
| Arthroscopy Pack W / Pouch - Standard | 31 |
| Arthroscopy Pack W / Pouch - Large | 32 |
| Arthroscopy Pack W / Pouch - Extra Large | 33 |
| Craniotomy W / Pouch Pack | 34 |
| E.N.T. Pack | 35 |
| Hip Pack U | 36 |
| Implant Pack | 37 |
| Single Pouch Ophthalmic Pack | 38 |
| Adhesive Drapes | 39 |
| Non Sterile Welcome Pack (Waterproof) | 40 |

STERILE PROCEDURE PACKS

| | |
|---|----|
| Major General Procedure Pack | 44 |
| Cardiology-Angiography Procedure Pack | 46 |
| Caesarean Procedure Pack | 48 |
| Open Heart CABG Procedure Pack | 50 |
| Gynaecology Procedure Pack | 52 |
| Urology Procedure Pack | 54 |
| Orthopedic Hip Replacement Procedure Pack | 56 |
| Orthopaedic Knee Arthroscopy Procedure Pack | 58 |
| Cataract Procedure Pack | 60 |

STERILE & NON-STERILE GOWNS

| | |
|---|----|
| Sterile Ultrasonic Stitch Surgical Gown | 64 |
| Non-Sterile Patient Gown | 66 |
| Non-Sterile Doctor Scrub Suit | 66 |

GLOVES

| | |
|---|----|
| Chloroprene Synthetic Sterile Surgical Gloves | 69 |
| Latex Sterile Surgical Gloves | 70 |
| Latex Examination Gloves - Powdered | 71 |
| Latex Examination Gloves - Powder Free | 72 |
| Vinyl Examination Gloves - Powdered | 73 |
| Vinyl Examination Gloves - Powder Free | 74 |
| Nitrile Examination Gloves | 75 |
| Nitrile Chemotherapy Examination Gloves | 76 |
| Pe Gloves | 77 |

STERILE PLASTIC PRODUCTS


| | |
|---|----|
| Flowmeter | 79 |
| Infusion (Serum) Set | 79 |
| Urine Bag / T-Value and Push & Pull Valve | 80 |
| Blood Transfusion Set | 81 |

MEDICAL DISPOSABLES

| | |
|-------------------------|----|
| Steril Surgical Blades | 83 |
| Blood Lancet | 84 |
| Wooden Tongue Depressor | 85 |
| Shoe Covers | 86 |
| Face Mask | 87 |
| Soft Bar Cap | 88 |

CERTIFICATES


| | |
|--------------|---------|
| Certificates | 89 - 92 |
|--------------|---------|

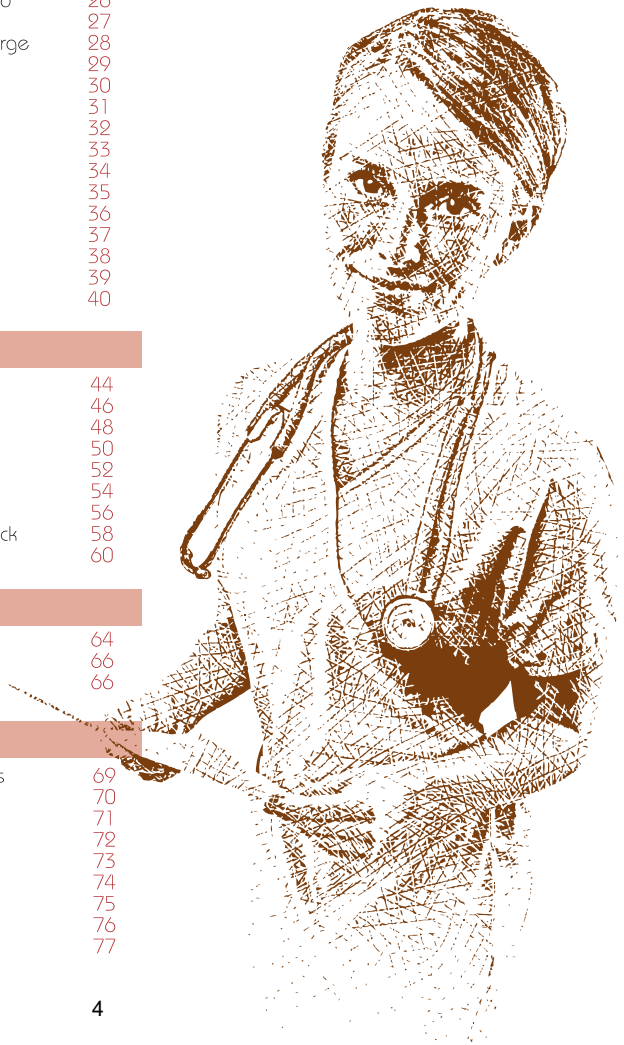

NONWOVEN FABRICS

Two-Layered Drape Materials

Perfect for many applications, they are the result of the combination of a low-linting nonwoven or tissue paper with high absorbing properties with an impervious film acting as a liquid barrier.


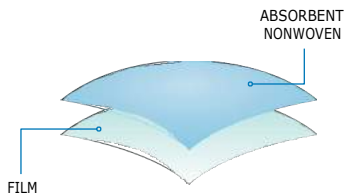


Absorbent Reinforcement Material for Critical Zones

BROCHE has developed a three-layered material specifically designed to enhance the absorption of liquids in critical zones.

Three-Layered Drape Materials

Capable of trapping liquid quickly and effectively, they are designed to be placed in direct contact with the skin of the patient and can be used for multiple purposes such as surgical drapes and kits.

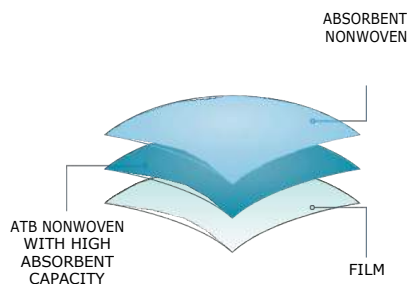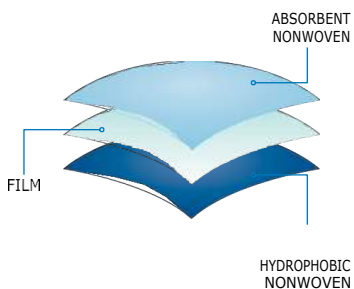

Product list

| PRODUCT CODE | APPLICATION | TOTAL BASIS WEIGHT (gsm) | COMPOSITION | |
|--------------|--|--------------------------|---|--------------------|
| | | | RAW MATERIAL | BASIS WEIGHT (gsm) |
| TDL | Two-Layered Surgical Drape | 54 | Hydrophilic Viscose Nonwoven | 25 |
| | | | Rubber Based Hot Melt Adhesive | 2 |
| | | | Micro-embossed Cast PE Film | 27 |
| TDL3 | Three-Layered Surgical Drape | 70 | Hydrophilic Viscose Nonwoven | 28 |
| | | | Rubber Based Hot Melt Adhesive | 2 |
| | | | Micro-embossed Cast PE Film | 25 |
| | | | White Hydrophobic SB Nonwoven | 15 |
| | | | | |
| SE | Absorbent Reinforcement Material for Surgical Drape | 80 | Hydrophilic Viscose Nonwoven | 28 |
| | | | Rubber Based Hot Melt Adhesive | 2 |
| | | | High-AbsorbencyViscose Nonwoven | 50 |
| SE3 | Absorbent Reinforcement Material for Surgical Drape (with PE Film) | 105 | Hydrophilic Viscose Nonwoven | 28 |
| | | | Rubber Based Hot Melt Adhesive | 2 |
| | | | High-AbsorbencyViscose Nonwoven | 50 |
| | | | Micro-embossed Cast PE Film | 25 |
| | | | | |
| DL | Raw Viscose | 28 | Viscose (Standard production) • Ranges from 20 gsm to 50 gsm | 28 |
| PE | PE Film | 25 | PE Film (Standard production) | 25 |
| | | | • Ranges from 20 gsm to 100 gsm | |
| | | | | |
| TABLE CLOTH | TABLE COVER | 60 | Micro-embossed Cast PE Film | 45 |
| | | | High-AbsorbencyViscose Nonwoven | 28 |

- Our products can be customized according to customer demands



EN 13795

European Standard for Surgical Drapes and Gowns

Introduction

This document provides an overview of the EN 13795 European Standard for surgical gowns and drapes, which outlines their performance requirements, test methodologies and explains the overall relevance to patients and the clinical staff.

The broad aim of EN 13795 is to establish an European recognised standard of quality and conformance to manufacturing, testing and performance specifications for all single-use and multiple-use surgical drapes and gowns.

Key aspects of Section 6



General requirements for Manufacturers, Processors and Products

Compliance with this Standard demonstrates that the device is fit for purpose and can be used on a patient as it conforms to a range of relevant testing procedures. This information must be fulfilled by the manufacturers and processors and all test methods and results must be made available as part of a quality assurance system, for both single-use and reusable devices.

It should be noted that surgical drapes and gowns are further categorised according to their performance and defined as **standard** or **high performance** devices.

General requirements

The manufacturer or processor must:

- for reusable devices: provide information on the appropriate process to allow re-use (cleaning, disinfection, packaging, sterilisation methods) including number of re-uses and any restriction to the re-use
- for sterile devices: provide instructions for sterilization methods
- differentiate between critical and less critical areas on the device, where appropriate, as well as physical identification of these areas
- upon request, reference test methods used, and corresponding test results (see Tables 1, 2, and 3), differentiating critical and less critical areas with appropriate rationale for the differentiation
- use validated manufacturing and processing procedures

General product requirements:

- it shall be possible to demonstrate that the product requirements of EN 13795 are met (see Tables 4, 5 and 6), and test results shall be recorded and retained
- the finished product (after sterilisation if appropriate) shall be tested prior to commercialisation
- during manufacturing and processing, testing shall be done according to the requirements of the manufacturer's or processor's quality system




Key aspects of Annex B

Test Methods

EN 13795 describes the standardised and harmonised test methodologies that all single-use and reusable surgical drapes, gowns and clean air suits must undergo, as part of a quality assurance system.

Test of resistance to microbial dry penetration - EN ISO 22612

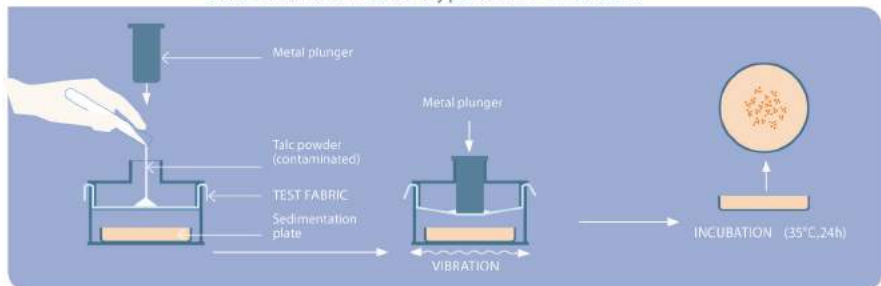


The test method is designed to determine the ability of materials to resist penetration of particles carrying micro-organisms under dry fabric conditions. The method establishes the quantity of micro-organisms that can penetrate through the test material being carried on talcum powder. Test results are expressed in CFU (colony forming units) that were observed on the agar plate.

Table 1 - Performance requirements for microbial dry penetration

| Unit | Surgical Gowns | | | | Surgical Drapes | | | |
|------|----------------------|--------------------|------------------|--------------------|----------------------|--------------------|------------------|--------------------|
| | Standard Performance | | High Performance | | Standard Performance | | High Performance | |
| | critical area | less critical area | critical area | less critical area | critical area | less critical area | critical area | less critical area |
| CFU | N/A | ≤ 300 * | N/A | ≤ 300 * | N/A | ≤ 300 * | N/A | ≤ 300 * |

a Test conditions: challenge concentration 10⁸ CFU/g talc, and 30 minutes vibration time.

Test of resistance to microbial wet penetration - EN ISO 22610

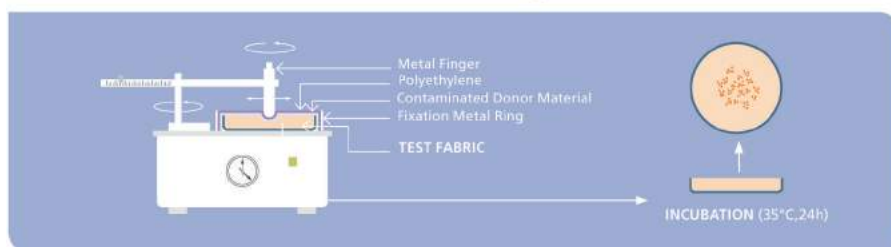

The purpose of this test is to evaluate the ability of fabrics to resist microbial penetration under conditions of liquid pooling on the fabric and mechanical stress. Test results are expressed in I_B "Barrier Index".


Table 2 - Performance requirements for microbial wet penetration

| Unit | Surgical Gowns | | | | Surgical Drapes | | | |
|-------|----------------------|--------------------|--------------------|--------------------|----------------------|--------------------|--------------------|--------------------|
| | Standard Performance | | High Performance | | Standard Performance | | High Performance | |
| | critical area | less critical area | critical area | less critical area | critical area | less critical area | critical area | less critical area |
| I_B | $\geq 2,8^b$ | N/A | 6,0 ^{b,c} | N/A | $\geq 2,8^b$ | N/A | 6,0 ^{b,c} | N/A |

b The Least Significant Difference (LSD) for I_B when estimated using EN ISO 22610, was found to be 0,98 at the 95% confidence level. This is the minimum difference needed to distinguish between two materials thought to be different. This means materials varying by up to 0,98 I_B are probably not different; materials varying by more than 0,98 I_B probably are different. (The 95% confidence level means that an observer would be correct 19 times out of 20 to accept these alternatives).

c $I_B = 6,0$ for the purpose of this standard means: no penetration. $I_B = 6,0$ is the maximum achievable value.

Test of microbial cleanliness - EN ISO 11737-1

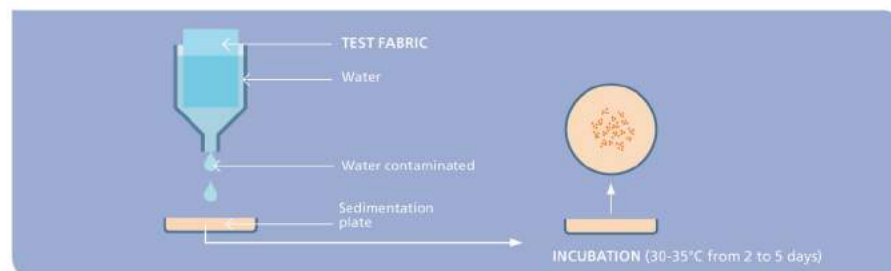

Microbial cleanliness determines the bioburden, meaning the number of viable micro-organisms on the product.

Microbial cleanliness is especially important to achieve sterilisation and a sterilisation assurance level of 10^{-6} as is required to label a product as sterile.

For products that are not sold as sterile, the test method allows assessment of their potential for microbial contamination.

The test results are expressed in a decimal logarithm of CFU/100cm². Lower numbers indicate better cleanliness.

Table 3 - Performance requirements for microbial cleanliness

| Unit | Surgical Gowns | | | | Surgical Drapes | | | |
|-------------------------|----------------------|--------------------|------------------|--------------------|----------------------|--------------------|------------------|--------------------|
| | Standard Performance | | High Performance | | Standard Performance | | High Performance | |
| | critical area | less critical area | critical area | less critical area | critical area | less critical area | critical area | less critical area |
| CFU/100 cm ² | ≤ 300 | ≤ 300 | ≤ 300 | ≤ 300 | ≤ 300 | ≤ 300 | ≤ 300 | ≤ 300 |


Table 5 - Characteristics to be evaluated and Performance Requirements for Surgical Drapes

| Performance requirements for Surgical Drapes | | | | | | |
|--|----------------|--------------------------------|-----------------------|----------------------------|-----------------------|----------------------------|
| Characteristic | Test method | Unit | Standard Performance | | High Performance | |
| | | | Critical product area | Less critical product area | Critical product area | Less critical product area |
| Resistance to microbial penetration – dry | EN ISO 22612 | CFU | N/A | ≤ 300 ^a | N/A | ≤ 300 ^a |
| Resistance to microbial penetration – wet | EN ISO 22610 | I_b | ≥ 2,8 ^b | N/A | 6,0 ^{b,c} | N/A |
| Cleanliness – microbial | EN ISO 11737-1 | CFU/100 cm ² | ≤ 300 | ≤ 300 | ≤ 300 | ≤ 300 |
| Cleanliness – particulate matter | EN ISO 9073-10 | IPM | ≤ 3,5 | ≤ 3,5 | ≤ 3,5 | ≤ 3,5 |
| Linting | EN ISO 9073-10 | log ₁₀ (lint count) | ≤ 4,0 | ≤ 4,0 | ≤ 4,0 | ≤ 4,0 |
| Resistance to liquid penetration | EN 20811 | cm H ₂ O | ≥ 30 | ≥ 10 | ≥ 100 | ≥ 10 |
| Bursting strength – dry | EN ISO 13938-1 | kPa | ≥ 40 | ≥ 40 | ≥ 40 | ≥ 40 |
| Bursting strength – wet | EN ISO 13938-1 | kPa | ≥ 40 | N/A | ≥ 40 | N/A |
| Tensile strength – dry | EN 29073-3 | N | ≥ 15 | ≥ 15 | ≥ 20 | ≥ 20 |
| Tensile strength – wet | EN 29073-3 | N | ≥ 15 | N/A | ≥ 20 | N/A |

a Test conditions: challenge concentration 10⁶ CFU/g talc. and 30 minutes vibration time.

b The Least Significant Difference (LSD) for I_b when estimated using EN ISO 22610, was found to be 0,98 at the 95% confidence level. This is the minimum difference needed to distinguish between two materials thought to be different. This means materials varying by up to 0,98 I_b are probably not different; materials varying by more than 0,98 I_b probably are different. (The 95% confidence level means that an observer would be correct 19 times out of 20 to accept these alternatives).

c $I_b = 6,0$ for the purpose of this standard means: no penetration. $I_b = 6,0$ is the maximum achievable value.



■ Critical area
■ Less critical area

Table 6 - Characteristics to be evaluated and performance requirements for Clean Air Suits

| Performance requirements for Clean Air Suits | | | |
|--|----------------|--------------------------------|--------------------------|
| Characteristic | Test method | Unit | Requirement ^b |
| Resistance to microbial penetration – dry | EN ISO 22612 | CFU | ≤ 300 ^a |
| Cleanliness – microbial | EN ISO 11737-1 | CFU/100 cm ² | ≤ 300 |
| Cleanliness – particulate matter | EN ISO 9073-10 | IPM | ≤ 3,5 |
| Linting | EN ISO 9073-10 | log ₁₀ (lint count) | ≤ 4,0 |
| Bursting strength – dry | EN ISO 13938-1 | kPa | ≥ 40 |
| Tensile strength – dry | EN 29073-3 | N | ≥ 20 |

a Test conditions: challenge concentration 10⁶ CFU/g talc. and 30 minutes vibration time.

b Performance requirements apply for all products areas of clean air suits.

WHY BROCHE NON WOVEDS

The Safest Route is Impermeable (Laminated) Fabrics

Healthcare facilities face similar challenges :

- Improving efficiencies and ensuring patient safety

Many hospitals specifically mention improving efficiencies as a key challenge and ensuring patient safety as their main focus.

- Multiresistant bacteria

It is a well known fact that there is an increasing threat from multiresistant bacteria and that surgical site infections are very expensive for hospitals and society in general.

- Surgical site infections

In spite of high hygiene and asepsis standards, there are approximately three million healthcare-associated infections in the European Union each year. Not all of these infections are critical to the patient but they are all critical in the sense that they are painful for the individual and consume valuable hospital resources.



Some call it impermeable drapes.

We call it optimal safety.

- BROCHE NONWOVENS are dedicated to infection control in and around the operating room. We have always taken great pride in supplying healthcare facilities, all around the world, with products and solutions to ensure patient safety. Impermeable materials are always the safest choice, which is why BROCHE NONWOVENS has made the entire drape product range from impermeable.


Why Impermeable (Laminated) Drapes?

When introduced, the fluid repellent single-use surgical drapes represented a real breakthrough in fabric technology. This material has served the global healthcare industry well, but as technology advances, we can now offer materials better suited to meet today's requirements.

No Compromises

Fluid repellent surgical drapes are vulnerable to liquid penetration despite meeting the standard EN13795. Today we know that fluid strikethrough can create a pathway for microorganisms, which can result in surgical site infections.

The wet bacterial penetration test shows that bacteria pass through a fluid repellent drape after 15 minutes of testing. The impermeable drape from BROCHE NONWOVENS showed no penetration of liquid and bacteria at all.

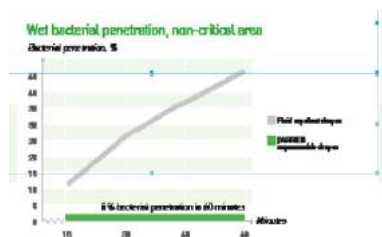

Fluid Repellent Surgical Drapes


- Impermeable only in the critical area
- Vulnerable to liquid penetration, strikethrough, outside of the critical area
- Increased risk of bacterial and viral (as well as other microorganisms such as fungi and spores) penetration compared to impermeable drapes

Impermeable (Laminated) Surgical Drapes

- Impermeable throughout the drape
- Provide the highest level of protection possible in surgical drapes
- Always the safest choice

The safest draping material is impermeable

BROCHE NONWOVENS range of impermeable drapes covers all types of surgical interventions. The range is available in 1–4 ply materials, depending on the needs of the specific procedure.

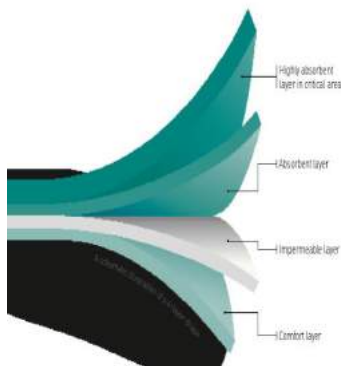


Why BROCHE NONWOVENS surgical drapes?

BROCHE NONWOVENS is dedicated to infection control. Overall improvements in design and material are part of the continuous work to always offer the safest choice.

- Comprehensive range of impermeable drapes available for all types of surgical interventions to fill all draping needs
- Continuous training and support to ensure optimised cost efficiencies and optimal usage of your products
- Introduction of new solutions when procedural needs change
- Supply and logistics system to ensure that the right products are available at the right time, spending a minimum of your resources.



General Surgery Pack - Standard

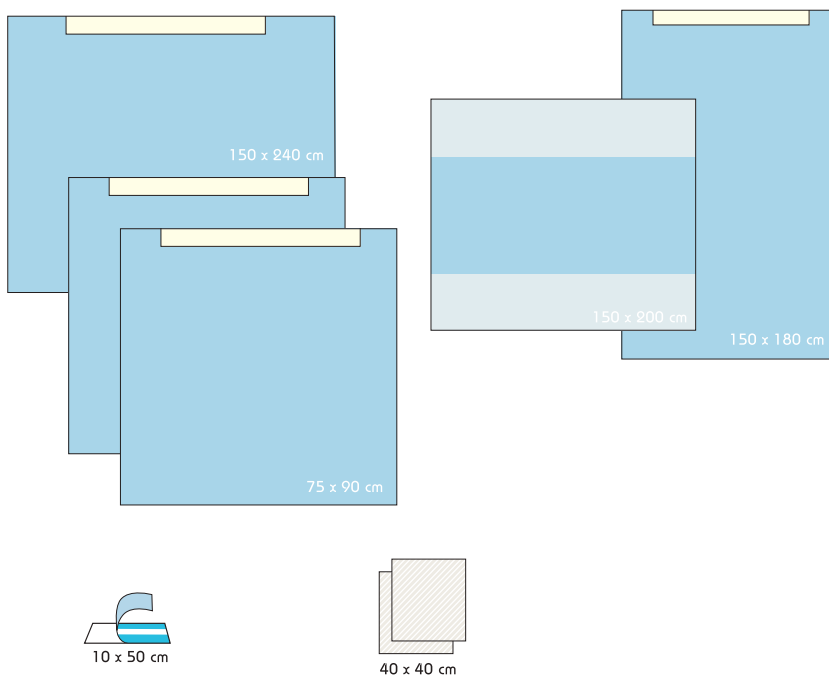


High Absorbent DL
 SMS
 PE Film
 Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|------------------------|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| ADS009 | Anesthesia Drape | 150 x 240 cm | 1 |
| ADS003 | Adhesive Drape | 75 x 90 cm | 2 |
| ADS008 | Adhesive Drape | 150 x 180 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

General Surgery Pack - Large

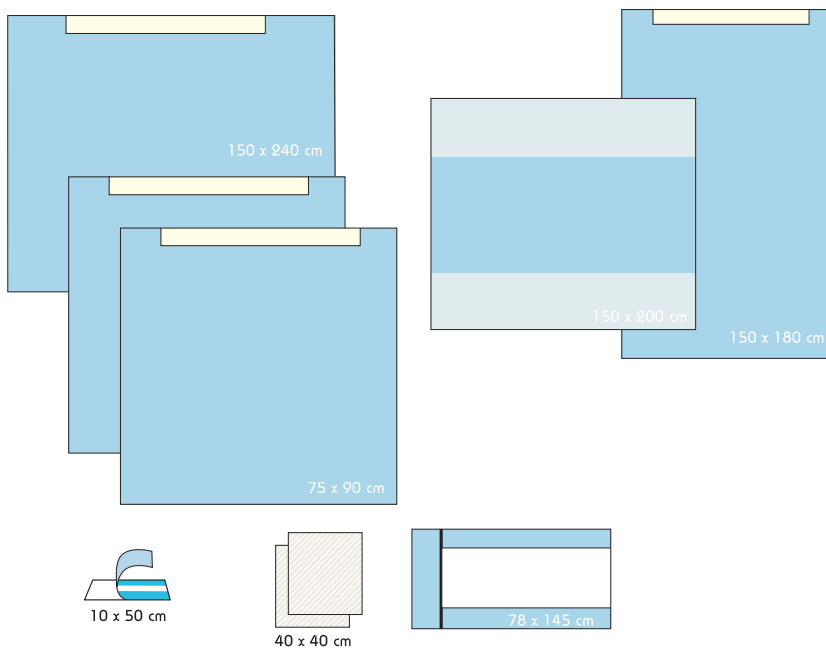


High Absorbent DL
 SMS
 PE Film
 Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|------------------------|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| ADS009 | Anesthesia Drape | 150 x 240 cm | 1 |
| ADS003 | Adhesive Drape | 75 x 90 cm | 2 |
| ADS008 | Adhesive Drape | 150 x 180 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

General Surgery Pack - Extra Large


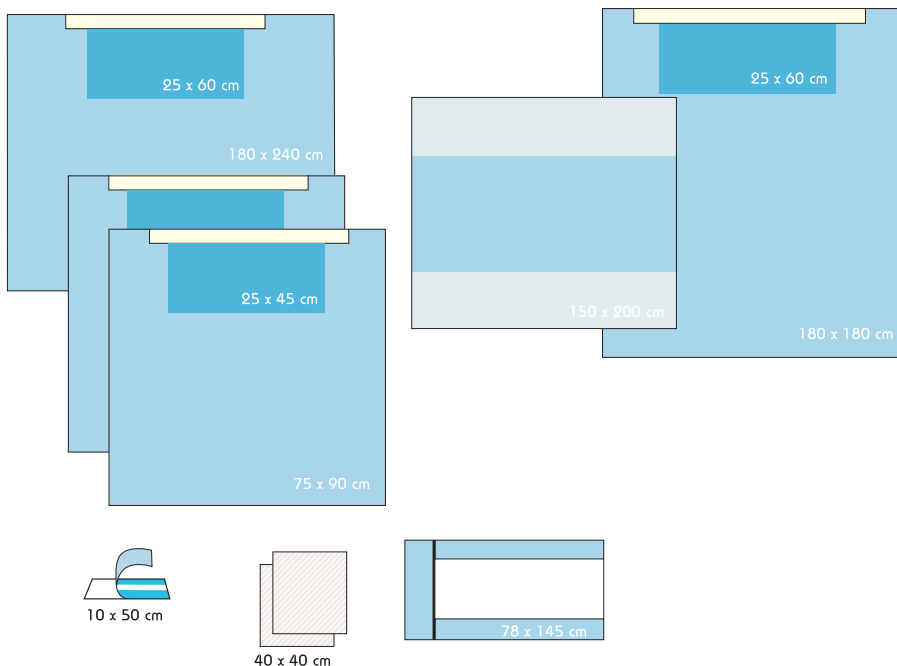


High Absorbent DL
 SMS
 Extra Absorbent
 PE Film
 Adhesive Tape

| Codes | Description | Dimension | Quantity |
|---------|--|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| ADS0011 | Anesthesia Drape, Extra Absorbing 25x60 cm | 180 x 240 cm | 1 |
| ADS003 | Adhesive Drape, Extra Absorbing 25x45 cm | 75 x 90 cm | 2 |
| ADS010 | Adhesive Drape, Extra Absorbing 25x60 cm | 180 x 180 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Laparoscopy Pack



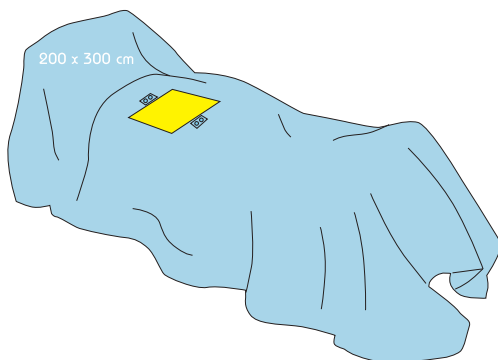


High Absorbent DL
 SMS
 PE Film
 Insice Film
 Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|--------------------------------------|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| LDS001 | Laparoscopy Drape, aperture 25x30 cm | 200 x 300 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Angiography Pack - Standard

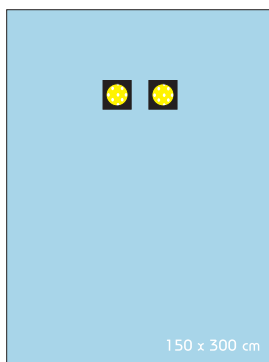


High Absorbent DL
 SMS
 PE Film
 Insicle Film

| Codes | Description | Dimension | Quantity |
|--------|-----------------------------------|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| APS002 | Angiography Drape, apertures 9 cm | 150 x 300 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Angiography Pack - Large

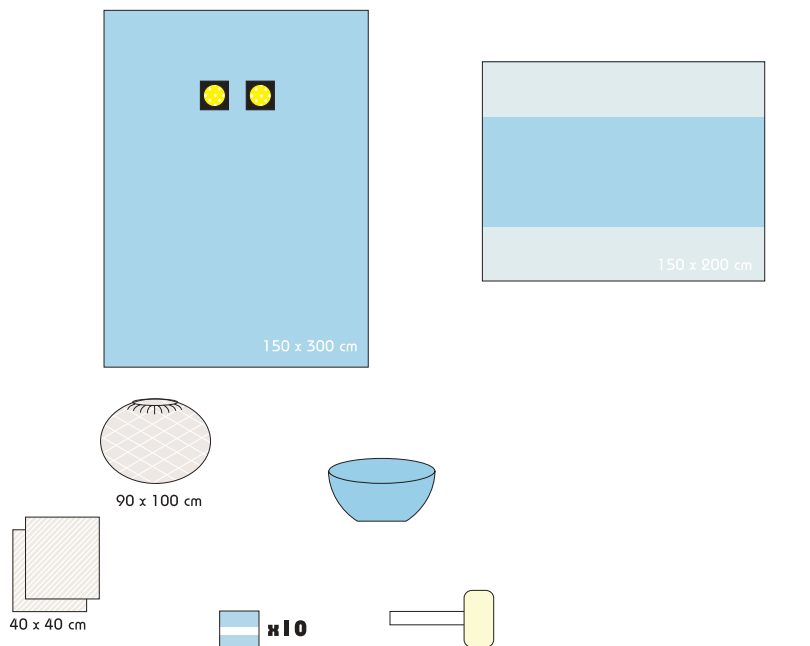

High Absorbent DL

SMS




PE Film

Insite Film

| Codes | Description | Dimension | Quantity |
|--------|-----------------------------------|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| APS002 | Angiography Drape, apertures 9 cm | 150 x 300 cm | 1 |
| FSC001 | Fluoroscopy Cover, PVC | 90 x 100 cm | 1 |
| BSS001 | Betadine Sponge | ST | 1 |
| SCS001 | Solution Cup | 500 cc | 1 |
| GSS001 | Gauze Swabs | 7,5 x 7,5 cm | 10 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Angiography Pack W / Transparent Panel Standard

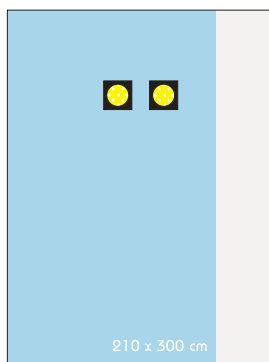


High Absorbent DL
 SMS
 PE Film
 Insice Film

| Codes | Description | Dimension | Quantity |
|--------|--|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| APS001 | Angiography Drape With Transparent Panel, apertures 9 cm | 210 x 300 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Angiography Pack W / Transparent Panel Large

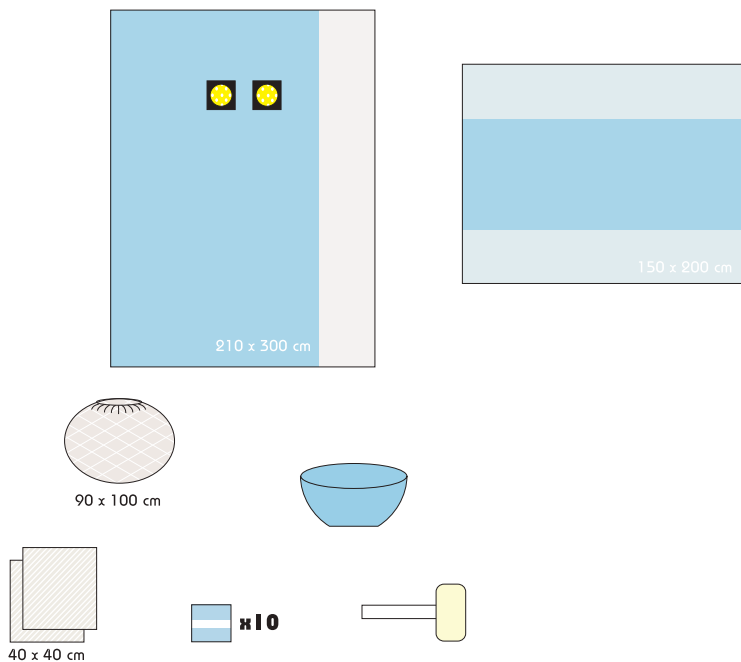

High Absorbent DL

SMS


PE Film

Insice Film

| Codes | Description | Dimension | Quantity |
|--------|---|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| APS001 | Angiography Drape With, Transparent Panel, apertures 9 cm | 210 x 300 cm | 1 |
| FCS001 | Fluoroscopy Cover, PVC | 90 x 100 cm | 1 |
| SCS001 | Solution Cup | 500 cc | 1 |
| BSS001 | Betadine Sponge | ST | 1 |
| GSS001 | Gauze Swabs | 7,5 x 7,5 cm | 10 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Cardiovascular Pack W / Pouch - Standard

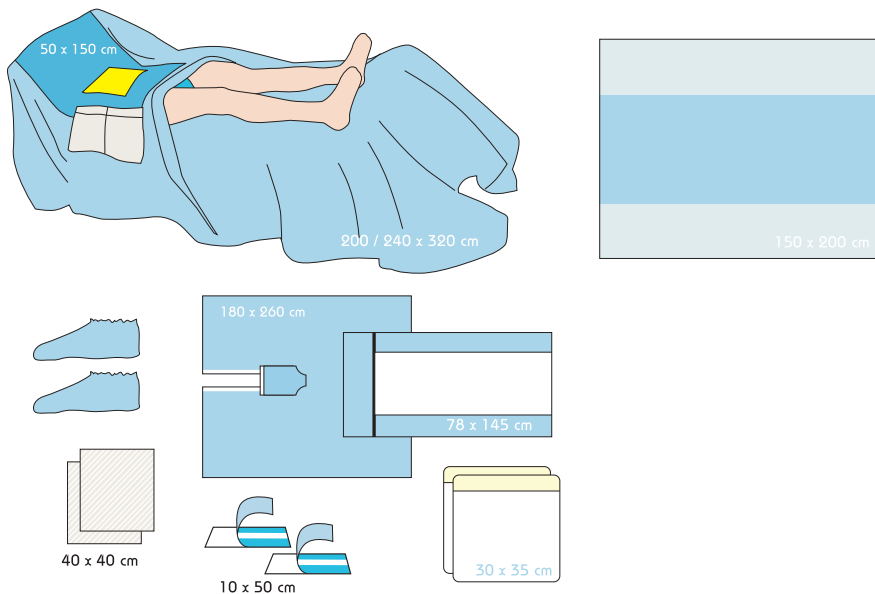


■ High Absorbent DL ■ Super Absorbent DL ■ SMS ■ PE Film ■ Insice Film

| Codes | Description | Dimension | Quantity |
|--------|---|------------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| UDS003 | U Split Perineal Drape, aperture 20 x 100 cm | 180 x 260 cm | 1 |
| CVS002 | Cardiovascular Drape, extra absorbing area 50 x 150 cm | 200/240 x 320 cm | 1 |
| FSS001 | Feet Socks | ST | 2 |
| OPS001 | Op Tapes | 10 x 50 cm | 2 |
| MPS001 | Mobile PVC Bag | 30 x 35 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Cardiovascular Pack W / Pouch - Large

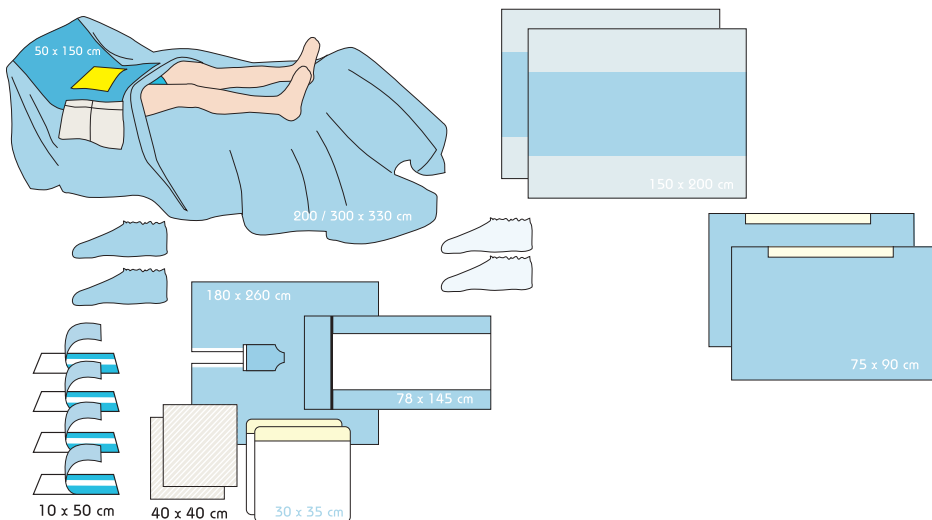


■ High Absorbent DL ■ Super Absorbent DL ■ SMS ■ PE Film ■ Insice Film

| Codes | Description | Dimension | Quantity |
|--------|---|------------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 2 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| UDS003 | U Split Perineal Drape, aperture 20 x 100 cm | 180 x 260 cm | 1 |
| CVS002 | Cardiovascular Drape, aperture 32 x 40 cm | 200/300 x 330 cm | 1 |
| FSS001 | Feet Socks | ST | 2 |
| FSS002 | Feet Socks | Transparent | 2 |
| ADS003 | Adhesive Drape | 75 x 90 cm | 2 |
| OPS001 | Op Tapes | 10 x 50 cm | 4 |
| MPS001 | Mobile PVC Bag | 30 x 35 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Tur Pack W / Pouch (Urology Set)

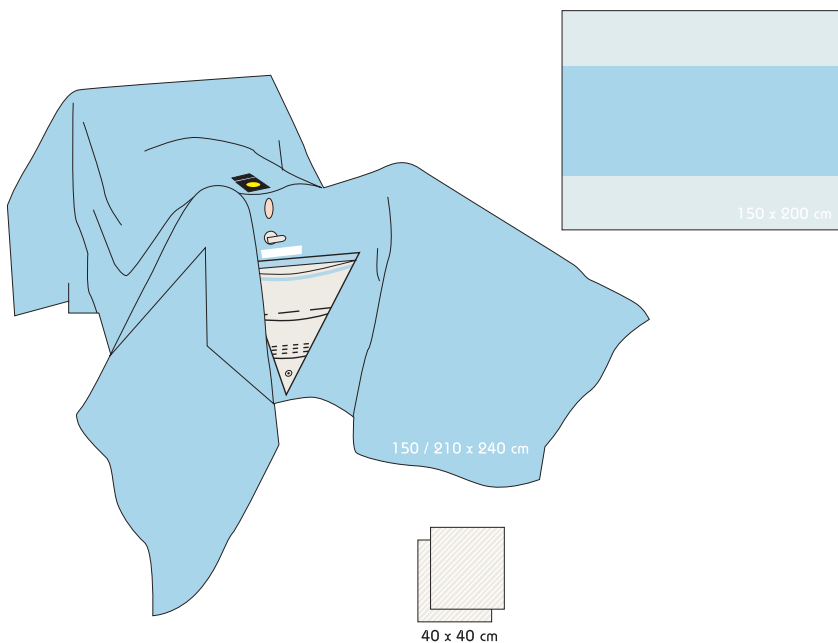

■ High Absorbent DL


■ SMS

■ PE Film

| Codes | Description | Dimension | Quantity |
|--------|---|--------------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| UDS001 | Urology Drape W / Pouch, apertures 8 cm and 5 cm | 150 / 210 x 240 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Lithotomic Gynaecology Pack W / Pouch

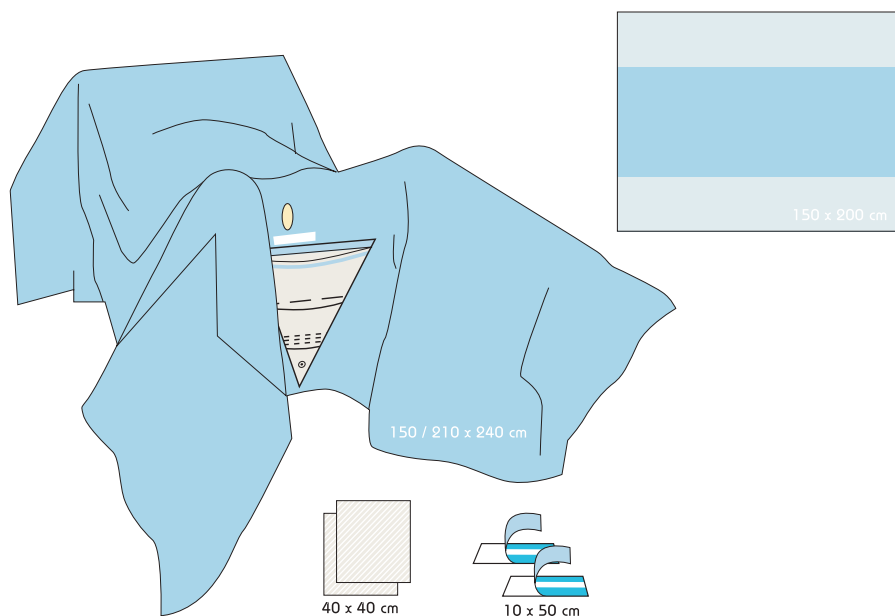

■ High Absorbent DL





■ SMS

■ PE Film

| Codes | Description | Dimension | Quantity |
|--------|--|--------------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| UDS001 | Lithotomic Gynaecology W / Pouch apertures 10 x 15 cm | 150 / 210 x 240 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Gynaecology / Cystoscopy Pack

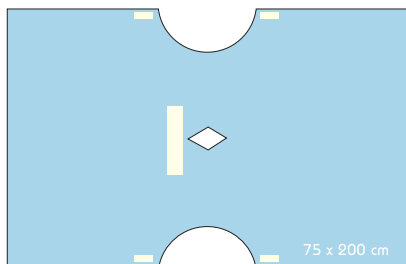

■ High Absorbent DL

■ SMS


■ PE Film

■ Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|---|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| CDS001 | Cystoscopy Drape W / Adhesive Tape, apertures 10 x 15 cm | 75 x 200 cm | 1 |
| LGS001 | Leggings | 75 x 120 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Caesarean Section Pack W / Pouch - Standard

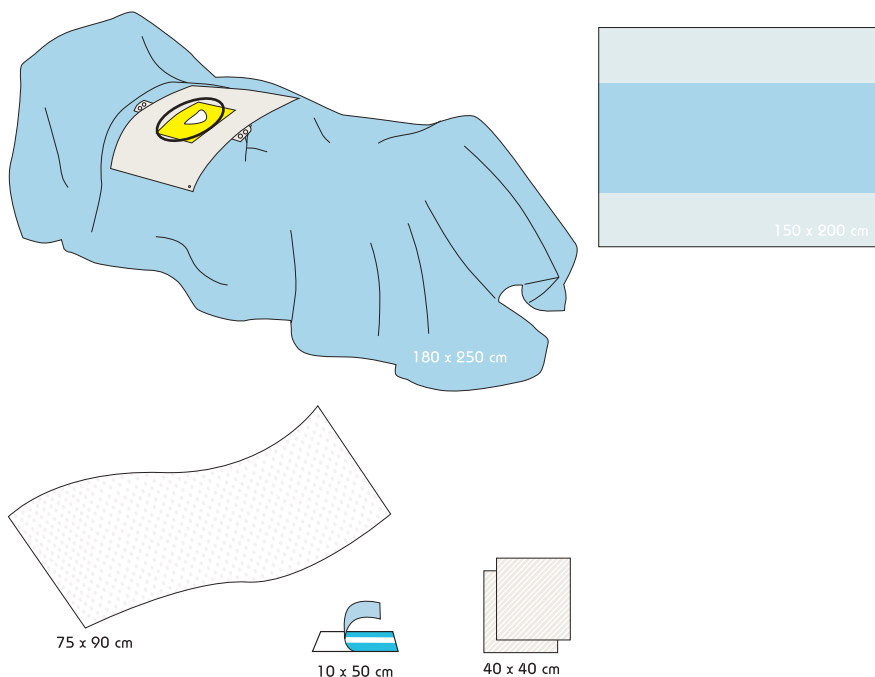


High Absorbent DL
 SMS
 PE Film
 Insicle Film

| Codes | Description | Dimension | Quantity |
|--------|---|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| CES001 | Caesarean Drape W / Pouch apertures 32 x 38 cm | 180 x 250 cm | 1 |
| BBS001 | Baby Blanket | 75 x 90 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Caesarean Section Pack W / Pouch - Large

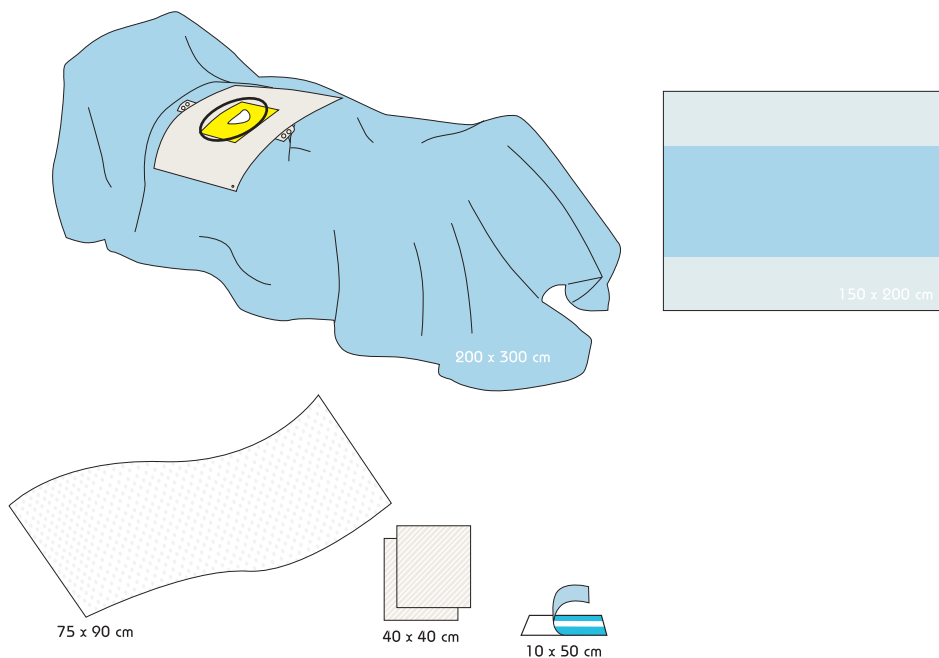


High Absorbent DL
 SMS
 PE Film
 Insicle Film

| Codes | Description | Dimension | Quantity |
|--------|---|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| CES002 | Caesarean Drape W / Pouch apertures 38 x 32 cm | 200 x 300 cm | 1 |
| BBS001 | Baby Blanket | 75 x 90 cm | 1 |
| OPS001 | Op-Tapes | 10 x50 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Caesarean Section Pack W / Pouch - Extra Large

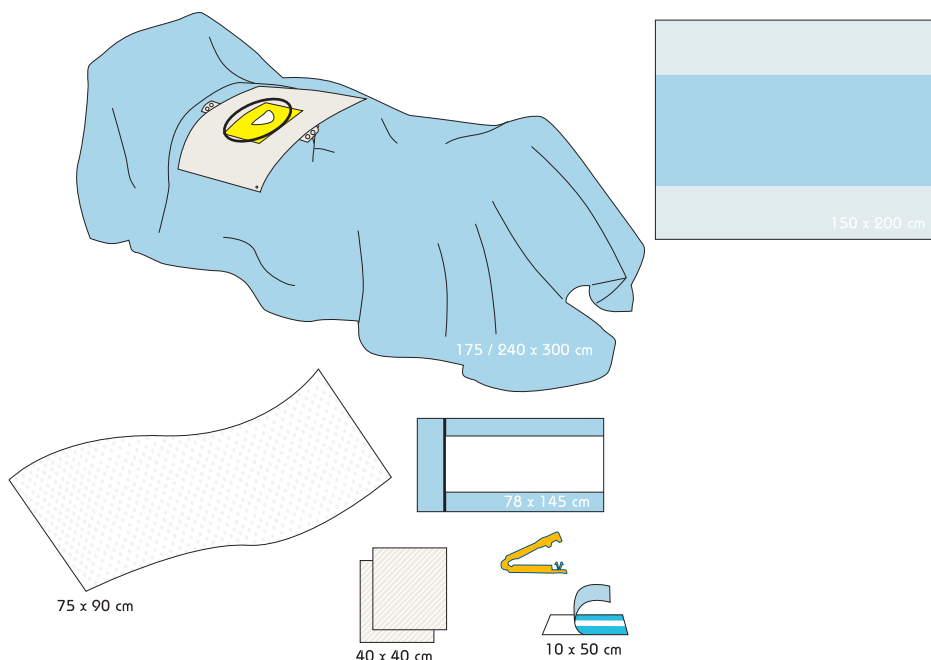

■ High Absorbent DL

■ SMS


■ PE Film

■ Insice Film

| Codes | Description | Dimension | Quantity |
|--------|---|--------------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| CES003 | Caesarean Drape W / Pouch apertures 38 x 32 cm | 175 / 240 x 300 cm | 1 |
| BBS001 | Baby Blanket | 75 x 90 cm | 1 |
| CLP001 | Umbilical Clamp | ST | 1 |
| OPS001 | Op-Tapes | 10 x50 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Delivery Pack

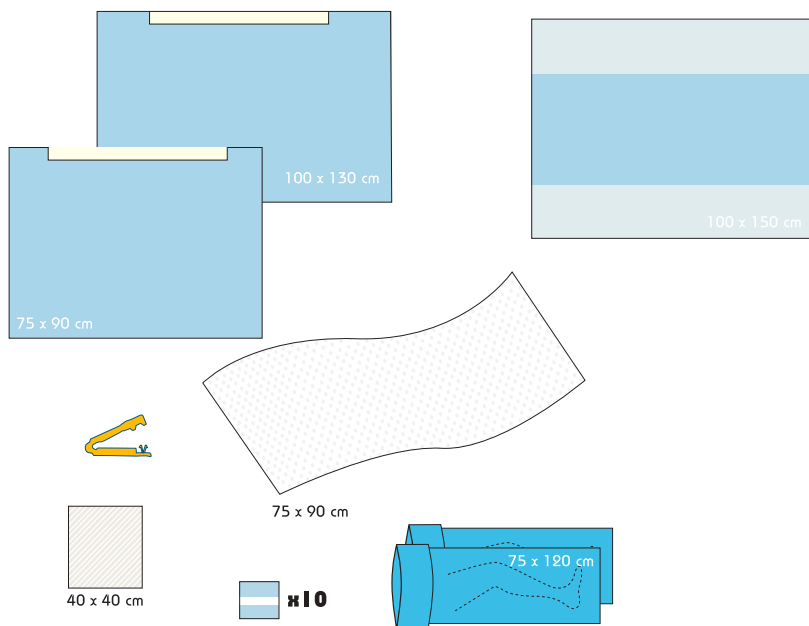


High Absorbent DL
 SMS
 PE Film
 Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|-----------------------------------|--------------|----------|
| ITS001 | Instrument Table Cover | 100 x 150 cm | 1 |
| UDS002 | Underbuttock Drape | 100 x 130 cm | 1 |
| ADS003 | Abdominal Drape W / Adhesive Tape | 75 x 90 cm | 1 |
| LGS002 | Leggings | 75 x 120 cm | 2 |
| CLP001 | Umbilical Clamp | ST | 1 |
| BBS001 | Baby Blanket | 75 x 90 cm | 1 |
| GSS001 | Gauze Swabs | 7,5 x 7,5 cm | 10 |
| HTS001 | Hand Towels | 40 x 40 cm | 1 |

*Product contents can be customized upon request

Delivery Pack W / Pouch

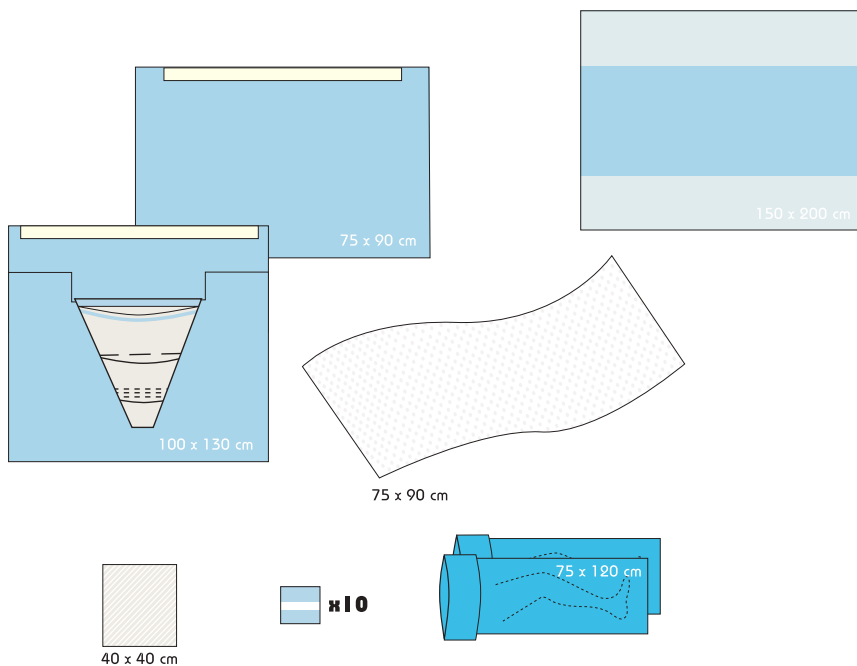


High Absorbent DL
 SMS
 PE Film
 Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|-----------------------------------|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| UDS005 | Underbuttock Drape W / Pouch | 100 x 130 cm | 1 |
| ADS003 | Abdominal Drape W / Adhesive Tape | 75 x 90 cm | 1 |
| LGS002 | Leggings | 75 x 120 cm | 2 |
| BBS001 | Baby Blanket | 75 x 90 cm | 1 |
| GSS001 | Gauze Swabs | 7,5 x 7,5 cm | 10 |
| HTS001 | Hand Towels | 40 x 40 cm | 1 |

*Product contents can be customized upon request

Arthroscopy Pack W / Pouch - Standard

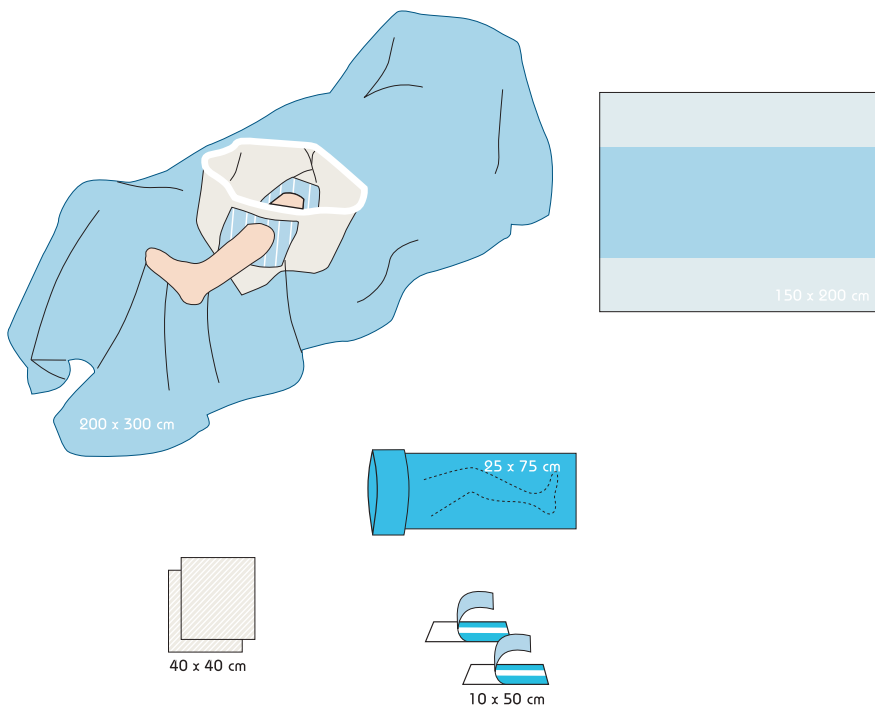


High Absorbent DL
 SMS
 PE Film
 Insicle Film

| Codes | Description | Dimension | Quantity |
|--------|---|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| ATS001 | Arthroscopy Drape W / Pouch, apertures 6 cm | 200 x 300 cm | 1 |
| SSS001 | Stockinet | 25 x 75 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Arthroscopy Pack W / Pouch - Large

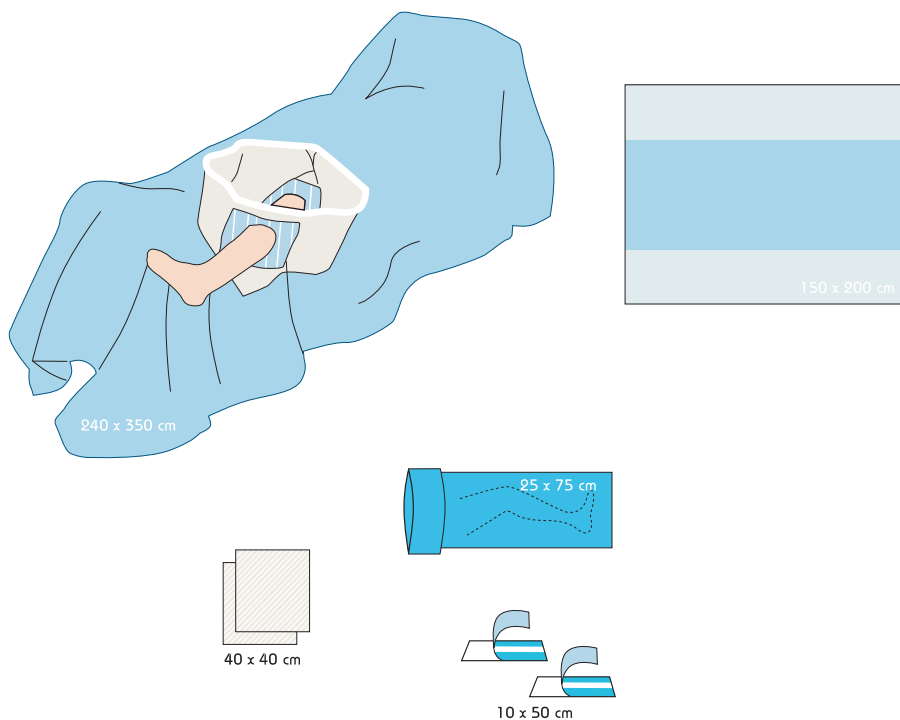


High Absorbent DL
 SMS
 PE Film
 Insicle Film

| Codes | Description | Dimension | Quantity |
|--------|---|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| ATS001 | Arthroscopy Drape W / Pouch, apertures 6 cm | 240 x 350 cm | 1 |
| SSS001 | Stockinet | 25 x 75 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Arthroscopy Pack W / Pouch - Extra Large

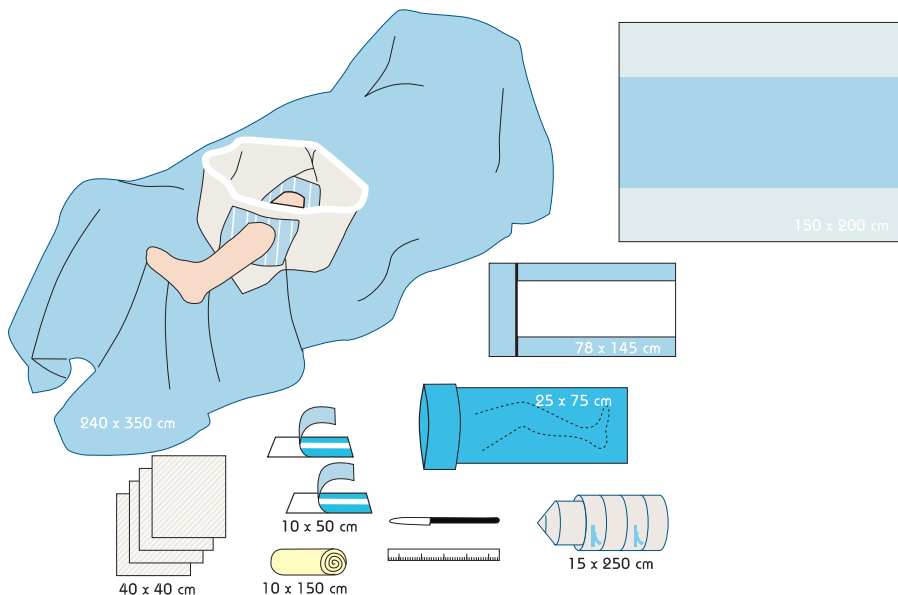

■ High Absorbent DL

■ SMS


■ PE Film

■ Insice Film

| Codes | Description | Dimension | Quantity |
|--------|---|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| ATS002 | Arthroscopy Drape W / Pouch, apertures 6 cm | 240 x 350 cm | 1 |
| CCS001 | Camera Cover | 15 x 250 cm | 1 |
| SMS001 | Skin Marker and Ruler | ST | 1 |
| €BS001 | Elastic Bandage | 10 x 150 cm | 1 |
| SSS001 | Stockinet | 25 x 75 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 4 |

*Product contents can be customized upon request

Craniotomy Pack W / Pouch






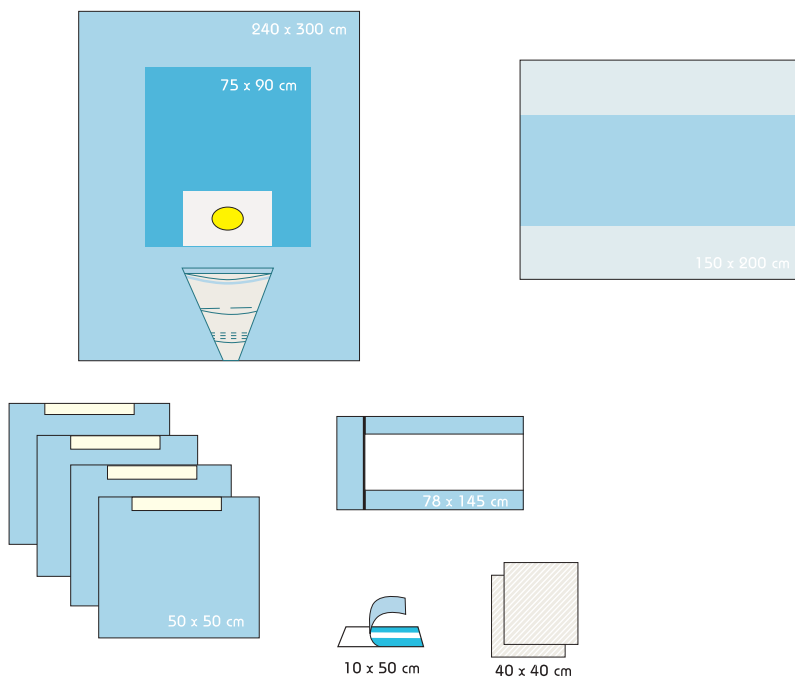


■ High Absorbent DL ■ Super Absorbent DL ■ SMS ■ PE Film ■ Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|--|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| CTS001 | Craniotomy Drape W / Pouch, aperture 20 x 30 cm, extra absorbing area 75 x 90 cm | 240 x 300 cm | 1 |
| ADS001 | Adhesive Drape | 50 x 50 cm | 4 |
| OPS001 | Op-Tapes | 10 x 50 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

E.N.T. Pack

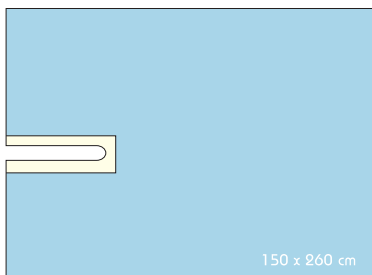

■ High Absorbent DL

■ SMS


■ PE Film

■ Inside Film

| Codes | Description | Dimension | Quantity |
|--------|--------------------------------------|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 1 |
| MYS001 | Mayo Stand Cover | 78 x 145 cm | 1 |
| UDS004 | U Split Drape, aperture 7 x 70 cm | 150 x 260 cm | 1 |
| ADS003 | Adhesive Drape | 75 x 90 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Hip Pack U

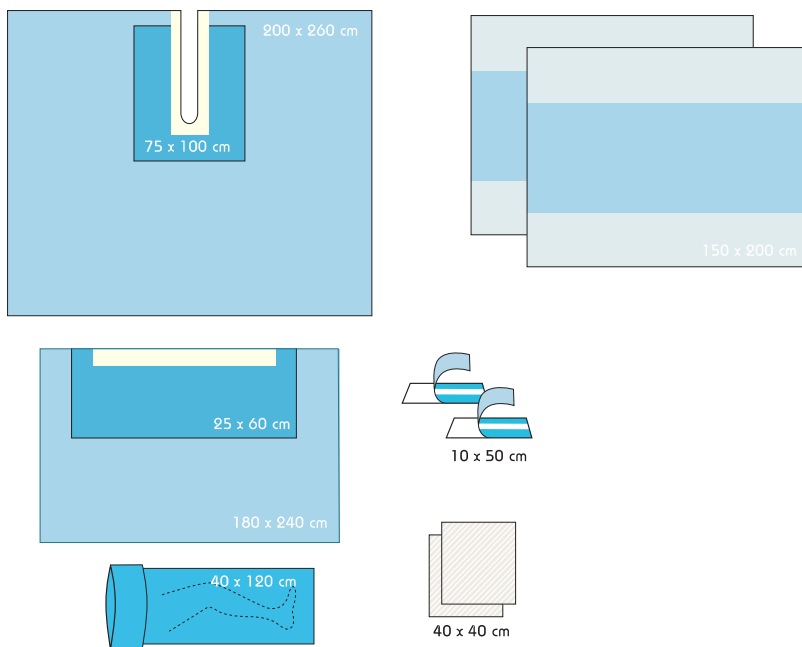


■ High Absorbent DL ■ Super Absorbent DL ■ SMS ■ PE Film ■ Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|---|--------------|----------|
| ITS003 | Instrument Table Cover | 150 x 200 cm | 2 |
| UDS006 | U Split Drape, aperture 20 x 100 cm, extra absorbing area 75 x 100 cm | 200 x 260 cm | 1 |
| ADS011 | Adhesive Drape, extra absorbing area 25 x 60 cm | 180 X 240 cm | 1 |
| LGS003 | Leggings | 40 x 120 cm | 1 |
| OPS001 | Op-Tapes | 10 x 50 cm | 2 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request

Implant Pack



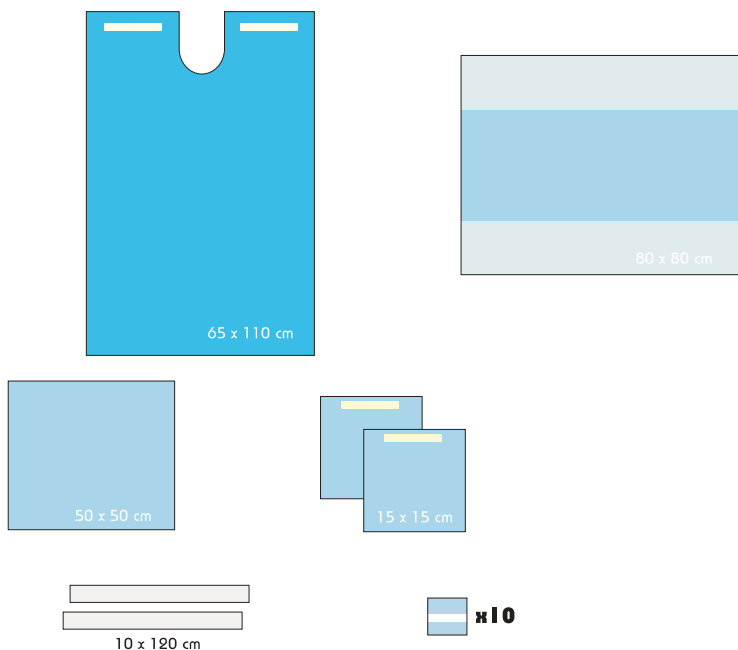


■ High Absorbent DL
 ■ SMS
 ■ PE Film
 ■ Adhesive Tape

| Codes | Description | Dimension | Quantity |
|--------|--------------------------------|--------------|----------|
| ITS002 | Instrument Table Cover | 80 x 80 cm | 1 |
| DPS001 | Dental Patient Gown W / Velcro | 65 x 110 cm | 1 |
| TDS001 | Table Drape | 50 x 50 cm | 1 |
| RDS001 | Reflector Drape | 15 x 15 cm | 2 |
| THS001 | Transparent Hose Cover | 10 x 120 cm | 2 |
| GSS001 | Gauze Swabs | 7,5 x 7,5 cm | 10 |

*Product contents can be customized upon request

Single Pouch Ophthalmic Pack

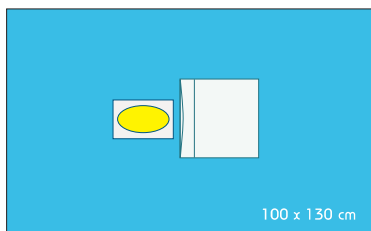

 SMS


 PE Film

 Inside Film

| Codes | Description | Dimension | Quantity |
|--------|--|--------------|----------|
| ITS001 | Instrument Table Cover | 100 x 150 cm | 1 |
| ODS001 | Single Pouch Ophthalmic Drape W / Pouch, aperture 10 x 10 | 100 x 130 cm | 1 |
| HTS001 | Hand Towels | 40 x 40 cm | 2 |

*Product contents can be customized upon request


Adhesive Drapes

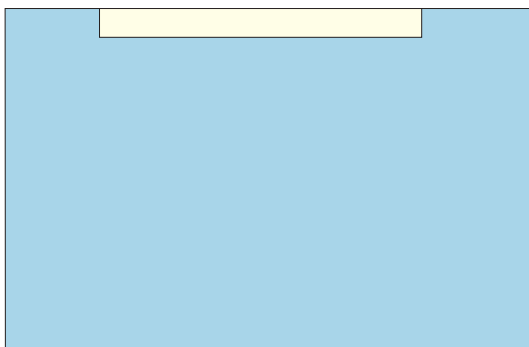

■ High Absorbent DL ■ Adhesive Tape

| Sterile Codes | Description | Dimension |
|---------------|----------------|--------------|
| ADS001 | Adhesive Drape | 50 x 50 cm |
| ADS002 | Adhesive Drape | 75 x 75 cm |
| ADS003 | Adhesive Drape | 75 x 90 cm |
| ADS004 | Adhesive Drape | 75 x 150 cm |
| ADS005 | Adhesive Drape | 100 x 100 cm |
| ADS006 | Adhesive Drape | 120 x 150 cm |
| ADS007 | Adhesive Drape | 120 x 240 cm |
| ADS008 | Adhesive Drape | 150 x 180 cm |
| ADS009 | Adhesive Drape | 150 x 240 cm |
| ADS010 | Adhesive Drape | 180 x 180 cm |
| ADS011 | Adhesive Drape | 180 x 240 cm |

Non Sterile Welcome Pack (Waterproof)

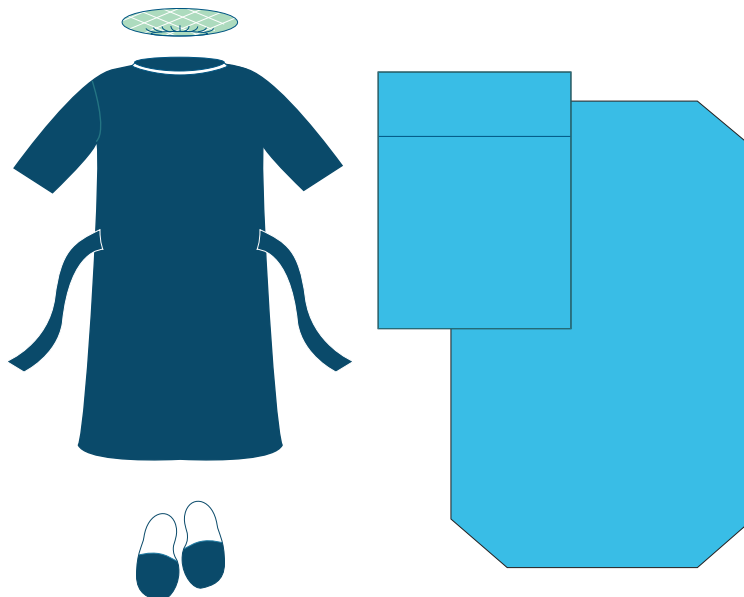

■ PP

■ SMS

| Codes | Description | Dimension | Quantity |
|----------|-----------------------------|--------------|----------|
| BCNS001 | Bed Cover W / Elastic Edges | 160 x 240 cm | 1 |
| PCNS001 | Pillow Cover | 50 x 70 cm | 1 |
| SLPNS | Slippers | ST | 1 |
| PGNSS001 | Patient Gown Short Sleeve | LARGE | 1 |
| SBCNS001 | Soft Bar Caps | ST | 1 |

Product Code Without Gown

WPNS001 - NG

*Product contents can be customized upon request



Broche[®]

Procedure Packs





| Description | Quantity |
|---------------------------------|----------|
| Paper or SMS wrap | 1 |
| Back table cover to wrap | 1 |
| Back table cover book folded | 1 |
| Mayo stand cover | 1 |
| Instrument diathermy pouch | 1 |
| Kidney bowl 700ml | 1 |
| Blade 21 | 1 |
| Blade 23 | 1 |
| Bowl 500ml | 1 |
| Bowl 1000ml | 1 |
| Bowl 250ml | 2 |
| Jug 1000ml | 1 |
| Cautery pencil | 1 |
| Cautery quiver | 1 |
| Cautery tip cleaner | 1 |
| Light handle cover | 2 |
| Incise or ioban | 1 |
| Drape laparotomy | 1 |
| Skin marker | 1 |
| Suction Yankauer | 1 |
| Suction tubing | 2 |
| Needle counter box or pad | 2 |
| Swab gauze small X-ray tied 5's | 2 |
| Swab gauze large X-ray tied 5's | 2 |
| Hand towel | 1 |
| Drape medium plain | 2 |
| Op tape | 2 |
| Dressing pad | 1 |
| Dressings adhesive | 1 |



| | | | | |
|---------------------------------|--------------------------|------------------------------------|---------------------------------------|--|
| HEPARIN <small>10000</small> | SODIUM CHLORIDE | VENOUS | KAMAL COCKTAIL | FLECAVINE |
| HEPARIN <small>10000</small> | SODIUM CHLORIDE | VERAPAMIL | CHIAZEMULS | DEXAMETHASONE |
| HEPARIN <small>10000</small> | CONTRAST | ADENOSINE | DIAMORPHINE <small>10mg/ml</small> | NALOXONE |
| HEPARINISED SALINE | CONTRAST | UDOCARNE <small>10mg/ml</small> | REOPRO | PILOCARPINE <small>1mg/ml</small> |
| HEPARINISED SALINE | 10 CONTRAST 10 SALINE | UDOCARNE <small>10mg/ml</small> | MIDAZOLAM | PILOCARPINE <small>1mg/ml</small> |
| HEPARINISED SALINE | ATROPINE | ATRATE | MIDAZOLAM | ADRENALINE |
| HEPARINISED SALINE | ARTERIAL | ATRATE | ISOPRENALINE | ANTIDOTIC |
| HEPARINISED SALINE | VENOUS | KAMAL COCKTAIL | ISOPRENALINE | CAUTION: AND SPIRITS TO DRY SURFACES ONLY |



| Description | Quantity |
|---|----------|
| Namic™ 2 port manifold | 1 |
| Galipot 120ml | 2 |
| Guidewire bowl | 1 |
| Syringe, P.E, 10ml, U/S | 4 |
| Syringe, P.E, 5ml, U/S | 1 |
| Label set | 1 |
| Needle 18G x 7cm (70mm) introducer needle | 1 |
| Needle 21G x 3.8cm hypo green | 1 |
| Needle 23G x 3cm hypo blue | 1 |
| Scalpel No.11 | 1 |
| Sponge stick medium 15cm | 2 |
| Swab gauze, 10 x 10cm, 12ply, 10 pack | 1 |
| Medium fluoro cover | 1 |
| Sharps needle containment device | 1 |
| Angio drape, 2 fenestrations, 3 ply laminate, no windows, 300cm | 1 |
| Equipment cover, P.E, 100 x 100cm | 1 |
| Bowl 250ml | 1 |
| Sponge bowl 500ml | 1 |



| Description | Quantity |
|------------------------------|----------|
| Paper or SMS wrap | 1 |
| Back table cover to wrap | 1 |
| Back table cover book folded | 1 |
| Bowl 6000ml or bowl liner | 1 |
| Baby blanket | 1 |
| Blade 21 | 1 |
| Blade 23 | 1 |
| Bowl 500ml | 1 |
| Umbilical clamp | 1 |
| Mayo stand cover | 1 |
| Cautery diathermy pencil | 1 |
| Drape medium plain | 1 |
| Drape C section | 1 |
| Light handle cover | 2 |
| Suction Yankauer | 1 |
| Needle counter box or pad | 1 |
| Maternity pad | 1 |
| Swab gauze small X-ray (5's) | 1 |
| Swab gauze large X-ray (5's) | 2 |
| Syringe 60ml catheter tip | 1 |
| Suction tubing | 2 |
| Adhesive dressing | 1 |
| Dressing pad | 1 |
| Placenta bowl | 1 |



| Description | Quantity |
|---|----------|
| Paper or SMS wrap | 1 |
| 1 Back table cover to wrap | 1 |
| 2 Back table cover book folded | 2 |
| 1 Mayo stand cover | 1 |
| 1 Instrument diathermy pouch | 1 |
| 2 Kidney bowl 700ml | 2 |
| 1 Blade 20 | 1 |
| 1 Blade 21 | 1 |
| 2 Blade 23 | 2 |
| 1 Bowl 500ml | 1 |
| 1 Bowl 1000ml | 1 |
| 2 Bowl 250ml | 2 |
| 1 Jug 1000ml | 1 |
| 1 Cautery diathermy pencil | 1 |
| 1 Cautery diathermy quiver | 1 |
| 1 Cautery diathermy tip cleaner | 1 |
| 1 Cautery diathermy blade | 1 |
| 3 Dressings adhesive | 3 |
| 2 Bandage crepe 15cm | 2 |
| 2 Bandage crepe 10cm | 2 |
| 5 Vessel loops various colours | 5 |
| 10 Suture boots | 10 |
| 2 Light handle cover | 2 |
| 1 Incise or ioban | 1 |
| 1 Drape cardiovascular | 1 |
| 1 Drape double split | 1 |
| 1 Drape foot covers pair | 1 |
| 1 Drape head / large with adhesive edge | 1 |
| 2 Drape medium plain | 2 |
| 4 Drape small plain utility | 4 |
| 1 Dressings adhesive | 1 |
| 1 Skin marker | 1 |
| 2 Suction Yankauer | 2 |
| 1 Handle suction frazier | 1 |
| 1 Suction tubing | 1 |
| 1 Needle counter box or pad | 1 |
| 2 Swab gauze small X-ray tied 5's | 2 |
| 2 Swab gauze large X-ray tied 5's | 2 |
| 1 Skin staples 35 wide | 1 |
| 2 Hand towel | 2 |
| 2 Steri strips wide | 2 |
| 2 Op tape | 2 |
| 1 Dressing pad | 1 |
| 2 Huck towels blue | 2 |







| Description | Quantity |
|---------------------------------|----------|
| Paper or SMS wrap | 1 |
| Back table cover to wrap | 1 |
| Kidney bowl 800ml | 1 |
| Blade 11 | 1 |
| Blade 15 | 1 |
| Drape legging | 2 |
| Bowl 1000ml | 1 |
| Mayo stand cover | 1 |
| Gallipot 120ml | 1 |
| Under buttock drape | 1 |
| Insufflation tubing | 1 |
| Veress needle | 1 |
| Fog free solution | 1 |
| Light handle cover | 2 |
| Suction Yankauer | 1 |
| Suction tubing | 1 |
| Needle counter box or pad | 1 |
| Maternity pad | 1 |
| Swab gauze small X-ray tied 5's | 2 |
| Hand towel | 1 |
| Velcro strip | 1 |
| Adhesive dressing | 2 |
| Drape w/ adhesive edge | 1 |
| Camera cover | 1 |




| Description | Quantity |
|-----------------------------------|----------|
| Paper or SMS wrap | 1 |
| 1 Back table cover to wrap | 1 |
| 1 Bowl 1000ml | 1 |
| 1 Gallipot 120ml | 1 |
| 1 Kidney bowl 800ml | 1 |
| 1 Jug 1000ml | 1 |
| 1 Drape TUR | 1 |
| 1 Irrigation tubing set | 1 |
| 2 Swab gauze small X-ray tied 5's | 2 |
| 2 Velcro strip | 2 |
| 1 Camera cover | 1 |
| 1 Suction tubing | 1 |
| 2 Hand towels | 2 |
| 1 Ellik bladder evacuator | 1 |



| Description | Quantity |
|------------------------------------|----------|
| Paper or SMS wrap | 1 |
| 1 Back table cover to wrap | 1 |
| 1 Back table cover book folded | 1 |
| 1 Mayo stand cover | 1 |
| 2 Kidney bowl 800ml | 2 |
| 2 Blade 23 | 2 |
| 1 Blade 20 | 1 |
| 1 Bandage crepe 15cm | 1 |
| 1 Bowl 500ml | 1 |
| 1 Bowl 1000ml | 1 |
| 1 Cautery pencil | 1 |
| 1 Cautery tip cleaner | 1 |
| 1 Cautery quiver | 1 |
| 2 Bowl 250ml | 2 |
| 1 Drape elliptical hip | 1 |
| 1 U drape | 1 |
| 1 Ioban | 1 |
| 2 Light handle cover | 2 |
| 1 Suction Yankauer | 1 |
| 1 Suction tubing | 1 |
| 1 Skin marker C/W ruler | 1 |
| 1 Needle counter box or pad | 1 |
| 1 Jug 1000ml | 1 |
| 1 Instrument diathermy pouch | 1 |
| 5 Swab gauze small X-ray tied 5's | 5 |
| 10 Swab gauze large X-ray tied 5's | 10 |
| 1 Stockinette (cotton/impervious) | 1 |
| 1 Syringe 60ml catheter tip | 1 |
| 1 Dressing adhesive | 1 |
| 1 Dressing pad | 1 |
| 1 Op tape | 1 |
| 1 Drape medium plain | 1 |

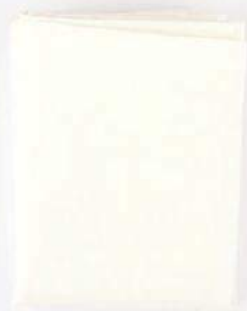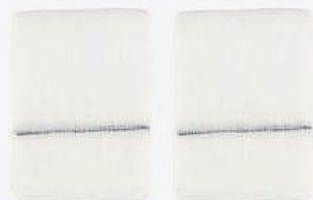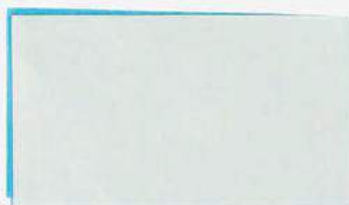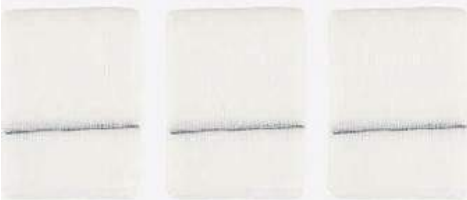

| Description | Quantity |
|---------------------------------|----------|
| Paper or SMS wrap | 1 |
| Back table cover to wrap | 1 |
| Kidney bowl 800ml | 1 |
| Blade 11 | 1 |
| Bandage crepe 15cm | 1 |
| Bowl 500ml | 1 |
| Bowl 250ml | 2 |
| Drape arthroscopy | 1 |
| Stockinette (cotton/impervious) | 1 |
| Skin marker | 1 |
| Needle counter box or pad | 1 |
| Needle white ivory 19g 5cm | 1 |
| Bandage ortho padding 15cm | 1 |
| Swab gauze small X-ray tied 5's | 5 |
| Syringe 20ml LS | 1 |
| Suction tubing | 1 |
| Op tape | 1 |
| Drape medium plain | 1 |
| Camera cover | 1 |

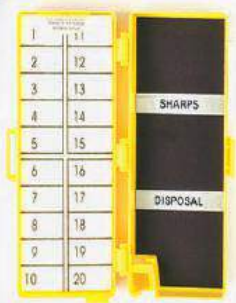

| Description | Quantity |
|-----------------------------------|----------|
| Back table cover to wrap | 1 |
| 1 Mayo stand cover | 1 |
| 1 Kidney bowl 700ml | 1 |
| 1 Bowl 500ml | 1 |
| 1 Gallipot 60ml | 1 |
| 1 Drape ophthalmic | 1 |
| 1 Eye spears (10 pack) | 1 |
| 1 Needle counter box or pad | 1 |
| 1 Needle orange 25G 5/8 inch | 1 |
| 1 Needle yellow 30G 1/2 inch | 1 |
| 1 Eye pad | 1 |
| 1 Eye shield clear | 1 |
| 2 Swab gauze small X-ray tied 5's | 2 |
| 1 Syringe 1ml LS | 1 |
| 1 Syringe 5ml LL | 1 |




Broche[®] *Gowns*





STERILE GOWNS

Disposable Sterile Ultrasonic Stitch Surgical Gown

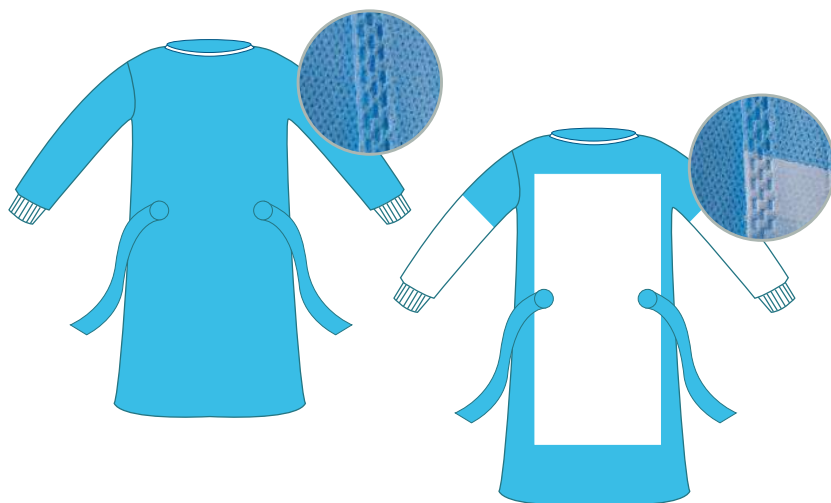

COLOR



BLUE

| DESCRIPTION | SIZE | CODE |
|---|--------|-----------------|
| SMS/SMMS STERILE ULTRASONIC STITCH STANDARD SURGICAL GOWN W/A TOWEL | L - XL | SGC001 - SGC002 |
| SMS/SMMS STERILE ULTRASONIC STITCH REINFORCED SURGICAL GOWN W/A TOWEL | L - XL | RG001 - RG002 |

GOWNS DETAILS


The surgical gowns are sterilized with ethylenoxide and are designed to cover the surgeon during surgical operations. The gowns are classified into two types according to the duration of the surgical operations and also according to the type of selected material - SMS/SMMS - and each of them may be equipped with liquid resistant lining. The elastic cuff on the sleeves are made from 95% cotton, 5% spandex.

- Water resistant
- Easy fit
- Comfortable design
- Air permeable
- Ultrasonic stitch

Gowns have the quality to allow respiration, and retain and repel alcohol, blood, water and any kind of body fluids without absorbing them. Gowns, which are produced with no-shred and non-woven SMS/SMMS fabric, do not let soaking up, thus, prevents infection spread, and provide a healthy and comfortable work environment for medical personnel.

NON-STERILE GOWNS

Disposable Non-Sterile Patient Gown

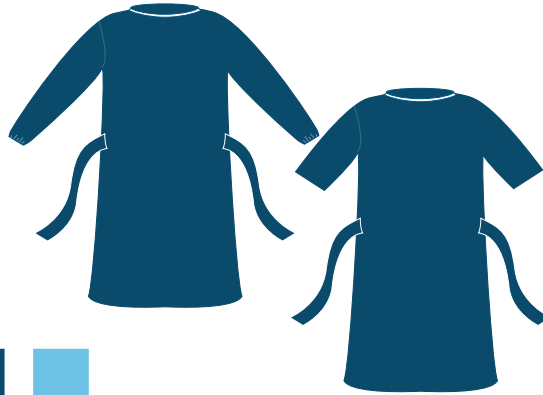

COLOR




NAVY



BLUE

| DESCRIPTION | SIZE | CODE |
|---|--------|-----------------|
| NON-STERILE PATIENT GOWN (LONG SLEEVE) | L - XL | PGL001 - PGL002 |
| NON-STERILE PATIENT GOWN (SHORT SLEEVE) | L - XL | PGS001 - PGS002 |

Disposable Non-Sterile Doctor Scrub Suits

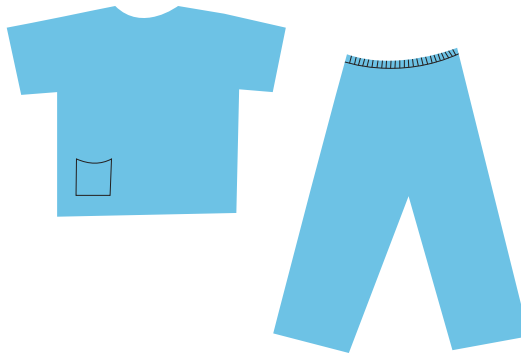

COLOR



BLUE

| DESCRIPTION | SIZE | CODE |
|---|--------|-----------------|
| NON-STERILE DISPOSABLE DOCTOR SCRUB SUITS | L - XL | DSS001 - DSS002 |



Broche[®] *Gloves*



STERILE GLOVES

Chloroprene Synthetic Sterile Surgical Gloves **NEO+PLUS**



DESCRIPTION

POWDER FREE
LATEX FREE, NON-ALLERGIC
BEADED CUFF
FOR SINGLE USE ONLY
50 PAIRS PER BOX
AQL 1,5
STERILE **R**

SIZE

6,5 - 7 - 7,5 - 8 - 8,5

COLOR



BROWN

STERILE GLOVES

Latex Sterile Surgical Gloves **+PLUS**



DESCRIPTION

POWDERED and POWDER FREE
BEADED CUFF
TEXTURED
WEIGHT REFERENCE SIZE 7,5: 16,8 gr/pair
FOR SINGLE USE ONLY
50 PAIRS PER BOX
AQL 1,5
STERILE **R**

SIZE

6,5 - 7 - 7,5 - 8 - 8,5

COLOR



NATURAL

NON-STERILE GLOVES

Latex Examination Gloves



DESCRIPTION

POWDERED

SMOOTH SURFACE

BEADED CUFF

AMBIDEXTROUS

FOR SINGLE USE ONLY

100 PCS PER BOX

SIZE

XS - S - M - L

COLOR



NATURAL



NON-STERILE GLOVES

Latex Examination Gloves



DESCRIPTION

POWDER FREE

TEXTURED

BEADED CUFF

AMBIDEXTROUS

FOR SINGLE USE ONLY

100 PCS PER BOX

SIZE

S - M - L

COLOR



NATURAL



NON-STERILE GLOVES

Vinyl Examination Gloves



DESCRIPTION

POWDERED

LATEX FREE

BEADED CUFF

AMBIDEXTROUS

FOR SINGLE USE ONLY

100 PCS PER BOX

AQL 1,5

SIZE

S - M - L

COLOR



CLEAR

NON-STERILE GLOVES

Vinyl Examination Gloves



DESCRIPTION

POWDER FREE

LATEX FREE

BEADED CUFF

AMBIDEXTROUS

FOR SINGLE USE ONLY

100 PCS PER BOX

AQL 1,5

SIZE

S - M - L

COLOR



CLEAR



LATEX LIKE



BLUE



NON-STERILE GLOVES

Nitrile Examination Gloves



DESCRIPTION

POWDER FREE
LATEX FREE, NON ALLERGIC
FINGER TEXTURED
BEADED CUFF
AMBIDEXTROUS
FOR SINGLE USE ONLY
100 PCS PER BOX
AQL 1,5

SIZE

S - M - L

COLOR



NON-STERILE GLOVES

Nitrile Chemotherapy Examination Gloves



DESCRIPTION

POWDER FREE
LATEX FREE, NON ALLERGIC
TESTED FOR USE WITH CHEMOTHERAPY DRUGS
4 MIL - 12" CUFF
FINGER TEXTURED
BEADED CUFF
AMBIDEXTROUS
FOR SINGLE USE ONLY
100 PCS PER BOX
AQL 1,5

SIZE

S - M - L

COLOR



BLUE



NON-STERILE GLOVES

PE Gloves



DESCRIPTION

FOR SINGLE USE ONLY

WEIGHT 7 KG / 10.000 pcs

100 PCS PER BAG

SIZE

L

COLOR



CLEAR

Broche[®] *Plastic Products*



PLASTIC PRODUCTS

Sterile Flowmeter



| DESCRIPTION | DESCRIPTION |
|---|---------------------|
| MATERIAL: MEDICAL GRADE POLY VINYL CHLORIDE | LUER LOCK |
| DROPPING VARIATION 5 TO 250 ML/h | FOR SINGLE USE ONLY |
| LATEX FREE | INDIVIDUAL PACKING |
| Y INJECTION PORT | EO STERILE |

Sterile Infusion (Serum) Set



| DESCRIPTION | DESCRIPTION |
|---|-------------------------------|
| MATERIAL: MEDICAL GRADE POLY VINYL CHLORIDE | WITH AIR VENT |
| WITH DRIP CHAMBER | FOR SINGLE USE ONLY |
| APPROPRIATE FOR INFUSION BOTTLES AND ALSO FOR INFUSION BAGS | INDIVIDUALLY PACKED IN PE BAG |
| FILTER IN DRIP CHAMBER | EO STERILE |
| WITH A FLOW REGULATOR | |

PLASTIC PRODUCTS

Sterile Urine Bag / T-Valve and Push & Pull Valve



DESCRIPTION

MATERIAL: MEDICAL GRADE PVC

2000 ML COLLECTING CAPACITY

WITH ANTI-REFLUX VALVE

REINFORCED HOLES FOR HANGING

LATEX FREE

FOR SINGLE USE ONLY

INDIVIDUALLY PACKED IN PE BAG

EO STERILE

PLASTIC PRODUCTS

Sterile Blood Transfusion Set



DESCRIPTION

MATERIAL: MEDICAL GRADE POLY VINYL CHLORIDE

WITH FLOW REGULATOR

WITH BLOOD FILTER

NON TOXIC and NON PYROGENIC

18 G HYPODERMIC NEEDLE

WITH AIR VENT

FOR SINGLE USE ONLY

INDIVIDUALLY PACKED IN PE BAG

EO STERILE

Broche[®] *Medical Disposables*



MEDICAL DISPOSABLES

Sterile Surgical Blades



DESCRIPTION

MATERIAL: CARBON STEEL

NO: 10 - 11 - 12 - 15 - 18 - 20 - 21 - 22 - 23 - 24 - 25

FOR SINGLE USE ONLY

100 PCS PER BOX

STERILE 



MEDICAL DISPOSABLES

Sterile Blood Lancet



DESCRIPTION

MATERIAL: CARBON STEEL

DISPOSABLE

FOR SINGLE USE ONLY


200 Pcs PER BOX

STERILE **R**



MEDICAL DISPOSABLES

Sterile / Non-Sterile Wooden Tongue Depressor

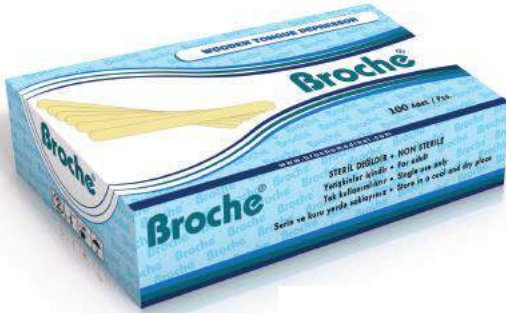

| DESCRIPTION | SIZE |
|--------------------------------|--------------------|
| MATERIAL: BIRCH TREE | ADULT 150mm X 18mm |
| SMOOTH SURFACE WITH ROUND ENDS | |
| FOR SINGLE USE ONLY | |
| 100 PCS PER BOX | |

MEDICAL DISPOSABLES

Shoe Covers



DESCRIPTION

MATERIAL: POLYETHYLENE
FOR SINGLE USE ONLY
100 PCS PER PACKET

COLOR



BLUE



MEDICAL DISPOSABLES

Face Mask



DESCRIPTION

MATERIAL: NONWOVEN POLYPROPYLENE SPUNBONDED FABRIC

2 PLY AND 3 PLY

ULTRASONIC STITCH

WITH ROUND ELASTIC EARLOOP OR WITH POLYPROPYLENE TIE

NOSE SUPPORT

FOR SINGLE USE ONLY

50 PCS PER BOX

COLOR



GREEN



WHITE



MEDICAL DISPOSABLES

Soft Bar Cap



| DESCRIPTION | SIZE |
|--|---------|
| MATERIAL: NONWOVEN POLYPROPYLENE SPUNBONDED FABRIC | 21 INCH |
| ULTRASONIC STITCH | |
| DOUBLE ELASTIC | |
| FOR SINGLE USE ONLY | |
| 100 PCS PE BAG | |

COLOR



GREEN



WHITE

SZUTEST

EC CERTIFICATE AT SERTİFİKA

According to Annex II of the Directive 93/42/EEC on Medical Devices

93/42/AT Tıbbi Cihaz Yönetmeliği Ek II'ye göre

Full Quality Assurance System
Tam Kalite Güvencesi

Certificate Number: 2195-MED-1412002
Sertifika Numarası

Manufacturer:
Üretici

Nurteks Tekstil ve Medikal Sanayi Dış Ticaret Anonim Şirketi
Head Office Köşklü Çeşme Mah. Yeni Bağdat Cad. No:124 Gebze / Kocaeli
/Merkez: Türkiye
Branch Office Oruç Reis Mah. Tekstilkent Cad. Tekstilkent Sitesi B Blok
/Şube: No:12A Kapı No:031 ve 034 Esenler / İstanbul Türkiye

Product(s):
Ürün(ler)

Sterile Disposable Surgical Drape, Gown and Drape Sets
Steril Tek Kullanımlık Cerrahi Örtü, Önlük ve Örtü Setleri

Reference Report No: MM0403-P005-R01, MM0403-P005-R02
Referans Rapor No

Szutest, Notified Body 2195, declares that the aforementioned manufacturer has implemented a quality assurance system according to Annex II (excluding section 4), Section 3 of the directive 93/42/EEC on medical devices. This quality assurance system covers those aspects of manufacturing concerned with securing and maintaining safe conditions of the respective product(s) and conforms to the provisions of this Directive. The approved quality system is subject to surveillance pursuant to Annex II, Section 5 of Directive 93/42/EEC and unannounced audits.

Szutest must be informed of any significant changes in the design and/or construction of the product(s).

2195 kimlik numaralı Onaylanmış Kuruluş Szutest, yukarıda belirtilen üreticinin 93/42/AT Tıbbi Cihaz Yönetmeliği EK II(madde 4 hariç) madde 3'üne göre bir kalite yönetim sistemi uyguladığını, bu yönetim sisteminin yönetmeliğin sadece bahsi geçen ürünün üretiminin güvenlik koşullarını sağlama ve devam ettirme ile ilgili gerekliliklerin karşıladığını beyan eder. Onaylanan bu kalite yönetim sistemi, 93/42/AT Tıbbi Cihaz Yönetmeliği EK II, Madde 5'e göre periyodik olarak gözetime ve habersiz saha denetimlerine tabidir. Üretici, ürünlerinin tasarımında ve yapısında gerçekleştirdiği önemli değişiklikleri Szutest'e bildirmek zorundadır.

This EC certificate is valid till 2024-04-28.
Bu AT Sertifikası 2024-04-28 tarihine kadar geçerlidir.

Issue Date/Yayın Tarihi: 2014-04-30
Revision No./ Revizyon No.: 04 Recertification/Yeniden Belgelendirme
Revision Date/ Revizyon Tarihi: 2019-04-29

Rukiye BALKAN
Deputy General Manager
Genel Müdür Yardımcısı

SZUTEST UYGUNLUK DEĞERLENDİRME A.Ş.

Tatlısu Mahallesi, Akif İnan Sk. No:1 Ümraniye 34774 İSTANBUL / TÜRKİYE

FR.MED.34 R.04

Szutest.com.tr

Broche®



TÜRK STANDARDLARI ENSTİTÜSÜ
TÜRK STANDARDLARINA UYGUNLUK BELGESİ
TURKISH STANDARDS INSTITUTION
CERTIFICATE OF CONFORMITY TO TURKISH STANDARDS



| | |
|---|---|
| BELGE NUMARASI REFERENCE NUMBER OF LICENCE | 071851-TSE-01/02 |
| BELGENİN İLK VERİLİŞ TARİHİ DATE OF FIRST ISSUE OF LICENCE | 15.04.2014 |
| BELGENİN SON GEÇERLİLİK TARİHİ LICENCE VALID UNTIL | 26.02.2020 |
| BELGE SAHİBİ KURULUŞUN ADI NAME OF THE LICENCE HOLDER | NURTEKS TEKSTİL VE MEDİKAL SANAYİ DİŞ TİCARET ANONİM ŞİRKETİ |
| BELGE SAHİBİ KURULUŞUN ADRESİ ADDRESS OF THE LICENCE HOLDER | KÖŞKLÜ ÇEŞME MAH. YENİ BAĞDAT CAD. NO:124 GEBZE KOCAELİ/TÜRKİYE |
| ÜRETİM YERİ ADI NAME OF THE MANUFACTURING PLACE | NURTEKS TEKSTİL VE MEDİKAL SANAYİ DİŞ TİCARET ANONİM ŞİRKETİ |
| ÜRETİM YERİ ADRESİ ADDRESS OF THE MANUFACTURING PLACE | KÖŞKLÜÇEŞME MAHALLESİ YENİ BAĞDAT CADDESİ NO : 124 GEBZE / KOCAELİ KOCAELİ / TÜRKİYE |
| İPTAL EDİLEN BELGE NUMARASI (Varsa) INDICATION OF SUPERSEDED LICENCE (if any) | 071851-TSE-01/01 |
| TESCİLLİ TİCARİ MARKASI REGISTERED TRADE MARK | BROCHE |
| İLGİLİ TÜRK STANDARDI RELATED TURKISH STANDARD | TS EN 13795+A1 / 12.06.2013 |
| BELGE KAPSAMI SCOPE OF LICENCE | SURGICAL DRAPES USED AS MEDICAL DEVICES FOR PATIENTS, CLINICAL STAFF AND EQUIPMENT -HIGH PERFORMANCE, SINGLE USE |

03.05.2019

On Behalf Of The Head Of Certification Center
AHMET NURSI KARTAL
MANAGER OF THE TSE İSTANBUL CERTIFICATION
DEPT.

*Bu belge, belgelenen ürünün, üretim yerinin Enstitümüzün bellediği şartları karşıladığını da gösterir.

*Bu belge ile bir sunu ile edilemez, kopya veya okunması zorlaştırılacak şekilde değiştirilemez, kopya ve satışı yapılamaz.

*TSE (İSTANBUL) BELGELENDİRME MÜDÜRLÜĞÜ - Adres: Çarşıoğlu Teneke İşhanı Yaka ÇARŞIYANCAZİTESİ - Tel: 3827231273 Faks: 3827231906

*TSE BELGELENDİRME MERKEZİ BAŞKANLIĞI Adres: Necatibey Cad. No:112 06100 BakanlıkANKARA - Tel: 0 312 416 84 81 / 416 84 27, Faks: 0 312 416 66 17

e-posta : tse@tse.org.tr , web : www.tse.org.tr

<https://evrakkontrol.tse.org.tr/BelgeDogrulama.aspx?pepiewrtdk> adresinden belgenin doğruluğunu ve geçerliliğini sorgulayınız.



1 / 1



CERTIFICATE

This certificate is granted to the organization,

NURTEKS TEKSTİL VE MEDİKAL SANAYİ DİŞ TİCARET ANONİM ŞİRKETİ

Köşklüçeşme Mahallesi Yeni Bağdat Caddesi No:124 Gebze / Kocaeli / Türkiye

PRODUCTION OF DISPOSABLE; STERILE SURGICAL GOWNS AND DRAPES, NONSTERILE GOWNS AND DRAPES
SALE OF DISPOSABLE STERILE PRODUCTS; (SURGICAL GLOVES, WOODEN TONGUE DEPRESSOR, SURGICAL
BLADES, FLOWMETER, INFUSION (SERUM) SET, URINE BAG, BLOOD TRANSFUSION SET, BLOOD LANCET)
SALE OF DISPOSABLE NONSTERILE PRODUCTS; (EXAMINATION GLOVES, PE GLOVES, MASK, CAPS, SHOE COVER,
WOODEN TONGUE DEPRESSOR, UNDERPADS, GOWNS AND DRAPES, NON-WOVEN PP FABRICS)

EA 14, 29

according to the scope,

ISO 9001:2015

to certify that Quality Management System in accordance with standard's clauses
is established and being implemented.

First Date of Issue : 03.04.2018
Date of Issue : 02.04.2019
Certificate Period : 3 Years
Reissue Due Date : 02.04.2020
Certificate No : 01.18.7249.112692.D

First Quality Certification
System Certificate Approved
Maltepe / İstanbul / Türkiye



FQC, India & Head Office
FQC First Quality Certification Pvt. Ltd.
909/37, Sector-12, Phase-IV - 134109, Faridkot, India
T: +91 172 6535875 / F: +91 172 4418931
www.fqc.com info@fqc.com

FQC, Turkey & Critical Location
FQC Uluslararası Belgelendirme ve Eğitim Hiz. A.Ş.
Hünkarı Cad. Private İş Merkezi No:10 Kat:Zemin Kat, Maltepe, İstanbul, Türkiye
T: +90 216 457 69 06 / F: +90 216 457 96 69
www.fqc.com.tr info@fqc.com.tr

Bu belge, müşterinin FQC'nin kuralına ve sözleşme şartlarına uyduğu sürece geçerlidir. Sertifika geçerlilik durumunu FQC'nin internet sitesinden takip edilebilir.
This document shall remain valid as long as the customer obeys FQC rules and terms of the contract. Certificate validity may be checked on FQC website.

CERTIFICATE of Registration



*This is to Certify that the
Medical Devices – Quality Management System
of*

NURTEKS TEKSTİL VE MEDİKAL SANAYİ DIŞ TİCARET A.Ş.

KÖŞKLÜ ÇEŞME MAH. YENİ BAĞDAT CAD. NO:124 GEBZE / KOCAELİ / TURKEY

**has been independently assessed and is compliant
with the requirements of**

ISO 13485:2016

This Certificate is applicable to the following product or service ranges:

PRODUCTION AND SALES OF DISPOSABLE PRODUCTS; STERILE SURGICAL GOWNS AND DRAPES, NONSTERILE GOWNS AND DRAPES, NONWOVEN FABRICS, NON-KNITTED FABRICS AND APPLICATIONS SALE OF DISPOSABLE STERILE PRODUCTS; (SURGICAL GLOVES, WOODEN TONGUE DEPRESSOR, SURGICAL BLADES, FLOWMETER, INFUSION (SERUM) SET, URINE BAG, BLOOD TRANSFUSION SET, BLOOD LANCET)
SALE OF DISPOSABLE NONSTERILE PRODUCTS; (EXAMINATION GLOVES, PE GLOVES, MASK, CAPS, SHOE COVER, WOODEN TONGUE DEPRESSOR, UNDERPADS, GOWNS AND DRAPES, NON-WOVEN PP FABRICS)
ÜRETİMİ VE SATIŞI YAPILAN TEK KULLANIMLIK ÜRÜNLER; STERİL CERRAHİ ÖNLÜKLER VE ÖRTÜLER, NONSTERİL ÖNLÜKLER VE ÖRTÜLER, DOKUNMAMIŞ KUMAŞLAR, ÖRÜLMEMİŞ KUMAŞLAR VE APLİKASYONLAR
SATIŞI YAPILAN TEK KULLANIMLIK STERİL ÜRÜNLER (CERRAHİ EL DİVENLER, TAHTA DİL BASAĞI, BİSTURİ UCU, DAMLA AYAR SETİ, SERUM SETİ, İDRAR TORBAS, KAN VERME SETİ, KAN LANSETİ)
SATIŞI YAPILAN TEK KULLANIMLIK NONSTERİL ÜRÜNLER (MUAYENE EL DİVENLERİ, PE EL DİVEN, MASKELER, BONELER, GALOŞLAR, TAHTA DİL BASAĞI, YATAK KORUYUCU ÖRTÜLER, ÖNLÜKLER VE DOKUNMAMIŞ PP KUMAŞLAR)

Certificate No.: TR51235H

| | |
|--|-------------------|
| Date of initial registration | 06 September 2019 |
| Date of this Certificate | 06 September 2019 |
| Surveillance audit on or before | 05 September 2020 |
| Recertification Due / Certificate expiry | 05 September 2022 |

This Certificate is property of Staunchly Management & System Services Pvt. Ltd. and remains valid subject to satisfactory surveillance audits.



Director

STAUNCHLY MANAGEMENT & SYSTEM SERVICES LTD.

Suite 48, 88-90 Hutton Garden, London, EC1N 8PN.

Phone : +44 345 680 0199

Email : info@staunchlyservices.com Web : www.staunchlyservices.com

SM5/F109A/17/REV52

For precise and updated information concerning the present certificate mail to info@staunchlyservices.com
This Certificate is the property of Staunchly Management & System Services Private Limited and shall be returned immediately when demanded

Broche®

Turgut Reis Mahallesi, Tekstilkent
Koza Plaza B Blok Kat. 3 No. 11
Esenler - İSTANBUL / TÜRKİYE

T: +90.212 438 02 42 Pbx
F: +90.212 438 02 48

info@brochemedical.com
www.brochemedical.com