

Letter of Authorization

To whom it may concern,

We, **Getein Biotech, Inc.** (No.9 Bofu Road, Luhe District, Nanjing, 211505, China), hereby authorize Sanmedico SRL (Address: Republic of Moldova, Chisinau, MD-2059, Petricani street, 88/1, office 10) as our official and non-exclusive distributor for registration, promoting, selling, distributing and providing after-sale services of under-mentioned product in the territory of Moldova only:

FIA8000 Quantitative Immunoassay Analyzer and Reagents

Getein1100 Immunofluorescence Quantitative Analyzer and Reagents

Getein1160 Immunofluorescence Quantitative Analyzer and Reagents

Getein 1600 Immunofluorescence Quantitative Analyzer and Reagents

Sanmedico SRL will comply with the laws and regulations of the countries and regions where they are located in and where they are selling mentioned product.

Sanmedico SRL will carry out marketing efforts to fulfill service and maintenance for above mentioned products and will provide with users benefits of having a local stock of above mentioned products and on-time delivery with every order, supported by a local service in local language.

This authorization starts from **1st Jan, 2024** and will be valid to **31th, December, 2024** .

Getein Biotech, Inc. has the right to terminate the authorization before validity and will inform Sanmedico SRL with 10 days in advance.


基蛋生物科技股份有限公司
Getein Biotech, Inc.
GETEIN BIOTECH, INC.
Seal & Signature

Authority Person Name: **Steven Zhou**

Authority Person Position: **Regional Manager**

Date: **2023.12.13**

Certificate of Registration

QUALITY MANAGEMENT SYSTEM - ISO 13485:2016

This is to certify that: **Getein Biotech, Inc.**
No.9 Bofu Road
Luhe District
Nanjing
Jiangsu
211505
China

基蛋生物科技股份有限公司
中国
江苏省
南京市
六合区
沿江工业开发区
博富路9号
邮编: 211505

Holds Certificate No: **MD 728432**

and operates a Quality Management System which complies with the requirements of ISO 13485:2016 for the following scope:

Please see scope page.

For and on behalf of BSI:

Graeme Tunbridge, Senior Vice President Medical Devices

Original Registration Date: 2020-05-29

Latest Revision Date: 2023-04-26

Effective Date: 2023-07-26

Expiry Date: 2026-07-25



Certificate No: **MD 728432**

Registered Scope:

Design & Development, Manufacture and Distribution of Chemiluminescence Immunoassay, Biochemistry Assay, Point of Care Assay (including Colloidal Gold Assay, Immunofluorescence Assay, Dry Chemistry Assay), PCR Assay and Colloidal Gold self-testing Assay to detect infectious disease. Design & Development, Manufacture and Distribution of Analyzers in use of Chemiluminescence Immunoassay, Biochemistry Assay, Point of Care Assay (including Colloidal Gold Assay, Immunofluorescence Assay, Dry Chemistry Assay), PCR Assay to detect infectious disease, Immunofluorescence self-testing Assay to detect dyslipidemia disease, Blood Coagulation Assay to detect thrombotic disease.

研发, 生产和销售化学发光法试剂, 生化试剂, 即时诊断 (包括胶体金法, 免疫荧光法, 干式化学法) 试剂, 传染病相关PCR分子诊断试剂和胶体金自测试剂。 研发, 生产和销售用于化学发光法试剂, 生化试剂, 即时诊断 (包括胶体金法, 免疫荧光法, 干式化学法) 试剂, 传染病相关PCR分子诊断试剂, 血脂异常疾病相关免疫荧光自测试剂, 血栓疾病相关血凝试剂配套使用的分析仪。



Original Registration Date: 2020-05-29

Latest Revision Date: 2023-04-26

Effective Date: 2023-07-26

Expiry Date: 2026-07-25

Page: 2 of 3

This certificate was issued electronically and remains the property of BSI and is bound by the conditions of contract.

An electronic certificate can be authenticated [online](#).

Printed copies can be validated at www.bsi-global.com/ClientDirectory or telephone +86 10 8507 3000.

Information and Contact: BSI, John M. Keynesplein 9, 1066 EP Amsterdam The Netherlands. Tel: +31 (0) 20 3460 780

BSI Group The Netherlands B.V., registered in the Netherlands under number 33264284, at John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands

A Member of the BSI Group of Companies.

Certificate No: **MD 728432**

Location

Getein Biotech, Inc.
No.9 Bofu Road
Luhe District
Nanjing
Jiangsu
211505
China
基蛋生物科技股份有限公司
中国
江苏省
南京市
六合区
沿江工业开发区
博富路9号
邮编: 211505

Registered Activities

Design & Development, Manufacture and Distribution of Chemiluminescence Immunoassay, Biochemistry Assay, Point of Care Assay (including Colloidal Gold Assay, Immunofluorescence Assay, Dry Chemistry Assay), PCR Assay and Colloidal Gold self-testing Assay to detect infectious disease. Design & Development, Manufacture and Distribution of Analyzers in use of Chemiluminescence Immunoassay, Biochemistry Assay, Point of Care Assay (including Colloidal Gold Assay, Immunofluorescence Assay, Dry Chemistry Assay), PCR Assay to detect infectious disease, Immunofluorescence self-testing Assay to detect dyslipidemia disease, Blood Coagulation Assay to detect thrombotic disease.
研发, 生产和销售化学发光法试剂, 生化试剂, 即时诊断 (包括胶体金法, 免疫荧光法, 干式化学法) 试剂, 传染病相关PCR分子诊断试剂和胶体金自测试剂。 研发, 生产和销售用于化学发光法试剂, 生化试剂, 即时诊断 (包括胶体金法, 免疫荧光法, 干式化学法) 试剂, 传染病相关PCR分子诊断试剂, 血脂异常疾病相关免疫荧光自测试剂, 血栓疾病相关血凝试剂配套使用的分析仪。

Getein Biotech, Inc.
No. 6 KeFeng Road
Jiangbei New District
Nanjing
Jiangsu
211505
China
基蛋生物科技股份有限公司
中国
江苏省
南京
江北新区
科丰路6号
邮编: 211505

Manufacture of Chemiluminescence Immunoassay, Biochemistry Assay, Point of Care Assay (including Colloidal Gold Assay, Immunofluorescence Assay, Dry Chemistry Assay), Colloidal Gold self-testing Assay to detect infectious disease. Manufacture of Analyzers in use of Chemiluminescence Immunoassay, Biochemistry Assay, Point of Care Assay (including Colloidal Gold Assay, Immunofluorescence Assay, Dry Chemistry Assay), PCR Assay to detect infectious disease, Immunofluorescence self-testing Assay to detect dyslipidemia disease, Blood Coagulation Assay to detect thrombotic disease.
生产化学发光法试剂, 生化试剂, 即时诊断 (包括胶体金法, 免疫荧光法, 干式化学法) 试剂和传染病相关胶体金自测试剂。 生产用于化学发光法试剂, 生化试剂, 即时诊断 (包括胶体金法, 免疫荧光法, 干式化学法) 试剂, 传染病相关PCR分子诊断试剂, 血脂异常疾病相关免疫荧光自测试剂, 血栓疾病相关血凝试剂配套使用的分析仪。

Original Registration Date: 2020-05-29

Effective Date: 2023-07-26

Latest Revision Date: 2023-04-26

Expiry Date: 2026-07-25

Page: 3 of 3

This certificate was issued electronically and remains the property of BSI and is bound by the conditions of contract.

An electronic certificate can be authenticated [online](#).

Printed copies can be validated at www.bsi-global.com/ClientDirectory or telephone +86 10 8507 3000.

Information and Contact: BSI, John M. Keynesplein 9, 1066 EP Amsterdam The Netherlands. Tel: +31 (0) 20 3460 780

BSI Group The Netherlands B.V., registered in the Netherlands under number 33264284, at John M. Keynesplein 9, 1066 EP Amsterdam, The Netherlands

A Member of the BSI Group of Companies.

EC Declaration of Conformity

according to Directive 98/79/EC, on in vitro diagnostic medical devices

Ref. No.:20220513-A05

Manufacturer
(Name, Address)


Getein Biotech, Inc.
No. 9 Bofu Road, Luhe District, Nanjing, 211505, China

Authorized Representative
(Name, Address)

CMC Medical Devices & Drugs S.L.
Add: C/ Horacio Lengo N° 18, CP 29006, Málaga, Spain

Medical device

No.	Product Name
1	Getein 1100 Immunofluorescence Quantitative Analyzer
2	Cardiac Troponin I Fast Test Kit (Immunofluorescence Assay)
3	NT-proBNP Fast Test Kit (Immunofluorescence Assay)
4	hs-CRP+CRP Fast Test Kit (Immunofluorescence Assay)
5	NT-proBNP/cTnI Fast Test Kit (Immunofluorescence Assay)
6	CK-MB/cTnI/Myo Fast Test Kit (Immunofluorescence Assay)
7	D-Dimer Fast Test Kit (Immunofluorescence Assay)
8	PCT Fast Test Kit (Immunofluorescence Assay)
9	CysC Fast Test Kit (Immunofluorescence Assay)
10	mAlb Fast Test Kit (Immunofluorescence Assay)
11	NGAL Fast Test Kit (Immunofluorescence Assay)
12	β 2-MG Fast Test Kit (Immunofluorescence Assay)
13	CK-MB/cTnI Fast Test Kit (Immunofluorescence Assay)
14	HCG+ β Fast Test Kit (Immunofluorescence Assay)
15	H-FABP Fast Test Kit (Immunofluorescence Assay)
16	PCT/CRP Fast Test Kit (Immunofluorescence Assay)
17	CK-MB/cTnI/H-FABP Fast Test Kit (Immunofluorescence Assay)
18	HbA1c Fast Test Kit (Immunofluorescence Assay)
19	NT-proBNP/NGAL Fast Test Kit (Immunofluorescence Assay)
20	CK-MB Fast Test Kit (Immunofluorescence Assay)
21	hs-cTnI Fast Test Kit (Immunofluorescence Assay)
22	T3 Fast Test Kit (Immunofluorescence Assay)
23	T4 Fast Test Kit (Immunofluorescence Assay)
24	TSH Fast Test Kit (Immunofluorescence Assay)
25	Scr Fast Test Kit (Immunofluorescence Assay)
26	PLGF Fast Test Kit (Immunofluorescence Assay)



- 27 HCY Fast Test Kit (Immunofluorescence Assay)
- 28 Anti-CCP Fast Test Kit (Immunofluorescence Assay)
- 29 25-OH-VD Fast Test Kit (Immunofluorescence Assay)
- 30 Lp-PLA2 Fast Test Kit (Immunofluorescence Assay)
- 31 FOB Fast Test Kit (Immunofluorescence Assay)
- 32 SAA Fast Test Kit (Immunofluorescence Assay)
- 33 H. pylori Fast Test Kit (Immunofluorescence Assay)
- 34 PRL Fast Test Kit (Immunofluorescence Assay)
- 35 Transferrin Fast Test Kit (Immunofluorescence Assay)
- 36 Insulin Fast Test Kit (Immunofluorescence Assay)
- 37 PG I /PG II Fast Test Kit (Immunofluorescence Assay)
- 38 LH Fast Test Kit (Immunofluorescence Assay)
- 39 FSH Fast Test Kit (Immunofluorescence Assay)
- 40 Anti-TP Fast Test Kit (Immunofluorescence Assay)
- 41 AFP/CEA Fast Test Kit (Immunofluorescence Assay)
- 42 AMH Fast Test Kit (Immunofluorescence Assay)
- 43 fT3 Fast Test Kit (Immunofluorescence Assay)
- 44 fT4 Fast Test Kit (Immunofluorescence Assay)
- 45 Total IgE Fast Test Kit (Immunofluorescence Assay)
- 46 Vit-B12 Fast Test Kit (Immunofluorescence Assay)
- 47 Prog Fast Test Kit (Immunofluorescence Assay)
- 48 Testosterone Fast Test Kit (Immunofluorescence Assay)
- 49 E2 Fast Test Kit (Immunofluorescence Assay)
- 50 RF Fast Test Kit (Immunofluorescence Assay)
- 51 ASO Fast Test Kit (Immunofluorescence Assay)
- 52 Ferritin Fast Test Kit (Immunofluorescence Assay)
- 53 ST2 Fast Test Kit (Immunofluorescence Assay)
- 54 CA125 Fast Test Kit (Immunofluorescence Assay)
- 55 CA19-9 Fast Test Kit (Immunofluorescence Assay)
- 56 CA15-3 Fast Test Kit (Immunofluorescence Assay)
- 57 RSV/Influenza A/B Fast Test Kit (Immunofluorescence Assay)
- 58 Influenza A/B Fast Test Kit (Immunofluorescence Assay)
- 59 RSV Fast Test Kit (Immunofluorescence Assay)
- 60 IL-6 Fast Test Kit (Immunofluorescence Assay)
- 61 BNP Fast Test Kit (Immunofluorescence Assay)
- 62 SAA/CRP Fast Test Kit (Immunofluorescence Assay)
- 63 Folate acid Fast Test Kit (Immunofluorescence Assay)
- 64 hs-CRP Fast Test Kit (Immunofluorescence Assay)
- 65 TnT Fast Test Kit (Immunofluorescence Assay)
- 66 PCT/IL-6 Fast Test Kit (Immunofluorescence Assay)



- 67 HBP Fast Test Kit (Immunofluorescence Assay)
- 68 S100-β Fast Test Kit (Immunofluorescence Assay)
- 69 CK-MB/hs-cTnI/Myo Fast Test Kit (Immunofluorescence Assay)
- 70 Cortisol Fast Test Kit (Immunofluorescence Assay)
- 71 CEA Fast Test Kit (Immunofluorescence Assay)
- 72 AFP/CEA Fast Test Kit (Immunofluorescence Assay)

Classification Other device (according to Annex II of the directive 98/79/EC)

Conformity assessment route Annex III of the 98/79/EC

Applicable coordination standards	EN 13612:2002	EN ISO 14971:2019	EN ISO15223-1:2016
	EN ISO 18113-1:2011	EN ISO 18113-2:2011	EN ISO 18113-3:2011
	EN ISO 23640:2015	EN ISO 13485:2016	ISO 780:2015
	EN 61326-2-6:2006	IEC 61326-1:2013	
	EN 61010-2-101:2002	IEC 61010-1:2010	

Signatory representative declares herein the above-mentioned device meets the basic requirements of the European Parliament and the Council's in vitro diagnostic medical devices directive: 98/79/EC Annex I.

This declaration of conformity is based on European Parliament and the Council's 98/79/EC directive Annex III. The compiled technical file and quality system document according to 98/79/EC directive Annex III are testified and the quality system certificate has issued by BSI Group The Netherlands B. V. The manufacturer is exclusively responsible for the declaration of conformity.

General Manager Enben Su

Nanjing
13th, May, 2022
 (place and date of issue)

 (name and signature or equivalent marking of authorized person)





CERTIFICATE

Getein Biotech

hereby certifies

Mr. Vitalie Goreacii

from Sanmedico SRL.

Completion of Getein Products Technical and Operational Training
& Qualification of After-sales Service

基蛋生物科技股份有限公司
GETEIN BIOTECH, INC.



Cardiac
Markers

Coagulation
Markers

Diabetes
Mellitus

Inflammation

Thyroid
Function

Metabolic
Marker

Renal
Function

Tumor
Markers

Reproduction
/Fertility

Infectious
Disease



OPTIMIZED POINT-OF-CARE SOLUTION

MAKING TEST EASY

Getein 1100

Immunofluorescence Quantitative Analyzer



Getein 1100

Immunofluorescence Quantitative Analyzer



HIGHLY EFFICIENT & ACCURATE

Advanced fluorescence immunoassay

Multiple quality control



REAL-TIME AND RAPID TEST


One-step test

3-15 min/test


5 sec/test for multiple tests

OPERATION MODES

Inside Mode (Single sample rapid test mode)



Sample Transfer



Test Card Insert



Click "Start" Icon




Result Show and Print


Outside Mode (Mass samples rapid test mode)



Sample Transfer



Timing the Reaction Manually

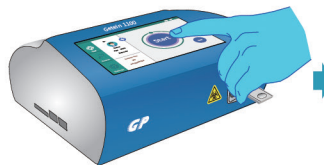

Click "Start" Icon



Result Show and Print



CONVENIENT OPERATION

RFID card calibration

Keyboard and mouse connectivity through USB port

Handwriting input available


Continuous test for 3 hours with optional lithium battery



USER-FRIENDLY INTERFACE

Android system

7-inch touch screen

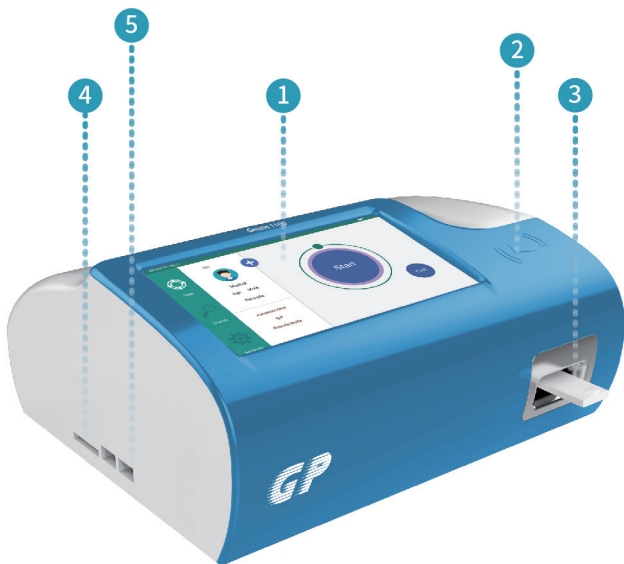

1 7-inch Touch Screen

2 SD Card Recognition Zone

3 Test Card Slot

4 SD Card Slot

5 USB Slot

6 Built-in Thermal Printer



PORTABLE DESIGN

Small in size: 261*241*115 mm

Light in weight: 2.0 kg



LARGE MEMORY

Up to 10,000 results storage capacity

TECHNICAL PARAMETERS

Methodology	Immunofluorescence	Screen	7-inch touch screen
Result	Quantitative	Power Supply	100-240 V ~ 50 Hz/60 Hz, 60 VA
Sample Type	WB, Plasma, Serum, Urine, Stool, Nasal swab, Saliva, Capillary blood	Working Environment	Temperature: 10-35°C Relative humidity ≤ 70% Air pressure 70.0 ~ 106.0 kpa
Storage Capacity	10,000 data	Dimensions	261 mm*241 mm*115 mm (D*W*H)
Language	English/Chinese/Spanish/Portuguese	Weight	2.0 kg

TEST ITEMS

Cat. #	TEST ITEMS	DISEASES	CUT-OFF VALUE	SAMPLE TYPES	MEASURING RANGE	SAMPLE VOLUME	REACTION TIME	QUALIFICATION
Cardiac Markers								
IF1001	cTnI	Myocardial infarction	0.10 ng/mL	S/P/WB	0.10-50.00 ng/mL	100 µL	10 min	NMPA CE
IF1098	TnT	Myocardial infarction	14.0 pg/mL	S/P/WB	10.0-10000.0 pg/mL	100 µL	15 min	NMPA CE
IF1089	BNP	Heart failure	100.0 pg/mL	P/WB	5.0-5000.0 pg/mL	100 µL	10 min	NMPA CE
IF1002	NT-proBNP	Heart failure	300 pg/mL	S/P/WB	100-35000 pg/mL	100 µL	10 min	NMPA CE
IF1004	NT-proBNP/cTnI	Heart failure/acute myocardial infarction/acute coronary syndrome	NT-proBNP: 185 pg/mL cTnI: 0.10 ng/mL	S/P/WB	100-15000 pg/mL 0.10-50.00 ng/mL	100 µL	10 min	NMPA CE
IF1005	CK-MB/cTnI/Myo	Myocardial damage /infarction	CK-MB: 5.00 ng/mL cTnI: 0.10 ng/mL Myo: 70.0 ng/mL	S/P/WB	2.50-80.00 ng/mL 0.10-50.00 ng/mL 30.0-600.0 ng/mL	100 µL	10 min	NMPA CE
IF1012	CK-MB/cTnI	Myocardial damage /infarction	CK-MB: 5.00 ng/mL cTnI: 0.10 ng/mL	S/P/WB	2.50-80.00 ng/mL 0.10-50.00 ng/mL	100 µL	10 min	NMPA CE
IF1014	H-FABP	Myocardial damage	6.36 ng/mL	S/P/WB	1.00-120.00 ng/mL	100 µL	3 min	NMPA CE
IF1016	CK-MB/cTnI/H-FABP	Myocardial damage /infarction	CK-MB: 5.00 ng/mL cTnI: 0.10 ng/mL H-FABP: 6.36 ng/mL	S/P/WB	2.50-80.00 ng/mL 0.10-50.00 ng/mL 2.00-100.00 ng/mL	100 µL	10 min	NMPA CE
IF1018	CK-MB	Myocardial injury	5.00 ng/mL	S/P/WB	2.50-80.00 ng/mL	100 µL	10 min	NMPA CE
NEW IF1087	ST2	AMI and chronic heart failure	35.0 ng/mL	S/P/WB	3.0-200.0 ng/mL	100 µL	15 min	CE
Coagulation Marker								
IF1006	D-Dimer	Venous thromboembolism	0.50 mg/L	P/WB	0.10-10.00 mg/L	100 µL	10 min	NMPA CE
Inflammation								
IF1003	hs-CRP+CRP	Cardiovascular inflammation /normal inflammation	3.0 mg/L 10.0 mg/L	S/P/WB/ Fingertip blood	0.5-200.0 mg/L	10 µL	3 min	NMPA CE
IF1007	PCT	Sepsis, bacterial infection	0.10 ng/mL	S/P/WB	0.05-50.00 ng/mL	100 µL	15 min	NMPA CE
IF1015	PCT/CRP	Sepsis, bacterial infection	PCT: 0.10 ng/mL CRP: 3.0 mg/L	S/P/WB	0.10-50.00 ng/mL 0.5-200.0 mg/L	20 µL	15 min	NMPA CE
IF1044	SAA	Bacterial/Virus infection	10.0 mg/L	S/P/WB/ Fingertip blood	5.0-200.0 mg/L	10 µL	5 min	NMPA CE
IF1090	SAA/CRP	Neonatal sepsis, Bacterial/virus infection	SAA: 10.0 mg/L CRP: 10.0 mg/L	S/P/WB/ Peripheral blood	5.0-200.0 mg/L 0.5-200.0 mg/L	10 µL	5 min	NMPA CE
IF1088	IL-6	Acute inflammation	7.0 pg/mL	S/P/WB/ Peripheral blood	1.5-4000.0 pg/mL	40 µL	15 min	NMPA CE
IF1096	hs-CRP	Cardiovascular disease, routine inflammation	Refer to user manual	S/P	0.5-200.0 mg/L	100 µL	3 min	NMPA CE
NEW IF1139	Calprotectin	Inflammatory bowel disease	<50.0 µg/g	Fecal specimen	10.0-600.0 µg/g	100 µL	15 min	CE
Renal Function								
IF1008	CysC	Acute and chronic renal diseases	0.51-1.09 mg/L	S/P/WB	0.50-10.00 mg/L	10 µL	3 min	NMPA CE
IF1009	mAlb	Diabetic nephropathy, hypertensive nephropathy	20.0 mg/L	Urine	10.0-200.0 mg/L	100 µL	3 min	NMPA CE
IF1010	NGAL	Acute kidney injury	Serum: 200.0 ng/mL Urine: 100.0 ng/mL	S/Urine	50.0-5000.0 ng/mL	10 µL	10 min	NMPA CE
IF1011	β ₂ -MG	Acute and chronic kidney diseases/tumours	0.80-3.00 mg/L	S/P/WB	0.50-20.00 mg/L	10 µL	3 min	NMPA CE
Diabetes Mellitus								
IF1017	HbA1c	Diabetes mellitus	3.80%-5.80%	WB	2.00%-14.00%	10 µL	5 min	NGSP IFCC NMPA CE
Metabolic Marker								
IF1031	25-OH-VD	Osteomalacia, osteoporosis	30.00-50.00 ng/mL	S/P/WB/ Capillary blood	8.00-70.00 ng/mL	20 µL	20 min	NMPA CE
NEW IF1112	Osteocalcin	Osteoporosis	Male: 14-70 ng/mL Female: 11-48 ng/mL	S/P/WB	1.5-300.0 ng/mL	100 µL	15 min	CE
Thyroid Function								
IF1024	TSH	Thyroid malfunction	0.27-4.20 µIU/mL	S/P	0.10-50.00 µIU/mL	100 µL	15 min	NMPA CE
IF1022	T3	Hyperthyroidism, hypothyroidism	1.30-3.10 nmol/L	S/P	0.30-10.00 nmol/L	100 µL	15 min	NMPA CE
IF1023	T4	Hyperthyroidism, hypothyroidism	59.00-154.00 nmol/L	S/P	5.40-320.00 nmol/L	100 µL	15 min	NMPA CE
IF1067	ft3	Hyperthyroidism, hypothyroidism	3.10-6.80 pmol/L	S/P/WB	0.60-50.00 pmol/L	100 µL	15 min	NMPA CE
IF1068	ft4	Hyperthyroidism, hypothyroidism	12.00-22.00 pmol/L	S/P/WB	0.30-100.00 pmol/L	100 µL	15 min	NMPA CE

Cat. #	TEST ITEMS	DISEASES	CUT-OFF VALUE	SAMPLE TYPES	MEASURING RANGE	SAMPLE VOLUME	REACTION TIME	QUALIFICATION
Reproduction/Fertility								
IF1013	HCG+β	Fertility	5.1 mIU/mL	S/P	5.0-100000.0 mIU/mL	100 μL	10 min	NMPA CE
IF1055	LH	PCOS, infertility evaluation	Refer to User Manual	S/P	0.20-150.00 mIU/mL	100 μL	15 min	NMPA CE
IF1056	FSH	PCOS, infertility evaluation and pituitary disorders	Refer to User Manual	S/P	0.20-150.00 mIU/mL	100 μL	15 min	NMPA CE
IF1066	AMH	Fertility, PCOS, gonadal function, precocious/late puberty	Refer to User Manual	S/P	0.10-20.00 ng/mL	100 μL	15 min	NMPA CE
IF1048	PRL	Infertility, gonadal disorders	Refer to User Manual	S/P	0.50-200.00 ng/mL	100 μL	15 min	NMPA CE
IF1071	Prog	Infertility, evaluation of ovulation	Refer to User Manual	S/P	0.10-40.00 ng/mL	100 μL	15 min	CE
NEW IF1073	Testosterone	Female polycystic ovary syndrome, male testosterone insufficiency	Male: 1.75-7.81 ng/mL Female: 0.10-0.75 ng/mL	S/P	0.10-16.00 ng/mL	100 μL	15 min	CE
NEW IF1138	Estradiol	Ovarian function	Refer to User Manual	S/P	40.0-4800.0 pg/mL	100 μL	15 min	CE
Tumor Markers								
IF1053	tPSA	Prostate cancer	4.00 ng/mL	S/P	0.40-100.00 ng/mL	100 μL	15 min	NMPA
IF1072	fPSA	Prostate cancer	1.00 ng/mL	S/P	0.03-30.00 ng/mL	100 μL	10 min	NMPA
IF1050	AFP	Liver cancer, cancer of ovaries or testicles, etc.	7.0 ng/mL	S/P	2.0-500.0 ng/mL	100 μL	15 min	NMPA CE
IF1051	CEA	Cancer marker: colon cancer etc.	4.7 ng/mL	S/P	2.0-500.0 ng/mL	100 μL	15 min	NMPA CE
NEW IF1079	CA125	Ovarian cancer	35.0 U/mL	S/P/WB	2-500.0 U/mL	100 μL	15 min	CE
NEW IF1080	CA19-9	Pancreatic cancer	27.0 U/mL	S/P/WB	2-1000.0 U/mL	100 μL	15 min	CE
NEW IF1081	CA15-3	Breast cancer	26.2 U/mL	S/P/WB	1.5-300.0 U/mL	100 μL	15 min	CE
Infectious Disease								
IF1057	Anti-HCV	Hepatitis C	1.00 S/CO	S/P	1.00-20.00 S/CO	100 μL	15 min	
IF1058	Anti-TP	Syphilis	1.00 S/CO	S/P	1.00-50.00 S/CO	100 μL	15 min	CE
IF1059	Anti-HIV	AIDS	1.00 S/CO	S/P	1.00-1000.00 S/CO	100 μL	15 min	
IF1064	HBsAg	Hepatitis B	1.00 IU/mL	S/P	1.00-100.00 IU/mL	100 μL	15 min	
IF1063	Anti-HBs	Hepatitis B	10.00 mIU/mL	S/P/WB	10.00-1000.00 mIU/mL	100 μL	15 min	
IF1091	SARS-CoV-2 Antigen	COVID-19	1.00 COI	Nasal swab		100 μL	15 min	CE
IF1047	<i>H. pylori</i>	<i>H. pylori</i> infection	5.0 ng/mL	Stool	1.0-200.0 ng/mL	10-50 mg	10 min	CE
IF1086	Influenza A/B	Respiratory viral infection	1.00 COI	Nasal swab		100 μL	15 min	CE
IF1136	Dengue NS1 Ag	Dengue virus infection	1.00 S/CO	S/P/WB	1.00-50.00 S/CO	100 μL	15 min	CE
Specific Protein and Rheumatism								
IF1075	RF	Rheumatoid arthritis	15.9 IU/mL	S/P/WB	10.0-640.0 IU/mL	10 μL	10 min	NMPA CE
IF1076	ASO	Rheumatic fever, acute glomerulonephritis, group A streptococcal infection	408.0 IU/mL	S/P/WB	60.0-1370.0 IU/mL	10 μL	10 min	NMPA CE
IF1029	Anti-CCP	Rheumatoid arthritis	25.0 U/mL	S/P/WB	10.0-400.0 U/mL	10 μL	15 min	CE
Others								
IF1077	Ferritin	Anemia/tumors	Male: 30.00-400.00 ng/mL Female: 13.00-150.00 ng/mL	S/P	0.50-1000.00 ng/mL	10 μL	15 min	NMPA CE
IF1069	Total IgE	Allergic disorders	Refer to User Manual	S/P/WB	1.00-2000.00 IU/mL	100 μL	15 min	CE
NEW IF1052	PG I/PG II	Atrophic gastritis, stomach cancer	PG I < 70.0 ng/mL PG I/PG II < 3.0 ng/mL	S/P	PG I: 1.0-200.0 ng/mL PG II: 1.0-100.0 ng/mL	100 μL	15 min	CE
IF1110	Cortisol	Adrenal cortex function	Refer to User Manual	S/P	11-1655 nmol/L	100 μL	15 min	CE

Coming soon: VB12, Folate...

GP Getein Biotech, Inc.

Add.: No.9 Bofu Road, Luhe District, Nanjing, 211505, China
Tel.: +86-25-68568508/68568594
Fax: +86-25-68568500
E-mail: overseas@getein.com.cn; marketing@getein.com.cn
Web.: www.getein.com



FSC

CE

NMPA



BGMP

NGSP

IFCC

IVD

