


1. Product Name and Product Code:

AL-1202-070.V001 - Adult Anesthesia Circuit Smoothbore PVC Tube

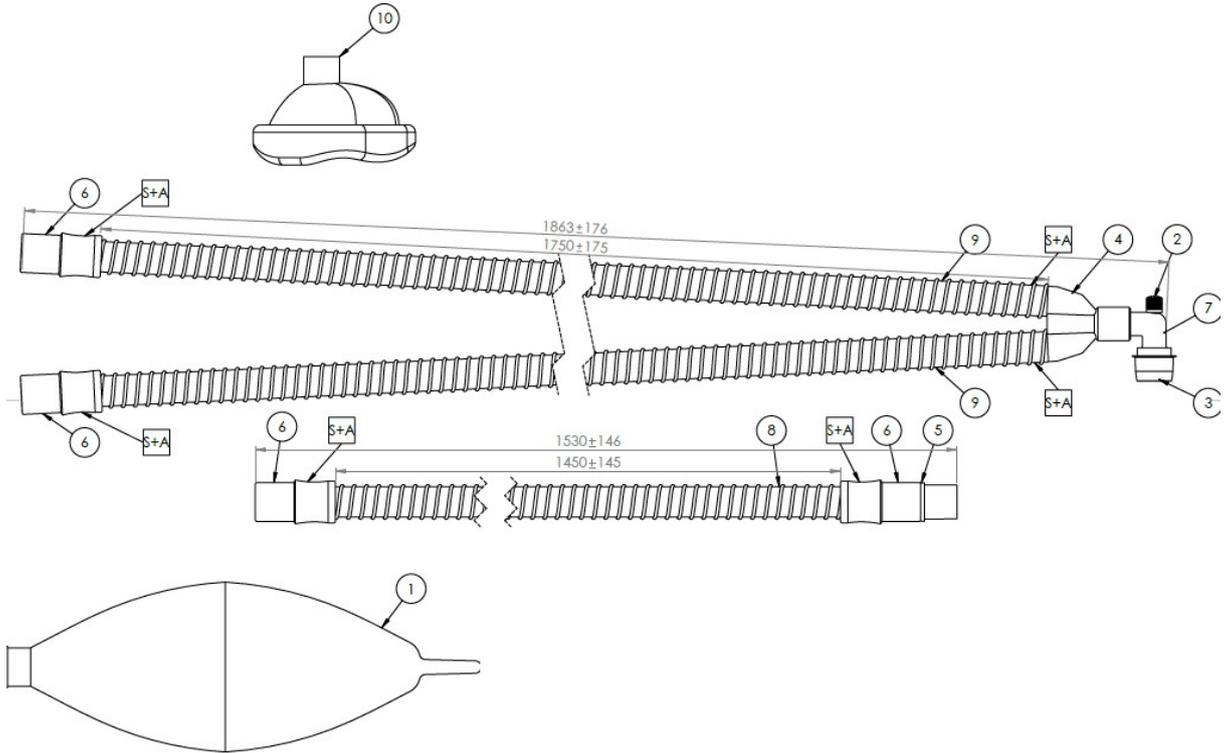

2. Manufacturer:

Meditera Tibbi Malzeme Sanayi ve Ticaret A.Ş.

3. Sterilization Method :

Ethylene oxide sterilization. This product line is provided both as sterile and nonsterile.

4. Packaging:

Nylon packaging. ISO Class 8 Clean Room Manufactured

5. Intended Use and Functional Description :

Disposable circuits used to conduct medical gases from the anaesthesia system to the patient. Anaesthetic gas exits the anaesthesia machine (via the common gas outlet) and then enters a breathing circuit. The function of the circuit is to deliver oxygen and anaesthetic gases to the patient and to eliminate CO₂. The CO₂ may be eliminated by gas inflow or by soda lime absorption.

6. Shelf life :

5 years from the date of production .

7. Product Description:

7.1. Classification: Class IIa Rule 2

7.2. This product does not contain any metallic parts

7.3. Specification of the product :

Item	Description	Quantity
AL-09004	ANESTHESIA MASK #4	1
150.07.040	2 LT NEOPRENE SINGLE FOLDED BREATHING BAG WITH STICKER(RIGID PP CONNECTOR)	1
150.11.036	ELBOW CONNECTOR LUER CAP	1
151.03.021.01	LONG CONNECTOR CAP RED	1
151.03.110	22-22MM STRAIGHT CONNECTOR	1
151.03.178.01	ELBOW CONNECTOR WITH CO ₂ PORT PP	1
151.03.237.02	19 MM PARALLEL Y CONNECTOR W/OUT PORTS (SBC)	1
151.03.248	22M/22F STRAIGHT CONNECTOR PVC NEW	4
151.05.03.004	19 MM SMOOTHBORE TUBING 145 CM CUT PVC	1
151.05.03.005	19 MM SMOOTHBORE TUBING 175 CM CUT PVC	2

8. Standarts:

EN ISO 13485:2003, 93/42/EEC Medical Device Directive, EN ISO 5367, EN ISO 5356-1, EN ISO 11607-1:2009, EN ISO 11607-2:2009, EN ISO11135-1:2007, EN ISO 23328-1, EN ISO 23328-2, EN ISO 594-1

9. Waste Method:

After use product will be “contaminated medical waste” and package will be “packaging waste” so they should be handled according to relevant national and international standards and regulations.