

Quality Control Report


AOZ ELISA kit

(Cat No: KA00106H)

Lot No.: H260103A10

Date of Production: 2026-01-07

Expired: 2027-01-06

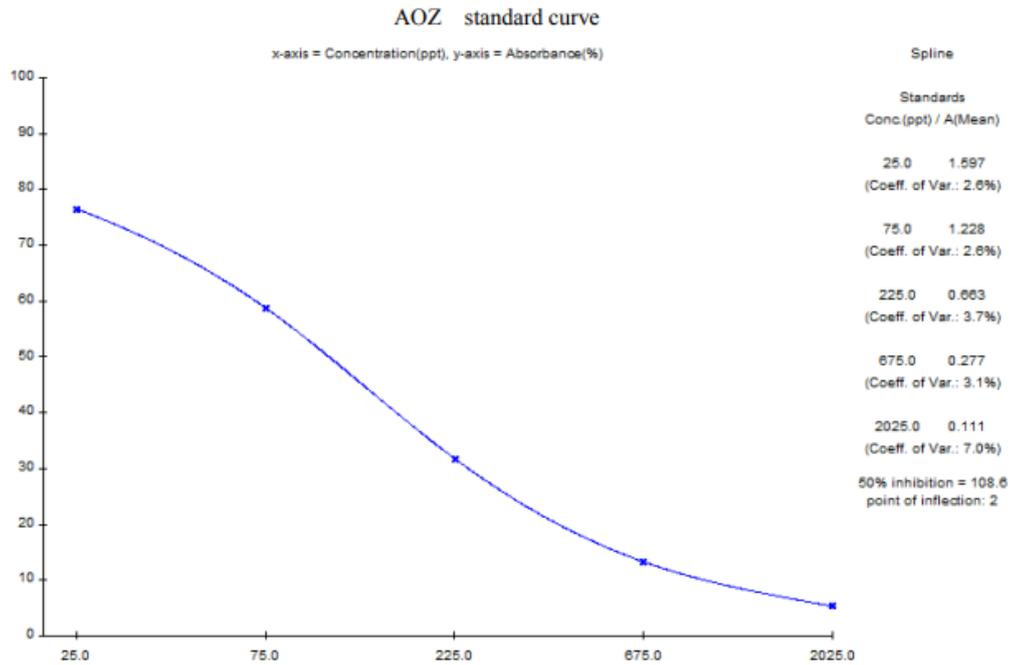

Standards						
Ser. No.	Concentration ppt	Absorbance (Mean)	(CV)	B/B0 (%)	calculated ppt	Deviation (%)
1	0.0	2.087	2.1	100.0		
2	25.0	1.597	2.6	76.5	25.0	0.0
3	75.0	1.228	2.6	58.8	74.9	0.1
4	225.0	0.663	3.7	31.8	225.3	0.1
5	675.0	0.277	3.1	13.3	675.8	0.1
6	2025.0	0.111	7.0	5.3	2020.2	0.2

Please notice: This QC report is only for reference, for the absorbance of the standard solutions may fluctuate in a certain range.

