



EuroProxima


AHD

CERTIFICATE OF ANALYSIS

Doc. No:	5091AHD-CA V11
Batch No:	220751
Code:	5091AHD
Exp. Date:	11-2023

This certificate relates to the above specified product batch and number only. The product has been tested according to our standard quality control program. The product is guaranteed when stored according to the instruction in the manual till the indicated expiry date.

Components:	Lot No:	Exp. Date:
Microtiter plate	220423	11-2023
Conjugate	220424	11-2023
Standards 2 - 1 - 0,5 - 0,25 - 0,125 - 0,0625 - 0 ng/ml	220425	05-2024
Standard 100 ng/ml	220426	05-2024
Sample Dilution Buffer	220530	06-2024
Dilution buffer	WN6820	11-2023
Rinsing buffer	220001	01-2024
TMB substrate	220573	12-2024
Stop solution	220106	02-2024
Protocol	Code 5091AHD [7] 12.20	

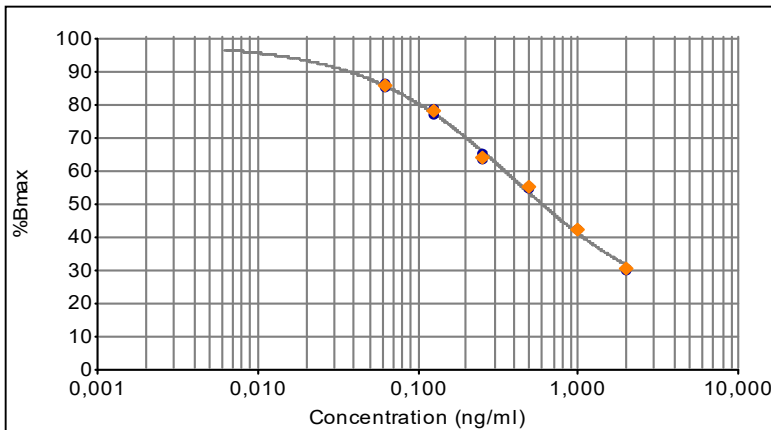

Validation criteria

Bmax > 0.8 OD.
Blank < 0.2 OD.

Concentration (ng/ml)	Accepted Range %Bmax	Mean %Bmax
STD 1	32 - 49	42
STD 0,5	45 - 64	55
STD 0,25	56 - 76	64
STD 0,125	71 - 89	78

Performed by:

KS

date: 08-08-2022

Accepted by:

QA/QC Manager



This product is produced under the control of a management system approved by Bureau Veritas certification in accordance with the standard ISO 9001: 2015 Bureau Veritas Certification N°3089368

