

Lot nr. 102 Brancarda sanitara (caracteristici de baza), MYS-950, Meyosis, Turcia

<i>Specificarea tehnică deplină solicitată, Standarde de referință</i>	<i>Specificarea tehnică deplină oferita, Standarde de referință</i>
Brancarda sanitara (caracteristici de baza) Cod 140370 Descriere Brancardă destinată pentru transportarea pacienților Parametru Specificație Poziționare Tredelinburg ≥ 15 grade Control manual Caracteristici Bare laterale da Roți Diametru ≥ 15 cm Frine ≥ 2 Sarcina maximă ≥ 200 kg Dimensiuni $\geq 200 \times 75$ cm Mînere pentru transportarea brancardei da Saltea, rezistentă la prelucrare și apă da, detașabilă Să fie dotată cu roțile/bamper de protecție în toate patru colțuri pentru evitarea lovirii de perete da	Brancarda sanitara (caracteristici de baza) Cod 140370 Descriere Brancardă destinată pentru transportarea pacienților Parametru Specificație Poziționare Tredelinburg ≥ 15 grade Control manual Caracteristici Bare laterale da Roți Diametru -20 cm Frine ≥ 2 Sarcina maximă - 250 kg Dimensiuni - 215 x 75 cm Mînere pentru transportarea brancardei da Saltea, rezistentă la prelucrare și apă da, detașabilă Dotată cu roțile/bamper de protecție în toate patru colțuri pentru evitarea lovirii de perete da

Anexa 104 Pat multifunctional pentru adulti (6-8 pozitii),MYS-5410NE, Meyosis, Turcia

Specificarea tehnică deplină solicitată, Standarde de referință	Specificarea tehnică deplină oferita, Standarde de referință
Pat multifunctional pentru adulți (6-8 poziții) Cod 140400 Descriere Paturi motorizate pentru secții de ATI și secții de reanimare Parametrul Specificația Tip multifuncțional cu 6-8 poziții Tip pacient adult Controlul pacientului tip Toate butoanele să fie însoțite de simboluri grafice Funcționalități poziționare sedentară poziționare Trendelenburg poziționare anti-Trendelenburg Controlul de către asistentă Blocarea control pacient da Greutatea maximă a pacientului Cu etichetă pe pat ≥ 220 kg Înălțime Ajustabilă ≥ 74 cm Rotile Diametru ≥ 12.5 cm Sistem de blocare la minim 2 rotile Parapete de protecție laterale da Sectiunea spate să aibă cadru pentru detector radiologic $\geq 43 \times 43$ cm Reglare manuală a părților importante în caz de lipsă de energie electrică opțională Alimentare 220 V, 50 Hz Saltele lavabile ortopedică da	Cod 140400 Descriere Paturi motorizate pentru secții de ATI și secții de reanimare Parametrul Specificația Tip multifuncțional cu 6-8 poziții Tip pacient adult Controlul pacientului tip Toate butoanele sunt însoțite de simboluri grafice Funcționalități poziționare sedentară poziționare Trendelenburg poziționare anti-Trendelenburg Controlul de către asistentă Blocarea control pacient da Greutatea maximă a pacientului Cu etichetă pe pat 250 kg Înălțime Ajustabilă 77,5 cm Rotile Diametru ≥ 12.5 cm Sistem de blocare la minim 2 rotile Parapete de protecție laterale da Sectiunea spate să aibă cadru pentru detector radiologic $\geq 43 \times 43$ cm Reglare manuală a părților importante în caz de lipsă de energie electrică opțională Alimentare 220 V, 50 Hz Saltele lavabile ortopedică da


MYS-950

HYDRAULIC STRETCHER



Meyosis®

TECHNICAL INFORMATION

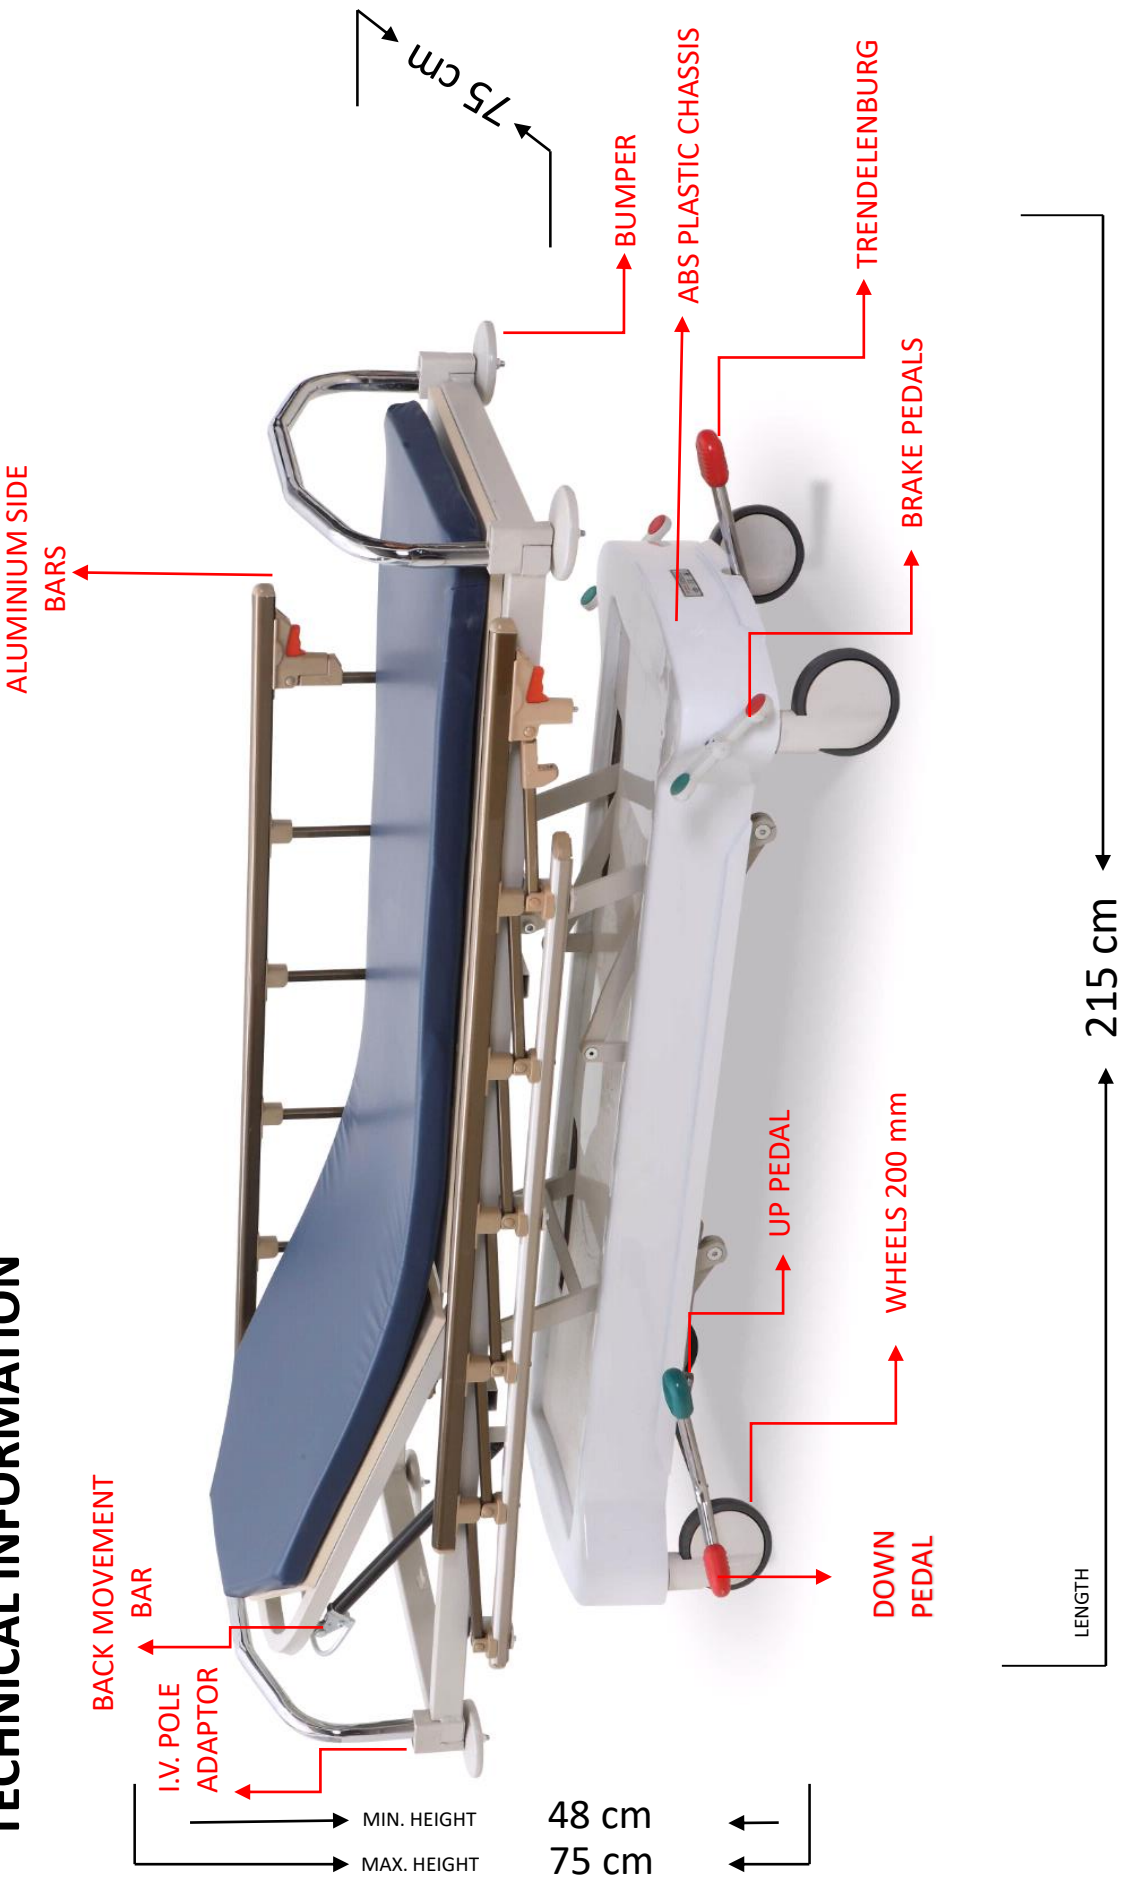

PATIENT MANAGEMENT SOLUTIONS

HYDRAULIC STRETCHER FOR TRANSFER AND EXAMINATION CASES.
ADVANCED MOBILITY, SAFETY AND EFFICIENCY.



BACK MOVEMENT

- Backrest adjustment by gas spring.




HEIGHT ADJUSTMENT

- Dual sided foot pedals for hi-lo



BUMPERS

- Bumpers on 4 corners of the stretcher.

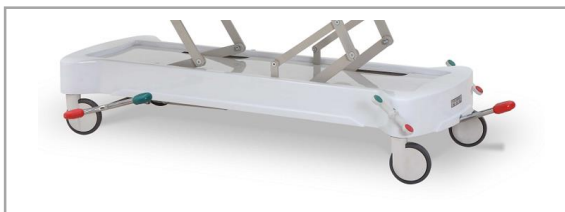

BRAKE SYSTEM

- 360° swivel wheels with central brake system and directional lock.

TRENDELENBURG

- Trendelenburg function by pedals on foot end chasis of the stretcher.
- 250 kg weight capacity





MEYOSİS HASTANE EKİPMANLARI SAN. VE TİC. A. Ş.

Headquarters: Küçükbakkalköy Mh. Dudullu Cd N:23-25/B

Brandium R2 Blok Kat:23 Daire: 217 Ataşehir – İstanbul

T:+902165746738 F:+902165746739

Manufacturing: Devekaldırımı Caddesi No :10 Bağcılar –
İstanbul - Turkey

www.meyosis.com



MYS-5410NE
ICU BED WITH 4 MOTORS



MEYOSİS HASTANE EKİPMANLARI SAN. VE TİC. A. Ş.

Headquarters: Küçükbakkalköy Mh. Kayışdağı Cd N:137/1 Çelik
Plaza Kat:4 Ataşehir – İstanbul

T:+902165746738 F:+902165746739

Manufacturing: Devekaldırım Caddesi No :10 Bağcılar – İstanbul

www.meyosis.com

PRODUCT:

TRADE MARK : MEYOSIS
MODEL : MYS-5410NE
NAME : ICU HOSPITAL BED WITH 4 MOTORS



1. TECHNICAL SPECIFICATIONS:

- a.** Backrest, leg rest, auto contour, height (up - down), Trendelenburg and reverse Trendelenburg positions are controlled by 4 DC motors.
- b.** Positions are controlled by “Hand Remote Control”.
- c.** Angle indicator on each side rail of the bed.
- d.** Head and foot boards are made of PP plastic and easily clearable. These parts can also be assembled and disassembled easily.
- e.** 4 pieces of restraint strap holder (2 pieces on each side).
- f.** Lying surface consists of 4 pieces easily clearable ABS plastic.
- g.** 4 pieces folding side rails are made of PP plastic and have release system assisted by gas spring.
- h.** Automatic back sliding and leg sliding functions are available in the bed.
- j.** Metal chassis is epoxy polyester electrostatic painted and covered with ABS plastic.
- k.** Bumpers are located at each corner of the bed to protect the bed against crushes.
- l.** Accessory sockets are located at each corner of the bed for IV poles or traction sets.
- m.** One adjustable IV pole is provided with the bed.
- n.** There are drainage bag holders at both sides of the bed.
- o.** Mattress is waterproof and zippered.
- p.** 125mm 360° swivel wheels with cross brake system.

2. DIMENSIONS:

- Full Length: 212,5 cm
- Full Width: 107 cm
- Minimum Height: 41,5 cm
- Maximum Height: 77,5 cm
- Mattress Length : 190 cm
- Mattress Width : 90 cm
- Weight Capacity: 250 kg



3. OPERATING ANGLES:

- Back Movement: 0°-70°
- Leg Movement: 0°-30°
- Vascular Position
- Knee Movement
- Hight Adjustment
- Trandelenburg & Reverse Trandelenburg 0°-17°
- Cardiac Position



4. MATTRESS:

- Waterproof and zipped cover,
- CNC cut,
- Adaptable to all movements
- **28 kg/m³** density foam
- 90 cm x 190 cm x 11 cm (h)



MYS-100S Mattress is included to all Meyosis Hospital Beds.

5. CONTROLS:

- Backrest, legrest, automatic contour and height (up - down), Trendelenburg, reverse Trendelenburg and CPR positions can be adjusted electronically by the help of the keys on **hand remote control and Nurse Control Panel, by foot end.**

CERTIFICATE

TÜRCERT Certification Body
with this document.

MEYOSİS HASTANE EKİPMANLARI SANAYİ VE TİCARET ANONİM ŞİRKETİ

Merkez: İnönü Mah. Kayışdağı Cad. No:128 D-1 Kandış İş Merkezi Ataşehir / İstanbul
Fabrika: Hadımköy Mah. 75.Yıl Cad. Dış Kapı No:26 D:İŞY2 Arnavutköy / İstanbul

of the manufacturer

«Production, sales and marketing of patient beds and mechanical,
hydraulic, electrical, motor, electromechanical, equipped patient beds,
technical services»

effective medical devices quality management system
and guarantees that you put in to apply.

2021051702MDQMS with the nr. examination report;

TS EN ISO 13485 : 2016

This certification has been completed according to TURCERT
audit and certification procedures and is valid until surveillance
audit . 16.05.2023

Certificate Registration Nr : 2021051702

Certificate First Issue Date : 17.05.2021

Date of Issue : 09.05.2022

Certificate Validity Date : 16.05.2023



Türccert A.Ş.
Certification on Behalf



51902430608 (MDQMS)

TÜRCERT TEKNİK KONTROL ve BELGELENDİRME ANONİM ŞİRKETİ
Adres: Merkez Mah. Dr. Sadık Ahmet Cad. No:38/44 A Güngören - İstanbul - Turkey
Tel: +90 212 702 40 00 www.turcert.com

Bu belge müşterinin TÜRCERT'in kurallarına ve sözleşme şartlarına uyduğu sürece geçerlidir.
This certificate is valid during the customer obeys the rules TÜRCERT procedures and agreements.





DECLARATION OF CONFORMITY

MEYOSİS HASTANE EKİPMANLARI SANAYİ VE TİCARET ANONİM ŞİRKETİ

İnönü Mah. Kayışdağı Cad. Kandış İş Merkezi No:128 kat: 1 D:1 Ataşehir/İstanbul, Türkiye

PRODUCTS:

Hydraulic Stretcher: MYS-950

CLASSIFICATION : Class 1

We herewith declare that the above mentioned products meet the provisions of the following EC Council Directives and Standards.

GENERAL APPLICABLE DIRECTIVES:

Medical Devices Directive 93/42/EEC of June 1993 concerning medical devices.


Date / Place of Issue : 04.01.2021 / İSTANBUL

Name : Mehmet Öğün Geyik

Position : Chairman

Signature:

MEYOSİS HASTANE EKİPMANLARI
SAN. VE TİC. A.Ş.
İnönü Mah. Kayışdağı Cad. No:128
K:1 Kandış İş Merkezi Ataşehir İST.
Koşuyatağı V.D. 742 048 2891
Tic. Sic. No:44513-5





DECLARATION OF CONFORMITY

MEYOSİS HASTANE EKİPMANLARI SANAYİ VE TİCARET ANONİM ŞİRKETİ

İnönü Mah. Kayışdağı Cad. Kandış İş Merkezi No:128 kat: 1 D:1 Ataşehir/İstanbul, Türkiye

PRODUCTS:

4 Motors ICU Hospital Bed: MYS-5410NE

CLASSIFICATION : Class 1

We herewith declare that the above mentioned products meet the provisions of the following EC Council Directives and Standards.

GENERAL APPLICABLE DIRECTIVES:

Medical Devices Directive 93/42/EEC of June 1993 concerning medical devices.

Standards:

EN 60601-1:2009 : Particular requirements for the basic safety and essential performance of medical beds

EN 60601-2-38:2003 : Particular requirements for the safety of electrically operated hospital beds

Date / Place of Issue : 04.01.2021 / İSTANBUL

Name : Mehmet Öğün Geyik

Position : Chairman

Signature :

MEYOSİS HASTANE EKİPMANLARI
SAN. VE TİC. A.Ş.
İnönü Mah. Kayışdağı Cad. No:128
K:1 Kandış İş Merkezi Ataşehir İST.
Koşuyolu V.D. 742 048 2891
Tic. Sic. No:44513-5

