




Sizing guide

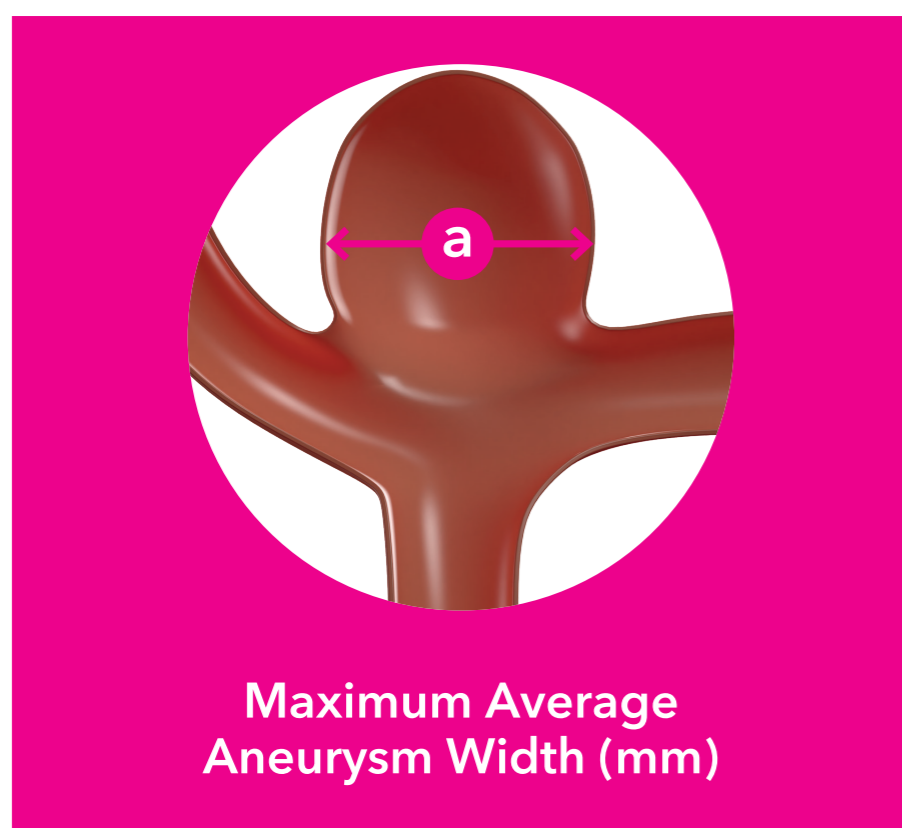

Maximum Average Aneurysm Width (mm)

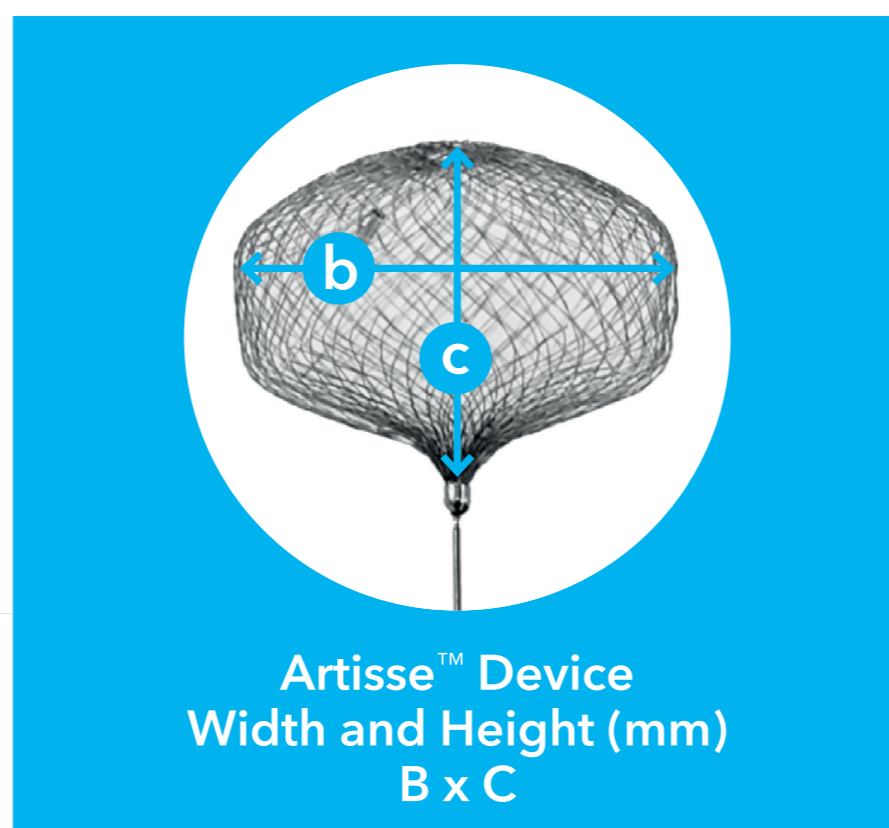

Artisse™ Device Width and Height (mm) B x C

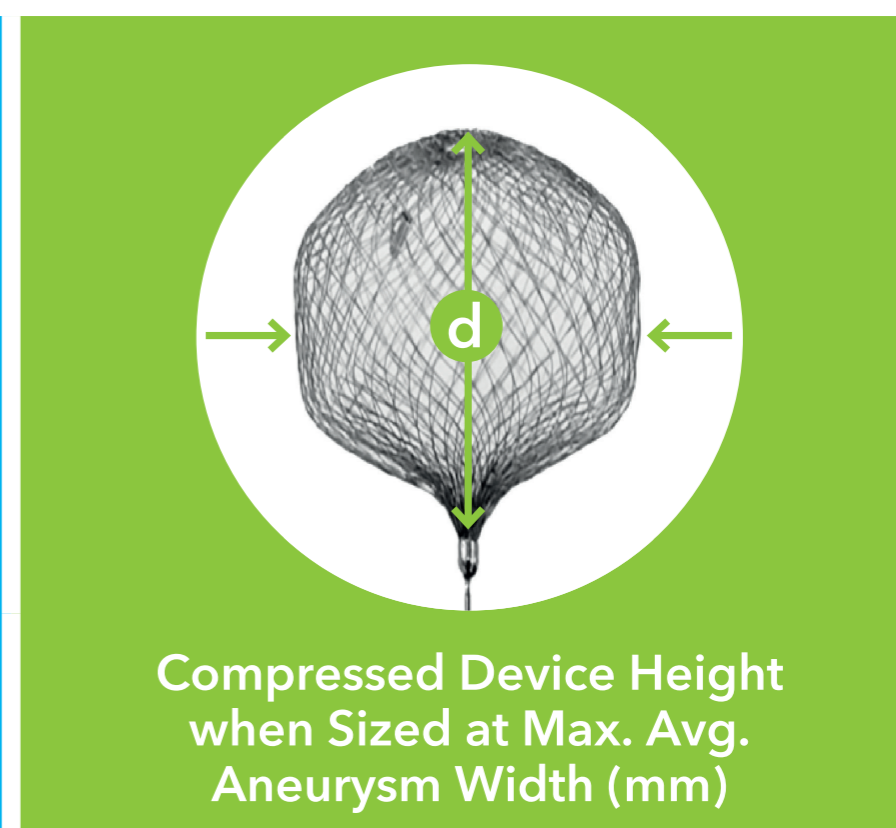

Compressed Device Height when Sized at Max. Avg. Aneurysm Width (mm)

3.4	4.5 x 3.0	4.5
3.4	4.5 x 4.0	5.2
3.8	5.0 x 3.0	4.9
3.8	5.0 x 4.0	5.5
4.1	5.5 x 3.0	5.2
4.1	5.5 x 4.0	5.9
4.1	5.5 x 5.0	6.9
4.5	6.0 x 3.0	5.6
4.5	6.0 x 4.0	6.2
4.5	6.0 x 5.0	7.2
4.9	6.5 x 3.0	5.9
4.9	6.5 x 4.0	6.6
4.9	6.5 x 5.0	7.6
5.3	7.0 x 3.0	6.3
5.3	7.0 x 4.0	7.0
5.3	7.0 x 5.0	7.9
5.6	7.5 x 4.0	7.4
5.6	7.5 x 5.0	8.3
6.0	8.0 x 4.0	7.8
6.0	8.0 x 5.0	8.7

Note 1: If the measured average aneurysm width is between widths **a**, target a larger group of devices while accounting for aneurysm height.

Note 2: Aneurysm Height \geq Compressed Device Height.

Estimated width oversizing factor

+1

+1.5

+2