

Letter of Authorization

To whom it may concern,

We, Getein Biotech, Inc. (No.9 BoFu Road, Luhe District, Nanjing, 211505, China), hereby authorize Sanmedico SRL as our official distributor for registering, promoting, selling, distributing, taking part in tenders, maintaining & after sale technical services of under-mentioned product in the territory of Moldova:

Sanmedico SRL will comply with the laws and regulations of the countries and regions where they are located in and where they are selling mentioned product to, otherwise, the risks and losses arising therefrom shall be undertaken by Sanmedico SRL

This authorization starts from Jan 1, 2022 and will be valid to December 31 2023

Getein Biotech, Inc. has the right to terminate the authorization before validity and will inform Sanmedico SRL with 10 days in advance.

Getein Biotech, Inc.

Name: Steven Zhou

Position: Overseas Sales Director

基蛋生物科技股份有限公司
GETEIN BIOTECH, INC.



Exclusive Distributor Agreement

This agreement is made and entered into by and between the parties concerned on 1th Jan, 2022 in Nanjing, China on the basis of equality and mutual benefit to develop business on terms and conditions mutually agreed upon as follows:

1. The Parties Concerned

Party A: Getein Biotech, Inc.

Add: No.9 Bofu Road, Luhe District, Nanjing (211505) China.

Tel: 86-25-68568519

Fax: 86-25-68568500

Party B: Sanmedico SRL

Add: Republic of Moldova, Chisinau, MD-2059, Petricani street, 88/1, office 10

Tel: 373 22 62 30 32

2. Appointment

Party A hereby appoints Party B as its exclusive distributor in the Republic of Moldova for the promotion, sales, and after-sale services etc. of products (Refer to Item3) from Party A and Party B accepts and assumes such appointment.

3. Products

List A

One Step Test for CK-MB/cTnI/Myo (Colloidal Gold)(Quantitative)
Cardiac Troponin I Fast Test Kit(Colloidal Gold)(Quantitative)
One Step Test for CK-MB (Colloidal Gold)(Quantitative)
One Step Test for CK-MB/cTnI (Colloidal Gold)(Quantitative)
One Step Test for H-FABP(Colloidal Gold)(Quantitative)
One Step Test for NT-proBNP/cTnI(Colloidal Gold)(Quantitative)
One Step Test for hs-CRP(Colloidal Gold)(Quantitative)
One Step Test for D-Dimer(Colloidal Gold)(Quantitative)
One Step Test for NT-proBNP(Colloidal Gold)(Quantitative)
One Step Test for HbA1c(Colloidal Gold)(Quantitative)
One Step Test for PCT(Colloidal Gold)(Quantitative)
One Step Test for HCG(Colloidal Gold)(Quantitative)
One Step Test for mAlb(Colloidal Gold)(Quantitative)
One Step Test for β 2-MG(Colloidal Gold)(Quantitative)
One Step Test for CysC(Colloidal Gold)(Quantitative)
One Step Test for NAGL(Colloidal Gold)(Quantitative)
One Step Test for TSH(Colloidal Gold)(Quantitative)

CK-MB/cTnl/Myo Fast Test Kit(Immunofluorescence Assay)
Cardiac Troponin I Fast Test Kit(Immunofluorescence Assay)
NT-proBNP/cTnl Fast Test Kit(Immunofluorescence Assay)
hs-CRP Fast Test Kit(Immunofluorescence Assay)
D-Dimer Fast Test Kit(Immunofluorescence Assay)
NT-proBNP Fast Test Kit(Immunofluorescence Assay)
PCT Fast Test Kit(Immunofluorescence Assay)
mAlb Fast Test Kit(Immunofluorescence Assay)
B2-MG Fast Test Kit(Immunofluorescence Assay)
CysC Fast Test Kit(Immunofluorescence Assay)
NAGL Fast Test Kit(Immunofluorescence Assay)
HbA1c Fast Test Kit(Immunofluorescence Assay)
TSH Fast Test Kit(Immunofluorescence Assay)
T3 Fast Test Kit(Immunofluorescence Assay)
T4 Fast Test Kit(Immunofluorescence Assay)
PRL Fast Test Kit(Immunofluorescence Assay)
LH Fast Test Kit(Immunofluorescence Assay)
FSH Fast Test Kit(Immunofluorescence Assay)
AMH Fast Test Kit(Immunofluorescence Assay)
tPSA Fast Test Kit(Immunofluorescence Assay)
25-OH-VD Fast Test Kit(Immunofluorescence Assay)
Gepin 1100 Immunofluorescence Quantitative Analyzer
Gepin 1600 Immunofluorescence Quantitative Analyzer

4. Territory:

In Republic of Moldova only.

Meanwhile Party B will not distribute for competitive firms identical or similar products, nor will associate directly or indirectly with the competitive firms in the field of products covered by this agreement; otherwise, party A has the right to decide whether to terminate the contract immediately or not.

5. Prices

Prices are stable for 12 months from the start of this agreement. Party A will not increase the prices subjectively, unless the raw material suppliers increase their prices. In case price increases have to be announced, Party B has to be informed at least one month (30 days) in advance.

This agreement shall come into force from Jan 1st,2022to Jan 1st,2024,is valid for 24 months.

6.Delivery

Party A shall establish a delivery term for each Party B's order, which shall not exceed 4 weeks after the payment is received. Party A will advise Party B about the day of dispatching, with all requested information concerning the dispatched products.

7. FORCE MAJEURE

If the performance of any part of this agreement interfered with new laws or governmental restrictions, war, civil commotions, riots, strike lockout, acts of God such as flood, fire or any other similar causes which are beyond the control of the parties, no party shall be responsible for delay or failure of performance of this agreement for such length of time and to the extent performance is made impossible. In this case, the parties shall immediately negotiate to what extent deliveries that could not be executed can be carried out executed.

8. Payment Term

Every order Party B shall pay 50% by TT in advance, the rest of 50% will be paid within 30-60 days after the goods arrives. Due to financial audition, all the credit payment should be cleared by December 31th, 2022.

If Party B is unable to pay, Party B will agree to use fixed assets or real estate to offset the loan. Party A has the right to bring a lawsuit against Party B in China according to relevant Chinese laws.

9. Sales target

Yearly sales volume is 200,000 USD, which include both analyzers and strips. Party B agrees and accepts the sales volume...

10. Governing Law

The agreement is subject to the International Trade Law. Any dispute concerning this agreement shall be settled in accordance with the International Trade Law either through negotiation or through legal proceedings if negotiation has failed.

11. Declaration of Conformity.

Getein Biotech, Inc. declares herein the above mentioned device (Refer to Item3) meets the basic requirements of the European Parliament and the Council' s in vitro diagnostic medical devices directive: 98/79/EC Annex III.

This declaration of conformity is based on European Parliament and the Council' s 98/79/EC directive Annex III. The compiled technical file and quality system document according to 98/79/EC directive Annex III are testified and the quality system certificate has issued by TÜV Rheinland (Shanghai) Co., Ltd.

12. Intellectual Property Agreement

Party A reserves the right of goods design, drawing, plane graph specification, technology, data and information, technological process, the marketing plan of intellectual property rights which included the

Party A provide technical services to the Party B in the process of producing intellectual achievements . Without the Party A 's written consent, the Party B shall not disassemble the goods and the accompanying software, decoding, encoding, or any other reverse engineering by themselves or other third party.

13. Final Provisions

Attachments are an integral part of this contract, have the same legal effect with this contract; This contract was made in English with two originals, each party holds one, it is effective at the same time, and have the same legal effect.

Any change, modification, cancellation of this contract, to be replaced shall be made after agreed by both parties in writing.

Party A: Getein Biotech, Inc.

Date:

Represented by: Steven Zhou

Regional Sales Manager

Party B: Sanmedico SRL

Date:

Represented by: Vitalie Goreacii

Director

基蛋生物科技股份有限公司
GETEIN BIOTECH, INC.



Declaration of Conformity



according to Directive 98/79/EC, on in vitro diagnostic medical devices

Maker (Name, Address)	Getein Biotech, Inc. No. 9 Bofu Road, Luhe District, Nanjing, 211505, China		
Authorized Representative (Name, Address)	Lotus NL B.V. Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague, Netherlands.		
Medical device	Description :		FIA8000 Quantitative Immunoassay Analyzer FIA8600 Quantitative Immunoassay Analyzer Cardiac Troponin I Fast Test Kit One Step Test for cTnI (Colloidal Gold) cTnI Rapid Test (Colloidal Gold Assay) One Step Test for NT-proBNP (Colloidal Gold) One Step Test for NT-proBNP/cTnI (Colloidal Gold) One Step Test for CK-MB/cTnI/Myo (Colloidal Gold) One Step Test for hs-CRP+CRP (Colloidal Gold) One Step Test for D-Dimer (Colloidal Gold) One Step Test for PCT (Colloidal Gold) One Step Test for β 2-MG (Colloidal Gold) One Step Test for mAlb (Colloidal Gold) One Step Test for NGAL (Colloidal Gold) One Step Test for CysC (Colloidal Gold) One Step Test for HCG+ β (Colloidal Gold) One Step Test for HbA1c (Colloidal Gold) One Step Test for PCT/CRP (Colloidal Gold) One Step Test for CK-MB/cTnI/H-FABP (Colloidal Gold) One Step Test for H-FABP (Colloidal Gold) One Step Test for CK-MB/cTnI (Colloidal Gold) One Step Test for CK-MB (Colloidal Gold) One Step Test for TSH (Colloidal Gold) One Step Test for T4/T3 (Colloidal Gold) One Step Test for T3 (Colloidal Gold) One Step Test for T4 (Colloidal Gold) One Step Test for 25-OH-VD (Colloidal Gold) One Step Test for FOB (Colloidal Gold) One Step Test for <i>H. pylori</i> (Colloidal Gold) One Step Test for SAA (Colloidal Gold) Getein1100 Immunofluorescence Quantitative Analyzer Getein1600 Immunofluorescence Quantitative Analyzer Getein1180 Immunofluorescence Quantitative Analyzer Getein1200 Immunofluorescence Quantitative Analyzer Cardiac Troponin I Fast Test Kit (Immunofluorescence Assay) NT-proBNP Fast Test Kit (Immunofluorescence Assay) hs-CRP+CRP Fast Test Kit (Immunofluorescence Assay) NT-proBNP/cTnI Fast Test Kit (Immunofluorescence Assay) CK-MB/cTnI/Myo Fast Test Kit (Immunofluorescence Assay) D-Dimer Fast Test Kit (Immunofluorescence Assay)



		PCT Fast Test Kit (Immunofluorescence Assay) β2-MG Fast Test Kit (Immunofluorescence Assay) mAlb Fast Test Kit (Immunofluorescence Assay) NGAL Fast Test Kit (Immunofluorescence Assay) CysC Fast Test Kit (Immunofluorescence Assay) CK-MB Fast Test Kit (Immunofluorescence Assay) CK-MB/cTnI Fast Test Kit (Immunofluorescence Assay) HCG+β Fast Test Kit (Immunofluorescence Assay) HbA1c Fast Test Kit (Immunofluorescence Assay) PCT/CRP Fast Test Kit (Immunofluorescence Assay) CK-MB/cTnI/H-FABP Fast Test Kit (Immunofluorescence Assay) H-FABP Fast Test Kit (Immunofluorescence Assay) 25-OH-VD Fast Test Kit (Immunofluorescence Assay) TSH Fast Test Kit (Immunofluorescence Assay) T3 Fast Test Kit (Immunofluorescence Assay) T4 Fast Test Kit (Immunofluorescence Assay) 25-OH-VD Fast Test Kit (Immunofluorescence Assay) FOB Fast Test Kit (Immunofluorescence Assay) <i>H. pylori</i> Fast Test Kit (Immunofluorescence Assay) SAA Fast Test Kit (Immunofluorescence Assay) LH Fast Test Kit (Immunofluorescence Assay) FSH Fast Test Kit (Immunofluorescence Assay) AMH Fast Test Kit (Immunofluorescence Assay) PRL Fast Test Kit (Immunofluorescence Assay) CK-MB Control cTnI Control Myo Control NT-proBNP Control D-Dimer Control CRP Control PCT Control β2-MG Control mAlb Control NGAL Control CysC Control H-FABP Control HbA1c Control HCG+β Control CK-MB/cTnI/Myo Control CK-MB/cTnI Control NT-proBNP/cTnI Control TSH Control T4/T3 Control T3 Control T4 Control	
	Classification of products according to directive	:	Others
	Batch/serial No. Type, production term (if applicable)	:	



Applicable coordination standards:	EN ISO 14971:2012	EN ISO 23640:2015	EN ISO 13485:2016
	EN 13612:2002	EN ISO15223-1:2012	EN ISO 18113-2:2011
	EN 1041:2008	EN ISO 18113-1:2011	EN ISO 18113-3:2011
	IEC 61010-1:2010	IEC 61010-2-081:2015	IEC 61010-2-101:2015
	IEC 61326-1:2013	IEC 61326-2-2:2013	

Signatory representative declares herein the above mentioned device meets the basic requirements of the European Parliament and the Council's in vitro diagnostic medical devices directive: 98/79/EC Annex III. This declaration of conformity is based on European Parliament and the Council's 98/79/EC directive Annex III. The compiled technical file and quality system document according to 98/79/EC directive Annex III are testified and the quality system certificate has issued by TÜV Rheinland (Shanghai) Co., Ltd.

General Manager: Enben Su

Nha Trang, 20th, Jul, 2019

(place and date of issue)

(name and signature or equivalent
marking of authorized person)



Certificate of Registration

QUALITY MANAGEMENT SYSTEM - ISO 13485:2016

This is to certify that: Getein Biotech, Inc.
No.9 Bofu Road
Luhe District
Nanjing
Jiangsu
211505
China

基蛋生物科技股份有限公司
中国
江苏省
南京市
六合区
沿江工业开发区
博富路9号
邮编: 211505

Holds Certificate No: **MD 728432**

and operates a Quality Management System which complies with the requirements of ISO 13485:2016 for the following scope:

Design & Development, Manufacture and Distribution of Chemiluminescence Immunoassay, Biochemistry Assay, Point of Care Assay (including Colloidal Gold Assay, Immunofluorescence Assay, Dry Chemistry Assay). Design & Development, Manufacture and Distribution of Analyzers in use of Chemiluminescence Immunoassay, Biochemistry Assay, Point of Care Assay (including Colloidal Gold Assay, Immunofluorescence Assay, Dry Chemistry Assay).
研发, 生产和销售化学发光法试剂, 生化试剂, 即时诊断 (包括胶体金法, 免疫荧光法, 干式化学法) 试剂。
研发, 生产和销售用于化学发光法试剂, 生化试剂, 即时诊断 (包括胶体金法, 免疫荧光法, 干式化学法) 试剂配套使用的分析仪。



For and on behalf of BSI:

Gary E Slack, Senior Vice President - Medical Devices

Original Registration Date: 2020-05-29

Latest Revision Date: 2020-07-22

Effective Date: 2020-07-26

Expiry Date: 2023-07-25

Page: 1 of 1



...making excellence a habit.™

CERTIFICATE

Getein Biotech

hereby certifies

Mr. Vitalie Goreacii

from Sanmedico SRL.

Completion of Getein Products Technical and Operational Training
& Qualification of After-sales Service

基蛋生物科技股份有限公司
GETEIN BIOTECH, INC.



Cardiac
Markers

Coagulation
Markers

Diabetes
Mellitus

Inflammation

Thyroid
Function

Metabolic
Marker

Renal
Function

Tumor
Markers

Reproduction
/Fertility

Infectious
Disease



OPTIMIZED POINT-OF-CARE SOLUTION
MAKING TEST EASY

Getein1100

Immunofluorescence Quantitative Analyzer



Getein1100

Immunofluorescence Quantitative Analyzer



HIGHLY EFFICIENT & ACCURATE

Advanced fluorescence immunoassay

Multiple quality control



REAL-TIME AND RAPID TEST


One-step test

3-15 min/test

5 sec/test for multiple tests

OPERATION MODES

Inside Mode (single sample rapid test mode)

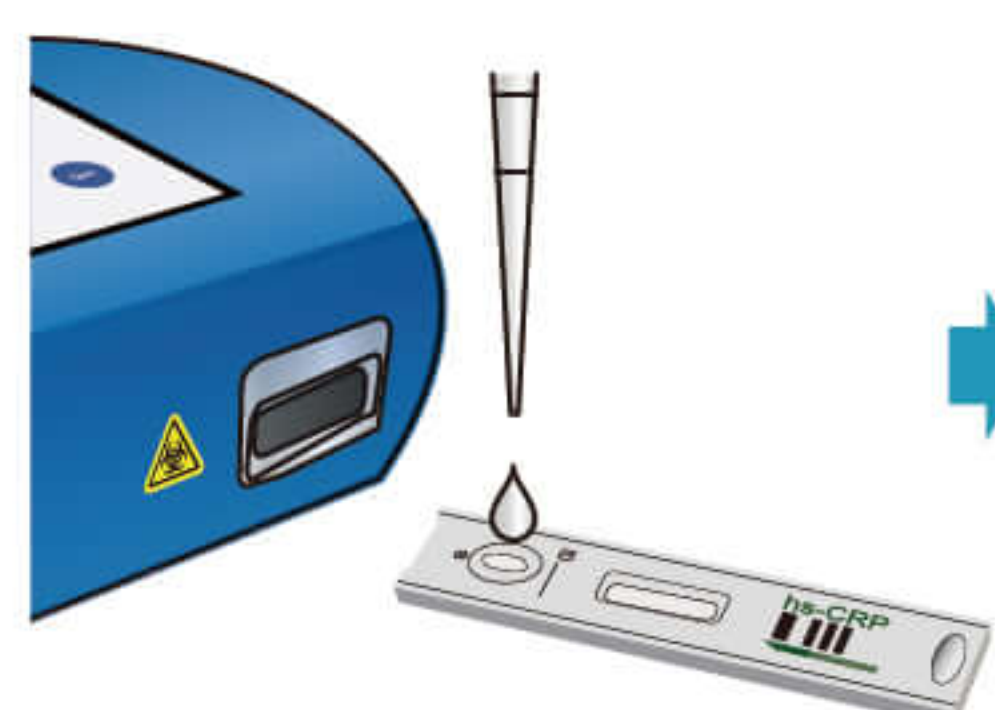

Sample Dispense



Test Card Insert




Click "Start" Icon




Result Show and Print

Quick mode (mass samples rapid test mode)

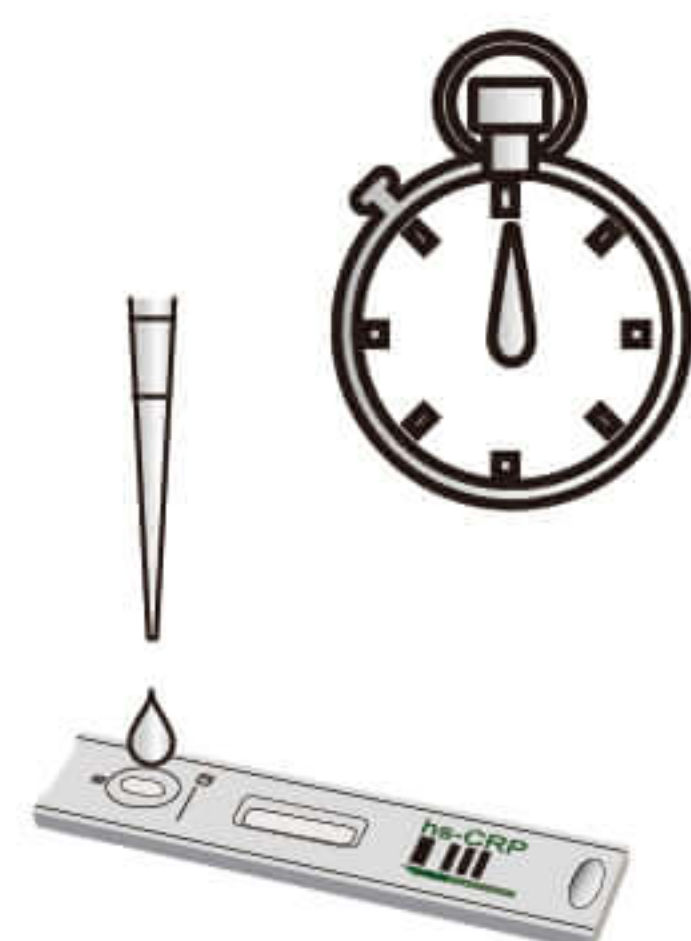

Sample Dispense

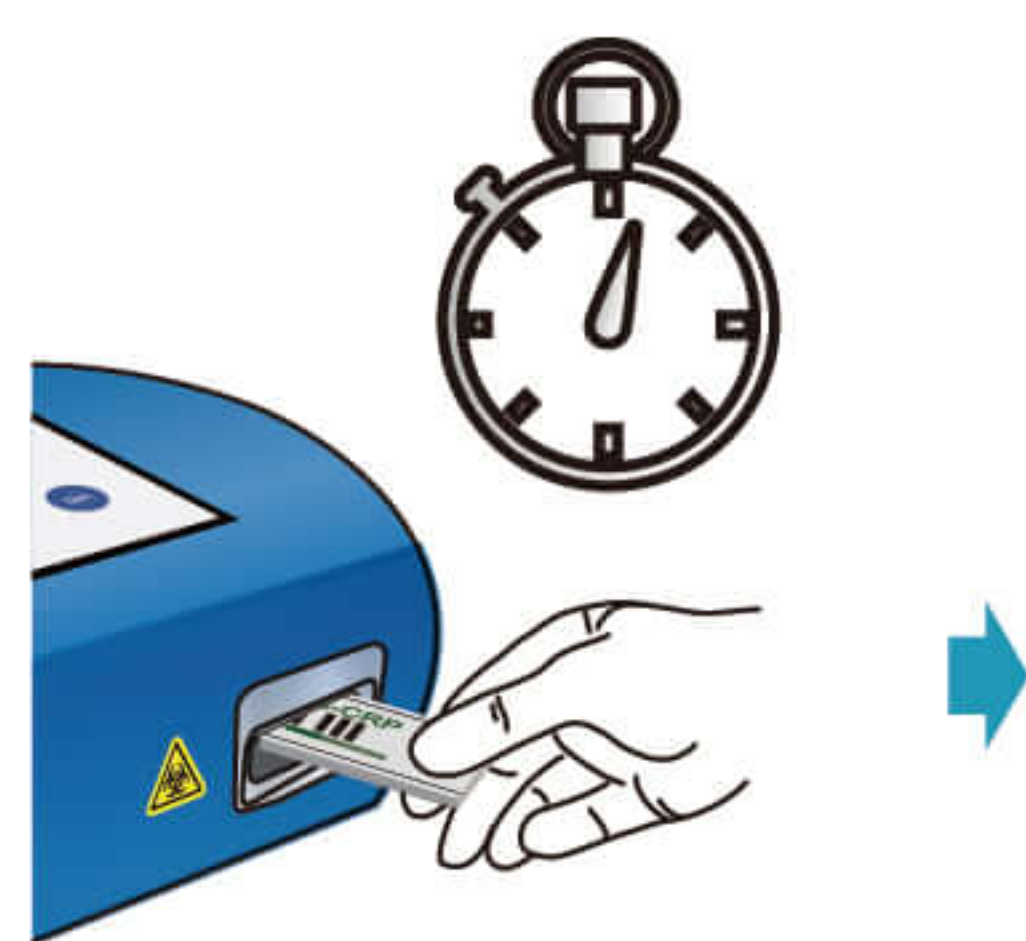

Timing the Reaction Manually



Click "Start" Icon



Result Show and Print



CONVENIENT OPERATION

RFID card calibration

Keyboard and mouse connectivity through USB port

Handwriting input available

Continuous test for 3 hours with lithium battery




USER-FRIENDLY INTERFACE

Android system

7 inch touch screen

FRONT VIEW

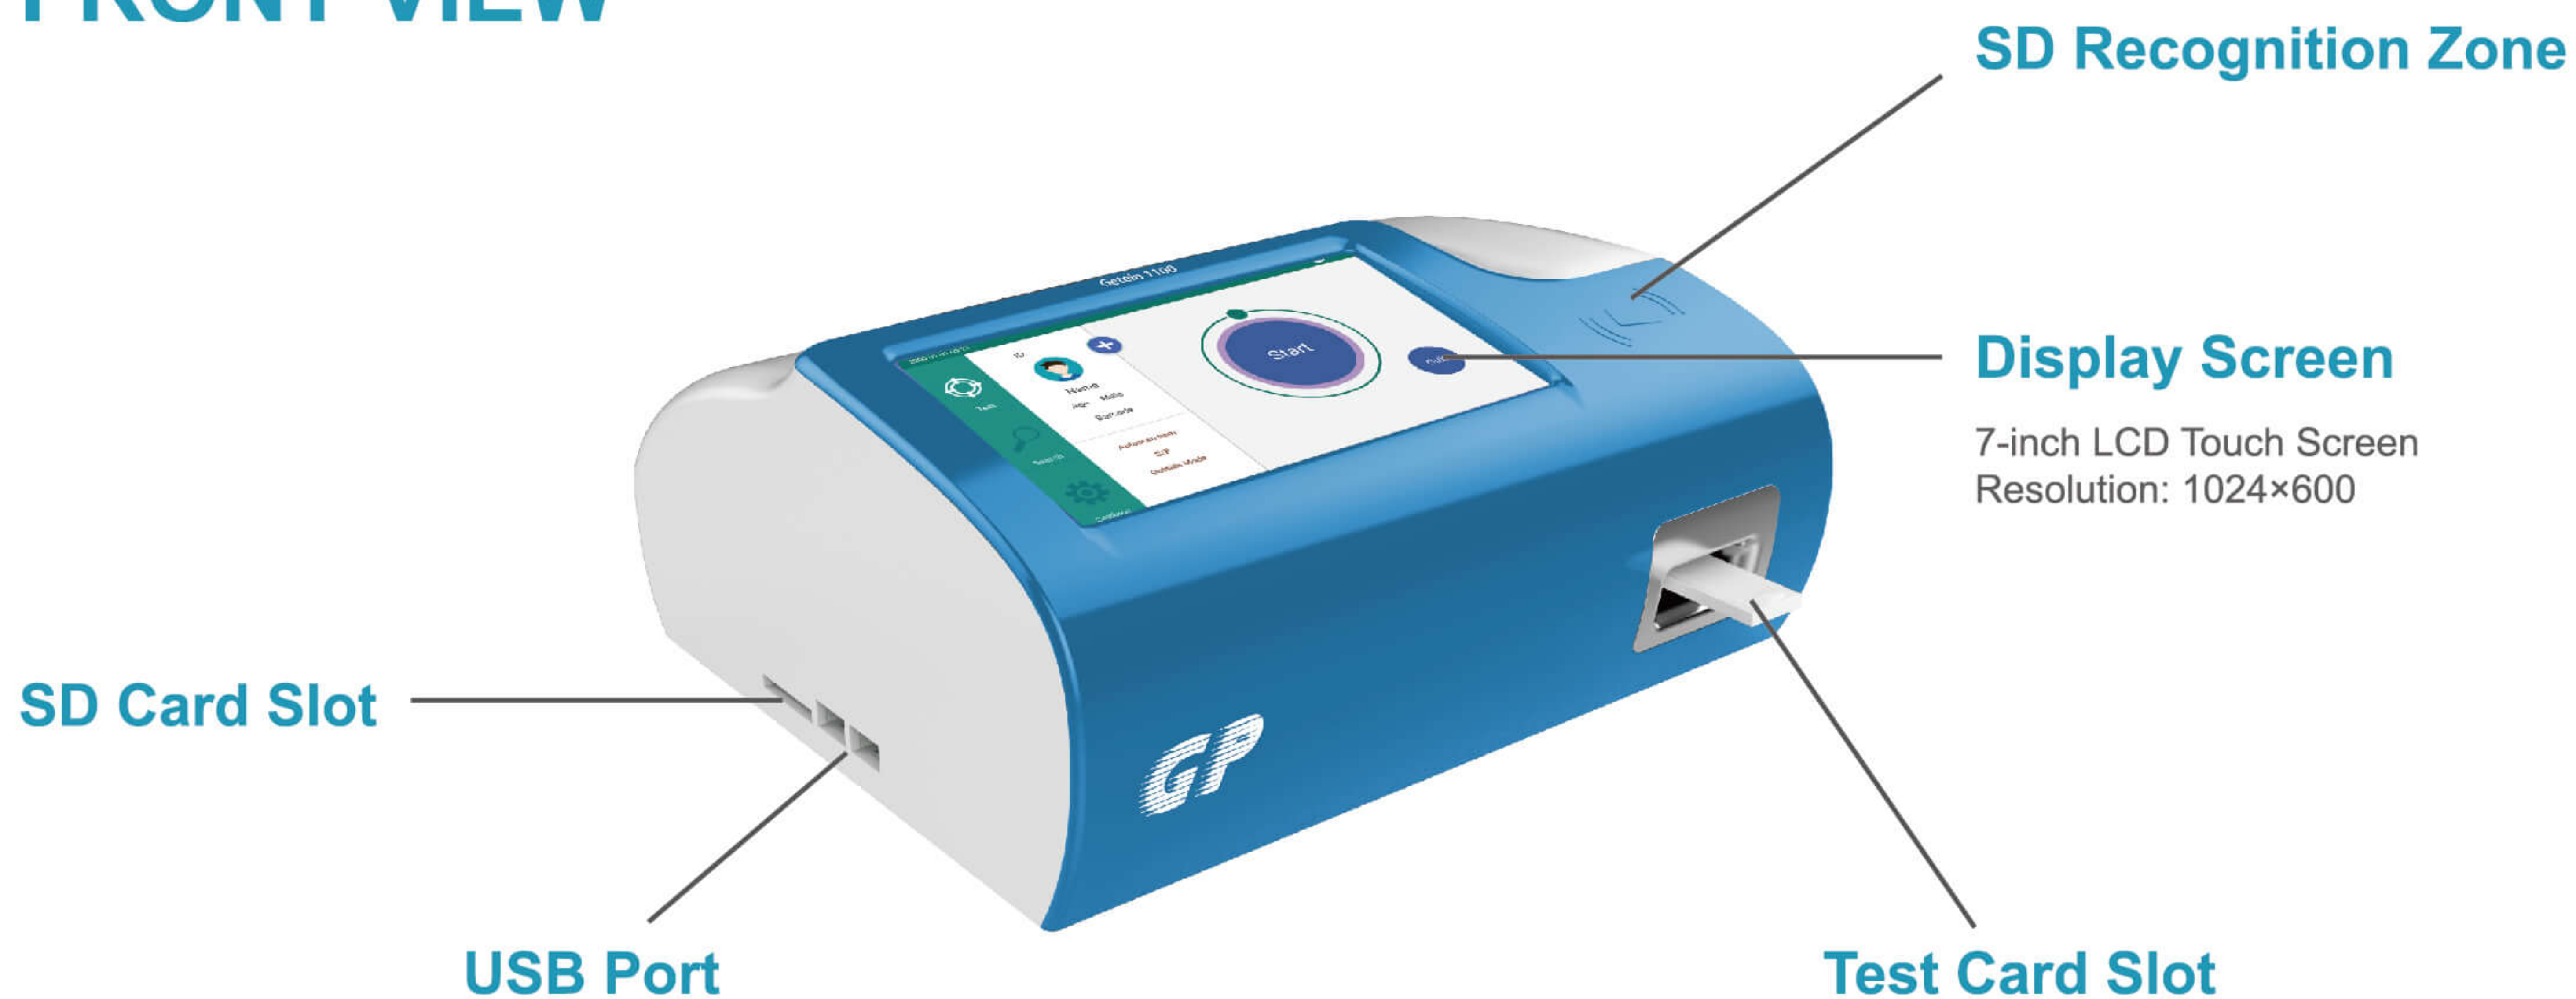



PORTABLE DESIGN

Small in size: 261 ×241 ×115 mm

Light in weight: 2.0 kg



LARGE MEMORY

Up to 10,000 results storage capacity

TECHNICAL PARAMETERS

Methodology	Immunofluorescence	Screen	7 inch touch screen
Result	Quantitative	Power Supply	100-240 V~50 Hz/60 Hz, 60 VA
Sample Type	WB, plasma, serum, urine, Stool, Nasal swab, Saliva, Capillary blood	Working Environment	Temperature: 10-35℃ Relative humidity ≤70% Air pressure 70.0~106.0 kpa
Storage Capacity	10000 data	Dimension	261 mm×241 mm×115 mm (D×W×H)
Language	English/Chinese/Spanish/Portuguese	Weight	2.0 kg

TEST ITEMS

Cat. #	TEST ITEMS	DISEASES	CUT-OFF VALUE	SAMPLE TYPES	MEASURING RANGE	SAMPLE VOLUME	REACTION TIME	QUALIFICATION	
Cardiac Markers									
IF1001	cTnI	Myocardial infarction	0.1 ng/mL	S/P/WB	0.1-50.0 ng/mL	100 µL	10 min	NMPA	CE
IF1089	BNP	Heart failure	100.0 pg/mL	P/WB	5.0-5000.0 pg/mL	100 µL	10 min	NMPA	CE
IF1002	NT-proBNP	Heart failure	300 pg/mL	S/P/WB	100-35000 pg/mL	100 µL	10 min	NMPA	CE
IF1005	CK-MB/cTnI/Myo	Myocardial damage /infarction	CK-MB: 5.0 ng/mL cTnI: 0.1 ng/mL Myo: 70 ng/mL	S/P/WB	2.5-80.0 ng/mL 0.1-50.0 ng/mL 30.0-600.0 ng/mL	100 µL	10 min	NMPA	CE
IF1012	CK-MB/cTnI	Myocardial damage /infarction	CK-MB: 5.0 ng/mL cTnI: 0.1 ng/mL	S/P/WB	2.5-80.0 ng/mL 0.1-50.0 ng/mL	100 µL	10 min	CE	
IF1014	H-FABP	Myocardial damage	6.36 ng/mL	S/P/WB	1.0-120.0 ng/mL	100 µL	3 min	NMPA	CE
IF1016	CK-MB/cTnI/H-FABP	Myocardial damage /infarction	CK-MB: 5.0 ng/mL cTnI: 0.1 ng/mL H-FABP: 6.36 ng/mL	S/P/WB	2.5-80.0 ng/mL 0.1-50.0 ng/mL 2.0-100.0 ng/mL	100 µL	10 min	NMPA	CE
IF1018	CK-MB	Myocardial injury	5.0 ng/mL	S/P/WB	2.5-80.0 ng/mL	100 µL	10 min	CE	
NEW IF1078	ST2	Heart failure	35.0 ng/mL	S/P/WB	3.1-200.0 ng/mL	100 µL	10 min	CE	
Coagulation Markers									
IF1006	D-Dimer	Venous thromboembolism	0.5 mg/L	P/WB	0.1-10.0 mg/L	100 µL	10 min	NMPA	CE
Inflammation									
IF1003	hs-CRP+CRP	Cardiovascular inflammation /normal inflammation	3 mg/L 10 mg/L	S/P/WB/ Fingertip blood	0.5-200 mg/L	10 µL	3 min	NMPA	CE
IF1007	PCT	Sepsis, bacterial infection	0.1 ng/mL	S/P/WB	0.1-50.0 ng/mL	100 µL	15 min	NMPA	CE
IF1015	PCT/CRP	Sepsis, bacterial infection	PCT: 0.1 ng/mL CRP: 3.0 mg/L	S/P/WB	0.1-50.0 ng/mL 0.5-200.0 mg/L	100 µL	15 min	NMPA	CE
IF1044	SAA	Bacterial/Virus infection	10.0 mg/L	S/P/WB/ Fingertip blood	5.0-200.0 mg/L	10 µL	5 min	NMPA	CE
IF1090	SAA/CRP	Neonatal sepsis, Bacterial/virus infection	SAA: 10.0 mg/L CRP: 10.0 mg/L	S/P/WB/ Capillary blood	5.0-200.0 mg/L 0.5-200.0 mg/L	10 µL	5 min	NMPA	CE
IF1088	IL-6	Acute inflammation	7.0 pg/mL	S/P/WB/ Peripheral blood	1.5-4000.0 pg/mL	100 µL	15 min	CE	
Renal Function									
IF1008	CysC	Acute and chronic renal diseases	0.51-1.09 mg/L	S/P/WB	0.5-10.0 mg/L	10 µL	3 min	NMPA	CE
IF1009	mAlb	Diabetic nephropathy, hypertensive nephropathy	20.0 mg/L	Urine	10.0-200.0 mg/L	100 µL	3 min	NMPA	CE
IF1010	NGAL	Acute kidney injury	Serum: 200 ng/mL Urine: 100 ng/mL	S/Urine	50-5000 ng/mL	10 µL	10 min	NMPA	CE
IF1011	β ₂ -MG	Acute and chronic kidney diseases/tumours	0.8-3.0 mg/L	S/P/WB	0.5-20.0 mg/L	10 µL	3 min	NMPA	CE
Diabetes Mellitus									
IF1017	HbA1c	Diabetes mellitus	3.8%-5.8%	WB	2%-14%	10 µL	5 min	NGSP NMPA IFCC	CE
Metabolic Marker									
IF1031	25-OH-VD	Osteomalacia, osteoporosis	30.0-50.0 ng/mL	S/P	8.0-70.0 ng/mL	40 µL	15 min	NMPA	CE
Thyroid Function									
IF1024	TSH	Thyroid malfunction	0.27-4.20 µIU/mL	S/P	0.10-50.00 µIU/mL	100 µL	15 min	NMPA	CE
IF1022	T3	Hyperthyroidism, hypothyroidism	1.30-3.10 nmol/L	S/P	0.30-10.00 nmol/L	40 µL	15 min	CE	
IF1023	T4	Hyperthyroidism, hypothyroidism	59.0-154.0 nmol/L	S/P	5.4-320.0 nmol/L	40 µL	15 min	CE	
IF1067	fT3	Hyperthyroidism, hypothyroidism	3.1-6.8 pmol/L	S/P	0.4-50.0 pmol/L	100 µL	15 min	CE	
IF1068	fT4	Hyperthyroidism, hypothyroidism	12.0-22.0 pmol/L	S/P	0.3-100.0 pmol/L	100 µL	15 min	CE	

Cat. #	TEST ITEMS	DISEASES	CUT-OFF VALUE	SAMPLE TYPES	MEASURING RANGE	SAMPLE VOLUME	REACTION TIME	QUALIFICATION
Reproduction/Fertility								
IF1013	HCG+β	Fertility	5.1 mIU/mL	S/P	5-100000 mIU/mL	100 μL	10 min	NMPA CE
IF1055	LH	Homeostasis fertility regulation	Refer to User Manual	S/P	0.2-150.0 mIU/mL	100 μL	15 min	CE
IF1056	FSH	PCOS, infertility evaluation and pituitary disorders	Refer to User Manual	S/P	0.2-150.0 mIU/mL	100 μL	15 min	CE
IF1066	AMH	Fertility, PCOS, gonadal function, precocious/late puberty	Refer to User Manual	S/P	0.10-20.00 ng/mL	200 μL	15 min	CE
IF1048	PRL	Infertility, gonadal disorders	Refer to User Manual	S/P	0.50-200.0 ng/mL	100 μL	15 min	CE
IF1071	Prog	Infertility, evaluation of ovulation	Refer to User Manual	S/P	0.10-40.00 ng/mL	100 μL	15 min	CE
Tumor Markers								
IF1053	tPSA	Prostate cancer	4.0 ng/mL	S/P	0.50-100.00 ng/mL	100 μL	15 min	
IF1072	fPSA	Prostate cancer	1.0 ng/mL	S/P	0.10-30.00 ng/ml	100 μL	10 min	
IF1050	AFP	Liver cancer, cancer of ovaries or testicles, etc.	7.0 ng/mL	S/P	2.0-500.0 ng/mL	100 μL	15 min	CE
IF1051	CEA	Cancer marker: colon cancer etc.	4.7 ng/mL	S/P/WB	2.0-500.0 ng/mL	100 μL	15 min	CE
Infectious Disease								
IF1057	Anti-HCV	Hepatitis C	1 S/CO	S/P	1.00-20.00 S/CO	100 μL	15 min	
IF1058	Anti-TP	Syphilis	1 S/CO	S/P	1.00-50.00 S/CO	100 μL	15 min	CE
IF1059	Anti-HIV	AIDS	1 S/CO	S/P	1.00-1000.00 S/CO	100 μL	15 min	
IF1064	HBsAg	Hepatitis B	1 IU/mL	S/P	1.00-100.00 IU/mL	100 μL	15 min	
NEW IF1063	Anti-HBs	Hepatitis B	10.00 mIU/mL	S/P/WB	10.00-1000.00 mIU/mL	100 μL	15 min	
IF1084	2019-nCoV IgM/IgG	COVID-19	1 COI	S/P/WB		100 μL	10 min	CE
NEW IF1091	SARS-CoV-2 Antigen	COVID-19	1 COI	Nasal swab/Saliva		100 μL	15 min	CE
NEW IF1092	SARS-CoV-2 Total Antibody/Neutralizing Antibody	COVID-19	Refer to User Manual	S/P/WB		100 μL	10 min	CE
NEW IF1095	SARS-CoV-2 Neutralizing Antibody	COVID-19	Refer to User Manual	S/P/WB		100 μL	10 min	
IF1047	<i>H. pylori</i>	<i>H. pylori</i> infection	5 ng/mL	Stool	1-200 ng/mL	150 mg	10 min	CE
Others								
NEW IF1077	Ferritin	Anemia/tumors	Male: 30-400 ng/mL Female: 13-150 ng/mL	S/P	0.50-2000.00 ng/mL	100 μL	15 min	CE
NEW IF1069	Total IgE	Allergic disorders	Refer to User Manual	S/P/WB	1.00-2000.00 IU/mL	100 μL	15 min	CE

Coming Soon: FOB, ASO, RF, anti-CCP, Folate...



Add: No.9 Bofu Road, Luhe District, Nanjing, 211505, China
Tel: +86-25-68568508/68568594
Fax: +86-25-68568500
E-mail: sales@getein.com.cn; overseas@getein.com.cn
Web: en.bio-gp.com.cn



FSC CE NMPA NGSP IFCC IVD

