



KONFORMITÄTSERKLÄRUNG

DECLARATION OF CONFORMITY

Doc#022/06-2014

Wir / We

TECO Medical Instruments Production and Trading GmbH

Name des Herstellers / Manufacturer's name

Dieselstrasse 1, D-84088 Neufahrn NB

Anschrift / Address

erklären in alleiniger Verantwortung, dass unsere im beigefügten Anhang (2 Seiten) spezifizierten Produkte wie folgt gemäß der Richtlinie für In-vitro-Diagnostika Medizinprodukte 98/79/EC klassifiziert sind:

declare under our own responsibility, that our products specified in the enclosed addendum (2 pages) classified as follows according to the directive on in vitro diagnostic medical devices 98/79/EC:

Übrige Produkte – Reagenzien für In-vitro-Diagnostika Other Products – Reagents for in vitro diagnostic

Allen anwendbaren Anforderungen der folgenden Richtlinien entsprechen: *Meet all applicable requirements of:*

Richtlinie 98/79/EG über In-vitro-Diagnostika
klassifiziert gemäß Artikel 9 als "alle anderen Produkte"

*Directive 98/79/EC on in-vitro-diagnostic medical devices
classified according to article 9 as „all other products“*

Das QM-System des Herstellers ist zertifiziert nach:

EN ISO 13485:2016

The QM-system of the manufacturer is certified for:

EN ISO 13485:2016

Die vorstehende Konformitätserklärung ist gültig für alle Chargen dieser Produkte, die nach dem Datum der Unterzeichnung in Verkehr gebracht wurden.

The above mentioned declaration of conformity is valid for all lots of this product, which are distributed after the date of signature.

Konformitätsbewertungsverfahren:

Conformity assessment procedure:

Gemäß Anhang III der Richtlinie 98/79/EG

According to Annex III of Directive 98/79/EC

Ort und Datum der Unterzeichnung:
Place and date of issue:

Neufahrn, 26.03.2019
Neufahrn, March 26, 2019


Christian Hötzel
General Manager



KONFORMITÄTSERKLÄRUNG – DECLARATION OF CONFORMITY

Übrige Produkte – Reagenzien für In-vitro-Diagnostika
Other products – Reagents for in vitro diagnostic

PT		
A0230-010	TEClot PT-S	5x2ml
A0230-040	TEClot PT-S	10x4ml
A0230-100	TEClot PT-S	10x10ml
A0260-020	TEClot PT-B Kit-20	Kit
A0260-050	TEClot PT-B Kit-50	Kit
PTT		
A0300-025	TEClot APTT-S, Kt-25	Kit
A0300-050	TEClot APTT-S, Kit-50	Kit
A0320-050	TEClot APTT-S	10x5ml
A0320-100	TEClot APTT-S	10x10ml
A0350-050	CaCl ₂ , 0,025M	10x5ml
A0350-100	CaCl ₂ , 0,025M	10x10ml
Fibrinogen		
A0501-010	TEClot FIB Kit-10	5x2ml
A0501-025	TEClot FIB Kit-25	5x5ml
A0511-020	TEClot FIB	10x2ml
A0511-050	TEClot FIB	10x5ml
A0590-125	IBS Buffer	1x125ml
TT		
A0401-020	TEClot TT	10x2ml
Protein S		
A0600-002	TEClot PS Kit	Kit
Lupus Anticoagulant		
A0700-020	TEClot LA Screen	10x2ml
A0800-010	TEClot LA Confirm	10x1ml
Factor V Leiden		
A0900-004	TEClot PCA Ratio Kit	Kit
Chromogenic Tests		
C1000-010	TEChrom AT (anti-Xa) Kit-10	Kit
C1010-020	TEChrom AT (anti-Xa) liquid	Kit
C1100-012	TEChrom PC Kit	Kit
Semiquantitative D-Dimer		
D2050-000	D-Dimer Agglutination Kit	Kit

KONFORMITÄTSERKLÄRUNG – DECLARATION OF CONFORMITY

Übrige Produkte – Reagenzien für In-vitro-Diagnostika
Other products – Reagents for in vitro diagnostic

Quantitative D-Dimer		
D2000-002	Dimex D-Dimer Kit-50	Kit
D2000-005	Dimex D-Dimer Kit-100	Kit
D2010-012	Red D-Dimer Kit	Kit
D2020-005	Blue D-Dimer LC Kit-65	Kit
D2020-010	Blue D-Dimer LC Kit-130	Kit
Control Plasma		
P6001-010	Tecontrol N	10x1ml
P6101-010	Tecontrol A	10x1ml
P6201-010	Tecontrol A+	10x1ml
P7100-005	TEControl LA positive	5x1ml
Reference Plasma		
P8001-010	TECal N	10x1ml
P8200-005	TECal DD	5x1ml
Deficient Plasma		
P5001-010	Deficient Plasma II	10x1ml
P5101-010	Deficient Plasma V	10x1ml
P5201-010	Deficient Plasma VII	10x1ml
P5301-010	Deficient Plasma VIII	10x1ml
P5401-010	Deficient Plasma IX	10x1ml
P5501-010	Deficient Plasma X	10x1ml
P5601-010	Deficient Plasma XI	10x1ml
P5701-010	Deficient Plasma XII	10x1ml



KONFORMITÄTSERKLÄRUNG

DECLARATION OF CONFORMITY

Doc#100/07-2021

Wir / We

TECO Medical Instruments Production and Trading GmbH

Name des Herstellers / Manufacturer's name
Dieselstrasse 1, 84088 Neufahrn, Germany
Anschrift / Address

erklären in alleiniger Verantwortung, dass die unten gelisteten IVD Zubehör Produkte:
declare under our own responsibility, that the IVD accessories products, listed below:

Doppelküvette / <i>Double cuvette</i>	Ref. 19 000 02
Einzelküvette / <i>Single cuvette</i>	Ref. 20 000 02, 24 100 00
4-fach Küvette / <i>Cuvette 4 pos/ea</i>	Ref. 80 521 10
6-fach Küvette / <i>Cuvette 6 pos/ea</i>	Ref. 80 560 00
6-fach Küvette (micro) / <i>Cuvette 6 pos/ea (micro)</i>	Ref. 80 570 00

allen anwendbaren Anforderungen folgender Richtlinien entsprechen: *meet all applicable requirements of:*

1. Richtlinie 98/79/EG über In-vitro Diagnostika und ihrem Zubehör, klassifiziert gemäß Artikel 9 als: "alle anderen Produkte"- im Sinne von Zubehör zu In vitro Diagnostika gemäß Artikel 1.

1. Directive 98/79/EC on In-vitro diagnostic medical devices and their accessories, classified according to article 9 as: "all other products" – and in term of accessories for in vitro diagnostics according to article 1.

2. Richtlinie 2011/65/EU (RoHS III)

2. Directive 2011/65/EU (RoHS III)

Das QM-System des Herstellers ist zertifiziert nach:

The QM-system of the manufacturer is certified for:

EN ISO 13485:2016

EN ISO 13485:2016

Konformitätsbewertungsverfahren gemäß:

Conformity assessment procedure according to:

Gemäß Anhang III der Richtlinie 98/79/EG

According to Annex III of Directive 98/79/EC

Ort und Datum der Unterzeichnung:
Place and date of issue:

Neufahrn, 27.07.2021
Neufahrn, July 27, 2021

Matthias Dieckmann
General Manager



TECO

MEDICAL INSTRUMENTS
PRODUCTION+TRADING GMBH

Dieselstraße 1
D-84088 Neufahrn N.B.
fon: +49-8773/707 80-0
fax: +49-8773/707 80-29

Neufahrn, 26/04/2018

TO WHOM IT MAY CONCERN

We confirm that the instruments Coatron X Eco, Coatron X Pro and Coatron X Top have a closed cuvette system. Cuvettes have to be purchased with voucher identification code from TECO GmbH.



Christian Hoetzl
General Manager
TECO Germany

CERTIFICATE

TECO

EN ISO 13485:2016

DEKRA Certification GmbH hereby certifies that the organization

TECO Medical Instruments, Production + Trading GmbH

Scope of certification:

Design, development, manufacturing, storage and sales of coagulation instruments and in-vitro-Diagnostic reagents used in the hemostaseology and coagulation

Certified location:

Dieselstraße 1, 84088 Neufahrn, Germany

has established and maintains a quality management system according to the above mentioned standard. The conformity was adduced with audit report no. 50788-Z5-00.

Certificate registration no.:	50788-14-01	Certificate valid from:	2019-05-31
Validity of previous certificate:	2019-05-30	Certificate valid to:	2022-05-30



Ruth Delbeck-Bayer
DEKRA Certification GmbH, Stuttgart, 2019-05-31





Quality Management

We are certified

Voluntary participation in regular monitoring according to ISO 9001:2008



MEDICAL INSTRUMENTS
PRODUCTION+TRADING GMBH

Dieselstraße 1
D-84088 Neufahrn N.B.
fon: +49-8773/707 80-0
fax: +49-8773/707 80-29

TO WHOM IT MAY CONCERN

To any governmental departments,
registration and/or trade offices
in Moldova

Distribution / Service Authorisation for the years 2019 - 2023

This letter confirms that company

SANMEDICO SRL

Str. Petricani 88/1, oficiul 10
Chisinau - Rep. Moldava MD-2059
MOLDOVA
Phone: 00373-22-623032
Email: sanmedico.office@gmail.com

is the **authorized, exclusive and sole** representative of **TECO Medical Instruments, Production + Trading GmbH, Dieselstrasse 1, 84088 Neufahrn i.NB, Germany**, for the territory of **Moldova**, only for all TECO products listed below. **Sanmedico** may participate in public and privat tenders, providing sales to all TECO customers in the territory. We as manufacturer, certify that our **warranty and service** is duly passed to the purchaser through **Sanmedico** for the price, delivery schedules, and the specifications of the published literature, catalogues and fully covering the commodities offered.

Validity:

August 20th, 2019 to December 31st, 2023

Termination:

Confirmation ends automatically on Dec. 31st of 2023
and must be then renewed.

TECO products:

- Coatron X (Eco, Pro, Top) new manual Coagulometers (1, 2 and 4 channel)
- Coatron A4, A6, A6 Plus Fully automated Coagulometers (4 and 6 channel)
- Complete line of Hemostasis Reagents, Consumables and Spareparts

This document is signed in Neufahrn, Germany, on August 20th, 2019.

TECO Medical Instruments, Production + Trading GmbH



MEDICAL INSTRUMENTS
PRODUCTION+TRADING GMBH
Dieselstraße 1
D-84088 Neufahrn N.B.
fon: +49-8773/70780-0

Christian Hoetzl
General Manager



Quality Management

We are certified

Voluntary participation in regular monitoring according to ISO 9001:2008



TECO

MEDICAL INSTRUMENTS
PRODUCTION+TRADING GMBH

Dieselstraße 1

D-84088 Neufahrn N.B.

fon: +49-8773/707 80-0

fax: +49-8773/707 80-29

CERTIFICATE

for: **Mr. Vitalie Goreacii**

Company: **Sanmedico SRL**
Str. Petricani 88/1, oficiul 10
Chisinau - Rep. Moldova MD-2059
MOLDOVA

have participated with success at the intensive training session:

Application and technical training for following instruments:

- **Coatron X series**
 - **Installation**
 - **Application**
 - **General use, also in combination with TECAM Software**
 - **Technical and After Sales Service**

Supervisors: **Mr. Chr. Hoetzi and Mrs. Wendy Guo**

Place of Training: **TECO – Germany**

Date: **November 18th, 2019**


Christian Hoetzi
General Manager



TOP
INNOVATION
2017 - 2018

Clotting
Chromogenic
Immunturbidimetric

Coatron

Semi-automated
Coagulation Analyzer Series

With 1, 2 or 4 optical channels



TECO

Innovation in Coagulation

A new area of manual and semi-automated Coagulation Analyser rise up

The Coatron X instrument line is a consequent continuation in the development of the Coatron product line. Over 25 years in experience and innovation is the reference for our new Coatron X instrumentation line.

The unique detection principle in combination with the high-level analytical algorithm calculates exact, precise and reproducible results.

Easy in operation – self instructing user dialogue - reliable

Highest optical resolution, enlarged optic range, smallest sample and reagent volume

0.1 mOD, 0 - 3800 mOD, just with 75 µL sample and reagent volume

Complete optical analysis

No further parts required, like balls, stirrers etc.

Adaptation of the light level

Automatic light level adjustment of the optic channels to each sample

Exclusion of disturbance

Stray light reduction, exact temperature control, all parameter are preset

“Complete range of Coagulation Analysis with the highest standard and reliability. The new generation of Coagulation instruments with optical detection are here.”

Coatron X - product family



With 1, 2 or 4 optical channels.

www.teco-medical.com

Prepared for the daily routine and the upcoming requirements

One instrument – many possibilities

The Coatron X family is prepared to work with one, two or four channels. The built-up and functionality is specifically designed to each instrument version and requirements. The operation with the intuitive user dialogue and handling of the detection results are easy and effective. The possibility to connect the instrument to the **TECO Cloud** offers new perspective of instrument, reagent and consumables verification and handling. The precise and correct patient result is what we want to secure.



Quality is our basic demand

TECO develop and produce with qualified and specialized companies, located in Germany. High reliability, nearly maintenance free instruments are our benefit. Our reference is 25 years, in worldwide laboratories, with satisfied users.



TECO Cloud Services – A strong data bank and application service behind

All instrument versions of the Coatron X family are connectable via Bluetooth to Smart-devices, like mobile devices, tablets, etc. with a specific APP or direct access to the TECO Cloud Services.



Coatron	Eco	Pro	Top
General			
Dimensions	230 x 148 x 94 mm (l, b, h)		
Display	Colored touch display 4.3"		
Pre-warm temperature	37°C		
Pre-warm cuvettes (pcs.)	10	20	20
Pre-warm reagent 24mm (pcs.)	1	1	1
Pre-warm reagent 22mm (pcs.)	2	2	2
Pre-warm reagent 11mm (pcs.)	2	2	2
Reagent mixing position	-	1	1
Power values	110-240Vac, 50-60Hz / 5Vdc, 3.3A		
Interfaces			
RS232 (2x)	Printer, Barcode reader		
USB (2x)	Network, Firmware update		
Bluetooth	TECO Cloud, App		
Optic / tests			
Optic channels	1	2	4
Wavelength (nm)	620 (red)	405 (UV)	405 (UV)
Global Coag. tests	PT, APTT, TT, FIB		
Specific Coag. tests	-	individual factors	
Chromogenic Coag. tests	-	AT, PC	
Latex based tests	D-Dimer		
Whole blood tests	PT-B	-	



The details make the difference

Coatron X

The remarkable details in every single component is achieved by selecting of premium suppliers.

The performance of a high level instrument is strongly depending on the concept in general and the perfect usability to reach the requirements of a modern laboratory analyser.

Priority No. 1 was to get a daily routine reliability and easy-to-use operation.

Software and connection possibilities


With the Coatron X product family starts a new time line in analysis management and service maintenance. Operation via intuitive, colored touchscreen, as well patient result management are perfectly optimized.

Operation details

Coatron	Eco	Pro	Top
Operation			
Touchscreen 4.3"	✓	✓	✓
Real time clock	✓	✓	✓
Stopwatch	✓	✓	✓
Language selection	✓	✓	✓
Interfaces			
USB to LIS	✓	✓	✓
Network to LIS (TECAM software required)	✓	✓	✓
Management			
Test calibration	✓	✓	✓
Tracking to Pat.ID, Patient ID, Sample ID or Auto ID	✓	✓	✓
Automatic optic start (no Starterpipette required)	✓	✓	✓
Double determination	✗	✓	✓
Sample management (ID)	✗	✓	✓
Reagent management (ID) (lot und expiry)	✗	✓	✓
Internal result databank	✗	✓	✓

Patient identification with barcode

optional

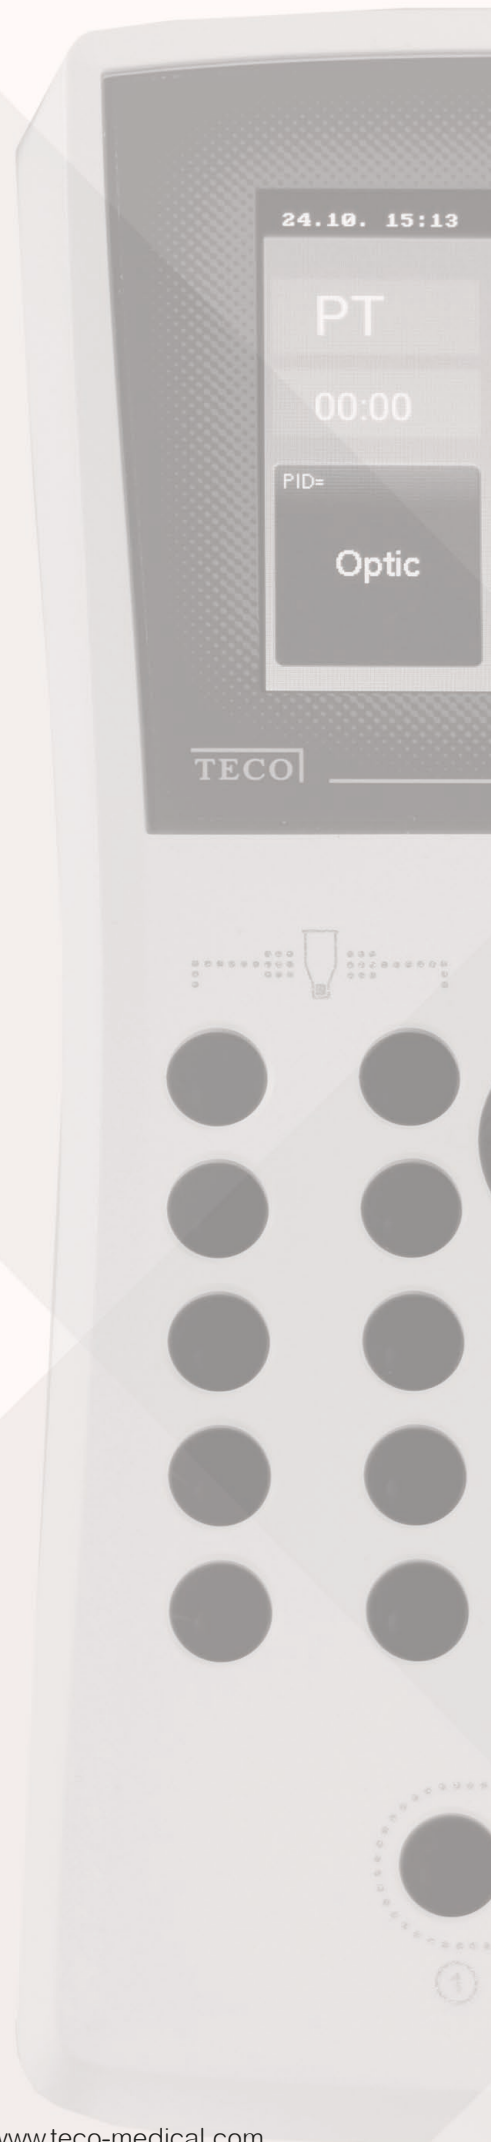



Intuitive operation and control

Clear and easy to operate user dialogue with a high quality colored touchscreen

- Direct usable
- Short learning phase
- Logic, intuitive operation
- Reliable touchscreen surface
- Quick touch response



For small and mediate laboratory requirements

Concept is suitable for daily routine work in Coagulation laboratories and hospitals

- Three different versions available, depending on number of samples per day
- In maximum up to 4 optic channels available

Interfaces

RS232 (2x)

- For external serial printer and external barcodereader

LIS/USB

Bluetooth



Integrated barcode scan for reagents.





TECO Cloud Services

A strong data bank and application service behind

All instrument versions of the Coatron X family are connectable via Bluetooth to Smart-devices, like mobile devices, tablets, etc. with a specific APP or direct access to the TECO Cloud Services.



For trading partners worldwide, please visit our web-page

TECO Medical Instruments Production + Trading GmbH
Dieselstr. 1, 84088 Neufahrn, Germany
Tel.: +49 (0) 8773 70780-0, Fax +49 (0) 8773 70780-29
info@teco-gmbh.com, www.teco-medical.com

TECO
Innovation in Coagulation



IVD

REF

A0230-010, A0230-040, A0230-100,

Intended Use

This product is used for the determination of prothrombin time (PT) in plasma according to Quick^{1,2}. The test is sensitive to the extrinsic pathway coagulation factors II, V, VII, X and fibrinogen and therefore used for oral anticoagulant therapy with Vitamin-K inhibitors like Warfarin or Marcumar and also for the quantitative determination of extrinsic coagulation factors. The PT measures the extrinsic clotting time (factor VII activation) of test plasma after the addition PT reagent.

Contents & Determinations

Product	TECLOT PT-S	TECLOT PT-S	TECLOT PT-S
Cat.No.	A0230-010	A0230-040	A0230-100
PT-S Reagent*	5x2 mL	10x4 mL	10x10 mL

Determinations

Coatlon M**	200 Det.	800 Det.	2000 Det.
Coatlon A4	100 Det.	400 Det.	1000 Det.
Coatlon A6	200 Det.	800 Det.	2000 Det.

*contains an extract of Rabbit brain with buffer, stabilizers and Calcium chloride.

**Micro method (75µL in total)

Preparation

Reconstitute with high purity water with the volume stated on the vial label.

A0230-010	A0230-040	A0230-100
2 mL	4 mL	10 mL

Let stand at room temperature with occasional swirling for at least 15 min. Then place reagent into instrument and let incubate for further 15 min. The reagent sediments and must be swirled before each testing. On Coatlon instruments, you can use a mixing bar for this.

Storage & Stability

Unopened reagents are stable until the expiration date shown on the label stored at 2°-8°C. Opened reagent:

	2-8 °C	20-25 °C	37°C
PT Reagent	5 days	36 hours	8 hours

Precautions

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV, HCV. However products from human blood should be considered as potentially infectious.

Specimen collection and storage⁴

- Obtain venous blood by clean vein puncture.
- Immediately mix 9 parts blood with 1 part 3.2% sodium citrate (0.105M) and mix well
- Centrifuge the specimen at 1500g for 10 min. (platelet < 10000/µL)
- Separate plasma after centrifugation and store in plastic or siliconised glass tube.
- Use plasma within 4 hours, otherwise store frozen and thaw just prior to use.

Stability of plasma: 4h at 18-26°C 8h at 2-8° 30d at -20°C 6m at -70°C

Procedure**A. Automated Method: Coatlon A**

Prothrombin Time	A4	A6		A4	A6		A4	A6
PAT Patient	50µl	CP1	25µl	CP1	Incubation	0s	SENS	2
BUF IBS Buffer	0µl	P39	0µl	P79	Maxtime	120s	POINTS	4
CLR -	0µl	-	0µl	-	Unit	251	MIX	No
DP -	0µl	P00	0µl	P00	Method	Coag	Clean	0 0
R0 -	0µl	P00	0µl	P00	Math	log XY	Multi	1 3
R1 -	0µl	P00	0µl	P00	CT-Mech	No	S-Corr	0%
R2 PT Reagent	100µl	P25	50µl	P46	Deadtime	7s	T-Corr	30% - 4s

B. Manual Method: Coatlon M system

- Incubate PT reagent at 37°C for at least 10 minutes
- Pipette **25 µl of sample** into a test cuvette. Incubate at 37°C for 1-2 minutes.
- Add **50 µl of PT reagent** (37°C) and simultaneously start test.
- Record the clotting time in seconds.

For other instrument, please refer to your instrument manual for more detailed instrument specific instructions.

Expected Results

Typical seconds: 11 – 18 sec
Normal range: 70 - 130% 0.85 – 1.15 INR

However results are influenced by instruments, technique, calibration etc. Each laboratory is recommended to establish its own range on the specific instrument used.

Standardisation and Calibration

The PT result is expressed as seconds or activity (% Quick) or INR (International Normalised Ratio).

INR results:

were calculated from normal time and ISI value (international sensitivity index). First is obtained by running fresh plasma from a pool of healthy individuals. The ISI value is stated in the LOT specific certificate of analysis.

$$INR = \left(\frac{Patient\ PT}{Normal\ PT} \right)^{ISI}$$

Activity % (Quick) result:

were calculated from a calibration curve, which is prepared from reference plasma (e.g. TECAL N) and dilutions in saline solution like 0.9% NaCl₂ or TECLOT IBS buffer. At least three or more calibration points are recommended. The calibration curve must be confirmed with control plasma in normal and abnormal range.

% of normal	100%*	50%	25%	12.5%**
diluted in saline	not dil.	1+1	1+3	1+7

*The median of at least 21 healthy individuals is defined as 100%.⁵

**12.5% dilution may cause "+++" results in some cases, because the level of fibrinogen is too high diluted for optical detection.

Quality Control

TEControl or other commercial control plasma should be used for reliable quality control of performance at a frequency in accordance with good laboratory practice (GLP). TEControl can be frozen one time after reconstitution. 120-150 µl stored in closed polypropylen tubes at -20°C is stable for 30 days

Limitations

Great care must be taken to minimize variations which may occur by seemingly insignificant factors.

A. Specimen Collection. AVOID:

- Use only plastic tubes or siliconised glass.
- Delayed mixing of blood with anticoagulant.
- Contamination with tissue thromboplastin.
- Improper ratio of anticoagulant with blood.
- Hemolyzed, icteric or lipemic samples may interfere optical systems

B. Laboratory Techniques

- Perform tests at 37°C.
- Use only high purity water.
- Optimum pH is 7.0-7.5.
- ISI value is not constant within the first 30 min after reconstitution.
- Reagent sediments and must be swirled before each testing.

Performance Characteristics**Typical performance on instrument Coatlon M4**

Precision: CV% (within run) CV% (inter-runs)
Normal control < 3,0 < 5,0
Abnormal control < 3,0 < 5,0

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

References

- Quick, A.J., The Hemorrhagic Diseases and the Physiology of Hemostasis. Charles C. Thomas: Springfield, IL. 1942.
- Quick, A.J., Hemorrhagic Diseases. Lea and Febiger: Philadelphia. 1957.
- Miale, J.B., Laboratory Medicine-Hematology, 4th Edition. C.V. Mosby: St. Louis. 1972.
- National Committee for Clinical Laboratory Standards: Guidelines for the Standardized Collection, Transport and Preparation of Blood Specimens for Coagulation Testing and Performance of Coagulation Assays.
- Besselaar A M H P van den, Lewis SM, Mannucci P n Poller L. 1993. Status of present and candidate International Reference Preparations (IRP) of thromboplastin for prothrombin time. Thromb Hemostas 69: 85
- Besselaar A M H P van den. 1991. The significance of the International Normalized Ratio (INR) for oral anticoagulant therapy. H17CC 3; 146153.

Symbol keys

	Expiry date		In Vitro Diagnostica		Biological hazard		Catalogue Number		Reconstitute with dest. water		Consult accompanying documents
	Store at 2-8°C		EU conformity		Manufacturer		Lot. Number		Ready to use		Authorized Representative



Calcium Chloride 0,025M

TECO

**IVD****REF****A0350-050, A0350-100**

Intended Use

This product is used in combination with reagent TEClot APTT-S (Cat.No. A0320) to determine the APTT or also for other 25mM CaCl₂ requiring coagulation tests.

Contents & Determinations

Product	Calcium Chloride	Calcium Chloride
Cat.No.	A0350-050	A0350-100
CaCl ₂ 0.025M	10x5 mL	10x10 mL

Determinations

Coatron M	2000 Det.	4000 Det.
Coatron A	1000 Det.	2000 Det.

Preparation

Ready to use.

Storage and Stability

Unopened reagents are stable until the expiration date shown on the label stored at 2-8°C.

Opened reagent is stable for 30 days at 2-8°C in the original vial.

Precautions

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material.

Calcium Chloride Solution contains sodium azide. Sodium azide under acid conditions yields Hydrazoic acid, an extremely toxic compound. Azide compounds should be diluted with running water before being discarded. Upon disposal, azide compounds should be flushed with large volumes of water. These precautions are recommended to avoid deposits in metal pipes in which explosive conditions may develop.

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	IVD In Vitro Diagnostica	Biological hazard	REF Catalogue Number	Consult accompanying documents
Store at 2-8°C	CE EU conformity	Manufacturer	LOT Lot. Number	EC REF Authorized Representative





IVD

REF

A0350-050, A0350-100

Verwendungszweck

Wird zusammen mit dem Reagenz TEClot APTT-S (Kat. Nr. A0320) zur Bestimmung von der APTT verwendet oder auch für andere Gerinnungstests, für die 25mM CaCl₂ benötigt wird.

Inhalt und Bestimmungen

Produkt	Kalzium Chlorid	Kalzium Chlorid
Kat. Nr.	A0350-050	A0350-100
CaCl ₂ 0.025M	10x5 mL	10x10 mL

Bestimmungen

Coatron M	2000 Det.	4000 Det.
Coatron A	1000 Det.	2000 Det.

Vorbereitung

Das Reagenz ist gebrauchsfertig

Lagerung und Stabilität

Ungeöffnete Reagenzien sind bei einer Lagerung zwischen 2-8°C bis zum auf dem Etikett angegebenen Verfallsdatum haltbar.

Geöffnete Reagenzien sind bei Lagerung zwischen 2-8°C im Originalfläschchen 30 Tage haltbar.

Vorsichtsmaßnahmen

Haut- und Augenkontakt vermeiden. Schutzkleidung tragen. Abfälle unter Beachtung der vorgeschriebenen internationalen, nationalen und lokalen Bestimmungen entsorgen.

Die Calcium Chlorid Lösung enthält Natriumazid. Unter sauren Bedingungen setzt Natriumazid Hydrogenazid frei, ein höchst giftiger Wirkstoff. Azidverbindungen sollten unter laufendem Wasser gelöst werden bevor sie entsorgt werden. Diese Vorsichtsmaßnahmen werden empfohlen, um Ablagerungen in Metallrohren zu verhindern, die explosive Bedingungen entwickeln könnten.

Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produktes den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Veräußlichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter





IVD

REF

A0501-010, A0501-025, A0511-020, A0511-050

Intended Use

The TECLOT FIB is intended for the quantitative determination of fibrinogen in human plasma according to method developed by Clauss.¹ Levels of fibrinogen can increase as a result of inflammation, pregnancy or oral contraceptive use². Decreased levels can be found in certain states such as liver disease and DIC. Congenital deficiencies include afibrinogenemia (no detectable fibrinogen), hypofibrinogenemia (<1 mg/ml) and dysfibrinogenemia (abnormal fibrinogen molecule).

Contents & Preparation

Product	TECLOT FIB Kit-10	TECLOT FIB Kit-25	TECLOT FIB	TECLOT FIB
Cat.No.	A0501-010	A0501-025	A0511-020	A0511-050
Thrombin Reagent	5x2 mL	5x5 mL	10x2 mL	10x5 mL
IBS Buffer	1x125 mL	1x125 mL	-	-
TECal Normal	1x1 mL	1x1 mL	-	-
TEControl A	1x1 mL	1x1 mL	-	-

Determinations

Coatrom M*	400 Det.	1000 Det.	800 Det.	2000 Det.
Coatrom A4	200 Det.	500 Det.	400 Det.	1000 Det.
Coatrom A6	200 Det.	500 Det.	400 Det.	1000 Det.

*Micro method (75µl in total)

- Thrombin Reagent:
Contains bovine thrombin (~80NIH) with stabilizers
REF: A0501-010/A0511-020: Reconstitute with 2mL purified water
REF: A0501-025/A0511-050: Reconstitute with 5mL purified water
- IBS Buffer: Ready to use. Contains Imidazole buffered saline
- TECal Normal: Reconstitute with 1 mL purified water.
Contains citrated human plasma.
- TEControl A: Reconstitute with 1 mL purified water.
Contains citrated human plasma.



Swirl gently after reconstitution and allow standing for 15 minutes at room temperature. Mix well before use. Do not shake.

Storage & Stability

Unopened reagents are stable until the expiration date shown on the label stored at 2°-8°C. Opened reagent:

Thrombin Reagent*	2-8 °C	15-25 °C	37 °C
	12 days	5 days	24 hours
TEControl or Plasma	2-8 °C	15-25 °C	-20 °C
	8 hours	4 hours	30 days

* Reagent must be protected from UV-light and evaporation

Precautions

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV, HCV. However products from human blood should be considered as potentially infectious.

Specimen collection and storage³

- Obtain venous blood by clean vein puncture.
- Immediately mix 9 parts blood with 1 part 3.2% sodium citrate (0.105M) and mix well
- Centrifuge the specimen at 1500g for 10 min. (platelet < 10000/µL)
- Separate plasma after centrifugation and store in plastic or siliconised glass tube.
- Use plasma within 4 hours, otherwise store frozen and thaw just prior to use.

Procedure**A. Automated Method. Coatrom A**

Fibrinogen	A4	A6		A4	A6		A4	A6
PAT Patient	10µl	CP1	10µl	CP1	Incubation	0s	SENS	0
BUF IBS Buffer	90µl	P39	90µl	P79	Maxtime	120s	POINTS	4
CLR -	0µl	-	0µl	-	Unit	769	MIX	No
DP -	0µl	P00	0µl	P00	Method	Coag	Clean	1 3
R0 -	0µl	P00	0µl	P00	Math	log XY	Multi	1 1
R1 -	0µl	P00	0µl	P00	CT-Mech	Yes	S-Corr	0%
R2 Fibrinogen	50µl	P29	50µl	P49	Deadtime	3s	T-Corr	0%

B. Manual Method: Coatrom M**1. Preparation of Standard, Control and Patient Dilutions**

Standard Dilution	Plasma	IBS Buffer
1:5	200µL Standard	800µL
1:10	500µL 1:5 STD	500µL
1:20	500µL 1:10 STD	500µL
1:40	500µL 1:20 STD	500µL
Patient or Control	100µL Plasma	900µL

2. Pipette **50 µl diluted standard or patient plasma** (1:10) into a test cuvette. Prewarm at 37°C for 1-2 minutes.

3. Add **25 µl Thrombin reagent** and simultaneously start test.

For other instrument, please refer to your instrument manual for more detailed instrument specific instructions.

Calibration

TECal Normal or other commercially prepared plasma standard in which Fibrinogen has been determined should be used as reference (200-300mg/dL). Plot the clotting time obtained with each of the FIB standard dilutions on the y-axis against the concentration of FIB (mg/dL) on the x-axis using log-log graph paper. The line of best fit should be determined by linear regression analysis. The fibrinogen in plasma samples can be determined by interpolation from the calibration curve.

Expected Results

Typical normal results are 180-450 mg/dL^{4,5}. However results are influenced by the method of clot detection and can vary from laboratory to laboratory. Each laboratory is recommended to establish its own normal range on the specific instrument used.

Quality Control

TEControl or other commercial control plasma should be used for reliable quality control of performance at a frequency in accordance with good laboratory practice (GLP). TEControl can be frozen one time after reconstitution. 120-150 µl stored in closed polypropylene tubes at -20°C is stable for 30 days

Limitations**A. Specimen Collection. AVOID:**

- Use only plastic tubes or siliconised glass.
- Delayed mixing of blood with anticoagulant.
- Contamination with tissue thromboplastin.
- Improper ratio of anticoagulant with blood.
- Hemolyzed, icteric or lipemic samples may interfere optical systems

B. Laboratory Techniques

- Perform tests at 37°C.
- Use only high purity water.
- Optimum pH is 7.0-7.5.

Performance Characteristics

Precision:	CV% (within run)	CV% (inter-runs)
Normal control	< 5.0	< 5.0
Abnormal control	< 5.0	< 10.0

(Typical performance on instrument Coatrom M4)

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

References

- Clauss, A., Gerinnungsphysiologische Schnellmethode zur bestimmung des Fibrinogens. Acta Haematol., 1957, 17: 237-246.
- Shaw, T.S., Assays for Fibrinogen and its Derivatives, CRC Crit. Rev. Clin. Lab. Sci., 1977, 8: 145-192.
- National Committee for the National Laboratory (NCCLS) Standards: Collection transport and preparation of blood specimens for coagulation testing and performance of coagulation assays. Document H21-A2, vol. 11, No. 23, 1991.
- Scully, R.E. et al., Normal Reference Laboratory Values, N. Eng. J. Med., 1980, 302(37) : 37-48.
- Okuno, T. and Selenko, V., Amer. J. Med. Tech., 1972, 38(6) : 196-201.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative





IVD

REF

A0501-010, A0501-025, A0511-020, A0511-050

Verwendungszweck

TECLOT FIB wird zur quantitativen Bestimmung von Fibrinogen im menschlichen Plasma nach einer von Clauss¹ entwickelten Methode verwendet. Der Fibrinogenpegel kann auf Grund von Entzündungen, Schwangerschaft und dem Gebrauch von Ovulationshemmern ansteigen². Geringere Konzentrationen können bei verschiedenen Krankheiten wie Leberversagen und DIC auftreten. Angeborene Defizite beinhalten Afibrinogenämie (kein auffindbares Fibrinogen), Hypofibrinogenämie (<1 mg/ml) und Dysfibrinogenämie (abnormale Fibrinogenmoleküle).

Inhalte und Vorbereitungen

Produkt	TECLOT FIB Kit-10	TECLOT FIB Kit-25	TECLOT FIB A0511-020	TECLOT FIB A0511-050
Kat. Nr.	A0501-010	A0501-025	A0511-020	A0511-050
Thrombin Reagenz	5x2 mL	5x5 mL	10x2 mL	10x5 mL
IBS Puffer	1x125 mL	1x125 mL	-	-
TECal Normal	1x1 mL	1x1 mL	-	-
TEControl A	1x1 mL	1x1 mL	-	-

Bestimmungen

Coatron M*	400 Det.	1000 Det.	800 Det.	2000 Det.
Coatron A4	200 Det.	500 Det.	400 Det.	1000 Det.
Coatron A6	200 Det.	500 Det.	400 Det.	1000 Det.

*Mikromethode (75µL insgesamt)

- Thrombin Reagenz:
Enthält Rinderthrombin (~80 NIH) mit Stabilisatoren.
REF: A0501-010/A0511-020: mit 2ml hochreinem Wasser anlösen
REF: A0501-025/A0511-050: mit 5ml hochreinem Wasser anlösen
- IBS Puffer: gebrauchsfertig, 125ml
Enthält gepufferte Natriumchlorid Lösung, pH 7,3-7,4
- TECal Normal: Mit 1ml hochreinem Wasser anlösen
Enthält mit Zitrat versetztes menschliches Plasma.
- TEControl A: Mit 1ml hochreinem Wasser anlösen
Enthält mit Zitrat versetztes menschliches Plasma.

Nach der Anlösung vorsichtig leicht schwenken und bei Raumtemperatur 15 Minuten stehen lassen. Vor Gebrauch gut mischen. Nicht schütteln.

Lagerung und Stabilität

Ungeöffnete Reagenzien sind bei Lagerung zwischen 2-8°C bis zum auf dem Etikett angegebenen Verfallsdatum haltbar. **Geöffnete Reagenzien:**

Thrombin Reagenz*	2-8 °C 12 days	15-25 °C 5 days	37 °C 24 Std
TEControl oder Plasma	2-8 °C 8 Std	15-25 °C 4 Std	-20 °C 30 Std

* Reagenz muss vor UV-Licht und Verdunstung geschützt werden.

Vorsichtsmaßnahme

Haut- & Augenkontakt vermeiden. Abfälle gemäß lokaler Richtlinien für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös behandelt werden.

Probenentnahme und Lagerung ³

- Verfüßes Blut mittels Venenpunktur unter sauberen Bedingungen entnehmen.
- Sofort 9 Teile Blut mit einem Teil 3,2% Natriumzitrat (0,105M) gut mischen.
- Probe bei 1500g 10 Minuten lang zentrifugieren (Thrombozyten <10000/µl)
- Plasma nach der Zentrifugierung entfernen und in einem Röhrchen aus Plastik oder silikonisiertes Glas aufbewahren.
- Plasma innerhalb von 4 Stunden verwenden, andernfalls gefroren lagern und kurz vor Gebrauch auftauen.

Verfahren**A. Automatenmethode: Coatron A**

Fibrinogen	A4	A6		A4	A6		A4	A6
PAT Patient	10µl	CP1	10µl	CP1	Incubation	0s	SENS	0
BUF IBS Buffer	90µl	P39	90µl	P79	Maxtime	120s	POINTS	4
CLR -	0µl	-	0µl	-	Unit	769	MIX	No
DP -	0µl	P00	0µl	P00	Method	Coag	Clean	1 3
R0 -	0µl	P00	0µl	P00	Math	log XY	Multi	1 1
R1 -	0µl	P00	0µl	P00	CT-Mech	Yes	S-Corr	0%
R2 Fibrinogen	50µl	P29	50µl	P49	Deadtime	3s	T-Corr	0%

Erklärung der Symbole:

	Verfallsdatum		In-Vitro Diagnostik		Biologische Gefahr		Katalog-Nummer		Begleitpapiere beachten
	Bei 2-8°C lagern		EU Konformität		Hersteller		Lot. - Nummer		Bevollmächtigter

B. Manuelle Methode: Coatron M

- Vorbereitung von Standard-, Kontroll- und Patientenlösungen

Standardlösung	Plasma	IBS Puffer
1:5	200µL Standard	800µL
1:10	500µL 1:5 STD	500µL
1:20	500µL 1:10 STD	500µL
1:40	500µL 1:20 STD	500µL
Patient oder Kontrolle	100µL Plasma	900µL

- 50µL verdünntes Standard- oder Patientenplasma (1:10) in eine Küvette pipettieren. Bei 37°C für 1-2 Minuten erwärmen
 - 25µL Thrombinreagenz hinzufügen und gleichzeitig Test starten.
- Wenn Sie ein anderes Gerät verwenden, lesen Sie bitte für genauere Informationen die entsprechende Geräteanleitung.

Kalibrierung

TECal Normal oder anderes kommerzielles Standardplasma, mit bekanntem Fibrinogengehalt, sollte als Referenz (200-300 mg/dl) verwendet werden. Geben Sie die Gerinnungszeit jeder FIB Standard Lösung auf der Y- Achse gegen die FIB Konzentration (mg/dl) auf der X- Achse an. Verwenden Sie Millimeterpapier. Die Reihe der besten Ergebnisse sollte durch lineare Regressionsanalyse bestimmt werden. Fibrinogen in den Plasmaproben kann durch Interpolation der Kalibrierungskurve bestimmt werden.

Erwartete Ergebnisse

Typische normale Ergebnisse sind 180-450mg/dl^{4,5}. Die Ergebnisse sind jedoch von der Methode, wie die Gerinnungszeit bestimmt wird, abhängig und können von Labor zu Labor variieren. Jedem Labor wird empfohlen, seinen eigenen normalen Ergebnisbereich auf dem verwendeten Instrument zu erstellen.

Qualitätskontrolle

TEControl oder anderes kommerzielles Kontrollplasma sollte, um eine gute Qualität sicherzustellen, in regelmäßigen Abständen entsprechend Laborrichtlinien gemessen werden. In regelmäßigen Abständen entsprechend Laborrichtlinien gemessen werden. TEControl kann einmalig wieder eingefroren werden. Hierfür 120-150µL in einem verschließbaren polypropylen Gefäß bei -20°C aufbewahren und innerhalb der nächsten 30 Tage verwenden.

Beschränkungen

A. Probenvorbereitung. Achten Sie auf:

- nur Plastikröhrchen oder silikonisiertes Glas verwenden
- verzögertes Mischen von Blut mit Antikoagulanzen vermeiden
- Kontamination mit Gewebethromboplastin vermeiden
- falsches Verhältnis von Antikoagulanzen und Blut vermeiden
- Hämolytische, lipämische oder ikterische Proben können optische Systeme stören

B. Labortechniken

- Tests bei 37°C durchführen
- nur hochreines Wasser verwenden
- der optimale pH Wert ist 7,0-7,5

Leistungsdaten

Präzision:	VK% (Einzellauf)	VK% (Mehrfachlauf)
Normale Kontrolle	< 5,0	< 5,0
Abnormale Kontrolle	< 5,0	< 10,0

(Typische Leistung beim Gerät Coatron M4)

Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produktes den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Veräußerlichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Referenzen

- Clauss, A., Gerinnungsphysiologische Schnellmethode zur Bestimmung des Fibrinogens. Acta Haematol., 1957, 17: 237-246.
- Shaw, T.S., Assays for Fibrinogen and its Derivatives, CRC Crit. Rev. Clin. Lab. Sci., 1977, 8: 145-192.
- National Committee for the National Laboratory (NCCLS) Standards: Collection transport and preparation of blood specimens for coagulation testing and performance of coagulation assays. Document H21-A2, vol. 11, No. 23, 1991.
- Scully, R.E. et al., Normal Reference Laboratory Values, N. Eng. J. Med., 1980, 302(37) : 37-48.
- Okuno, T. and Selenko, V., Amer. J. Med. Tech., 1972, 38(6) : 196-201.



**Revisions-Übersicht:**

Rev.	am	Änderung durch	Gültig für	Freigabe am	Freigabe durch
1	5.4.11	WG	Technoclone FIB		
	Beschreibung:	New box insert for Technoclone FIB.			
2	21.12.11	CB	Technoclone FIB	21.12.11	CH
	Beschreibung:	Neue Stabilitätsangaben. Die Vorgaben wurden dem Technoclone Stability Test Report „TC6E0C.01“ vom 5.5.2010 entnommen.			
3	11.11.13	CB	Technoclone FIB		
	Beschreibung:	- Protokoll für A4+A6 - Stabilitätsdaten neu			
4	16.10.17	AR	Technoclone FIB	16.10.17	CH
	Beschreibung:	Technoclone Puffer (A0591-090) wird ersetzt durch IBS (A0590-125) (wegen deutlicher Messunterschiede bei Coatron A und X Serie) Werteermittlung für das CoA erfolgt ebenso mit IBS (A0590-125)			
5	23.01.18	VG	Technoclone FIB	23.01.18	VG
	Beschreibung:	Neue Stabilitätsangaben von Technoclone vom Thrombin Reagent.			



IVD

REF

A0590-125

Intended Use

The IBS Buffer solution is optimally formulated for use on Coagulation Analyzers. Use in accordance with the recommended Operators Manuals for installing and replacing Owrens Veronal Buffer (OVb). The IBS can be used as the diluent for preparing plasma dilutions in the performance of Fibrinogen determinations and Coagulation Factor Assays with all manual, mechanical, or photo-optical means of clot detection. Follow Reagent manufacturer's recommended procedures for preparation of plasma dilutions using Imidazole Buffered Saline.

Contents & Determinations

Product	IBS Buffer
Cat.No.	A0590-125
IBS Buffer	1x125 mL

Preparation

IBS: pH 7.3 - 7.4, liquid
Ready to use.

Storage and Stability

Unopened reagents are stable until the expiration date shown on the label stored at 2-8°C.

Precautions

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material.

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative





IVD

REF

P6001-010

Intended Use

Use as a normal control for following coagulation tests:

PT, APTT, Thrombintime and Fibrinogen.

Contents

10 x 1mL freeze dried citrate-anticoagulated human plasma

Preparation

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

Storage & Stability

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C
1 month	8 hours	4 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

Precautions

This product contains substance from human origin!
Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

Expected Results

Refer to "Certificate of Analysis".

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative





IVD

REF

P6001-010

Verwendungszweck

Als normale Kontrolle für folgende Gerinnungstests verwenden:

PT, APTT, Thrombinzeit und Fibrinogen.

Inhalt

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

Vorbereitung

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TECLOT PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

Lagerung und Stabilität

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C
1 Monat	8 Stunden	4 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

Vorsichtsmaßnahmen

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.

Erwartete Ergebnisse

Lesen Sie das Analysenzertifikat

Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Veräußlichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter



IVD

REF

P6001-010

Revisions-Übersicht:

Rev.	am	Änderung durch	Gültig für	Freigabe am	Freigabe durch
1	5.4.11	WG	Technoclone Coagulation Control N		
	Beschreibung:	New box insert for Technoclone Coagulation Control N.			





IVD

REF

P6101-010

Intended Use

Use as an abnormal control for following coagulation tests:

PT, APTT, Thrombin time and Fibrinogen.

Contents

10 x 1mL freeze dried citrate-anticoagulated human plasma

Preparation

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

Storage & Stability

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C
1 month	8 hours	4 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

Precautions

This product contains substance from human origin!

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

Expected Results

Refer to "Certificate of Analysis".

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative





IVD

REF

P6101-010

Verwendungszweck

Als abnormale Kontrolle für folgende Gerinnungstests verwenden:

PT, APTT, Thrombinzeit und Fibrinogen.

Inhalt

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

Vorbereitung

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TEClot PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

Lagerung und Stabilität

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C
1 Monat	8 Stunden	4 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

Vorsichtsmaßnahmen

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.

Erwartete Ergebnisse

Lesen Sie das Analysenzertifikat

Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Veräußlichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot.- Nummer	Bevollmächtigter



IVD

REF

P8001-010

Intended Use

Use as a calibrator or normal control for following coagulation tests:

**PT, APTT, Thrombin time, Fibrinogen,
Factors: II, V, VII, VIII, IX, X, XI, XII,
Antithrombin, Protein-C, Protein-S**

Contents

10 x 1mL freeze dried citrate-anticoagulated human plasma

Preparation

Reconstitute individual vials with **1,0 ml** distilled water. Allow to stand at room temperature, with occasional swirling, for 15 min before use. Be certain all particulate matter is well dissolved.

PT whole blood (TEClot PT-B): Reconstitute individual vials with **1,7 ml** distilled water.

Storage & Stability

Unopened vials are stable until the expiration date shown on the label stored at 2°-8°C.

Dissolved plasma change analytic levels below 10% if stored as following:

-20 °C	2-8 °C	20-25 °C	37°C
30 days	24h	8h	2 hours

Dissolved plasma can be refrozen only one time in aliquots (120-150µL). Stored at -20°C in closed polypropylene tubes, the aliquots must be used within 30 days.

Precautions

This product contains substance from human origin!
Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV and HCV. However products from human blood should be considered as potentially infectious.

Expected Results

Refer to "Certificate of Analysis".

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

Symbols key:

Expiry date	In Vitro Diagnostica	Biological hazard	Catalogue Number	Consult accompanying documents
Store at 2-8°C	EU conformity	Manufacturer	Lot. Number	Authorized Representative





IVD

REF

P8001-010

Verwendungszweck

Als Kalibrator oder Normalkontrolle für folgende Gerinnungstests verwenden:

**PT, APTT, Thrombinzeit, Fibrinogen,
Faktoren: II, V, VII, VIII, IX, X, XI, XII,
Antithrombin, Protein-C, Protein-S**

Inhalt

10 x 1mL gefriergetrocknetes mit Zitrat versetztes gerinnungshemmendes Humanplasma

Vorbereitung

Die einzelnen Fläschchen mit 1,0ml destilliertem Wasser anlösen. Fläschchen bei Raumtemperatur bis zur Anwendung unter gelegentlichen Verwirbeln 15 Minuten lang stehen lassen. Stellen Sie sicher, dass alle Partikel gut aufgelöst sind.

Vollblut PT (TEClot PT-B): einzelne Fläschchen mit 1,7ml destilliertem Wasser anlösen.

Lagerung und Stabilität

Ungeöffnete Fläschchen sind bei Lagerung zwischen 2-8°C zum bis auf dem Etikett angegebenen Verfallsdatum haltbar.

Gelöstes Plasma verändern die analytischen Levels unter 10% wenn wie folgt gelagert:

-20 °C	2-8 °C	20-25 °C	37°C
30 Tage	24 Stunden	8 Stunden	2 Stunden

Gelöstes Plasma kann einmalig wiedereingefroren werden. Die Aliquots (120-150µL) sind 30 Tage haltbar, wenn sie in polypropylen Gefäßen bei -20°C aufbewahrt werden.

Vorsichtsmaßnahmen

Dieses Produkt enthält Substanzen humanen Ursprungs! Haut- und Augenkontakt vermeiden. Angemessene Schutzkleidung tragen. Abfälle laut lokaler Regelungen für infektiöse Materialien entsorgen. Alle Bestandteile wurden auf HIV, HBV und HCV getestet. Trotzdem müssen Produkte aus menschlichem Blut immer als potentiell infektiös angesehen werden.

Erwartete Ergebnisse

Lesen Sie das Analysenzertifikat

Garantie

Es wird garantiert, dass die Wirkungsweise dieses Produkts den Angaben auf der Packung und in der Produktliteratur entspricht. TECO haftet weder für die Veräußlichkeit oder Eignung dieses Produktes für irgendwelche andere Zwecke noch für irgendwelche Folgeschäden, die sich aus der vorstehenden, expliziten Garantie ergeben.

Erklärung der Symbole:

Verfallsdatum	In-Vitro Diagnostik	Biologische Gefahr	Katalog-Nummer	Begleitpapiere beachten
Bei 2-8°C lagern	EU Konformität	Hersteller	Lot. - Nummer	Bevollmächtigter



IVD

REF

A0300-025, A0300-050, A0320-050, A0320-100

Intended Use

This product is intended for determination of Activated Partial Thromboplastin Time (APTT) using silicate as activator. The determination of the APTT is used for the global evaluation of the intrinsic pathway and detecting deficiencies of the intrinsic coagulation factors VIII, IX, XI, XII, and Fletcher Factor as well as for monitoring heparin anticoagulant therapy or other coagulation methods where an APTT reagent is required^{1,2}. The APTT reagent in the kit contains phospholipids and silica to ensure a highly consistent and stable product³. The APTT reagent is lupus anticoagulant insensitive. Lupus anticoagulant insensitive reagents yield more reliable factor assay results than reagents, which are sensitive to lupus inhibitors⁴. Prolonged clotting times may be observed in the following situations: deficiency of intrinsic coagulation factors, presence of heparin, in liver diseases, vitamin K Deficiency or other anticoagulants, which affect the intrinsic pathway.

Contents & Determinations

Product	TECLOT APTT-S Kit-25	TECLOT APTT-S Kit-50	TECLOT APTT-S A0320-050	TECLOT APTT-S A0320-100
Cat.No.	A0300-025	A0300-050	A0320-050	A0320-100
APTT-S Reagent*	5x5 mL	5x10 mL	10x5 mL	10x10 mL
CaCl ₂ 0.025M**	5x5 mL	5x10 mL	-	-

Determinations

Coatlon M***	1000 Det.	2000 Det.	2000 Det.	4000 Det.
Coatlon A4	500 Det.	1000 Det.	1000 Det.	2000 Det.
Coatlon A6	1000 Det.	2000 Det.	2000 Det.	4000 Det.

*APTT-S Reagent contains colloidal silicate with phospholipids, buffer and preservatives.

**CaCl₂ contains sodium azide.

***Micro method (75µL in total)

Preparation

Components of kit are ready to use. Allow CaCl₂ to prewarm 15 min at 37 °C and mix APTT reagent gently prior usage

Storage & Stability

Unopened reagents are stable until the expiration date shown on the label stored at 2°-8°C. Opened reagent:

	2-8 °C	20-25 °C	37 °C
APTT-S Reagent	30 days	8 days	8 hours

Precautions

Avoid contact with skin and eyes. Wear suitable protective clothing. Dispose components in compliance with local regulations for infectious material. All components are checked for HIV, HBV, HCV. However products from human blood should be considered as potentially infectious.

Specimen collection and storage⁵

1. Obtain venous blood by clean vein puncture.
2. Immediately mix 9 parts blood with 1 part 3.2% sodium citrate (0.105M) and mix well
3. Centrifuge the specimen at 1500g for 10 min. (platelet < 10000/µL)
4. Separate plasma after centrifugation and store in plastic or siliconised glass tube.
5. Use plasma within 4 hours, otherwise store frozen and thaw just prior to use.

Stability of plasma: 4h at 18-26°C 8h at 2-8° 14d at -20°C 6m at -70°C

Procedure**A. Automated Method: Coatlon A**

APTT-S	A4	A6		A4	A6		A4	A6
PAT Patient	50µl	CP1	25µl	CP1		Incubation	180s	
BUF -	0µl	P00	0µl	P00		Maxtime	180s	
CLR -	0µl	-	0µl	-		Unit	17	
DP -	0µl	P00	0µl	P00		Method	Coag	
R0 -	0µl	P00	0µl	P00		Math	-	
R1 APTT-S	50µl	P31	25µl	P60		CT-Mech	No	
R2 CaCl 25mM	50µl	P26	25µl	P47		Deadtime	17s	
						SENS	1	
						POINTS	0	
						MIX	No	
						Clean	0	0
						Multi	1	3
						S-Corr	0%	
						T-Corr	15% - 6s	

B. Manual Method: Coatlon M

1. Prewarm CaCl₂ (0.025M) at 37°C for at least 10 min
2. Pipette 25 µl of sample into a test cuvette. Prewarm at 37°C for 1-2 minutes.
3. Add 25 µl APTT-S reagent and incubate exactly for 3 min at 37°C.
4. Add 25 µl of CaCl₂ (0.025M) and simultaneously start test.
5. Record the clotting time in seconds.

Expected Results

Typical normal results are 27-42 sec. However results are influenced by the method of clot detection and can vary from laboratory to laboratory. Each laboratory is recommended to establish its own normal range on the specific instrument used.

Quality Control

TEControl or other commercial control plasma should be used for reliable quality control of performance at a frequency in accordance with good laboratory practice (GLP). TEControl can be frozen one time after reconstitution. 120-150 µl stored in closed polypropylen tubes at -20°C is stable for 30 days

Limitations**A. Specimen Collection. AVOID:**

1. Use only plastic tubes or siliconised glass.
2. Delayed mixing of blood with anticoagulant.
3. Contamination with tissue thromboplastin.
4. Improper ratio of anticoagulant with blood.
5. Hemolyzed, icteric or lipemic samples may interfere optical systems

B. Laboratory Techniques

1. Perform tests at 37°C.
2. Use only high purity water.
3. Optimum pH is 7.0-7.5.

Performance Characteristics**Typical performance on instrument Coatlon M4**

Precision:	CV% (within run)	CV% (inter-runs)
QC control	<3,0	<5,0

Factor & Heparin sensitivity:

Factor (%)	APTT Clotting time (s)		
	FVIII	FIX	FXI
<1%	100	80	103
10%	53	52	58
40%	40	39	41
100%	35	35	358

Heparin (U/mL)	0 U/mL	0,2 U/mL	0,4 U/mL
APTT clotting time (s)	35	70	180

These values should be used as guidelines only. Each laboratory should establish factor or heparin sensitivity using its own instruments and techniques.

Warranty

This product is warranted to perform in accordance with its labelling and literature. TECO disclaims any implied warranty of merchantability or fitness for any other purpose, and in no event will TECO be liable for any consequential damages arising out of aforesaid express warranty.

References

1. Proctor RR, Rapaport SI. The partial thromboplastin time with kaolin. A simple screening test for first stage plasma clotting factor deficiencies. *Am J Clin Pathol* 36, 212-219 (1961).
2. Triplett DA, Harms CS, Koepke JA. The effect of heparin on the activated partial thromboplastin time. *Am J Clin Pathol* 70, 556-569 (1978).
3. Stevenson KJ, Easton AC, Thomson JM, Poller L. The reliability of activated partial thromboplastin time methods and the relationship to lipid composition and ultrastructure. *Thromb Haemost* 55, 250-258 (1986).
4. Denis-Magdelaine A, Flahault A, Verdy E. Sensitivity of sixteen APTT reagents for the presence of lupus anticoagulants. *Haemostasis* 25, 98-105 (1995).
5. NCCLS: Guidelines for the Standardized Collection, Transport and Preparation of Blood Specimens for Coagulation Testing and Performance of Coagulation Assays

Symbols key:

	Expiry date		In Vitro Diagnostica		Biological hazard		Catalogue Number		Consult accompanying documents
	Store at 2-8°C		EU conformity		Manufacturer		Lot. Number		Authorized Representative

