

CERTIFICATE

Vertou, 13th January 2020

I, Noujoud WAHBI, pharmacist on the committee of Scientific Expertise for the company Christeyns France, hereby certify that the products

Phago'spore

And

Clinlabs block spray

And

1226

have the same formula and that disinfection tests were passed under these denominations.

CHRISTEYNS France S.A.

S.A. au Capital de 1.500.000 Euros
31, rue de la Maladrie - BP 2421
44124 VERTOU CEDEX
Tél. 02 40 80 27 27 - Fax 02 40 03 09 73
R.C.S. NANTES B 321 302 689 00013 - APE 2041Z

Noujoud WAHBI
Pharmacist



Essai de suspension pour l'évaluation de l'activité bactéricide des désinfectants chimiques utilisés pour les instruments en médecine selon NF EN 13727 : 2004

Produit : 1226 IND01

Donneur d'ordre : **CHRISTEYNS France**
Division santé Laboratoire Phagogène
9 rue Marcel Sembat
44100 NANTES

Loos, le 07 juin 2013.

Le directeur :


Raphaël DUGUÉ.

L'accréditation du COFRAC atteste de la compétence des laboratoires pour les seuls essais couverts par l'accréditation.

La reproduction de ce rapport d'essai n'est autorisée que sous sa forme intégrale.

Ce rapport d'essais ne concerne que les échantillons soumis à essais.

Page 1 sur 6

1 PRINCIPE :

L'activité bactéricide a été déterminée selon la norme européenne **NF EN 13727: "Antiseptiques et désinfectants chimiques - Essai quantitatif de suspension pour l'évaluation de l'activité bactéricide des désinfectants chimiques pour les instruments utilisés en médecine - Méthode d'essai et exigences (Phase 2, étape 1) – juillet 2004."**

Souche(s) de référence testée(s) : **voir tableau(x) page(s) suivante(s).**

2 IDENTIFICATION DE(S) ECHANTILLON(S) :

Nom(s) : **1226 IND01.**

Société : **CHRISTEYNS France.**

Date de réception au laboratoire : **22/04/13.**

Conditions de stockage au laboratoire : **Température ambiante, à l'abri de la lumière.**

3 METHODES D'ESSAI ET VALIDATION:**3.1 Dilution neutralisation :**

Diluant : **neutralisant CEN tamponné**

3.2 Filtration sur membrane.

Nature des membranes : **Millipore type HAWG 0,45 *m.**

Liquide de rinçage : **Eau distillée stérile.**

Volume de chaque rinçage : **100 ml.**

Nombre de rinçages : **4.**

Neutralisant ajouté au milieu de dénombrement : **TSB Capitol IV à raison de 10% (v/v) du milieu gélosé.**

4 CONDITIONS EXPERIMENTALES:

Période d'analyse : **Du 14/05/13 au 03/06/13.**

Diluant du produit utilisé au cours des essais: **Eau distillée (produit prêt à l'emploi).**

Concentration(s) du produit soumis à essai : **voir tableau(x) page(s) suivante(s).**

Aspect des dilutions de produit : **dilutions homogènes.**

Température de contact : **20°C +/- 1°C.**

Temps de contact additionnel : **5 minutes +/- 10 secondes.**

Substance interférente : **Albumine bovine 3,0 g/l + erythrocytes de mouton 3,0 ml/l (conditions de saleté). Préparée selon les indications de la norme NF EN 13 727.**

Stabilité du mélange de la substance interférente et des produits soumis aux essais: **pas de précipité observé**

Température d'incubation: **37°C +/- 1°C.**

5 RESULTATS EXPERIMENTAUX:

Vérification de la méthodologie et de la validation de la méthode de neutralisation du produit soumis à l'essai dans les conditions expérimentales décrites ci-avant :

Essai 1 : neutralisation par dilution

Souche(s) :	Nombre de cellules viables (UFC/ml) :				
	Suspension bactérienne Nv₀	Témoin des conditions expérimentales : A	Témoin de non toxicité du neutralisant : B	Validation de la méthode de dilution-neutralisation Concentration du produit : 80% C	Conclusion :
<i>Pseudomonas aeruginosa</i> CIP 103467	Vc: 42 ; 36 Nv ₀ : 39,0	Vc: 42 ; 40 A: 41,0	Vc: 38 ; 42 B: 40,0	Vc: 0 ; 0 C: 0,0	Non validée
<i>Staphylococcus aureus</i> CIP 4. 83	Vc: 44 ; 42 Nv ₀ : 39,0	Vc: 46 ; 50 A: 41,0	Vc: 50 ; 48 B: 49,0	Vc: 0 ; 0 C: 0,0	Non validée
<i>Enterococcus hirae</i> CIP 58 55	Vc: 48 ; 42 Nv ₀ : 45,0	Vc: 40 ; 38 A: 39,0	Vc: 46 ; 40 B: 43,0	Vc: 0 ; 0 C: 0,0	Non validée

Vc : nombre d' ufc comptées.
N : Nombre d'ufc/ml de la suspension bactérienne d'essai (5.4.1.4.).
Nv₀ : N/10 soit Nombre d'ufc/ml de la suspension bactérienne de validation (5.4.1.5.).
Na : Nombre d'ufc/ml dans le mélange d'essai (5.5.2.2.).
A :Nombre d'ufc/ml dans l'essai de validation des conditions expérimentales (5.5.2.3 ou 5.5.3.3).
B : Nombre d'ufc/ml dans l'essai de validation de la non-toxicité du neutralisant (5.5.2.4) ou du témoin de filtration sur membrane (5.5.3.4).
C : Nombre d'ufc/ml dans l'essai de validation de l'inactivation par dilution neutralisation (5.5.2.5) ou par filtration sur membrane (5.5.3.5).
Critères de validation :
A, B, C supérieurs ou égaux à 0,5 x Nv₀
Nv₀ compris entre 30 et 160 UFC/ml
N compris entre 1,5.10⁶ et 5,0.10⁸
N₀ compris entre 1,5.10⁷ et 5,0.10⁷
log N₀ compris entre 7,17 et 7,70
Quotient moyenne pondérée compris entre 5 et 15

Conclusion : La méthode de neutralisation par dilution n'est pas validée.

Essai 2 : neutralisation par filtration sur membrane :
(Essais réalisés en parallèle à l'essai proprement dit)

Souche(s) :	Nombre de cellules viables (UFC/ml) :				
	Suspension bactérienne Nv₀	Témoin des conditions expérimentales : A	Témoin de filtration : B	Validation de la méthode de Filtration sur membrane Concentration du produit : 80% C	Conclusion :
<i>Pseudomonas aeruginosa</i> CIP 103467	Vc: 53 ; 58 Nv ₀ : 55,5	Vc: 56 ; 54 A: 55,0	Vc: 54 ; 56 B: 55,0	Vc: 52 ; 54 C: 53,0	Validée
<i>Staphylococcus aureus</i> CIP 4. 83	Vc: 42 ; 46 Nv ₀ : 44,0	Vc: 38 ; 44 A: 41,0	Vc: 42 ; 46 B: 44,0	Vc: 44 ; 45 C: 44,5	Validée
<i>Enterococcus hirae</i> CIP 58 55	Vc: 60 ; 64 Nv ₀ : 62,0	Vc: 61 ; 57 A: 59,0	Vc: 59 ; 64 B: 61,5	Vc: 66 ; 55 C: 60,5	Validée

Vc : nombre d' ufc comptées.
N : Nombre d'ufc/ml de la suspension bactérienne d'essai (5.4.1.4.).
Nv₀ : N/10 soit Nombre d'ufc/ml de la suspension bactérienne de validation (5.4.1.5.).
Na : Nombre d'ufc/ml dans le mélange d'essai (5.5.2.2).
A : Nombre d'ufc/ml dans l'essai de validation des conditions expérimentales (5.5.2.3 ou 5.5.3.3).
B : Nombre d'ufc/ml dans l'essai de validation de la non-toxicité du neutralisant (5.5.2.4) ou du témoin de filtration sur membrane (5.5.3.4).
C : Nombre d'ufc/ml dans l'essai de validation de l'inactivation par dilution neutralisation (5.5.2.5) ou par filtration sur membrane (5.5.3.5).
Critères de validation :
A, B, C supérieurs ou égaux à 0,5 x Nv₀
Nv₀ compris entre 30 et 160 UFC/ml
N compris entre 1,5.10⁸ et 5,0.10⁸
N₀ compris entre 1,5.10⁷ et 5,0.10⁷
log N₀ compris entre 7,17 et 7,70
Quotient moyenne pondérée compris entre 5 et 15

Conclusion : La méthode de neutralisation par filtration sur membrane est validée.

Essais proprement dit (méthode par filtration sur membrane) :

Souche(s) :	Suspension d'essai : N et N ₀	Nombre de cellules viables (UFC/ml) pour le mélange d'essai pour les concentrations en % (v/v) de : Na			
		0,08	0,8	8,0	80,0
<i>Pseudomonas aeruginosa</i> CIP 103467	10 ⁻⁶ : Vc1 : 218 Vc2 : 224 10 ⁻⁷ : Vc1 : 25 Vc2 : 27 N : 2,3 x 10 ⁸ N ₀ : 2,3 x 10 ⁷ log N ₀ : 7,36	Vc1 : > 330 Vc2 : > 330 Na : > 3,30 x 10 ³ log Na : > 3,52	Vc1 : > 330 Vc2 : > 330 Na : > 3,30 x 10 ³ log Na : > 3,52	Vc1 : < 14 Vc2 : < 14 Na : < 1,40 x 10 ² log Na : < 2,15	Vc1 : < 14 Vc2 : < 14 Na : < 1,40 x 10 ² log Na : < 2,15
<i>Staphylococcus aureus</i> CIP 4 83	10 ⁻⁶ : Vc1 : 174 Vc2 : 178 10 ⁻⁷ : Vc1 : 18 Vc2 : 20 N : 1,8 x 10 ⁸ N ₀ : 1,8 x 10 ⁷ log N ₀ : 7,26	Vc1 : > 330 Vc2 : > 330 Na : > 3,30 x 10 ³ log Na : > 3,52	Vc1 : > 330 Vc2 : > 330 Na : > 3,30 x 10 ³ log Na : > 3,52	Vc1 : < 14 Vc2 : < 14 Na : < 1,40 x 10 ² log Na : < 2,15	Vc1 : < 14 Vc2 : < 14 Na : < 1,40 x 10 ² log Na : < 2,15
<i>Enterococcus hirae</i> CIP 5855	10 ⁻⁶ : Vc1 : 207 Vc2 : 208 10 ⁻⁷ : Vc1 : 22 Vc2 : 23 N : 2,1 x 10 ⁸ N ₀ : 2,1 x 10 ⁷ log N ₀ : 7,32	Vc1 : > 330 Vc2 : > 330 Na : > 3,30 x 10 ³ log Na : > 3,52	Vc1 : > 330 Vc2 : > 330 Na : > 3,30 x 10 ³ log Na : > 3,52	Vc1 : < 14 Vc2 : < 14 Na : < 1,40 x 10 ² log Na : < 2,15	Vc1 : < 14 Vc2 : < 14 Na : < 1,40 x 10 ² log Na : < 2,15

Réduction du nombre de cellules viables aux concentrations d'essai :

	0,08	0,8	8,0	80,0
<i>Pseudomonas aeruginosa</i> CIP 103467	log R : < 3,82	log R : < 3,82	log R : > 5,21	log R : > 5,21
<i>Staphylococcus aureus</i> CIP 4 83	log R : < 3,74	log R : < 3,74	log R : > 5,11	log R : > 5,11
<i>Enterococcus hirae</i> CIP 5855	log R : < 3,80	log R : < 3,80	log R : > 5,17	log R : > 5,17
Critères de validation :				
N compris entre 1,5 x 10 ⁸ et 5,0 x 10 ⁸				
N ₀ compris entre 1,5 x 10 ⁷ et 5,0 x 10 ⁷				
log N ₀ compris entre 7,17 et 7,70				

6 CONCLUSION :

Conformément à la norme européenne **NF EN 13727** (juillet 2004),

- En **5 minutes de contact à 20°C**, [conditions optionnelles],
- Dans les **conditions de saleté (Albumine bovine 3,0 g/l + erythrocytes de mouton 3,0 ml/l)**,
- Vis-à-vis des souches de
Pseudomonas aeruginosa CIP 103467,
Staphylococcus aureus CIP 4. 83,
Enterococcus hirae CIP 58 55,

Le produit **1226 IND01** dilué à **8,0% (v/v)** présente une **activité bactéricide**.



Test report No. sd2319

EVALUATION OF MYCOBACTERICIDAL ACTIVITY OF CHEMICAL DISINFECTANTS IN THE MEDICAL AREA INCLUDING INSTRUMENT DISINFECTANTS (EN 14348)

Name of the product: 1226

Batch number: 367929

Date of test report: 08.02.2019

Client, representative:

Christeyns France

31 Rue de la Maladrie 44124 Vertou

Jérôme Dubourgeois; +33 (0)2 40 57 56 23

Test report No. sd2319

EVALUATION OF MYCOBACTERICIDAL ACTIVITY (EN 14348)

Name of the product: 1226
Batch number: 367929
Order number: 18018
Manufacturer: Christeyns France
Client, representative: Christeyns France; 31 Rue de la Maladrie 44124 Vertou; Jérôme Dubourgeois; +33 (0)2 40 57 56 23
Date of delivery: 12.10.2018
Test material conditions: No specific features, sample in the manufacturers tare
Storage conditions: In room temperature, dark;
Active substance – conc.: Peracetic acid: 340 ppm; Hydrogen peroxide: 3.26%
Appearance of the product: Transparent liquid
Test concentration: 80%; 40%; 20%
Test conditions: Dirty conditions
Contact time: 5 min; 15 min; 60 min (obligatory)
Interfering substance: 3 g/l bovine albumin + 3 ml/l sheep blood erythrocytes
Test neutralizer: Polysorbate 80 30 g/l; lecithin 3 g/l; sodium thiosulphate 12g/l
Rinsing liquid: -
Test organisms: *Mycobacterium terrae* ATCC 15755;
Mycobacterium avium ATCC 15769
Testing method base: EVS-EN 14348:2005 – Chemical disinfectants and antiseptics - Quantitative suspension test for the evaluation of mycobactericidal activity of chemical disinfectants in the medical area including instrument disinfectants - Test methods and requirements (phase 2, step 1)
Testing date: 26.11.2018 – 18.12.2018
Results: look appendix 1-3


Allar Laaneleht
Chief specialist
Date of test report: 08.02.2019

Appendix 3

Interpretation

The EN 14348 standard was used for testing a product **1226** – (Batch No. 367929) at 20 °C ± 1 °C, with the contact times of 5 min, 15 min and 60 min (obligatory) under dirty conditions. The dilution-neutralization method was used for testing products' effectiveness against the reference strains: *Mycobacterium terrae* ATCC 15755, *Mycobacterium avium* ATCC 15769. Under dirty conditions the tested 80% of product was active against both of the testorganisms for all contact times; 40% within .15 min, 60 min and 20% within 60 min.

Conclusion


The surviving count of mycobacterial reference strains showed at least 4 lg reduction meaning that **under dirty conditions the 80% solution of product 1226 is mycobactericidal within 5 min, 40% solution within 15 min and 20% solution within 60 min.**



Allar Laaneleht

Chief specialist

08.02.2019

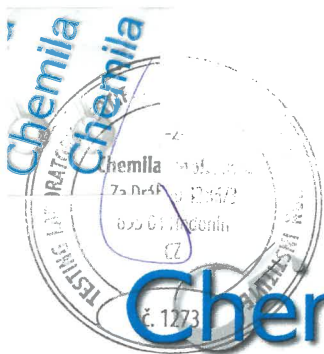

Chemila, spol. s r.o., Za Dráhou 4386/3, Hodonín 69501, Phone +420518340919, chemila@chemila.cz
Chemical and Microbiological Laboratory, Testing Laboratory No. 1273 certified by Czech Accreditation Institute
according to ČSN EN ISO/IEC 17025:2005.

Copy No.: 1
Issue No.: 1

Test report No. S268-1/2018

DETERMINATION OF FUNGICIDAL (EN 13624:2013) ACTIVITY OF THE PRODUCT 1226

Sample ID: S268/2018

Sample name: 1226

Client: Christeyn France S.A., 31, Rue de la Maladrie, 44124 Vertou, France

Producer: Christeyn France S.A., 31, Rue de la Maladrie, 44124 Vertou, France

Sampling point: Christeyn France S.A., 31, Rue de la Maladrie, 44124 Vertou, France

Page: 1

From pages: 8

Incoming date:
10.10.2018

Delivery date:
14.2.2019

Hodonín, 14.2.2019



.....
Ing. Jana Šlitrová, Head of Laboratory

The report may be reproduced only as a whole, in parts only upon written permission of the laboratory. The test results relate only to the samples stated in the Test Report. The Lab does not take any guarantee for the identity of samples not taken by the lab personnel.

Description: *Testing the efficacy of chemical disinfectants and antiseptics*

Sample ID: S268/2018

Rep No: 161

Sample name: **1226**

Sampled: by client

Sampling point: Christeyn France S.A., Vertou

Client: Christeyn France S.A., 31, Rue de la Maladrerie, Vertou

Sampling date: 8.10.2018

Sample delivered: 10.10.2018

Testing date: 8.11. – 11.11.2018

Delivered amount: 800 ml

Batch No: 367929

Page: 2

Subject of testing:

Determination of fungicidal activity of the product.

Identification of the sample:

Name of the product:

1226

Batch number:

267929

Date of manufacture:

12/01/2018

Expiry date:

12/01/2021

Manufacturer:

Christeyn France S.A., 31, Rue de la Maladrerie, 44124 Vertou, France

Incoming date:

10.10.2018

Storage conditions:

5 – 30 °C

Active compounds and concentrations:

CAS 7722-84-1 hydrogen peroxide 3.26 %

CAS 79-21-0 peracetic acid 0.034 %

Experimental conditions:

Testing of disinfecting efficiency of chemical disinfecting and antiseptic agents by suspension method

SOP-M-19-00 (EN 13624:2013)

Period of analysis:

8.11. – 11.11.2018

Test temperature:

20 °C ± 1 °C

Test method:

dilution neutralization method

Neutralization medium:

Dey-Engley Neutralizing Broth M 1062

Appearance of the product:

colourless liquid

Test concentration:

100% (concentrated) *

Contact time:

5 min

Interfering substances:

3 g/l BSA and 3 ml/l sheep erythrocytes (dirty conditions)

Test organisms:

Candida albicans ATCC 10231

Aspergillus brasiliensis (niger) ATCC 16404

Incubation conditions:

30 °C ± 1 °C, 48 hours and additional period of 24 or 48 hours

Test procedure:

1. Preparation of test suspension
2. Preparation of product test solutions
3. Quantitative suspension test
4. Incubation and calculation
5. Expression and interpretation of results

Note:

Presence of a high concentration (at least 75%) of *Aspergillus brasiliensis* spiny spores in the test suspension – yes.

Fungicidal activity – the capability of a product to produce a reduction in the number of viable fungi belonging to reference strains under defined conditions by at least a 4 lg reduction (10^4).

Yeasticidal activity – the capability of a product to produce a reduction in the number of viable yeast cells of relevant test organisms under defined conditions by at least a 4 lg reduction (10^4).

$R = N_0 / N_a$ = the reduction in viability, or $\lg R = \lg N_0 - \lg N_a$

* The product can only be tested at a concentration of 97% (RTU product, used modified method) or less, as some dilution is always produced by adding the inoculum and interfering substance.

The standard:

EN 13624:2013 Chemical disinfectants and antiseptics – Quantitative suspension test for the evaluation of fungicidal or yeasticidal activity in the medical area - Test method and requirements (phase 2, step 1) September 2013

Description: *Testing the efficacy of chemical disinfectants and antiseptics*

Sample ID: S268/2018
 Rep No: 161
 Sample name: **1226**
 Sampled: by client
 Sampling point: Christeyn France S.A., Vertou
 Client: Christeyn France S.A., 31, Rue de la Maladrie, Vertou

Sampling date: 8.10.2018
 Sample delivered: 10.10.2018
 Testing date: 8.11. – 11.11.2018
 Delivered amount: 800 ml
 Batch No: 367929
 Page: 3

The Number of CFU in the tested product: 0 CFU/ml

1. Testing the efficacy of chemical disinfectant **1226** on *Candida albicans* ATCC 10231

Tab No. 1.1 Verification of methodology, dirty conditions

Validation of suspension (N _{V0})			Validation of selected experimental conditions (A)			Neutralizer toxicity control (B)			Method validation (C) Product conc.: 100%*		
V _{e1}	35	Φ _{N_{V0}} = 31	V _{e1}	35	Φ _A = 30.5	V _{e1}	29	Φ _B = 28.5	V _{e1}	14	Φ _C = 20
V _{e2}	27		V _{e2}	26		V _{e2}	28		V _{e2}	26	
30 ≤ Φ _{N_{V0}} ≤ 160			Φ _A ≥ 0.5 Φ _{N_{V0}}			Φ _B ≥ 0.5 Φ _{N_{V0}}			Φ _C ≥ 0.5 Φ _{N_{V0}}		
x	yes	no	x	yes	no	x	yes	no	x	yes	no
Validation of suspension (N _{VB})											
V _{e1}	27	V _{e2}	36	Φ _{N_{VB}}	31.5	30 ≤ Φ _{N_{VB}} (N _{VB} /1000) ≤ 160					
									x	yes	no

Tab No. 1.2 Test suspension

Test suspension N	N	V _{e1}	V _{e1}	Test suspension N ₀ (time = 0)
Φ = 305 x 10 ⁶ = lg 8.48	10 ⁻⁶	296	313	lg N ₀ = lg N/100 = lg 6.48
8.17 ≤ lg N ≤ 8.70	10 ⁻⁷	29	32	6.17 ≤ lg N ₀ ≤ 6.70
				x
				yes
				no

Tab No. 1.3 Testing the efficacy of chemical disinfectant **1226** on *Candida albicans* ATCC 10231

Test concentration (%) / contact time (min) / conditions	Dilution after test procedure	V _{e1}	V _{e2}	lg N _a = lg (Φ _a x 10)	lg R (lg N ₀ = lg 6.48)
100* / 5 / dirty	10 ⁰	<14	<14	< 2.15	≥ 4.33

2. Testing the efficacy of chemical disinfectant **1226** on *Aspergillus brasiliensis* (*niger*) ATCC 16404

Tab No. 2.1 Verification of methodology, dirty conditions

Validation of suspension (N _{V0})			Validation of selected experimental conditions (A)			Neutralizer toxicity control (B)			Method validation (C) Product conc.: 100%*		
V _{e1}	39	Φ _{N_{V0}} = 45.5	V _{e1}	38	Φ _A = 35	V _{e1}	44	Φ _B = 35	V _{e1}	41	Φ _C = 37.5
V _{e2}	52		V _{e2}	32		V _{e2}	26		V _{e2}	34	
30 ≤ Φ _{N_{V0}} ≤ 160			Φ _A ≥ 0.5 Φ _{N_{V0}}			Φ _B ≥ 0.5 Φ _{N_{V0}}			Φ _C ≥ 0.5 Φ _{N_{V0}}		
x	yes	no	x	yes	no	x	yes	no	x	yes	no
Validation of suspension (N _{VB})											
V _{e1}	47	V _{e2}	41	Φ _{N_{VB}}	44	30 ≤ Φ _{N_{VB}} (N _{VB} /1000) ≤ 160					
									x	yes	no

Tab No. 2.2 Test suspension

Test suspension N	N	V _{e1}	V _{e1}	Test suspension N ₀ (time = 0)
Φ = 19 x 10 ⁷ = lg 8.28	10 ⁻⁶	>165	>165	lg N ₀ = lg N/100 = lg 6.28
8.17 ≤ lg N ≤ 8.70	10 ⁻⁷	22	16	6.17 ≤ lg N ₀ ≤ 6.70
				x
				yes
				no

Tab No. 2.3 Testing the efficacy of chemical disinfectant **1226** on *Aspergillus brasiliensis* (*niger*) ATCC 16404

Test concentration (%) / contact time (min) / conditions	Dilution after test procedure	V _{e1}	V _{e2}	lg N _a = lg (Φ _a x 10)	lg R (lg N ₀ = lg 6.28)
100* / 5 / dirty	10 ⁰	<14	<14	< 2.15	≥ 4.13

Note: V_e = value is the number of cfu per ml, Φ = average V_{e1} a V_{e2} (1. + 2. duplicate V_e values), N = the number of cfu/ml of the test suspension, N₀ = the number of cfu/ml of the test suspension at the beginning of the contact time = 0, N_V = the number of cfu/ml of the test suspension for validation, N_{V0} (A,C), N_{VB} (B) = the number of cfu/ml of the test suspensions for validation in the test mixture A, B, C at the beginning of the contact time = 0, N_a = the number of surviving fungi per ml in the test mixture, A, B, C = the number of surviving fungi per ml in control tests (A – experimental conditions control, B – neutralizer toxicity validation, C – method validation), R = N₀ / N_a = the reduction in viability, or lg R = lg N₀ – lg N_a

* The product can only be tested at a concentration of 97% (RTU product, used modified method) or less, as some dilution is always produced by adding the inoculum and interfering substance.

Description: Testing the efficacy of chemical disinfectants and antiseptics

Sample ID: S268/2018

Rep No: 161

Sample name: **1226**

Sampled: by client

Sampling point: Christeyn France S.A., Vertou

Client: Christeyn France S.A., 31, Rue de la Maladrie, Vertou

Sampling date: 8.10.2018

Sample delivered: 10.10.2018

Testing date: 8.11. – 11.11.2018

Delivered amount: 800 ml

Batch No: 367929

Page: 4

3. Evaluation of fungicidal activity of the product **1226**

Tab No. 3.1 The efficacy of chemical disinfectant **1226** on test strains – fungicidal activity

Fungicidal activity of the product (EN 13624:2013)						
Strain	Test temperature [°C]	Contact time [min]	Product test concentrations [%]*	Interfering substances - conditions	lg R EN 13624:2013	lg R
<i>Candida albicans</i> ATCC 10231	20	5	100	dirty	≥ 4	> 4
<i>Aspergillus brasiliensis (niger)</i> ATCC 16404	20	5	100	dirty	≥ 4	> 4

Note: V_c = value is the number of cfu per ml, Φ = average V_{c1} a V_{c2} (1. + 2. duplicate V_c values), N = the number of cfu/ml of the test suspension, N_0 = the number of cfu/ml of the test suspension at the beginning of the contact time = 0, N_v = the number of cfu/ml of the test suspension for validation, N_{v0} (A,C), N_{vB} (B) = the number of cfu/ml of the test suspensions for validation in the test mixture A, B, C at the beginning of the contact time = 0, N_a = the number of surviving fungi per ml in the test mixture, A, B, C = the number of surviving fungi per ml in control tests (A – experimental conditions control, B – neutralizer toxicity validation, C – method validation), $R = N_0 / N_a$ = the reduction in viability, or $lg R = lg N_0 - lg N_a$

* The product can only be tested at a concentration of 97% (RTU product, used modified method) or less, as some dilution is always produced by adding the inoculum and interfering substance.

Prepared by: Ing. Barbora Stoklásková, Lab Technician

Description: *Testing the efficacy of chemical disinfectants and antiseptics*

Sample ID: S268/2018

Rep No: 161

Sample name: **1226**

Sampled: by client

Sampling point: Christeyn France S.A., Vertou

Client: Christeyn France S.A., 31, Rue de la Maladrie, Vertou

Sampling date: 8.10.2018

Sample delivered: 10.10.2018

Testing date: 8.11. – 11.11.2018

Delivered amount: 800 ml

Batch No: 367929

Page: 5

Experimental conditions:

Testing of disinfecting efficiency of chemical disinfecting and antiseptic agents by suspension method

SOP-M-19-00 (EN 13624:2013)

Period of analysis:

8.11. – 11.11.2018

Test temperature:

20 °C ± 1 °C

Test method:

dilution neutralization method

Neutralization medium:

Dey-Engley Neutralizing Broth M 1062

Product diluent:

distilled water

Appearance of the product:

colourless liquid

Test concentration:

20%, 40%, 100% (concentrated)*

Contact time:

5 min

Interfering substances:

3 g/l BSA and 3 ml/l sheep erythrocytes (dirty conditions)

Test organisms:

Candida albicans ATCC 10231

Aspergillus brasiliensis (niger) ATCC 16404

Incubation conditions:

30 °C ± 1 °C, 48 hours and additional period of 24 or 48 hours

Test procedure:

1. Preparation of test suspension
2. Preparation of product test solutions
3. Quantitative suspension test
4. Incubation and calculation
5. Expression and interpretation of results

Note:

Presence of a high concentration (at least 75%) of *Aspergillus brasiliensis* spiny spores in the test suspension – yes.

Fungicidal activity – the capability of a product to produce a reduction in the number of viable fungi belonging to reference strains under defined conditions by at least a 4 lg reduction (10^4).

Yeasticidal activity – the capability of a product to produce a reduction in the number of viable yeast cells of relevant test organisms under defined conditions by at least a 4 lg reduction (10^4).

$R = N_0 / N_a$ = the reduction in viability, or $\lg R = \lg N_0 - \lg N_a$

* Product can only be tested at a concentration of 80% or less, as some dilution is always produced by adding the test organisms and interfering substance.

The standard:

EN 13624:2013 Chemical disinfectants and antiseptics – Quantitative suspension test for the evaluation of fungicidal or yeasticidal activity in the medical area - Test method and requirements (phase 2, step 1) September 2013

Description: Testing the efficacy of chemical disinfectants and antiseptics

Sample ID: S268/2018

Rep No: 161

Sample name: 1226

Sampled: by client

Sampling point: Christeyn France S.A., Vertou

Client: Christeyn France S.A., 31, Rue de la Maladrie, Vertou

Sampling date: 8.10.2018

Sample delivered: 10.10.2018

Testing date: 8.11. – 11.11.2018

Delivered amount: 800 ml

Batch No: 367929

Page: 6

4. Testing the efficacy of chemical disinfectant 1226 on *Candida albicans* ATCC 10231

Tab No. 4.1 Verification of methodology, dirty conditions

Validation of suspension (N_{V0})				Validation of selected experimental conditions (A)				Neutralizer toxicity control (B)				Method validation (C) Product conc.: 100%**					
V_{c1}	27	$\Phi_{N_{V0}} = 35$	$\Phi_A = 33.5$	V_{c1}	37	$\Phi_B = 31.5$	$\Phi_C = 26.5$	V_{c1}	35	$\Phi_B = 31.5$	$\Phi_C = 26.5$	V_{c1}	25	$\Phi_C = 26.5$	$\Phi_C = 26.5$		
V_{c2}	43			V_{c2}	30			V_{c2}	28			V_{c2}	28				
$30 \leq \Phi_{N_{V0}} \leq 160$				$\Phi_A \geq 0.5 \Phi_{N_{V0}}$				$\Phi_B \geq 0.5 \Phi_{N_{V0}}$				$\Phi_C \geq 0.5 \Phi_{N_{V0}}$					
x	yes		no	x	yes		no	x	yes		no	x	yes		no		
Validation of suspension (N_{VB})				V_{c1}	41	V_{c2}	31	Φ_{NVB}	36	$30 \leq \Phi_{NVB} (N_{VB}/1000) \leq 160$							
												x	yes		no		

Tab No. 4.2 Test suspension

Test suspension N	N	V_{c1}	V_{c1}	Test suspension N_0 (time = 0)			
$\Phi = 34 \times 10^6 = \lg 7.53$	10^{-5}	> 330	> 330	$\lg N_0 = \lg N/10 = \lg 6.53$			
$7.17 \leq \lg N \leq 7.70$	10^{-6}	33	35	$6.17 \leq \lg N_0 \leq 6.70$			
				x	yes		no

Tab No. 4.3 Testing the efficacy of chemical disinfectant 1226 on *Candida albicans* ATCC 10231

Test concentration (%) / contact time (min) / conditions	Dilution after test procedure	V_{c1}	V_{c2}	$\lg N_a = \lg (\Phi_a \times 10)$	$\lg R$ ($\lg N_0 = \lg 6.53$)
20 / 5 / dirty	10^0	<14	<14	< 2.15	≥ 4.38
40 / 5 / dirty	10^0	<14	<14	< 2.15	≥ 4.38
100* / 5 / dirty	10^0	<14	<14	< 2.15	≥ 4.38

5. Testing the efficacy of chemical disinfectant 1226 on *Aspergillus brasiliensis* (niger) ATCC 16404

Tab No. 5.1 Verification of methodology, dirty conditions

Validation of suspension (N_{V0})				Validation of selected experimental conditions (A)				Neutralizer toxicity control (B)				Method validation (C) Product conc.: 100%**					
V_{c1}	42	$\Phi_{N_{V0}} = 46.5$	$\Phi_A = 44$	V_{c1}	54	$\Phi_B = 35$	$\Phi_C = 41.5$	V_{c1}	48	$\Phi_B = 35$	$\Phi_C = 41.5$	V_{c1}	53	$\Phi_C = 41.5$	$\Phi_C = 41.5$		
V_{c2}	51			V_{c2}	34			V_{c2}	22			V_{c2}	30				
$30 \leq \Phi_{N_{V0}} \leq 160$				$\Phi_A \geq 0.5 \Phi_{N_{V0}}$				$\Phi_B \geq 0.5 \Phi_{N_{V0}}$				$\Phi_C \geq 0.5 \Phi_{N_{V0}}$					
x	yes		no	x	yes		no	x	yes		no	x	yes		no		
Validation of suspension (N_{VB})				V_{c1}	53	V_{c2}	41	Φ_{NVB}	47	$30 \leq \Phi_{NVB} (N_{VB}/1000) \leq 160$							
												x	yes		no		

Tab No. 5.2 Test suspension

Test suspension N	N	V_{c1}	V_{c1}	Test suspension N_0 (time = 0)			
$\Phi = 45 \times 10^6 = \lg 7.65$	10^{-5}	> 165	> 165	$\lg N_0 = \lg N/10 = \lg 6.65$			
$7.17 \leq \lg N \leq 7.70$	10^{-6}	37	53	$6.17 \leq \lg N_0 \leq 6.70$			
				x	yes		no

Tab No. 5.3 Testing the efficacy of chemical disinfectant 1226 on *Aspergillus brasiliensis* (niger) ATCC 16404

Test concentration (%) / contact time (min) / conditions	Dilution after test procedure	V_{c1}	V_{c2}	$\lg N_a = \lg (\Phi_a \times 10)$	$\lg R$ ($\lg N_0 = \lg 6.65$)
20 / 5 / dirty	10^{-3}	26	19	5.35	1.30
40 / 5 / dirty	10^0	<14	<14	< 2.15	≥ 4.50
100* / 5 / dirty	10^0	<14	<14	< 2.15	≥ 4.50

Note: V_c = value is the number of cfu per ml, Φ = average V_{c1} a V_{c2} (1. + 2. duplicate V_c values), N = the number of cfu/ml of the test suspension, N_0 = the number of cfu/ml of the test suspension at the beginning of the contact time = 0, N_V = the number of cfu/ml of the test suspension for validation, N_{V0} (A,C), N_{VB} (B) = the number of cfu/ml of the test suspensions for validation in the test mixture A, B, C at the beginning of the contact time = 0, N_a = the number of surviving fungi per ml in the test mixture, A, B, C = the number of surviving fungi per ml in control tests (A – experimental conditions control, B – neutralizer toxicity validation, C – method validation), $R = N_0 / N_a$ = the reduction in viability, or $\lg R = \lg N_0 - \lg N_a$

* Product can only be tested at a concentration of 80% or less, as some dilution is always produced by adding the test organisms and interfering substance.

Description: Testing the efficacy of chemical disinfectants and antiseptics

Sample ID: S268/2018

Rep No: 161

Sample name: **1226**

Sampled: by client

Sampling point: Christeyn France S.A., Vertou

Client: Christeyn France S.A., 31, Rue de la Maladie, Vertou

Sampling date: 8.10.2018

Sample delivered: 10.10.2018

Testing date: 8.11. – 11.11.2018

Delivered amount: 800 ml

Batch No: 367929

Page: 7

6. Evaluation of fungicidal activity of the product **1226**

Tab No. 6.1 The efficacy of chemical disinfectant **1226** on test strains – fungicidal activity

Fungicidal activity of the product (EN 13624:2013)						
Strain	Test temperature [°C]	Contact time [min]	Product test concentrations [%]	Interfering substances - conditions	lg R EN 13624:2013	lg R
<i>Candida albicans</i> ATCC 10231	20	5	20	dirty	≥ 4	> 4
<i>Aspergillus brasiliensis (niger)</i> ATCC 16404	20	5	20	dirty	≥ 4	< 4
<i>Candida albicans</i> ATCC 10231	20	5	40	dirty	≥ 4	> 4
<i>Aspergillus brasiliensis (niger)</i> ATCC 16404	20	5	40	dirty	≥ 4	> 4
<i>Candida albicans</i> ATCC 10231	20	5	100*	dirty	≥ 4	> 4
<i>Aspergillus brasiliensis (niger)</i> ATCC 16404	20	5	100*	dirty	≥ 4	> 4

Note: V_c = value is the number of cfu per ml, Φ = average V_{c1} a V_{c2} (1. + 2. duplicate V_c values), N = the number of cfu/ml of the test suspension, N_0 = the number of cfu/ml of the test suspension at the beginning of the contact time = 0, N_V = the number of cfu/ml of the test suspension for validation, N_{V0} (A,C), N_{VB} (B) = the number of cfu/ml of the test suspensions for validation in the test mixture A, B, C at the beginning of the contact time = 0, N_a = the number of surviving fungi per ml in the test mixture, A, B, C = the number of surviving fungi per ml in control tests (A – experimental conditions control, B – neutralizer toxicity validation, C – method validation), $R = N_0 / N_a$ = the reduction in viability, or $lg R = lg N_0 - lg N_a$

* Product can only be tested at a concentration of 80% or less, as some dilution is always produced by adding the test organisms and interfering substance.

Prepared by: Ing. Barbora Stoklásková, Lab Technician

Description: Testing the efficacy of chemical disinfectants and antiseptics

Sample ID: S268/2018

Rep No: 161

Sample name: **1226**

Sampled: by client

Sampling point: Christeyn France S.A., Vertou

Client: Christeyn France S.A., 31, Rue de la Maladrie, Vertou

Sampling date: 8.10.2018


Sample delivered: 10.10.2018

Testing date: 8.11. – 11.11.2018

Delivered amount: 800 ml

Batch No: 367929

Page: 8

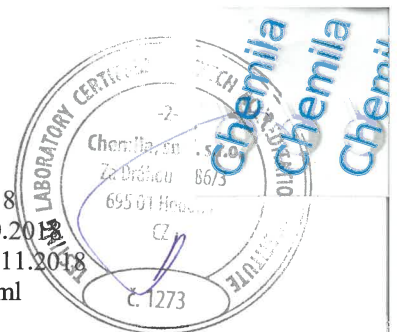

Interpretation:

Results of tests are in Tabs.

According to EN 13624:2013 the tested product **1226**, batch No. 367929, in the concentrations 100%(97%)*, 100%(80%)*, 40% and 20%, diluted in distilled water, in the contact time 5 min under dirty conditions at temperature 20 °C ± 1 °C by the dilution neutralization method **decreased** the number vegetative yeast cells of *Candida albicans* ATCC 10231 by at least a 4 lg reduction.

According to EN 13624:2013 the tested product **1226**, batch No. 367929, in the concentrations 100%(97%)*, 100%(80%)* and 40%, diluted in distilled water, in the contact time 5 min under dirty conditions at temperature 20 °C ± 1 °C by the dilution neutralization method **decreased** of mould spores of *Aspergillus brasiliensis (niger)* ATCC 16404 by at least a 4 lg reduction.

* Product can only be tested at a concentration of 97% (RTU product) or less, as some dilution is always produced by adding the test organisms and interfering substance or product can only be tested at a concentration of 80% or less, as some dilution is always produced by adding the test organisms and interfering substance.

** The test strain was used according to client's request.

Conclusion:

The product **1226** is capable of reducing the number vegetative yeast cells and the number of mould spores of the relevant organisms under defined conditions to the declared values, and consequently, may be called fungicidal.

12.2.2019, Hodonín

Ing. Eva Kremlová, Leader of Study


**Evaluation des activités bactéricide et levuricide sur des surfaces non poreuses
selon la norme NF EN 16615 : 2015**

Produit : 1226– lot PR436-1226.170317

Donneur d'ordre : **Christeyns France**
31, rue de la Maladrie
44120 Vertou
France

Loos, le 30/05/2017

Mélinda MAUX, Ph.D
Responsable du laboratoire



Le rapport d'essai comporte : 5 pages
*L'accréditation du COFRAC atteste de la compétence des laboratoires pour les seuls essais couverts par l'accréditation.
La reproduction de ce rapport d'essai n'est autorisée que sous sa forme intégrale.
Ce rapport d'essai ne concerne que l'échantillon soumis à essais.*

1 PRINCIPE

Les activités bactéricides et levuricide ont été déterminées selon la norme **NF EN 16615** : "Antiseptiques et désinfectants chimiques – Méthode d'essai quantitative pour l'évaluation de l'activité bactéricide et levuricide sur de surfaces non poreuses, avec action mécanique à l'aide de lingettes dans le domaine médical (Essai à 4 zones) – Méthode d'essai et prescriptions (Phase 2, étape 2)." Mai 2015.

2 IDENTIFICATION DE(S) ECHANTILLON(S)

Nom(s) : **1226– lot PR436-1226.170317**

Société : **Christeyns France**

Date de réception au laboratoire : **21/03/2017**

Conditions de stockage au laboratoire : **Température ambiante, à l'abri de la lumière**

Aspect du produit à réception : **liquide, incolore**

3 METHODE D'ESSAI ET VALIDATION

- Méthode de neutralisation : **Dilution neutralisation** (dénombrement par inclusion)

- Diluant neutralisant : **thiosulphate Sodium 14 g/l**

4 CONDITIONS EXPERIMENTALES

Période d'analyse : **Du 23/03/2017 au 27/04/2017**

Souche(s) de référence testée(s) : **voir tableau(x) page(s) suivante(s)**

Conservation et entretien au laboratoire conformément à la norme **EN 12353**

Concentration(s) du produit soumis à essai : **voir tableau(x) page(s) suivante(s)**

Diluant du produit utilisé au cours des essais: **Eau distillée**

Aspect des dilutions de produit : **incolore, homogène.**

Substance interférente : **Albumine bovine 3g/L + érythrocytes de mouton 3 mL/L** (conditions de saleté)

Température de contact : **20°C ± 2.5 °C**

Temps de contact : **5 minutes ± 15 secondes**

Température d'incubation : **37°C ± 1°C**

Identification surface d'essai : **PVC avec revêtement polyuréthane en surface** (dimension 20 cm x 50 cm)

Identification de la masse unitaire : **Bloc de granit** (dimension 12 cm x 8,6 cm x 8,6 cm)

Identification de la lingette utilisée : **Lingette de référence** (dimension 17,5 cm x 28cm : 55% pâte de bois, 45% polyéthylènetéréphthalate (PET))

Conditions de séchage : **<60 minutes** à la température de l'essai

5 RESULTATS EXPERIMENTAUX

Vérification de la méthodologie et de la validation de la méthode dilution-neutralisation

(Essais réalisés en parallèle à l'essai proprement dit)

Souche(s) d'essai	Nombre de cellules viables (UFC/ml)		
	Suspension de validation Nv ₀	Témoin du neutralisant B	Validation de la méthode C product concentration: 100%
<i>Pseudomonas aeruginosa</i> DSM 939	VC1 : 73 VC2 : 94 Nv ₀ : 83.5	VC1 : 98 VC2 : 91 B : 94.5	VC1 : 79 VC2 : 81 C : 80
<i>Enterococcus hirae</i> DSM 3320	VC1 : 145 VC2 : 126 Nv ₀ : 135.5	VC1 : 133 VC2 : 137 B : 135	VC1 : 119 VC2 : 119 C : 119
<i>Staphylococcus aureus</i> DSM 799	VC1 : 36 VC2 : 42 Nv ₀ : 39	VC1 : 34 VC2 : 34 B : 34	VC1 : 46 VC2 : 41 C : 43.5
<i>Candida albicans</i> DSM 1386	VC1 : 130 VC2 : 135 Nv ₀ : 132.5	VC1 : 126 VC2 : 136 B : 131	VC1 : 140 VC2 : 141 C : 140.5

10* : nombre d'UFC comptées à la dilution x

Critères de validation :
Nv₀ compris entre 30 UFC/mL et 160 UFC/mL
B ≥ 0,5 Nv₀
C ≥ 0,5 Nv₀

Contrôles pour l'essai proprement-dit (méthode par dilution-neutralisation)

Souche(s) d'essai	Nombre de cellules viables pour l'essai T sur les zones tests 2 à 4 (UFC/25 cm ²) pour le mélange d'essai aux concentrations v/v)		Nombre de cellules viables pour le Témoin eau NW sur les zones tests 2 à 4 (UFC/25 cm ²) pour le mélange d'essai aux concentrations (v/v)
	1%	100%	1%
<i>Pseudomonas aeruginosa</i> DSM 939	VC T ₂ : 16 ; 16 VC T ₃ : 36 ; 32 VC T ₄ : 118 ; 97 V T _{2 à 4} : 262.5	VC T ₂ : 0 ; 0 VC T ₃ : 0 ; 0 VC T ₄ : 0 ; 0 V T _{2 à 4} : <14	VC T ₂ : >330 ; >330 VC T ₃ : >330 ; >330 VC T ₄ : 198 ; 217 V _{Nw T_{2 à 4}} : >1650
<i>Enterococcus hirae</i> DSM 3320	VC T ₂ : 166 ; 126 VC T ₃ : 14 ; 16 VC T ₄ : 0 ; 0 V T _{2 à 4} : 268.3	VC T ₂ : 0 ; 0 VC T ₃ : 0 ; 0 VC T ₄ : 0 ; 0 V T _{2 à 4} : <14	VC T ₂ : >330 ; >330 VC T ₃ : >330 ; >330 VC T ₄ : >330 ; >330 V _{Nw T_{2 à 4}} : >1650
<i>Staphylococcus aureus</i> DSM 799	VC T ₂ : 14 ; 18 VC T ₃ : 7 ; 9 VC T ₄ : 43 ; 36 V T _{2 à 4} : 106	VC T ₂ : 0 ; 0 VC T ₃ : 0 ; 0 VC T ₄ : 0 ; 0 V T _{2 à 4} : <14	VC T ₂ : 22 ; 15 VC T ₃ : 34 ; 34 VC T ₄ : 4 ; 0 V _{Nw T_{2 à 4}} : 90.8
<i>Candida albicans</i> DSM 1386	VC T ₂ : 51 ; 54 VC T ₃ : 26 ; 30 VC T ₄ : 0 ; 0 V T _{2 à 4} : 134.17	VC T ₂ : 0 ; 0 VC T ₃ : 0 ; 0 VC T ₄ : 0 ; 0 V T _{2 à 4} : <14	VC T ₂ : >330 ; >330 VC T ₃ : 51 ; 74 VC T ₄ : 60 ; 60 V _{Nw T_{2 à 4}} : >1650

Critères de validation :
V_{T_{2 à 4}} ≤ 50 UFC / 25 cm²
V_{Nw T_{2 à 4}} > 10 UFC / 25 cm²

Résultats de l'essai proprement-dit vis-à-vis des bactéries

Souche(s) d'essai	Suspension d'essai N et No	Témoin de séchage D _{co}	Témoin temps de contact D _{ct}	Nombre de cellules viables pour la zone d'essai 1 Na (UFC/ml) pour le mélange d'essai aux concentrations (v/v)	
				1%	100%
<i>Pseudomonas aeruginosa</i> DSM 939	10 ⁻⁷ : >330 ; >330 10 ⁻⁸ : 38 ; 41 Log N : 9.60 Log No : 8.30	10 ⁻⁴ : 212 ; 225 10 ⁻⁵ : 24 ; 21 Log Dco : 7.04	10 ⁻⁴ : 175 ; 169 10 ⁻⁵ : 17 ; 17 Log Dct : 6.93	10 ⁰ : >330 ; >330 10 ⁻¹ : 46 ; 41 Na : 2.18x10 ³ Log Na : 3.38	10 ⁰ : 0 ; 0 10 ⁻¹ : 0 ; 0 Na : <70 Log Na : <1.85
<i>Enterococcus hirae</i> DSM 3320	10 ⁻⁷ : 163 ; 163 10 ⁻⁸ : 17 ; 18 Log N : 9.22 Log No : 7.91	10 ⁻⁴ : 155 ; 137 10 ⁻⁵ : 27 ; 20 Log Dco : 6.89	10 ⁻⁴ : 161 ; 171 10 ⁻⁵ : 10 ; 14 Log Dct : 6.92	10 ⁰ : >330 ; >330 10 ⁻¹ : >330 ; >330 Na : >1.6x10 ³ Log Na : >3.22	10 ⁰ : 0 ; 0 10 ⁻¹ : 0 ; 0 Na : <70 Log Na : <1.85
<i>Staphylococcus aureus</i> DSM 799	10 ⁻⁷ : 152 ; 165 10 ⁻⁸ : 16 ; 18 Log N : 9.20 Log No : 7.90	10 ⁻⁴ : >330 ; >330 10 ⁻⁵ : 261 ; 255 Log Dco : 8.11	10 ⁻⁴ : >330 ; >330 10 ⁻⁵ : 192 ; 152 Log Dct : 7.93	10 ⁰ : >330 ; >330 10 ⁻¹ : >330 ; >330 Na : >1.6x10 ³ Log Na : >3.22	10 ⁰ : 0 ; 0 10 ⁻¹ : 0 ; 0 Na : <70 Log Na : <1.85
10 ^x : nombre d'UFC comptées à la dilution x					
Critères de validation: Log N compris entre 9.17 et 9.70 Log Dco et Log Dct compris entre 6.88 et 8.40					

Réduction (R) du nombre de cellules viables aux concentrations d'essai testées (v/v) :

Souche(s) d'essai	1%	100%
<i>Pseudomonas aeruginosa</i> DSM 939	Log R : 3.55	Log R : >5.08
<i>Enterococcus hirae</i> DSM 3320	Log R : <1.85	Log R : >5.07
<i>Staphylococcus aureus</i> DSM 799	Log R : <4.71	Log R : >6.08
Réduction R : log R = log Dct - log Na		
Critères d'interprétation : concentration active si R ≥ 5 concentration non active si R < 5		

Résultats de l'essai proprement-dit vis-à-vis de la levure

Souche(s) d'essai	Suspension d'essai N et No	Témoin de séchage D _{co}	Témoin temps de contact D _{ct}	Nombre de cellules viables pour la zone d'essai 1 Na (UFC/ml) pour le mélange d'essai aux concentrations (v/v)	
				1%	100%
<i>Candida albicans</i> DSM 1386	10 ⁻⁶ : 161 ; 169 10 ⁻⁷ : 24 ; 18 Log N : 8.23 Log No : 6.93	10 ⁻³ : 256 ; 265 10 ⁻⁴ : 41 ; 42 log Dco : 6.14	10 ⁻³ : 166 ; 178 10 ⁻⁴ : 18 ; 22 log Dct : 5.94	10 ⁰ : >330 ; >330 10 ⁻¹ : 96 ; 107 Na : 3.71 Log Na : 2.23	10 ⁰ : 0 ; 0 10 ⁻¹ : 0 ; 0 Na : <70 Log Na : <1.85
10 ^x : nombre d'UFC comptées à la dilution x					
Critères de validation: Log N compris entre 8.17 et 8.70 Log Dco et Log Dct compris entre 5.88 et 7.40					

Réduction (R) du nombre de cellules viables aux concentrations d'essai testées (v/v) :

Souche(s) d'essai	1%	100%
<i>Candida albicans</i> DSM 1386	Log R : 2.23	Log R : >4.09
Réduction R : log R = log Dct - log Na		
Critères d'interprétation : concentration active si R ≥ 4 concentration non active si R < 4		

6 CONCLUSION

Selon la norme NF EN 16615 (mai 2015), le produit 1226– lot PR436-1226.170317, présente une activité bactéricide et levuricide sur les surfaces, testé à la concentration de 100 % (v/v), après 5 minutes de contact à 20° C, en conditions de saleté (3,0 g/l d'albumine bovine + érythrocytes de mouton).

DR. JOCHEN STEINMANN
Resp. techn. et scient.
chez MikroLab GmbH

Norderoog 2
D-28259 Bremen

Tél.:+49 (421) 27819102
Fax:+49 (421) 2760283
<http://www.mikrolab-gmbh.de>
E-mail: MikroLab.GmbH@t-online.de

MikroLab GmbH, Norderoog 2, D-28259 Bremen

11.06.2013
Dr St/NM

Christeyns France SA
9, rue Marcel Sembat
44100 NANTES
FRANCE

**Efficacité contre polio virus du produit 1226 IND01 lors d'un essai de suspension
quantitatif à 20 °C en conditions de saleté**

RAPPORT D'EXPERTISE

Le désinfectant pour les surfaces 1226 IND01 de Christeyns France SA a été testé pour son efficacité à inactiver poliovirus type 1, souche LSc-2ab suivant la norme prEN 14476:2011.

Dans la norme prEN 14476:2011, on conclut à l'efficacité anti-virus d'un désinfectant si, après un temps d'action défini, la réduction du titre viral initial est supérieure ou égale à ≥ 4 unités \log_{10} (inactivation $\geq 99,99$ %).

Le désinfectant pour les surfaces 1226 IND01 a été utilisé non dilué à 20 °C, en 5, 10 et 15 minutes de temps de contact. Après 15 minutes une réduction du titre de virus \geq quatre unités \log_{10} a été constatée. L'efficacité est donc obtenue avec 1226 IND01:

non dilué 15 minutes


Dr. Jochen Steinmann
Norderoog 2
D-28259 Bremen



11.06.2013

Test report P13ML1536-2Po

Evaluation of the effectiveness of **1226 IND01**

Test virus: poliovirus type 1 strain LSc-2ab

Method: prEN 14476:2011 (dirty conditions)

quantitative suspension test for the evaluation of
virucidal activity of chemical disinfectants and
antiseptics used in human medicine

Sponsor:

Christeyns France SA
9, rue Marcel Sembat
44100 NANTES





1. Introduction

The objective of this study was to evaluate the virus-inactivating properties of the surface disinfectant 1226 IND01 against poliovirus type 1 using a quantitative suspension assay according to prEN 14476:2011 (1) under dirty conditions.

2. Test laboratory

MikroLab GmbH, Norderoog 2, D-28259 Bremen

3. Identification of the sample

Manufacturer	Christeyns France SA
Name of product	1226 IND01
Batch number	16.04.13
Application	surface disinfection
Production date	16.04.2013
Expiry date	-
Active compound (s) (100 g)	peracetic acid (CAS no.: 79-21-0)
Appearance, odour	clear, colourless liquid product specific
pH-values (in WSH)	undiluted: 2.21 (20 °C)
Storage conditions	room temperature in the dark (area with restricted access)
Date of arrival in the laboratory	25.04.2013

4. Materials

4.1 Culture medium and reagents

- Dulbecco`s Modified Eagle`s Medium (DMEM, Lonza Group Ltd., catalogue no. BE12-707F)
- Fetal calf serum (Biochrom AG, article no. S 0115)
- 1.4 % formaldehyde solution (Chemisch-technologisches Laboratorium Dr. Melzer, D-28199 Bremen)
- Aqua bidest. (Fresenius Kabi Deutschland, article no. P2N 1636071)
- PBS (Invitrogen, article no. 18912-014)
- BSA (Sigma-Aldrich-Chemie GmbH, article no. CA-2153)



- sheep erythrocytes (Fiebig-Nährstofftechnik; article no. 31100100).

4.2 Virus and cells

The poliovirus type 1 strain LSc-2ab (Chiron-Behring) was obtained from PD Dr. Olaf Thraenhart, Eurovir, D-14943 Luckenwalde.

BGM cells (*buffalo green monkey* = permanent monkey kidney cell line; supplied by Prof. Dr. Lindl, Institut für angewandte Zellkultur, D-81669 München, Germany) were cultivated in a 175 cm² flask with Dulbecco`s Modified Eagle`s Medium (DMEM) and 10 % fetal calf serum (FCS).

The cells (passage 34) were inspected regularly for morphological alterations and for contamination by mycoplasmas. No morphological alterations of cells and no contamination by mycoplasmas could be detected.

4.3 Apparatus, glassware and small items of equipment

- CO₂ incubator, Nunc GmbH & Co. KG, model QWJ 350
- Agitator (Vortex Genie Mixer, type G 560E)
- pH measurement 315i (WTW, article no. 2A10-100)
- Centrifuge (Sigma-Aldrich-Chemie GmbH, type 113)
- Microscope (Olympus, type CK 30)
- Centrifuge 5804 R (Eppendorf AG)
- Water bath (JULABO, Julabo U 3)
- Adjustable volume automatic pipettes (Eppendorf AG)
- Polysterol 96-well microtitre plate (Nunc GmbH & Co. KG, Wiesbaden, Germany)
- Cell culture flask (Nunc GmbH & Co. KG, Wiesbaden, Germany)
- Sealed test tubes (Sarstedt AG & Co., Nümbrecht, Germany).



5. Experimental conditions

Test temperature	20 °C ± 1 °C
Concentration of test product	undiluted (97.0 % and 80.0 %) and as 10.0 % (non-active range) solution
Contact times	5, 10 and 15 minutes
Interfering substance(s)	dirty conditions: 3.0 g/l bovine serum albumin (BSA) + 3.0 g/l erythrocytes
Diluent	water (10.0 % solution)
Stability of product in the mix with virus and interfering substance (97.0 % and 80.0 % solutions)	no flocculation
Procedure to stop action of product	immediate dilution
Test virus	poliovirus type 1 strain LSc-2ab (Chiron-Behring)
Period of analysis	25.04.2013 – 11.06.2013
End of testing	11.06.2013

6. Methods

6.1 Preparation of test virus suspension

For preparation of test virus suspension according to prEN 5.4.1, *BGM cells* were infected with a multiplicity of infection of 0.1 at 37 °C. After cells showed a cytopathic effect, they were subjected to a threefold freeze/thaw procedure followed by a low speed centrifugation (10 min and 1000 x g) in order to sediment cell debris. After aliquotation of the supernatant, test virus suspension was stored at -80 °C.

6.2 Disinfectant

The test product was tested undiluted under dirty conditions (1 part test virus suspension + 1 part interfering substance + 8 parts disinfectant). Due to the addition of test virus suspension and interfering substance an 80.0 % solution resulted. Additionally, the 97.0 % solution under dirty conditions was evaluated (0.1 parts virus suspension + 0.2 interfering substance (5x) + 9.7 parts disinfectant).

Furthermore the product was examined as 10.0 % (demonstration of non-active range) solution. This solution was prepared with water immediately before the inactivation tests.



6.3 Infectivity assay

Infectivity was determined as endpoint titration according to prEN 5.5 transferring 0.1 ml of each dilution into eight wells of a microtitre plate to 0.1 ml of freshly trypsinised *BGM cells* ($10\text{-}15 \times 10^3$ cells per well), beginning with the highest dilution. Microtitre plates were incubated at 37 °C in a 5 % CO₂-atmosphere. The cytopathic effect was read by using an inverted microscope after seven days. Calculation of the infective dose TCID₅₀/ml was calculated with the method of Spearman (2) and Kärber (3) with the following formula:

$$-\log_{10}\text{TCID}_{50} = X_0 - 0.5 + \sum r/n$$

meaning

X_0 = log₁₀ of the lowest dilution with 100 % positive reaction

r = number of pos. determinations of lowest dilution step with 100 % positive and all higher positive dilution steps

n = number of determinations for each dilution step.

6.4 Calculation and verification of virucidal activity

The virucidal activity of the test disinfectant was evaluated by calculating the decrease in titre in comparison with the control titration without disinfectant. The difference is given as reduction factor (RF).

According to the prEN 14476:2011, a disinfectant or a disinfectant solution at a particular concentration is having virus-inactivating efficacy if the titre is reduced at least by four log₁₀ steps within the recommended exposure period. This corresponds to an inactivation of ≥ 99.99 %.

6.5 Inactivation assay

Determination of virucidal activity has been carried out in accordance to prEN 5.5. The test product 1226 IND01 was examined undiluted (97.0 % and 80.0 %) and as 10.0 % solution at 20 °C. 5, 10 and 15 minutes were chosen as exposure times.

Due to a more convenient handling, the volumes in this assay were 0.1 ml test virus suspension, 0.1 ml interfering substance and 0.8 ml test product (80.0 % assay) or 0.01 ml test virus suspension and 0.02 ml interfering substance and 0.97 ml test product (97.0 % assay). Immediately at the end of a chosen contact time, activity of the disinfectant was stopped by dilution to 10⁻⁸.



Titration of the virus control was performed after the longest exposure time (prEN 5.5.7).

Furthermore, a cell control (only addition of medium) was incorporated.

Inactivation tests were carried out in sealed test tubes in a water bath at $20\text{ °C} \pm 1.0\text{ °C}$. Aliquots were retained after appropriate exposure times, and residual infectivity was determined.

6.6 Determination of cytotoxicity

Determination of cytotoxicity was performed according to prEN 5.5.4.1 with 100 µl water, 100 µl interfering substance and 800 µl test product (80.0 % assay) and with 10 µl water, 20 µl interfering substance (5x) and 970 µl test product (97.0 % assay).

6.7 Cell sensitivity to virus

For the control of cell sensitivity to virus 0.3 parts by volume hard water were mixed with 9.7 parts by volume of the lowest apparently non-cytotoxic dilution of the product. This mixture or PBS as control was added to a volume of double concentrated cell suspension. After 1 h at 37 °C the cells were centrifuged and re-suspended in cell culture medium (prEN 6.6.4.2b). Finally, a comparative titration of the test virus suspension was performed on the pre-treated (disinfectant) and non-pre-treated (PBS) cells as described above.

6.8 Control of efficacy for suppression of disinfectant activity

Furthermore, a control of efficiency for suppression of disinfectant activity was included (prEN 5.5.4.1).

6.9 Reference virus inactivation test

As reference for test validation a 0.7 % formaldehyde solution according to prEN 5.5.6.1 was included. 5, 15, 30 and 60 minutes were chosen as contact times. In addition, cytotoxicity of formaldehyde test solution was determined following prEN 6.6.7.2 with dilutions up to 10^{-5} .

7. Verification of the methodology

The following criteria as mentioned in prEN 5.7 were fulfilled:

- a) The titre of the test virus suspension allowed the determination of a $\geq 4\text{ log}_{10}$ reduction.



- b) The test product was cytotoxic in the 1:100 dilutions (97.0 % and 80.0 %) thus allowing the demonstration of a 4 log₁₀ reduction.
- c) The difference of the logarithmic titre of the virus control minus the logarithmic titre of the test virus in the reference inactivation test (see prEN 5.7b) was 1.88 ± 0.66 (between 0.5 - 2.5) after 30 min and 3.13 ± 0.57 (between 2.0 - 4.5) after 60 min for poliovirus type 1.
- d) The comparative titration on pre-treated (disinfectant) and non-pre-treated (PBS) *BGM cells* showed no significant difference ($< 1 \log_{10}$; prEN 5.7) of virus titre: 8.13 ± 0.45 (PBS) versus 8.00 ± 0.44 (1:1,000 dilutions of disinfectant) log₁₀TCID₅₀/ml.
- e) The control of efficacy for suppression of disinfectant activity (undiluted, 97.0 % solution) showed no decrease in virus titre.

Since all criteria according prEN 5.7 were fulfilled, examination with poliovirus type 1 according to prEN 14476:2011 is valid.

8. Results

Results of examination are shown in tables 1 to 8. Tables 1 to 7 demonstrate the raw data, whereas table 8 (a + b) gives a summary of results.

The test product (97.0 %) was able to inactivate poliovirus type 1 after 15 minutes exposure time in this quantitative suspension test. The following reduction factors were measured at this time point: 4.25 ± 0.33 and $\geq 4.13 \pm 0.43$ (mean value $\geq 4.19 \pm 0.27$) (Tables 1 and 2). This corresponded to an inactivation of ≥ 99.99 %.

Tested in an 80.0 % assay, 1226 IND01 was not active within 15 minutes exposure time (Table 3).

The 10.0 % solution of 1226 IND01 was in addition not active against the poliovirus type 1 after 15 minutes of exposure time as well (Table 4).



9. Summary

The surface disinfectant 1226 IND01 demonstrated activity under dirty conditions against poliovirus type 1 undiluted (97.0 %) after a contact time of 15 minutes. Due to the lack of virological guidelines simulating practical conditions in Europe (phase 2, step 2 tests) the data of this quantitative suspension test lead to the recommendation to use 1226 IND01 for inactivation of poliovirus type 1 as follows:

undiluted 15 minutes

Bremen, 11.06.2013



- Dr. Jochen Steinmann -



10. Quality control

The Quality Assurance of the results was maintained by performing the determination of the virus-inactivating properties of the disinfectant in accordance with Good Laboratory Practice regulations:

- 1) Chemicals Act of Germany, Appendix 1, dating of 01.08 1994 (BGBl. I, 1994, page 1703). Appendix revised at 14. 05. 1997 (BGBl. I, 1997, page 1060).
- 2) OECD Principles of Good Laboratory Practice (revised 1997); OECD Environmental Health and Safety Publications; Series on Principles of Good Laboratory Practice and Compliance Monitoring – Number 1. Environment Directorate, Organization for Economic Co-operation and Development, Paris 1998.

The plausibility of the results was additionally confirmed by controls incorporated in the inactivation assays.

11. Records to be maintained

All testing data, protocol, protocol modifications, the final report, and correspondence between MikroLab GmbH and the sponsor will be stored in the archives at MikroLab GmbH.

The use of the MikroLab GmbH name, logo or any other representation of MikroLab GmbH, other than distribution of this report in it's entirety, without the written approval of MikroLab GmbH is prohibited. In addition, MikroLab GmbH may not be referred to in any form of promotional materials, press releases, advertising or similar materials (whether by print, broadcast, communication or electronic means) without the express permission of MikroLab GmbH.



12. Literature

1. prEN 14476:2011: Chemical disinfectants and antiseptics – Quantitative suspension test for the evaluation of virucidal activity of chemicals disinfectants and antiseptics in human medicine test - Test method and requirements (phase 2, step 1)
2. Spearman, C.: The method of `right or wrong cases` (constant stimuli) without Gauss's formulae.
Brit J Psychol; 2, 1908, 227-242
3. Kärber, G.: Beitrag zur kollektiven Behandlung pharmakologischer Reihenversuche.
Arch Exp Path Pharmac; 162, 1931, 480-487



Appendix:

Table 1:	Raw data for 1226 IND01 (97.0 %) tested against poliovirus type 1 at 20 °C (1 st assay)
Table 2:	Raw data for 1226 IND01 (97.0 %) tested against poliovirus type 1 at 20 °C (2 nd assay)
Table 3:	Raw data for 1226 IND01 (80.0 %) tested against poliovirus type 1 at 20 °C
Table 4:	Raw data for 1226 IND01 (10.0 %) tested against poliovirus type 1 at 20 °C
Table 5:	Raw data for formaldehyde solution (0.7 %) tested against poliovirus type 1 at 20 °C
Table 6:	Raw data for control of efficacy for suppression of disinfectant activity (97.0 %)
Table 7:	Raw data (poliovirus type 1) for cell sensitivity (97.0 %)
Table 8 (a+b):	Summary of results with 1226 IND01 and poliovirus type 1



Table 1: Raw data for 1226 IND01 (97.0 %) tested against poliovirus type 1 at 20 °C (quantal test; 8 wells) (3219) (1st assay)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)									
				1	2	3	4	5	6	7	8	9	
test product	97.0%	dirty conditions	5	tttt	tttt	4444	4444	4444	0040	0000	0000	n.d.	
				tttt	tttt	4444	4444	4444	0440	4000	0000	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product cytotoxicity	97.0%	dirty conditions	15	tttt	tttt	4444	0000	0000	0000	0000	0000	n.d.	
				tttt	tttt	4444	0000	0000	0000	0000	0000	0000	n.d.
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
formaldehyde	0.7% (m/V)	PBS	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
formaldehyde cytotoxicity	0.7% (m/V)	PBS	15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
virus control	n.a.	dirty conditions	30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
virus control	n.a.	dirty conditions	60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
virus control	n.a.	dirty conditions	0	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
virus control	n.a.	dirty conditions	60	4444	4444	4444	4444	4444	4444	4444	4444	0044	
				4444	4444	4444	4444	4444	4444	4444	4444	4444	0000

n.a. = not applicable

n.d. = not done

0 = no virus present; t = cytotoxic

1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 2: Raw data for 1226 IND01 (97.0 %) tested against poliovirus type 1 at 20 °C (quantal test; 8 wells) (3238) (2nd assay)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)											
				1	2	3	4	5	6	7	8	9			
test product	97.0%	dirty conditions	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			10	tttt	tttt	4444	4444	0404	0000	0000	0000	0000	n.d.	n.d.	
			15	tttt	tttt	4440	0000	0000	0000	0000	0000	0000	0000	0000	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product cytotoxicity	97.0%	dirty conditions	n.a.	tttt	tttt	0000	0000	0000	0000	n.d.	n.d.	n.d.	n.d.	n.d.	
			5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
formaldehyde	0.7% (m/V)	PBS	15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
formaldehyde cytotoxicity	0.7% (m/V)	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			0	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
virus control	n.a.	dirty conditions	60	4444	4444	4444	4444	4444	4444	4444	4444	4444	4044	0000	
				4444	4444	4444	4444	4444	4444	4444	4444	4444	4044	0000	

n.a. = not applicable
n.d. = not done

0 = no virus present; t = cytotoxic
1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 3: Raw data for 1226 IND01 (80.0 %) tested against poliovirus type 1 at 20 °C (quantal test; 8 wells) (3219)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)									
				1	2	3	4	5	6	7	8	9	
test product	80.0%	dirty conditions	5	tttt	tttt	4444	4444	4444	0004	0000	0000	0000	n.d.
				tttt	tttt	4444	4444	0400	0000	0000	0000	n.d.	
			10	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product cytotoxicity	80.0%	dirty conditions	15	tttt	tttt	4444	4444	4444	0000	0000	0000	0000	n.d.
				tttt	tttt	4444	4444	4044	0000	0000	0000	n.d.	
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
formaldehyde	0.7% (m/V)	PBS	n.a.	tttt	tttt	0000	0000	0000	n.d.	n.d.	n.d.	n.d.	n.d.
			5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
formaldehyde cytotoxicity	0.7% (m/V)	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
virus control	n.a.	dirty conditions	0	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			60	4444	4444	4444	4444	4444	4444	4444	0044	0000	0000

n.a. = not applicable
n.d. = not done

0 = no virus present; t = cytotoxic
1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 4: Raw data for 1226 IND01 (10.0 %) tested against poliovirus type 1 at 20 °C (quantal test; 8 wells) (3238)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)										
				1	2	3	4	5	6	7	8	9		
test product	10.0%	dirty conditions	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			10	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			15	4444	4444	4444	4444	4444	4444	4444	0440	0000	n.d.	
				4444	4444	4444	4444	4444	4444	4444	0044	0000	n.d.	
test product cytotoxicity	10.0%	dirty conditions	n.a.	tttt	0000	0000	0000	0000	0000	0000	0000	n.d.	n.d.	
			5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
formaldehyde	0.7% (m/V)	PBS	15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
				60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
formaldehyde cytotoxicity	0.7% (m/V)	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			0	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
virus control	n.a.	dirty conditions	60	4444	4444	4444	4444	4444	4444	4444	4444	4000	0000	
			4444	4444	4444	4444	4444	4444	4044	0400	0000	0000		

n.a. = not applicable

n.d. = not done

0 = no virus present; t = cytotoxic

1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 5: Raw data for formaldehyde solution (0.7 %) tested against poliovirus type 1 at 20 °C (quantal test; 8 wells) (3238)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)													
				1	2	3	4	5	6	7	8	9					
test product	n.a.		5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.		
			10	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product cytotoxicity	n.a.	n.a.	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.		
formaldehyde	0.7% (m/V)	PBS	5	tttt	tttt	4444	4444	4444	4444	4444	4444	4440	0000	0000	0000	n.d.	
			15	tttt	tttt	4444	4444	4444	4444	4444	4444	4444	0000	0000	0000	0000	n.d.
			30	tttt	tttt	4444	4444	4444	4444	4444	4444	4404	0000	0000	0000	0000	n.d.
			60	tttt	tttt	4444	4444	4444	0404	4340	0000	0000	0000	0000	0000	0000	n.d.
			n.a.	tttt	tttt	0000	0000	0000	0000	0000	0000	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			0	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
formaldehyde cytotoxicity	0.7% (m/V)	PBS	n.a.	tttt	tttt	4444	4444	4444	4444	4444	4444	4444	4444	4444	0000		
virus control	n.a.	PBS	60	4444	4444	4444	4444	4444	4444	4444	4444	4444	4444	0404	0400	0000	
				4444	4444	4444	4444	4444	4444	4444	4444	4444	4444	0444	0000	0000	

n.a. = not applicable
n.d. = not done
0 = no virus present; t = cytotoxic
1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 6: Raw data for control of efficacy for suppression of disinfectant activity (97.0 %) (3238)

Product	Interfering substance	dilutions (log ₁₀)										
		1	2	3	4	5	6	7	8	9		
test product	PBS	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product	clean conditions	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product	dirty conditions	tttt tttt	tttt tttt	4444 4444	4444 4444	4444 4444	4444 4444	0440 0000	0440 0044	0440 0000	0000 0000	0000 0000

n.a. = not applicable

n.d. = not done

0 = no virus present; t = cytotoxic

1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 7: Raw data (poliovirus type 1) for cell sensitivity (97.0 %) (3238)

Product	comparative virus titration with	Dilution	Dilutions (log ₁₀)										
			1	2	3	4	5	6	7	8	9		
PBS	dirty conditions	-	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4000 4044	0400 0000	n.d. n.d.
test product	dirty conditions	1:10	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product	dirty conditions	1:100	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product	dirty conditions	1:1,000	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	0040 0440	0000 0400	n.d. n.d.

n.a. = not applicable
 n.d. = not done

0 = no virus present; t = cytotoxic
 1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 8a: Summary of results with 1226 IND01 and poliovirus type 1

Product	Con- centration	Interfering substance	Level of cytotoxicity	log ₁₀ TCID ₅₀ /ml aftermin					> 4 log ₁₀ reduction after ... min
				5	10	15	30	60	
test product	97.0%	dirty	3.50	7.00±0.44	n.d.	4.50±0.00	n.d.	n.d.	15 (RF = 4.25±0.33)
test product	97.0%	dirty	3.50	n.d.	5.88±0.37	≤4.38±0.25	n.d.	n.d.	15 (RF ≥ 4.13±0.43)
test product	80.0%	dirty	3.50	6.75±0.33	n.d.	6.13±0.37	n.d.	n.d.	> 15
test product	10.0%	dirty	2.50	n.d.	n.d.	8.00±0.38	n.d.	n.d.	> 15

n.a. = not applicable n.d. = not done



Table 8b: Summary of results with 1226 IND01 and poliovirus type 1

Product	Con- centration	Interfering substance	Level of cytotoxicity	log ₁₀ TCID ₅₀ /ml aftermin					> 4 log ₁₀ reduction after ... min
				0	5	15	30	60	
formaldehyde	0.7% (w/v)	PBS	3.50	n.d.	7.63±0.41	6.75±0.33	6.38±0.49	5.13±0.37	> 60.0
virus contr.	n.a.	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	8.25±0.44	n.a.
virus contr. 1	97.0% assay	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	8.75±0.33	n.a.
virus contr. 2	97.0% assay	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	8.50±0.35	n.a.
virus contr. 1	80.0% assay	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	8.13±0.37	n.a.
virus contr. 2	80.0% assay	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	8.13±0.45	n.a.
suppression control	97.0 %	dirty	3.50	n.d.	n.d.	n.d.	7.13±0.45	n.d.	n.a.
sens.control PBS	n.a.	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	8.13±0.45	n.a.
sens. control test product	97.0% → 1:1,000	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	8.00±0.44	n.a.

n.a. = not applicable n.d. = not done sens. = sensitivity



05.07.2013

Test report P13ML1536-2A

Evaluation of the effectiveness of
1226 IND01

Test virus: adenovirus type 5 strain Adenoid 75


Method: prEN 14476:2011 (dirty conditions)

quantitative suspension test for the evaluation of
virucidal activity of chemical disinfectants and
antiseptics used in human medicine

TEST REPORT

Sponsor:

Christeyns France SA
9, rue Marcel Sembat
44100 NANTES

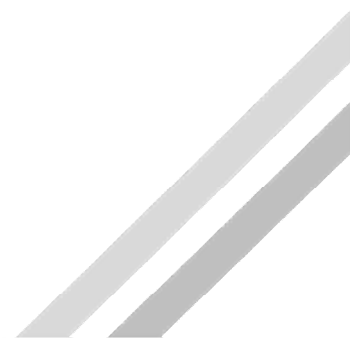



1. Introduction

The objective of this study was to evaluate the virus-inactivating properties of the surface disinfectant 1226 IND01 against adenovirus type 5 using a quantitative suspension assay according to the prEN 14476:2011 (1) under dirty conditions.

2. Test laboratory

MikroLab GmbH, Norderoog 2, D-28259 Bremen

3. Identification of the sample

Manufacturer	Christeyns France SA
Name of product	1226 IND01
Batch number	16.04.13
Application	surface disinfection
Production date	16.04.2013
Expiry date	-
Active compound (s) (100 g)	peracetic acid (CAS no.: 79-21-0)
Appearance, odour	clear, colourless liquid product specific
pH-values (in WSH)	undiluted: 2.21 (20 °C)
Storage conditions	room temperature in the dark (area with restricted access)
Date of arrival in the laboratory	25.04.2013

4. Materials

4.1 Culture medium and reagents

- Eagle`s Minimum Essential Medium with Earle`s BSS (EMEM, Lonza Group Ltd., catalogue no. BE12-125F)
- Fetal calf serum (Biochrom AG, article no. S 0115)
- 1.4 % formaldehyde solution (Chemisch-technologisches Laboratorium Dr. Melzer, D-28199 Bremen)
- Aqua bidest. (Fresenius Kabi Deutschland, article no. P2N 1636071)
- PBS (Invitrogen, article no. 18912-014)
- BSA (Sigma-Aldrich-Chemie GmbH, article no. CA-2153)



-
- sheep erythrocytes (Fiebig-Nährstofftechnik; article no. 31100100)

4.2 Virus and cells

The adenovirus type 5 strain adenoid 75 was obtained from PD Dr. A. Heim, Institute of Medical Virology, Hannover Medical School, Hannover, Germany. Before the inactivation assays, the virus had been passaged 3 times in *A549 cells* (human lung epithelial carcinoma cells).

The *A549 cells* also originated from the Institute of Medical Virology, Hannover Medical School.

The cells were inspected regularly for morphological alterations and for contamination by mycoplasmas. No morphological alterations of cells and no contamination by mycoplasmas could be detected.

4.3 Apparatus, glassware and small items of equipment

- CO₂ incubator, Nunc GmbH & Co. KG, model QWJ 350
- Agitator (Vortex Genie Mixer, type G 560E)
- pH measurement 315i (WTW, article no. 2A10-100)
- Centrifuge (Sigma-Aldrich-Chemie GmbH, type 113)
- Microscope (Olympus, type CK 30)
- Water bath (JULABO, Julabo U 3)
- Adjustable volume automatic pipettes (Eppendorf AG)
- Polyesterol 96-well microtiter plate (Nunc GmbH & Co. KG, Wiesbaden, Germany)
- Cell culture flask (Nunc GmbH & Co. KG, Wiesbaden, Germany)
- Sealed test tubes (Sarstedt AG & Co., Nümbrecht, Germany)



5. Experimental conditions

Test temperature(s)	20 °C ± 1 °C
Concentration(s) of test product	undiluted (80.0 %), 50.0 % and 10.0 % (non-active range) solutions
Contact time(s)	5 and 15 minutes
Interfering substance(s)	dirty conditions: 3.0 g/l BSA + 3.0 g/l erythrocytes
Diluent	water (50.0 % and 10.0 % solutions)
Stability of product in the mix with virus and interfering substance (80.0 %)	no flocculation
Procedure to stop action of product	immediate dilution
Test virus	adenovirus type 5 strain adenoid 75 (ATCC VR-5)
Period of analysis	25.04.2013 – 05.07.2013
End of testing	05.07.2013

6. Methods

6.1 Preparation of test virus suspension

For preparation of test virus suspension according to prEN 5.4.1 *A549 cells* were cultivated in a 175 cm² flask with Eagle`s Minimum Essential Medium with Earle`s BSS and 10 % fetal calf serum (FCS). Adenovirus type 5 (stock virus suspension) was added to the monolayer for 1 h at 37 °C with gentle shaking every 15 min. After cells showed a cytopathic effect, they were treated with ultrasound (HD 2200, Bandelin electronic GmbH & Co. KG, D-12207 Berlin) followed by a low speed centrifugation (10 min and 1000 x g) in order to sediment cell debris. After aliquotation, test virus suspension was stored at –80 °C.

6.2 Disinfectant

The test product was evaluated undiluted. Due to the addition of test virus suspension and interfering substance an 80.0 % solution resulted. Furthermore, the product was additionally examined as 50.0 % and 10.0 % (demonstration of non-active range) solutions.

The 50.0 % and 10.0 % solutions were prepared with water immediately before the inactivation tests.

6.3 Infectivity assay

Infectivity was determined as endpoint titration according to prEN 5.5.2 transferring 0.1 ml of each dilution into eight wells of a microtitre plate, beginning with the highest dilution. This was followed by the addition of 0.1 ml of freshly trypsinized *A549 cells*. This cell suspension



was adjusted to reach $10\text{-}15 \times 10^3$ cells per well. Microtitre plates were incubated at $37\text{ }^\circ\text{C}$ in a 5% CO_2 -atmosphere. The cytopathic effect was read by using an inverted microscope after ten days. Calculation of the infective dose $\text{TCID}_{50}/\text{ml}$ was calculated with the method of Spearman (2) and Kärber (3) with the following formula:

$$-\log_{10}\text{TCID}_{50} = X_0 - 0.5 + \sum r/n$$

meaning

X_0 = \log_{10} of the lowest dilution with 100% positive reaction

r = number of pos. determinations of lowest dilution step with 100% positive and all higher positive dilution steps

n = number of determinations for each dilution step.

6.4 Calculation and verification of virucidal activity

The virucidal activity of the test disinfectant was evaluated by calculating the decrease in titre in comparison with the control titration without disinfectant. The difference is given as reduction factor (RF).

According to the prEN 14476:2011, a disinfectant or a disinfectant solution at a particular concentration is having virus-inactivating efficacy if the titre is reduced at least by four \log_{10} steps within the recommended exposure period.

6.5 Inactivation assay

Investigations for determination of virucidal activity followed prEN 5.5. 1226 IND01 was examined undiluted (80.0%) and as 50.0% and 10.0% solutions at $20\text{ }^\circ\text{C}$. 5 and 15 minutes were chosen as exposure times.

Due to a more convenient handling, the volumes in this assay were 0.1 ml test virus suspension, 0.1 ml interfering substance and 0.8 ml test product. Immediately at the end of a chosen contact time, activity of the disinfectant was stopped by dilution to 10^{-8} .

Titration of the virus control was performed at contact times 0 min and 60 min (prEN 5.5.7).

Furthermore, a cell control (only addition of medium) was incorporated.



Inactivation tests were carried out in sealed test tubes in a water bath at $20\text{ }^{\circ}\text{C} \pm 1.0\text{ }^{\circ}\text{C}$. Aliquots were retained after appropriate exposure times, and residual infectivity was determined.

6.6 Determination of cytotoxicity

Determination of cytotoxicity was performed according to prEN 5.5.4.1 with 100 μl water, 100 μl interfering substance and 800 μl test product.

6.7 Cell sensitivity to virus

For the control of cell sensitivity to virus the lowest apparently non-cytotoxic dilution of the test product or PBS as control were added to a volume of double concentrated cell suspension. After 1 h at $37\text{ }^{\circ}\text{C}$ the cells were centrifuged and re-suspended in cell culture medium (prEN 5.5.4.2b).

Finally, a comparative titration of the test virus suspension was performed on the pre-treated (disinfectant) and non-pre-treated (PBS) cells as described above.

6.8 Control of efficacy for suppression of disinfectant activity

Furthermore, a control of efficiency for suppression of disinfectant activity was included (prEN 5.5.6).

6.9 Reference virus inactivation test

As reference for test validation 0.7 % formaldehyde according to prEN 5.5.6.1 was included. Contact times were 5, 15, 30 and 60 min. In addition, cytotoxicity of formaldehyde test solution was determined following prEN 5.5.6.2 with dilutions up to 10^{-5} .

7. Verification of the methodology

The following criteria as mentioned in prEN 5.7 were fulfilled:

- a) The titre of the test virus suspension allowed the determination of $\geq 4\text{ log}_{10}$ reduction.
- b) The test product was cytotoxic in the 1:100 (80.0 % and 50.0 % solutions) dilutions thus allowing the detection of a four log_{10} reduction of the virus titre.
- c) The difference of the logarithmic titre of the virus control minus the logarithmic titre of the test virus in the reference inactivation test (see prEN 5.7b) was $\geq 3.13 \pm 0.25$ (between 3.0 – 5.0) after 30 min and $\geq 3.13 \pm 0.25$ (between 3.5 – 5.5) after 60 min for adenovirus



type 5. The required value (3.50) after 60 min exposure time was not reached because the initial virus titre (7.63) was too low to reach 3.50 as RF with a cytotoxicity of 4.50. The virus titre had to reach 8.00 to demonstrate a \log_{10} reduction of 3.50 ($4.50 + 3.50 = 8.00$). Therefore, despite this too low reduction of virus titre after 60 minutes exposure time the test is valid.

- d) The comparative titration on pre-treated (disinfectant) and non-pre-treated (PBS) A549 cells showed an acceptable difference ($<1 \log_{10}$; prEN 5.7) of virus titre: 7.13 ± 0.37 (PBS) versus 6.88 ± 0.37 (1:1,000 dilutions of disinfectant, 80.0 % solution).
- e) The control of efficacy for suppression of disinfectant activity demonstrated a reduction of viral infectivity after 30 minutes of exposure time due to the fact that even the 10.0 % solution produced a \log_{10} reduction of 3.63 ± 0.60 after 15 minutes. For these examinations the activity of the disinfectant was stopped by immediate dilution.

Since all criteria according to prEN 5.7 were fulfilled, examination with adenovirus type 5 according to prEN 14476:2011 was valid.

8. Results

The surface disinfectant 1226 IND01 was examined undiluted (80.0 % solutions) and as 50.0 % and 10.0 % solutions at 20 °C under dirty conditions.

Results of examinations are shown in tables 1 to 7. Tables 1 to 6 demonstrate the raw data, whereas table 7 (a+b) gives a summary of results.

The undiluted solution of the test product (80.0 %) was able to inactivate adenovirus type 5 after 5 minutes in this quantitative suspension test. The following reduction factor was measured at this time point: $\geq 4.00 \pm 0.34$. This corresponded to an inactivation of ≥ 99.99 % (Table 1).

The 50.0 % solution was additionally active against adenovirus type 5. After 5 minutes exposure time, the following reduction factor was measured: $\geq 4.00 \pm 0.34$ (≥ 99.99 %) (Table 2).

The 10.0 % solution was not sufficient active against adenovirus type 5. After 15 minutes exposure time, the following reduction factor was achieved: 3.63 ± 0.60 (Table 3).



9. Summary

In summary, a sufficient reduction of virus titre could be achieved by 1226 IND01 undiluted after an exposure time of 5 minutes. Due to the lack of virological guidelines simulating practical conditions in Europe (phase 2, step 2 tests) the data of this quantitative suspension test lead to the recommendation to use the surface disinfectant 1226 IND01 for inactivation of adenovirus type 5 under dirty conditions as follows:

undiluted 5 minutes

Bremen, 05.07.2013

Dr. Jochen Steinmann



10. Quality control

The Quality Assurance of the results was maintained by performing the determination of the virus-inactivating properties of the disinfectant in accordance with Good Laboratory Practice regulations:

- 1) Chemicals Act of Germany, Appendix 1, dating of 01.08 1994 (BGBl. I, 1994, page 1703). Appendix revised at 14. 05. 1997 (BGBl. I, 1997, page 1060).
- 2) OECD Principles of Good Laboratory Practice (revised 1997); OECD Environmental Health and Safety Publications; Series on Principles of Good Laboratory Practice and Compliance Monitoring – Number 1. Environment Directorate, Organization for Economic Co-operation and Development, Paris 1998.

The plausibility of the results was additionally confirmed by controls incorporated in the inactivation assays.

11. Records to be maintained

All testing data, protocol, protocol modifications, the final report, and correspondence between MikroLab GmbH and the sponsor will be stored in the archives at MikroLab GmbH.

The use of the MikroLab GmbH name, logo or any other representation of MikroLab GmbH, other than distribution of this report in it's entirety, without the written approval of MikroLab GmbH is prohibited. In addition, MikroLab GmbH may not be referred to in any form of promotional materials, press releases, advertising or similar materials (whether by print, broadcast, communication or electronic means) without the express permission of MikroLab GmbH.

The test results in this test report relate only to the items examined.



12. Literature

1. prEN 14476:2011: Chemical disinfectants and antiseptics – Quantitative suspension test for the evaluation of virucidal activity of chemicals disinfectants and antiseptics in human medicine test - Test method and requirements (phase 2, step 1)
2. Spearman, C.: The method of `right or wrong cases` (constant stimuli) without Gauss's formulae.
Brit J Psychol; 2 1908, 227-242
3. Kärber, G.: Beitrag zur kollektiven Behandlung pharmakologischer Reihenversuche.
Arch Exp Path Pharmac; 162, 1931, 480-487



Appendix

- Table 1: Raw data of 1226 IND01 (80.0 %) tested against adenovirus type 5 at 20 °C under dirty conditions
- Table 2: Raw data of 1226 IND01 (50.0 %) tested against adenovirus type 5 at 20 °C under dirty conditions
- Table 3: Raw data of 1226 IND01 (10.0 %) tested against adenovirus type 5 at 20 °C under dirty conditions
- Table 4: Raw data of formaldehyde solution (0.7 %) tested against adenovirus type 5 at 20 °C
- Table 5: Control of efficacy for suppression of disinfectant activity (80.0 %)
- Table 6: Raw data (adenovirus type 5) for cell sensitivity to virus (80.0 %)
- Table 7 (a+b): Results with 1226 IND01 and adenovirus type 5 (summary)



Table 1: Raw data of 1226 IND01 (80.0 %) tested against adenovirus type 5 (quantal test; 8 wells) at 20 °C (3257)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)										
				1	2	3	4	5	6	7	8	9		
product	80.0%	dirty conditions	5	tttt tttt	tttt tttt	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.	
			15	tttt tttt	tttt tttt	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
product cytotoxicity	80.0%	dirty conditions	n.a.	tttt tttt	tttt tttt	0000 0000	0000 0000	0000 0000	n.d.	n.d.	n.d.	n.d.	n.d.	
formaldehyde	0.7% (m/V)	PBS	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
formaldehyde cytotoxicity	0.7% (m/V)	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
virus control	n.a.	dirty conditions	0	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4403 2444	0040 0040	0000 0000	n.d.		
			60	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	0202 3422	0000 0300	4000 0000	n.d.		

n.a. = not applicable
 n.d. = not done

0 = no virus present; t = cytotoxic
 1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 2: Raw data of 1226 IND01 (50.0 %) tested against adenovirus type 5 (quantal test; 8 wells) at 20 °C (3257)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)										
				1	2	3	4	5	6	7	8	9		
product	50.0%	dirty conditions	5	tttt tttt	tttt tttt	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.	
			15	tttt tttt	tttt tttt	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.	
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
product cytotoxicity	50.0%	dirty conditions	n.a.	tttt tttt	tttt tttt	0000 0000	0000 0000	0000 0000	n.d.	n.d.	n.d.	n.d.	n.d.	
formaldehyde	0.7% (m/V)	PBS	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
formaldehyde cytotoxicity	0.7% (m/V)	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
virus control	n.a.	dirty conditions	0	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4403 2444	0040 0040	0000 0000	n.d.		
			60	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	0202 3422	0000 0300	4000 0000	n.d.		

n.a. = not applicable
 n.d. = not done

0 = no virus present; t = cytotoxic
 1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 3: Raw data of 1226 IND01 (10.0 %) tested against adenovirus type 5 (quantal test; 8 wells) at 20 °C (3257)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)								
				1	2	3	4	5	6	7	8	9
product	10.0%	dirty conditions	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			15	tttt tttt	4444 4444	0400 0403	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
product cytotoxicity	10.0%	dirty conditions	n.a.	tttt tttt	0000 0000	0000 0000	0000 0000	0000 0000	n.d.	n.d.	n.d.	n.d.
formaldehyde	0.7% (m/V)	PBS	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
formaldehyde cytotoxicity	0.7% (m/V)	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
virus control	n.a.	dirty conditions	0	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4403 2444	0040 0040	0000 0000	n.d.
			60	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	0202 3422	0000 0300	4000 0000	n.d.

n.a. = not applicable
 n.d. = not done

0 = no virus present; t = cytotoxic
 1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 4: Raw data of formaldehyde solution (0.7 %) tested against adenovirus type 5 (quantal test; 8 wells) (3257)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)									
				1	2	3	4	5	6	7	8	9	
product	n.a.	n.a.	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
product cytotoxicity	n.a.	n.a.	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
formaldehyde	0.7% (m/V)	PBS	5	tttt tttt	tttt tttt	tttt tttt	4444 4444	1333 1424	0000 0000	0000 0000	0000 0000	0000 0000	n.d.
			15	tttt tttt	tttt tttt	tttt tttt	3000 2010	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.
			30	tttt tttt	tttt tttt	tttt tttt	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.
			60	tttt tttt	tttt tttt	tttt tttt	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.
formaldehyde cytotoxicity	0.7% (m/V)	PBS	n.a.	tttt tttt	tttt tttt	tttt tttt	0000 0000	0000 0000	n.d.	n.d.	n.d.	n.d.	
virus control	n.a.	PBS	0	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			60	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	2133 3443	0004 0000	0000 0000	0000 0000	

n.a. = not applicable
 n.d. = not done

0 = no virus present; t = cytotoxic
 1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 5: Control of efficacy for suppression of disinfectant activity (80.0 %) (3257)

Product	Interfering substance	Dilutions (log ₁₀)								
		1	2	3	4	5	6	7	8	9
product	PBS	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
product	clean	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
product	dirty	ttt ttt	0000 0004	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	0000 0000	n.d.

n.a. = not applicable
n.d. = not done

0 = no virus present; t = cytotoxic
1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 6 : Raw data (adenovirus type 5) for cell sensitivity to virus (80.0 %) (3257)

Product	Interfering substance	Dilution	Dilutions (log ₁₀)									
			1	2	3	4	5	6	7	8	9	
PBS	-	without	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	3322 4000	0000 0000	0000 0000	n.d.
test product	PBS	1:100	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
		1:1,000	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product	clean conditions	1:100	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
		1:1,000	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
test product	dirty conditions	1:100	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
		1:1,000	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	4444 4444	3000 1003	0000 0000	0000 0000	n.d.

n.a. = not applicable
 n.d. = not done

0 = no virus present; t = cytotoxic
 1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 7a : Summary of results with 1226 IND01 and adenovirus type 5

Product	Con- centration	Interfering substance	Level of cytotoxicity	log ₁₀ TCID ₅₀ /ml aftermin					> 4 log ₁₀ reduction after ... min
				5	10	15	30	60	
test product	80.0%	dirty	3.50	≤3.50±0.00	n.d.	≤3.50±0.00	n.d.	n.d.	5 (RF = ≥4.00±0.34)
test product	50.0%	dirty	3.50	≤3.50±0.00	n.d.	≤3.50±0.00	n.d.	n.d.	5 (RF = ≥4.00±0.34)
test product	10.0%	dirty	2.50	n.d.	n.d.	3.88±0.37	n.d.	n.d.	> 15 (RF = 3.63±0.60)

n.a. = not applicable n.d. = not done



Table 7b: Summary of results with 1226 IND01 and adenovirus type 5

Product	Concentration	Interfering substance	Level of cytotoxicity	log ₁₀ TCID ₅₀ /ml aftermin					> 4 log ₁₀ reduction after ... min
				0	5	15	30	60	
formaldehyde	0.7% (w/v)	PBS	4.50	n.d.	6.50±0.00	4.88±0.37	≤4.50±0.00	≤4.50±0.00	≥ 30.0
virus contr.	n.a.	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	7.63±0.25	n.a.
virus contr.	n.a.	dirty	n.a.	7.63±0.41	n.d.	n.d.	n.d.	7.50±0.48	n.a.
suppression control	n.a.	dirty	3.50	n.d.	n.d.	n.d.	≤2.63±0.25	n.d.	n.a.
sens.control PBS	n.a.	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	7.13±0.37	n.a.
sens. control test product	80.0% à 1:1,000	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	6.88±0.37	n.a.

n.a. = not applicable n.d. = not done sens. = sensitivity

DR. JOCHEN STEINMANN
Resp. techn. et scient.
chez MikroLab GmbH

Norderoog 2
D-28259 Bremen

Tél.:+49 (421) 27819102
Fax:+49 (421) 2760283
<http://www.mikrolab-gmbh.de>
E-mail: info@mikrolab-gmbh.de

MikroLab GmbH, Norderoog 2, D-28259 Bremen

20.06.2013
Dr St/NM

Christeyns France SA
9, rue Marcel Sembat
44100 NANTES
FRANCE

Efficacité contre le norovirus murin du produit 1226 IND01 lors d'un essai de suspension quantitatif à 20 °C en conditions de saleté

RAPPORT D'EXPERTISE

Le désinfectant pour les surfaces 1226 IND01 de Christeyns France SA a été testé pour son efficacité à inactiver le norovirus murin suivant la norme prEN 14476:2011.

Dans la norme prEN 14476:2011, on conclut à l'efficacité anti-virus d'un désinfectant si, après un temps d'action défini, la réduction du titre viral initial est supérieure ou égale à ≥ 4 unités \log_{10} (inactivation $\geq 99,99$ %).

Le désinfectant pour les surfaces 1226 IND01 a été utilisé non dilué à 20 °C, en 5 et 15 minutes de temps de contact. Après 5 minutes une réduction du titre de virus \geq quatre unités \log_{10} a été constatée. L'efficacité est donc obtenue avec 1226 IND01:

non dilué

5 minutes


Dr. Jochen Steinmann



20.06.2013

Test report P13ML1536-2M

Evaluation of the effectiveness of 1226 IND01

Test virus: murine norovirus (as surrogate for human
norovirus)

Method: prEN 14476:2011 (dirty conditions)

quantitative suspension test for the evaluation of
virucidal activity of chemical disinfectants and
antiseptics used in human medicine

TEST REPORT

Sponsor:

Christeyns France SA
9, rue Marcel Sembat
44100 NANTES





1. Introduction

The objective of this study was to evaluate the virus-inactivating properties of the surface disinfectant 1226 IND01 against murine norovirus (MNV) as surrogate for human norovirus using a quantitative suspension assay according to prEN 14476:2011 (1) under dirty conditions.

2. Test laboratory

MikroLab GmbH, Norderoog 2, D-28259 Bremen

3. Identification of the sample

Manufacturer	Christeyns France SA
Name of product	1226 IND01
Batch number	16.04.13
Application	surface disinfection
Production date	16.04.2013
Expiry date	-
Active compound (s) (100 g)	peracetic acid (CAS no.: 79-21-0)
Appearance, odour	clear, colourless liquid product specific
pH-values (in WSH)	undiluted: 2.21 (20 °C)
Storage conditions	room temperature in the dark (area with restricted access)
Date of arrival in the laboratory	25.04.2013

4. Materials

4.1 Culture medium and reagents

- Dulbecco's Modified Eagle's Medium (DMEM, Lonza Group Ltd., catalogue no. BE12-614F)
- Fetal calf serum (Thermo Fisher, article no. CH30160.02)
- 1.4 % formaldehyde solution (Chemisch-technologisches Laboratorium Dr. Melzer, D-28199 Bremen)



- Aqua bidest. (Fresenius Kabi Deutschland, article no. P2N 1636071)
- PBS (Invitrogen, article no. 18912-014)
- BSA (Sigma-Aldrich-Chemie GmbH, article no. CA-2153).
- sheep erythrocytes (Fiebig-Nährstofftechnik; article no. 31100100).

4.2 Virus and cells

MNV was obtained from PD. Dr. E. Schreier, Head of FG15 Molecular Epidemiology of Viral Pathogens at the Robert Koch-Institute (RKI) in Berlin. Prior to inactivation, MNV was passaged three times in *RAW 264.7 cells* (a macrophage-like, Abelson leukemia virus transformed cell line derived from BALB/c mice, ATCC TIB-71).

The cells were inspected regularly for morphological alterations and for contamination by mycoplasmas. No morphological alterations of cells and no contamination by mycoplasmas could be detected.

4.3 Apparatus, glassware and small items of equipment

- CO₂ incubator, Nunc GmbH & Co. KG, model QWJ 350
- Agitator (Vortex Genie Mixer, type G 560E)
- pH measurement 315i (WTW, article no. 2A10-100)
- Centrifuge (Sigma-Aldrich-Chemie GmbH, type 113)
- Microscope (Olympus, type CK 30)
- Water bath (JULABO, Julabo U 3)
- Adjustable volume automatic pipettes (Eppendorf AG)
- Polysterol 96-well microtiter plate (Nunc GmbH & Co. KG, Wiesbaden, Germany)
- Cell culture flask (Nunc GmbH & Co. KG, Wiesbaden, Germany)
- Sealed test tubes (Sarstedt AG & Co., Nümbrecht, Germany).



5. Experimental conditions

Test temperature	20 °C ± 1.0 °C
Concentration of test product	undiluted (80.0 %) and as 50.0 % and 10.0 % solutions
Contact times	5 and 15 minutes
Interfering substance (s)	dirty conditions: 3.0 g/l bovine serum albumin (BSA) + 3.0 g/l erythrocytes
Diluent	water (50.0 % and 10.0 % solutions)
Procedure to stop action of disinfectant	immediate dilution
Stability of product in the mix with virus and interfering substance (80.0 % solution)	flocculation
Test virus	murine norovirus (Berlin 06 / 06 / DE Isolat S99)
Period of analysis	02.04.2013 – 20.06.2013
End of testing	20.06.2013

6. Methods

6.1 Preparation of test virus suspension

To prepare the test virus suspension, *RAW 264.7 cells* that had been cultured with Dulbecco's Modified Eagle's Medium with 4.5 g/l glucose and 10 % fetal calf serum with low endotoxin were inoculated with MNV (stock virus solution) in a 175 cm² cell culture flask. Once a cytopathic effect had been induced (approx. 1-3 days), freezing and thawing was carried out two times. The cell debris was removed by centrifugation at 770 x g and 4 °C for ten minutes and the supernatant was recovered as test viral suspension, aliquoted and stored at -80 °C.

6.2 Disinfectant

The test product was evaluated undiluted. Due to the addition of test virus suspension and interfering substance an 80.0 % solution resulted.

Furthermore the product was evaluated as 50.0 % and 10.0 % solutions (demonstration of non-active range). These solutions were prepared with water immediately before the inactivation tests.



6.3 Infectivity assay

Infectivity was determined according to prEN 5.5.2 by means of end point dilution method using the microtitre process. For this, 100 µl aliquots of the samples, which had been serially diluted with ice-cold DMEM, were transferred to eight wells of a 96-well microtitre plate. This was followed by the addition of 100 µl aliquots of *RAW 264.7 cells* (approx. $1-1.5 \times 10^4$ cells) freshly prepared by scraping. Incubation took place at 37 °C in a CO₂ incubator (5 % CO₂ content) for five days. Finally, cultures were observed for cytopathic effects with a reversed microscope and the infective dose TCID₅₀/ml was calculated with the method of Spearman (2) and Kärber (3) with the following formula:

$$-\log_{10}TCID_{50} = X_0 + 0.5 - \sum r/n$$

meaning

X_0 = log₁₀ of the lowest dilution with 100 % positive reaction

r = number of positive determinations of lowest dilution step with 100 % positive and all higher positive dilution steps

n = number of determinations for each dilution step.

6.4 Calculation and verification of virucidal activity

The virucidal activity of the test disinfectant was evaluated by calculating the decrease in titre in comparison with the control titration without disinfectant. The difference is given as reduction factor (RF).

According to prEN 14476:2011, a disinfectant or a disinfectant solution at a particular concentration is having virus-inactivating efficacy if the titre is reduced at least by four log₁₀ steps within the recommended exposure period.

6.5 Inactivation assay

Investigations for determination of virucidal activity followed prEN 5.5. The test product 1226 IND01 was examined undiluted (80.0 %) and as 50.0 % and 10.0 % solutions at 20 °C. 5 and 15 minutes were chosen as contact times.

Due to a more convenient surfaceling, the volumes in this assay were 0.1 ml test virus suspension, 0.1 ml interfering substance and 0.8 ml test product.



Immediately at the end of a chosen contact time, activity of the disinfectant was stopped by serial dilution.

Titration of the virus control was performed at maximum contact times (prEN 5.5.7).

Furthermore, a cell control (only addition of medium) was incorporated.

Inactivation tests were carried out in sealed test tubes in a water bath at $20\text{ °C} \pm 1.0\text{ °C}$. Aliquots were retained after appropriate exposure times, and residual infectivity was determined.

6.6 Determination of cytotoxicity

Determination of cytotoxicity was determined according to prEN 5.5.4.1 with 100 μl water, 100 μl interfering substance and 800 μl test product.

Values are given as $\log_{10}\text{CD}_{50}/\text{ml}$ (in analogy to $\log_{10}\text{TCID}_{50}/\text{ml}$).

6.7 Cell sensitivity to virus

For the control of cell sensitivity to virus two parts by volume water were mixed with eight parts by volume of the lowest apparently non-cytotoxic dilution of the product. This mixture or PBS as control was added to a volume of double concentrated cell suspension. After 1 h at 37 °C the cells were centrifuged and re-suspended in cell culture medium (prEN 5.5.4.2b).

Finally, a comparative titration of the test virus suspension was performed on the pre-treated (disinfectant) and non-pre-treated (PBS) cells as described above.

6.8 Control of efficacy for suppression of disinfectant activity

In accordance with prEN 5.5.6, a control of efficiency for suppression of disinfectant activity was included.

6.9 Reference virus inactivation test

A 0.7 (w/v) % formaldehyde solution was included as reference for test validation according to prEN 5.5.6.1. Contact times were 5, 15, 30 and 60 minutes. In addition, cytotoxicity of formaldehyde test solution was determined following prEN 5.5.6.2 with dilutions up to 10^{-5} .



7. Verification of the methodology

The following criteria as mentioned in prEN 5.7 were fulfilled:

- a) The titre of the test virus suspension allowed the determination of 4 log₁₀ reduction.
- b) The test product was cytotoxic in the 1:100 dilutions (80.0 % solution).
- c) The comparative titration on pre-treated (disinfectant in the lowest apparently non-cytotoxic dilution) and non-pre-treated (PBS) *RAW 264.7 cells* showed a difference < 1 log₁₀ of virus titre: 7.38 ± 0.25 (PBS) versus 7.50 ± 0.00 (dirty conditions, 1:1,000 dilutions of disinfectant) log₁₀TCID₅₀/ml.
- d) The control of efficacy for suppression of disinfectant activity demonstrated no reduction of viral infectivity after 30 minutes of exposure time (7.38 ± 0.41 versus 7.75 ± 0.33).

Since all criteria following prEN 5.7 were fulfilled, examinations with MNV according to prEN 14476:2011 were valid.

8. Results

Results of examination are shown in tables 1 to 7. Tables 1 to 6 demonstrate the raw data, whereas tables 7 (a + b) gives a summary of results.

The product tested undiluted (80.0 %) was able to inactivate MNV after 5 minutes in this quantitative suspension test under clean conditions (Table 1). The reduction factor was ≥ 4.13 ± 0.41.

Tested as 50.0 % solution 1226 IND01 was active against the MNV within 15 minutes of exposure time (table 2) (RF ≥ 4.00 ± 0.46).

Finally, 1226 IND01 was not active within 15 minutes of exposure time (table 3).

9. Summary

The surface disinfectant 1226 IND01 demonstrated an activity against MNV undiluted after a contact time of 5 minutes at 20 °C. Due to the lack of virological guidelines simulating practical conditions in Europe (phase 2, step 2 tests) the data of this quantitative suspension



test lead to the recommendation to use the surface disinfectant 1226 IND01 for inactivation of MNV (surrogate for human norovirus) as follows:

undiluted 5 minutes

Bremen, 20.06.2013



- Dr. J. Steinmann -



10. Quality control

The Quality Assurance of the results was maintained by performing the determination of the virus-inactivating properties of the disinfectant in accordance with Good Laboratory Practice regulations:

- 1) Chemicals Act of Germany, Appendix 1, dating of 01.08 1994 (BGBl. I, 1994, page 1703). Appendix revised at 14. 05. 1997 (BGBl. I, 1997, page 1060).
- 2) OECD Principles of Good Laboratory Practice (revised 1997); OECD Environmental Health and Safety Publications; Series on Principles of Good Laboratory Practice and Compliance Monitoring – Number 1. Environment Directorate, Organization for Economic Co-operation and Development, Paris 1998.

The plausibility of the results was additionally confirmed by controls incorporated in the inactivation assay.

11. Records to be maintained

All testing data, protocol, protocol modifications, the final report, and correspondence between MikroLab GmbH and the sponsor will be stored in the archives at MikroLab GmbH.

The use of the MikroLab GmbH name, logo or any other representation of MikroLab GmbH, other than distribution of this report in its entirety, without the written approval of MikroLab GmbH is prohibited. In addition, MikroLab GmbH may not be referred to in any form of promotional materials, press releases, advertising or similar materials (whether by print, broadcast, communication or electronic means) without the express permission of MikroLab GmbH. The test report results in this test report relate only to the items examined.



12. Literature

1. prEN 14476:2011: Chemical disinfectants and antiseptics – virucidal quantitative suspension test - Test method and requirements (phase 2, step 1)
2. Spearman, C.: The method of `right or wrong cases` (constant stimuli) without Gauss's formulae.
Brit J Psychol; 2 1908, 227-242
3. Kärber, G.: Beitrag zur kollektiven Besurfacelung pharmakologischer Reihenversuche.
Arch Exp Path Pharmac; 162, 1931, 480-487



Appendix:

Table 1: Raw data for 1226 IND01 (80.0 %) tested against MNV under dirty conditions

Table 2: Raw data for 1226 IND01 (50.0 %) tested against MNV under dirty conditions

Table 3: Raw data for 1226 IND01 (10.0 %) tested against MNV under dirty conditions

Table 4: Raw data for formaldehyde (0.7 %) tested against MNV

Table 5: Control of efficacy for suppression of disinfectant activity (80.0 %)

Table 6: Raw data (MNV) for cell sensitivity (80.0 %)

Table 7 (a + b): Summary of results with 1226 IND01 and MNV



Table 1: Raw data for 1226 IND01 (80.0 %) tested against MNV (quantal test; 8 wells) (3249)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)											
				1	2	3	4	5	6	7	8	9			
Test product	80.0%	dirty	5	tttt	tttt	0000	0000	0000	0000	0000	0000	0000	0000	n.d.	
				tttt	tttt	4000	0000	0000	0000	0000	0000	0000	0000	0000	0000
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
Test product cytotoxicity	80.0%	dirty	n.a.	tttt	tttt	0000	0000	0000	0000	0000	0000	0000	0000	n.d.	
				tttt	tttt	0000	0000	0000	0000	0000	0000	0000	0000	0000	0000
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
Formaldehyde	0.7% (w/v)	PBS	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
Formaldehyde cytotoxicity	0.7% (w/v)	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
Virus control	n.a.	dirty	60	4444	4444	4444	4444	4444	4444	4444	4444	4444	4444	4444	
				4444	4444	4444	4444	4444	4444	4444	4444	4444	4444	4444	4444
				4444	4444	4444	4444	4444	4444	4444	4444	4444	4444	4444	4444

n.a. = not applicable

n.d. = not done

0 = no virus present; t = cytotoxic

1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 2 : Raw data for 1226 IND01 (50.0 %) tested against MNV (quantal test; 8 wells) (3249)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (\log_{10})											
				1	2	3	4	5	6	7	8	9			
Test product	50.0%	dirty	5	tttt	tttt	4400	0000	0000	0000	0000	0000	0000	0000	n.d.	
				tttt	tttt	0440	0000	0000	0000	0000	0000	0000	0000	0000	n.d.
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
Test product cytotoxicity	50.0%	dirty	15	tttt	tttt	0004	0000	0000	0000	0000	0000	0000	0000	n.d.	
				tttt	tttt	0040	0000	0000	0000	0000	0000	0000	0000	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
Formaldehyde	0.7% (w/v)	PBS	30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				tttt	tttt	0000	0000	0000	0000	0000	0000	0000	0000	n.d.	
				tttt	tttt	0000	0000	0000	0000	0000	0000	0000	0000	n.d.	
Formaldehyde cytotoxicity	0.7% (w/v)	PBS	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
Virus control	n.a.	dirty	15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
Virus control	n.a.	dirty	30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
Virus control	n.a.	dirty	60	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
Virus control	n.a.	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
				n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
Virus control	n.a.	dirty	0	4444	4444	4444	4444	4444	4444	4444	4440	0000	0000	n.d.	
				4444	4444	4444	4444	4444	4444	4444	3444	3000	0000	0000	n.d.
				4444	4444	4444	4444	4444	4444	4444	4443	0030	0000	0000	n.d.
Virus control	n.a.	dirty	60	4444	4444	4444	4444	4444	4444	4444	4434	4000	0000	n.d.	
				4444	4444	4444	4444	4444	4444	4444	4434	4000	0000	0000	n.d.
				4444	4444	4444	4444	4444	4444	4444	4434	4000	0000	0000	n.d.

n.a. = not applicable

n.d. = not done

0 = no virus present; t = cytotoxic

1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 4 : Raw data for formaldehyde (0.7 %) tested against MNV (quantal test; 8 wells) (3247)

Product	Concentration	Interfering substance	Contact time (min)	Dilutions (log ₁₀)											
				1	2	3	4	5	6	7	8	9			
Test product	n.a.	n.a.	5	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			10	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			15	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
			30	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
Test product cytotoxicity	n.a.	n.a.	n.a.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.		
			5	tttt	tttt	4444	4444	4444	4444	4444	4444	4444	0000	0000	n.d.
Formaldehyde	0.7% (w/v)	PBS	15	tttt	tttt	4444	4444	4444	4444	3343	0000	0000	0000	n.d.	
			30	tttt	tttt	4444	4444	4444	4444	3443	0000	0000	0000	0000	n.d.
			60	tttt	tttt	4444	4444	4444	4044	0404	0000	0000	0000	0000	n.d.
Formaldehyde cytotoxicity	0.7% (w/v)	PBS	n.a.	tttt	tttt	0000	0000	0000	0000	0000	n.d.	n.d.	n.d.		
			60	tttt	tttt	0000	0000	0000	0000	0000	0000	0000	0000	0000	
Virus control	n.a.	PBS	0	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	
			60	4444	4444	4444	4444	4444	4444	4444	4444	4444	0004	0000	n.d.

n.a. = not applicable
n.d. = not done

0 = no virus present; t = cytotoxic
1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 5: Control of efficacy for suppression of disinfectant activity (80.0 %) (3249)

Product	Interfering substance	Dilutions (log ₁₀)									
		1	2	3	4	5	6	7	8	9	
Test product	PBS	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
Test product	clean conditions	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.	n.d.
Test product	dirty conditions	tttt tttt	tttt tttt	4444 4444	4444 4444	4444 4444	4404 3044	4000 0000	0000 0000	n.d.	n.d.

n.a. = not applicable

n.d. = not done

0 = no virus present; t = cytotoxic

1 to 4 = virus present (degree of CPE in 8 cell culture units) (wells of microtitre plates)



Table 7a: Summary of results with 1226 IND01 and MNV

Product	Con- centration	Interfering substance	Level of cytotoxicity	log ₁₀ TCID ₅₀ /ml aftermin					> 4 log ₁₀ reduction after ... min
				5	10	15	30	60	
test product	80.0%	dirty	3.50	≤3.63±0.25	n.d.	≤3.50±0.00	n.d.	n.d.	5 (4.13±0.41)
test product	50.0%	dirty	3.50	≤4.00±0.38	n.d.	≤3.75±0.33	n.d.	n.d.	15 (4.00±0.46)
test product	10.0%	dirty	2.50	n.d.	n.d.	5.25±0.33	n.d.	n.d.	> 15.0

n.a. = not applicable n.d. = not done



Table 7b: Summary of results with 1226 IND01 and MNV

Product	Con- centration	Interfering substance	Level of cytotoxicity	log ₁₀ TCID ₅₀ /ml aftermin					> 4 log ₁₀ reduction after ... min
				0	5	15	30	60	
formaldehyde	0.7% (w/v)	PBS	3.50	n.d.	7.38±0.25	6.50±0.00	6.38±0.41	5.63±0.41	> 60
virus contr.	n.a.	PBS	n.a.	n.d.	n.d.	n.d.	n.d.	7.75±0.33	n.a.
virus contr.	n.a.	dirty	n.a.	7.50±0.35	n.d.	n.d.	n.d.	7.75±0.33	n.a.
suppression control	n.a	dirty	3.50	n.d.	n.d.	n.d.	7.38±0.41	n.d.	n.a.
sens.control PBS	n.a.	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	7.38±0.25	n.a.
sens. control test product	80.0% (1:1,000)	dirty	n.a.	n.d.	n.d.	n.d.	n.d.	7.50±0.00	n.a.

n.a. = not applicable n.d. = not done


Activité bactéricide selon NF EN 13 704 (avril 2002)

Produit : 1226 IND01 (le 16/04/13)

Donneur d'ordre : **CHRISTEYNS France**
Division santé Laboratoire Phagogène
9 rue Marcel Sembat
44100 NANTES

Loos, le 13 mai 2013.

Le directeur :


Raphaël DUGUÉ.

La reproduction de ce rapport d'essai n'est autorisée que sous sa forme intégrale.

Ce rapport d'essais ne concerne que les échantillons soumis à essais.

Page 1 sur 5

I. PRINCIPE :

L'activité sporicide a été déterminée selon la norme européenne **NF EN 13 704: "Désinfectants chimiques - Essai quantitatif de suspension pour l'évaluation de l'activité sporicide des désinfectants chimiques utilisés dans le domaine de l'agro-alimentaire, dans l'industrie, dans les domaines domestiques et en collectivité. - Méthode d'essai et prescriptions - (Phase 2, étape 1) – Avril 2002."**

Souche(s) de référence testée(s) : **voir tableau(x) page(s) suivante(s).**

II. IDENTIFICATION DE(S) ECHANTILLON(S) :

Nom(s) : **1226 IND01 (le 16/04/13).**

Société : **CHRISTEYNS France.**

Aspect du produit : **Liquide incolore.**

Date de réception au laboratoire : **22/04/13.**

Conditions de stockage au laboratoire : **Température ambiante, à l'abri de la lumière.**

III. METHODE D'ESSAI ET VALIDATION:**- Dilution neutralisation :**

1. Diluant : neutralisant CEN tamponné

2. Filtration sur membrane.

Nature des membranes : **Millipore type HAWG 0,45 µm.**

Liquide de rinçage : **Eau distillée stérile.**

Volume de chaque rinçage : **100 ml.**

Nombre de rinçages : **4.**

Neutralisant ajouté au milieu de dénombrement : **TSB Capitol IV à raison de 10% (v/v) du milieu gélosé.**

IV. CONDITIONS EXPERIMENTALES:

Période d'analyse : **Du 23/04/13 au 10/05/13.**

Diluant du produit utilisé au cours des essais: **Eau distillée (produit prêt à l'emploi).**

Concentration(s) du produit soumis à essai : **voir tableau(x) page(s) suivante(s).**

Aspect des dilutions de produit : **limpides.**

Température de contact : **20°C +/- 1°C.**

Temps de contact additionnel : **15 minutes +/- 10 secondes.**

Substance interférente : **Albumine bovine 0,3 g/l (conditions de propreté).**

Stabilité du mélange de la substance interférente et des produits soumis aux essais: **précipité non décelé.**

Température d'incubation: **30°C +/- 1°C.**

V. RESULTATS EXPERIMENTAUX:

I. Vérification de la méthodologie et de la validation de la méthode de neutralisation du produit soumis à l'essai dans les conditions expérimentales décrites ci-avant :

Essai 1 : neutralisation par dilution (Essais réalisés en parallèle à l'essai proprement dit)

Souche(s) :	Nombre de cellules viables (u.f.c/ml) :					
	Suspension de validation (spores) : Nv₀	Témoin des conditions expérimentales : A	Témoin de non toxicité du neutralisant : B	Concentration du produit mise en œuvre pour la validation :	Validation de la méthode de dilution-neutralisation C	Conclusion :
<i>Bacillus subtilis</i> DSM 347	Vc : 200 ; 213 Nv : $2,1 \times 10^3$	Vc : 198 ; 203 Nv : $2,0 \times 10^2$	Vc : 188 ; 179 Nv : $1,8 \times 10^2$	80% (v/v)	Vc : 3 ; 4 Nv : < 15	Non validée
<p><i>Nv</i> : Nombre d'ufc/ml de la suspension de spores (B.2.). <i>A</i> : Nombre d'ufc/ml dans l'essai de validation des conditions expérimentales (B. 4.1.2 a ou B.4.2.2 a). <i>B</i> : Nombre d'ufc/ml dans l'essai de validation de la non-toxicité du neutralisant (B.4.1.2.b) ou du témoin de filtration sur membrane (B.4.2.2 b). <i>C</i> : Nombre d'ufc/ml dans l'essai de validation de l'inactivation par dilution neutralisation (B.4.1.2 c) ou par filtration sur membrane (B.4.2.2 c).</p> <p>Critères de validation : <i>Nv</i> compris entre 6×10^2 et 3×10^3 UFC / ml. <i>A</i> et <i>B</i> supérieurs ou égaux à $0,05 \times Nv$ <i>C</i> supérieur ou égal à $0,5 \times B$</p>						

Conclusion : La méthode de neutralisation par dilution n'est pas validée.

Essai 2 : neutralisation par filtration
(Essais réalisés en parallèle à l'essai proprement dit)

Souche(s) :	Nombre de cellules viables (u.f.c/ml) :					
	Suspension de validation (spores) : Nv₀	Témoin des conditions expérimentales : A	Témoin de non toxicité du neutralisant : B	Concentration du produit mise en œuvre pour la validation :	Validation de la méthode de filtration sur membranes: C	Conclusion :
<i>Bacillus subtilis</i> DSM 347	Vc : 200 ; 186 Nv : $1,9 \times 10^3$	Vc : 172 ; 188 Nv : $1,8 \times 10^2$	Vc : 182 ; 193 Nv : $1,9 \times 10^2$	80% (v/v)	Vc : 185 ; 172 Nv : $1,8 \times 10^2$	Validée
<p><i>Nv</i> : Nombre d'ufc/ml de la suspension de spores (B.2.). <i>A</i> : Nombre d'ufc/ml dans l'essai de validation des conditions expérimentales (B. 4.1.2 a ou B.4.2.2 a). <i>B</i> : Nombre d'ufc/ml dans l'essai de validation de la non-toxicité du neutralisant (B.4.1.2.b) ou du témoin de filtration sur membrane (B.4.2.2 b). <i>C</i> : Nombre d'ufc/ml dans l'essai de validation de l'inactivation par dilution neutralisation (B.4.1.2 c) ou par filtration sur membrane (B.4.2.2 c).</p> <p>Critères de validation : <i>Nv</i> compris entre 6×10^2 et 3×10^3 UFC / ml. <i>A</i> et <i>B</i> supérieurs ou égaux à $0,05 \times Nv$ <i>C</i> supérieur ou égal à $0,5 \times B$</p>						

Conclusion : La neutralisation est validée avec la méthode de filtration testée.

Essai proprement-dit (méthode par filtration sur membranes) :

Souche(s) :	Suspension d'essai de spores : N	Nombre de cellules viables (u.f.c/ml) pour le mélange d'essai pour les concentrations en % (v/v) de :		
		20%	40%	80%
<i>Bacillus subtilis</i> DSM 347	10 ⁻⁴ : 212 10 ⁻⁵ : 240 N = 2,25 x 10 ⁶	Vc1 : > 300 Vc2 : > 300 Na : > 3,0 x 10 ³	Vc1 : 112 Vc2 : 95 Na : 1,1 x 10 ³	Vc1 : < 15 Vc2 : < 15 Na : < 1,5 x 10 ²

Réduction du nombre de cellules viables aux concentrations d'essai en % (v/v) :

	20%	40%	80%
<i>Bacillus subtilis</i> DSM 347	log R : < 0,75 x 10 ²	log R : 2,05 x 10 ²	log R : > 1,5 x 10 ³
<p>Critères de validation : N compris entre 1,5 x 10⁶ et 5,0 x 10⁶</p> <p>Vc : nombre d'ufc comptées. N : Nombre d'ufc/ml de la suspension d'essai de spores (5.4.1.3.). Nv : Nombre d'ufc/ml de la suspension de spores (B.2.). Na : Nombre d'ufc/ml dans le mélange d'essai (5.5.2.2.3. ou 5.5.2.3.3). R : Réduction du nombre de cellules viables (5.6.3.)</p>			

VI. CONCLUSION :

Conformément à la norme européenne **NF EN 13 704** (avril 2002),

- En **15 minutes de contact à 20°C** [conditions optionnelles],
- Dans les **conditions de propreté (0,3 g/l d'albumine bovine)**,
- Vis-à-vis de la souche *Bacillus subtilis* DSM 347,

Le produit **1226 IND01 (le 16/04/13)** dilué à **80,0% (v/v)** présente une activité sporicide.

BILAN TEST PHAGOSPORE

Philippe SALIOU*, Anne LE GRAND*, Madeleine RAGUENES**

* Service Hygiène Hospitalière CHRU BREST

** DAHL CHRU BREST

Introduction :

Phagospore est un produit nettoyant-désinfectant pour sol et surfaces hautes formulé à base d'acide peracétique (300 ppm). En plus des activités bactéricide (EN 13727) et fongicide (EN 13697) classiques pour ce type de produit, Phagospore est virucide (EN 14476) et sporicide (*Clostridium difficile* selon EN 13704).

De novembre 2013 à avril 2014, Phagospore a été testé, dans trois services du CHRU de BREST (2 services de SSR et un service de médecine à orientation gériatrique).

Pendant la première phase de l'essai, Phagospore était utilisé 15 jours consécutifs pour nettoyer et désinfecter le sol (bidon de 5 litres) et les surfaces hautes (flacon de 750 mL) d'une chambre afin de s'assurer de sa compatibilité avec les matériaux.

Pendant la seconde phase, Phagospore était utilisé dans la chambre des malades ayant une gastroentérite aiguë (GEA) à Norovirus ou une diarrhée à *Clostridium difficile* afin de vérifier, son acceptabilité par les professionnels.

Pendant l'essai, les utilisateurs remplissaient une fiche d'évaluation comprenant 6 parties : conditionnement, tolérance (odeur, cutanée, respiratoire), efficacité (vitesse de séchage, pouvoir nettoyant, facilité d'utilisation, aspect des surfaces après utilisation, traces), compatibilité avec les matériaux, comparaison avec l'eau de javel (odeur, aspect surfaces après utilisation, facilité d'utilisation, tolérance, compatibilité avec les matériaux) et commentaires libres.

Résultats :

49 fiches d'évaluations ont été remplies et analysées.

95,6% des utilisateurs sont satisfaits ou très satisfaits du flacon 750 ml et du pulvérisateur. Mais, 1/3 sont peu ou pas satisfaits du bidon de 5 litres jugé trop lourd et peu maniable.

L'ensemble des utilisateurs trouve l'odeur du Phagospore parfumé à la menthe satisfaisante, et plus agréable que celle de l'eau de javel. Mais ils étaient 74% à ne pas apprécier l'odeur initiale (parfum Niaouli), 57% trouvaient l'odeur d'acide acétique (vinaigre) trop marquée. Près de la moitié (47%) trouvait son odeur moins agréable que celle de l'eau de javel.

Près de 80% des utilisateurs jugent que la tolérance cutanée du Phagospore est bonne et 70% d'entre eux qu'elle est meilleure que celle de l'eau de javel. Ces deux produits doivent être utilisés avec des gants de protection.

Presque tous les utilisateurs apprécient le pouvoir détergent du Phagospore (98%) et sa rapidité de séchage (96%). La majorité (77%) juge l'aspect des surfaces satisfaisant ou très satisfaisant (absence de trace : 70%) et 70% jugent le résultat meilleur qu'avec l'eau de javel. Cependant, 6 utilisateurs notent que Phagospore mousse lors de son application sur le sol ou que celui-ci est collant après son utilisation. Enfin 82% trouvent Phagospore facile d'utilisation, et 85% plus facile d'utilisation que l'eau de javel.

Discussion :

L'entretien des chambres se fait avec des produits détergents désinfectants bactéricides et fongicides. Les surfaces de la chambre d'un malade ayant une GEA à Norovirus ou une diarrhée à *Clostridium difficile*, doivent être désinfectées à de l'eau de javel (1, 2). Cette désinfection nécessite de réaliser un bionettoyage en 5 étapes (nettoyage, rinçage, séchage, désinfection javel, séchage). Cette désinfection lourde à mettre en place et chronophage est souvent difficile à appliquer surtout en période d'épidémie, notamment à Norovirus, qui touche les malades et le personnel. Phagospore, produit nettoyant désinfectant permet de réduire ce protocole à deux étapes (application du produit et séchage). L'eau de Javel nécessite un temps de contact de 10 minutes. Phagospore est actif en 10 minutes sur *Clostridium difficile* selon la norme EN 13704 et en 5 minutes sur Norovirus selon la norme EN 14476.

L'essai montre que Phagospore parfum menthe a une odeur jugée agréable par les utilisateurs. Aucun effet secondaire cutané ou respiratoire notable n'a été signalé dans la mesure où les précautions d'utilisation (port de gants) sont respectées.

Il n'a pas été constaté d'altération ou d'incompatibilité avec le matériel et les surfaces traitées durant la période de l'essai.

La facilité d'utilisation, le pouvoir nettoyant et la qualité du nettoyage sont jugés excellents par la majorité des utilisateurs.

Références :

- 1- Avis relatif à la maîtrise de la diffusion des infections à *Clostridium difficile* dans les établissements de santé français. Haut Conseil de la Santé Publique juin 2008, 11 pages.
- 2- Recommandations relatives aux conduites à tenir devant des gastro-entérites aiguës en établissement d'hébergement pour personnes âgées. Commission spécialisée Maladies transmissibles Haut Conseil de la Santé Publique janvier 2010, 77 pages.

RAPPORT D'ESSAI
N° 3410-1

55 Boulevard Jules Verger
35803 DINARD Cedex
Tél. 02 99 16 50 72
Fax. 02 99 16 52 75

Imprimé le : 19/09/14
Date de 1^{ère} impression : 19/09/14
Page 1 sur 5

Test d'efficacité sporicide
contre les spores de *Clostridium difficile* CIP 104282
selon une méthodologie adaptée de la norme
NF EN 13697 (Novembre 2001)
1226 IND01

DESTINATAIRE : CHRISTEYNS FRANCE

I- IDENTIFICATION DU DONNEUR D'ORDRE

Monsieur Jérôme DUBOURGEOIS
CHRISTEYNS FRANCE
31 rue de la Maladrie
44 120 VERTOU
Tél.02-40-80-27-27 - Fax. 02-40-03-09-73

II- IDENTIFICATION DE L'ECHANTILLON

- Nom du produit : **1226 IND01**
- Numéro de lot : PR178-4
- Fabricant : CHRISTEYNS FRANCE
- Date de fabrication : 02/07/14
- Date de péremption : non communiquée
- Date de réception au laboratoire : 18/07/14
- Aspect du produit : Produit limpide transparent
- Conditions de stockage : à température ambiante et à l'abri de la lumière
- Diluant du produit recommandé par le fabricant : non concerné
- Matière(s) active(s) : Non communiquées

RAPPORT D'ESSAI N° 3410-1

55 Boulevard Jules Verger
35803 DINARD Cedex
Tél. 02 99 16 50 72
Fax. 02 99 16 52 75

Imprimé le : 19/09/14
Date de 1^{ère} impression : 19/09/14
Page 2 sur 5

III- METHODE D'ESSAI

Méthodologie adaptée de la norme NF EN 13697 (Novembre 2001) : « Essai quantitatif de surface non-poreuse pour l'évaluation de l'activité bactéricide et/ou fongicide des désinfectants chimiques utilisés dans le domaine de l'agro-alimentaire, dans l'industrie, dans les domaines domestiques et en collectivité ». (Phase 2, étape 2)

Réduction recherchée demandée par le client : 4 Log.

Neutralisant : 3% Polysorbate 80 ; 3% Saponine ; 0,3% lécithine d'œuf ; 0,1% L-Histidine ; 0,5% Thiosulfate de sodium (stérilisé à 121°C pendant 20 minutes).

IV- CONDITIONS EXPERIMENTALES

- Période d'analyse : du 16/09/14 au 19/09/14
- Analyse réalisée par : AF. GABILLET
- Diluant du produit utilisé au cours de l'essai : eau distillée
- Concentrations de produit testé (V/V) : 10%-50% et 100%
- Aspect des dilutions : limpides
- Temps de contact : 15 minutes (+/- 10 secondes)
- Température d'essai : 20°C (+/-1°C)
- Substance interférente : 3 g/ d'albumine bovine (conditions de saleté)
- Température d'incubation : 37°C (+/-1°C) en anaérobiose
- Identification des spores utilisées :
 - Spores de *Clostridium difficile* CIP 104282 (séchage pendant 35 minutes à 37°C +/-1°C)

**RAPPORT D'ESSAI
N°3410-1**

55 Boulevard Jules Verger
35803 DINARD Cedex
Tél. 02 99 16 50 72
Fax. 02 99 16 52 75

Imprimé le : 19/09/14
Date de 1^{ère} impression : 19/09/14
Page 3 sur 5

V- RESULTATS D'ESSAI

Vc : nombre de colonies comptées sur les boîtes,

N: nombre de cellules dénombrées par 0,05 ml dans la suspension microbienne d'essai et de la suspension de validation,

Nd: logarithme du nombre d'UFC/surface d'essai pour l'essai avec le désinfectant,

Nc: logarithme du nombre d'UFC/surface d'essai pour le témoin d'eau,

NC: logarithme du nombre d'UFC/surface d'essai du témoin de neutralisation,

NT : logarithme du nombre d'UFC/surface d'essai de neutralisation,

ME : effet microbicide (ME= Nc-Nd).

RAPPORT D'ESSAI

N°3410-1

55 Boulevard Jules Verger
 35803 DINARD Cedex
 Tél. 02 99 16 50 72
 Fax. 02 99 16 52 75

Imprimé le : 19/09/14
 Date de 1^{ère} impression : 19/09/14
 Page 4 sur 5

Essai sur les spores de Clostridium difficile CIP 104282

Souche testée	Suspension microbienne d'essai	Essai de validation		
		Témoin d'eau (Nc)	Témoin de neutralisation (NC)	Essai de neutralisation (NT)
<i>Spores de Clostridium difficile</i> CIP 104282	10^{-5} : Vc1 = 63 Vc2 = 31	10^{-2} : Vc1 = 134 Vc2 = 114	10^{-2} : Vc1 = 93 Vc2 = 91	10^{-2} : Vc1 = 91 Vc2 = 75
	10^{-6} : Vc1 = 3 Vc2 = 4	10^{-3} : Vc1 = 13 Vc2 = 24	10^{-3} : Vc1 = 25 Vc2 = 12	10^{-3} : Vc1 = 21 Vc2 = 14
	N = 6,37	Nc = 6,09 Nts > 100	NC = 5,96	NT = 5,92

L'essai est validé si :

N-Nc est inférieur ou égal à 2 Log

N-NC est inférieur ou égal à 2 Log

NC-NT est inférieur ou égal à +/- 0,3

Nts est inférieur à 100 UFC pour les concentrations actives. Pour les concentrations non actives, Nts peut ne pas être dénombrable.

Souche testée		Concentrations testées (V/V)				
		10%	50%	100%		
<i>Spores de Clostridium difficile</i> CIP 104282	10^0	>300 ; >300	0 ; 0	0 ; 0		
	10^{-1}	>300 ; >300	0 ; 0	0 ; 0		
	10^{-2}	67 ; 77	0 ; 0	0 ; 0		
	Dénombrement surface (Nts)	>100	0	0		
	Nd	5,86	<1	<1		
	ME	0,23	>5,09	>5,09		

(la technique de dénombrement utilisée est la technique par étalement en surface de 0,1 ml)

RAPPORT D'ESSAI
N° 3410-1

55 Boulevard Jules Verger
35803 DINARD Cedex
Tél. 02 99 16 50 72
Fax. 02 99 16 52 75

Imprimé le : 19/09/14
Date de 1^{ère} impression : 19/09/14
Page 5 sur 5

VI- CONCLUSION

Selon une méthodologie adaptée de la norme NF EN 13697 (Novembre 2001), le lot PR178-4 du produit 1226 INDO1 de la société CHRISTEYNS FRANCE, présente une réduction supérieure à 5,09 Log sur les surfaces, lorsqu'il est testé à 50% et 100% (V/V), en présence d'albumine bovine à 3 g/l (conditions de saleté), en 15 minutes de temps de contact, à la température de 20°C vis-à-vis des spores de *Clostridium difficile* CIP 104282.




Les spores ont été soumises à essai une seule fois.

Commentaires :

Les spores ont été dénombrées sur de la gélose cœur/cerveille additionnée de 5% de sang de mouton et de 0,1% de taurocholate. L'incubation est de 3 jours à 37°C (+/-1°C) sous atmosphère anaérobie.

VII-SIGNATURES

Fait à DINARD, le

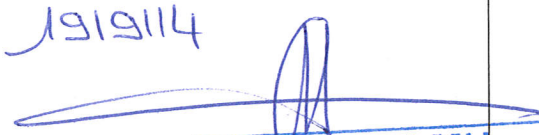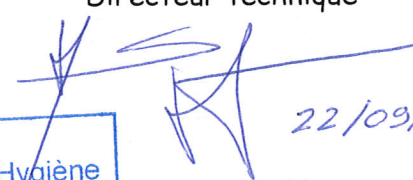Rédigé par	Validé par
<p>AF. GABILLET Responsable d'essai</p> <p>19/09/14</p> 	<p>M. SESQUES Docteur en microbiologie Directeur technique</p>  <p>22/09/2014</p>
 <p>LMH Laboratoire Microbiologie et Hygiène 55 Boulevard Jules Verger - BP 10180 35803 DINARD CEDEX Tél. 02 99 16 50 72 - Fax 02 99 16 52 75</p>	