



***Manufacturer: Zhenjiang Huayang Latex Products Co., Ltd.
Address: Lianhe Village, Xinba Town, Yanzhong City, Jiangsu
Province, 212212, P.R. China***

Product Technical Specifications

**Sterile Latex Surgical Gloves
Reference Number: SCMDG001**



Manufacturer: Zhenjiang Huayang Latex Products Co., Ltd.
Address: Lianhe Village, Xinba Town, Yanzhong City, Jiangsu Province, 212212, P.R. China

1. Types/specifications of sterile latex surgical gloves and instructions of its classificaton

1.1 Sterile Latex Surgical Gloves

1.2 Sizes:

6# 6.5# 7# 7.5# 8# 8.5# 9#

1.3 Types and specifications of Sterile Latex Surgical Gloves should meet the requirements of sheet 1

Sheet 1 Surgical Gloves specifications and basic sizes

Order	6	6.5	7	7.5	8	8.5	9	Franchise
A	76	83	89	95	102	108	114	±6mm
B	0.13	0.13	0.13	0.13	0.13	0.13	0.13	min
C	265	265	265	265	265	265	265	min

1.4 Powder:


Powdered or Powder-free

1.5 Purpose:

Protection of the wearer from contamination with blood, secretions, and excretions and the associated risk of contamination with pathogens capable of reproduction.
Protection from chemicals.



Manufacturer: Zhenjiang Huayang Latex Products Co., Ltd.
Adress: Lianhe Village, Xinba Town, Yanzhong City, Jiangsu Province, 212212, P.R. China

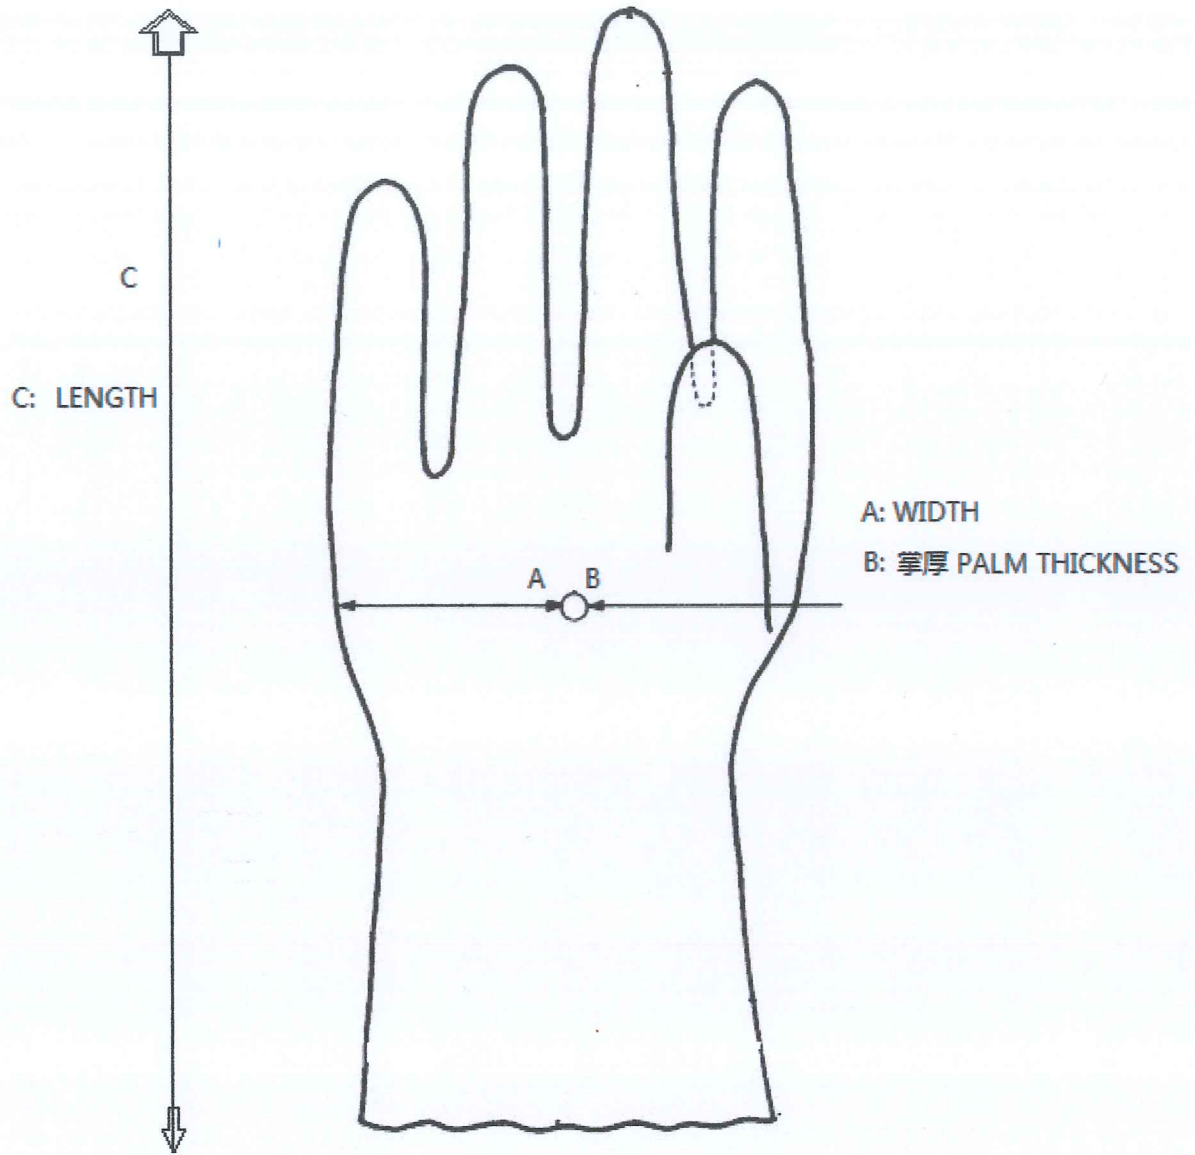



Manufacturer: Zhenjiang Huayang Latex Products Co., Ltd.
Address: Lianhe Village, Xinba Town, Yanzhong City, Jiangsu Province, 212212, P.R. China

2. Material Descriptions

Sterile latex surgical gloves are mainly made of natural rubber.

All material information--Natural rubber.

3. Requirement of the Product appearance

3.1 Product appearance

Sterile latex surgical gloves have no obvious stains, holes and edges.

3.2 Main Product Performance

	<i>Requirement</i>	<i>Results</i>
<i>BEFORE AGING TENSILE STRENGTH Mpa</i>	≥ 24	≥ 29.2
<i>BEFORE AGING ULTIMA ELONGATION %</i>	≥ 750	≥ 835
<i>AFTER ACCELERATED AGING TENSILE STRENGTH</i>	≥ 18	≥ 22.3
<i>AFTER ACCELERATED ULTIMATE ELONGATION</i>	≥ 560	≥ 645

3.3 Standards:

EN 455-1 EN 455-2, EN 455-3, ASTM D3577



Manufacturer: Zhenjiang Huayang Latex Products Co., Ltd.
Adress: Lianhe Village, Xinba Town, Yanzhong City, Jiangsu Province, 212212, P.R. China

3.4 Sterile

Sterile Latex Surgical Gloves should be supplied aseptically and should be made sterile by an sterilization process .

Sterilization - gamma rays

4. Package

pairsof surgical+1 inne paper+1 pouch /paper 50pairs pouch/1paper box ,10 paper boxes/paper carton.

5. Certificates:

ISO 13485, CE

6.Valid day

Under the specified storage conditions,the period of validity is 3 years from the date of production.

