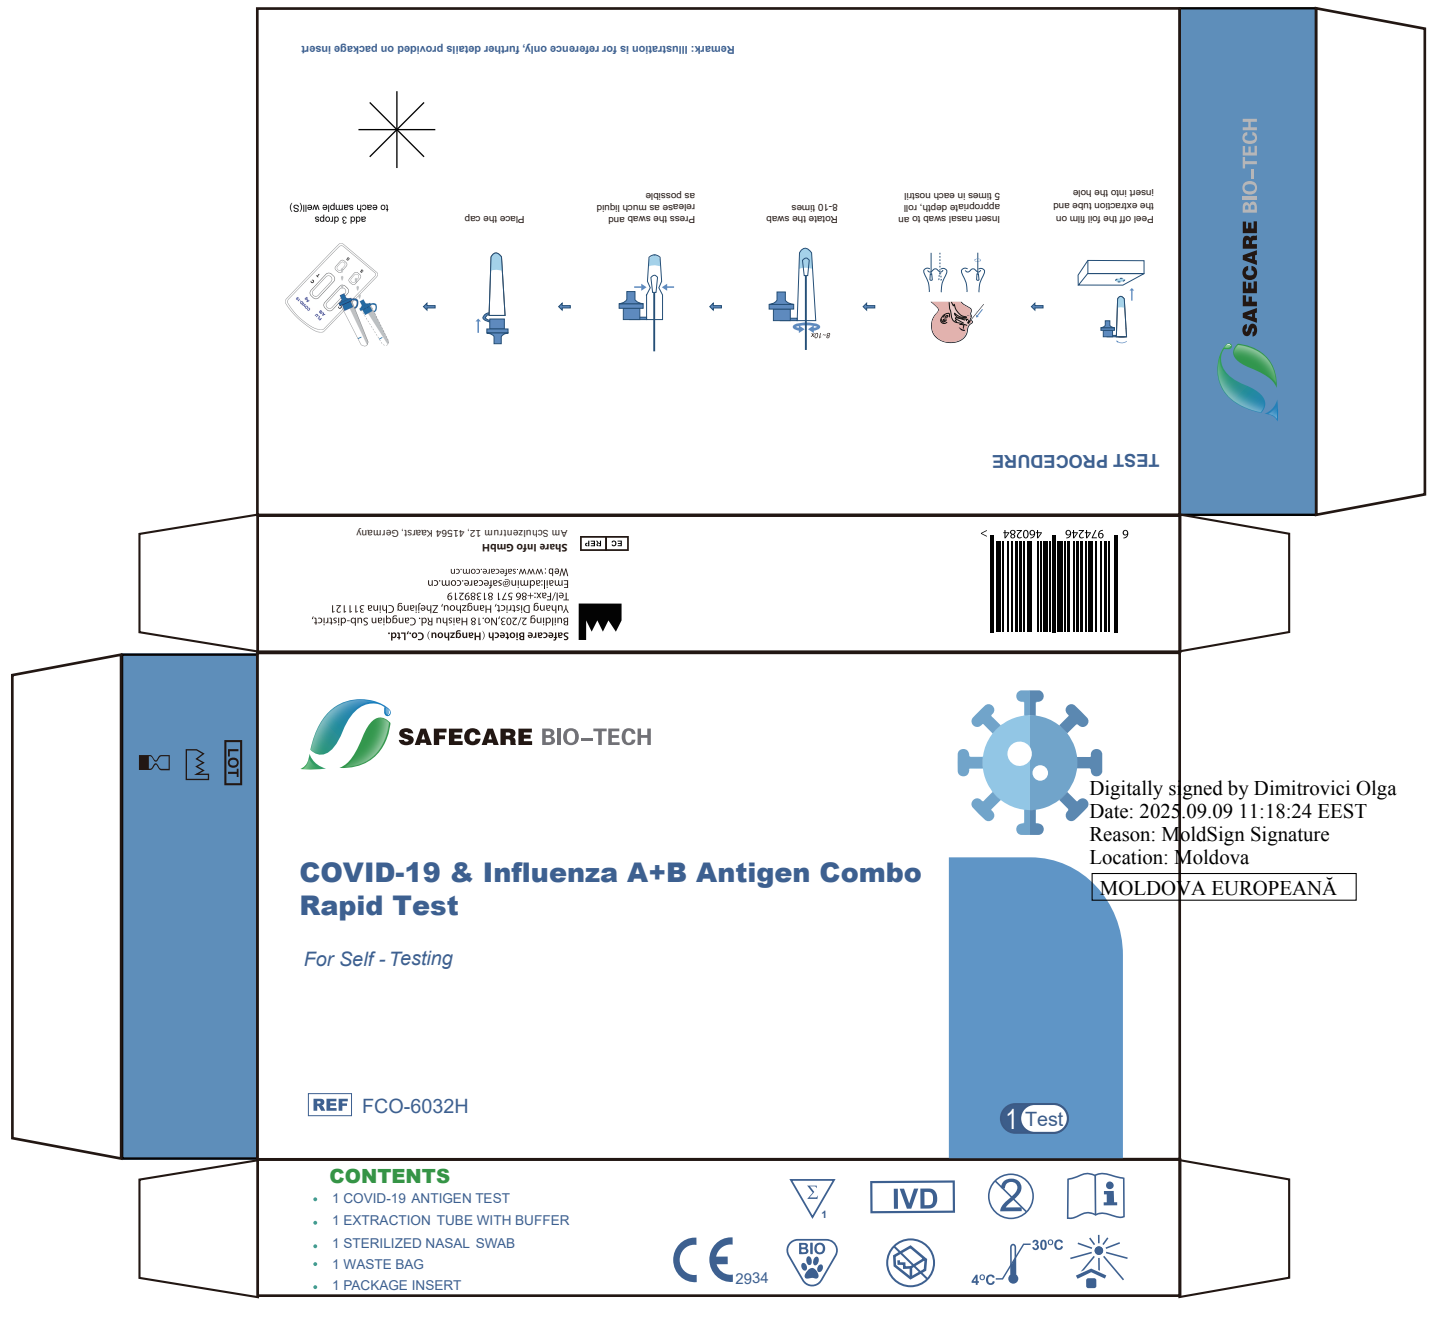

Digitally signed by Dimitrovici Olga
Date: 2025.09.09 11:18:24 EEST
Reason: MoldSign Signature
Location: Moldova

MOLDOVA EUROPEANĂ

SAFECARE BIO–TECH

TEST PROCEDURE

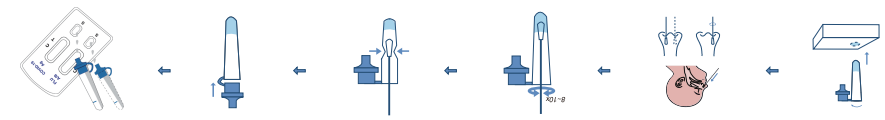

Peel off the foil film on the extraction tube and insert into the hole

Insert nasal swab to an appropriate depth, roll 5 times in each nostril

Rotate the swab 8-10 times

Press the swab and release as much liquid as possible

Place the cap

add 3 drops to each sample well(S)

Remark: Illustration is for reference only, further details provided on package insert

Safecare Biotech (Hangzhou) Co.,Ltd.
Building 2/203,No.18 Haishu Rd. Cangqian Sub-district, Yuhang District, Hangzhou, Zhejiang China 311121
Tel/Fax:+86 571 81389219
Email:admin@safecare.com.cn
Web:www.safecare.com.cn

EC REP **Share Info GmbH**
Am Schulzentrum 12, 41564 Kaarst, Germany

6 974246 462240 >

LOT

SAFECARE BIO–TECH

COVID-19 & Influenza A+B Antigen Combo Rapid Test

For Self - Testing

REF FCO-6032H

2 Test

CONTENTS

- 2 COVID-19 ANTIGEN TESTS
- 2 EXTRACTION TUBE WITH BUFFER
- 2 STERILIZED NASAL SWABS
- 2 WASTE BAGS
- 1 PACKAGE INSERT

Σ 2 IVD 2

CE 2934 BIO 4°C–30°C

SAFECARE BIO-TECH

COVID-19 & Influenza A+B Antigen Combo Rapid Test

For Self - Testing

REF FCO-6032H

5 Tests

TEST PROCEDURE



Remark: Illustration is for reference only, further details provided on package insert

SAFECARE BIO-TECH

Safecare Biotech (Hangzhou) Co.,Ltd.
Building 2/203,No.18 Haishu Rd, Cangqian Sub-district,
Yuhang District, Hangzhou, Zhejiang China 311121
Tel/Fax:+86 571 81389219
Email:admin@safecare.com.cn
Web:www.safecare.com.cn

EC REP **Share Info GmbH**
Am Schulzentrum 12, 41564 Kaarst, Germany

CONTENTS

- 5 COVID-19 ANTIGEN TESTS
- 5 EXTRACTION TUBES WITH BUFFER
- 5 STERILIZED NASAL SWABS
- 5 WASTE BAGS
- 1 PACKAGE INSERT

Σ 5

IVD

4°C–30°C

CE 2934

BIO

SAFECARE BIO-TECH

LOT

6 974246 460291

SAFECARE BIO-TECH

COVID-19 & Influenza A+B Antigen Combo
Rapid Test

For Self - Testing

REF FCO-6032H

10 Tests

TEST PROCEDURE



Remark: Illustration is for reference only, further details provided on package insert

SAFECARE BIO-TECH

Safecare Biotech（Hangzhou）Co.,Ltd.
Building 2/203,No.18 Haishu Rd. Cangqian Sub-district,
Yuhang District, Hangzhou, Zhejiang China 311121
Tel/Fax:+86 571 81389219
Email:admin@safecare.com.cn
Web:www.safecare.com.cn

EC REP **Share Info GmbH**
Am Schulzentrum 12, 41564 Kaarst, Germany

CONTENTS

- 10 COVID-19 ANTIGEN TESTS
- 10 EXTRACTION TUBES WITH BUFFER
- 10 STERILIZED NASAL SWABS
- 10 WASTE BAGS
- 1 PACKAGE INSERT
- 1 WORKSTATION

Σ 10 IVD 4°C 30°C CE 2934 BIO

SAFECARE BIO-TECH

LOT

6 974246 460307

SAFECARE BIO-TECH

COVID-19 & Influenza A+B Antigen Combo Rapid Test

For Self - Testing

REF FCO-6032H

20 Tests

TEST PROCEDURE

Peel off the foil film on the extraction tube and insert into the hole of workstation

Insert nasal swab to an appropriate depth, roll 5 times in each nostril

Rotate the swab 8-10 times

Press the swab and release as much liquid as possible

Place the cap

add 3 drops to each sample well(S)

Remark: Illustration is for reference only, further details provided on package insert

SAFECARE BIO-TECH

Safecare Biotech（Hangzhou）Co.,Ltd.
Building 2/203,No.18 Haishu Rd. Cangqian Sub-district,
Yuhang District, Hangzhou, Zhejiang China 311121
Tel/Fax:+86 571 81389219
Email:admin@safecare.com.cn
Web:www.safecare.com.cn

EC REP **Share Info GmbH**
Am Schulzentrum 12, 41564 Kaarst, Germany

CONTENTS

- 20 COVID-19 ANTIGEN TESTS
- 20 EXTRACTION TUBES WITH BUFFER
- 20 STERILIZED NASAL SWABS
- 20 WASTE BAGS
- 1 PACKAGE INSERT
- 1 WORKSTATION

Σ 20

IVD

4°C 30°C

CE 2934

BIO

SAFECARE BIO-TECH

LOT

6 974246 460314

SAFECARE BIO-TECH

COVID-19 & Influenza A+B Antigen Combo Rapid Test

For Self - Testing

REF FCO-6032H

25 Tests

TEST PROCEDURE



Peel off the foil film on the extraction tube and insert into the hole of workstation

Insert nasal swab to an appropriate depth, roll 5 times in each nostril

Rotate the swab 8-10 times

Press the swab and release as much liquid as possible

Place the cap

add 3 drops to each sample well(S)

Remark: Illustration is for reference only, further details provided on package insert

SAFECARE BIO-TECH

Safecare Biotech (Hangzhou) Co.,Ltd.
Building 2/203,No.18 Haishu Rd. Cangqian Sub-district, Yuhang District, Hangzhou, Zhejiang China 311121
Tel/Fax:+86 571 81389219
Email:admin@safecare.com.cn
Web:www.safecare.com.cn

EC REP Share Info GmbH
Am Schulzentrum 12, 41564 Kaarst, Germany

CONTENTS

- 25 COVID-19 ANTIGEN TESTS
- 25 EXTRACTION TUBES WITH BUFFER
- 25 STERILIZED NASAL SWABS
- 25 WASTE BAGS
- 1 PACKAGE INSERT
- 1 WORKSTATION

SAFECARE BIO-TECH

LOT

6 974246 460321

open notch 15mm

open notch 15mm

SAFECARE BIO–TECH

COVID-19 & Influenza A+B Antigen Combo Rapid Test

For Self - Testing

REF FCO-6032H

Σ 1 IVD 4°C–30°C CE 2934

LOT

Safecare Biotech (Hangzhou) Co.,Ltd.
Building 2/203,No.18 Haishu Rd. Cangqian Sub-district,
Yuhang District, Hangzhou, Zhejiang China 311121
Tel/Fax:+86 571 81389219
Email:admin@safecare.com.cn
Web:www.safecare.com.cn

EC REP **Share Info GmbH**
Am Schulzentrum 12, 41564 Kaarst, Germany