

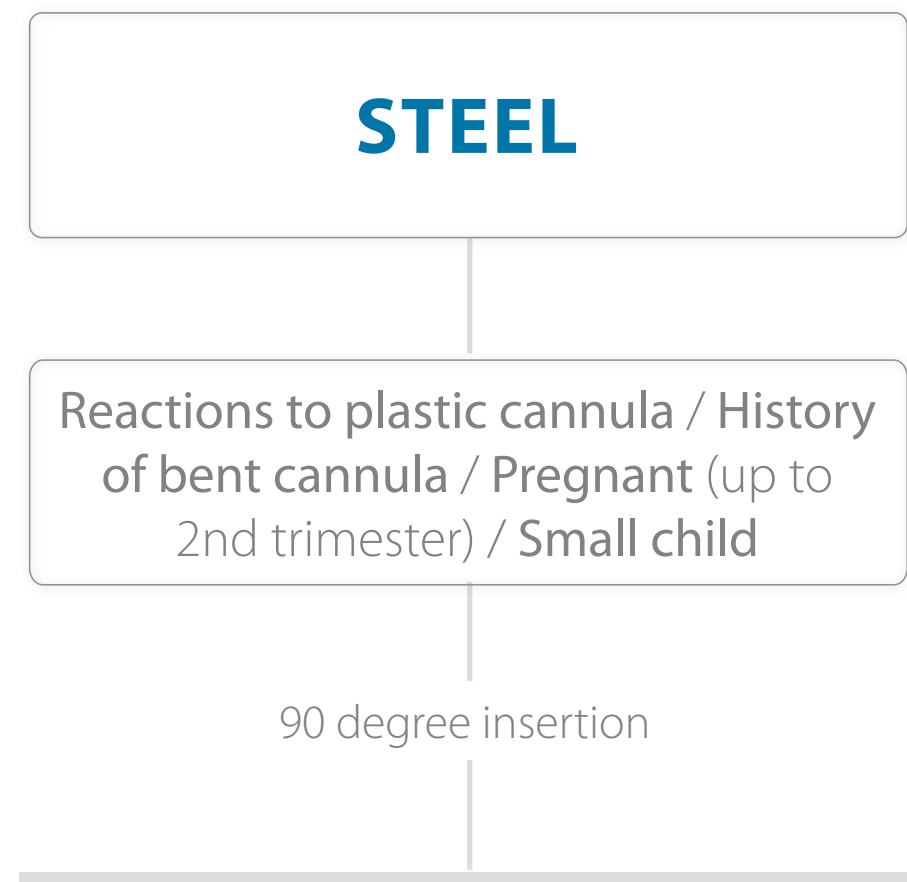
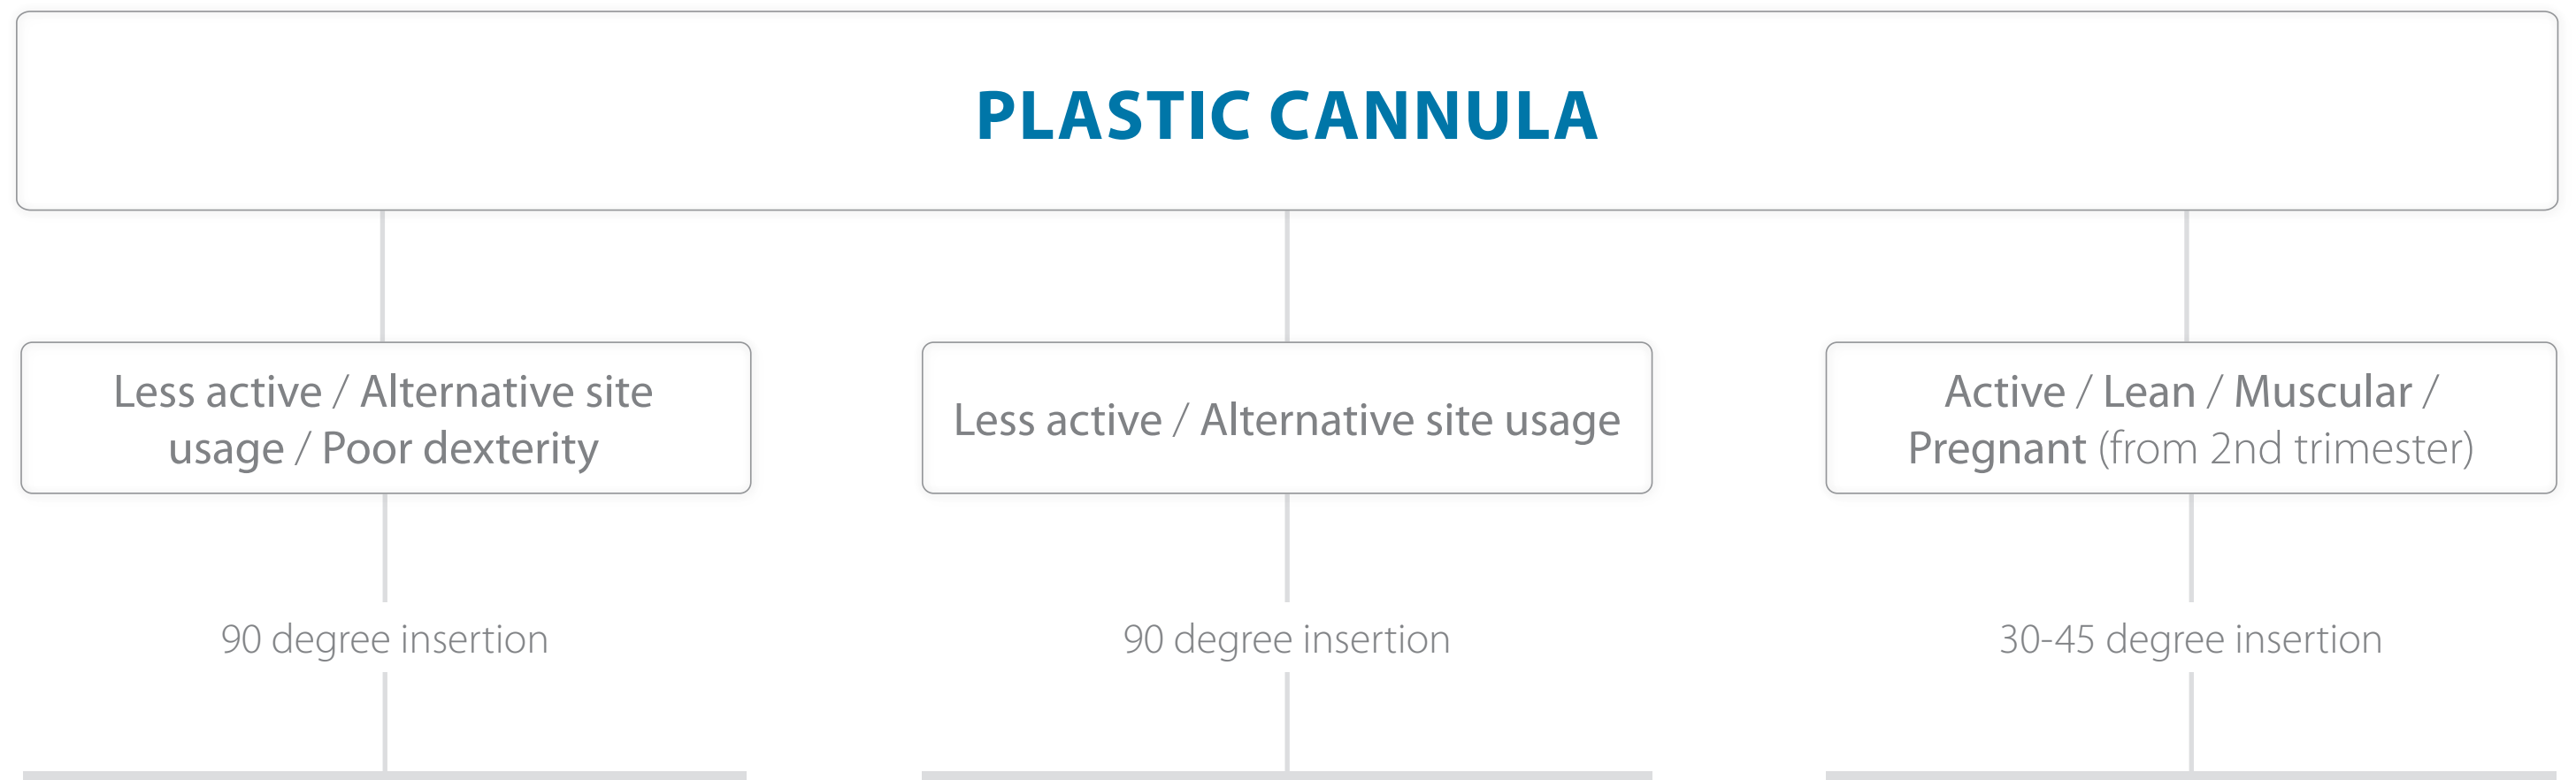




Which infusion set is right for you?

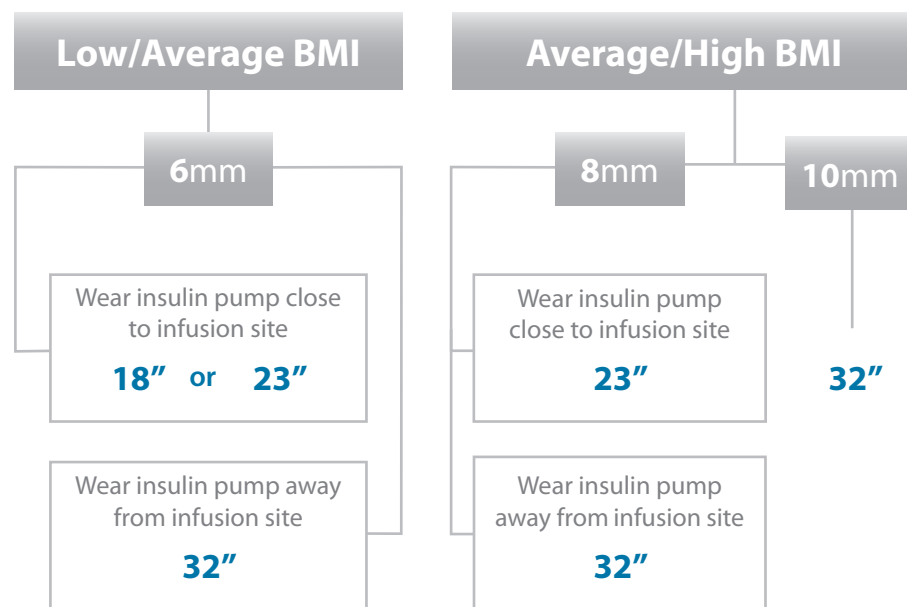


Sure-T® infusion set
Simple steel needle infusion set

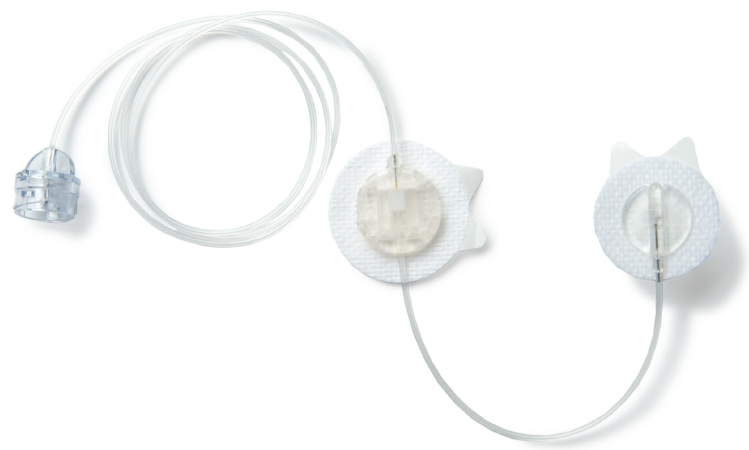


Quick-set® infusion set
Our most popular infusion set

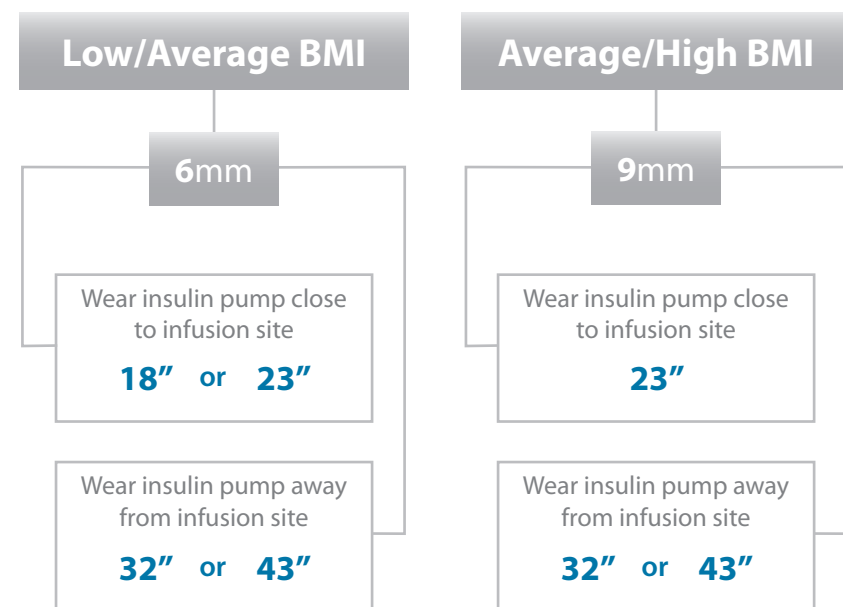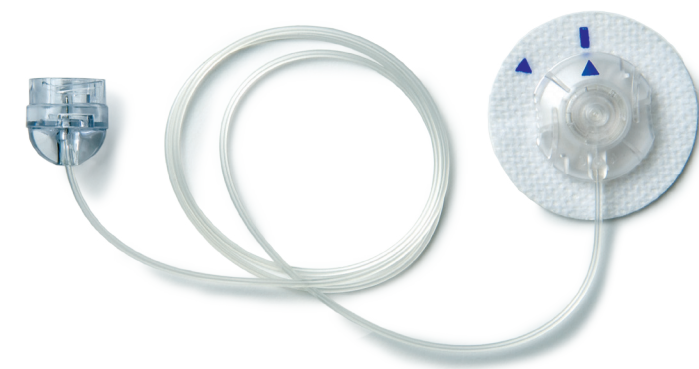

mio® infusion set
Convenient "all in one" infusion set

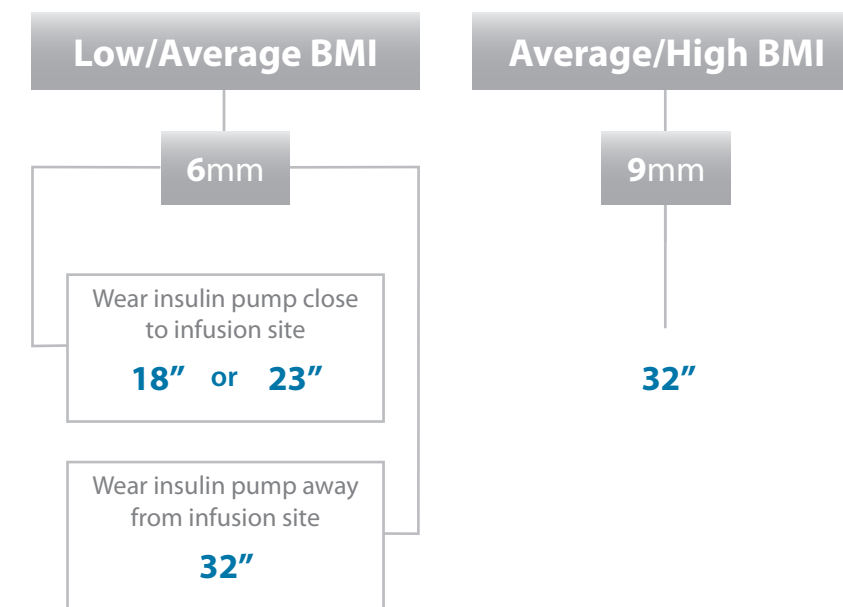

Silhouette® infusion set
Flexible insertion angle infusion set

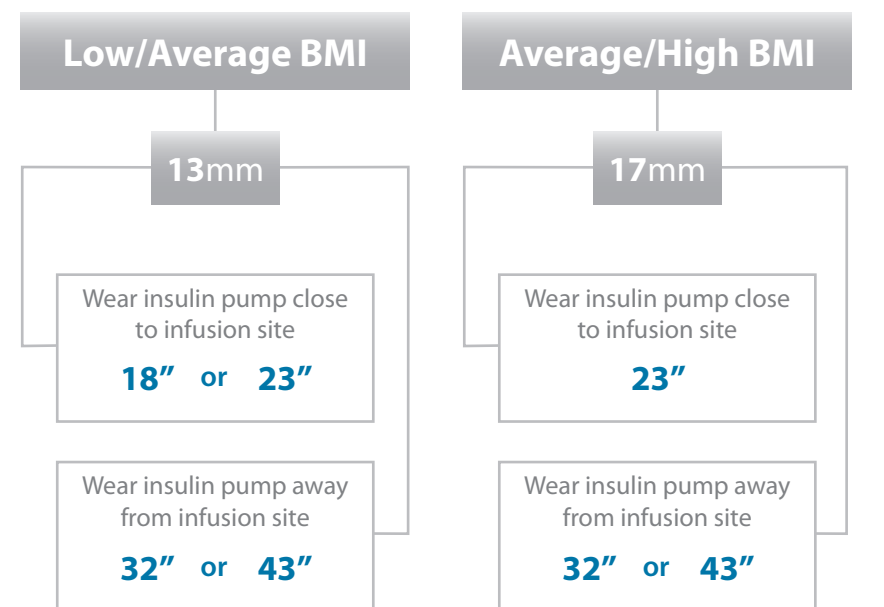

Recommendation based on Insulin Pump Therapy: Best practices in choosing and using infusion devices. American Association of Diabetes Educators, 2011. Data on file.

BMI stands for Body Mass Index which is calculated based on an individual's weight and height.

Safety Information
Infusion sets are indicated for the subcutaneous infusion of medication, including insulin, from infusion pumps. They are neither intended nor indicated for intravenous (IV) infusion or the infusion of blood or blood products. Inaccurate medication, delivery, infection and/or site irritation may result from improper insertion and maintenance of the infusion insertion and maintenance of the infusion site. Replace the infusion set every 48-72 hours, or per your healthcare professional's instructions.
Mio, Quick-set, Silhouette, and Sure-T are registered trademarks of Medtronic MiniMed, Inc.