



CE-DOC-H033
Version 2.0

EC Declaration of Conformity

In accordance with Directive 98/79/EC

Legal Manufacturer: *Healgen Scientific Limited Liability Company*

Legal Manufacturer Address: *3818 Fuqua Street, Houston, TX 77047, USA*

Declares, that the products
Product Name and Model(s)

Troponin I Rapid Test Cassette (Serum/Plasma)	GDTRO-302a
---	------------

Classification: *Other*

Conformity assessment route: *Annex III (EC DECLARATION OF CONFORMITY)*

We, the Manufacturer, herewith declare with sole responsibility that our product/s mentioned above meet/s the provisions of the Directive 98/79/EC of the European Parliament and of the Council on In-Vitro Diagnostic Medical Devices.

We hereby explicitly appoint

EC Representative's Name: QARAD BV

EC Representative's Address: Ciplastraat 3, 2440 Geel, BELGIUM

to act as our European Authorized Representative as defined in the aforementioned Directive.

I, the undersigned, hereby declare that the medical devices specified above conform with the directive 98/79/EC on in vitro diagnostic medical devices and pertinent essential requirements.

Date Signed: March 4, 2022

Name of authorized signatory: Joyce Pang
Position held in the company: Vice-President

Troponin I Rapid Test Cassette (Whole Blood/Serum/Plasma)

A rapid visual immunoassay for the qualitative presumptive detection of cardiac Troponin I in human whole blood, serum, or plasma specimens.
For professional *in vitro* diagnostic use only.

INTENDED USE

The Troponin I Rapid Test Cassette (Whole Blood/Serum/Plasma) is a rapid visual immunoassay for the qualitative presumptive detection of cardiac Troponin I in human whole blood, serum, or plasma specimens. This kit is intended to be used as an aid in the diagnosis of myocardial infarction (MI).

SUMMARY

Cardiac Troponin I (cTnI) is a protein found in cardiac muscle with a molecular weight of 22.5 kDa.¹ Troponin I is part of a three subunit complex comprising of Troponin T and Troponin C. Along with tropomyosin, this structural complex forms the main component that regulates the calcium sensitive ATPase activity of actomyosin in striated skeletal and cardiac muscle.² After cardiac injury occurs, Troponin I is released into the blood 4-6 hours after the onset of pain. The release pattern of cTnI is similar to CK-MB, but while CK-MB levels return to normal after 72 hours, Troponin I remains elevated for 6-10 days, thus providing for a longer window of detection for cardiac injury. The high specificity of cTnI measurements for the identification of myocardial damage has been demonstrated in conditions such as the perioperative period, after marathon runs, and blunt chest trauma.³ cTnI release has also been documented in cardiac conditions other than acute myocardial infarction (AMI) such as unstable angina, congestive heart failure, and ischemic damage due to coronary artery bypass surgery.⁴ Because of its high specificity and sensitivity in the myocardial tissue, Troponin I has recently become the most preferred biomarker for myocardial infarction.⁵

PRINCIPLE

The Troponin I Rapid Test Cassette (Whole Blood/Serum/Plasma) has been designed to detect cardiac Troponin I through visual interpretation of color development in the strip. The membrane was immobilized with anti-cTnI antibodies on the test region. During the test, the specimen is allowed to react with colored anti-cTnI antibodies colloidal gold conjugates, which were precoated on the sample pad of the test. The mixture then moves on the membrane by a capillary action, and interact with reagents on the membrane. If there were enough cTnI in specimens, a colored band will form at the test region of the membrane.

Presence of this colored band indicates a positive result, while its absence indicates a negative result. Appearance of a colored band at the control region serves as a procedural control. This indicates that proper volume of specimen has been added and membrane wicking has occurred.

PRECAUTIONS

- For professional *in vitro* diagnostic use only.
- Warning: the reagents in this kit contain sodium azide which may react with lead or copper plumbing to form potentially explosive metal azides. When disposing of such reagents, always flush with large volumes of water to prevent azide build-up.
- Do not use it if the tube/pouch is damaged or broken.
- Test is for single use only. Do not re-use under any circumstances.
- Handle all specimens as if they contain infectious agents. Observe established standard procedure for proper disposal of specimens
- Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are assay.
- Humidity and temperature can adversely affect results

STORAGE AND STABILITY

All reagents are ready to use as supplied. Store unused test device unopened at 2°C-30°C. If stored at 2°C-8°C, ensure that the test device is brought to room temperature before opening. The test is not stable out off the expiration date printed on the sealed pouch. Do not freeze the kit or expose the kit over 30°C.

SPECIMEN COLLECTION AND PREPARATION

- The Troponin I Rapid Test Cassette (Whole Blood/Serum/Plasma) is intended only for use with human whole blood, serum, or plasma specimens.
- Only clear, non-hemolyzed specimens are recommended for use with this test.
- Serum or plasma should be separated with soonest possible opportunity to avoid hemolysis.
- Perform the testing immediately after the specimen collection. Do not leave the specimens at room temperature for prolonged periods. Specimens may be stored at 2-8°C for up to 3 days. For long term storage, specimens should be kept below -20°C.
- Bring specimens to room temperature prior to testing. Frozen specimens must be completely thawed and mixed well prior to testing. Avoid repeated freezing and thawing of specimens.

- Pack the specimens in compliance with applicable regulations for transportation of etiological agents, in case they need to be shipped.
- Icteric, lipemic, hemolyzed, heat treated and contaminated sera may cause erroneous results.
- There is a slight possibility that some whole blood specimens with very high viscosity or which have been stored for more than 2 days may not run properly on the test device. Repeat the test with a serum or plasma specimen from the same patient using a new test device.

MATERIALS

Materials Provided

- 25 Sealed pouches each containing a test cassette, a dropper and a desiccant
- 1 Buffer, 4.0 mL
- 1 Package insert

Materials Required But Not Provided

- Specimen collection containers
- Clock or timer
- Centrifuge (for plasma only)

DIRECTIONS FOR USE

Allow test device, specimen, buffer and/or controls to equilibrate to room temperature (15-30°C) prior to testing.

- Remove the test from its sealed pouch, and place it on a clean, level surface. Label the device with patient or control identification. To obtain a best result, the assay should be performed within one hour.
- Transfer 2 drops of serum or plasma to the specimen well of the device with a disposable pipette provided in the kit, and then start the timer.

OR



Transfer 3 drops of whole blood specimen to the specimen well of the device with a disposable pipette provided in the kit, then add 1 drop of buffer, and start the timer.

OR

Allow 3 hanging drops of fingerstick whole blood specimen to fall into the center of the specimen well (S) on the device, then add 1 drop of buffer, and start the timer. Avoid trapping air bubbles in the specimen well (S), and do not drop any solution in observation window.

As the test begins to work, you will see color move across the membrane.

- Wait for the colored band(s) to appear. The result should be read at 10 minutes. Do not interpret the result after 20 minutes.

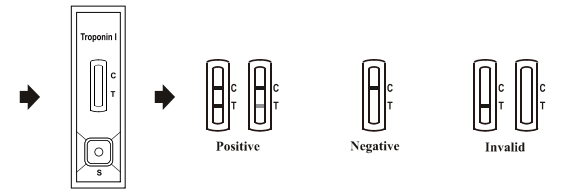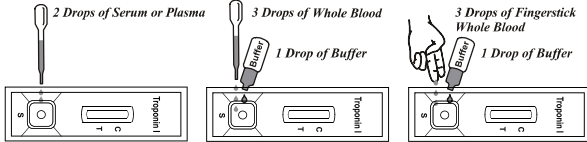

INTERPRETATION OF RESULTS

(Please refer to the illustration above)

POSITIVE: Two colored bands appear on the membrane. One band appears in the control region (C) and another band appears in the test region (T).

NEGATIVE: Only one colored band appears in the control region (C). No apparent colored band appears in the test region (T).

INVALID: Control band fails to appear. Results from any test which has not produced a control band at the specified reading time must be discarded.

Please review the procedure and repeat with a new test. If the problem persists, discontinue using the kit immediately and contact your local distributor.

NOTE:

- Insufficient specimen volume, incorrect operation procedure, or performing expired tests are the most likely reasons for control band failure.

QUALITY CONTROL

Internal procedural controls are included in the test. A colored band appearing in the control region (C) is considered an internal positive procedural control. It confirms sufficient specimen volume and correct procedural technique.

External controls are not supplied with this kit. It is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

LIMITATIONS

- The Troponin I Rapid Test Cassette (Whole Blood/Serum/Plasma) is for professional *in vitro* diagnostic use, and should be used for the qualitative detection of cardiac Troponin I only. There is no meaning attributed to linen color intensity or width.
- The Troponin I Rapid Test Cassette (Whole Blood/Serum/Plasma) will only indicate the presence of Troponin I in the specimen and should not be used as the sole criteria for the diagnostic of acute myocardial infarction (AMI).
- If the test result is negative and clinical symptoms persist, additional testing using other clinical methods is recommended. The test cannot detect less than 0.5 ng/mL of cTnI in specimens. Thus, a negative result does not at anytime rule out the existence of Troponin I in blood, because the antibodies may be absent or below the minimum detection level of the test.
- Like with all diagnostic tests, a confirmed diagnosis should only be made by a physician after all clinical and laboratory findings have been evaluated.
- Some specimens containing unusually high titers of heterophile antibodies or rheumatoid factor (RF) may affect expected results. Even if the test results are positive, further clinical evaluation should be considered with other clinical information available to the physician.

PERFORMANCE CHARACTERISTICS

Table: Troponin I Rapid Test vs. EIA

Method	Troponin I Rapid Test Cassette			Total Results
	Results	Positive	Negative	
EIA	Positive	138	2	140
	Negative	1	315	316
Total Results		139	317	456

Relative Sensitivity: 98.6% (94.9%-99.8%)*

Relative Specificity: 99.7% (98.3%-99.9%)*

Overall Agreement: 99.3% (98.1%-99.9%)*

*95% Confidence Interval

BIBLIOGRAPHY

- Adams, et al. Biochemical markers of myocardial injury, Immunoassay Circulation 88: 750-763, 1993.
- Mehegan JP, Tobacman LS. Cooperative interaction between troponin molecules bound to the cardiac thin filament. J.Biol.Chem. 266:966, 1991.
- Adams, et al. Diagnosis of Perioperative myocardial infarction with measurements of cardiac troponin I. N.Eng.J.Med 330:670, 1994.
- Hossein-Nia M, et al. Cardiac troponin I release in heart transplantation. Ann. Thorac. Surg. 61: 227, 1996.
- Alpert JS, et al. Myocardial Infarction Redefined, Joint European Society of Cardiology American College of Cardiology: J. Am. Coll. Cardio., 36(3):959, 2000.

INDEX OF SYMBOLS

	Consult instructions for use		Tests per kit		Authorized Representative
	For <i>in vitro</i> diagnostic use only		Use by		Do not reuse
	Store between 2-30°C		Lot Number		Catalog#

Zhejiang Orient Gene Biotech Co.,Ltd
Address: 3787#, East Yangguang Avenue, Dipu Street,
Anji 313300, Huzhou, Zhejiang, China.
TEL: +86-572-5226111
FAX: +86-572-5226222
Website: www.orientgene.com

Shanghai International Holding Corp. GmbH (Europe)
Add: Eiffestrasse 80, 20537 Hamburg, Germany

GDTRO-402a