

DECLARATION OF CONFORMITY FOR MATERIALS

Hereby we declare that Aptaca S.p.A. In Vitro Medical Diagnostic Devices (Directive 98/79/CE) and Medical Device (93/42/CE):

1. During devices manufacturing no materials containing natural rubber, latex, synthetic rubber are used (except for Articles of latex). The statement is formulated on the basis of information and statements provided by the producers of the raw materials used.
2. Devices are produced with materials that do not contain substances submitted to restrictions provided by 10/2001/EU Regulation and respect the global and specific migration limits in accordance with the following conditions:
 - Simulant A (distilled water) -40°C for 10 days
 - Simulant B (acetic acid solution 3% p/v) – 40°C for 10 days
 - Simulant C (Ethyl alcohol solution 10% v/v) - 40°C for 10 days
 - Simulant D1 (ethyl alcohol solution at 50% v/v) - 40°C for 10 days
 - Simulant D2 (Vegetable oil - Try substitute made with 95% ethyl alcohol as indicated by the Italian Ministerial Decree 34 of 21.03.1973) - 40°C for 10 days

The global migration limit, together with all other specific restrictions which monomers and/or additives present in the material can be exposed to, are respected in the use conditions here above. Notes and/or simulant used for migration tests allow to fix the food or the group of food, admitted to the contact with food. The statement is formulated on the basis of analytical tests made by our qualified Laboratory and information and statements provided by the producers of the raw materials used

3. Devices are produced with materials that satisfy the follow requirements:
 - Directive (UE) 2015/863 (substances use restriction – phthalates, sulphates) and following updates and changes
 - 1272/2008 Regulation (labeling and use of dangerous substances) and following updates and changes
 - 10/2011 Regulation (specific migration limits) and following updates and changes 1895/2005/CE Rule (substances use restriction for food contact) and following updates and changes
 - 2011/65/UE Directive (heavy metals, RoHS) and following updating and changes
 - 1895/2005/UE Regulation (objects intended to come in contact with food) and following updates and changes

The use in an industrial or commercial venue of the material indicated in this statement does not exclude the determination of its compliance with applicable rules of competence as well as the technological suitability for the purpose which it is intended by the user.

Canelli, 22 January 2020


Bruno Duilio
Quality and Regulatory Affairs Manager

DICHIARAZIONE DI CONFORMITA' DEI MATERIALI

Con la presente si dichiara che i Dispositivi Medico Diagnostici in Vitro (Direttiva 98/79/CE e s.m.i.) e i Dispositivi Medici (93/42/CE e s.m.i.) della società Aptaca S.p.A.:

1. sono stati prodotti utilizzando materiali che non contengono gomma naturale, latex, gomme sintetiche che contengono gomme naturali (ad esclusione degli articoli in lattice). L'affermazione è formulata sulla base delle informazioni e dichiarazioni fornite dai produttori delle materie prime utilizzate.
2. sono realizzati con materiali che non contengono sostanze sottoposte a restrizioni secondo il Regolamento 10/2011 (limiti di migrazione) e s.m.i. e rispettano i limiti di migrazione globale e specifica (ove applicabile) alle seguenti condizioni:
 - simulante **A** (acqua distillata) - 40°C per 10 giorni
 - simulante **B** (soluzione di acido acetico al 3% p/v) - 40°C per 10 giorni
 - simulante **C** (soluzione di alcool etilico al 10% v/v) - 40°C per 10 giorni
 - simulante **D1** (soluzione di alcool etilico al 50% v/v) - 40°C per 10 giorni
 - simulante **D2** (Olio vegetale - Prova sostitutiva effettuata con alcool etilico al 95% secondo quanto indicato dal DM 34 del 21.03.1973) - 40°C per 10 giorni

Il limite di migrazione globale, unitamente alle altre restrizioni specifiche alle quali possono essere sottoposti i monomeri e/o gli additivi presenti nel materiale, sono rispettati nelle condizioni d'uso sopra menzionate. Le note e/o i simulanti impiegati per le prove di migrazione consentono di determinare il prodotto alimentare o il gruppo di prodotti alimentari, ammessi al contatto con alimenti.

L'affermazione è supportata da prove analitiche da noi condotte presso Laboratori qualificati in accordo con il Regolamento citato e sulla base delle informazioni e dichiarazioni fornite dai produttori delle materie prime utilizzate.

3. sono realizzati con materiali che soddisfano i seguenti dettati legislativi:
 - Direttiva Delegata (UE) 2015/863 (restrizione d'uso sostanze - ftalati, solfati,) e s.m.i.
 - Regolamento 1272/2008 (etichettatura e uso sostanze pericolose) e s.m.i.
 - Direttiva 2011/65/UE (metalli pesanti, RoHS) e s.m.i.
 - Regolamento 1895/2005/CE (restrizione d'uso sostanze per contatto con alimenti) e s.m.i.
 - Regolamento 10/2011 (limiti di migrazione) e s.m.i.

L'utilizzazione in sede industriale o commerciale del materiale indicato nella presente dichiarazione non esclude l'accertamento della sua conformità alle norme vigenti di competenza nonché della idoneità tecnologica allo scopo cui è destinato da parte dell'utilizzatore.

Canelli, lì 22.01.2020

Buono Duilio
Quality and Regulatory Manager



CERTIFICATO N° 505SGQ06

CERTIFICATE N° 505SGQ06

Si certifica che il
this is to certify that

Sistema di Gestione per la Qualità

Quality Management System

messo in atto da
implemented by

APTACA S.p.A.

Via Monte Bianco, 4 – IT 20900 MONZA (MB)

nella Sede Operativa di
Operative Unit

Regione Monforte, 30 – IT 14053 CANELLI (AT)

è conforme alla norma
is in compliance with the standard

UNI EN ISO 9001-2015 (ISO 9001-2015)

per i seguenti Processi
concerning the following kinds of Processes

Gestione della fabbricazione e immissione in commercio di tamponi sterili per il prelievo di campioni biologici in orifizi naturali e in ambito chirurgico. Progettazione e fabbricazione di dispositivi medico diagnostici per laboratori di analisi e dispositivi medici di classe I non sterile. Commercializzazione di dispositivi medici invasivi e non di classe IIa, Is, I e diagnostici in vitro. Commercializzazione di articoli da laboratorio.

Management of the manufacturing and placing on the market of sterile tampons for sampling of biological specimens in natural orifice and in surgical field.

Design and manufacturing of diagnostic medical devices for laboratories of analysis and non-sterile class I medical devices.

Marketing of invasive and non-invasive medical devices of class IIa, Is, I and in vitro diagnostics. Marketing of laboratory items.


Il presente Certificato è soggetto al rispetto delle condizioni stabilite dai Regolamenti per la certificazione in vigore applicabili.

This Certificate shall satisfy the requirements established in the Rules for the certification in force applicable.

In caso di discordanza tra le lingue utilizzate nella traduzione del contenuto del presente certificato, fare riferimento alla lingua italiana

In cases of discrepancy between the languages used in the translation of the content of this certificate, please refer to the Italian language

L'AMMINISTRATORE DELEGATO
MANAGING DIRECTOR



Dr. Ing. Roberto Cusolito

Data di Prima Emissione
First Issue Date

1998-07-23

Data di Prima Emissione ITALCERT
First Issue Date ITALCERT

2011-10-30

Data di Rinnovo
Renewal Date

2023-10-24

Data di Scadenza
Expiration Date

2026-10-29

Settore IAF 14 - 29



SGQ N° 023A

Membro degli Accordi di Mutuo Riconoscimento EA, IAF e ILAC
Signatory of EA, IAF and ILAC Mutual Recognition Agreements

CERTIFICATO N° 505DM09

CERTIFICATE N° 505DM09

Si certifica che il
this is to certify that

Sistema di Gestione per la Qualità

Quality Management System

messo in atto da
implemented by

APTACA S.p.A.

Via Monte Bianco, 4 – IT 20900 MONZA (MB)

nella Sede Operativa di
Operative Unit

Regione Monforte, 30 – IT 14053 CANELLI (AT)

è conforme alla norma
is in compliance with the standard

UNI CEI EN ISO 13485-2021 (ISO 13485-2016)

per i seguenti Processi
concerning the following kinds of Processes

Gestione della fabbricazione e immissione in commercio di tamponi sterili per il prelievo di campioni biologici in orifizi naturali e in ambito chirurgico. Progettazione e fabbricazione di dispositivi medico diagnostici per laboratori di analisi e dispositivi medici di classe I non sterile.

Commercializzazione di dispositivi medici invasivi e non di classe IIa, Is, I e diagnostici in vitro.

Management of the manufacturing and placing on the market of sterile tampons for sampling of biological specimens in natural orifice and in surgical field.

Design and manufacturing of diagnostic-medical devices for laboratories of analysis and non-sterile class I medical devices.

Marketing of invasive and non-invasive medical devices of class IIa, Is, I and in-vitro diagnostics.

Il presente Certificato è soggetto al rispetto delle condizioni stabilite dai Regolamenti per la certificazione in vigore applicabili.

This Certificate shall satisfy the requirements established in the Rules for the certification in force applicable.

In caso di discordanza tra le lingue utilizzate nella traduzione del contenuto del presente certificato, fare riferimento alla lingua italiana

In cases of discrepancy between the languages used in the translation of the content of this certificate, please refer to the Italian language

L'AMMINISTRATORE DELEGATO
MANAGING DIRECTOR



Dr. Ing. Roberto Cusolito

Data di Prima Emissione
First Issue Date
2007-10-30

Data di Prima Emissione ITALCERT
First Issue Date ITALCERT
2011-10-30

Data di Rinnovo
Renewal Date
2023-10-24

Data di Scadenza
Expiration Date
2026-10-29



SGQ N° 023A

Membro degli Accordi di Mutuo Riconoscimento EA, IAF e ILAC
Signatory of EA, IAF and ILAC Mutual Recognition Agreements

Instrument Training

Vital Scientific BV hereby declares that the participant has attended a four days seminar for service engineers and the participant is now a certified engineer for the declared instruments.


Participant: Mr. A. Legun

Company: Global Biomarketing Group-Moldova SRL
Moldova

Instrument: Vitalab: XL Series
E Series
Junior Series
Dry ISE
Micro Series
ProXS


Date of training: April 20th – April 23rd, 2010

System Support Manager:

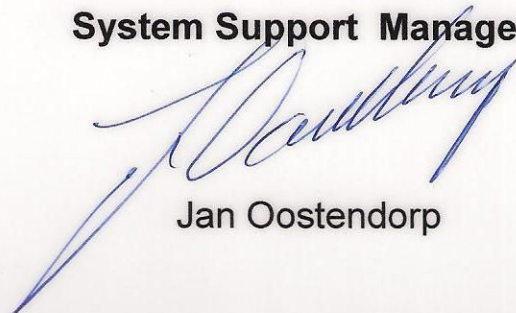

Jan Oostendorp

System Support Engineer:

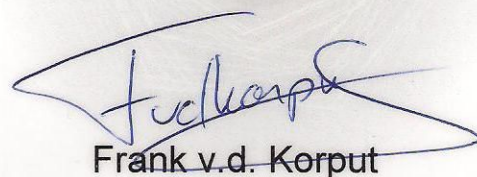

Frank v.d. Kerput



Medica Corporation
5 Oak Park Drive
Bedford, Massachusetts 01730
Tel 781 275 4892
Fax 781 275 2731
www.medicacorp.com

Declaration of Conformity

Product Name:

EasyLyte and accessories per attachment

EasyElectrolytes and accessories per attachment

Model/Type:

EasyLyte Na/K, Na/K/Cl, Na/K/Li, Na/K/Cl/Li,
Na/K/Ca/pH, Na/K/Cl/Ca/Li

EasyElectrolytes Na/K/Cl, Na/K/Li

Manufacturer

 Medica Corporation
5 Oak Park Drive, Bedford, Massachusetts, 01730, USA

Representative

 Emergo Europe, Prinsessegracht 20,
2514 AP The Hague, The Netherlands
Tel: +31 70 345 8570
Fax: +31 70 346 7299

Means of Conformity

Medica Corporation declares that the products listed are covered by Annex III of Directive 98/79/EC. These products are self-certified since they are for professional use only and are not listed on Annex II, List A or Annex II, List B of Directive 98/79/EC. In addition, they are in conformity with the Annex I, "Essential Requirements" and provisions of council Directive 98/79/EC for In Vitro Diagnostic Medical Devices, Directive 2011/65/EU Restriction of Hazardous Substance in Electrical and Electronic Equipment, and the corresponding national laws of the Member States.

Place and Date: Bedford, Massachusetts, USA, September 27, 2018

Signature:



Name: Photios Makris, Ph.D.

Title: VP, Regulatory Affairs

EasyLyte Accessories

Catalog No.	Accessory	EDMA Code
2004	EasyLyte Na/K Analyzer	21 07 11 02
2014	EasyLyte Plus Na/K/Cl Analyzer	21 07 11 02
2015	EasyLyte Lithium Na/K/Li Analyzer	21 07 11 02
2016	EasyLyte Calcium Na/K/Ca/pH Analyzer	21 07 11 02
2021	EasyLyte Na/K/Cl/Li Analyzer	21 07 11 02
2030	EasyLyte EXPAND Analyzer, Na/K/Cl/Ca-Li	21 07 11 02
2070	EasyLyte EasySampler	21 07 11 02
2101	EasyLyte K+ Electrode	11 04 01 06
2102	EasyLyte Na+ Electrode	11 04 01 07
2113	EasyLyte Cl- Electrode	11 04 01 03
2106	EasyLyte Li+ Electrode	11 04 01 04
2150	EasyLyte Ca++ Electrode	11 04 01 02
2151	EasyLyte pH Electrode	11 70 31 02
2152	EasyLyte Disposable Reference Electrode	11 04 04 01
2103	EasyLyte Reference Electrode	11 04 04 01
2258	EasyLyte Membrane Assembly	21 07 11 02
2120	EasyLyte Na/K 800 ml Solutions Pack	11 04 04 02
2121	EasyLyte Na/K/Cl 800mL Solutions Pack	11 04 04 02
2122	EasyLyte Na/K/Li 800mL Solutions Pack	11 04 04 02
2123	EasyLyte Na/K/Ca/pH 800mL Solutions Pack	11 04 04 02
2028	EasyLyte Na/K/Cl/Li 400mL Solution Pack	11 04 04 02
2109	EasyLyte Na/K 400mL Solutions Pack	11 04 04 02
2112	EasyLyte Na/K/Cl 400mL Solutions Pack	11 04 04 02
2115	EasyLyte Na/K/Li 400mL Solutions Pack	11 04 04 02
2114	EasyLyte Na/K/Ca/pH 400mL Solutions Pack	11 04 04 02
2026	EasyLyte Na/K/Cl/Li 800mL Solution Pack	11 04 04 02
2124	EasyLyte Na/K/Cl/Ca-Li 800ml Solutions Pack	11 04 04 02
2814	EasyQC Bi-Level Quality Control Kit	11 50 02 04
2815	EasyQC Tri-Level Quality Control Kit	11 50 02 04
2843	EasyLyte Quality Control Sample Cups (60)	21 07 11 02
2118	Daily Cleaning Solution Kit	11 01 01 27
2598	EasyLyte Daily Cleaner Cup	21 07 11 02
2108	EasyLyte Solutions Valve	21 07 11 02
2107	EasyLyte Sample Probe	21 07 11 02
2257	EasyLyte Sample Detector	21 07 11 02

EasyLyte Accessories, continued

Catalog No.	Accessory	EDMA Code
2104	EasyLyte Tubing Kit	21 07 11 02
2100	EasyLyte Calcium Tubing Kit	21 07 11 02
2492	EasyLyte Internal Filling Solution (125mL)	11 04 04 90
2309	EasyLyte Wash Solution (50mL)	11 04 04 90
2111	EasyLyte Urine Diluent (500mL)	11 04 04 90
2577	EasyLyte Standard Solution, Urine (50mL)	11 04 04 90
2323	EasyLyte Probe Wipers (6)	21 07 11 02
2541	EasyLyte Printer Paper (3 rolls)	21 07 11 02
2595	EasyLyte EasySampler Sample Cups, 500uL (500)	21 07 11 02
2596	EasyLyte Sample Cups 2.0mL (500)	21 07 11 02
10745	Anti-Evaporation Caps (500)	21 07 11 02
2293	EasyLyte Capillary Tubes	21 07 11 02
2590	EasyLyte Capillary Adaptor Kit	21 07 11 02
2292	EasyLyte Capillary Adaptor Cleaning Kit	21 07 11 02
2578	EasyLyte Red Dye Test Solution (50mL)	11 30 01 11
2572	EasyLyte Troubleshooting Kit	21 07 11 02
2571	EasyLyte Troubleshooting Kit (Na/K/Ca/pH and Na/K/Cl/Li)	21 07 11 02
2105	EasyLyte Quarterly Operating Kit	21 07 11 02
2095	EasyLyte Maintenance Kit	21 07 11 02
2076	EasyLyte Sample Tray	21 07 11 02
2074	EasyLyte Sample Cup Retainer Ring	21 07 11 02
7118	Daily Rinse/Cleaning Solution Kit	11 01 01 27
2544	EasyLyte C Series Printer Paper (5 rolls)	21 07 11 02
2934	EasyLyte Barcode Reader Kit	21 07 11 02

EasyElectrolytes Accessories

Catalog No.	Accessory	EDMA Code
4002	EasyElectrolyte Na/K/Cl Analyzer	21 07 11 02
4003	EasyElectrolyte Na/K/Li Analyzer	21 07 11 02
4102	Reagent Module, Na/K/Cl	11 04 04 02
4103	Reagent Module, Na/K/Li	11 04 04 02
7205	EasyElectrolyte/EasyStat Na+ Electrode	11 04 01 07
7206	EasyElectrolyte/EasyStat K+ Electrode	11 04 01 06
4203	EasyElectrolyte Cl- Electrode	11 04 01 03
4204	EasyElectrolyte Li+ Electrode	11 04 01 04
6204	EasyElectrolyte/EasyStat/EasyBloodGas Reference Electrode	11 04 04 01
4207	EasyElectrolyte Spacer Electrode	11 04 01 90
4301	EasyElectrolyte Troubleshooting Kit	21 07 11 02
2118	Daily Cleaning Solution Kit	11 01 01 27
4402	EasyStat/EasyBloodGas/EasyElectrolyte Red Test Dye Solution	11 30 01 11
4403	EasyElectrolyte Urine Diluent	11 04 04 90
2814	Bi-Level Quality Control Kit	11 50 02 04
2815	Tri-Level Quality Control Kit	11 50 02 04
4405	EasyElectrolyte Na/K/Cl Demonstration Kit	21 07 11 02
4406	EasyElectrolyte Na/K/Li Demonstration Kit	21 07 11 02
4404	EasyElectrolyte Capillary Tube Kit	21 07 11 02
4306	EasyElectrolyte Sampler	21 07 11 02
6504	EasyBloodGas/EasyElectrolyte Pump Tube	21 07 11 02
6505	EasyStat/EasyBloodGas/EasyElectrolyte Printer Paper	21 07 11 02
4506	EasyElectrolyte Sensor Module	21 07 11 02
4507	EasyElectrolyte Valve Module	21 07 11 02
4508	EasyStat/EasyBloodGas/EasyElectrolyte Compression Plate	21 07 11 02
7302	Probe Wipers	21 07 11 02
4522	EasyElectrolyte Daily Cleaner Sample Cups	21 07 11 02
4539	EasyElectrolyte Sensor Module, Li+	21 07 11 02
6537	EasyElectrolyte/EasyStat/EasyBloodGas Serial Cable, 9-pin	21 07 11 02
6520	EasyElectrolyte/EasyStat/EasyBloodGas Barcode Reader Kit	21 07 11 02

EasyBloodGas™ analyzer
EasyLyte® analyzer

EasyElectrolytes® analyzer
EasyStat® analyzer

Training Certificate

This is to certify that

Mr. Sergiu Sorocovici

Of GBG-MLD S.R.L.

has completed training for the operation and service of the

EasyBloodGas™ analyzer, EasyElectrolytes® analyzer, EasyLyte® analyzer and EasyStat® analyzer

04/22/2016
DATE



Medica Corporation

David Hagopian
Director of Technical Support



**Self-Declaration of Conformity To European Parliament and Council Directive 98/79/EC
In Vitro Diagnostic Medical Device Directive (IVDD)**

Product name: Nova Stat Profile Prime Plus Analyzer System including Reagents, Calibrators and Controls

Catalog Numbers: List Attached (Two Pages)

Classification: Other/General

Manufacturer: Nova Biomedical Corporation
200 Prospect Street
Waltham, MA 02454 USA

Representative: William Jacques, Director of Regulatory and Quality

Authorized Representative: Nova Biomedical GmbH
Hessenring 13 A, Geb. G
64546 Mörfelden-Walldorf
Germany
Tel: +49 6105 4505-0

Conformity Assessment Route: Annex III

Nova Biomedical, Inc. declares that the products listed are in conformity with the provisions of the Council Directive 98/79/EC for in vitro diagnostic medical devices, including applicable essential requirements of Annex I for legal application of the CE Mark. All supporting documentation is retained under the premises of the manufacturer.

Nova Biomedical, Inc. declares that the electronic products listed are in conformity with the provisions of the Council Directive 2011/65/EC on the restriction of the use of certain hazardous substances in electrical and electronic equipment (RoHS).

Standards Applied:

EN ISO 13485:2016	Medical devices - Quality management systems - Requirements for regulatory purposes
EN 50581:2012	Technical Documentation for the Assessment of Electrical and Electronic Products with Respect to the Restriction of Hazardous Substances
EN 61010-1:2010	Safety requirements for electrical equipment for measurement, control, and laboratory use - Part 1: General requirements
EN 61010-2:101:2015	Safety requirements for electrical equipment for measurement, control, and laboratory use - Part 2-101: Particular requirements for in vitro diagnostic (IVD) medical equipment

Signature:

William Jacques, Director of Regulatory and Quality



Date:

Jul/24/2020

List of Catalog Items Covered:

Catalog Number	Product Name	Global Medical Device Nomenclature (GMDN) Name	GMDN Number	DIMDI EDMS Code
57400	Stat Profile Prime Plus® Analyzer	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02
59508	Stat Profile Prime Plus® Analyzer (Remanufactured)	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02
57820	Stat Profile Prime Plus MicroSensor Card™ with COOX	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02
57821	Stat Profile Prime Plus MicroSensor Card™ BUN, Creatinine	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02
57822	Stat Profile Prime Plus MicroSensor Card™ with COOX (High Volume)	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02
57823	Stat Profile Prime Plus Reference Cartridge	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02
57825	Stat Profile Prime Plus Calibrator Cartridge 100 Sample	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57826	Stat Profile Prime Plus Calibrator Cartridge 200 Sample	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57827	Stat Profile Prime Plus Calibrator Cartridge 300 Sample	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57828	Stat Profile Prime Plus Calibrator Cartridge 400 Sample	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57829	Stat Profile Prime Plus Calibrator Cartridge 500 Sample	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57831	Stat Profile Prime Plus Calibrator Cartridge 100 Sample with Creat / BUN	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57832	Stat Profile Prime Plus Calibrator Cartridge 200 Sample with Creat / BUN	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57833	Stat Profile Prime Plus Calibrator Cartridge 300 Sample with Creat / BUN	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57834	Stat Profile Prime Plus Calibrator Cartridge 400 Sample with Creat / BUN	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57835	Stat Profile Prime Plus Calibrator Cartridge 500 Sample with Creat / BUN	Multiple blood gas/haemoximetry/electrolyte analyte IVD, calibrator	52859	11-04-04-03-00
57838	Stat Profile Prime Plus Auto QC Cartridge 160 Sample	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
57839	Stat Profile Prime Plus Auto QC Cartridge 320 Sample	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
57840	Stat Profile Prime Plus Auto QC Cartridge 480 Sample	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
57841	Stat Profile Prime Plus Auto QC Cartridge 105 Sample with Creat / BUN	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
57842	Stat Profile Prime Plus Auto QC Cartridge 210 Sample with Creat / BUN	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
57843	Stat Profile Prime Plus Auto QC Cartridge 315 Sample with Creat / BUN	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
57844	Stat Profile Prime Plus Ampuled Controls BG, COOX Levels 1, 2, 3	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
57845	Stat Profile Prime Plus Ampuled Controls Chemistry Levels 4,5	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
58379	Stat Profile Prime Plus BUN, Creatinine - Blank Sensor Card	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02
58642	Stat Profile Prime Plus MicroSensor Card™	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02
58643	Stat Profile Prime Plus MicroSensor Card™ (High Volume)	Point-of-care single channel clinical chemistry analyzer IVD	56681	21-02

Catalog Number	Product Name	Global Medical Device Nomenclature (GMDN) Name	GMDN Number	DIMDI EDMS Code
55229	Nova Linearity Level 1,2,3,4	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-01-00
56198	Linearity Standard Set G Multipack	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-90-00
61656	Nova Linearity Creatinine/BUN/Hct Levels 1,2,3,4	Multiple blood gas/haemoximetry/electrolyte analyte IVD, control	52860	11-50-90-90-00



Certificate

No. Q5 020747 0242 Rev. 02

Holder of Certificate: **Nova Biomedical Corporation**
200 Prospect Street
Waltham MA 02454
USA

Certification Mark:



Scope of Certificate: Design and Development, Production, Distribution, Installation, Servicing and Technical Support of In-Vitro Diagnostic Reagents (Calibrators, Controls, Reagents, Sensors and Test Cartridges) and Instruments for Clinical Chemistry, Blood Gas and Hematology, including Near Patient / Point of Care and Self-Testing devices; The provision of manufacturing services of In-Vitro Diagnostic Reagents (Calibrators, Controls) for Clinical Chemistry, Blood Gas and Hematology, In-Vitro Diagnostic General Use Consumables; and Distribution of Lancets.

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). All applicable requirements of the Testing, Certification, Validation and Verification Regulations TÜV SÜD Group have to be complied with. For details and certificate validity see: [www.tuvsud.com/ps-cert?q=cert:Q5 020747 0242 Rev. 02](http://www.tuvsud.com/ps-cert?q=cert:Q5_020747_0242_Rev_02)

Report No.: 72198686

Valid from: 2024-10-25
Valid until: 2027-10-24

Date, 2024-10-04

Christoph Dicks
Head of Certification/Notified Body

Certificate

No. Q5 020747 0242 Rev. 02

Applied Standard(s): ISO 13485:2016
(EN ISO 13485:2016/AC:2018, EN ISO 13485:2016/A11:2021)
Medical devices - Quality management systems -
Requirements for regulatory purposes

Facility(ies): **Nova Biomedical Corporation**
200 Prospect Street, Waltham MA 02454, USA

Design and Development, Production, Distribution, Installation,
Servicing and Technical Support of In-Vitro Diagnostic Reagents
(Calibrators, Controls, Reagents, Sensors and Test Cartridges)
and Instruments for Clinical Chemistry, Blood Gas and
Hematology, including Near Patient / Point of Care and Self-
Testing devices; the provision of manufacturing services of In-Vitro
Diagnostic Reagents (Calibrators, Controls) for Clinical Chemistry,
Blood Gas and Hematology and In-Vitro Diagnostic General Use
Consumables.

Nova Biomedical Corporation
39 Manning Road, Billerica MA 01821, USA

Production of Self-Testing and Near Patient / Point of Care test
strips.

Nova Biomedical Corporation
165 Lexington Road, Billerica MA 01821, USA

Production of Self-Testing and Near Patient / Point of Care
Instruments

Nova Biomedical Corporation
4 Enterprise Road, Billerica MA 01821, USA

Production of In-Vitro Diagnostic Instruments including Near
Patient / Point of Care; Distribution of Finished Goods; Distribution
of Lancets.

NOVA
biomedical

CERTIFICATE OF COMPLETION

This is to certify that

Sergiu Sorocovici

*has successfully completed Stat Profile Prime Plus Service and Application
Training.*

April 10-11, 2023

Date of Training

Chişinău / Moldova

Location of Training



Huseyin Dibekkaya

**Support Training Program Facilitator
International Regional Support Manager**

PRIME PLUS / VET SHELF-LIFE & WARRANTY INFORMATION

REV: 07/2021

Stat Profile® Prime Plus and Stat Profile Prime Plus VET



DESCRIPTION		WARRANTY	SHELF LIFE
Sensors Cards			
57820	Prime-Plus Sensor Card: w/ COOx (Standard)	14 Days/200 Samples*	12 Mos
57822	Prime-Plus Sensor Card: w/ COOx (High Volume)	14 Days/400 Samples*	12 Mos
58642	Prime-Plus Sensor Card: NO COOx (Standard)	14 Days/200 Samples*	12 Mos
58643	Prime-Plus Sensor Card: NO COOx (High Volume)	14 Days/400 Samples*	12 Mos
57821	Prime-Plus: Renal Micro Sensor Card	7 Days/200 Samples*	12 Mos
58577	Prime-Plus VET- Sensor Card: w/ COOx (High Volume)	14 Days/400 Samples*	12 Mos
58578	Prime-Plus VET- Sensor Card: NO COOx (High Volume)	14 Days/400 Samples*	12 Mos
58581	Prime-Plus VET- Renal Micro Sensor Card	7 Days/200 Samples*	12 Mos
58379	Prime-Plus Sensor Card- BLANK RENAL Sensor Card: (Clinical & VET)	Free of Defects	n/a
57823	Reference Sensor- Prime-Plus (w/ W/R Pump Tubing) (CLINICAL)	Free of Defects	18 Mos
59345	Reference Sensor- Prime-Plus (w/ W/R Pump Tubing) (VET)	Free of Defects	18 Mos
Calibrators			
57825	Stat Profile Prime Plus® Calibrator Cartridge 100 Sample	100 Samples or 35 Days	18 Mos
57826	Stat Profile Prime Plus® Calibrator Cartridge 200 Sample	200 Samples or 35 Days	18 Mos
57827	Stat Profile Prime Plus® Calibrator Cartridge 300 Sample	300 Samples or 35 Days	18 Mos
57828	Stat Profile Prime Plus® Calibrator Cartridge 400 Sample	400 Samples or 35 Days	18 Mos
57829	Stat Profile Prime Plus® Calibrator Cartridge 500 Sample	500 Samples or 35 Days	18 Mos
57831	Stat Profile Prime Plus® Calibrator Cartridge 100 Sample with Creat / BUN	100 Samples or 21 Days	18 Mos
57832	Stat Profile Prime Plus® Calibrator Cartridge 200 Sample with Creat / BUN	200 Samples or 21 Days	18 Mos
57833	Stat Profile Prime Plus® Calibrator Cartridge 300 Sample with Creat / BUN	300 Samples or 21 Days	18 Mos
57834	Stat Profile Prime Plus® Calibrator Cartridge 400 Sample with Creat / BUN	400 Samples or 21 Days	18 Mos
57835	Stat Profile Prime Plus® Calibrator Cartridge 500 Sample with Creat / BUN	500 Samples or 21 Days	18 Mos
58395	Stat Profile Prime Plus® VET Calibrator Cartridge 200 Sample	200 Samples or 35 Days	18 Mos
58396	Stat Profile Prime Plus® VET Calibrator Cartridge 500 Sample	500 Samples or 35 Days	18 Mos
58405	Stat Profile Prime Plus® VET Calibrator Cartridge 200 Sample with Creat / BUN	200 Samples or 21 Days	18 Mos
58404	Stat Profile Prime Plus® VET Calibrator Cartridge 500 Sample with Creat / BUN	500 Samples or 21 Days	18 Mos
AQC Packs			
57838	Stat Profile Prime Plus® Auto QC Cartridge 160 Sample	160 Samples or 32 Days	18 Mos
57839	Stat Profile Prime Plus® Auto QC Cartridge 320 Sample	320 Samples or 32 Days	18 Mos
57840	Stat Profile Prime Plus® Auto QC Cartridge 480 Sample	480 Samples or 32 Days	18 Mos
57841	Stat Profile Prime Plus® Auto QC Cartridge 105 Sample with Creat / BUN	105 Samples or 21 Days	18 Mos
57842	Stat Profile Prime Plus® Auto QC Cartridge 210 Sample with Creat / BUN	210 Samples or 21 Days	18 Mos
57843	Stat Profile Prime Plus® Auto QC Cartridge 315 Sample with Creat / BUN	315 Samples or 21 Days	18 Mos
58406	Stat Profile Prime Plus® VET Auto QC Cartridge 160 Sample	160 Samples or 32 Days	18 Mos
58407	Stat Profile Prime Plus® VET Auto QC Cartridge 480 Sample	480 Samples or 32 Days	18 Mos
58408	Stat Profile Prime Plus® VET Auto QC Cartridge 105 Sample with Creat / BUN	105 Samples or 21 Days	18 Mos
58409	Stat Profile Prime Plus® VET Auto QC Cartridge 315 Sample with Creat / BUN	315 Samples or 21 Days	18 Mos
57844	Stat Profile Prime Plus® Ampuled Controls BG, COOX Levels 1, 2, 3	Free of Defects	12 Mos
57845	Stat Profile Prime Plus® Ampuled Controls Chemistry Levels 4,5	Free of Defects	12 Mos

57812	Stat Profile Prime Plus® VET Ampuled Controls BG, COOX Levels 1, 2, 3	Free of Defects	12 Mos
57813	Stat Profile Prime Plus® VET Ampuled Controls Chemistry Levels 4,5	Free of Defects	12 Mos

Miscellaneous:

52669	Luer Station Safety Port (5/pack) (Prime/Prime-Plus)	Free of Defects
52582	Probe/S-Line Assy : Prime/Prime-Plus	Free of Defects
49200	Printer Paper (rolls: 5/pkg) (small-style)	Free of Defects

Electro-Mechanical Components & Assemblies

***Whichever comes first.**

NOTE: THE WARRANTED USE EXPRESSED ABOVE IS ONLY VALID IF IT OCCURS

PRIOR TO THE "USE BEFORE DATE" LISTED ON THE PACKAGE LABEL.

CERTIFICATE

ELECTROMAGNETIC COMPATIBILITY

Applicant	: Vital Scientific B.V.
Contact person	: Mrs. C. v.d. Broek
Address	: Van Rensselaerweg 4
Postal code, Place	: 6956 AV Spankeren/Dieren
Country	: The Netherlands
Manufacturer	: Vital Scientific B.V.
Address	: Van Rensselaerweg 4
Postal code, Place	: 6956 AV Spankeren/Dieren
Country	: The Netherlands
Electrical apparatus	: Clinical Analyser
Trademark	: Elitech Clinical Systems
Type designations	: Flexor EL200, Selectra ProM

Environment : **Laboratory**

EN 61326-1:2006 : Equipment for measurement, control and laboratory use
EN 61326-2-6:2006 : Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 2-6: particular requirements – In vitro diagnostic (IVD) medical equipment, from which:

EN 55011:2007	: Emission - Class A
+A2:2007	
EN 61000-3-2:2006	: Limit for harmonic currents emissions
EN 61000-3-3:1995	: Limitation of voltage fluctuations and flicker
+A1:2001+A2:2005	
EN 61000-4-2:1995	: Electrostatic discharge (ESD) immunity
A1:1998+A2:2001	
EN 61000-4-3:2006	: Radiated Electro-Magnetic field immunity
+A1:2008	
EN 61000-4-4:2004	: Electrical fast transient (EFT) immunity
EN 61000-4-5:2006	: Surge transient immunity
EN 61000-4-6:2007	: Conducted Radio-Frequency disturbances immunity
EN 61000-4-8:1993	: Power frequency magnetic field immunity
+A1:2001	
EN 61000-4-11:2004	: Voltage dips and interruptions immunity

The undersigned declares that the described product meets the requirements of the mentioned standards, based on a non-recurrent examination. The test results lay down in our test reports with reference 2129388.0501-QUA/EMC and 2136226.0501-QUA/EMC.

KEMA Quality B.V.
 (Notified Body EMC)
 Arnhem, September 20, 2010

A.T. van der Meijden
 Certification Manager EMC

Certificate nr. **2136226.0551-QUA/EMC**

Integral publication of this certificate and adjoining reports is allowed.

KEMA Quality B.V. Utrechtseweg 310, 6812 AR Arnhem P.O. Box 5185, 6802 ED Arnhem The Netherlands
 T +31 26 3 56 20 00 F +31 26 3 52 58 00 www.kemaquality.com Registered Arnhem 09085396