

Documents of FFP2 Earloop

1. Detail of Package-----	04
2. 2020 (F) - 0376 EN 149-FFP2 without valve CCQS	
XingGuang- FFP2 Test Report-----	05-14
3. CE-PC-200331-168-01-9A Xingguang issued Module B-----	15-16
4. CE-PC-200331-168-FPC-A Xingguang issued Module C2---	17-18
5. EU Declaration of Conformity-----	19
★ 6. White list on China Ministry of Commerce Website-----	20



FFP2 PARTICLE FILTERING HALF MASK

CE 2834

Model : XGM-95
EN149:2001+A1:2009



Product Photos

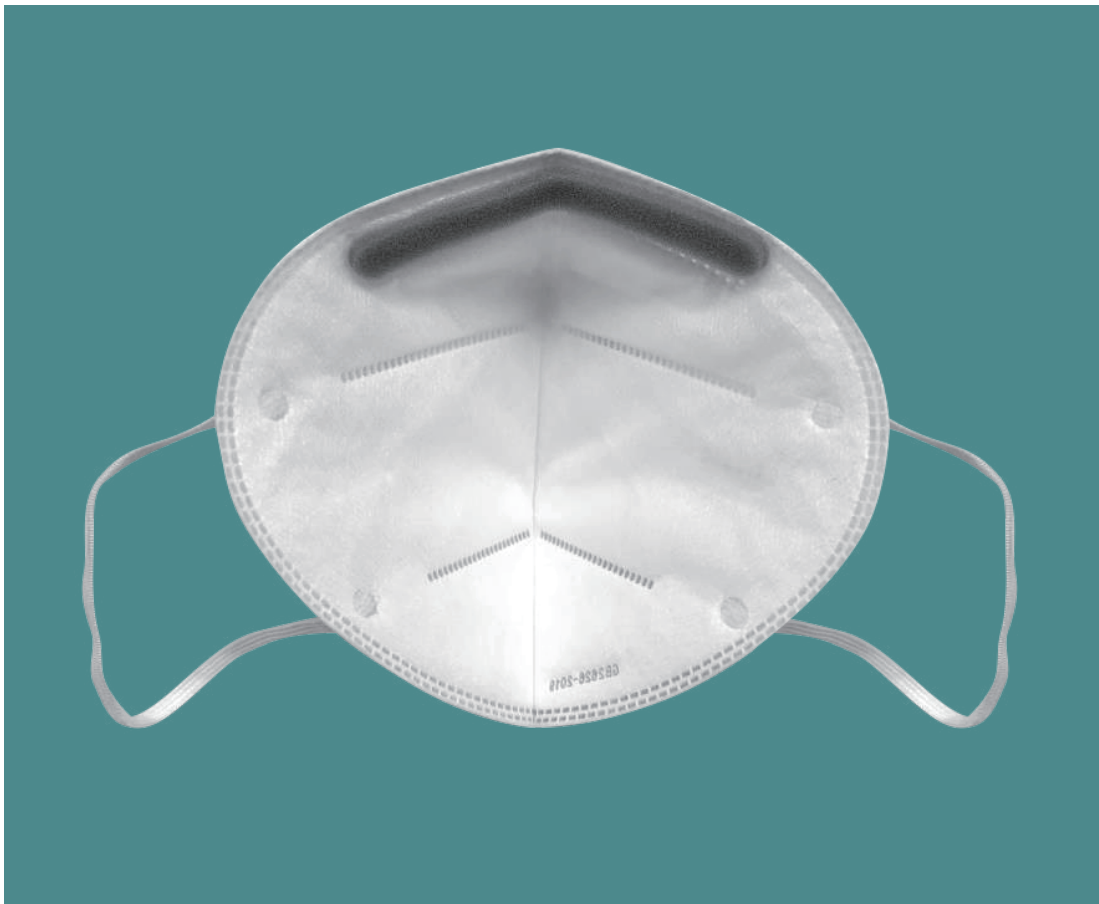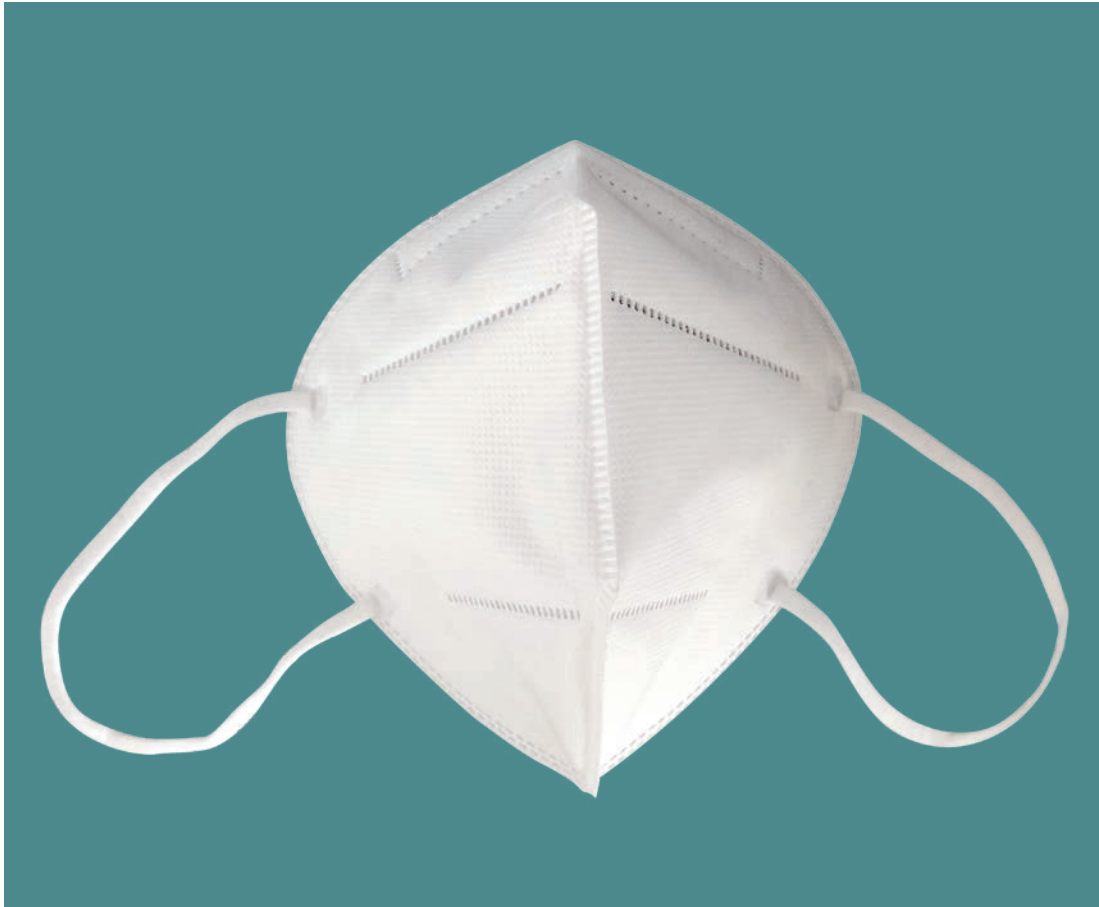

PACKING MANNER



2pcs/bag*25



Package Details	Box Details		Cation Details		
2pcs/bag, 25bag in a box,30box per carton	145*125*220mm	G.M 0.42KGS	650*455*355mm	1500pcs	G.W 20.08KGS





中国认可
国际互认
检测
TESTING
CNAS L1499

National Quality Supervision and Testing Center for Personal
Protective Equipment (Beijing)
(Testing Laboratory for Labour Protection Products of Beijing
Municipal Institute for Labour Protection)

No.55 Taoranting Street, Xicheng District, Beijing, China.
Phone: +86 10 63519250 +86 10 63520770 +86 10 83530311
Fax: +86 10 63519250 +86 10 63520770

The Testing Center is accredited for compliance with ISO/IEC 17025.

The results of tests, calibrations and/or measurements included in this document are traceable to Chinese/national standards.

CNAS is a signatory to the ILAC mutual recognition arrangement for the mutual recognition of the equivalence of testing, calibration and inspection reports.

TEST REPORT

Particulate respirator-half facepiece

EN 149: 2001 +A1: 2009 Respiratory protective devices — Filtering half masks to protect against particles —
Requirements, testing, marking

Product: Particle filtering half mask
Report No: 2020 (F) - 0376
Client: CCQS Certification Services Limited
Model (s): XGM-95
Date(s) of tests: 2020.07.23-2020.08.23

DESCRIPTION OF SAMPLES

General Information	Classification	Main Components
Manufacturer	FFP2 NR	White folding mask
Manufacturer Address	Shandong Xingguang Perotective Products Co., Ltd. Business room 315, Zhilan Village 3, Gaomi Economic Development Zone, Gaomi City, Shandong Province, P. R. China	

Signed:

Issued: 2020.8.24

陈倬为 Chen Zhuowei

Authorized Signatory, Lab Director

Page 1 of 10



This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

国家劳动保护用品质量监督检验中心(北京)

Conditions:

The test results presented in this report relate to the samples tested only.

This report may be reproduced and distributed to your clients, provided that it is reproduced and distributed in full.

The authenticity of this test report and its contents can be verified by contacting the laboratory.

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

Test Results

<p>7.3 Visual inspection</p> <p>The visual inspection shall include the marking and information supplied by the manufacturer. Note1: As requested by the client, marking and information supplied by the manufacturer was not inspected.</p>	Not tested¹						
<p>7.4 Package</p> <p>Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use. Note2: In accordance with the requirement.</p>	Pass²						
<p>7.5 Material</p> <p>Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used.</p> <p>Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer.</p> <p>After undergoing the conditioning described in 8.3.1 none of the particle filtering half masks shall have suffered mechanical failure of the facepiece or straps.</p> <p>When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse. Note3: No mechanical failure after undergoing the conditioning described in 8.3.1. No collapse when conditioned in accordance with 8.3.1 and 8.3.2.</p>	Pass³						
<p>7.6 Cleaning and disinfecting</p> <p>If the particle filtering half mask is designed to be re-usable, the materials used shall withstand the cleaning and disinfecting agents and procedures to be specified by the manufacturer. Note4: Single shift use only.</p>	N/A⁴						
<p>7.7 Practical performance</p> <p>The particle filtering half mask shall undergo practical performance tests under realistic conditions. Note5: No imperfections.</p>	Pass⁵						
<p>7.8 Finish of parts</p> <p>Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs. Note6: No sharp edges or burrs.</p>	Pass⁶						
<p>7.9.1 Total inward leakage</p> <p>For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than: 25% for FFP1, 11% for FFP2, 5% for FFP3</p> <p>and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than 22% for FFP1, 8% for FFP2, 2% for FFP3 Note7: FFP2 respirator. Test results are shown in Annex A Table 7.9.1-A&B.</p>	Pass⁷						
<p>7.9.2 Penetration of filter material</p> <p>The penetration of the filter of the particle filtering half mask shall meet the requirements of Table 1.</p> <table border="0" style="width: 100%; margin-left: 40px;"> <tr> <td style="width: 30%;"></td> <td style="width: 35%; text-align: center;">Sodium chloride test 95 l/min</td> <td style="width: 35%; text-align: center;">Paraffin oil test 95 l/min</td> </tr> <tr> <td>FFP1</td> <td style="text-align: center;">≤20%</td> <td style="text-align: center;">≤20%</td> </tr> </table>		Sodium chloride test 95 l/min	Paraffin oil test 95 l/min	FFP1	≤20%	≤20%	Pass⁸
	Sodium chloride test 95 l/min	Paraffin oil test 95 l/min					
FFP1	≤20%	≤20%					

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

FFP2	≤6%	≤6%
FFP3	≤1%	≤1%

Note8: FFP2 respirator. Test results are shown in Annex A Table 7.9.2.

7.10 Compatibility with skin

Pass⁹

Materials that may come into contact with the wearer’s skin shall not be known to be likely to cause irritation or any other adverse effect to health.

Note9: No irritation or any other adverse effect to health.

7.11 Flammability

Pass¹⁰

When tested, the particle filtering half mask shall not burn or not to continue to burn for more than 5 s after removal from the flame.

Note10: Test results are shown in Annex A Table 7.11.

7.12 Carbon dioxide content of the inhalation air

Pass¹¹

The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume)

Note11: Test results are shown in Annex A Table 7.12.

7.13 Head harness

Pass¹²

The head harness shall be designed so that the particle filtering half mask can be donned and removed easily. The head harness shall be adjustable or self-adjusting and shall be sufficiently robust to hold the particle filtering half mask firmly in position and be capable of maintaining total inward leakage requirements for the device.

Note12: Head harness can be donned and removed easily, adjustable or self-adjusting and have sufficiently robust to hold the particle filtering half mask firmly.

7.14 Field of vision

Pass¹³

The field of vision is acceptable if determined so in practical performance tests.

Note13: Pass the practical performance tests.

7.15 Exhalation valve

N/A¹⁴

A particle filtering half mask may have one or more exhalation valve(s), which shall function correctly in all orientations.

If an exhalation valve is provided it shall be protected against or be resistant to dirt and mechanical damage and may be shrouded or may include any other device that may be necessary for the particle filtering half mask to comply with 7.9.

Exhalation valve(s), if fitted, shall continue to operate correctly after a continuous exhalation flow of 300 l/min over a period of 30 s.

When the exhalation valve housing is attached to the faceblank, it shall withstand axially a tensile force of 10 N applied for 10 s.

Note14: No exhalation valve.

7.16 Breathing resistance

Pass¹⁵

Classification	Maximum permitted resistance (mbar)		
	Inhalation		Exhalation
	30 l/min	95 l/min	160 l/min
FFP1	0.6	2.1	3.0
FFP2	0.7	2.4	3.0
FFP3	1.0	3.0	3.0

Note15: FFP2 respirator. Test results are shown in Annex A Table 7.16.

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

7.17 CloggingN/A¹⁶**7.17.2 Breathing resistance**

Valved particle filtering half masks:

After clogging the inhalation resistances shall not exceed:

FFP1: 4 mbar, FFP2: 5 mbar, FFP3: 7 mbar at 95L/min continuous flow

The exhalation resistance shall not exceed 3 mbar at 160 L/min continuous flow

Valveless particle filtering half masks

After clogging the inhalation and exhalation resistances shall not exceed:

FFP1: 3 mbar, FFP2: 4 mbar, FFP3: 5 mbar at 95L/min continuous flow

7.17.3 Penetration of filter material

	Sodium chloride test 95 l/min	Paraffin oil test 95 l/min
FFP1	≤20%	≤20%
FFP2	≤6%	≤6%
FFP3	≤1%	≤1%

Note16: Single shift use only.

7.18 Demountable partsPass¹⁷

All demountable parts (if fitted) shall be readily connected and secured, where possible by hand

Note17: In accordance with the requirement.

9 Marking

Not tested

9.1 Packaging

The following information shall be clearly and durably marked on the smallest commercially available packaging or legible through it if the packaging is transparent.

9.1.1 The name, trademark or other means of identification of the manufacturer or supplier.

9.1.2 Type-identifying marking.

9.1.3 Classification

The appropriate class (FFP1, FFP2 or FFP3) followed by a single space and then: "NR" if the particle filtering half mask is limited to single shift use only. Example: FFP3 NR, or "R" if the particle filtering half mask is re-usable.

Example: FFP2 R D.

9.1.4 The number and year of publication of this European Standard.

9.1.5 At least the year of end of shelf life. The end of shelf life may be informed by a pictogram as shown in Figure 12a, where yyyy/mm indicates the year and month.

9.1.6 The sentence 'see information supplied by the manufacturer', at least in the official language(s) of the country of destination, or by using the pictogram as shown in Figure 12b.

9.1.7 The manufacturer's recommended conditions of storage (at least the temperature and humidity) or equivalent pictogram, as shown in Figures 12c and 12d.

9.1.8 The packaging of those particle filtering half masks passing the dolomite clogging test shall be additionally marked with the letter "D". This letter shall follow the classification marking preceded by a single space.

9.2 Particle filtering half mask

Particle filtering half masks complying with this European Standard shall be clearly and durably marked with the following:

9.2.1 The name, trademark or other means of identification of the manufacturer or supplier.

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

9.2.2 Type-identifying marking.

9.2.3 The number and year of publication of this European Standard.

9.2.4 Classification

The appropriate class (FFP1, FFP2 or FFP3) followed by a single space and then: "NR" if the particle filtering half mask is limited to single shift use only. Example: FFP3 NR, or "R" if the particle filtering half mask is re-usable. Example: FFP2 R D.

9.2.5 If appropriate the letter D (dolomite) in accordance with clogging performance. This letter shall follow the classification marking preceded by a single space

9.2.6 Sub-assemblies and components with considerable bearing on safety shall be marked so that they can be identified.

End of Test Results

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

Annex A: Summarization of Test Data**Table 7.9.1-A Inward leakage test data**

Test specification: EN 149-2001 Clause 8.5

Subject	Sample No.	Condition	Walk(%)	Head Side/side(%)	Head up/down(%)	Talk(%)	Walk(%)	Mean(%)
Yi	1	A.R.	8.42	8.79	8.96	8.76	8.57	8.7
Gong	2	A.R.	5.35	5.84	5.97	5.45	5.77	5.7
Yu	3	A.R.	5.64	6.10	6.36	6.08	5.77	6.0
Hu	4	A.R.	5.24	5.37	5.64	5.47	5.24	5.4
Xu	5	A.R.	6.36	6.82	7.23	6.65	6.43	6.7
Deng	6	T.C.	6.74	6.85	7.17	7.05	6.82	6.9
Zhang	7	T.C.	7.43	7.58	7.84	7.57	7.36	7.6
Zhi	8	T.C.	6.21	6.52	6.63	6.26	6.13	6.3
Fang	9	T.C.	6.83	7.07	7.36	7.11	6.96	7.1
Lv	10	T.C.	6.32	6.74	6.89	6.55	6.42	6.6
All 50 individual exercise results were not greater than <u>11</u> % 9 out of 10 individual wearer arithmetic means were not greater than <u>8</u> %							Pass	

Table 7.9.1-B Facial dimension

Subject	Face length	Face Width	Face Depth	Mouth Width
Yi	120	130	109	59
Gong	122	140	115	65
Yu	119	160	139	55
Hu	112	122	119	63
Xu	110	130	118	60
Deng	115	119	110	59
Zhang	112	123	113	55
Liu	103	130	100	50
Zhi	118	139	130	63
Fang	115	129	120	50
Chen	116	150	132	56
Lv	110	121	110	53

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

Table -7.9.2 Penetration of filter material

Test specification: EN 149-2001 Clause 8.11

Aerosol	Condition	Sample No.	Penetration (%)	Assessment
Sodium chloride test	As received	11	0.591	Pass
		12	0.654	
		13	0.517	
	Simulated wearing treatment	14	0.763	
		15	0.828	
		16	0.786	
	Mechanical strength+ Temperature conditioned	17	1.13	
		18	1.07	
		19	1.01	
Paraffin oil test	As received	20	3.17	Pass
		21	3.04	
		22	2.99	
	Simulated wearing treatment	23	3.25	
		24	3.41	
		25	3.36	
	Mechanical strength+ Temperature conditioned	26	3.72	
		27	3.69	
		28	3.81	
Flow conditioning: Single filter: 95.0 L/min				

Table 7.11 Flammability

Test specification: EN 149-2001 Clause 8.6

Condition	Sample No.	Result	Assessment
As received	29	Burn for 1 s	Pass
	30	Burn for 1 s	
Temperature conditioned	31	Burn for 2 s	
	32	Burn for 2 s	

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

Table 7.12 Carbon dioxide content of the inhalation air

Test specification: EN 149-2001 Clause 8.7

Condition	Sample No.	Result	Assessment
As received	33	0.42%	Mean value 0.4%
	34	0.40%	
	35	0.38%	
			Pass

Table 7.16 Breathing resistance (mbar)

Test specification: EN 149-2001 Clause 8.9

As received	Flow rate		36					37					38				
			A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
Inhalation	30 l/min		0.4	0.5	0.4	0.5	0.5	0.5	0.4	0.5	0.5	0.5	0.5	0.5	0.5	0.5	0.5
	95 l/min		1.2	1.3	1.3	1.3	1.3	1.3	1.3	1.3	1.3	1.3	1.3	1.2	1.2	1.3	1.3
Exhalation	160 l/min		1.9	2.0	1.9	2.0	2.0	2.0	2.0	1.9	2.0	2.0	2.0	2.0	2.0	2.0	2.0
Simulated wearing treatment	Flow rate		39					40					41				
			A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
Inhalation	30 l/min		0.5	0.5	0.5	0.5	0.5	0.4	0.4	0.5	0.5	0.5	0.4	0.4	0.5	0.4	0.5
	95 l/min		1.3	1.3	1.2	1.3	1.3	1.3	1.3	1.3	1.3	1.2	1.3	1.2	1.3	1.2	1.3
Exhalation	160 l/min		2.0	2.0	2.0	2.0	2.0	2.0	2.0	2.0	1.9	1.9	1.9	2.0	1.9	2.0	2.0
Temperature conditioned	Flow rate		42					43					44				
			A	B	C	D	E	A	B	C	D	E	A	B	C	D	E
Inhalation	30 l/min		0.5	0.5	0.5	0.4	0.5	0.5	0.5	0.4	0.5	0.5	0.4	0.5	0.4	0.4	0.5
	95 l/min		1.2	1.3	1.3	1.2	1.2	1.3	1.2	1.3	1.3	1.3	1.3	1.2	1.3	1.3	1.3
Exhalation	160 l/min		1.9	1.9	2.0	2.0	2.0	2.0	2.0	2.0	1.9	2.0	2.0	2.0	2.0	1.9	2.0
Assessment			Pass														


A: facing directly ahead; B: facing vertically upwards; C: facing vertically downwards; D: lying on the left side; E: lying on the right side

Test	Uncertainty
Total inward leakage	4.1%
Penetration of filter material	1.1%
Flammability	5.0%
Carbon dioxide content of the inhalation air	2.6%
Breathing resistance	1.8%

End of Annex A

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.

ANNEX B PHOTOS OF SAMPLES

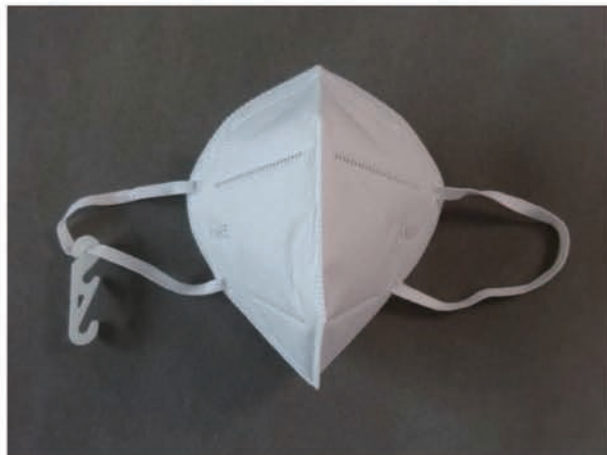

End of Annex B

This report may not be published except in full unless permission for the publication of an approved extract has been obtained in writing.



Module B EU Type-Examination Certificate

For the requirements of PPE Regulation 2016/425

Certificate No.: CE-PC-200331-168-01-9A

Certificate holder:	Shandong Xingguang Protective Products Co., Ltd. Business Room 315, Zhilan Village 3, Gaomi Economic Development Zone, Gaomi City, Shandong Province, P.R.China
Product:	Particle filtering half mask Detailed product description listed in the Annex
Model(s):	XGM-95
Standard(s):	EN 149:2001+A1:2009 Respiratory protective devices - Filtering half masks to protect against particles - Requirements, testing, marking
Issue date:	2020-10-23
Revision date:	2020-10-23
Expiry date:	2021-10-22



The product(s) on this certificate and the Technical File have been assessed and found to be in conformance with the applicable Essential Health and Safety Requirements in Annex II of the PPE regulation 2016/425.

Any changes to the design, manufacturing location or manufacture of the PPE product certified here must be advised to CCQS Certification Services Limited for review.

CE marking shall not be applied until the requirements of all the PPE Regulation 2016/425 and relevant EN Harmonised standards and/or Technical specifications have been met.

If the certified product is Category III then this certificate is only valid if used in conjunction with Conformity Assessment against Module C2 or Module D.

This certificate remains the property of CCQS and maybe withdrawn at any time if it is considered that the equipment is no longer in conformity with the requirements of the PPE Regulation 2016/425.



Approved by Ireland Government as a Notified Body for CE Marking No.2834



CCQS Certification Services Limited

Block 1 Blanchardstown Corporate Park, Ballycoolin Road, Blanchardstown, Dublin15, D15 AKK1, Ireland

Tel: +00 353 1 588 6920 Website: www.ccqs.co.uk E-mail: verify@ccqs.ie

If in any doubt about the integrity of this certificate, please contact CCQS by email to verify.



Module B EU Type-Examination Certificate

Annex

For the requirements of PPE Regulation 2016/425



Certificate No.: CE-PC-200331-168-01-9A

Applicable standards and specification:

EN 149:2001+A1:2009 Respiratory protective devices - Filtering half masks to protect against particles - Requirements, testing, marking

Model reference	Product description
XGM-95	Folding filtering half mask fitted with ear loops with head harness clip, no valves, internal metal nose clip Mask body color: White Classification: FFP2 NR Test report No.: 2020(F) - 0376

Certificate Revision	Revision date	Revision details
A	2020-10-23	Initial issue

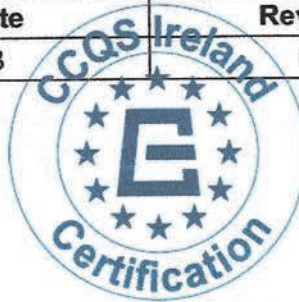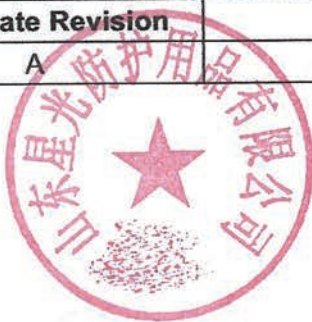

CCQS Certification Services Limited

Block 1 Blanchardstown Corporate Park, Ballycoolin Road, Blanchardstown, Dublin 15, D15 AKK1, Ireland

Tel: +00 353 1 588 6920 Website: www.ccqs.co.uk E-mail: verify@ccqs.ie

If in any doubt about the integrity of this certificate, please contact CCQS by email to verify.





Certificate of Module C2 production monitoring for equipment within the scope of Personal Protective Equipment Regulation (EU) 2016/425 Category III

FPC Certificate No.: CE-PC-200331-168-FPC-A

Certificate holder:	Shandong Xingguang Protective Products Co., Ltd. Business Room 315, Zhilan Village 3, Gaomi Economic Development Zone, Gaomi City, Shandong Province, P.R.China
Manufacturing location:	Business Room 315, Zhilan Village 3, Gaomi Economic Development Zone, Gaomi City, Shandong Province, P.R.China
The scope of the certification for:	The manufacture of respiratory protective device See annex for articles covered by this certificate
Validity from:	2020-10-23
Revision date:	2020-10-23
To:	2021-10-22



CCQS Certification Services Limited in its role as a Notified Body for PPE Regulation, is monitoring that the manufacturer is producing PPE in conformity with the type described in the EU type-examination certificate and associated technical file and which satisfies the Essential Health and Safety Requirements of the Regulation. The equipment covered by this certificate is listed in the accompanying schedule. This certificate is not complete and has no validity without the accompanying schedule and revision index. The manufacturer is hereby authorized to affix our Notified Body number, 2834, to each item of PPE mentioned in the schedule which accompanies this certificate whilst this certificate remains valid. This certificate and the accompanying schedule remain the property of CCQS and maybe withdrawn or revised at any time if CCQS considers that the equipment is no longer in conformity with the requirements of the Regulation.



Approved by Ireland Government as a Notified Body for CE Marking No.2834



CCQS Certification Services Limited

Block 1 Blanchardstown Corporate Park, Ballycoolin Road, Blanchardstown, Dublin15, D15 AKK1, Ireland

Tel: +00 353 1 588 6920 Website: www.ccqs.co.uk E-mail: verify@ccqs.ie

If in any doubt about the integrity of this certificate, please contact CCQS by email to verify.



Schedule of Module C2 production monitoring for equipment within the scope of Personal Protective Equipment Regulation (EU) 2016/425 Category III

Schedule to CCQS FPC Certificate No.: CE-PC-200331-168-FPC-A

Product reference and description		Reference standard
Particle Filtering Half Mask	Model: XGM-95	EN 149:2001+A1:2009

Certificate Revision	Revision date	Revision details
A	2020-10-23	Initial issue

This schedule has no validity without the accompanying certificate.

This schedule and the accompanying certificate remain the property of CCQS and maybe withdrawn or revised at any time if CCQS considers that the equipment is no longer in conformity with the requirements of the Regulation.



CCQS Certification Services Limited

Block 1 Blanchardstown Corporate Park, Ballycoolin Road, Blanchardstown, Dublin 15, D15 AKK1, Ireland

Tel: +00 353 1 588 6920 Website: www.ccqs.co.uk E-mail: verify@ccqs.ie

If in any doubt about the integrity of this certificate, please contact CCQS by email to verify.

Page 2 of 2
(Fm 220-015, Rev.2)



EU Declaration of Conformity

Annex IX PPE Regulation (EU) 2016/425

This EU Declaration of conformity refers to the following products

1. The basic information is as follows:

Product Name	Model	Classification/Type	Batch No./Serial No./Identifier
Particle Filtering half mask	XGM-95	FFP2 NR	

2. The Manufacturer 's name and address is as follows:


Name:	Shandong Xingguang Protective Products Co., Ltd.
Address:	Business room 315, Zhilan village 3, Gaomi Economic Development Zone, Gaomi City, Shandong Province, P. R. China

3. This Declaration of Conformity is issued under the sole responsibility of the Manufacturer.

4. Detailed description of the PPE to allow traceability/identification of the PPE.

Model: XGM-95; Classification/Type: FFP2 NR

Description: White folding half mask without valve

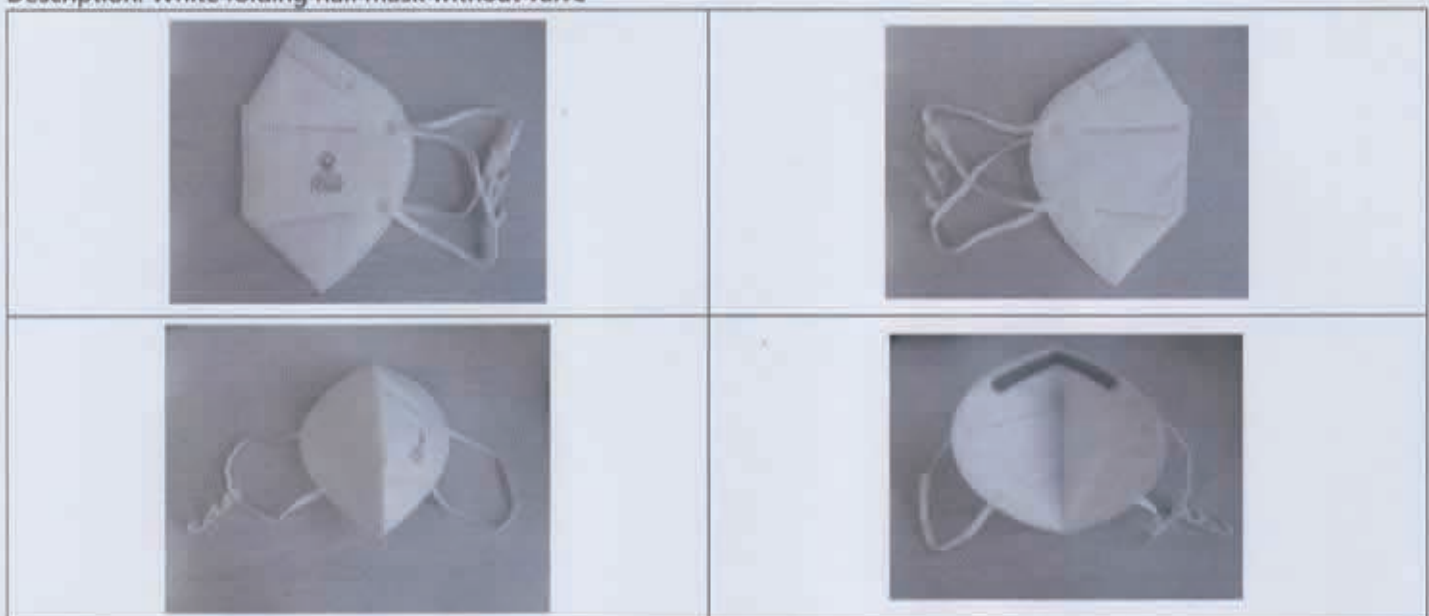

5. The article identified in (4) above is in conformance with the relevant Union Harmonization Legislation Regulation (EU) 2016/425.

6. References to the relevant harmonized standards used, including the date of the standard, or references to the other technical specifications, including the date of the specification, in relation to which conformity is declared:

No.	Harmonized standard name
1	EN 149:2001+A1:2009

7. CCQS Certification Services Limited. (NB 2834) performed the EU Type Examination (Module B) and issued the Type Examination Certificate Number:

No.	EU Type Examination (Module B) Certificate Number
1	

8. Product Category:

- This product is Category II.
- This product is Category III and is subject to Module C2 internal production control plus supervised product checks at random intervals and is under the surveillance of CCQS Certification Services Limited. (NB 2834)
- This product is Category III and is subject to Module D Conformity to type based on quality assurance of the production process and is under the surveillance of CCQS Certification Services Limited. (NB 2834)

Signature: Date: 2020/10/23 Company stamp and/or legal signature



2020/11/18

动态更新：取得国外标准认证或注册的非医用口罩生产企业清单



中国医药保健品进出口商会
服 务 产 业 链 | 助 力 国 际 化

English (<http://en.ccmhpie.org.cn/>)

请输入关键词

关于商会 ▾ 新闻中心 ▾ 行业服务 ▾

新闻中心 > 通知公告

权威发布 ▾ 商会会刊 ▾ 企业风采 会员之家 ▾

首页

动态更新：取得国外标准认证或注册的非医用口罩生产企业清单

推荐阅读

2020年11月18日 中国医药保健品进出口商会

分享

取得国外标准认证或注册的非医用口罩生产企业清单

动态更新：2020年11月17日下载

序号	生产企业	统一社会信用代码	国外注册认证情况
1057	山东星光防护用品有限公司 Shandong Xingguang Protective Products Co.,Ltd	91370785MA3Q0X8M7T	欧盟 CE