

DECLARAȚIE PRIVIND NOTIFICAREA PENTRU ÎNREGISTRAREA DISPOZITIVELOR MEDICALE ÎN REGISTRUL DE STAT AL DISPOZITIVELOR MEDICALE CARE DEȚIN MARCAJ CE

Către: **CENTRUL PENTRU ACHIZITII PUBLICE CENTRALIZATE IN SANATATE**
Adresa: **MD-2009, MOLDOVA, mun.Chişinău, MD-2009, Republica Moldova, str.
Cosmescu 3**

Numărul licitației: **Achizitii.md ID nr. 21089033 din 18 august 2023,**
MTender ID ocds-b3wdp1-MD-1692348758524,

Subsemnata, **Natalia GUMIONAIA** reprezentant împuternicit al companiei „**KIRANTONI**“ SRL, în calitate de ofertant la procedura de licitație publică Achizitii.md ID nr. 21089033 din 18 august 2023, MTender ID ocds-b3wdp1-MD-1692348758524, pentru atribuirea contractului de achiziție publică având ca obiect Achiziția Dispozitivelor medicale conform necesităților IMSP beneficiare (listă suplimentară nr. 22), codul CPV 33100000-1 , confirm că, în cazul pozițiilor castigate, vom înainta spre înregistrare în Registrul de Stat al Dispozitivelor Medicale a Agenției Medicamentului și Dispozitivelor Medicale bunurile contractate și până la momentul livrării acestora vom prezenta numărul de înregistrare, în cazul în care aceste bunuri intra sub incidența legislației republicii Moldova , privind dispozitivele medicale .

Data completării: **18.09.2023**

Semnat: _____

Nume/prenume: **Natalia GUMIONAIA**
Funcția în cadrul persoanei juridice: **ADMINISTRATOR**
Denumirea persoanei juridice: „**KIRANTONI**” SRL

BANK DETAILS

IDNO 1011600001572
TVA 0609491

IBAN MD12MO2224ASV42758107100 (MDL)
IBAN MD17MO2224ASV16072337100 - (EUR)

Bank: Mobiasbanca - OTP Group S.A.
bd. Ștefan cel Mare și Sfânt 81A, mun. Chişinău, MD-2012

Către: **Agenția Medicamentului
și Dispozitivelor Medicale****NOTIFICARE**pentru înregistrarea dispozitivelor medicale în Registrul de stat
al dispozitivelor medicale
nr. din

Solicitantul „**KIRANTONI**” SRL,
cu sediul **str. M.Costin 18, of 132 , mun. Chişinău, MD-2068 Republica Moldova**,
tel: mob.: (+373) 673 80 252 ; (+373) 600 85 449 ;
e-mail: office@kirantoni.com ; e-mail: manager@kirantoni.com ; www.kirantoni.com
solicit exminarea și înregistrarea în Registrul de stat al dispozitivelor medicale a următoarelor categorii
și tipuri de dispozitive medicale, pentru introducerea și punerea la dispoziție pe piață, in cazul in care
aceste bunuri intra sub incidenta legislației republicii Moldova, privind dispozitivele medicale:

Nr. d/o	Nr. Comanda	DENUMIRE	PRODUCATOR
1.	L003071	LAUDA Hydro H 2 P - BAIE PENTRU ȚESUTURI HIGRO FLOTANTE, 230 V; 50/60 Hz cod tarifiar 84194000	LAUDA DR. R. WOBSE R GMBH & CO. KG, Germania
2.	L003015 + A000138	MONO DISTILATOR LAUDA Puridest, model PD 8 R, 8 litri / oră, cu rezervor de stocare de 16 litri, 400 V / 3 ~ / N / PE +/-10 %, 50 / 60 Hz, 6,0 kW, cu Cablu de conectare la rețea. cod tarifiar 8419400	LAUDA DR. R. WOBSE R GMBH & CO. KG, Germania

Se anexează următoarele acte:

1. LETTER of AUTHORIZED DEALER Agreement – autorizatie de la producatorul LAUDA DR. R. WOBSE R GMBH & CO. KG GFL TECHNOLOGY, Germania
2. MANUAL de instructiun OPERATING INSTRUCTION LAUDA Hydro H 2 P Tissue Float Bath
3. MANUAL de instructiuni Q4DT-E_13_009_Puridest Distillation Apparatus R_V1_EN
4. DECLARATIE DE CONFORMITATE Hydro H 2 P Tissue Float Bath
5. DECLARATIE DE CONFORMITATE Distilator PURIDEST
6. Declaratie de la producator, referitor la dispozitive medicale , Kirantoni MD_Manufacturere Statement_06.09.2023
7. DECLARAȚIE PE PROPRIE RĂSPUNDERE
8. Declaratie KIRANTON SRL, privind inregistrarea echipamentelor.

Data _____

Semnătura _____

Tablelul de recepționare a notificării

(se completează de către Agenție în momentul depunerii notificării de către solicitant)

Comentarii cu privire la acceptul/refuzul recepționării notificării, inclusiv motivul refuzului	
Data/nr. de ordine atribuit notificării de către Agenție (în cazul acceptării recepționării)	
Numele, prenumele, funcția persoanei responsabile de recepționarea dosarului	
Semnătura persoanei responsabile	

BANK DETAILSIDNO 1011600001572
TVA 0609491IBAN MD12MO2224ASV42758107100 (MDL)
IBAN MD17MO2224ASV16072337100 - (EUR)Bank: Mobiasbanca - OTP Group S.A.
bd. Ștefan cel Mare și Sfânt 81A, mun. Chişinău, MD-2012

Lauda-Königshofen, January 27th, 2023

To whom it may concern

Letter of Authorized Dealer Agreement

This is to certify that:

Company: KIRANTONI SRL
Miron Costin street, nr. 18-132
MD-2068, Chisinau, Republic of Moldova

is an authorized distributor for Republic of Moldova of products manufactured by:

LAUDA DR. R. WOBSEY GMBH & CO. KG, Branch Facility
Burgwedel, Schulze-Delitzsch-Str. 4+5, 30938 Burgwedel, Germany

This agreement is to stand good from January 27th 2023 until December 31st, 2023.

LAUDA DR. R. WOBSEY
GMBH & CO. KG



ppa. Dr. Ralf Hermann
Chief Sales Officer



LAUDA DR. R. WOBSEY
GMBH & CO. KG
Lauda-Platz 1
97922 Lauda-Königshofen
Deutschland/Germany

LAUDA DR. R. WOBSEY GMBH & CO. KG
Pfarrstraße 41/43 · 97922 Lauda-Königshofen
Postfach 1251 · 97912 Lauda-Königshofen · DE

T +49 (0) 9343 503-0 · F +49 (0) 9343 503-222
info@lauda.de · www.lauda.de
WEEE-Reg.-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen
Registergericht Mannheim · HRA 560069

Persönlich haftende Gesellschafterin:
LAUDA DR. R. WOBSEY Verwaltungs-GmbH
Sitz Lauda-Königshofen
Registergericht Mannheim · HRB 560226

Geschäftsführer:
Dr. Gunther Wobser (Vors.), Dr. Mario Englert
Dr. Marc Stricker
Beirat: Dr. Gerhard Wobser

EC DECLARATION OF CONFORMITY

Hereby we,

LAUDA-GFL Gesellschaft für Labortechnik mbH
Schulze-Delitzsch-Str. 4+5
30938 Burgwedel
Federal Republic of Germany

declare that the below stated **Hydro Tissue float bath** model:

H 2 P

with the technical data:

**230 V, 50 / 60 Hz
0.3 kW**

are in conformity with the following EC Directives:

I	2014/35/EU	(Low Voltage Directive)
II	2014/30/EU	(EMC Directive)
III	2011/65/EU + (EU) 2015/863	(RoHS Directive)

For conformity **with I** the following standards were applied:

**EN 61010-1:2010
EN 61010-2-010:2014**


For conformity **with II** the following standard was applied:

EN 61326-1:2013

Authorized representative for the compilation of the technical documentation:

Mr Florian Wunderling at LAUDA-GFL

LAUDA-GFL Ges. für Labortechnik mbH



Andreas Degmayr
Managing director

Burgwedel, 01 July 2020



EC DECLARATION OF CONFORMITY

Manufacturer: LAUDA DR. R. WOBSEY GMBH & CO. KG
Schulze-Delitzsch-Straße 4+5, 30938 Burgwedel, Germany

We hereby declare under our sole responsibility that the machines described below

Product Line: Puridest **Serial number:** from 220____

Types: PD 2, PD 4,
PD 2 D, PD 4 D, PD 8 D,
PD 2 G, PD 2 DG, PD 4 G, PD 4 DG, PD 8 G,
PD 2 R, PD 4 R, PD 8 R and PD 12 R

comply with all relevant provisions of the EC Directives listed below due to their design and type of construction in the version brought on the market by us:

Machinery Directive	2006/42/EC
EMC Directive	2014/30/EU
RoHS Directive	2011/65/EU in connection with (EU) 2015/863

The protective objectives of the Machinery Directive with regard to electrical safety are complied with in accordance with Annex I Paragraph 1.5.1 in conformity with the Low Voltage Directive 2014/35/EU.

Applied standards:

- EN 61326-1:2013
- EN 61010-1:2010/A1:2019/AC:2019-04
- EN IEC 61010-2-010:2020

Authorized representative for the composition of the technical documentation:

Dr. Jürgen Dirscherl, Head of Research & Development

Burgwedel, 05.06.2023

Dr. Alexander Dinger,
Head of Quality and Environmental Management

Date: 06.09.2023

RFB No.: md ID no. 21089033 of August 18, 2023

MTender ID ocds-b3wdp1-MD-1692348758524

MANUFACTURER'S STATEMENT

To: CENTER FOR CENTRALIZED PUBLIC PROCUREMENT IN HEALTH -
CENTRUL PENTRU ACHIZITII PUBLICE CENTRALIZATE IN SANATATE
MD-2009, MOLDOVA, Chisinau municipality, MD-2009, Republic of Moldova, 3 Cosmescu str.

WHEREAS we, M/s LAUDA DR. R. WOBSEY GMBH & CO. KG, who are the official manufacturers of:

- LAUDA Hydro H 2 P Water Bath L003071,
- LAUDA Puridest PD 8 R Distiller L003015,
- LAUDA Hose Set for Distiller A000138

having factories at Laudaplatz 1, 97922 Lauda-Koenigshofen, Germany,

do hereby confirm that our equipment will be delivered new, unused, not refurbished and of the most recent or current models, produced not earlier than 2022 and that they incorporate all recent improvements in design and materials for the bid reference: Achizitii.md ID no. 21089033 of August 18, 2023, MTender ID ocds-b3wdp1-MD-1692348758524 for the above goods manufactured by us.

We confirm hereby that the above mentioned products are not considered and / or registered as a medical equipment.

LAUDA DR.R.WOBSEY
GMBH & CO. KG


LAUDA DR. R. WOBSEY
GMBH & CO. KG
Laudaplatz 1
97922 Lauda - Königshofen
Deutschland / Germany

Dr. Marta Garijo Añorbe
Area Sales Manager

LAUDA DR. R. WOBSEY GMBH & CO. KG
Laudaplatz 1 · 97922 Lauda-Königshofen
Postfach 1251 · 97912 Lauda-Königshofen · DE

T +49 (0) 9343 503-0 · F +49 (0) 9343 503-222
info@lauda.de · www.lauda.de
WEEE-Reg-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen
Registergericht Mannheim · HRA 560069

Persönlich haftende Gesellschafterin:
LAUDA DR. R. WOBSEY Verwaltungs-GmbH
Sitz Lauda-Königshofen
Registergericht Mannheim · HRB 560226

Geschäftsführer:
Dr. Gunther Wobser (Vors.), Dr. Mario Englert
Dr. Marc Stricker
Beirat: Dr. Gerhard Wobser

Manufacturer's Authorization

Date: 06.09.2023

RFB No.: md ID no. 21089033 of August 18, 2023

MTender ID ocds-b3wdp1-MD-1692348758524

To: CENTER FOR CENTRALIZED PUBLIC PROCUREMENT IN HEALTH -
CENTRUL PENTRU ACHIZITII PUBLICE CENTRALIZATE IN SANATATE
MD-2009, MOLDOVA, Chisinau municipality, MD-2009, Republic of Moldova, 3 Cosmescu str.

WHEREAS we, M/s LAUDA DR. R. WOBSEY GMBH & CO. KG, who are the official manufacturers of:

- LAUDA Hydro H 2 P Water Bath L003071,
- LAUDA Puridest PD 8 R Distiller L003015,
- LAUDA Hose Set for Distiller A000138

having factories at Laudaplatz 1, 97922 Lauda-Koenigshofen, Germany, do hereby authorize KIRANTONI Srl, Miron Costin street, nr. 18-132, Chisinau MD-2068, Republica Moldova, to submit a bid the purpose of which is to provide the above-mentioned Goods, manufactured by us and to subsequently negotiate and sign the Contract.

We hereby extend our full guarantee and 12 months warranty in accordance with our terms and conditions, with respect to the goods offered by the above firm.

We confirm that we do not engage or employ forced labor or persons subject to trafficking or child labor.

LAUDA DR.R.WOBSEY
GMBH & CO. KG


LAUDA DR. R. WOBSEY
GMBH & CO. KG
Laudaplatz 1
97922 Lauda - Königshofen
Deutschland / Germany

Dr. Marta Garjjo Añorbe
Area Sales Manager

LAUDA DR. R. WOBSEY GMBH & CO. KG
Laudaplatz 1 · 97922 Lauda-Königshofen
Postfach 1251 · 97912 Lauda-Königshofen · DE

T +49 (0) 9343 503-0 · F +49 (0) 9343 503-222
info@lauda.de · www.lauda.de
WEEE-Reg.-Nr.: DE 66 42 40 57

Kommanditgesellschaft: Sitz Lauda-Königshofen
Registergericht Mannheim · HRA 560069

Persönlich haftende Gesellschafterin:
LAUDA DR. R. WOBSEY Verwaltungs-GmbH
Sitz Lauda-Königshofen
Registergericht Mannheim · HRB 560226

Geschäftsführer:
Dr. Gunther Wobser (Vors.), Dr. Mario Englert
Dr. Marc Stricker
Beirat: Dr. Gerhard Wobser

Anexa nr. 2
La Procedurile administrative pentru notificarea
dispozitivelor medicale care dețin marcajul CE

Către Agenția Medicamentului și Dispozitive Medicale

DECLARAȚIE PE PROPRIE RĂSPUNDERE

Solicitant: „**KIRANTONI**” SRL ,
cu sediul **str. M.Costin 18, of 132 , mun. Chișinău, MD-2068 Republica Moldova**,
declar pe proprie răspundere, cunoscând prevederile art. 3521, Codul Penal al Republicii Moldova cu
privire la falsul în declarații, că documentele și datele furnizate pentru notificarea dispozitivelor medicale:

Nr. d/o	Nr. Comanda	DENUMIRE	Producator
1.	L003071	LAUDA Hydro H 2 P - BAIE PENTRU ȚESUTURI HIGRO FLOTANTE, 230 V; 50/60 Hz cod tarifiar 84194000	LAUDA DR. R. WOBSEER GMBH & CO. KG, Germania
2.	L003015 + A000138	MONO DISTILATOR LAUDA Puridest, model PD 8 R, 8 litri / oră, cu rezervor de stocare de 16 litri, 400 V / 3 ~ / N / PE +/-10 %, 50 / 60 Hz, 6,0 kW, cu Cablu de conectare la rețea. cod tarifiar 8419400	LAUDA DR. R. WOBSEER GMBH & CO. KG, Germania

Sunt autentice și corespund realității.

Data completării: **18.09.2023**

Semnat: _____

Nume/prenume: **Natalia GUMIONAIA**
Funcția în cadrul persoanei juridice: **ADMINISTRATOR**
Denumirea persoanei juridice: „**KIRANTONI**” SRL

BANK DETAILS

IDNO 1011600001572
TVA 0609491

IBAN MD12MO2224ASV42758107100 (MDL)
IBAN MD17MO2224ASV16072337100 - (EUR)

Bank: Mobiasbanca - OTP Group S.A.
bd. Ștefan cel Mare și Sfânt 81A, mun. Chișinău, MD-2012

Către: **Agenția Medicamentului
și Dispozitivelor Medicale**

DECLARAȚIE PRIVIND ÎNREGISTRAREA DISPOZITIVELOR MEDICALE ÎN REGISTRUL DE STAT AL DISPOZITIVELOR MEDICALE CARE DEȚIN MARCAJ CE

Subsemnata, **Natalia GUMIONAIA** reprezentant împuternicit al companiei „**KIRANTONI**“ SRL, cu sediul **str. M.Costin 18, of 132 , mun. Chișinău, MD-2068 Republica Moldova**, tel: mob.: (+373) 673 80 252 ; (+373) 600 85 449 ; e-mail: office@kirantoni.com ; e-mail: manager@kirantoni.com ; www.kirantoni.com **declar pe propria răspundere, că echipamentele de laborator :**

- **LAUDA Hydro H 2 P - BAIE PENTRU ȚESUTURI HIGRO FLOTANTE, 230 V; 50/60 Hz , Nr. Comanda L003071, Producator: LAUDA DR. R. WOBSEER GMBH & CO. KG, Germania**
- **MONO DISTILATOR LAUDA Puridest, model PD 8 R, 8 litri / oră, cu rezervor de stocare de 16 litri , 400 V / 3 ~ / N / PE +/-10 %, 50 / 60 Hz, 6,0 kW, cu Cablu de conectare la rețea. Nr. Comanda L003015 , livrat cu set de furtuni de conectare, Nr. Comanda:A000138, Producator: LAUDA DR. R. WOBSEER GMBH & CO. KG GFL TECHNOLOGY, Germania**

NU SUNT DISPOZITIVE MEDICALE și nu intră sub INCIDENȚA DIRECTIVELOR NAȚIONALE SAU INTERNAȚIONALE, PRIVIND DISPOZITIVELE MEDICALE ȘI NU POT FI INREGISTRATE ÎN REGISTRUL DE STAT AL DISPOZITIVELOR MEDICALE, CARE DEȚIN MARCAJ CE in conformitate cu documentele anexate : :

- MANUAL de instrucțiuni OPERATING INSTRUCTION LAUDA Hydro H 2 P Tissue Float Bath
- MANUAL de instrucțiuni Q4DT-E_13_009_Puridest Distillation Apparatus R_V1_EN
- DECLARAȚIE DE CONFORMITATE Hydro H 2 P Tissue Float Bath
- DECLARAȚIE DE CONFORMITATE Distilator PURIDEST
- Declarație de la producător, referitor la dispozitive medicale , Kirantoni MD_Manufacturere Statement_06.09.2023 in care este producătorul menționează , ca **aceste dispozitive nu pot fi considerate sau înregistrate ca dispozitive medicale.**

MANUAL de instrucțiuni_OPERATING INSTRUCTION LAUDA Hydro H 2 P Tissue Float Bath

Sau <https://www.lauda.de/en/services/download-center/filter/Operating-instruction/Hydro/default/default/English>

Pag. 7

1.2 Improper Use

Operating Instructions Hydro Tissue Float Bath H 2 P

Tissue Float Baths operated in a laboratory **are no medical devices.** They neither fall under national nor international Medical Device Directives nor have to be used and applied accordingly.

Pag. 7

1.2 Utilizare necorespunzătoare

BANK DETAILS

IDNO 1011600001572
TVA 0609491

IBAN MD12MO2224ASV42758107100 (MDL)
IBAN MD17MO2224ASV16072337100 - (EUR)

Bank: Mobiasbanca - OTP Group S.A.
bd. Ștefan cel Mare și Sfânt 81A, mun. Chișinău, MD-2012

Băile pentru țesuturi hidro flotante , operate într-un laborator **nu sunt dispozitive medicale**. Acestea **nu intră sub incidența directivelor naționale sau internaționale privind dispozitivele medicale și nici nu trebuie să fie utilizate și aplicate în consecință**

Manual de instrucțiuni Q4DT-E_13_009_Puridest Distillation Apparatus R_V1_EN_Translation_web (2)
Sau <https://www.lauda.de/en/services/download-center/filter/Operating-instruction/Puridest/default/default/English>

Pag 7.

1.2 Improper Use

LAUDA Puridest Distillation Apparatus, operated in a laboratory, **are no Medical Devices**. They fall neither under national nor international Medical Device Directives and have to be used and applied accordingly.

Pag.7.

1.2 Utilizare necorespunzătoare

Aparatele de distilare LAUDA Puridest, operate într-un laborator, **nu sunt dispozitive medicale**. Acestea nu intră sub incidența directivelor naționale sau internaționale privind dispozitivele medicale și trebuie utilizate și aplicate în consecință.

Aceste documente sunt autentice și corespund realității.

Data completării: **18.09.2023**

Semnat: _____

Nume/prenume: **Natalia GUMIONAIA**

Funcția în cadrul persoanei juridice: **ADMINISTRATOR**

Denumirea persoanei juridice: **„KIRANTONI” SRL**

BANK DETAILS

IDNO 1011600001572
TVA 0609491

IBAN MD12MO2224ASV42758107100 (MDL)
IBAN MD17MO2224ASV16072337100 - (EUR)

Bank: Mobiasbanca - OTP Group S.A.
bd. Ștefan cel Mare și Sfânt 81A, mun. Chișinău, MD-2012



Operating Instructions

Hydro Tissue Float Bath

H 2 P



The LAUDA Hydro Tissue Float Bath H 2 P is a special bath for histological, pathological, clinical and bacteriological laboratories, for stretching and drying of cut tissue samples. The outer housing is made of powder coated aluminium, the bath body as well as the rims of the bath to dry the cut tissues are made of black anodised aluminium.

The units' temperature can be set via an electro-mechanical temperature controller with capillary tube sensor in a temperature range of 5 K above ambient to approx. 80 °C and is protected by a temperature cut-out in case of dry running of the heating element. The Bath is heated indirectly, heating plate, sensor of the thermostat and temperature cut-out are situated below the bath.

Before installation, please check whether contents of package are in good order and complete.

Should you note any damages or have any reasons for complaint, please contact your supplier or directly:

LAUDA DR. R. WOBSE GMBH & CO. KG

Schulze-Delitzsch-Str. 4+5

30938 Burgwedel - Germany

Phone: +49 (0)5139 9958 0

Fax: +49 (0)5139 9958 21

Email: info@lauda.de

Internet: <https://www.lauda.de>

Translation of the original operating instructions

Q4DT-E_13-003-EN-01, 29.06.2023

© 2023 LAUDA DR. R. WOBSE GMBH & CO. KG

Contents

Operating Instructions	1
1 Use of the Tissue Float Bath	7
1.1 Intended Use	7
1.2 Improper Use	7
2 Warranty conditions.....	7
3 Before installation	8
4 Set-Up and Location of the Tissue Float Bath	8
5 Operating Voltage.....	8
6 Thermometer	9
7 Filling Water into the Tissue Float Bath	9
8 Installation, Temperature Regulation and Shutdown	9
9 Temperature Monitoring in Case of an Error	9
10 Maintenance, Support and Repair.....	10
10.1 Technical support.....	10
11 Disposal of Old Appliances	10
12 Technical Data	11
13 Circuit diagram	12
14 Examples for connection to the mains supply.....	13
14.1 Electrical fuses	13
14.2 Examples for connection to the mains	14
15 Accessories.....	15
16 Notes	16
17 Ordering spare parts / LAUDA Service	17
18 Product Returns and Clearance Declaration	18
19 EC Declaration of Conformity and certificates	19

1 Use of the Tissue Float Bath

1.1 Intended Use

LAUDA Hydro Tissue Float Baths are used to heat up distilled or desalinated water in a temperature range of 5 K above ambient to approx. 80 °C, in order to flatten cut tissues to prepare them for further studies, to transfer them to microscope slides and to dry them on the indirectly heated rim of the bath.

The information contained in this operating instruction must be read and observed by all means. Only then a perfect operation of the LAUDA Hydro Evaporation Water Bath can be guaranteed. The units may only be installed and operated by persons who have made themselves familiar with these operating instructions.



Caution:

Hot surfaces at temperatures above 50 °C. Danger of burns and danger of scaldings through steam released when opening the lid of the Tissue Float Bath. It is recommended to wear suitable safety gloves.

1.2 Improper Use

Do not use tap water as lime deposits on the black anodised bottom of the bath will prevent clear visibility of the cut tissues. Only use water in the bath; other media, e. g. oils or acids, will lead to damages and might even cause total unit failure. The temperature work must not create an explosive atmosphere nearby of the unit. LAUDA Hydro Tissue Float Baths are not suitable for direct temperature work of foodstuffs, drinks and tobacco or for medical-technical and pharmaceutical products. Direct temperature work means unprotected contact of the substances with the bath filling. It is not permissible to either heat up or vaporise aggressive media, e. g. hydrochloric acid, in the unit itself or in the vicinity. LAUDA Hydro Tissue Float Baths operated in a laboratory are no medical devices. They neither fall under national nor international Medical Device Directives nor have to be used and applied accordingly.

2 Warranty conditions

LAUDA offers a standard 12 month manufacturer's warranty from the date of purchase.

3 Before installation

The information given in the present manual must by all means be carefully read and observed. Only then can a perfect functioning of the Evaporation Water Bath be guaranteed. Safety precautions are additionally marked with the following symbols.



Read and observe the operating instructions



Warning of hot liquids and vapour




Warning of hot surfaces



Warning of dangerous electrical voltage



General warning



Before maintenance and repair disconnect the unit all-pole from the electrical mains (pull the plug from the socket).

4 Set-Up and Location of the Tissue Float Bath



Place on solid, even and level surfaces inside buildings only. Make sure to place the unit only on a water-tight, temperature-resistant and non-flammable surface. The unit is not suitable for use in potentially explosive surroundings.

5 Operating Voltage



The main switch of the Tissue Float Bath must be off (position O). The operating voltage on the name-plate (at the back of the unit) must be the same as the mains voltage. The supplied connection cable disposes of a high-temperature coupling on one end, which is to be plugged into the unit's socket at the back of the unit, and a shock-proof plug that serves as the mains plug and is to be connected to the mains socket. The Water Bath must be connected to a correctly installed shock-proof socket. The bath is a protection class I electrical appliance, a connection to the earth conductor (PE) must be ensured. For information on the required mains fuse please view the technical data, chapter 11 of this manual. The electrical connection must ensure an all-pole separation from the mains supply at any time. The mains cable must not touch hot surfaces of the unit anywhere. It may not be led underneath the unit. In case of compliance, connect the unit to the mains.

6 Thermometer

Fix the thermometer holder to the bath rim, opposite the control panel, and place the glass thermometer into the holder. The thermometer must not touch the bottom of the bath.

7 Filling Water into the Tissue Float Bath



Before initiation, fill either distilled or desalinated water up to approx. 1 - 2 cm beneath the rim of the bath. The maximum filling quantity can be found in the technical data, chapter 12 of these instructions.

8 Installation, Temperature Regulation and Shutdown

Switch on the main switch. The green pilot lamp to the left above the main switch will light up. Set the required temperature on the turning knob of the temperature regulator. The temperature range of the bath is between approx. 5 K above ambient to maximum approx. 80 °C. After setting the required temperature, the heating element is powered. The yellow pilot lamp to the left above the temperature regulator lights up. The thermometer shows the current temperature. For safe heating up to the maximum temperature cover the bath with a lid (accessory).

Caution, please observe by all means.

To turn off for longer shut-down periods switch the main switch to position \bigcirc and disconnect the unit from the mains. Empty the Evaporation Water Bath and dry the cabinet interior to prevent bacterial contamination.



Caution:


Hot surfaces at temperatures above 50 °C. Danger of burns. Take extreme care when handling the unit because of the high operating temperatures.

9 Temperature Monitoring in Case of an Error

The Tissue Float Bath is protected against destruction by running dry or defective temperature controller by a temperature cut-out (non readjustable, temperature-dependent cut-out). The cut-out cuts the power to the heating. A defective temperature cut-out must be exchanged against an identical cut-out.

10 Maintenance, Support and Repair

The LAUDA Hydro Tissue Float Bath is constructed to withstand even rough service conditions. Nevertheless, the unit should only be subjected to increased strain within sensible limits.



Make sure to prevent liquids coming into contact with cable connections or the inside of the electrical appliance.

Before opening and/or cleaning the unit, pull the plug from the socket.

Danger of electrical shock!



The black anodised bath as well as the off-white powder-coated surfaces may be cleaned with mild, non-abrasive and pH neutral detergents. Never use detergents containing solvents.

It is advisable to exchange the water in the bath in regular intervals in order to prevent bacterial contamination.

10.1 Technical support

You can call our customer service at any time for technical support relating to LAUDA Hydro Tissue Float Baths appliances.

Phone : +49 (0) 9343 / 503-350

Fax : +49 (0)9343 503-283

Email : service@lauda.de

Maintenance, repairs and modifications must be carried out by a qualified electrician (section 2 (3) DGUV Regulation 3) according to the General Rules of Technology (section 2 (2) DGUV Regulation 3). Only original spare parts may be used. Request that the person performing the work provides written confirmation of the type and scope of the work carried out (company, date, signature).

11 Disposal of Old Appliances

LAUDA will take responsibility, within the scope of the legal directives, for an environmentally sound handling and disposal of all used LAUDA units as of the production year 1995 that are returned to us free of charge and will have them materially recycled. Before a unit is returned, a legally binding declaration must be provided from the sender confirming that the unit is free from harmful and/or hazardous contaminations as well as from hazardous substances caused by the previous use of the unit.


LAUDA laboratory apparatus are exclusively designed for industrial use and may not be disposed of through public waste disposal authorities.

EAR Registration Number WEEE-ID.NO 67770231

12 Technical Data

Exterior dimensions (diameter / height)	280 mm / 100 mm
Interior dimensions (diameter / height)	200 mm / 60 mm
Usable bath height	50 mm
max. filling quantity (in litres)	1.6 l
Temperature range	approx. 5 K above ambient to +80 °C
Temperature control	Capillary thermostat
Temperature setting	on the turning knob
Temperature constancy, temporal	approx. +/- 0,5 K
Over-temperature cut-out	Temperature cut-out, > 130 °C non readjustable
Electrical connection	230 V, 50 / 60 Hz or as a special make (see nameplate) 115 V, 50 / 60 Hz
Power	0,3 kW
Mains connection	Shock-proof plug
Mains fuse	min. 10 A – max. 16 A
Protection type / protection class	IP20 / I
Ambient conditions	Use only indoors (not in potentially explosive surroundings)
Height above sea level	up to 2000 m NN
Ambient temperature	+10 °C to +40 °C
Humidity	max. 80 % relative humidity up to 31 °C, decreasing to 50 % relative humidity at 40 °C
Weight	2 kg

13 Circuit diagram

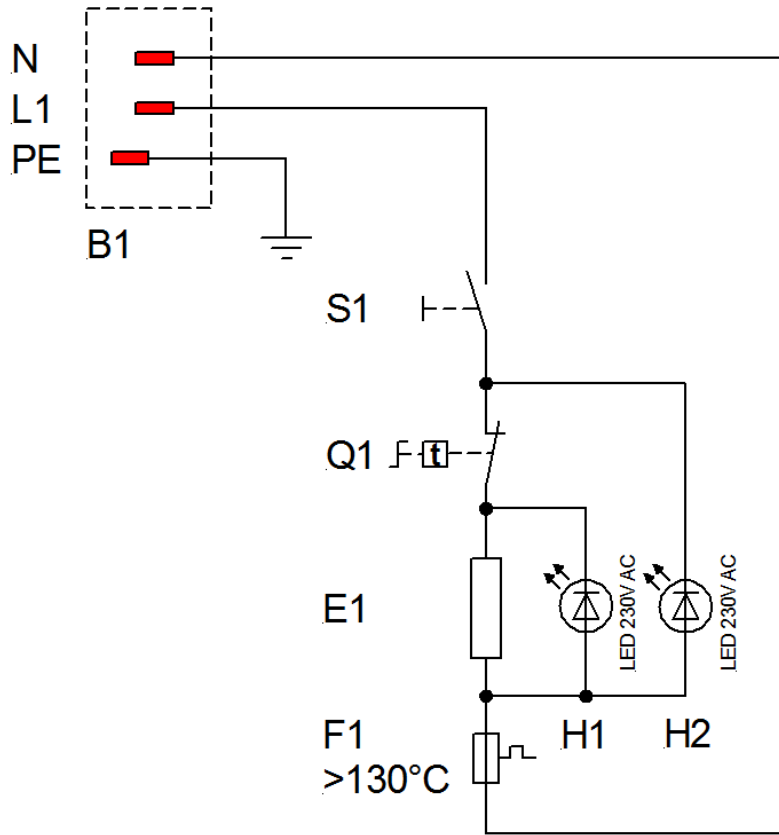

- B1 Socket for unit
- E1 Heating element 300 W
- F1 Over-temperature cut-out > 130 °C
- H1 LED Pilot lamp operation, yellow
- H2 LED Pilot lamp mains, green
- S1 Main switch
- Q1 Temperature regulator

14 Examples for connection to the mains supply

Tissue Float Baths are supplied with a pre-assembled, cast-on shock-proof plug. Make sure to connect to a protective conductor terminal.

Colour coding of mains cable	Mains supply
ge/gr – yellow/green	PE (Protective earth)
bl – blue	N
sw – black	L1

All Tissue Float Baths supplied for 230 V (see information on the nameplate) can be connected to all power supplies of 220 V or 230 V. Maximum grid impedance $Z_{max} = 0,135 \Omega$. If necessary, this value should be requested from the responsible energy supply company.


14.1 Electrical fuses

Model	Power	Power consumption at mains voltage *	Mains fuse (F4, F5)
H 2 P	0,3 kW	1,3 A at 230 V	10 A / Amp (max. 16 A / Amp.)

14.2 Examples for connection to the mains


Components

- B1 Earthing contact socket (on-site)
- B2 Earthing contact plug (mounted on the unit)
- F4 Mains fuse (on-site)
- F5 Mains fuse (on-site)

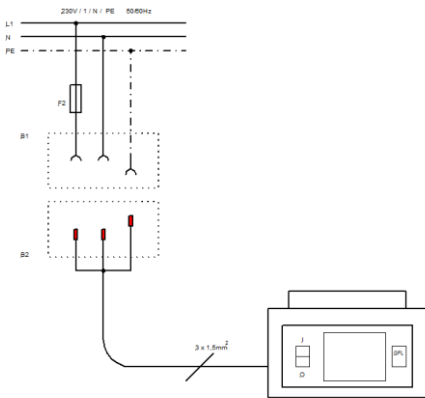


H 2 P

for 230 V with power supply 230 V / N / PE / 50/60 Hz,
connected through 3-pole shock-proof (Schuko) plug system.

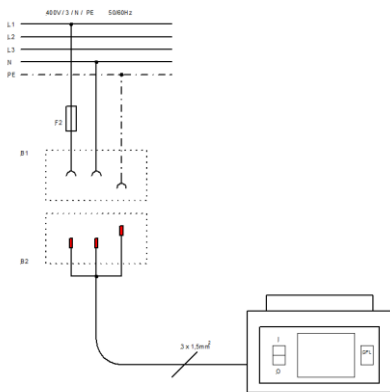

H 2 P

for 230 V with power supply 400 V / 3 / N / PE / 50/60 Hz,
connected through 3-pole shock-proof (Schuko) plug system.

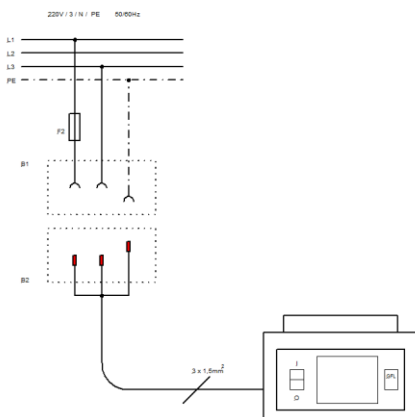

H 2 P

for 230 V with power supply 220 V / 3 / N / PE / 50/60 Hz,
connected through 3-pole shock-proof (Schuko) plug system.

15 Accessories



Lid, to cover the bath interior, made of black anodised aluminium, with ball handle.

Order no: A000040

17 Ordering spare parts / LAUDA Service

When ordering spare parts, please state the serial number (type plate) to avoid queries and wrong deliveries.

Your partner for maintenance and competent service support:

LAUDA Service
Phone: +49 (0)9343 503-350
Fax: +49 (0)9343 503-283
Email: service@lauda.de

We are always at your disposal for questions and suggestions!

LAUDA DR. R. WOBSE GMBH & CO. KG
Laudaplatz 1
97922 Lauda-Königshofen
Germany
Phone: +49 (0)9343 503-0
Fax: +49 (0)9343 503-222
Email info@lauda.de
Internet: <http://www.lauda.de/>

18 Product Returns and Clearance Declaration



Product Returns and Clearance Declaration

Product Returns

Would you like to return a LAUDA product you have purchased to LAUDA? For the return of goods, e.g. for repair or due to a complaint, you will need the approval of LAUDA in the form of a *Return Material Authorization (RMA)* or *processing number*. You can obtain the RMA number from our customer service department at +49 (0) 9343 503 350 or by email service@lauda.de.

Return address

LAUDA DR. R. WOBSEY GMBH & CO. KG

Laudaplatz 1

97922 Lauda-Königshofen

Deutschland/Germany

Clearly label your shipment with the RMA number. Please also enclose this fully completed declaration.

RMA number	Product serial number
Customer/operator	Contact name
Contact email	Contact telephone
Zip code	Place
Street & house number	
Additional explanations	

Clearance Declaration

The customer/operator hereby confirms that the product returned under the above-mentioned RMA number has been carefully emptied and cleaned, that any connections have been sealed to the farthest possible extent, and that there are no explosive, flammable, environmentally hazardous, biohazardous, toxic, radioactive or other hazardous substances in or on the product.

Place, date	Name in block letters	Signature

Version 02 - EN

LAUDA

EC DECLARATION OF CONFORMITY

Manufacturer: LAUDA DR. R. WOBSEY GMBH & CO. KG
Schulze-Delitzsch-Straße 4+5, 30938 Burgwedel, Germany

We hereby declare under our sole responsibility that the machines described below

Product Line: Hydro **Serial number:** from 220_____

Types: H 4, H 8, H 8 A, H 16, H 16 A, H 22, H 24 and H 41
H 20 S, H 20 SW and H 20 SOW
H 5 V, H 6 V, H 9 V, H 11 V and H 19 V
H 2 P

comply with all relevant provisions of the EC Directives listed below due to their design and type of construction in the version brought on the market by us:

Machinery Directive	2006/42/EC
EMC Directive	2014/30/EU
RoHS Directive	2011/65/EU in connection with (EU) 2015/863

The protective objectives of the Machinery Directive with regard to electrical safety are complied with in accordance with Annex I Paragraph 1.5.1 in conformity with the Low Voltage Directive 2014/35/EU.

Applied standards:

- EN 61326-1:2013
- EN 61010-1:2010/A1:2019/AC:2019-04
- EN IEC 61010-2-010:2020

Authorized representative for the composition of the technical documentation:

Dr. Jürgen Dirscherl, Head of Research & Development

Burgwedel, 05.06.2023



Dr. Alexander Dinger,
Head of Quality and Environmental Management

QSWA-QA13-028-EN-01

*FAHRENHEIT. *CELSIUS. *LAUDA.

LAUDA DR. R. WOBSEER GMBH & CO. KG

Schulze-Delitzsch-Straße 4+5 • 30938 Burgwedel • Germany

Phone.: +49 (0) 5139 9958-0 • Fax +49 (0) 5139 9958-21

Email: info@lauda.de • Internet: <https://www.lauda.de>



Operating Instructions

Puridest Distillation Apparatus

PD 2 R, PD 4 R, PD 8 R, PD 12 R



LAUDA Puridest Distillation Apparatus models PD 2 R, PD 4 R, PD 8 R and PD 12 R with storage tank produce highly-pure, bacteria and pyrogen free distillate with a very low conductivity (approx 2.3 $\mu\text{S} / \text{cm}$ at 25 °C). The distillate is in conformity with DAB regulations and the regulations of many international pharmacopeia..



I II III



IV

- I Main switch
- II Pilot lamp Clean
- III Operation pilot lamp
- IV Distillate withdrawal

Before installation, please check whether contents of package are in good order and complete.
Should you note any damages or have any reasons for complaint, please contact your supplier or directly.

LAUDA DR. R. WOBSE R GMBH & CO. KG
Schulze-Delitzsch-Str. 4+5
30938 Burgwedel - Germany
Phone: +49 (0)5139 9958 0
Fax: +49 (0)5139 9958 21
Email: info@lauda.de
Internet: <https://www.lauda.de>

Translation of the original operating instructions
Q4DT-E_13-009-EN-01, 28.06.2023
© 2023 LAUDA DR. R. WOBSE R GMBH & CO. KG

Content

Operating Instructions	1
1 Use of the Distillation Apparatus	7
1.1 Intended Use.....	7
1.2 Improper Use	7
2 Warranty conditions.....	7
3 Before Initiation	8
4 Set-up and Location of the Distillation Apparatus	8
5 Operation Voltage.....	9
6 Water Connections	9
6.1 Distillate withdrawal ①	10
6.2 Drain boiler ②	10
6.3 Cooling water outlet ③	10
6.4 Tap water inlet ④	10
7 Initiation	11
7.1 Before initial starting	11
7.2 Initiation.....	11
8 Functional Description	11
9 Maintenance, Service and Trouble Shooting	12
9.1 Descaling	12
9.2 Pilot Lamp Clean	12
9.2.1 <i>Foam formation caused by polluted water in the boiler.....</i>	<i>12</i>
9.2.2 <i>Back water in the boiler</i>	<i>13</i>
9.3 Re-initiation after low water	13
9.4 Technical support.....	13
10 Disposal of Old Units.....	13
11 Technical Data	14
11.1 Distillation Apparatus Puridest models PD 2 R, PD 4 R	14
11.2 Distillation Apparatus Puridest models PD 8 R, PD 12 R	15
12 Circuit Diagram.....	16
12.1 PD 2 R.....	16
12.2 PD 4 R.....	17
12.3 PD 8 R - version 230 V / 1 ~ for permanent connection to the mains.....	17
12.4 PD 8 R / PD 12 R - version 220 V / 3 ~ for permanent connection to the mains	18

12.5	PD 8 R / PD 12 R – version 400 V / 3 ~ for permanent connection to the mains	18
13	Connection to the Mains.....	19
13.1	Examples for connection to the mains supply	20
13.1.1	<i>PD 2 R and PD 4 R for 230 V for a mains supply of 220 V / 3 ~ / PE / 50 / 60 Hz.....</i>	<i>20</i>
13.1.2	<i>PD 2 R / PD 4 R for 230 V for a mains supply of 400 V / 3 ~ / N / PE / 50 / 60 Hz.....</i>	<i>20</i>
13.1.3	<i>PD 8 R for 230 V / 1 ~ for a mains supply of 220 V / 3 ~ / PE / 50 / 60 Hz.....</i>	<i>21</i>
13.1.4	<i>PD 8 R for 230 V / 1 ~ for a mains supply of 400 V / 3 ~ / N / PE / 50 / 60 Hz.....</i>	<i>21</i>
13.1.5	<i>PD 8 R and PD 12 R for 220 V / 3 ~ for a mains supply of 220 V / 3 ~ / PE / 50 / 60 Hz.....</i>	<i>22</i>
13.1.6	<i>PD 8 R and PD 12 R for 220 V / 3 ~ for a mains supply of 220 V / 3 ~ / PE / 50 / 60 Hz.....</i>	<i>22</i>
13.1.7	<i>PD 8 R and PD 12 R for 400 V / 3 ~ for a mains supply of 400 V / 3 ~ / N / PE 50 / 60 Hz.....</i>	<i>23</i>
13.1.8	<i>PD 8 R and PD 12 R for 400 V / 3 ~ for a mains supply of 400 V / 3 ~ / N / PE 50 / 60 Hz.....</i>	<i>23</i>
14	Accessories and Options	24
15	Notes.....	26
16	Ordering spare parts / LAUDA Service.....	27
17	Product Returns and Clearance Declaration	28
18	EC Declaration of Conformity and certificates.....	29

1 Use of the Distillation Apparatus

1.1 Intended Use

In LAUDA Puridest Distillation Apparatus models PD 2 R, PD 4 R, PD 8 R and PD 12 R electric heating elements serve to boil water and evaporate it. The steam is led through steam tubes into the storage tank where it condenses on a water-cooled cooling coil. The produced distillate drips into the storage tank. The storage tank level is electronically monitored, the Distillation Apparatus heating element(s) and cooling water supply will be switched off when the tank is full. Depending on the model, the distillate quantity per hour ranges between 2 litres (PD 2 R), 4 litres (PD 4 R), 8 litres (PD 8 R) and 12 litres (PD 12 R).

Depending on the tap water quality, the produced distillate has a conductivity of approx. $2.3 \mu\text{S} / \text{cm}$ at $25 \text{ }^\circ\text{C}$. To feed the Distillation Apparatus, preferably use tap water of drinking quality. Please also observe the information in chapters 16.2 to 16.4 of these instructions on the possible use of filters and cartridges to pretreat the tap water.

The Distillation Apparatus must be operated within the user's field of vision.



The information contained in these operating instructions must by all means be read and observed. Only then a perfect operation of the Distillation Apparatus can be guaranteed. The units may only be installed and operated by persons who have made themselves familiar with these operating instructions.



Caution:

The accessible inner parts of the housing, that can be reached after lifting the outer lid get strongly heated up during operation. These parts may only be touched after they have cooled down, or when wearing suitable safety gloves.

1.2 Improper Use


LAUDA Puridest Distillation Apparatus, operated in a laboratory, are no Medical Devices. They fall neither under national nor international Medical Device Directives and have to be used and applied accordingly. The Distillation Apparatus must not be used in potentially explosive surroundings. The Distillation Apparatus must neither be set up nor operated in laboratory areas with aggressive or corrosive ambient conditions.

2 Warranty conditions

LAUDA offers a standard 12 month manufacturer's warranty from the date of purchase.

3 Before Initiation

Important information are marked in bold letters in these instructions, safety indications are additionally marked by the following warning symbols and mandatory signs.

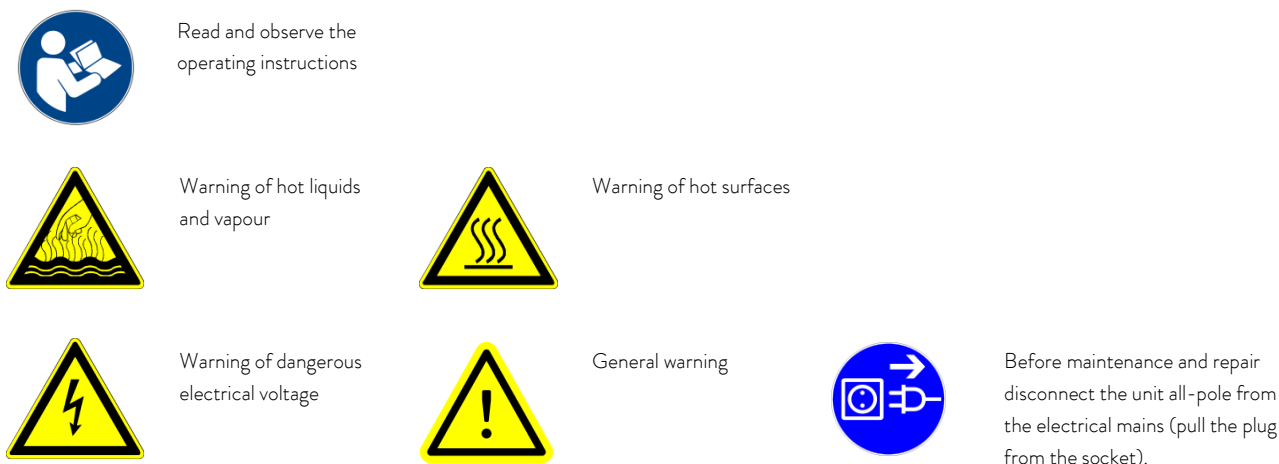

4 Set-up and Location of the Distillation Apparatus



Protect yourself and the unit during transport and setup by working carefully and avoid danger of e. g. shifting or tilting the unit as well as risk of injury by lifting heavy loads.

Caution, Distillation Apparatus models PD 4 R (net weight 21.8 kg), PD 8 R (net weight 35.8 kg) and PD 12 R (net weight 40.9 kg) must be lifted, carried and transported to the location by at least two persons. The Distillation Apparatus can be held between the four stands of the unit and lifted for setup.

The unit is suitable for both bench and wall mounting. It is only suitable for indoor use. Table-top setting-up on solid, even and level surfaces only. Make sure to place the unit only on a watertight, temperature-resistant, non-flammable surface.

The location must provide sufficient space as well as the necessary carrying capacity for the total weight of the unit (unit weight as per technical data, chapter 11 of this manual, plus weight of the filling).

For setting-up on the wall, check the carrying capacity of the wall in connection with the total weight of the unit (appliance plus water filling, see Technical Data). Make sure to check the on-site fixing elements in order to guarantee safe hold of the Distillation Apparatus. The fixing material must be suitable for the substrate. Use only tested and proven fixing material.

There are two keyholes for wall mounting at the back of the Distillation Apparatus. Place two fixing screws (not included in the scope of supply) in the wall in the distance of the two keyholes and nest the Distillation Apparatus on the keyholes. The unit is delivered without fixing material.

Model	/	Distance of screws
PD 2 R	/	40 cm
PD 4 R	/	48 cm
PD 8 R	/	64 cm
PD12 R	/	64 cm

The unit is not suitable for use in potentially explosive surroundings, e. g. during anaesthesia with inflammable gas or steam types!

5 Operation Voltage



The Distillation Apparatus must be connected to the mains supply either by a correctly installed shock-proof socket, or, with a fixed connection, to an on-site main switch. The Distillation Apparatus is a protection class I electrical appliance, a connection to the earth conductor (PE) must be ensured. For information on the required mains fuse please view Technical Data, chapter 11 of this manual.

The electrical proof sockets or in such a way as



connection must ensure an all-pole separation from the mains at any time. Shock-main switches to separate the Distillation Apparatus from the mains must be installed to ensure they can be clearly identified and are easily accessible at any time.




The mains connection cable must not touch any hot surfaces of the unit. It may not lead underneath the unit. The main switch (I) of the Distillation Apparatus must be off (position O). The voltage on the nameplate (at the left-hand side of the unit) must be identical to the mains voltage. If they are identical, connect the unit to the mains. Please also refer to chapter 14 of these operating instructions "Connection to the Mains".

6 Water Connections

All water connections of the Distillation Apparatus, except the distillate withdrawal tap on the front, are situated on the right-hand side of the unit.

Hoses for water inlet and outlet are not included in the standard scope of supply.

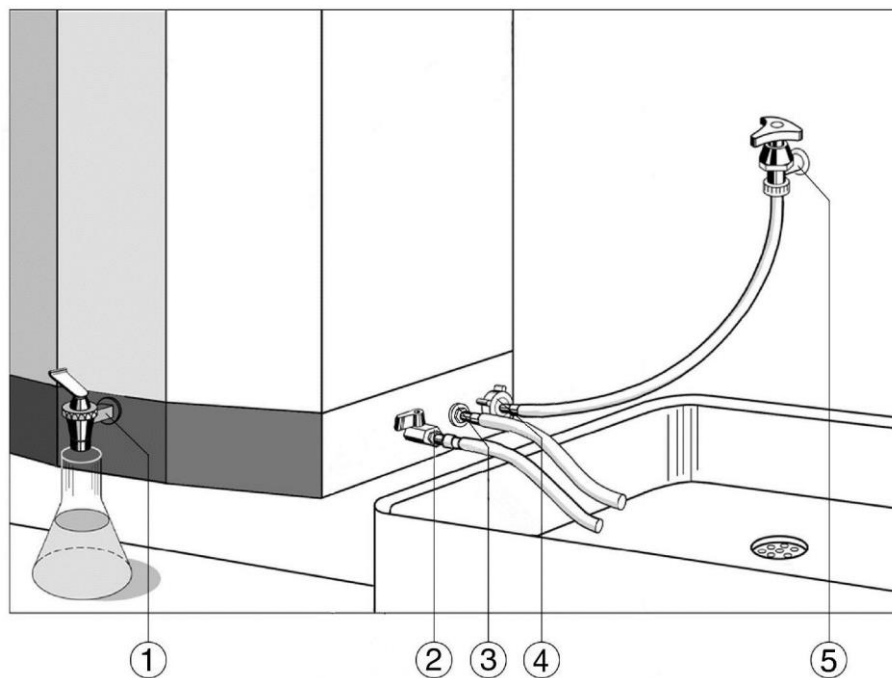

6.1 Distillate withdrawal ①

Distillate is withdrawn from the unit through the black plastic tap on the front of the unit. It can be opened in continuous or interval positions. A laboratory hose with an inner diameter of approx. 15 mm can be connected to the tap, the hose has to be secured from slipping off with a hose clip.



Caution:

The distillate leaves the Distillation Apparatus with a temperature of more than 50 °C.
Danger of scaldings!

6.2 Drain boiler ②

Connect a ½" hose to drain the boiler when cleaning the unit and/or carrying out maintenance works.



Caution:

the water leaves the boiler of the Distillation Apparatus with a temperature of up to 100 °C.
Danger of scaldings!

6.3 Cooling water outlet ③

Connect a ¾" temperature-resistant hose to the cooling water outlet. It may have a maximum length of approx. 1.5 m. It must be led into an open drain on a lower level and must have a slope on its complete length.

Make sure the cooling water can drain without back draughts.



Caution:

cooling water leaves the Distillation Apparatus with a temperature of up to 70 °C.
Danger of scaldings!

6.4 Tap water inlet ④

The tap water inlet supplies water to the Distillation Apparatus through a solenoid valve. The hose connection of the valve must be connected with the water mains through a ½" pressure hose and a blockable water connection (⑤, hand stop valve).


It is absolutely essential to use hose clips to secure both hose connections!

7 Initiation

7.1 Before initial starting

Before initial starting, the Distillation Apparatus has to be hand-filled with water. To do so, remove the outer and left-hand inner lids (marked L) as well as the deflector beneath the inner lid. Caution, when working on the deflector, make sure to observe the correct position of the wire electrode in the container. It may neither be bent nor come into contact with the housing. The boiler must now be filled with water until the heating element(s) at the bottom of the container are below water level. The deflector as well as the two individually marked inner lids must be re-assembled and safely nested on the containers before initiation of the unit.

Marking L
front of the
left-hand inner lid
(boiler)

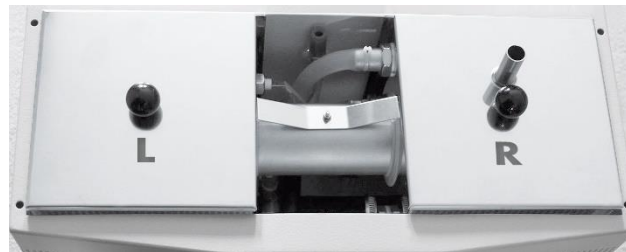

Marking R
front of the
right-hand inner lid
(storage tank)

7.2 Initiation



I II III

To initiate the Distillation Apparatus after assembly of all power and water connections, open the hand-stop valve of the water mains supply (5) and switch on the main switch (I). The first few litres of produced distillate should not be used. Discard the first two to three complete fillings of distilled water in the storage tank.



To switch off the unit for longer down-times, first switch the main switch (I) to position O, and disconnect the unit from the mains. Close the on-site hand-stop valves of the water supply, then empty and dry storage tank and boiler in order to avoid germ contamination.

8 Functional Description

LAUDA Puridest Distillation Apparatuses work automatically. After switching on the Distillation Apparatus main switch, the green pilot lamp in the main switch (I) as well as the right-hand, yellow operation pilot lamp (III) will light up. The built-in solenoid valve opens. Water flows through the cooling coil in the storage tank and a mechanical water level regulator that controls the water level in the boiler. Excess water that is not used to evaporate, runs off through the cooling water outlet. The heating elements are powered on and bring the water in the alembic to the boil. A thermostatic low water cut-off protects the heating elements from dry running. The produced steam is led through a steam tube to the cooling coil where it condenses and drips as distillate into the storage tank.

The water level in the storage tank (right-hand container) is controlled through a wire electrode. Once the container is full, the Distillation Apparatus will be switched off by an electronic controller. The solenoid valve interrupts the cooling water supply, the heating elements are switched off and the yellow pilot lamp (III) goes out. Distillate is withdrawn through the black plastic tap at the front of the unit.


After withdrawal of distillate, the unit will be switched on again automatically, so that the storage tank is refilled.

Carbon dioxide is degassed through a vent on the top of the unit.

9 Maintenance, Service and Trouble Shooting



Caution:
Prior to maintenance and service on the unit let the Distillation Apparatus cool down!
Danger of burns!

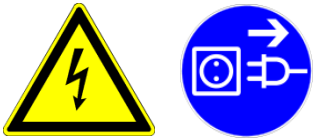

Caution:
Before opening the Distillation Apparatus as well as prior to cleaning, separate the unit from the mains supply! (Pull the plug or switch off main switch).
Danger of electrical shock!

9.1 Descaling

Depending on the degree of hardness of the tap water, the Distillation Apparatus must be cleaned regularly of scale formations. First remove the outer and the left-hand inner lids (L), then unscrew the deflector and remove it, too. A suitable descaling agent is a mixture of 10 % formic acid, 10 % acetic acid and 80 % distilled water. Fill the solvent into the boiler until it covers the topmost scale deposits and heat up to maximum approx. 70 °C. Make absolutely certain not to bring the mixture to a boil. In order to do so, close the hand-stop valve of the water mains supply ⑤ and switch on the Distillation Apparatus until the temperature is reached. After approx. 30 minutes drain the solvent and scale mixture through the drain cock "drain boiler" ② and rinse the boiler thoroughly with water several times.

Commercial descaling agents, suitable for use with stainless steel, can also be used according to the manufacturer's instructions (e.g. rea-calc® of M/s CHEMOTEC GmbH, 63486 Bruchköbel, Germany). Never use any products containing hydrochloric acid! These will lead to damages to heating element, boiler, temperature sensor and the ducts of the screw connections. Restart the unit as described in chapter 7 Initiation.

After descalings, the first few litres of distillate should not be used as it might contain traces of evaporated descaling agent. Discard the first two to three complete fillings of distilled water in the storage tank.

9.2 Pilot Lamp Clean

9.2.1 Foam formation caused by polluted water in the boiler



I II

Depending on the degree of impurities in the feed water as well as on the growing contamination of the water in the boiler, caused by the distillation process, the boiling water will foam up. Once the foam gets in contact with the electrode in the boiler (L), an electronic impurity detector will switch off the unit, and the red pilot lamp Clean (II) will light up.

The boiler must now be emptied through the drain cock "drain boiler" ② and be rinsed several times with clean water..

The operational interruption "Clean" is reset by switching the unit's main switch off and then on again. The subsequent re-initiation is to be carried out as described in chapter 7.

The "Cleaning" function's purpose is to exchange polluted water in the boiler against clean water.

9.2.2 Back water in the boiler

If the water level in the boiler rises up to the wire electrode in the left-hand container (L), the electronic impurity detector (A1 in the circuit diagram) switches the unit off and the red pilot lamp "Clean" (II) lights up. This means that more water entered the unit than could flow off. Possible causes are tubes outside the unit that are not installed as described (see chapter 6), or scale formations that cause a blockage in the water outlet tube inside the unit. A defective quantity regulator in the outlet of the solenoid valve (see cooling water requirement, chapter 11) might also cause more water to flow into the unit than can flow off. For trouble shooting purposes, an additional function drawing of the internal water flow is available on request.

9.3 Re-initiation after low water



To re-initiate, let the unit cool down and fill in water to cover the heating elements as described in chapter 7 Initiation.

The triggered low water cut-off must be reset. To do so, loosen the black cap nut at the bottom left-hand side of the Distillation Apparatus. Inside the thread a small white plastic pin can be seen that has to be gently pressed inside (e.g. with a pen) until a clicking sound can be heard.

Only then switch the unit back on again.

The LAUDA Puridest Distillation Apparatus is made of first-class material. Nevertheless, the unit should only be subjected to mechanical strain within sensible limits.

9.4 Technical support

You can call our customer service at any time for technical support relating to LAUDA Puridest Distillation Apparatuses appliances.

Phone : +49 (0) 9343 / 503-350

Fax : +49 (0)9343 503-283

Email : service@lauda.de

Maintenance, repairs and modifications must be carried out by a qualified electrician (section 2 (3) DGUV Regulation 3) according to the General Rules of Technology (section 2 (2) DGUV Regulation 3). Only original spare parts may be used. Request that the person performing the work provides written confirmation of the type and scope of the work carried out (company, date, signature).

10 Disposal of Old Units

LAUDA will take responsibility, within the scope of the legal directives, for an environmentally sound handling and disposal of all used LAUDA units as of the production year 1995 that are returned to us free of charge and will have it materially recycled. Before the unit is returned, a legally binding declaration must be provided from the sender confirming that the unit is free from harmful and/or hazardous contaminations as well as from hazardous substances caused by the previous use of the unit.

LAUDA laboratory apparatus are exclusively designed for industrial use and may not be disposed of through public waste disposal authorities.

EAR Registration Number WEEE-ID.NO.DE 67770231

11 Technical Data

11.1 Distillation Apparatus Puridest models PD 2 R, PD 4 R

	PD 2 R	PD 4 R
Exterior dimensions (W x D x H)	530 mm x 280 mm x 455 mm	615 mm x 320 mm x 495 mm
Storage tank	4 litres distillate	8 litres distillate
Distillation capacity	2 l / h distillate	4 l / h distillate
Distillate quality	Mono distillate approx. 2.3 $\mu\text{S} / \text{cm}$ at 25 °C in conformity with DAB, bacteria and pyrogen free, low gas content	Mono distillate approx. 2.3 $\mu\text{S} / \text{cm}$ at 25 °C in conformity with DAB, bacteria and pyrogen free, low gas content
<p>The conductivity of the distilled water is directly related to the chemical composition of the raw water. Components of the raw water having the same or a lower evaporation point than water may deteriorate the conductivity.</p>		
Cooling water requirement	30 l / h	48 l / h
Low water cut-off	Electromechanical temperature limiter, with capillary tube sensor. Switch-off temperature 135 °C / -15 K	Electromechanical temperature limiter, with capillary tube sensor. Switch-off temperature 135 °C / -15 K
Water pressure min. / max.	> 3 bar / 7 bar > 43.5 psi / 101.5 psi	> 3 bar / 7 bar > 43.5 psi / 101.5 psi
Electrical connection	230 V +/- 10 %,	230 V +/- 10 %,
Mains supply	50 / 60 Hz, 1.5 kW shock-proof plug	50 / 60 Hz, 3.0 kW shock-proof plug
<p>Caution! Mains voltage deviations, even with the mentioned limits, influence the quantity of distillate produced.</p>		
Fuses		
On-site fuse	16 Amp.	16 Amp.
Internal mains fuse	10 Amp. T	16 Amp. T
Protection class / - type	I / IP20	I / IP20
Surrounding conditions	Use only inside buildings (not in potentially explosive areas).	Use only inside buildings (not in potentially explosive areas).
Height above MSL	up to 2000 m MSL	up to 2000 m MSL
Ambient temperature	+10 °C to +40 °C	+10 °C to +40 °C
Humidity	max. 80 % rel. humidity to 31 °C, decreasing to 40 % rel. humidity at 40 °C	max. 80 % rel. humidity to 31 °C, decreasing to 40 % rel. humidity at 40 °C
Net Weight	16.0 kg	21.8 kg
Weight with water filling	22.0 kg	32.4 kg


11.2 Distillation Apparatus Puridest models PD 8 R, PD 12 R

	PD 8 R	PD 12 R
Exterior dimensions (W x D x H)	780 mm x 405 mm x 575 mm	780 mm x 405 mm x 705 mm
Storage tank	16 litres distillate	24 litres distillate
Distillation capacity	8 l / h distillate	12 l / h distillate
Distillate quality	Mono distillate approx. 2.3 $\mu\text{S} / \text{cm}$ at 25 °C in conformity with DAB, bacteria and pyrogen free, low gas content	Mono distillate approx. 2.3 $\mu\text{S} / \text{cm}$ at 25 °C in conformity with DAB, bacteria and pyrogen free, low gas content
<p>The conductivity of the distilled water is directly related to the chemical composition of the raw water. Components of the raw water having the same or a lower evaporation point than water may deteriorate the conductivity.</p>		
Cooling water requirement	72 l / h	198 l / h
Low water cut-off	Electromechanical temperature limiter, with capillary tube sensor. Switch-off temperature 135 °C / -15 K	Electromechanical temperature limiter, with capillary tube sensor. Switch-off temperature 135 °C / -15 K
Water pressure min. / max.	> 3 bar / 7 bar > 43.5 psi / 101.5 psi	> 3 bar / 7 bar > 43.5 psi / 101.5 psi
Electrical connection	230 V +/- 10 %, 50 / 60 Hz, 6.0 kW	220 V / 3 ~ / PE +/- 10 %, 50 / 60 Hz, 9.0 kW
Mains supply	Connection box for permanent connection to the mains Netzsicherung / on-site-fuse 35 Amp.	Mains connection cable for permanent connection to the mains / on-site-fuse 3 x 25 Amp.
On-site fuse	220 V / 3 ~ / PE +/- 10 %, 50 / 60 Hz, 6.0 kW Mains connection cable for permanent connection to the mains / on-site-fuse 3 x 16 Amp. 400 V / 3 ~ / N / PE +/- 10 %, 50 / 60 Hz, 6.0 kW Mains connection cable for permanent connection to the mains / on-site-fuse 3 x 16 Amp.	400 V / 3 ~ / N / PE +/- 10 %, 50 / 60 Hz, 9.0 kW Mains connection cable for permanent connection to the mains / on-site-fuse 3 x 16 Amp.
<p>Caution! Mains voltage deviations, even with the mentioned limits, influence the quantity of distillate produced.</p>		
Protection class / - type	I / IP20	I / IP20
Surrounding conditions	Use only inside buildings (not in potentially explosive areas).	Use only inside buildings (not in potentially explosive areas).
Height above MSL	up to 2000 m MSL	up to 2000 m MSL
Ambient temperature	+10 °C to +40 °C	+10 °C to +40 °C
Humidity	max. 80 % rel. humidity to 31 °C, decreasing to 40 % rel. humidity at 40 °C	max. 80 % rel. humidity to 31 °C, decreasing to 40 % rel. humidity at 40 °C
Net Weight	35.8 kg	40.9 kg
Weight with water filling	56.5 kg	70.4 kg


12 Circuit Diagram

A1	Electronic level switch
E1	Tubular heating element
E2	Tubular heating element
E3	Tubular heating element
H1	LED red "cleaning"
H2	LED yellow "operation"
Elektr. 1	Electrode "cleaning in boiler"
Elektr. 2	Electrode "water blocking"
Elektr. 3	Electrode "max. level storage tank"
F1	Mains fuse internal, Model PD 2 R, 10 Amp. inert
	Model PD 4 R, 15 Amp. inert
F2	Mains fuse internal, Model PD 2 R, 8 Amp. inert
	Model PD 4 R, 15 Amp. inert
F3	Low water cut-off (thermostat)
K1	Contactor
M	Earth (housing)
S1	Main switch
Y1	Solenoid valve


12.1 PD 2 R

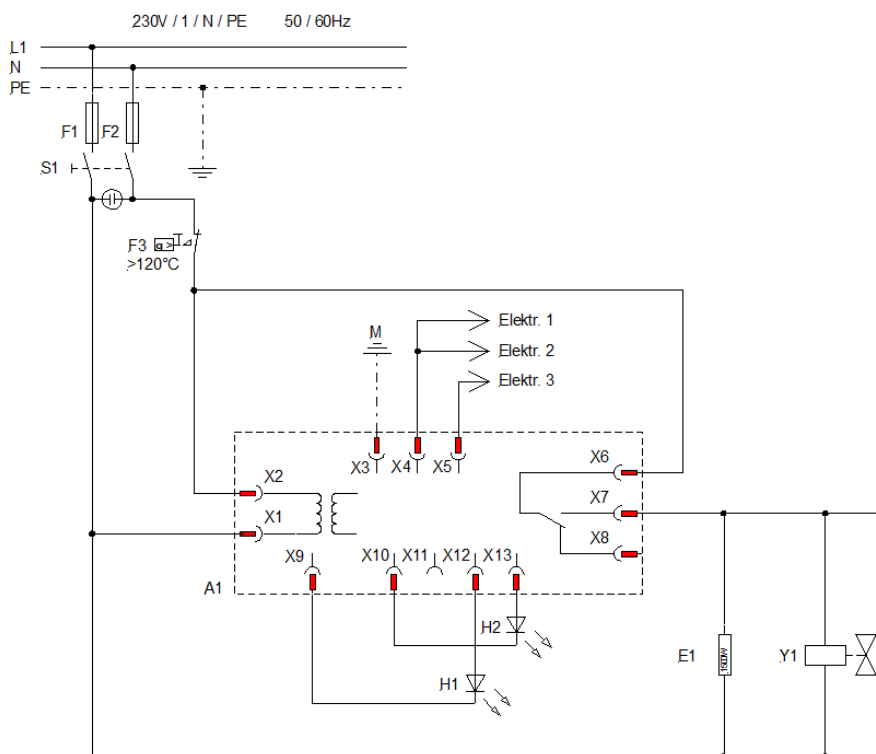


12.2 PD 4 R

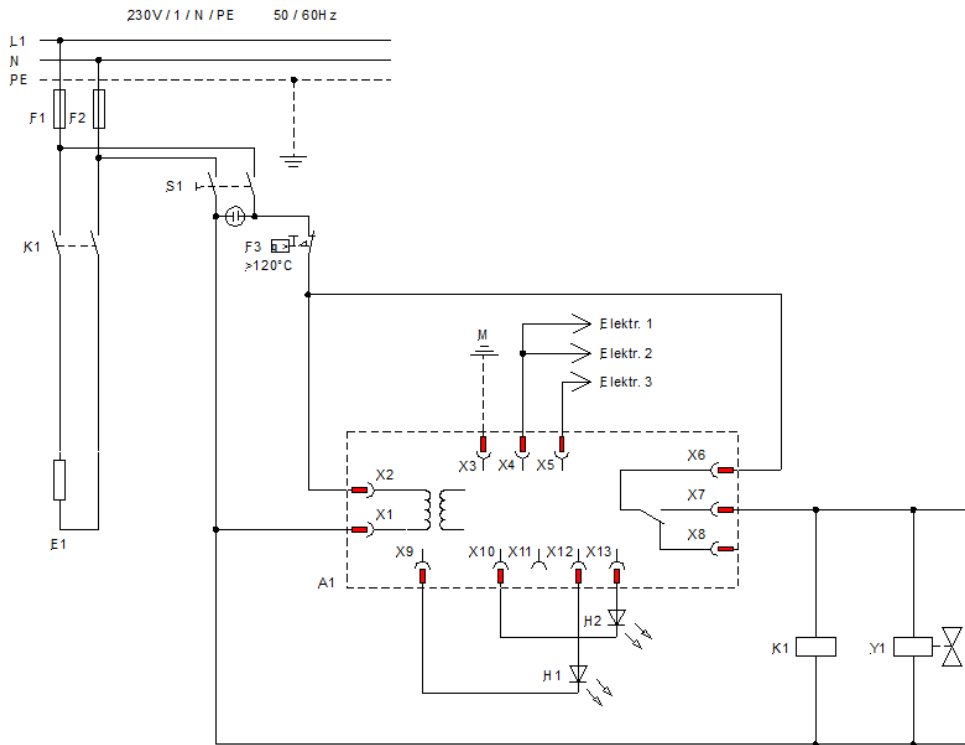


12.3 PD 8 R - version 230 V / 1 ~ for permanent connection to the mains (see nameplate)

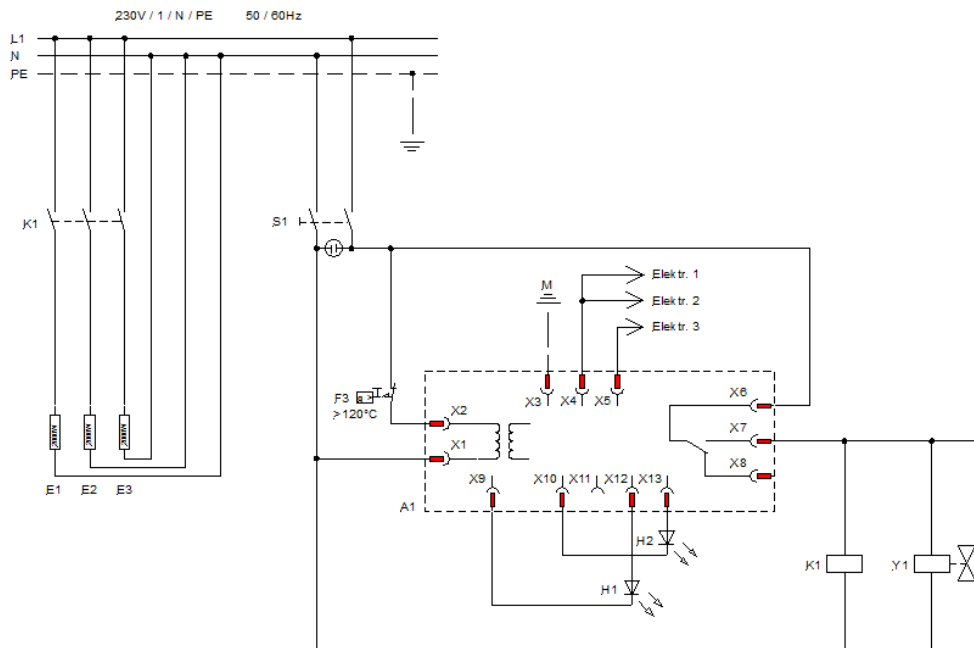

12.4 PD 8 R / PD 12 R - version 220 V / 3 ~ for permanent connection to the mains
 (see nameplate)

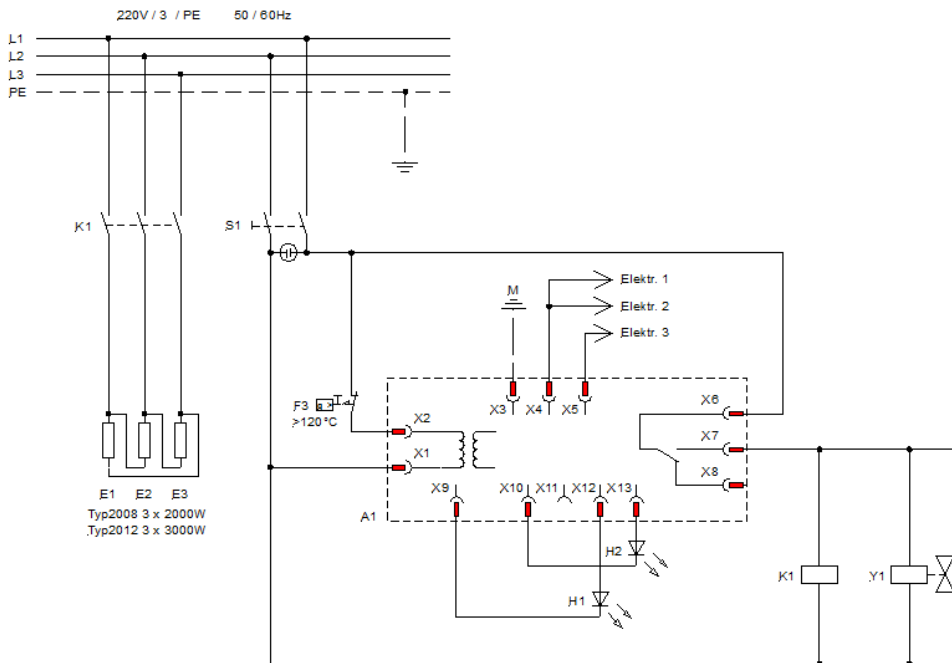

12.5 PD 8 R / PD 12 R - version 400 V / 3 ~ for permanent connection to the mains
 (see nameplate)

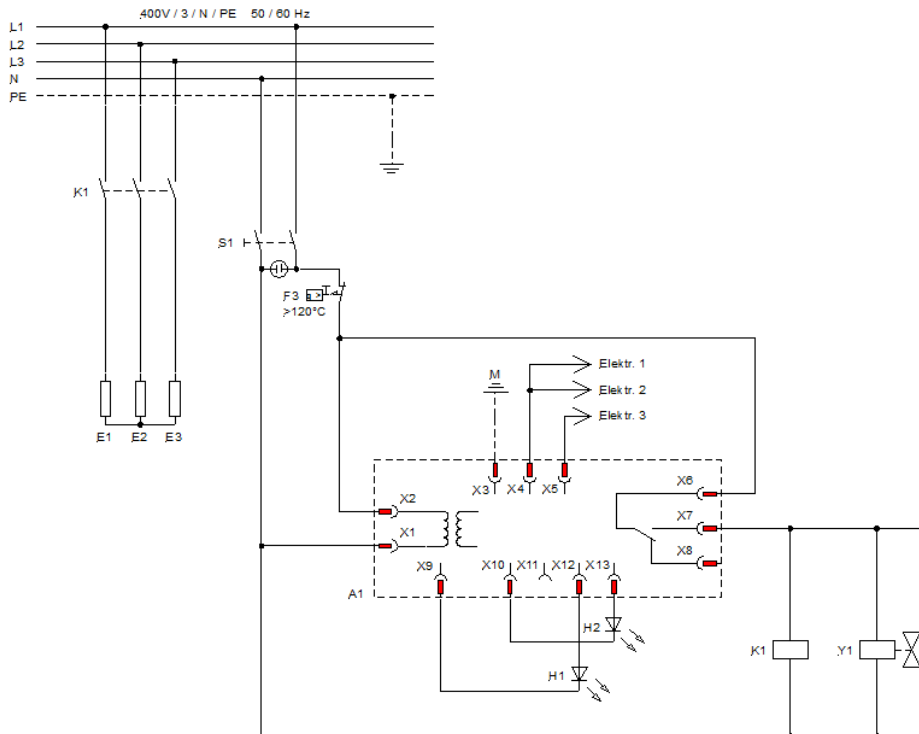

13 Connection to the Mains

The electrical connection must ensure an all-pole separation from the mains supply. Installed assembly parts, such as shock-proof sockets or main switches, must be installed so as to ensure clear identification and they must be within easy reach in an emergency case. Distillation Apparatus models PD 8 R and PD 12 R must have a permanent connection with the mains. This may only be implemented through an on-site main switch or through a CEE plug in conformity with IEC standard 60309-2 (see examples for connection to the mains in chapter 13.1).

Colour decoding of the individual leads of the mains connection cables for models PD 8 R and PD 12 R:

Colour decoding	Mains supply	
	220 V / 3 ~ / PE 50 / 60 Hz	400 V / 3 ~ / N / PE 50 / 60 Hz
ge/gr – gelb/grün	PE (Protective earth)	PE (Protective earth)
bl – blue		N
sw – black	L1	L1
br – brown	L2	L2
gra – grey	L3	L3

Distillation Apparatuses can be supplied in different versions for connection to different mains supplies.

Models PD 2 R and PD 4 R for connection to 230 V (see nameplate) can be connected to all mains supplies with 220 V or 230 V.

Models PD 8 R and PD 12 R for connection to 220 V / 3 ~ (see nameplate) can only be connected to mains supplies with 220 V / 3. ~ / PE.

Models PD 8 R and PD 12 R for connection to 400 V / 3 ~ (see nameplate) can only be connected to mains supplies with 400 V / 3. ~ / N / PE.

Electrical fuses

Model	Power	Power consumption at mains voltage *	Mains fuse (F2–F4)
PD 2 R	1.5 kW	6.5 A at 230 V	10 Amp
PD 4 R	3.0 kW	13.0 A at 230 V	16 Amp
PD 8 R	6.0 kW	26.1 A at 230 V	35 Amp
	6.0 kW	15.8 A at 220 V / 3 ~ / PE	16 Amp
	6.0 kW	8.7 A at 400 V / 3 ~ / N / PE	10 Amp
PD 12 R	9.0 kW	23.6 A at 230 V / 3 ~ / PE	25 Amp
	9.0 kW	13.0 A at 400 V / 3 ~ / N / PE	16 Amp

* see nameplate


13.1 Examples for connection to the mains supply

Components

- B1 Shock-proof socket (on-site)
- B2 Shock-proof plug (mounted on the unit)
- B3 CEE plug, not mounted, in conformity with IEC standard 60309-2
- B4 Connection box, mounted on the unit
- F2 Mains fuse (on-site)
- F3 Mains fuse (on-site)
- F4 Mains fuse (on-site)
- S4 Main switch (on-site)

13.1.1 PD 2 R and PD 4 R for 230 V for a mains supply of 220 V / 3 ~ / PE / 50 / 60 Hz

(see nameplate)

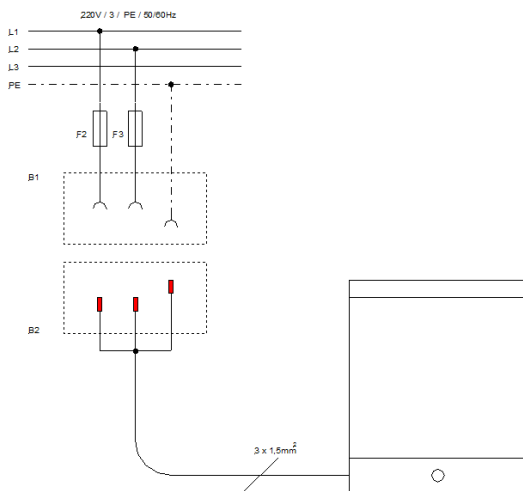


PD 2 R and PD 4 R

Mains connection through shock-proof plug CEE 7/7 (pre-assembled), all-pole separable from the mains.

13.1.2 PD 2 R / PD 4 R for 230 V for a mains supply of 400 V / 3 ~ / N / PE / 50 / 60 Hz

(see nameplate)

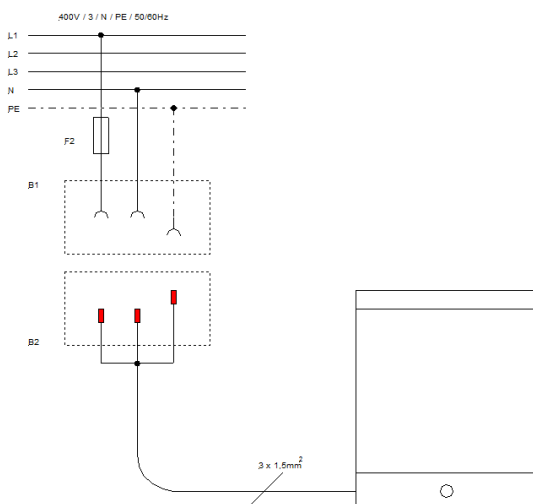


PD 2 R and PD 4 R

Mains connection through shock-proof plug CEE 7/7 (pre-assembled), all-pole separable from the mains.

13.1.3 PD 8 R for 230 V / 1 ~ for a mains supply of 220 V / 3 ~ / PE / 50 / 60 Hz

(see nameplate)

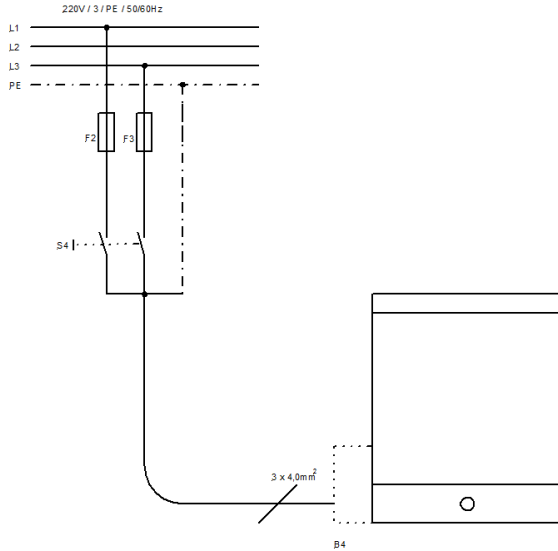


PD 8 R

Mains connection through on-site switch S4, all-pole separable from the mains. Connection cable not in scope of supply.

13.1.4 PD 8 R for 230 V / 1 ~ for a mains supply of 400 V / 3 ~ / N / PE / 50 / 60 Hz


(see nameplate)

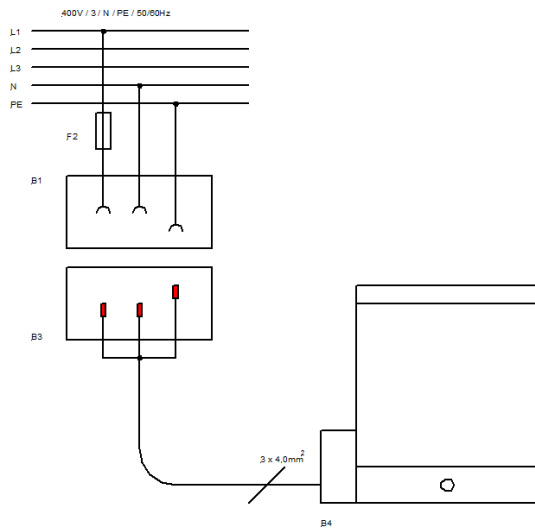

PD 8 R


Mains connection through CEE plug in conformity with IEC standard 60309-2, all-pole separable from the mains. Connection cable and CEE plug not in scope of supply.

13.1.5 PD 8 R and PD 12 R for 220 V / 3 ~ for a mains supply of 220 V / 3 ~ / PE / 50 / 60 Hz
 (see nameplate)

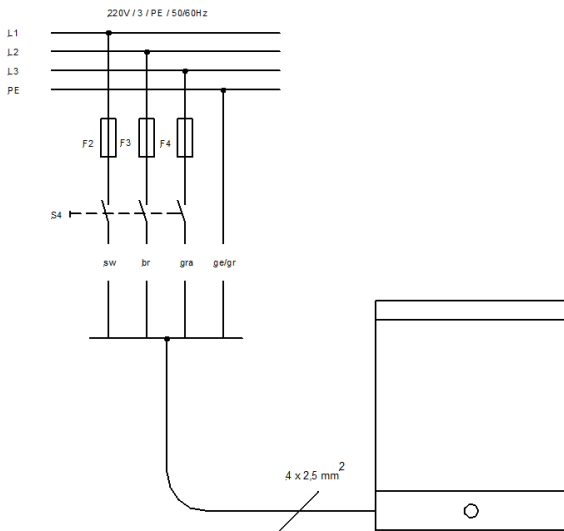


PD 8 R, PD 12 R
 Mains connection through on-site switch S4, all-pole separable from the mains.

13.1.6 PD 8 R and PD 12 R for 220 V / 3 ~ for a mains supply of 220 V / 3 ~ / PE / 50 / 60 Hz
 (see nameplate)

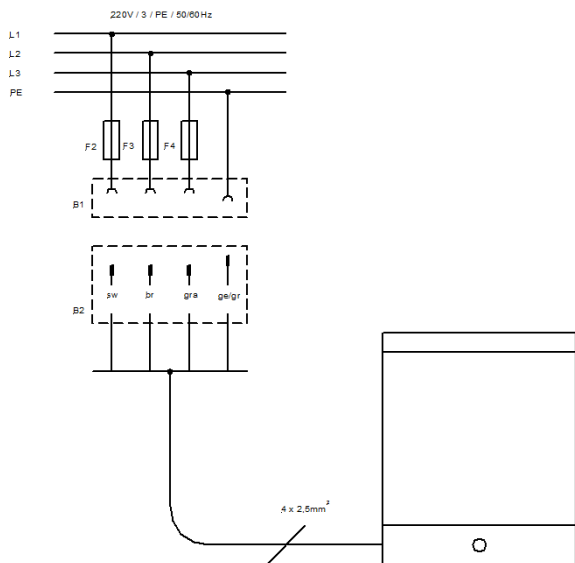

PD 8 R, PD 12 R
 Mains connection through CEE plug in conformity with IEC standard 60309-2 (plug not pre-assembled), all-pole separable from the mains.


13.1.7 PD 8 R and PD 12 R for 400 V / 3 ~ for a mains supply of 400 V / 3 ~ / N / PE 50 / 60 Hz
(see nameplate)

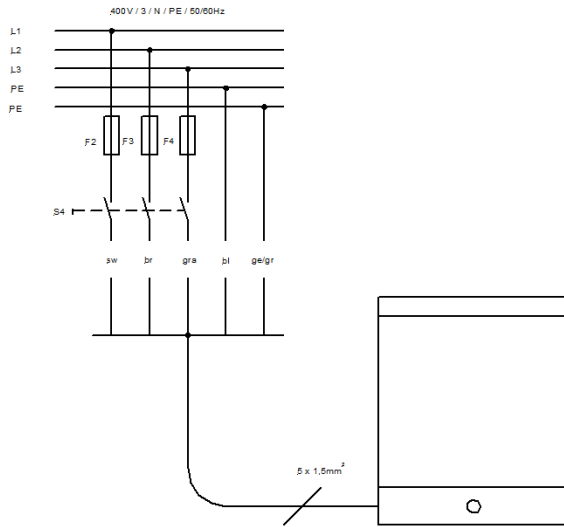

PD 8 R, PD 12 R

Mains connection through on-site switch S4, all-pole separable from the mains.

13.1.8 PD 8 R and PD 12 R for 400 V / 3 ~ for a mains supply of 400 V / 3 ~ / N / PE 50 / 60 Hz
(see nameplate)

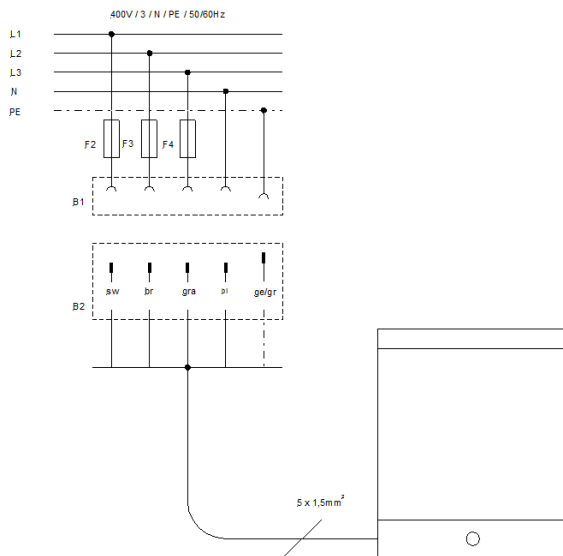

PD 8 R, PD 12 R

Mains connection through CEE plug in conformity with IEC standard 60309-2 (plug not pre-assembled), all-pole separable from the mains.

14 Accessories and Options

Separate Water Supply, to feed the boiler with softened or desalinated water (pressure > 1 bar / 14.5 psi) and the cooling coil with phosphatised or normal tap water (pressure > 3 bar / 43.5 psi). Accessory must be installed in our works. When a separate water supply is installed, the hourly capacity of distilled water is reduced by approx. 10-15 %.

Separate Water Supply

Only factory installation into models PD 2 R to PD 12 R is possible.

When the storage is full, the inlet of pretreated water is not automatically switched off. Part-No. is depending on the Model of the Distillation Apparatus (without illustration).

Separate Water Supply with solenoid valve

Only factory installation into models PD 2 R to PD 12 R is possible.

When the storage tank is full, the solenoid valve switches off pretreated water automatically. Part-No. is depending on the Model of the Distillation Apparatus (without illustration).

Dechlorite Filter, eliminates chlorine particles in tap water added by the local waterworks. Complete with connections for pressure hose ½ inch, with first filling.



Dechlorite-Filter
Part-No. A000129



Spare filling
Part-No. A000130

Phosphate cartridge, prevents scale formation in the condenser by phosphatising of tap water. Can be used from 4 to 15 °dH (German hardness), equivalent to approx. 0.7 to 2.7 mMol / l. With connection for pressure hose ½ inch, with first filling.



Phosphate cartridge
Part-No. A000131



Spare filling
Part-No. A000132

Pre-Filter 1 µm, for pre-cleaning the tap water, and to protect the unit from premature contamination. Complete with connections for pressure hose ½" (inner diameter 12.7 mm), including filter candle. The candle should be replaced at least every six months.



Pre-Filter with candle
Part-No. A000133



Spare candle
Part-No. A000134

Wall bracket, for one filter or for filter combinations of two or three filters, including sleeves to connect the filters as well as screws to fix the filters to the wall bracket.

A data sheet on possible connection variants of articles A000129, A000131 and A000133 can be supplied on request.



Wall bracket for one filter
Part-No. A000136



Set of all 3 filters, incl. wall bracket
and fillings, mounted completely
Part-No. A000135

Hose Set, consisting of hoses for water inlet and outlet (length 1.5 m), including hose clips.



Hose Set
Part-No. A000138

Level Control Switch

Only factory installation into models PD 2 R to PD 12 R is possible.

When connecting an external storage tank (not included in the scope of supply) to the Distillation Apparatus, it is recommended to equip the unit with a Level Control Switch which controls the water level in the external storage tank and switches off power and water when the external storage tank is full. When using an external storage tank in connection with Level Control Switch, the internal storage tank is only usable to a limited extent due to different levels of the internal and external tanks. Part-No. is depending on the Model of the Distillation Apparatus.



Level Control Switch

16 Ordering spare parts / LAUDA Service

When ordering spare parts, please state the serial number (type plate) to avoid queries and wrong deliveries.

Your partner for maintenance and competent service support:

LAUDA Service
Phone: +49 (0)9343 503-350
Fax: +49 (0)9343 503-283
Email: service@lauda.de

We are always at your disposal for questions and suggestions!

LAUDA DR. R. WOBSE GMBH & CO. KG
Laudaplatz 1
97922 Lauda-Königshofen
Germany
Phone: +49 (0)9343 503-0
Fax: +49 (0)9343 503-222
Email info@lauda.de
Internet: <http://www.lauda.de/>

17 Product Returns and Clearance Declaration



Product Returns and Clearance Declaration

Product Returns

Would you like to return a LAUDA product you have purchased to LAUDA? For the return of goods, e.g. for repair or due to a complaint, you will need the approval of LAUDA in the form of a *Return Material Authorization (RMA)* or *processing number*. You can obtain the RMA number from our customer service department at +49 (0) 9343 503 350 or by email service@lauda.de.

Return address

LAUDA DR. R. WOBSEY GMBH & CO. KG

Laudaplatz 1

97922 Lauda-Königshofen

Deutschland/Germany

Clearly label your shipment with the RMA number. Please also enclose this fully completed declaration.

RMA number	Product serial number
Customer/operator	Contact name
Contact email	Contact telephone
Zip code	Place
Street & house number	
Additional explanations	

Clearance Declaration

The customer/operator hereby confirms that the product returned under the above-mentioned RMA number has been carefully emptied and cleaned, that any connections have been sealed to the farthest possible extent, and that there are no explosive, flammable, environmentally hazardous, biohazardous, toxic, radioactive or other hazardous substances in or on the product.

Place, date	Name in block letters	Signature



EC DECLARATION OF CONFORMITY

Manufacturer: LAUDA DR. R. WOBSEY GMBH & CO. KG
Schulze-Delitzsch-Straße 4+5, 30938 Burgwedel, Germany

We hereby declare under our sole responsibility that the machines described below

Product Line: Puridest **Serial number:** from 220_____

Types: PD 2, PD 4,
PD 2 D, PD 4 D, PD 8 D,
PD 2 G, PD 2 DG, PD 4 G, PD 4 DG, PD 8 G,
PD 2 R, PD 4 R, PD 8 R and PD 12 R

comply with all relevant provisions of the EC Directives listed below due to their design and type of construction in the version brought on the market by us:

Machinery Directive	2006/42/EC
EMC Directive	2014/30/EU
RoHS Directive	2011/65/EU in connection with (EU) 2015/863

The protective objectives of the Machinery Directive with regard to electrical safety are complied with in accordance with Annex I Paragraph 1.5.1 in conformity with the Low Voltage Directive 2014/35/EU.

Applied standards:

- EN 61326-1:2013
- EN 61010-1:2010/A1:2019/AC:2019-04
- EN IEC 61010-2-010:2020

Authorized representative for the composition of the technical documentation:

Dr. Jürgen Dirscherl, Head of Research & Development

Burgwedel, 05.06.2023

Dr. Alexander Dinger,
Head of Quality and Environmental Management

LAUDA DR. R. WOBSE GMBH & CO. KG

Schulze-Delitzsch-Straße 4+5 ° 30938 Burgwedel ° Germany

Phone.: +49 (0) 5139 9958-0 ° Fax +49 (0) 5139 9958-21

Email: info@lauda.de ° Internet: <https://www.lauda.de>