

**RT<sup>®</sup>ED**  
**SUTURE**



**山东海迪科医用制品有限公司**  
SHANDONG HAIDIKE MEDICAL PRODUCTS CO.,LTD.

Add: Plant No. 1, Science and Technology Enterprise Incubator Park,  
Shan County, Heze City, Shandong Province, China  
Tel: +86-530-4660062  
Fax: +86-530-4660055  
Mobile: +86-13105409308  
E-mail: [info@suturescn.com](mailto:info@suturescn.com)  
Web: [www.suturescn.com](http://www.suturescn.com)




**SHANDONG HAIDIKE MEDICAL PRODUCTS CO.,LTD.**

山东海迪科医用制品有限公司

Shandong Haidike Medical Products Co., Ltd. is a leading and world famous medical devices manufacturer with CE, ISO, FSC, CFDA and FDA certificates. RTMED has registered as Madrid trademark. We have established good cooperation with Tsinghua University and Shandong Academy of Sciences, having great R & D center and research team. Our products are sold in over 100 countries.

- ◆ Absorbable surgical sutures approved by CE certificate
- ◆ NO.1 catgut suture plant in the world
- ◆ Lifting Threads for Beauty, Cosmetic
- ◆ Orthopedic casting tapes & splints
- ◆ Medical protection products
- ◆ Electric Wheelchair & Manual Wheelchair
- ◆ Pet Food, Vet Suture

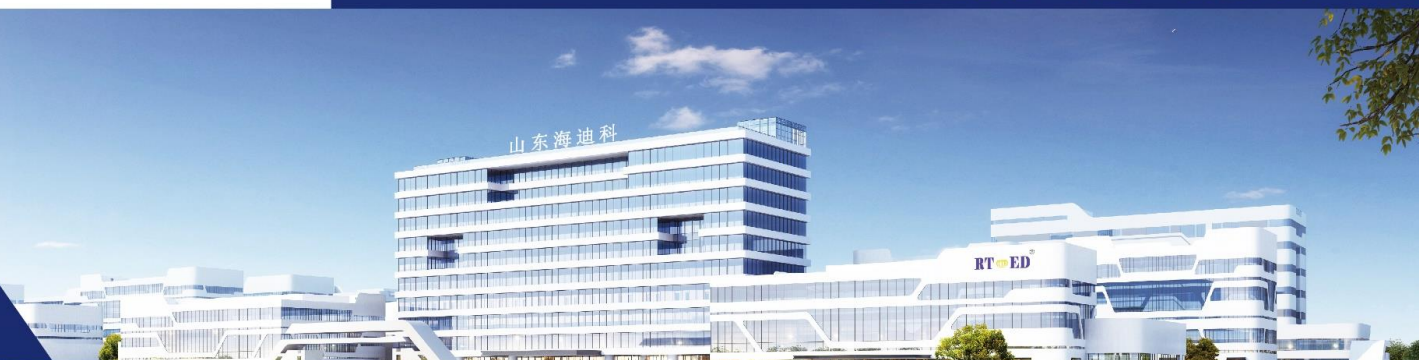

BUSINESS LICENSE



MEDICAL DEVICE PRODUCTION LICENSE



SGS AND ALIBABA JOINT CERTIFICATION



CE CERTIFICATE FOR SURGICAL SUTURE



CE CERTIFICATES FOR VARIOUS PROTECTIVE PRODUCTS



BANDAGE SPLINT MEDICAL CONSUMABLES FDA CERTIFICATE




BANDAGE SPLINT MEDICAL CONSUMABLES FDA CERTIFICATE



U.S. FOOD & DRUG ADMINISTRATION



SURGICAL SUTURE ISO13485 CERTIFICATE



MADRID TRADEMARK



### Needle Shapes



### Advantages

- 1 Strong Hardness
- 2 Outstanding Sharpness
- 3 Excellent Tenacity And Ductility

- Round bodied (heavy)
- ▲ Curved cutting (heavy)
- ▼ Reverse cutting (heavy)
- ⊙ Taper cutting
- ⊙ Microfine spatula curved
- Blunt point
- Straight round bodied
- ▲ Straight curved cutting



## PGA POLYGLYCOLIC ACID

### Properties:

Structure: Multifilament, Braided  
 Colour: Violet, Undyed  
 Chemical composition: Polyglycolic acid  
 Coating: Polycaprolactone + Calcium Stearate  
 Sizes: USP 8/0 - USP 4  
 Type of absorption: Hydrolysis  
 Sterilization: Ethylene Oxide  
 Absorption: 60 - 90 days

### Advantages:

- High initial tensile strength
- Excellent knotting ability
- Reliable absorbability
- Easy to handle
- Outstanding holding power through the critical wound periode
- Smooth surface, slides smoothly through the tissue



## PGLA POLYGLACTIN 910

### Properties:

Structure: Multifilament, Braided  
 Colour: Violet, Undyed  
 Chemical composition: Poly(glycolide-co-l-lactide 90/10)  
 Coating: Poly(glycolide-co-l-lactide 30/70) + Calcium Stearate  
 Sizes: USP 8/0 - USP 2  
 Type of absorption: Hydrolysis  
 Sterilization: Ethylene Oxide  
 Absorption: 56 - 70 days

### Advantages:

- High tensile strength
- Smooth tissue passage
- Easy knotting and tie down
- Excellent knot security
- Reliable absorbability



## PDO POLYDIOXANONE

### Properties:

Structure: Monofilament  
 Colour: Violet, Undyed  
 Chemical composition: Poly (p-dioxanone)  
 Sizes: USP 7/0 - USP 2  
 Type of absorption: Hydrolysis  
 Sterilization: Ethylene Oxide  
 Absorption: 180 - 210 days

### Advantages:

- High initial tensile strength
- Prolonged wound support
- Minimal tissue reaction
- Lower incidence of infection and trauma due to smooth surface




## PGCL POLIGLECAPRONE 25

### Properties:

Structure: Monofilament  
 Colour: Violet, Undyed  
 Chemical composition: Poly (glycolide-co-caprolactone)  
 Sizes: USP 6/0 - USP 2  
 Type of absorption: Hydrolysis  
 Sterilization: Ethylene Oxide  
 Absorption: 90 - 120 days

### Advantages:

- High initial tensile strength
- Easy handling
- Smooth passage through tissue
- Excellent knotting ability






## CHROMIC CATGUT

### Properties:

Colour: Dark brown  
Composition: Purified connective tissue  
Sizes: USP 7/0 - USP 4  
Type of absorption: Proteolysis  
Sterilization: Gamma radiation  
Absorption: 90 - 100 days

### Advantages:

- High tensile strength
- Excellent handling properties
- Minimal tissue reaction
- Uniform absorption



## PLAIN CATGUT

### Properties:

Colour: Beige  
Composition: Purified connective tissue  
Sizes: USP 7/0 - USP 4  
Type of absorption: Proteolysis  
Sterilization: Gamma radiation  
Absorption: 60 - 70 days

### Advantages:

- High tensile strength
- Smooth tissue passage
- Easy knotting and tie down
- Excellent knot security
- Reliable absorbability



## SILK

### Properties:

Structure: Braided  
Colour: Black, White  
Composition: Natural silk filaments  
Coating: Silicon / wax  
Sizes: USP 8/0 - USP 4  
Sterilization: Ethylene Oxide

### Advantages:

- Excellent handling properties
- High tensile strength
- Highly smooth and flexible
- Good knot security




## POLYPROPYLENE

### Properties:

Structure: Monofilament  
Colour: Blue  
Chemical composition: Polypropylene  
Sizes: USP 7/0 - USP 3  
Sterilization: Ethylene Oxide

### Advantages:

- High tensile strength
- Smooth tissue passage
- Easy and secure knotting
- Minimal acute inflammatory reaction in tissues
- Excellent and permanent tissue support



## NYLON

### Properties:

Structure: Monofilament  
 Colour: Blue, Black  
 Chemical composition: polyamide 6 - 6.6  
 Sizes: USP 12/0 - USP 4  
 Sterilization: Ethylene Oxide

### Advantages:

- High tensile strength
- Smooth tissue passage
- Easy and secure knotting
- Excellent and permanent tissue support



## POLYESTER

### Properties:

Structure: Braided  
 Colour: Green, White  
 Chemical composition: Polyethylene terephthalate  
 Coating: Silicon  
 Sizes: USP 6/0 - USP 4  
 Sterilization: Ethylene Oxide

### Advantages:

- High tensile strength
- Excellent handling properties
- Minimal tissue reaction
- Good knot security



## THREADS

## NEEDLES

	THREADS TYPE		THREADS DIAMETER		THREADS LENGTH			
	THREADS TYPE		THREADS DIAMETER		THREADS LENGTH			
ABSORBABLE	POLYGLYCOLIC ACID (size: 5-8/0)	PGA	10/0	10	15cm	A	1/2 circle round bodied	01
	POLYGLYCOLIC ACID RAPID (size: 5-8/0)	PGAR	9/0	90	30cm	B	3/8 circle round bodied	02
	POLYGLYCOLIC ACID PLUS (size: 5-8/0)	PGA+	8/0	80	45cm	C	1/2 circle curved cutting	03
	POLYGLACTIN 910 (size: 2-8/0)	PGLA	7/0	70	60cm	D	3/8 circle curved cutting	04
	POLYGLYGLACTIN 910 RAPID (size: 2-8/0)	PGLAR	6/0	60	70cm	E	1/2 circle reverse cutting	05
	POLYGLYGLACTIN 910 PLUS (size: 2-8/0)	PGLA+	5/0	50	75cm	F	3/8 circle reverse cutting	06
	POLYDIOXANONE (size: 2-7/0)	PDO	4/0	40	90cm	G	straight round bodied	07
	POLYDIOXANONE RAPID (size: 2-7/0)	PDOR	3/0	30	100cm	H	straight curved cutting	08
	POLYDIOXANONE PLUS (size: 2-7/0)	PDO+	2/0	20	125cm	I	1/2 circle taper cutting	09
	CHROMIC CATGUT (size: 4-7/0)	CC	0	00	150cm	J	3/8 circle taper cutting	10
	PLAIN CATGUT (size: 4-7/0)	PC	1	01	180cm	K	blunt point	11
	POLIGLECAPRONE 25 (size: 2-6/0)	PGCL	2	02	200cm	L	1/2 circle spatula curved	12
	POLIGLECAPRONE 25 RAPID (size: 2-6/0)	PGCLR	3	03	250cm	M	3/8 circle spatula curved	13
	POLIGLECAPRONE 25 PLUS (size: 2-6/0)	PGCL+	4	04	300cm	N	1/4 circle round bodied	14
					400cm	O	1/2 circle round bodied heavy	15
					50cm	P	without needle	16
NON-ABSORBABLE	SILK (size: 4-6/0)	SK					double needle	-2
	NYLON (size: 4-12/0)	NL						
	POLYPROPYLENE (size: 3-7/0)	PP						
	POLYESTER (size: 4-7/0)	PB						

PGA 20 F 01 -2

PGA20F0126-2

Polyglycolic Acid 2/0 75mm 1/2 circle round bodied double needles 26mm

## Lifting Threads Needle

### SHARP



Basic type, generally used for linear filling and simple lifting, Beginners can also operate effortlessly.

### L TYPE



L type blunt needle, reduce the damage of blood vessels, bruising and hematoma. The pain was significantly reduced.

### W TYPE



Circular head, reducing the damage to the skin tissue. After the injection, the needle can be taken out then correct the position and depth of the needle, which improves the lack of a stitch of the other types.

### U-COG



Double needle is used for eyebrow lifting and other parts requiring strong lifting. U-COG is a special structure line with strong lifting ability. The local lifting effect is almost as good as the little facelift.

## PDO/PCL Lifting Thread



### Mono

**Needle** Sharp Needle

**Parts** Face, Body

**Effects** Tightening, Filling, Wrinkles Removing, Whitening



### Tornado Screw

**Needle** Sharp Needle

**Parts** Eye, Neck, Crow's Feet, Cheek

**Effects** Tightening, Filling, Whitening, Wrinkles Removing



### KONK

**Needle** L type Blunt Needle

**Parts** Nasal columella, Nasal bridge

**Effects** Rhinoplasty, Nose Shaping



### COG Lifting

**Needle** L/W type Blunt Needle

**Parts** Lifting Eyebrow, Apple Zone, Cheek, Chest

**Effects** Face Lifting, V Face, Chest Lifting



### Multi Threads

**Needle** L type Blunt Needle

**Parts** Face, Neck, Eye Bag, Crow's Feet

**Effects** Tightening, Filling, Whitening, Wrinkles Removing



### Molding COG

**Needle** W type Blunt Needle

**Parts** Face, Neck, Crow's Feet, Eye Bag

**Effects** Tightening, Filling, Whitening, Wrinkles Removing



### Forehead

Multi Threads / Tornado Screw / Mono Screw

### Crow's feet / Eye bags / Eye Corner's Lifting

Blunt Needle For Eye 30G-25mm

### Apple Zone

Multi Threads / Tornado Screw / Mono Screw

### Nasolabial folds / Mouth Corner's Lifting

Multi Threads / Tornado Screw / Mono Screw



### Face Lifting

18G-100mm / 19G-100mm

### Nose Dorsum / Nose Bridge


19G-60mm

### Nose Columella

19G-38mm

### Cervical Stripe / Neck Lifting

23G-38mm / 18G-100mm

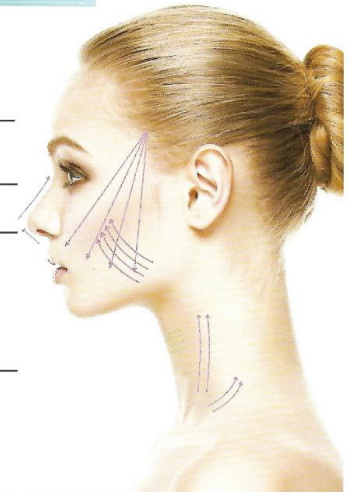



## Medical Cooling Gel Patch



### Usage Method



Step one:  
Thoroughly clean facial  
skin before using facial  
mask.



Step two:  
Remove the facial  
mask, spread it on the  
face and adjust it to  
the skin.



Step three:  
Apply for 15-20 minutes,  
so that the skin can  
absorb the essence of  
the facial mask.



Step four:  
Remove the facial mask,  
gently massage the face  
with the fingers, absorb  
the residual essence, and  
clean the face.

## Hyaluronic Acid Hydrating Mask



Net : 25ml  
Silk membrane cloth

WWW.HDKSUTURE.COM

## Peptide Repair Lyophilized Powder



- ① Peptide element repair lyophilized powder
- ② Peptide element repairing solvent



Step one:  
Open the aluminum cover and rubber plug.



Step two:  
Pour bottle ② of liquid into bottle ①.



Step three:  
Put on the dropper and shake the liquid in  
bottle ① evenly.



Step four:  
Squeeze the dropper, take a proper amount of  
liquid and evenly smear it on the face.

## Skin Care Products



Mild Cleaning Foam	150mL
Soothing Moisturizing Toner	120mL
Moisturizing Repairing Lotion	100mL
Brightening Recovery Essence	40mL
Multi-effect Nourishing Repairing Cream	50g

WWW.SUTURESUN.COM

## Hernia Repair Mesh



### Large mesh aperture

Promotes liquid circulation and smoothes tissue growth.


### Less micropores

Greatly reduces the possibility of bacteria hiding and is not easy to infect.


### Light weight

Reduce postoperative pain and foreign body sensation.

Hernia Example



After Mesh Repair




## Disposable Surgical Face Masks



### 3 Ply Flat type Ear Loop EN 14683:2019 Type IIR

Name	Parameter
Size	17.5 cm x 9.5 cm
Material	Polypropylene spunbond nonwoven fabric, polypropylene melt-blown nonwoven, metal wire with plastic covering nose clip, polyester/nylon spandex blend ear loops
Product performance:	The bacterial filtration efficiency of the mask should be not less than 98%.
Application	It is worn by clinical staff during non-invasive procedures, covering the user's mouth, nose, and jaw, providing a certain physical barrier to prevent direct penetration of pathogenic microorganisms, particulate matter, in patients, etc.
Expiration date	2 years after production
Storage	Store at room temperature, the relative humidity should not exceed 80%, non-corrosive gas and well-ventilated room. Transportation means should be clean and isolated from fire sources.

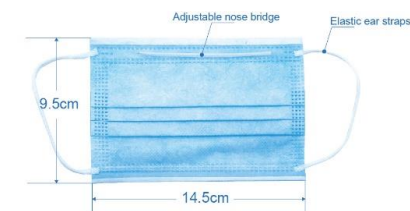

### 3 Ply Flat type Ear Loop EN 14683:2019 Type IIR

Name	Parameter
Size	14.5 cm x 9.5 cm
Material	Polypropylene spunbond nonwoven fabric, polypropylene melt-blown nonwoven, metal wire with plastic covering nose clip, polyester/nylon spandex blend ear loops
Product performance:	The bacterial filtration efficiency of the mask should be not less than 98%.
Application	It is worn by clinical staff during non-invasive procedures, covering the user's mouth, nose, and jaw, providing a certain physical barrier to prevent direct penetration of pathogenic microorganisms, particulate matter, in patients, etc.
Expiration date	2 years after production
Storage	Store at room temperature, the relative humidity should not exceed 80%, non-corrosive gas and well-ventilated room. Transportation means should be clean and isolated from fire sources.



## Disposable Medical Face Mask



3 Ply Flat type Ear Loop EN 14683:2019 Type I	
<b>Name</b>	<b>Parameter</b>
Size	17.5 cm x 9.5 cm
Material	Polypropylene spunbond nonwoven fabric, polypropylene melt-blown nonwoven, metal wire with plastic covering nose clip, polyester/nylon spandex blend ear loops
Product performance:	The bacterial filtration efficiency of the mask should be not less than 95%.
Application	It is worn by clinical staff during non-invasive procedures, covering the user's mouth, nose, and jaw, providing a certain physical barrier to prevent direct penetration of pathogenic microorganisms, particulate matter, in patients, etc.
Expiration date	2 years after production
Storage	Store at room temperature, the relative humidity should not exceed 80%, non-corrosive gas and well-ventilated room. Transportation means should be clean and isolated from fire sources.



3 Ply Flat type Ear Loop EN 14683:2019 Type IIR	
<b>Name</b>	<b>Parameter</b>
Size	17.5 cm x 9.5 cm
Material	Polypropylene spunbond nonwoven fabric, polypropylene melt-blown nonwoven, metal wire with plastic covering nose clip, polyester/nylon spandex blend ear loops
Product performance:	The bacterial filtration efficiency of the mask should be not less than 98%.
Application	It is worn by clinical staff during non-invasive procedures, covering the user's mouth, nose, and jaw, providing a certain physical barrier to prevent direct penetration of pathogenic microorganisms, particulate matter, in patients, etc.
Expiration date	2 years after production
Storage	Store at room temperature, the relative humidity should not exceed 80%, non-corrosive gas and well-ventilated room. Transportation means should be clean and isolated from fire sources.



3 Ply Flat type Ear Loop EN 14683:2019 Type I	
<b>Name</b>	<b>Parameter</b>
Size	14.5 cm x 9.5 cm
Material	Polypropylene spunbond nonwoven fabric, polypropylene melt-blown nonwoven, metal wire with plastic covering nose clip, polyester/nylon spandex blend ear loops
Product performance:	The bacterial filtration efficiency of the mask should be not less than 95%.
Application	It is worn by clinical staff during non-invasive procedures, covering the user's mouth, nose, and jaw, providing a certain physical barrier to prevent direct penetration of pathogenic microorganisms, particulate matter, in patients, etc.
Expiration date	2 years after production
Storage	Store at room temperature, the relative humidity should not exceed 80%, non-corrosive gas and well-ventilated room. Transportation means should be clean and isolated from fire sources.




5 Ply Folding type EN 14683:2019 Type IIR	
<b>Name</b>	<b>Parameter</b>
Size	11.5 cm x 15 cm
Material	Polypropylene spunbond nonwoven fabric, polypropylene melt-blown nonwoven, nose clip, polyester/nylon spandex blend ear loops
Product performance:	The bacterial filtration efficiency of the mask should be not less than 98%.
Application	It is worn by clinical staff during non-invasive procedures, covering the user's mouth, nose, and jaw, providing a certain physical barrier to prevent direct penetration of pathogenic microorganisms, particulate matter, in patients, etc.
Expiration date	2 years after production
Storage	Store at room temperature, the relative humidity should not exceed 80%, non-corrosive gas and well-ventilated room. Transportation means should be clean and isolated from fire sources.



### 3 Ply Cup type Head Loop EN 14683:2019 Type IIR

Name	Parameter
Size	13.5 cm x 13.5 cm
Material	Polypropylene spunbond nonwoven fabric, polypropylene melt-blown nonwoven, nose clip, polyester/nylon spandex blend ear loops
Product performance:	The bacterial filtration efficiency of the mask should be not less than 98%.
Application	It is worn by clinical staff during non-invasive procedures, covering the user's mouth, nose, and jaw, providing a certain physical barrier to prevent direct penetration of pathogenic microorganisms, particulate matter, in patients, etc.
Expiration date	2 years after production
Storage	Store at room temperature, the relative humidity should not exceed 80%, non-corrosive gas and well-ventilated room. Transportation means should be clean and isolated from fire sources.



### 5 Ply Folding type Head Loop N95-V1

Name	Parameter
Size	11.5 cm x 15 cm
Material	Polypropylene spunbond nonwoven fabric, polypropylene melt-blown nonwoven, nose clip, polyester/nylon spandex blend ear loops
Product performance:	The bacterial filtration efficiency of the mask should be not less than 95%.
Application	It is worn by clinical staff during non-invasive procedures, covering the user's mouth, nose, and jaw, providing a certain physical barrier to prevent direct penetration of pathogenic microorganisms, particulate matter, in patients, etc.
Expiration date	11 months after production
Storage	Store at room temperature, the relative humidity should not exceed 80%, non-corrosive gas and well-ventilated room. Transportation means should be clean and isolated from fire sources.

## Medical Goggle



#### Model specifications

□White □Black □Transparent  
□Large □Medium □Small

#### Product description

It is composed of a protective cover made of polymer material, a foam strip and a fixing device. Non-sterile, single use.

#### Expiration date

3 years after production

#### Storage

This product should be stored in a dry, ventilated, non-corrosive gas warehouse.

## Medical Isolation Mask



### Model: Ear hook type / Headband type

EN166:2001  
EN167:2002

#### Product description

It is composed of a protective cover made of polymer material, a foam strip and a fixing device. Non-sterile, single use.

#### Expiration date

3 years after production

#### Storage

This product should be stored in a dry, ventilated, non-corrosive gas warehouse.

## Isolation Gown



### Isolation Gown - TYPE A



Isolation gowns - type A Specifications: 120cm×120cm

**Material** 100% Non-woven fabric

**Product description** Non-woven fabrics are usually used as the main raw materials, which are made by cutting and sewing. Non-sterile, single-use.

**Expiration date** 3 years after production

**Storage** This product should be stored in a dry, ventilated, non-corrosive gas warehouse.

## Isolation Gown

- Good air permeability
- Strong barrier performance
- Non-sterile
- Do not reuse



100% Non-woven fabric



zipper



Elastic cuffs

### Isolation Gown - TYPE B



Isolation gowns - type B Specifications: One-size-fits-all

**Material** 100% Non-woven fabric


**Product description** Non-woven fabrics are usually used as the main raw materials, which are made by cutting and sewing. Non-sterile, single-use.

**Expiration date** 3 years after production

**Storage** This product should be stored in a dry, ventilated, non-corrosive gas warehouse.



## Medical Disposable Protective Clothing

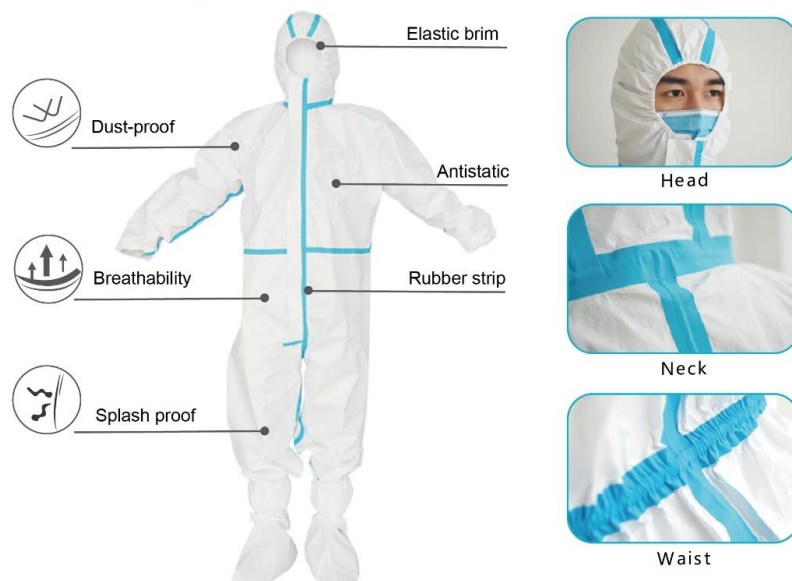

### Executive Standard: GB 19082-2009 EN 14126:2003



Specifications: One-piece Sizes: □ 160 □ 165 □ 170 □ 175 □ 180 □ 185

#### Raw materials of Components:

Items No.	Components	Raw materials
1	Fabrics	PP+PE (Polypropylene + polyethylene breathable membrane) composite material
2	Rubber strip	EVA low temperature glue, polymer basic cloth

**Intended use:** It is used to provide barrier and protection for the potentially infectious patients' blood, body fluids, secretions, etc. that clinical medical personnel come into contact with at work. It cannot be used to isolate places with strict microbiological index control requirements such as intensive care unit (room).

**Expiration date** 2 years after production

**Storage:** Store at room temperature, in non-corrosive gas, dry, avoid the sunlight, good ventilation, clean environment, away from fire.

WWW.HDKSUTURE.COM

## Surgical Gowns



CE BS EN 13795-1:2019



Model: □ S □ M □ L □ XL □ XXL □ XXXL □ XXXXL

Specifications: □ High performance type □ Standard type

**Material** 100% Non-woven fabric

**Intended use** For the surgical staff to wear, reduce the source of infection to the patient's surgical wound to prevent postoperative wound infection.

**Expiration date** 3 years after production

**Storage** Store in an environment with relative humidity not exceeding 80%, no corrosive gas, cool, dry, well ventilated and clean.

WWW.SUTURESCHN.COM

## Medical Isolation Shoe Cover



size: ☐Long ☐Short    Style: ☐Non-woven fabric ☐PVC ☐PP+PE

<b>Product description</b>	Made of suitable materials, with sufficient strength and barrier properties. Non sterile.
<b>Expiration date</b>	3 years after production
<b>Storage</b>	Store in an environment with relative humidity not exceeding 80%, no corrosive gas, cool, dry, well ventilated and clean.
Medical isolation shoe cover	Long-style / Short-style    Blue / White    FZ/T64005-2011

## Medical Cap

**Model specifications** Round cap.  $\phi$ 25.5cm FZ/T64005-2011

**Product description** Non-woven fabric is usually used as the main raw material, which is made by cutting and sewing. Non-sterile, single-use.

**Material** ☐Non-woven fabric ☐PP+PE

**Colour** Blue

**Storage** This product should be stored in a dry, ventilated, non-corrosive gas warehouse.



## Medical Scrubs Uniforms



**Model:** type A: split type; type B: gown type.



**Specifications** ☐S ☐M ☐L ☐XL ☐XXL

**Product Description** Usually made of cotton fiber or non-woven fabric. The medical scrubs uniforms is short-sleeve or long-sleeve style that have the function of blocking dandruff, and do not have liquid barrier properties. It is non-sterile supply and can be reused. It should be sterilized before using.

**Expiration date** 3 years after production

**Storage** The product should be stored in a clean warehouse without corrosive gas, well ventilated, cool and dry.

## Medical Bed Sheet



**Materials:** 70% Polypropylene, 30% Polyethylene non-woven fabric

<b>Product description</b>	It is made by compounding or sewing non-woven fabric and plastic film. Non-sterile, single use.
<b>Expiration date</b>	3 years after production
<b>Storage</b>	This product should be stored in a dry, ventilated, non-corrosive gas warehouse.



## Disposable Virus Specimen Collection Tube



Disposable sampler

**Model:** Inactivated and non-inactivated



<b>Product description</b>	Disposable virus specimen collection tube is composed of swabs and/or collection cups and tubes containing storage solution. Non-sterile.
<b>Expiration date</b>	12 months
<b>Storage</b>	The product should be stored in a non-corrosive gas and well-ventilated warehouse at room temperature.

### Medical examination gloves



**Model/Specification:** According to the different materials used, it is divided into: polyvinyl chloride, butyronitrile; according to the size, it is divided into: XS, S, M, L, XL.

**Product Description:** Usually made of materials such as polyvinyl chloride. Have sufficient strength and barrier properties. Non-sterile supply, single use.

**Intended use:** It will be wore by doctor to do checking for the patients or lab testing.

### Medical rubber gloves



**Model/Specification:** XS, S, M, L, XL.

**Product Description:** Usually made of materials such as polyvinyl chloride and rubber. Have sufficient strength and barrier properties. Non-sterile supply, single use.

**Intended use:** It will be wore by doctor to do checking for the patients or lab testing.



## Orthopedic Casting Tape



### USE INSTRUCTION

- Apply 1~2 layers stockinet over the affected body part;
- Wear surgical gloves;
- Choose proper size orthopedic casting tape, then open the package;
- Immerse the casting tape in normal temperature(20℃~30℃) water for 5~6 seconds and squeeze 2~3 times. Then remove from the water and squeeze out the excess water. The curing time of orthopedic casting tape is directly related to the temperature of water. The curing time is shorter in high temperature water than in low temperature water. If the water temperature is over 27℃, the curing time is too short to increase the difficulty of the operation.
- Wrap the casting tape spirally around the affected body part, overlapping the previous layer by one-half or two-thirds the width of the tape. The tension is moderate. If it is too loose, it will weaken the adhesion of the orthopedic casting tape. If it is too tight, it will affect the blood circulation.
- The intensity of the casting tape is related to the number of overlapped layers. Overlap 3~4 layers for the non-weight bearing parts, while overlap 5~6 layers for the weight bearing parts. If more layers are needed, please ensure the adhesivity between the layers.
- To increase the adhesion between layers, the casting tape will be shaped after wrapped. The operating time should be in 3~5 minutes. The adhesion and shaping effect cannot reach the best if the operating time is longer or the immersed time is too long. The patients do not allow to move freely in 10 minutes before the orthopedic casting tape are completely hardened.
- The electric plaster saw is needed if the affected parts need to open a window or remove the orthopedic casting tape.

Orthopedic Casting Tape				
Product Description	Sizes	Specification(W×L)	Packaging	Operating Part
Fiberglass Orthopedic Casting Tape	RT002	5.0cm × 360cm	10bags/box 12boxes/ctn	Wrists/Childrens
Fiberglass Orthopedic Casting Tape	RT003	7.5cm × 360cm	10bags/box 12boxes/ctn	Arms
Fiberglass Orthopedic Casting Tape	RT004	10.0cm × 360cm	10bags/box 12boxes/ctn	Arms / Legs
Fiberglass Orthopedic Casting Tape	RT005	12.5cm × 360cm	10bags/box 9boxes/ctn	Legs
Fiberglass Orthopedic Casting Tape	RT006	15.0cm × 360cm	10bags/box 9boxes/ctn	Legs

## Polymer Splint



Wrist Fixation  
Recommended sizes:  
312 (7.5cmX30cm)  
415 (10cmX40cm)

Thumb Fixation  
Recommended sizes:  
312 (7.5cmX30cm)  
415 (10cmX40cm)

The Fourth and Fifth Finger Fixation  
Recommended sizes:  
312 (7.5cmX30cm)  
415 (10cmX40cm)

Elbow Fixation  
Recommended sizes:  
312 (7.5cmX30cm)  
415 (10cmX40cm)



Forearm Fixation  
Recommended sizes:  
335 (7.5cmX90cm)  
430 (10cmX75cm)

Horseshoe Fixation  
Recommended sizes:  
335 (7.5cmX90cm)  
430 (10cmX75cm)

Ankle Fixation  
Recommended sizes:  
430 (10cmX75cm)  
530 (12.5cmX75cm)

Legs Fixation  
Recommended sizes:  
335 (7.5cmX90cm)  
545 (12.5cmX115cm)

### Polymer splint

Product Description	Sizes Specification(WxL)	Packaging	Operating part
Medical Polymer Splint	312 7.50cmX30cm	20bags/box 6boxes/ctn	wrists/Childrens
Medical Polymer Splint	335 7.50cmX90cm	10bags/box 6boxes/ctn	arms/legs
Medical Polymer Splint	415 10.0cmX40cm	15bags/box 6boxes/ctn	arms/legs
Medical Polymer Splint	430 10.0cmX75cm	10bags/box 6boxes/ctn	legs
Medical Polymer Splint	530 12.5cmX75cm	10bags/box 6boxes/ctn	legs
Medical Polymer Splint	545 12.5cmX115cm	5bags/box 6boxes/ctn	legs
Medical Polymer Splint	630 15.0cmX75cm	10bags/box 6boxes/ctn	legs
Medical Polymer Splint	645 15.0cmX115cm	5bags/box 6boxes/ctn	legs



Tissue Scissors



Stitch Scissors



Umbilical Scissors



Hemostatic Forceps



Tissue Forceps



Needle Forceps




Edison Forceps



Dissecting Forceps



Dressing Forceps

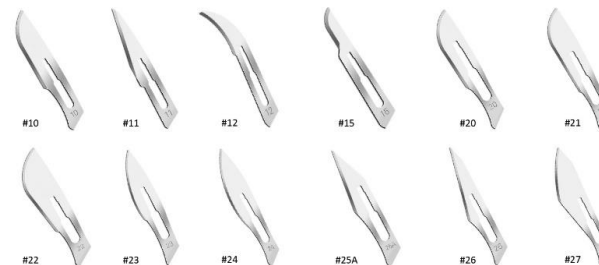

Surgical Blade



Scalpel 3#



Scalpel 4#




Scalpel 7#



Bone Hook




Skin Retractor



Surgery Suction Pipe

## Electric Wheelchair

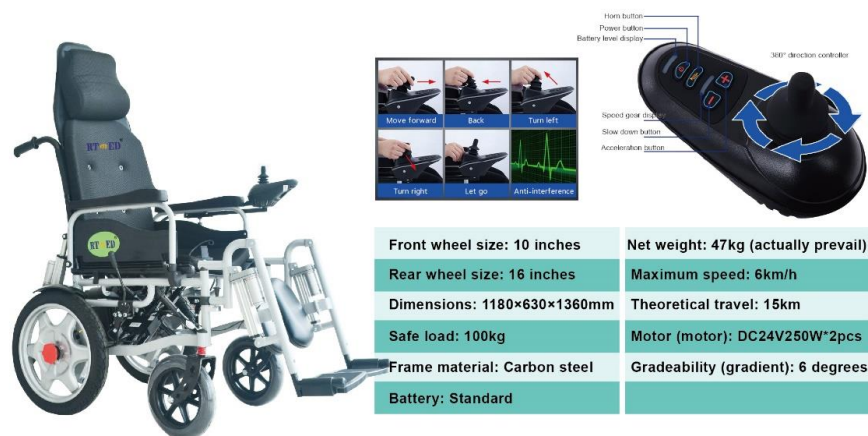

## Manual Wheelchair





## Seniors Shopping Cart

A good helper for parents in life



Tie-rod brake design



Comfortable seat



Wear-resistant reinforced brake rear wheel



## New Generation Multi-claw Crutches

Material upgrade



### Smooth all the way

- Anti-stumbling design
- Steady walk without hindrance
- The inside and outside width design is balanced and stable.



### Feel comfortable

- High wear-resistant handrail
- Surface cracked anti-skid treatment, anti-skid and wear-resistant, Ergonomic design, Fits to the hand without getting tired from holding for a long time.



### Firmer and stronger

- 1.2mm wall thickness Thicken reinforcement
- Lightweight and load-bearing



### Firm and convenient

- Annular clavicle clamp
- Fixed main pole Three simple steps



## Medical Grade Crutches

Stable and non-slip height adjustable



### PE environmentally friendly foam material arm rest

Thick PE foam material, high resilience, non-slip, soft and comfortable, strong abrasion resistance, not tired after long-term use.



### Leg height adjustment in 9 positions

The height of 9 levels is adjustable to meet the needs of people of different heights. Strengthen the aluminum alloy to provide super good support.



Two-way marbles

### Grip three-position adjustment

The grip has three gears adjustment, the adjustment part is locked firmly and stably, and it is convenient to use and feel comfortable and soft



Adjusting screw

### Non-slip durable rubber pad

The rubber pad is made of rubber, which is thicker, stable and non-slip, and the built-in metal gasket is wear-resistant and durable



## Nursing Bed

Bent leg angle: -45~25°

Back angle: 0~80°

Rollover angle: 0~55°

Toilet hole size: 280×215mm


Product Size: 2100×900×550mm

Bed size: 1970×900mm

Bed material: Thickened steel pipe

For people: Elderly, paralyzed patients, etc

Product accessories: Wash basin, infusion stand, mattress, dining table, guardrail, castor, bedpan

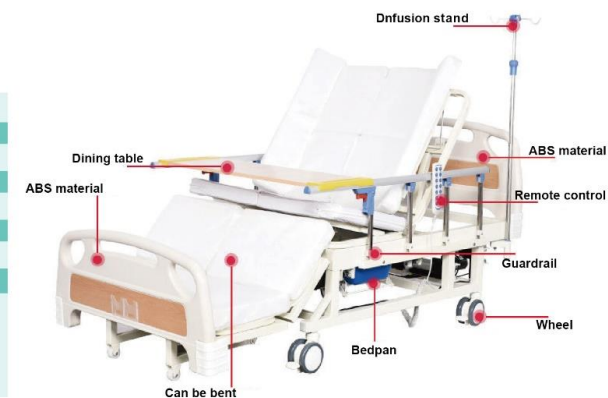



## Cassette Sutures

Length	25m 50m 75m 100m
Absorbable	Chromic catgut, Plain catgut PGA, PGLA, PDO
Non-absorbable	Silk, Nylon, Polyester, Polypropylene



## Suture Materials



## Self-adhesive Elastic Bandage

Standard	Features
5.0cm×450cm	Self-adhesive
7.5cm×450cm	High elasticity
10cm×450cm	Waterproof
15cm×450cm	Easy to tear

## Milkshake



## Pet Staple Food



## Cat Food / Dog Food



## Acupoint Pressure Stimulation Patch



Specification model:  $\phi 7\text{cm} \times 1\text{ paste} \times 40\text{ paste}$ , paste core  $\phi 3\text{cm}$

Product description: This product is composed of spheres and medical tape. It is attached to acupuncture points of the human body and only exerts pressure stimulation by external force.

Intended use: It is used to stick to acupuncture points of the human body for external stimulation. Non-invasive.

## Nasal Irrigator



Press once to release the water



Press again to stop the water

