

-----:
ORDIN DE PLATA NR.: 1409 TIP.DOC. 1 :
DATA EMITERII:15 iunie 2022 :
=====:
PLATITI: 5000-00 LEI: Cinci Mii lei 00 bani :
:
:
=====:
PLATITOR: (R) "BIOSISTEM CONTUL DE PLATI/CODUL IBAN :
MLD" S.R.L. MD95ML000000002251429243 :
CODUL FISCAL :1010600028048 / :
:
:
=====:
PRESTATORUL PLATITOR CODUL BANCII:
BC"Moldindconbank"S.A. fil."Invest" Chisinau :MOLDMD2X329:
=====:
BENEFICIAR (R) Centrul pen CONTUL DE PLATI/CODUL IBAN :
tru achizitii publice central MD23TRPCCC518430B01859AA :
izate in sanatate CODUL FISCAL :1016601000212 / :
:
:
=====:
PRESTATORUL BENEFICIAR CODUL BANCII:
Ministerul Finantelor - Trezoreria de Stat :TREZMD2X :
=====:
DESTINATIA PLATII:/Pl02/5000,00 Pentru g: TIPUL TRANSFERULUI :
arantia pentru oferta la procedura de ac: NORMAL/URGENT :N:
hizi?ie publica nr. ocds-b3wdpl-MD-16518: :
48654885 din 16.06.2022 :
:
:
: L.S. :
=====:
CODUL TRANZACTIEI:101: :
DATA PRIMIRII:15/06/2022 : SEMNATURILE :
DATA EXECUTARII: : EMITENTULUI :
:-----:
CONDUCTATOR:Web Poiata Vitalie :
MIIGYwYJKoZIhvcNAQcCoIIGVDCCBlACAQExCzAJBgUrDgMCGGUAMAsGCSqGSIB3:
DQEHAAACBGwwggRoMIIDUKADAgECAhNHAACjbilrgFksQ0G4AAAAAKNuMA0GCSqG:
SIB3DQEBcCwUAMCIXIDAeBgNVBAMTF0NFULQxLUNBLUL1vbGRpbmRjb25iYW5rMB4X:
DTIxMDEyODExMzgwNVVoXDTI0MDEyODExNDgwNVowZ8xCzAJBgNVBAYTAk1EMRAw:
YDVQQIEwdNb2xkb3ZhmREwDwYDVQQHEwhDaGlzaW5hdTEWMBQGA1UEChMNQmlv :
:
(semnatura electronica) :
CONTABIL-SEF:Web Nasedchin Alexandr :
MIIGZwYJKoZIhvcNAQcCoIIGWDCCBlQCAQExCzAJBgUrDgMCGGUAMAsGCSqGSIB3:
DQEHAAACBHAWggRsMIIDVKADAgECAhNHAACjcahRKqbJeg8QAAAAAKNxMA0GCSqG:
SIB3DQEBcCwUAMCIXIDAeBgNVBAMTF0NFULQxLUNBLUL1vbGRpbmRjb25iYW5rMB4X:
DTIxMDEyODExMzkwOFoXDTI0MDEyODExNDkxOFowgaMxCzAJBgNVBAYTAk1EMRAw:
YDVQQIEwdNb2xkb3ZhmREwDwYDVQQHEwhDaGlzaW5hdTEWMBQGA1UEChMNQmlv :
:
L.S. (semnatura electronica) :
CONDUCTATOR: :
(semnatura manuala) :
CONTABIL-SEF: :
(semnatura manuala) :
SEMNATURA PRESTATORUL L.S. :
:-----:
MOTIVUL REFUZULUI : L.S. :
-----:

CERTIFICAT
privind lipsa sau existența restanțelor față de bugetul public național

Nr.
№ **A2210514**

din
OT **03.06.2022**

1. Destinația / Назначение

Pentru participarea la proceduri de achiziții publice

2. Date despre contribuabil / Информация о налогоплательщике

Denumirea Наименование	Codul fiscal / Numărul de identificare Фискальный код / Идентификационный номер
BIOSISTEM MLD S.R.L.	1010600028048
Adresa sediului de bază (strada, numărul) Адрес основного месторасположения (улица, номер)	Codul - Denumirea localității Код - Наименование населенного пункта
Albisoara nr.16 bl.1 of.7	0150-SEC.RISCANI

3. Atestarea lipsei sau existenței restanțelor conform datelor Sistemului Informațional Automatizat /
Подтверждение отсутствия или наличия недоимки согласно данных Информационной автоматизированной системы

La data emiterii prezentului certificat restanța față de bugetul public național constituie/ На дату выдачи данной справки недоимка перед национальным публичным бюджетом составляет:
0,00 lei/лей.

4. Valabil până la / Действителен до 18.06.2022

5. Autentificarea Serviciului Fiscal de Stat / Подтверждение Государственной налоговой службы

**Șef DDF Rîșcani
a DGDF**

Funcția/Dолжность

L.Ș/ М.П.

Executor: **Claudia GOJAN**

Numele și prenumele/Фамилия и имя

Tel.(022)823102



Semnatura/Подпись

Ana STOICOV

Numele și prenumele/Фамилия и имя

Este extras din Sistemul Informațional al SFS SIA „Contul curent al contribuabilului”// 03.06.2022 ora 11:51:41
cu aplicarea prevederilor pct. 82-83 Ordin IFPS nr.400 din 14.03.2014 (Monitorul Oficial 72-77/399, 28.03.2014)

NOTA (0,00)



BC "MOLDINDCONBANK" S.A.

Filiala "Invest"

Republica Moldova, MD-2068
mun. Chișinău, bd. Moscovei, 14/1
Tel. : (373-22) 43-44-81, 43-46-24
Fax : (373-22) 43-44-22
cod: MOLDMD2X329

Data 14. IAN. 2016
Nr. 03/2 - 19/23

Республика Молдова, MD-2068
мун. Кишинэу, бул. Московской, 14/1
Тел. : (373-22) 43-44-81, 43-46-24
Факс : (373-22) 43-44-22
код: MOLDMD2X329

Filiala „Invest” BC „Moldindconbank” SA confirmă existența contului curent în moneda națională al **“BIOSISTEM MLD” S.R.L. (c/f 1010600028048)**, cu **IBAN MD95ML000000002251429243**.

Codul băncii MOLDMD2X329.

Director

Nina Turcan

Director financiar



Nina Balmuș

Ex. Diana Brinza
Tel. 43-45-96

REPUBLICA



MOLDOVA

CERTIFICAT DE ÎNREGISTRARE

Societatea cu Răspundere Limitată "BIOSISTEM MLD"
— ESTE ÎNREGISTRATĂ LA CAMERA ÎNREGISTRĂRII DE STAT —

Numărul de identificare de stat - codul fiscal
1010600028048

Data înregistrării

12.08.2010

Data eliberării

12.08.2010

Svirepova Ludmila, registrator

*Funcția, numele, prenumele persoanei
care a eliberat certificatul*

L. Svirepova
semnătura

MD 0101250





I.P. "AGENȚIA SERVICII PUBLICE"

Departamentul înregistrare și licențiere a unităților de drept

EXTRAS

din Registrul de stat al persoanelor juridice

nr. 8506 din 28.04.2021

Denumirea completă: **Societatea cu Răspundere Limitată «BIOSISTEM MLD».**

Denumirea prescurtată: **«BIOSISTEM MLD» S.R.L.**

Forma juridică de organizare: **Societate cu Răspundere Limitată.**

Numărul de identificare de stat și codul fiscal: **1010600028048.**

Data înregistrării de stat: **12.08.2010.**

Sediul: **MD-2001, str. Albișoara, 16/1, ap.(of.) 7, mun. Chișinău, Republica Moldova.**

Obiectul principal de activitate:

- 1 Activitatea farmaceutică;**
- 2 Importul, fabricarea, comercializarea, asistența tehnică și (sau) reparația dispozitivelor medicale și (sau) a opticii;**
- 3 Acordarea asistenței medicale de către instituțiile medico-sanitare private;**
- 4 Comerțul cu ridicata al calculatoarelor, echipamentelor periferice și software-ului;**
- 5 Întreținerea și repararea mașinilor de birou și a tehnicii de calcul;**
- 6 Consultații în domeniul sistemelor de calcul.**

Capitalul social: **5400 lei.**

Administrator: POIATA VITALIE,

Asociați:

- 1. POIATA VITALIE 33,40 %**
- 2. NASEDCHIN ALEXANDR 33,30 %**
- 3. KOJEVNIKOV DMITRII 33,30 %.**

Prezentul extras este eliberat în temeiul art. 34 al Legii nr. 220-XVI din 19 octombrie 2007 privind înregistrarea de stat a persoanelor juridice și a întreprinzătorilor individuali și confirmă datele din Registrul de stat la data de: 28.04.2021.

Specialist coordonator
tel. 022-207-840



Lazari Aliona



EB 0358735

Lista fondatorilor Biosistem-mld SRL

Nr.	Nume, Prenume	IDNP
1.	Vitalie Poiata	0983103892591
2.	Alexandr Nasedchin	2002001070747
3.	Dmitrii Kojevnikov	0972305012362

SITUAȚIILE FINANCIARE
pentru perioada 01.01.2021 - 31.12.2021

Entitatea: BIOSISTEM MLD S.R.L.
Cod CUIO: 40717392
Cod IDNO: 1010600028048

Sediul:
MD:
Raionul(municipiul): 106, DDF RISCANI
Cod CUATM: 0150, SEC.RISCANI
Strada: SECTORUL RISCANI STR.Albisoara nr.16 bl.1 of.7

Activitatea principală: G4646, Comert cu ridicata al produselor farmaceutice
Forma de proprietate: 16, Proprietate colectivă
Forma organizatorico-juridică: 530, Societăți cu răspundere limitată

Date de contact:
Telefon: +37322808719
WEB:
E-mail: zmii13@mail.ru
Numele și coordonatele al contabilului-șef: DI (dna) Tel.

Numărul mediu al salariaților în perioada de gestiune: 3 persoane.

Persoanele responsabile de semnarea situațiilor financiare* Nasedchin Alexandr

Unitatea de măsură: leu

BILANȚUL

Anexa 1

Nr. cpt.	Indicatori	Cod rd.	Sold la	
			Începutul perioadei de gestiune	Sfârșitul perioadei de gestiune
1	2	3	4	5
	A C T I V			
	ACTIVE IMOBILIZATE			
	I. Imobilizări necorporale			
	1. Imobilizări necorporale în curs de execuție	010		
	2. Imobilizări necorporale în exploatare, total	020		
	din care:	021		
	2.1. concesiuni, licențe și mărci			
	2.2. drepturi de autor și titluri de protecție	022		
	2.3. programe informatice	023		
	2.4. alte imobilizări necorporale	024		
	3. Fond comercial	030		
	4. Avansuri acordate pentru imobilizări necorporale	040		
	Total imobilizări necorporale (rd.010 + rd.020 + rd.030 + rd.040)	050		
	II. Imobilizări corporale			
	1. Imobilizări corporale în curs de execuție	060		
	2. Terenuri	070		
	3. Mijloace fixe, total	080	2793637	3559998
	din care:	081		
	3.1. clădiri			
	3.2. construcții speciale	082		
	3.3. mașini, utilaje și instalații tehnice	083	2791637	3533108
	3.4. mijloace de transport	084		

A.	3.5. inventar și mobilier	085		26890
	3.6. alte mijloace fixe	086	2000	
	4. Resurse minerale	090		
	5. Active biologice imobilizate	100		
	6. Investiții imobiliare	110		
	7. Avansuri acordate pentru imobilizări corporale	120		1162136
	Total imobilizări corporale (rd.060 + rd.070 + rd.080 + rd.090 + rd.100 + rd.110 + rd.120)	130	2793637	4722134
	III. Investiții financiare pe termen lung			
	1. Investiții financiare pe termen lung în părți neafiliate	140		
	2. Investiții financiare pe termen lung în părți afiliate, total	150		
	din care:			
	2.1. acțiuni și cote de participație deținute în părțile afiliate	151		
	2.2 împrumuturi acordate părților afiliate	152		
	2.3 împrumuturi acordate aferente intereselor de participare	153		
	2.4 alte investiții financiare	154		
	Total investiții financiare pe termen lung (rd.140 + rd.150)	160		
	IV. Creanțe pe termen lung și alte active imobilizate			
	1. Creanțe comerciale pe termen lung	170		
	2. Creanțe ale părților afiliate pe termen lung	180		
	inclusiv: creanțe aferente intereselor de participare	181		
	3. Alte creanțe pe termen lung	190		
	4. Cheltuieli anticipate pe termen lung	200		
	5. Alte active imobilizate	210		
	Total creanțe pe termen lung și alte active imobilizate (rd.170 + rd.180 + rd.190 + rd.200 + rd.210)	220		
	TOTAL ACTIVE IMOBILIZATE (rd.050 + rd.130 + rd.160 + rd.220)	230	2793637	4722134
B.	ACTIVE CIRCULANTE			
	I. Stocuri			
	1. Materiale și obiecte de mică valoare și scurtă durată	240	51978	5346
	2. Active biologice circulante	250		
	3. Producția în curs de execuție	260		
	4. Produse și mărfuri	270	7221203	9147976
	5. Avansuri acordate pentru stocuri	280		
	Total stocuri (rd.240 + rd.250 + rd.260 + rd.270 + rd.280)	290	7273181	9153322
	II. Creanțe curente și alte active circulante			
	1. Creanțe comerciale curente	300	3912218	2182471
	2. Creanțe ale părților afiliate curente	310		
	inclusiv: creanțe aferente intereselor de participare	311		
	3. Creanțe ale bugetului	320	74631	208171
	4. Creanțele ale personalului	330		
	5. Alte creanțe curente	340		
	6. Cheltuieli anticipate curente	350	2	
	7. Alte active circulante	360	5756117	1608597
	Total creanțe curente și alte active circulante (rd.300 + rd.310 + rd.320 + rd.330 + rd.340 + rd.350 + rd.360)	370	9742968	3999239
	III. Investiții financiare curente			
	1. Investiții financiare curente în părți neafiliate	380		
	2. Investiții financiare curente în părți afiliate, total	390		
	din care:			
	2.1. acțiuni și cote de participație deținute în părțile afiliate	391		
	2.2. împrumuturi acordate părților afiliate	392		
	2.3. împrumuturi acordate aferente intereselor de participare	393		

	2.4. alte investiții financiare în părți afiliate	394		
	Total investiții financiare curente (rd.380 + rd.390)	400		
	IV. Numerar și documente bănești	410	3942779	9861933
	TOTAL ACTIVE CIRCULANTE (rd.290 + rd.370 + rd.400 + rd.410)	420	20958928	23014494
	TOTAL ACTIVE (rd.230 + rd.420)	430	23752565	27736628
	P A S I V			
C.	CAPITAL PROPRIU			
	I. Capital social și neînregistrat			
	1. Capital social	440	5400	5400
	2. Capital nevărsat	450	()	()
	3. Capital neînregistrat	460		
	4. Capital retras	470	()	()
	5. Patrimoniul primit de la stat cu drept de proprietate	480		
	Total capital social și neînregistrat (rd.440 + rd.450 + rd.460 + rd.470 + rd.480)	490	5400	5400
	II. Prime de capital	500		
	III. Rezerve			
	1. Capital de rezervă	510		
	2. Rezerve statutare	520		
	3. Alte rezerve	530		
	Total rezerve (rd.510 + rd.520 + rd.530)	540		
	IV. Profit (pierdere)			
	1. Corecții ale rezultatelor anilor precedenți	550	X	
	2. Profit nerepartizat (pierdere neacoperită) al anilor precedenți	560	20060126	16230339
	3. Profit net (pierdere netă) al perioadei de gestiune	570	X	10403995
	4. Profit utilizat al perioadei de gestiune	580	X	()
	Total profit (pierdere) (rd.550 + rd.560 + rd.570 + rd.580)	590	20060126	26634334
	V. Rezerve din reevaluare	600		
	VI. Alte elemente de capital propriu	610		
	TOTAL CAPITAL PROPRIU (rd.490 + rd.500 + rd.540 + rd.590 + rd.600 + rd.610)	620	20065526	26639734
D.	DATORII PE TERMEN LUNG			
	1. Credite bancare pe termen lung	630		
	2. Împrumuturi pe termen lung	640		
	din care:	641		
	2.1. împrumuturi din emisiunea de obligațiuni			
	inclusiv: împrumuturi din emisiunea de obligațiuni convertibile	642		
	2.2. alte împrumuturi pe termen lung	643		
	3. Datorii comerciale pe termen lung	650		
	4. Datorii față de părțile afiliate pe termen lung	660		
	inclusiv: datorii aferente intereselor de participare	661		
	5. Avansuri primite pe termen lung	670		
	6. Venituri anticipate pe termen lung	680		
	7. Alte datorii pe termen lung	690		
	TOTAL DATORII PE TERMEN LUNG (rd.630 + rd.640 + rd.650 + rd.660 + rd.670 + rd.680 + rd.690)	700		
	DATORII CURENTE			
	1. Credite bancare pe termen scurt	710		
	2. Împrumuturi pe termen scurt, total	720		

E.	din care:	721		
	2.1. împrumuturi din emisiunea de obligațiuni			
	inclusiv: împrumuturi din emisiunea de obligațiuni convertibile	722		
	2.2. alte împrumuturi pe termen scurt	723		
	3. Datorii comerciale curente	730	3252667	343711
	4. Datorii față de părțile afiliate curente	740		
	inclusiv: datorii aferente intereselor de participare	741		
	5. Avansuri primite curente	750	188105	355528
	6. Datorii față de personal	760	50	350
	7. Datorii privind asigurările sociale și medicale	770		
	8. Datorii față de buget	780	187676	150263
	9. Datorii față de proprietari	790		
	10. Venituri anticipate curente	800		
	11. Alte datorii curente	810	58541	247042
	TOTAL DATORII CURENTE (rd.710 + rd.720 + rd.730 + rd.740 + rd.750 + rd.760 + rd.770 + rd.780 + rd.790 + rd.800 + rd.810)	820	3687039	1096894
F.	PROVIZIOANE			
	1. Provizioane pentru beneficiile angajaților	830		
	2. Provizioane pentru garanții acordate cumpărătorilor/clientilor	840		
	3. Provizioane pentru impozite	850		
	4. Alte provizioane	860		
	TOTAL PROVIZIOANE (rd.830 + rd.840 + rd.850 + rd.860)	870		
	TOTAL PASIVE (rd.620 + rd.700 + rd.820 + rd.870)	880	23752565	27736628

SITUAȚIA DE PROFIT ȘI PIERDERE

de la pînă la

Anexa 2

Indicatori	Cod rd.	Perioada de gestiune	
		precedenta	curenta
1	2	3	4
Venituri din vânzări, total	010	25963175	38680547
din care:			
venituri din vânzarea produselor și mărfurilor	011	25044358	37724557
venituri din prestarea serviciilor și executarea lucrărilor	012	918817	951393
venituri din contracte de construcție	013		
venituri din contracte de leasing	014		
venituri din contracte de microfinanțare	015		
alte venituri din vânzări	016		4597
Costul vânzărilor, total	020	15186814	24434231
din care:			
valoarea contabilă a produselor și mărfurilor vândute	021	15186814	24433364
costul serviciilor prestate și lucrărilor executate terților	022		
costuri aferente contractelor de construcție	023		
costuri aferente contractelor de leasing	024		
costuri aferente contractelor de microfinanțare	025		
alte costuri aferente vânzărilor	026		867
Profit brut (pierdere brută) (rd.010 - rd.020)	030	10776361	14246316
Alte venituri din activitatea operațională	040	247603	5189
Cheltuieli de distribuire	050	19740	6076
Cheltuieli administrative	060	1259776	1788732
Alte cheltuieli din activitatea operațională	070	640169	1870642
Rezultatul din activitatea operațională: profit (pierdere) (rd.030 + rd.040 - rd.050 - rd.060 - rd.070)	080	9104279	10586055

Venituri financiare, total	090	519239	1517765
din care:			
venituri din interese de participare	091		
inclusiv: veniturile obținute de la părțile afiliate	092		
venituri din dobânzi	093	25612	30619
inclusiv: veniturile obținute de la părțile afiliate	094		
venituri din alte investiții financiare pe termen lung	095		
inclusiv: veniturile obținute de la părțile afiliate	096		
venituri aferente ajustărilor de valoare privind investițiile financiare pe termen lung și curente	097		
venituri din ieșirea investițiilor financiare	098		
venituri aferente diferențelor de curs valutar și de sumă	099	493627	1487146
Cheltuieli financiare, total	100	597528	249562
din care:			
cheltuieli privind dobânzile	101		
inclusiv: cheltuielile aferente părților afiliate	102		
cheltuieli aferente ajustărilor de valoare privind investițiile financiare pe termen lung și curente	103		
cheltuieli aferente ieșirii investițiilor financiare	104		
cheltuieli aferente diferențelor de curs valutar și de sumă	105	597528	249562
Rezultatul: profit (pierdere) financiar(ă) (rd.090 - rd.100)	110	-78289	1268203
Venituri cu active imobilizate și excepționale	120		
Cheltuieli cu active imobilizate și excepționale	130		
Rezultatul din operațiuni cu active imobilizate și excepționale: profit (pierdere) (rd.120 - rd.130)	140		
Rezultatul din alte activități: profit (pierdere) (rd.110 + rd.140)	150	-78289	1268203
Profit (pierdere) pînă la impozitare (rd.080 + rd.150)	160	9025990	11854258
Cheltuieli privind impozitul pe venit	170	1051159	1450263
Profit net (pierdere netă) al perioadei de gestiune (rd.160 - rd.170)	180	7974831	10403995

SITUAȚIA MODIFICĂRILOR CAPITALULUI PROPRIU

de la pînă la

Anexa 3

Nr. d/o	Indicatori	Cod rd	Sold la începutul perioadei de gestiune	Majorări	Diminuări	Sold la sfîrșitul perioadei de gestiune
1	2	3	4	5	6	7
I.	Capital social și neînregistrat					
	1. Capital social	010				
	2. Capital nevărsat	020	()	()	()	()
	3. Capital neînregistrat	030				
	4. Capital retras	040	()	()	()	()
	5. Patrimoniul primit de la stat cu drept de proprietate	050				
	Total capital social și neînregistrat (rd.010 + rd.020 + rd.030 + rd.040 + rd.050)	060				
II.	Prime de capital	070				
III.	Rezerve					
	1. Capital de rezervă	080				
	2. Rezerve statutare	090				
	3. Alte rezerve	100				
	Total rezerve (rd.080 + rd.090 + rd.100)	110				
	Profit (pierdere)					
	1. Corecții ale rezultatelor anilor precedenți	120	X			

IV.	2. Profit nerepartizat (pierdere neacoperită) al anilor precedenți	130				
	3. Profit net (pierdere netă) al perioadei de gestiune	140	X			
	4. Profit utilizat al perioadei de gestiune	150	X	()	()	()
	Total profit (pierdere) (rd.120 + rd.130 + rd.140 + rd.150)	160				
V.	Rezerve din reevaluare	170				
VI.	Alte elemente de capital propriu	180				
	Total capital propriu (rd.060 + rd.070 + rd.110 + rd.160 + rd.170 + rd.180)	190				

SITUAȚIA FLUXURILOR DE NUMERAR

de la pînă la

Anexa 4

Indicatori	Cod rd	Perioada de gestiune	
		precedentă	curentă
1	2	3	4
Fluxuri de numerar din activitatea operațională			
Încasări din vânzări	010		
Plăți pentru stocuri și servicii procurate	020		
Plăți către angajați și organe de asigurare socială și medicală	030		
Dobînzi plătite	040		
Plata impozitului pe venit	050		
Alte încasări	060		
Alte plăți	070		
Fluxul net de numerar din activitatea operațională (rd.010 - rd.020 - rd.030 - rd.040 - rd.050 + rd.060 - rd.070)	080		
Fluxuri de numerar din activitatea de investiții			
Încasări din vânzarea activelor imobilizate	090		
Plăți aferente intrărilor de active imobilizate	100		
Dobînzi încasate	110		
Dividende încasate	120		
inclusiv: dividende încasate din străinătate	121		
Alte încasări (plăți)	130		
Fluxul net de numerar din activitatea de investiții (rd.090 - rd.100 + rd.110 + rd.120 ± rd.130)	140		
Fluxuri de numerar din activitatea financiară			
Încasări sub formă de credite și împrumuturi	150		
Plăți aferente rambursării creditelor și împrumuturilor	160		
Dividende plătite	170		
inclusiv: dividende plătite nerezidenților	171		
Încasări din operațiuni de capital	180		
Alte încasări (plăți)	190		
Fluxul net de numerar din activitatea financiară (rd.150 - rd.160 - rd.170 + rd.180 ± rd.190)	200		
Fluxul net de numerar total (± rd.080 ± rd.140 ± rd.200)	210		
Diferențe de curs valutar favorabile (nefavorabile)	220		
Sold de numerar la începutul perioadei de gestiune	230		
Sold de numerar la sfîrșitul perioadei de gestiune (± rd.210 ± rd.220 + rd.230)	240		

[Версия для печати](#)
[Сохранить](#)

Расписка 2

Респондент

Фискальный код: 1010600028048, наименование: BIOSISTEM MLD S.R.L.

Предоставил отчёт: RSF1_21

На фискальный период: A/2021

Дата предоставления: 29.03.2022

Временная метка отчёта зарегистрированного в Информационной Системе НБС : 29.03.2022 17:25:45

National Bureau of Statistics (NBS) received the electronic version of the report, sent by you. The data provided is verified by NBS.

[Версия для печати](#)

[Сохранить](#)

Расписка

Респондент

Фискальный код: 1010600028048, наименование: BIOSISTEM MLD S.R.L.

Предоставил отчёт: RSF1_21

На фискальный период: A/2021

Дата предоставления: 29.03.2022

Временная метка отчёта зарегистрированного в Системе Электронной Отчётности и отправленного в Информационную Систему БНС : 29.03.2022 14:51:06



AGENȚIA DE MEDIU

ENVIRONMENTAL AGENCY

MD-2005 mun.Chișinău, str. Albișoara, 38
Tel. (022) 820-770, Email: am@am.gov.md

CONFIRMARE

privind înregistrarea în „Lista producătorilor” de produse
supuse reglementărilor de responsabilitate extinsă a producătorului
(echipamente electrice și electronice)

În scopul plasării pe piață a produselor de echipamente electrice și electronice, în conformitate cu prevederile art. 12 alin. (5) și alin. (14) lit. b) din Legea nr. 209 din 29.07.2016 privind deșeurile, și punctele 46 – 50 din Regulamentul privind deșeurile de echipamente electrice și electronice, aprobat prin Hotărârea Guvernului nr. 212 din 07.03.2018, se emite numărul de înregistrare

MD2021-10-EEE-005

pentru BIOSISTEM MLD, IDNO: 1010600028048, cu adresa juridică: mun. Chișinău, str. Albișoara 16/1, ap. 1.

Numărul de înregistrare este valabil începând cu data de 02.11.2021 până la data de 02.11.2024.

Director adjunct interimar
Gavril GÎLCA

Features

- Built-in incubator.
- Automatic stirring system.
- Five points calibration.
- Accurate measurement without influence from pathological sample during test.
- Open system for reagent, low reagent consumption (50µl-100µl).
- Automatic storage, printout calculation parameter curve.
- Large memory and review system.
- User friendly software.

Assay Report Specifications

PT	Prothrombin Time.
APTT	Activated Partial Thromboplastin Time.
TT	Thrombin Time.
Fbg	Fibrinogen Concentration.
Clotting Factors	Clotting factors are expressed in the of time (sec.), ratio or INR.

Technical Specifications

Item	CA-01	CA-02
Channel	Single	Double
Built-in Incubator	37°C±0.2°C, capacity for 16 sample positions and 2 reagent positions.	37°C±0.2°C, capacity for 2×16 sample positions and 2×2 reagent positions.
Measuring System	Photometric	
Beam Source	LED	
Magnetic Stirring Motor	For measuring cuvette	
Data Input	Membrane keypad	
Display	Back-illuminated LCD	
Printer	Built-in thermal printer	
Operation Language	English, other languages on request	
Power Supply	AC 110V 60Hz / 220V 50Hz	
Dimensions	30cmx35cmx15cm	30cmx35cmx15cm
Weight	4.0kgs	4.0kgs

CLINDIAG...

The Reference for Quality and Service

CLINDIAG
CLINDIAG SYSTEMS B.V.B.A.



CA-01/02

Coagulometer



ISO9001:2008 & ISO13485:2003

Headquarters

Add: Steenberg 66, Pollare/Ninove(9401), Belgium
Tel: 0032 54 250 936
Fax: 0032 54 243 058
Website: <http://www.clindiag.be>
E-mail: marketing@clindiag.be

U.S. Office

Add: 1351 S. Leavitt Ave, Suite 104 Orange City, Florida 32763 USA
Tel: 001 386 456 1235
Fax: 001 407 358 5024
E-mail: info@clindiagusa.com

India Office

Add: B-1177-78, G.D. Colony Mayur Vihar Phase-III, Delhi-110096
Ph: 0091 11 22618779
Fax: 0091 11 22618780
E-mail: contact@clindiagindia.com

SEMI AUTO BIOCHEMISTRY ANALYZER (CLINDIAG SA-20)



Light Source	6V 10W long-life halogen lamp
Filters	7 standard filters from 340 to 800nm, 2 more open filter positions; ± 2 nm pass-band
Wavelength Accuracy	± 2 nm
Measuring Range	0-3.500 O.D
Photometric Linearity	$\pm 2\%$ from 0 to 2.000 O.D.
Photometric Accuracy	$\pm 2\%$ from 0 to 2.000 O.D.
Drift	less than 0.001 O.D.
Carry Over	$\leq 1\%$
Incubator Temperature control	25degree.centigrade ,30degree.centigrade ,37degree.centigrade, Precision: ± 0.1 degree.centigrade
Reagent Volume	200-500 ul
Printer	Built-in thermal printer, 57mm width paper
Power Supply	110V 60HZ / 220V 50HZ, 60VA
Dimensions	34cm*38cm*18cm

Better Usability



Minimum size with the footprint similar to that of a 17 inch laptop, with space saving design that allows internal storage of lyse giving small labs more space.

10.4 inch TFT touch screen together with our powerful software enhances user operations and experience.



New technology that eliminates the need for cleanser and rinse, reducing the number of reagents needed while at the same time lowering overall reagent consumption.

Flexible packaging of reagents, with normal and small sizes to better cater to the needs of different daily sample volumes.

Enhanced Performance

Higher throughput at 70 tests per hour.



Micro sample volume at 9.0uL for whole blood mode with capillary whole blood samples supported, perfect for pediatric samples.

BC-30s

Auto Hematology Analyzer

Technical Specifications

Principles

Impedance method for WBC, RBC and PLT counting
Cyanide free reagent for hemoglobin test

Performance

Parameter	Linearity Range	Precision (CV %)	Carryover
WBC($10^9/L$)	0-200	$\leq 3.5\%$ (4.0-6.9) $\leq 2.0\%$ (7.0 -15.0)	$\leq 0.5\%$
RBC($10^{12}/L$)	0-8.00	$\leq 1.5\%$ (3.5-6.5)	$\leq 0.5\%$
HGB(g/L)	0-280	$\leq 1.5\%$ (100 -180)	$\leq 0.5\%$
MCV(fL)		$\leq 1.0\%$ (70 -110)	
PLT($10^9/L$)	0-4000	$\leq 5.0\%$ (100 -149) $\leq 4.0\%$ (150 -500)	$\leq 1.0\%$

Parameters

21 parameters: WBC, Lymph#, Mid#, Gran#, Lymph%, Mid%, Gran%, RBC, HGB, HCT, MCV, MCH, MCHC, RDW-CV, RDW-SD, PLT, MPV, PDW, PCT, P-LCR, P-LCC
3 histograms for WBC, RBC and PLT

Reagent

M-30D DILUENT
M-30CFL LYSE
PROBE CLEANSER

Sample Volume

Prediluted mode 20 μ L
Whole blood mode 9 μ L

Throughput

70 samples per hour

Display

10.4 inch TFT Touch Screen

Multi-language

Chinese, English, Spanish, Portuguese, Russian, French, Bahasa Indonesia

Data Storage Capacity

Up to 500,000 results including numeric and graphical information

Communication

LAN Port supports HL7 protocol
Support bi-directional LIS

Interface

4 USB port (for external printer, software upgrade, barcode reader, WIFI adapter, keyboard and mouse), LAN port (1)

Printout

Thermal recorder, 50 mm wide paper, various printouts formats
External printer optional

Operating Environment

Temperature: 10°C~40°C
Humidity: 10%~90%
Air pressure: 70kPa~106kPa

Power Requirement

100V-240V
 $\leq 300VA$
50Hz/60Hz

Dimension and Weight

Dimension: Depth(410 mm) x width(300 mm) x height(400 mm)
Weight: $\leq 20Kg$

Mindray Building, Keji 12th Road South,
High-tech Industrial Park, Nanshan, Shenzhen 518057, P.R. China
Tel: +86 755 8188 8998 Fax: +86 755 26582680
E-mail: intl-market@mindray.com www.mindray.com

Mindray is listed on the NYSE under the symbol "MR"

mindray

are registered trademarks or trademarks owned by Shenzhen Mindray Bio-medical Electronics Co., LTD.

©2015 Shenzhen Mindray Bio-Medical Electronics Co., Ltd. All rights reserved. Specifications subject to changes without prior notice.

P/N: ENG-BC-30s-210285x6-20150623

mindray



BC-30s

Auto Hematology Analyzer

Minimum Size,
Maximum Capability



mindray
healthcare within reach

BC-30s

Auto Hematology Analyzer

What a 3-part should be

At Mindray we pride ourselves in our dedication and experience in developing better solutions for small labs. Our new line of 3-part hematology analyzers is the culmination of that effort. Compact yet powerful, full featured yet affordable, the BC-30s is what a 3-part analyzer should be.

Exclusive Feature




Detailed flag information never before seen on a 3-part analyzer. Provides information useful for diagnosis including WBC flag, RBC flag and PLT flag.

Different flag information provided according to parameter results together with histograms.




Sample 1 : BC-30s shows flags "Leucopenia", "Lymph decreased", "Pancytopenia" which mean white blood cell decreased, the low number of Lymphocyte and decreased of leukocyte, erythrocyte and plate count. Meanwhile "R3" flag is also displayed. Two kinds of flag messages are both supported to ensure clinicians have better understanding of sample results.

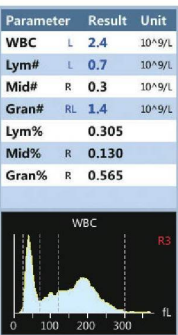


Leucopenia
Lymph decreased
Pancytopenia

Sample 2 : Flag "Anemia" means that the sample has the possibility of anemia.

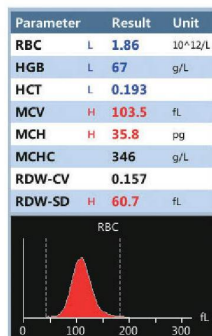


Anemia

Sample 3 : Flag "Thrombopenia" indicator is shown together with Platelets low flag.

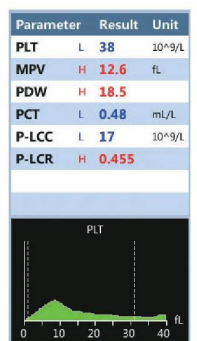


Thrombopenia

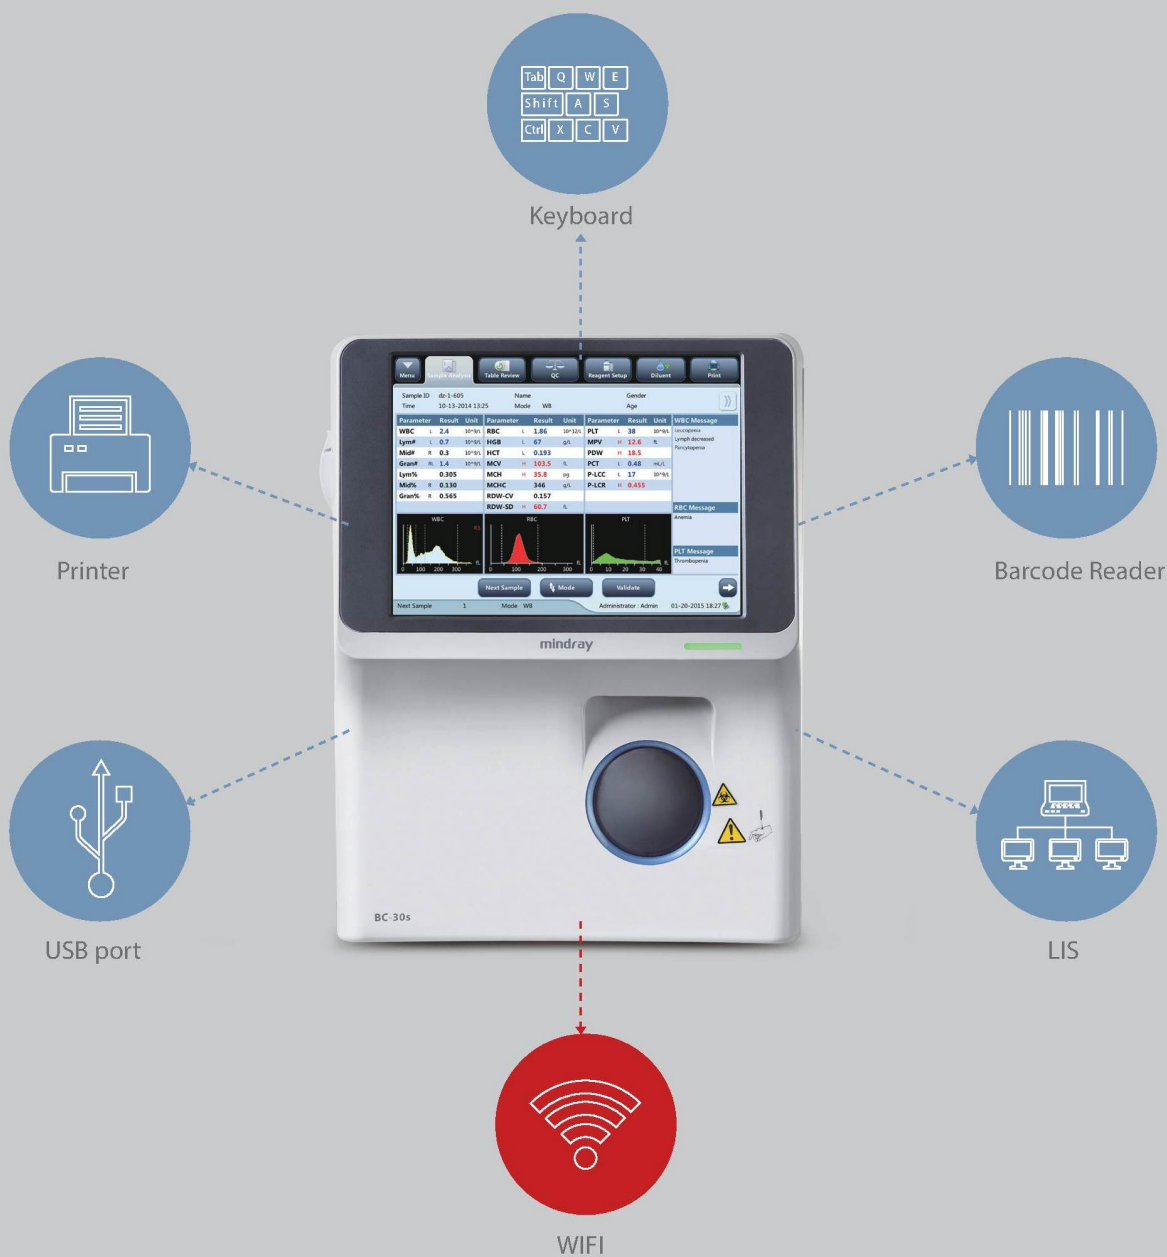

WIFI capability provides you an added option for data communication together with bi-directional LIS, USB port and LAN port, barcode reader, printer and keyboard.



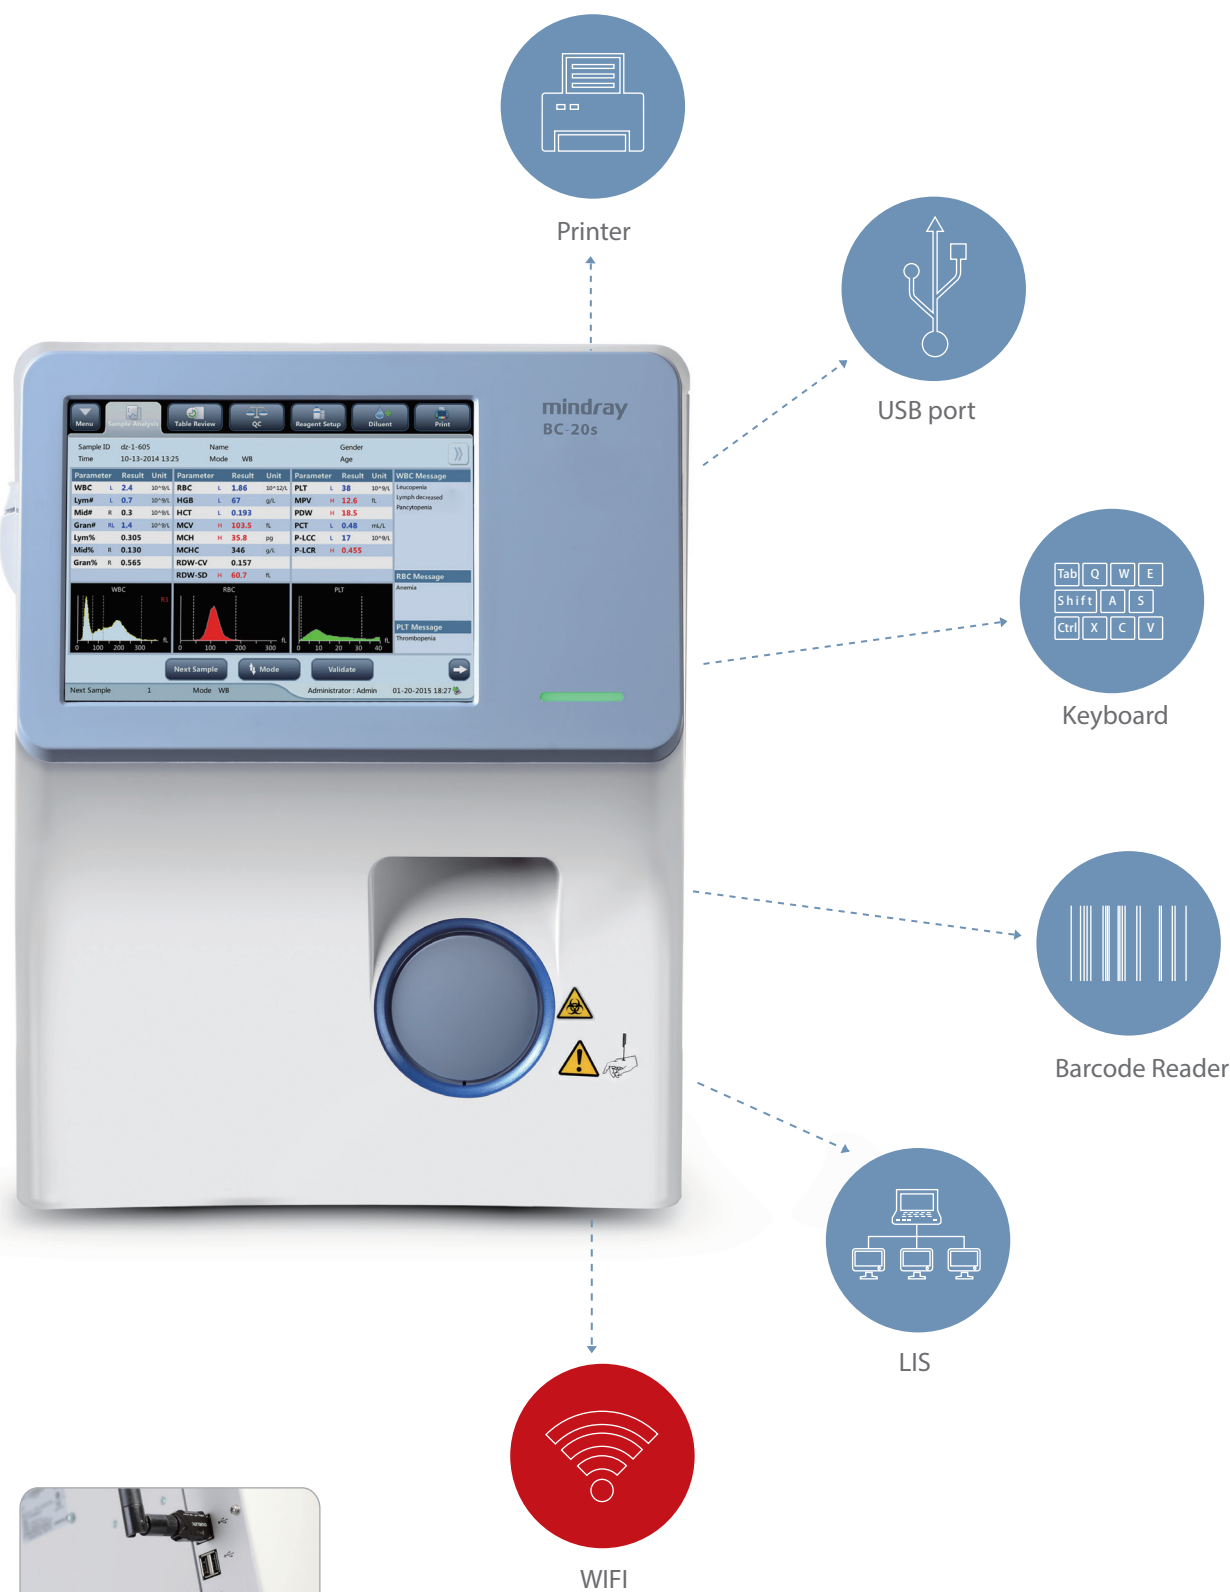

WIFI capability provides you an added option for data communication together with bi-directional LIS, USB port and LAN port, barcode reader, printer and keyboard.

BC-20s

Auto Hematology Analyzer

Technical Specifications

Principles

Impedance method for WBC, RBC and PLT counting
Cyanide free reagent for hemoglobin test

Performance

Parameter	Linearity Range	Precision (CV %)	Carryover
WBC($10^9/L$)	0-100	$\leq 3.5\%$ (4.0-6.9) $\leq 2.0\%$ (7.0-15.0)	$\leq 0.5\%$
RBC($10^{12}/L$)	0-8.00	$\leq 1.5\%$ (3.5-6.5) $\leq 1.0\%$ (70-110)	$\leq 0.5\%$
HGB(g/L)	0-280	$\leq 1.5\%$ (100-180) $\leq 1.0\%$ (100-149)	$\leq 0.5\%$
MCV(fL)		$\leq 1.0\%$ (150-500)	
PLT($10^9/L$)	0-1000	$\leq 5.0\%$ (100-149) $\leq 4.0\%$ (150-500)	$\leq 1.0\%$

Parameters

19 parameters: WBC, Lymph#, Mid#, Gran#, Lymph%, Mid%, Gran%, RBC, HGB, HCT, MCV, MCH, MCHC, RDW-CV, RDW-SD, PLT, MPV, PDW, PCT
3 histograms for WBC, RBC and PLT

Reagent

M-30D DILUENT
M-30CFL LYSE
PROBE CLEANSER

Sample Volume

Prediluted mode 20 μ L
Whole blood mode 9 μ L

Throughput

40 samples per hour

Display

8.4 inch TFT Touch Screen

Data Storage Capacity

Up to 200,000 results including numeric and graphical information

Communication

LAN Port supports HL7 protocol
Support bi-directional LIS

Interface

4 USB port (for external printer, software upgrade, barcode reader, WIFI adapter, keyboard and mouse), LAN port (1)

Printout

Thermal recorder, 50 mm wide paper, various printouts formats
External printer optional

Operating Environment

Temperature: 10°C~40°C
Humidity: 10%~90%
Air pressure: 70kPa~106kPa

Power Requirement

100V-240V
 ≤ 300 VA
50Hz/60Hz

Dimension and Weight


Dimension: Depth(410 mm) x width(300 mm) x height(400 mm)
Weight: ≤ 20 Kg



BC-20s

Auto Hematology Analyzer

Minimum Size,
Maximum Capability

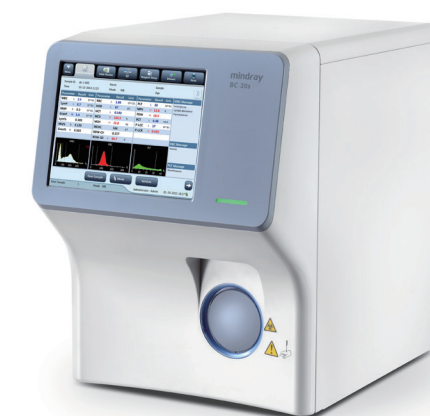

Mindray Building, Keji 12th Road South,
High-tech Industrial Park, Nanshan, Shenzhen 518057, P.R. China
Tel: +86 755 8188 8998 Fax: +86 755 26582680
E-mail: intl-market@mindray.com www.mindray.com
Mindray is listed on the NYSE under the symbol "MR"

mindray are registered trademarks or trademarks owned by Shenzhen Mindray Bio-medical Electronics Co., Ltd.
© 2015 Shenzhen Mindray Bio-Medical Electronics Co., Ltd. All rights reserved. Specifications subject to changes without prior notice.
P/N: ENG-BC-20s-210285x6-20150331

mindray

mindray
healthcare within reach



What a 3-part should be

At Mindray we pride ourselves in our dedication and experience in developing better solutions for small labs. Our new line of 3-part hematology analyzers is the culmination of that effort. Compact yet powerful, full featured yet affordable, the BC-20s is what a 3-part analyzer should be.



Exclusive Feature

Detailed flag information never before seen on a 3-part analyzer. Provides information useful for diagnosis including WBC flag, RBC flag and PLT flag.


BC-20s Auto Hematology Analyzer

Sample 1 : BC-20s shows flag “Lymph increased” which means a high number of Lymphocytes and/or immature cells. Meanwhile R1 flag is also displayed. Two kinds of flag messages are both supported to ensure clinicians have better understanding of sample results.

Sample 2 : Flag “Anemia” and “HGB Abn./Interfere?” are displayed. They mean the sample has shows either signs of Anemia, Abnormal Hemoglobin or sample is interfered such as by high value of Leukocytes or Agglutinated Erythrocytes.

Sample 3 : Flag “Thrombopenia” indicator is shown together with Platelets low flag.

Different flag information provided according to parameter results together with histograms.

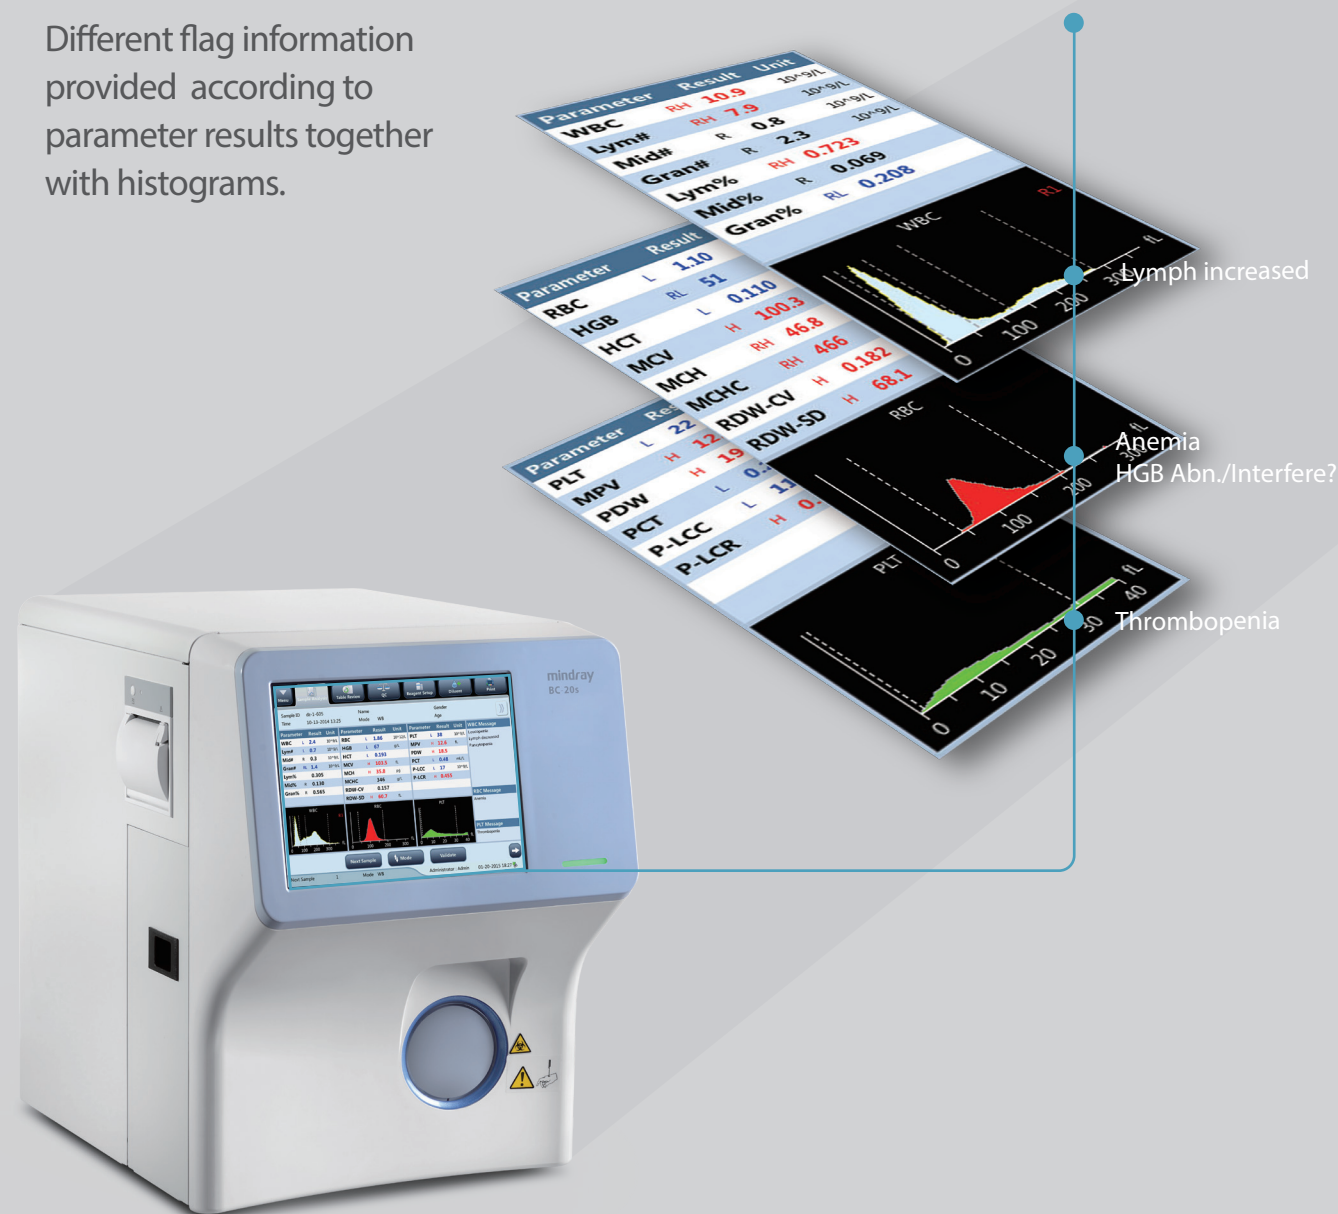

Better Usability

Minimum size with the footprint similar to that of a 17 inch laptop, with space saving design that allows internal storage of lyse giving small labs more space. 8.4 inch TFT touch screen together with our powerful software enhances user operations and experience.

Higher Efficiency

New technology that eliminates the need for cleanser and rinse, reducing the number of reagents needed while at the same time lowering overall reagent consumption. Flexible packaging of reagents, with normal and small sizes to better cater to the needs of different daily sample volumes.



Enhanced Performance

Higher throughput at 40 tests per hour.

Micro sample volume at 9.0uL for whole blood mode with capillary whole blood samples supported, perfect for pediatric samples.



Declaration of Conformity

This is to state that Technical Documentation (CL001, rev. 2.0) for product(s)

Coaguometer

(Model:CA-01, CA-02)

(IVD products other than those covered by Annex II, IVD for self-testing and devices for Performance evaluation according to manufacturer's declaration)

Manufactured by

CLINDIAG SYSTEMS CO., LTD

No.29 Zhiyuan Road, Jurong Economic Development Zone,

Zhenjiang, Jiangsu Province, China

Has been assessed as meeting the Essential Requirements and relevant provisions of EC Directive 98/79/EEC for in Vitro Diagnostic Medical Device



For and on behalf of
CLINDIAG SYSTEMS CO.,LTD.


.....
Authorized Signature(s)

Mr. Xu Xin

General Manager

Valid from May, 2018 to May, 2023





Certificate CN19/42081

The management system of

CLINDIAG SYSTEMS CO., LTD.

29, Zhiyuan Road, Jurong Economic Development Zone,
Zhenjiang City, Jiangsu Province, 212400, P.R. China.

has been assessed and certified as meeting the requirements of

ISO 13485:2016 EN ISO 13485:2016

For the following activities

**Design, Development, Production, Marketing and Service of Fully
Automatic Biochemistry Analyzer, Semi-Automatic Biochemistry
Analyzer, Haematology Analyzer, Microplate Reader, Coagulometer,
Microplate Washer, Platelet Function Analyzer, Electrolyte Analyzer,
Auto POCT Chemistry Analyzer**

This certificate is valid from 4 June 2019 until 3 June 2022
and remains valid subject to satisfactory surveillance audits.

Re certification audit due before 29 March 2022

Issue 1. Certified since 4 June 2019

Multiple certificates have been issued for this scope
The main certificate is numbered CN19/42078.00

Authorised by

SGS United Kingdom Ltd
Rossmore Business Park, Ellesmere Port, Cheshire, CH65 3EN, UK
t +44 (0)151 350-6666 f +44 (0)151 350-6600 www.sgs.com

HC SGS 13485 2016 0118

Page 1 of 1



0005



This document is issued by the Company subject to its General Conditions of Certification Services accessible at www.sgs.com/terms_and_conditions.htm. Attention is drawn to the limitations of liability, indemnification and jurisdictional issues established therein. The authenticity of this document may be verified at <http://www.sgs.com/en/certified-clients-and-products/certified-client-directory>. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.



REGISTRATION NO. 04719Q10805R0S

CERTIFICATE OF QUALITY MANAGEMENT SYSTEM

This is to certify that the quality management system of

Clindiag Systems Co., Ltd.

Registered Address: No.29 Zhiyuan Road, Jurong Economic Development
Zone, Jiangsu Province, P.R.China Postcode: 212400

Manufacturing Address: No.29 Zhiyuan Road, Jurong Economic
Development Zone, Jiangsu Province, P.R.China

Has been assessed and conformed to the following standard(s)

GB/T19001-2016 idt ISO 9001:2015

The certificate is valid for the following scope:

**The Design, Development, Production and Service of
Semi-Automatic Biochemistry Analyzer, Coagulometer Analyzer,
Semi-Automatic Electrolyte Analyzer, Semi-Automatic Microplate
Reader, Microplate Washer, Automatic Urine Analyzer And Urine
Test Strips, Fully Automatic Biochemistry Analyzer, Fully
Automatic Hematology Analyzer,**

Date of issue: July 16, 2019

Date of expiry: July 15, 2024

Director: *Zhugangchen*

**BEIJING HUA GUANG CERTIFICATION
OF MEDICAL DEVICES CO., LTD.**



**MANAGEMENT SYSTEM
CNAS C047 - Q**



Note: The Certificate Information are available on the official website of Certification and Accreditation Administration of the People's Republic of China (www.cnca.gov.cn) or the Website of CMD (www.cmdc.com.cn).

Statement of Compliance

This is to state that Technical Documentation (BS001, Rev 1.0) for Product(s)

Semi-Automatic Biochemistry Analyzer
(Model: SA-30A,SA-30B,SA-30C,SA-20,SA-10)

(IVD products other than those covered by Annex II, IVD for self-testing and devices for Performance evaluation according to manufacturer's declaration)

Manufactured by

CLINDIAG SYSTEMS CO., LTD.

29 Zhiyuan Road, Jurong Economic Development Zone, Zhenjiang,
Jiangsu Province, P.R.China

Has been assessed as meeting the Essential Requirements and relevant provisions of EC Directive 98/79/EEC for in Vitro Diagnostic Medical Device

For SGS-CSTC Standards Technical Services Co., Ltd.
System & Services Certification Division

Reference No: CN/SZH8791-1

Valid from Jan.2018 to Jan.2023

Issued Certificate since Jan.2018



**SGS-CSTC Standards Technical
Services Co., Ltd. Shanghai
Branch**

SGS Bldg, 11/F, Building B, No. 900,
Yishan Road, Xuhui District, Shanghai,
China

While all due care and skill was exercised in carrying out this assessment, SGS-CSTC accepts responsibility only for proven gross negligence. This certificate relates only to the medical device as described in the technical file reviewed on the date shown. Conformance to all the regulatory requirements is the sole responsibility of the manufacturer including the manufacture and quality control of the products. This is not a legal document and cannot be used as such. This certificate remains the property of SGS-CSTC Standards Technical Services Co., Ltd. to whom it must be returned on

Declaration of Conformity



Manufacturer: Shenzhen Mindray Bio-Medical Electronics Co., Ltd.
Mindray Building, Keji 12th Road South, Hi-tech Industrial
Park, Nanshan, Shenzhen, 518057, P. R. China

EC-Representative: Shanghai International Holding Corp. GmbH (Europe)
Eiffestraße 80
20537 Hamburg, Germany

Product: Auto Hematology Analyzer

Model: BC-20s

Including reagents as following:

M-30D DILUENT

M-30CFL LYSE

PROBE CLEANSER

Classification: The device not in IVDD annex II and not for self
testing/performance evaluation

Conformity Assessment Route: IVDD Annex III(excluding Section 6)

We herewith declare that the above mentioned products meet the provisions of the Directive 98/79/EC on In Vitro Diagnostic Medical Devices. All supporting documentations are retained under the premises of the manufacturer.

Standards Applied:

List of (harmonized) standards for which documented evidence for compliance can be provided as attachment.

Start of CE-Marking: 2015-3-31

Place, Date of Issue: Shenzhen, 2015-3-31

Signature:

Name of Authorized Signatory: Mr.tan ChuanBin

Position Held in Company: Manager ,Technical Regulation

Declaration of Conformity



Manufacturer: Shenzhen Mindray Bio-Medical Electronics Co., Ltd.
Mindray Building, Keji 12th Road South, Hi-tech Industrial
Park, Nanshan, Shenzhen, 518057, P. R. China

EC-Representative: Shanghai International Holding Corp. GmbH (Europe)
Eiffestraße 80
20537 Hamburg, Germany

Product: Auto Hematology Analyzer

Model: BC-30s
Including reagents as following:
M-30D DILUENT
M-30CFL LYSE
PROBE CLEANSER

Classification: The device not in IVDD annex II and not for self
testing/performance evaluation

Conformity Assessment Route: IVDD Annex III(excluding Section 6)

We herewith declare that the above mentioned products meet the provisions of the Directive 98/79/EC on In Vitro Diagnostic Medical Devices. All supporting documentations are retained under the premises of the manufacturer.

Standards Applied:

List of (harmonized) standards for which documented evidence for compliance can be provided as attachment.

Start of CE-Marking: 2015-3-31

Place, Date of Issue: Shenzhen, 2015-3-31

Signature:

Name of Authorized Signatory: Mr.tan ChuanBin

Position Held in Company: Manager ,Technical Regulation

Declaration of Conformity V 1.0

Applied Standards List

Product: **Auto Hematology Analyzer**

BC-20s、BC-30s

Including reagents as following:

M-30D DILUENT

M-30CFL LYSE

PROBE CLEANSER

Applied Standards:

EN ISO 18113-1:2011	In vitro diagnostic medical devices — Information supplied by the manufacturer (labelling) Part 1: Terms, definitions and general requirements
EN ISO 18113-2:2011	In vitro diagnostic medical devices - Information supplied by the manufacturer (labelling) - Part 2: In vitro diagnostic reagents for professional use
EN ISO 18113-3:2011	In vitro diagnostic medical devices — Information supplied by the manufacturer (labeling) Part 3: In vitro diagnostic instruments for professional use
EN ISO 15223-1:2012	Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied — Part 1: General requirements
EN 13612: 2002	Performance evaluation of in vitro diagnostic medical devices
ISO 14971:2012	Medical devices – Application of risk management to medical devices
EN 61010-1:2001	Safety requirements for electrical equipment for measurement, control, and laboratory use Part 1: General requirement
EN 61010-2-081:2002+A1: 2003+A1: 2003	Safety requirements for electrical equipment for measurement, control and laboratory use - Part 2-081: Particular requirements for automatic and semi-automatic laboratory equipment for analysis and other purposes
EN 61010-2-101: 2002	Safety requirements for electrical equipment for measurement, control, and laboratory use - Part 2-101: Particular requirements for in vitro diagnostic (IVD) medical equipment
IEC 61010-2-010: 2005	Safety requirements for electrical equipment for measurement, control and

Declaration of Conformity V 1.0

	laboratory use - Part 2-010: Particular requirements for laboratory equipment for the heating of materials
EN 61326-1:2006	Electrical equipment for measurement, control and laboratory use - EMC requirements - Part 1: General requirements
EN 61326-2-6:2006	Electrical equipment for measurement, control and laboratory use - EMC requirements - Part 2-6: Particular requirements - In vitro diagnostic (IVD) medical equipment
EN 62304:2006	Medical device software- Software life cycle processes
EN 62366:2008	Medical devices — Application of usability engineering to medical devices
EN 13640: 2002	Stability testing of in vitro diagnostic medical devices
EN ISO13485:2012	Medical devices - Quality management systems - Requirements for regulatory purposes



America

CERTIFICATE

No. QS5 044751 0140 Rev. 02

Certificate Holder:

**Shenzhen Mindray Bio-Medical
Electronics Co., Ltd.**
Mindray Building
Keji 12th Road South
High-Tech Industrial Park
Nanshan
518057 Shenzhen
PEOPLE'S REPUBLIC OF CHINA

Certification Mark:



Scope of Certificate:

See Page 2 for Overall Scope Statement.

Standard(s):

ISO 9001:2015

The Certification Body of TÜV SÜD America Inc. certifies that the company mentioned above has established and is maintaining a quality management system that meets the requirements of the listed standards.

Report No.:

SH2005501

Effective Date:

2020-08-12

Expiry Date:

2023-06-30

Page 1 of 4

Date of Issue: 2020-08-20

Tina Israel
Manager, US Certification Body,
Medical and Health Services



America

CERTIFICATE

No. QS5 044751 0140 Rev. 02

Overall Scope Statement

Design and Development, Production and Distribution of Medical Electronic Equipment (including Patient Monitor and Accessories, Vital Signs Monitor, Center Monitoring System, Telemetry Monitoring System, Pulse Oximeter, Temperature Probe, Flow Sensor, Ambulatory Blood Pressure Monitor, Defibrillator / Monitor and Accessories, Electrocardiograph, Anesthesia Machine and Accessories, Ventilator, Air Compressor, Endoscope Camera System, Ultrasonic Diagnostic Equipment and Accessories, Digital Radiography System, Radiography System, Hematology Analyzer, Clinical Chemistry Analyzer, Urine Analyzer, Microplate Reader, Microplate Washer for In-Vitro Diagnostic Use, Chemiluminescence Immunoassay Analyzer, Flow Cytometer, (Auto) Sample Processing System, Auto Slide Maker and Stainer, Glycohemoglobin Analyzer, Specific Protein Analyzer), Reagents for Hematology Analyzer, Reagents for Clinical Chemistry Analyzer, Chemiluminescence Immunoassay Reagents, Chemiluminescence Immunoassay Calibrators and Controls, Reagents for Flow Cytometer, Reagents for Glycohemoglobin Analyzer, Calibrators and Controls for Glycohemoglobin Analyzer, Disposable Anesthesia Mask, Reusable Anesthesia Mask, Respiratory Mask, Disposable Breathing Circuit, Reusable Breathing Circuit, Heat and Moisture Exchanger, Filter, Breathing Bag

Page 2 of 4

Date of Issue: 2020-08-20

Tina Israel
Manager, US Certification Body,
Medical and Health Services



America

CERTIFICATE

No. QS 044751 0140 Rev. 02

Facility(ies):

Shenzhen Mindray Bio-Medical Electronics Co., Ltd.
Mindray Building, Keji 12th Road South, High-Tech
Industrial Park, Nanshan, 518057, Shenzhen,
PEOPLE'S REPUBLIC OF CHINA

Facility Scopes:

Design and Development, Production and Distribution of Medical Electronic Equipment (including Patient Monitor and Accessories, Vital Signs Monitor, Center Monitoring System, Telemetry Monitoring System, Pulse Oximeter, Temperature Probe, Flow Sensor, Ambulatory Blood Pressure Monitor, Defibrillator / Monitor and Accessories, Electrocardiograph, Anesthesia Machine and Accessories, Ventilator, Air Compressor, Endoscope Camera System, Ultrasonic Diagnostic Equipment and Accessories, Digital Radiography System, Radiography System, Hematology Analyzer, Clinical Chemistry Analyzer, Urine Analyzer, Microplate Reader, Microplate Washer for In-Vitro Diagnostic Use, Chemiluminescence Immunoassay Analyzer, Flow Cytometer, (Auto) Sample Processing System, Auto Slide Maker and Stainer, Glycohemoglobin Analyzer, Specific Protein Analyzer), Reagents for Hematology Analyzer, Reagents for Clinical Chemistry Analyzer, Chemiluminescence Immunoassay Reagents, Chemiluminescence Immunoassay Calibrators and Controls, Reagents for Flow Cytometer, Reagents for Glycohemoglobin Analyzer, Calibrators and Controls for Glycohemoglobin Analyzer, Disposable Anesthesia Mask, Reusable Anesthesia Mask, Respiratory Mask, Disposable Breathing Circuit, Reusable Breathing Circuit, Heat and Moisture Exchanger, Filter, Breathing Bag

Page 3 of 4

Date of Issue: 2020-08-20

Tina Israel
Manager, US Certification Body,
Medical and Health Services



America

CERTIFICATE

No. QS5 044751 0140 Rev. 02

Facility(ies)

Shenzhen Mindray Bio-Medical Electronics Co., Ltd.
1203 Nanhuan Avenue, Guangming District, 518106
Shenzhen, PEOPLE'S REPUBLIC OF CHINA

Facility Scopes:

Design and Development, Production and Distribution of Medical Electronic Equipment (including Patient Monitor and Accessories, Vital Signs Monitor, Center Monitoring System, Telemetry Monitoring System, Pulse Oximeter, Temperature Probe, Flow Sensor, Ambulatory Blood Pressure Monitor, Defibrillator / Monitor and Accessories, Electrocardiograph, Anesthesia Machine and Accessories, Ventilator, Air Compressor, Endoscope Camera System, Ultrasonic Diagnostic Equipment and Accessories, Digital Radiography System, Radiography System, Hematology Analyzer, Clinical Chemistry Analyzer, Urine Analyzer, Microplate Reader, Microplate Washer for In-Vitro Diagnostic Use, Chemiluminescence Immunoassay Analyzer, Flow Cytometer, (Auto) Sample Processing System, Auto Slide Maker and Stainer, Glycohemoglobin Analyzer, Specific Protein Analyzer), Reagents for Hematology Analyzer, Reagents for Clinical Chemistry Analyzer, Chemiluminescence Immunoassay Reagents, Chemiluminescence Immunoassay Calibrators and Controls, Reagents for Flow Cytometer, Reagents for Glycohemoglobin Analyzer, Calibrators and Controls for Glycohemoglobin Analyzer, Disposable Anesthesia Mask, Reusable Anesthesia Mask, Respiratory Mask, Disposable Breathing Circuit, Reusable Breathing Circuit, Heat and Moisture Exchanger, Filter, Breathing Bag

Page 4 of 4

Date of Issue: 2020-08-20

Tina Israel
Manager, US Certification Body,
Medical and Health Services



Product Service

Certificate

No. Q5 044751 0164 Rev. 02

Holder of Certificate: **Shenzhen Mindray Bio-Medical Electronics Co., Ltd.**

Mindray Building
Keji 12th Road South
High-Tech Industrial Park
Nanshan
518057 Shenzhen
PEOPLE'S REPUBLIC OF CHINA

Certification Mark:



Scope of Certificate: **Design and development, production and distribution of Active medical devices (intended) for monitoring, diagnosis, anesthesia, breathing and intensive care; In-vitro diagnostic instruments; Non-active accessories for breathing therapy and anesthesia; In-vitro diagnostic reagents and kits (intended) for hematology, clinical chemistry, immunology and cell analysis (For detail information see following pages)**

The Certification Body of TÜV SÜD Product Service GmbH certifies that the company mentioned above has established and is maintaining a quality management system, which meets the requirements of the listed standard(s). See also notes overleaf.

Report No.: SH2005501

Valid from: 2020-09-01
Valid until: 2023-08-31

Date, 2020-07-24

Christoph Dicks
Head of Certification/Notified Body

Certificate

No. Q5 044751 0164 Rev. 02

Applied Standard(s): EN ISO 13485:2016
Medical devices - Quality management systems -
Requirements for regulatory purposes
(ISO 13485:2016)
DIN EN ISO 13485:2016

Facility(ies): Shenzhen Mindray Bio-Medical Electronics Co., Ltd.
Mindray Building, Keji 12th Road South, High-Tech Industrial Park,
Nanshan, 518057 Shenzhen, PEOPLE'S REPUBLIC OF CHINA

Shenzhen Mindray Bio-Medical Electronics Co., Ltd.
1203 Nanhuan Avenue, Guangming District, 518106 Shenzhen,
PEOPLE'S REPUBLIC OF CHINA

Certificate

No. Q5 044751 0164 Rev. 02

For the product(s)/product category (ies):

Patient Monitor and Accessories, Vital Signs Monitor,
Center Monitoring System, Telemetry Monitoring System,
Pulse Oximeter, Temperature Probe, Flow Sensor,
Ambulatory Blood pressure Monitor,
Defibrillator/Monitor and Accessories, Electrocardiograph,
Anesthesia Machine and accessories, Ventilator,
Air compressor, Endoscope Camera System,
Ultrasonic Diagnostic Equipment and Accessories,
Digital Radiography System, Radiography System,
Hematology Analyzer, Clinical Chemistry Analyzer,
Urine Analyzer, Microplate Reader,
Microplate Washer for invitro diagnostic use,
Chemiluminescence Immunoassay Analyzer,
Flow Cytometer, (Auto) Sample Processing System,
Auto Slide Maker&Stainer, Glycohemoglobin Analyzer,
Specific Protein Analyzer, Reagents for Hematology Analyzer,
Reagents for Clinical Chemistry Analyzer,
Chemiluminescence Immunoassay Reagents,
Chemiluminescence Immunoassay Calibrators and Controls,
Reagents for Flow Cytometer,
Reagents for Glycohemoglobin Analyzer,
Calibrators and Controls for Glycohemoglobin Analyzer,
Disposable Anesthesia Mask, Reusable Anesthesia Mask,
Respiratory Mask, Disposable Breathing Circuit,
Reusable Breathing Circuit, Heat and Moisture Exchanger,
Filter, Breathing Bag.