

Nystatin NS 100 Units

SD025

Nystatin NS 100 Units discs are used for antimicrobial susceptibility testing of fungal cultures

Composition

*Ingredients	Concentration
Nystatin	100 Units/disc

Susceptibility Test Procedure:

Preparation of Inoculum:

1. Inoculum is prepared by picking five distinct colonies of approximately 1mm from 24 hours old culture grown on Sabouraud Dextrose Agar (M063) and incubated at $35 \pm 2^\circ\text{C}$. Colonies are suspended in 5ml of sterile 0.85% Saline.
2. Vortex the resulting suspension and adjust the turbidity to yield $1 \times 10^6 - 5 \times 10^6$ cells /ml (i.e. 0.5 McFarland standard).

Test Procedure:

1. Prepare plates with Muller Hinton Agar + 2% Glucose + 0.5 mcg/ml Methylene Blue Dye (M1825) for carrying out susceptibility of antifungal discs. The medium in the plates should be sterile and have a depth of about 4 mm.
2. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum (turbidity so adjusted, as to obtain semi confluent growth on the petri plate) and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
3. Apply the discs using aseptic technique. Deposit the discs with centers at least 24 mm apart.
4. Invert the plates and place in an incubator set to $35 \pm 2^\circ\text{C}$ within 15 minutes after the discs are applied.
5. Examine each plate after 20 - 24 hours of incubation. If plate was satisfactorily streaked the resulting zones of inhibition will be uniformly circular and there will be a semi-confluent lawn of growth. Read at 48 hours only when insufficient growth is observed after 24 hours incubation.

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "NS 100" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Muller Hinton Agar + 2% Glucose + 0.5 mcg/ml Methylene Blue Dye after 24-48 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>C.albicans</i> (90028)*	19-27
<i>C.parapsilosis</i> (22019)*	16-25
<i>C.tropicalis</i> (750)*	16-21
<i>C.krusei</i> (6528)*	15-20
<i>C.albicans</i> (10231)	15-23
<i>S.cerevisiae</i> (9763)	17-25

* = Q.C. Strains recommended by CLSI

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Method for Antifungal Disk Diffusion Susceptibility Testing of Yeasts; Approved Guidelines-Second edition Vol.29 No.17, August- 2009 CLSI document M44-A2. For more details refer to this volume

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

* Not for Medicinal Use

IVD

In vitro diagnostic medical device



CE Marking

On receipt store at -20°C



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Revision : 03 / 2022

Polymyxin-B**PB 300 Units****SD029**

Polymyxin-B PB 300 Units discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Polymyxin-B	300 Units/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at $35 \pm 2^\circ\text{C}$ and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Polymyxin-B 300 Units	<i>P.aeruginosa</i>	12	-	11

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "PB 300" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	13-19
<i>P.aeruginosa</i> (27853)	14-18

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

*** Not for Medicinal Use**

In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Revision : 02 / 2022

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Rifampicin**RIF 5mcg****SD030**

Rifampicin RIF 5mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Rifampicin	5mcg /disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Rifampicin 5mcg	<i>Staphylococcus</i> , <i>Enterococcus</i> , <i>Haemophilus influenzae</i> & <i>Haemophilus parainfluenzae</i>	20	17-19	16
	<i>Neisseria meningitidis</i>	25	20-24	19
	<i>S.pneumoniae</i>	19	17-18	16

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "RIF 5" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	8-10
<i>S.aureus</i> (25923)	26-34

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)

*** Not for Medicinal Use**

In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Disclaimer :

Revision : 02 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Streptomycin

S 10 mcg

SD031

Streptomycin S 10mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

Ingredients	Concentration
Streptomycin	10mcg /disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Streptomycin 10mcg	<i>Enterobacteriaceae</i>	15	12-14	11

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "S 10" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	12-20
<i>S.aureus</i> (25923)	14-22

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)

*** Not for Medicinal Use**

In vitro diagnostic medical device



CE Marking

On receipt store at -20°C



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Revision : 02 / 2022

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Amikacin AK 30 mcg

SD035

Amikacin AK 30mcg discs are used for antimicrobial susceptibility testing of of bacterial cultures as per Kirby-Bauer Method

Composition

, Ingredients

"Amikacin

Concentration

30mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby-Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby-Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive mm or more	Intermediate mm	Resistant mm or less
Amikacin 30mcg	<i>Enterobacteriaceae</i> , <i>P.aeruginosa</i> , <i>Acinetobacter</i> , <i>Staphylococcus spp</i>	17	15-16	14

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "AK 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E. coli</i> (25922)	19-26
<i>S.aureus</i> (25923)	20-26
<i>P.aeruginosa</i> (27853)	18-26
<i>S.aureus</i> (29213)	18-24

*= Interpretive criteria & QC ranges as per CLSI & EUCAST standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

* **Not for Medicinal Use**



In vitro diagnostic medical device



CE Marking

On receipt store at -20°C



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Revision : 03 / 2022

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Tetracycline**TE 30 mcg****SD037**

Tetracycline TE 10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby-Bauer Method

Composition

*Ingredients	Concentration
Tetracycline	30 mcg /disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby-Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby-Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial Agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Tetracycline TE 30 mcg	<i>Enterobacteriaceae</i> , <i>Acinetobacter</i>	15	12-14	10
	<i>Staphylococcus</i> , <i>Enterococcus</i> spp. & <i>Neisseria meningitidis</i>	19	15-18	14
	<i>Haemophilus influenzae</i> & <i>Haemophilus parainfluenzae</i>	29	26-28	25
	<i>Neisseria gonorrhoeae</i>	38	31-27	30
	<i>S.pneumoniae</i>	28	25-27	24
	<i>Streptococcus</i> spp. Beta haemolytic group & <i>Viridians</i> group	23	19-22	18

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "TE 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)
<i>E.coli</i> (25922)	18-25
<i>S.aureus</i> (25923)	24-30
<i>S.aureus</i> (29213)*	23-31

* = Interpretive criteria & QC ranges as per EUCAST standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)



In vitro diagnostic medical device



CE Marking

On receipt store at -20°C



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

*** Not for Medicinal Use**

Revision : 02 / 2022

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Cefotaxime CTX 30 mcg (Cephotaxime)

SD040

Cefotaxime (Cephotaxime) CTX 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby-Bauer Method

Composition

Ingredients	Concentration
Cefotaxime (Cephotaxime)	30 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby-Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby-Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Cefotaxime (Cephataxime) CTX 30 mcg	<i>Enterobacteriaceae</i>	26	23-25	22
	<i>P.aeruginosa, Acinetobacter & Staphylococcus</i>	23	15-22	14
	<i>Haemophilus influenzae & Haemophilus parainfluenzae</i>	26	-	-
	<i>Neisseria meningitidis</i>	34	-	-
	<i>Neisseria gonorrhoeae</i>	31	-	-
	<i>Streptococcus spp. Viridians group</i>	28	26-27	25
	<i>Streptococcus spp. beta haemolytic group</i>	24	-	-

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CTX 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	29 - 35
<i>S.aureus</i> (25923)	25 - 31
<i>P.aeruginosa</i> (27853)	18 - 22

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.



In vitro diagnostic medical device



CE Marking

On receipt store at  -20°
Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,

www.cepartner4u.eu

Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Cefoxitin (Cephoxitin)**CX****30 mcg****SD041**

Cefoxitin (Cephoxitin) CX 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby- Bauer Method

Composition***Ingredients**

	Concentration
Cefoxitin (Cephoxitin)	30 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby- Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby- Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Cefoxitin (Cephoxitin) 30 mcg	<i>Enterobacterales</i>	16	13-15	14
	<i>For S.aureus & S.lugdunensis</i>	22	-	21
	<i>For Coagulase- negative Staphylococci except S.lugdunensis & S.pseudintermedius</i>	25	-	24
	<i>Neisseria gonorrhoeae</i>	28	24-27	23

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CX 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	23-29
<i>S.aureus</i> (25923)	23-29

* = Interpretive criteria & QC ranges as per CLSI & EUCAST standards.

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

*** Not for Medicinal Use**

In vitro diagnostic medical device



CE Marking




Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Revision : 03 / 2022

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Tobramycin

TOB 10 mcg

SD044

Tobramycin TOB 10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Tobramycin	10 mcg /disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Tobramycin 10 mcg	<i>Enterobacteriaceae</i> , <i>P.aeruginosa</i> , <i>Acinetobacter</i> & <i>Staphylococcus</i>	15	13-14	12

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "TOB 10" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	18-26
<i>S.aureus</i> (25923)	19-29
<i>P.aeruginosa</i> (27853)	19-25

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)

*** Not for Medicinal Use**

In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Disclaimer :

Revision : 02 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Cefazolin CZ 30 mcg**SD047**

Cefazolin CZ 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby- Bauer Method

Composition

*Ingredients	Concentration
Cefazolin	30 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby- Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby- Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Cefazolin 30 mcg	<i>Enterobacterales</i>	23	20-22	19
	<i>Enterobacterales</i> (uncomplicated UTI's)	15	-	14
	<i>Staphylococcus spp</i>	18	15-17	14

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CZ 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	21-27
<i>S.aureus</i> (25923)	29-35

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

* **Not for Medicinal Use**



In vitro diagnostic medical device



CE Marking

On receipt store at



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Revision : 02 / 2022

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Clindamycin**CD 2 mcg****SD051**

Clindamycin CD 2 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

, Ingredients	Concentration
Clindamycin	2 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Clindamycin 2 mcg	<i>Staphylococcus</i>	21	15-20	14
	<i>S.pneumoniae</i> , <i>Streptococcus</i> spp. <i>Viridians</i> group, <i>Streptococcus</i> spp. <i>beta haemolytic</i> group	19	16-18	15

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CD 2" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>S.aureus</i> (25923)	24-30

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood


For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

*** Not for Medicinal Use**

In vitro diagnostic medical device



CE Marking




Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U, Esdoornlaan 13, 3951
DB Maam The Netherlands,
www.cepartner4u.eu

Revision : 03 / 2022

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Norfloxacin NX 10 mcg**SD057**

Norfloxacin NX 10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition***Ingredients Concentration**

Norfloxacin 10 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Norfloxacin 10 mcg	<i>Enterobacteriaceae</i> , <i>P.aeruginosa</i> , <i>Staphylococcus</i> & <i>Enterococcus</i>	17	13-16	12

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "NX 10" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	28-35
<i>S.aureus</i> (25923)	17-28
<i>P.aeruginosa</i> (27853)	22-29
<i>S.aureus</i> (29213)	18-24
<i>E.faecalis</i> (29212)	16-22

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)


* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Disclaimer :

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Revision : 03 / 2022

Ciprofloxacin**CIP 5 mcg****SD060**

Ciprofloxacin CIP 5 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Ciprofloxacin	5 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Ciprofloxacin 5 mcg	<i>Enterobacteriaceae other than S.Typhi</i> and extraintestinal <i>Salmonella</i> spp., <i>P.aeruginosa</i> , <i>Acinetobacter</i> , <i>Staphylococcus</i> & <i>Enterococcus</i>	21	16-20	15
	For <i>S.Typhi</i> and extraintestinal <i>Salmonella</i> spp.	31	21-30	20
	<i>Haemophilus influenzae</i> & <i>Haemophilus parainfluenzae</i>	21	-	-
	<i>Neisseria meningitidis</i>	35	33-34	32
	<i>Neisseria gonorrhoeae</i>	41	28-40	27

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CIP 5" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	29-37
<i>S.aureus</i> (25923)	22-30
<i>P.aeruginosa</i> (27853)	25-33
<i>S.aureus</i> (29213)	21-27
<i>E.faecalis</i> (29212)	19-25

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test


For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : *Haemophilus* Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

* Not for Medicinal Use

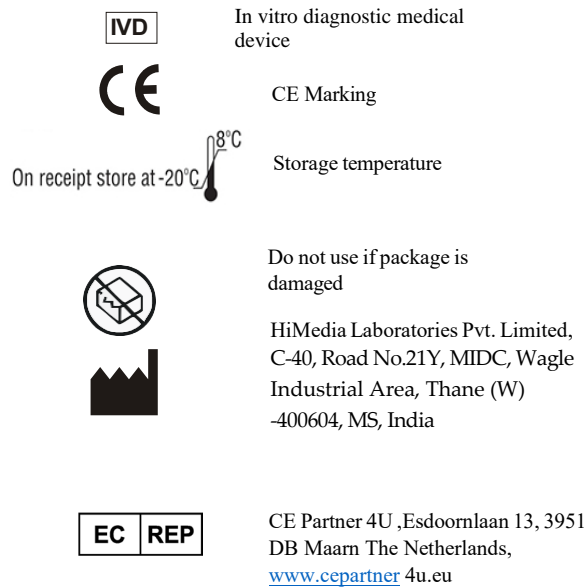

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Cefuroxime**CXM 30 mcg****SD061**

Cefuroxime CXM 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Cefuroxime	30 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Cefuroxime 30 mcg	<i>Enterobacteriaceae</i> & <i>Staphylococcus</i>	18	15-17	14
	<i>Haemophilus influenzae</i> & <i>Haemophilus parainfluenzae</i>	20	17-19	16
	<i>Neisseria gonorrhoeae</i>	31	26-30	25

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CXM 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	20-26
<i>S.aureus</i> (25923)	27-35

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

* **Not for Medicinal Use**

Ceftazidime**CAZ 30 mcg****SD062**

Ceftazidime CAZ 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Ceftazidime	30 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Ceftazidime 30 mcg	<i>Enterobacteriaceae, B.cepacia</i>	21	18-20	17
	<i>P.aeruginosa, Acinetobacter & Staphylococcus</i>	18	15-17	14
	<i>Haemophilus influenzae & Haemophilus parainfluenzae</i>	26	-	-
	<i>Neisseria gonorrhoeae</i>	31	-	-

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CAZ 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	25-32
<i>S.aureus</i> (25923)	16-20
<i>P.aeruginosa</i> (27853)	22-29
<i>K.pneumoniae</i> (700603)	10-18

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood


For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

*** Not for Medicinal Use**

IVD

In vitro diagnostic medical
device

CE Marking

On receipt store at 

Storage temperature

Do not use if package is
damagedHiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India

EC REP

CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu**Disclaimer :**

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Ceftazidime CAZ 10 mcg

SD062A

Ceftazidime CAZ 10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Kirby- Bauer Method

Composition

*Ingredients	Concentration
--------------	---------------

Ceftazidime	10 mcg/disc
-------------	-------------

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Kirby- Bauer Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at $35 \pm 2^\circ\text{C}$ and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Kirby- Bauer Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CAZ 10" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	23 - 29
<i>P.aeruginosa</i> (27853)	21 - 27
<i>K.pneumoniae</i> (700603)	6 - 12

* = QC ranges as per EUCAST standards

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



On receipt store at

Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Amoxyclav AMC 30 mcg (Amoxycillin/Clavulanic acid) (20/10mcg)

SD063

Amoxyclav (Amoxycillin/Clavulanic acid) AMC 30mcg (20/10mcg) discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Amoxyclav (Amoxycillin/Clavulanic acid)	30mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive mm or more	Intermediate mm	Resistant mm or less
Amoxyclav (Amoxycillin/Clavulanic acid) 30mcg (20/10mcg)	<i>Enterobacteriaceae</i>	18	14-17	13
	<i>Haemophilus influenzae</i> & <i>Haemophilus parainfluenzae</i>	20	-	19

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "AMC 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E. coli</i> (25922)	18-24
<i>S. aureus</i> (25923)	28-36
<i>E. coli</i> (35218)	17-22

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S. pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C. Agar +1% defined growth supplement (M434 + FD025)

*** Not for Medicinal Use****IVD**

In vitro diagnostic medical device



CE Marking

On receipt store at 

Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India

EC REP

CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Ceftriaxone**CTR 30 mcg****SD065**

Ceftriaxone CTR 30 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Ceftriaxone	30 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Ceftriaxone 30 mcg	<i>Enterobacteriaceae</i>	23	20-22	19
	<i>P.aeruginosa, Acinetobacter & Staphylococcus</i>	21	14-20	13
	<i>Haemophilus influenzae & Haemophilus parainfluenzae</i>	26	-	-
	<i>Neisseria meningitidis</i>	34	-	-
	<i>Neisseria gonorrhoeae</i>	35	-	-
	<i>Streptococcus spp. Viridians group</i>	27	25-26	24
	<i>Streptococcus spp. beta haemolytic group</i>	24	-	-

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CTR 30" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	29-35
<i>S.aureus</i> (25923)	22-28
<i>P.aeruginosa</i> (27853)	17-23
<i>K.pneumoniae</i> (700603)	16-24

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spp : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spp : G.C.Agar +1% defined growth supplement (M434 + FD025)

* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking



On receipt store at


Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Cefoperazone CPZ 75 mcg

SD072

Cefoperazone CPZ 75 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Cefoperazone	75 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Cefoperazone 75 mcg	<i>Enterobacteriaceae, P.aeruginosa</i>	21	16-20	15

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "CPZ 75" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	28-34
<i>S.aureus</i> (25923)	24-33
<i>P.aeruginosa</i> (27853)	23-29

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

Discs should always be stored at -20°C to +8°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

* Not for Medicinal Use



In vitro diagnostic medical device



CE Marking

On receipt store at -20°C



Storage temperature



Do not use if package is damaged



HiMedia Laboratories Pvt. Limited,
C-40, Road No.21Y, MIDC, Wagle
Industrial Area, Thane (W)
-400604, MS, India



CE Partner 4U ,Esdoornlaan 13, 3951
DB Maarn The Netherlands,
www.cepartner4u.eu

Disclaimer :

Revision : 03 / 2022

User must ensure suitability of the product(s) in their application prior to use. Products conform solely to the information contained in this and other related HiMedia™ publications. The information contained in this publication is based on our research and development work and is to the best of our knowledge true and accurate. HiMedia™ Laboratories Pvt Ltd reserves the right to make changes to specifications and information related to the products at any time. Products are not intended for human or animal diagnostic or therapeutic use but for laboratory, research or further manufacturing use only, unless otherwise specified. Statements contained herein should not be considered as a warranty of any kind, expressed or implied, and no liability is accepted for infringement of any patents.

Imipenem IPM 10 mcg**SD073**

Imipenem IPM 10 mcg discs are used for antimicrobial susceptibility testing of bacterial cultures as per Bauer-Kirby Method

Composition

*Ingredients	Concentration
Imipenem	10 mcg/disc

Susceptibility Test Procedure:

1. Prepare plates with Mueller Hinton Agar (M173/M1084) for rapidly growing aerobic organisms as per Bauer-Kirby Method. The medium in the plates should be sterile and should have a depth of about 4 mm.
2. Inoculate 4-5 similar colonies with a wire, needle or loop to 5 ml Tryptone Soya Broth (M011) and incubate at 35-37°C for 2-8 hours until light to moderate turbidity develops. Compare the inoculum turbidity with that of standard 0.5 McFarland (prepared by mixing 0.5 ml of 1.175% barium chloride and 99.5 ml of 0.36N sulfuric acid). Dilute the inoculum or incubate further as necessary to attain comparative turbidity. Alternatively, the inoculum can be standardized by other appropriate optical method (0.08 - 0.13 OD turbid suspension at 625 nm)
3. Dip a sterile non-toxic cotton swab on a wooden applicator into the standardized inoculum and rotate the soaked swab firmly against the upper inside wall of the tube to express excess fluid. Streak the entire agar surface of the plate with the swab three times, turning the plate at 60° angle between each streaking. Allow the inoculum to dry for 5 - 15 minutes with lid in place.
4. Apply the discs using aseptic technique. When using cartridges, the discs can be applied using the specially designed applicator. When the vials are used, apply the discs using sterile forceps.
5. Deposit the discs with centers at least 24 mm apart. For fastidious organisms and for Penicillins and Cephalosporins, the discs should preferably be deposited with centers 30 mm apart.
6. Incubate immediately at 35 ± 2°C and examine after 16-18 hours or longer, if necessary. For fastidious organisms incubate at appropriate temperature and time.
7. Measure the zones showing complete inhibition and record the diameters of the zones to the nearest millimeter using a calibrated instrument like zone scales (PW096/PW297)

Principle:

Antimicrobial susceptibility testing (AST) of bacterial and fungal isolates is a common and important technique in most clinical laboratories. The results of these tests are used for selection of the most appropriate antimicrobial agent(s) for treatment against the infectious organisms. Till the 1950s, laboratories were lacking in the methodologies and equipments for the accurate determination of in vitro responses of organisms to antimicrobial agents. Bauer et al (1) began the development of standardized methods for antimicrobial susceptibility testing, using disc diffusion system. However the susceptibility results may not always correlate with the patient's response to therapy. The response of an infected patient to antimicrobial agent(s) is a complex interrelationship of host responses, drug dynamics and microbial activity. Antimicrobial susceptibility tests are either quantitative or qualitative. Disc diffusion test is a qualitative test method. The National Committee for Clinical Laboratory Standards (NCCLS), now known as Clinical Laboratory Standards Institute (CLSI) has published comprehensive documents regarding the disc diffusion systems. The agar disc diffusion test is the most convenient and widely used method for routine antimicrobial susceptibility testing. In subsequent and current practice, antimicrobial impregnated paper discs are applied onto the agar surface. Based on the Bauer-Kirby Method, standardized reference procedures for the disc systems were published by WHO and FDA and are periodically updated by the CLSI (formerly NCCLS)(2). For any antimicrobial testing, Quality control or clinical testing, the method to be followed is the same as mentioned above.

However few precautions are to be maintained while handling of the Sensitivity discs,

- On receipt the discs are to be immediately stored at the recommended temperature.
- Medium preparation, Inoculum preparation and incubation to be done as specified.

Interpretation:

Use following interpretive criteria for susceptibility categorization*

Antimicrobial agent	Interpretative criteria for	Sensitive	Intermediate	Resistant
		mm or more	mm	mm or less
Imipenem 10 mcg	<i>Enterobacteriaceae</i>	23	20-22	19
	<i>P.aeruginosa</i>	19	16-18	15
	<i>Acinetobacter, Staphylococcus</i>	16	14-15	13
	<i>Haemophilus influenzae & Haemophilus parainfluenzae</i>	16	-	-

Quality Control:

Appearance: Filter paper discs of 6mm diameter with printed "IPM 10" on centre of each side of the disc.

Cultural response: Average diameter of zone of inhibition observed on Mueller Hinton Agar (M173) after 18 hours incubation at 35-37°C for standard cultures.

Organisms (ATCC)	Std. zone of diameter (mm)*
<i>E.coli</i> (25922)	26-32
<i>P.aeruginosa</i> (27853)	20-28
<i>E.faecalis</i> (29212)	24-30

* = Interpretive criteria & QC ranges as per CLSI standards.

Storage and Shelf-life:

On receipt discs should always be stored at -20°C under dry conditions, along with the dessicator provided in individual pack. Use before expiry date on the label.

References:

1. Bauer, Kirby, Sherris and Turck, 1966, Am. J. Clin. Path., 45: 493
2. Performance standards of Antimicrobial Disc Susceptibility Tests, M100S, 32nd Ed., CLSI Vol. 42 No.2, Feb-2022.
3. EUCAST, Breakpoint tables for interpretation of MIC's & zone diameters, version 12.0, valid from 01.01.2022.

Note :

Use following media to carry out susceptibility test

For rapidly growing aerobic organisms : Mueller Hinton Agar (M173/M1084)

For *Haemophilus* spps : Haemophilus Test Agar (M1259 + FD117)

For *S.pneumoniae* : Muller Hinton Agar supplemented with 5% Sheep Blood

For *Neisseria* spps : G.C.Agar +1% defined growth supplement (M434 + FD025)

* **Not for Medicinal Use**