


VASCO+10 & VASCO+18

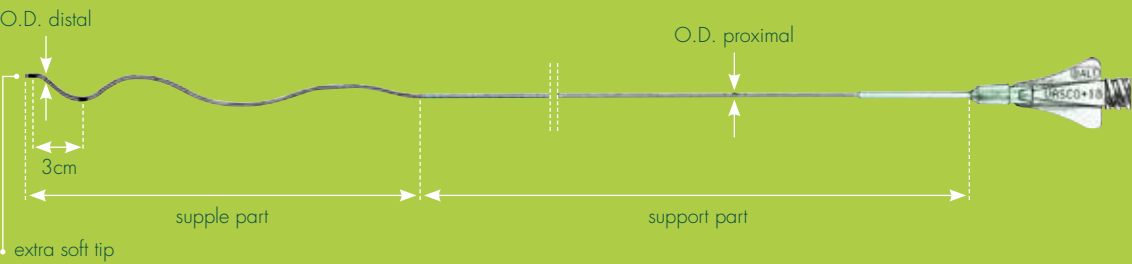

ordering information

Developed portfolio with large range

Vasco+	Reference	Proximal O.D. - Distal O.D.	I.D.	Total length (cm)	Recommended max guidewire	No. of ORX markers	Curve
	VASCO+10 (D-MP)	2,2F to 1,9F	.017"	155	.014"	2	Straight (D)
	VASCO+10MH (D-MP)					3	
	VASCO+18 (D-MP)	2,7F to 2,1F	.021"	155	.018"	2	Multipurpose (MP)
	VASCO+21 (D-MP)	2,7F to 2,4F	.024"	155	.021"	1	
	VASCO+25 (D-MP)	3,3F to 3,0F	.029"	155	.025"	1	
	VASCO+28 (D-MP)	3,4F to 3,3F	.032"	155	.028"	1	
	VASCO+35 (D-MP)	4,0F to 3,8F	.040"	135	.035"	1	
	VASCO+35ASPI (D-MP)	5,1F to 5,1F	.040"	140	.035"	1	

VASCO+ Delivery compatibilities

	LEO+	SILK+	CATCH+	CATCHVIEW	COILS/PARTICLES	Other device
VASCO+10	LEO+ baby 2,0 to 3,0		CATCH+ MINI	CATCHVIEW MINI	Optima coils, Barricade coils & other coils*	compatible with I.D. .017"*
VASCO+10MH						
VASCO+18			CATCH+	CATCHVIEW & CATCHVIEW MAXI	other coils*	compatible with I.D. .021"*
VASCO+21	LEO+ 3,5	SILK+ 2,0 to 4,5	CATCH+ MAXI		Particle injection*	compatible with I.D. .024"*
VASCO+25	LEO+ 4,5	SILK+ 5,0 & 5,5			Particle injection*	compatible with I.D. .029"*
VASCO+28	LEO+ 5,5				Particle injection*	compatible with I.D. .032"*
VASCO+35					Particle injection*	compatible with I.D. .040"*

*check compatibility on products labelling

Vasco+ is a reinforced micro-catheter intended: for injection of diagnostic or therapeutic products; to position pushable coils "SPIRALES" or detachable coils especially the ones of MDS « mechanical detachment system »; for the use of the self-expanding stent LEO+ or SILK+. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. Not reimbursed. First CE marking: 2004. The self-expandable SILK+ stents and SILK Vista Baby are designed for the treatment of intracranial aneurysms and should be used only by clinicians trained in the placement of intracranial stents. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. Not reimbursed. First CE marking: 2012. The self-expandable LEO+/LEO+ Baby stent is designed for the treatment of intracranial aneurysms in association with embolization coils. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. French reimbursement codes 3101316 and 3171593. First CE marking: 2007 (LEO+), 2012 (LEO+Baby). CATCH+ and CATCHView are designed for use in the flow restoration of patients with ischemic stroke due to large intracranial vessel occlusion. They are indicated to restore blood flow in the neurovasculature of patients who are ineligible for intravenous tissue plasminogen activator (IV t-PA), who fail IV t-PA therapy or as a supplement treatment of initiated IV t-PA therapy. The CATCH+ and CATCHView thromboembolectomy devices should only be used by physicians trained in interventional neuroradiology and treatment of ischemic stroke. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT EXTRUSION SAS. Carefully read the instructions for use before use. Not reimbursed. First CE marking: 2012 (CATCH+), 2018 (CATCHView). The Optima Coil System is intended for use in the peripheral and neuro-vasculature to endovascularly obstruct or occlude blood flow in vascular abnormalities of the neurovascular and peripheral vessels. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT USA, LLC. Carefully read the instructions for use before use. French reimbursement code 3162217. First CE marking: 2017. The Barricade Coil System (BCS) is intended for the endovascular embolization of intracranial aneurysms and other neurovascular abnormalities such as arteriovenous malformations and arteriovenous fistulae. The BCS is also intended for vascular occlusion of blood vessels within the neurovascular system to permanently obstruct blood flow to an aneurysm or other vascular malformation and for arterial and venous embolizations in the peripheral vasculature. The device should only be used by physicians who have undergone pre-clinical training in all aspects of BCS procedures as prescribed by Balt. Class III CE0297 in compliance with Medical Device Directive (MDD 93/42/EEC amended by 2007/47/EC). Manufactured by BALT USA, LLC. Carefully read the instructions for use before use. First CE-Mark: 2012.

The content of this document, in particular data, information, trademarks and logos is BALT SAS and affiliate's sole property. © 2019 BALT SAS and affiliates, all rights reserved. All representation and/or reproduction, whether in part or in full, is forbidden and would be considered a violation of BALT SAS and affiliates' copyrights and other intellectual proprietary rights. This document with associated pictures is non-contractual and is solely dedicated to healthcare professionals and BALT's distributors (BALT's supplier's distributors). The products commercialized by BALT shall exclusively be used in accordance with the instructions for use included in the boxes. DC045GB (05/19)

Balt
10, rue de la Croix Vigneron, 95160 Montmorency, France
Tél. : +33 (0)1 39 89 46 41
Fax : +33 (0)1 34 17 03 46
www.balt.fr




vasco⁺
selective braided
microcatheter



vasco⁺

Selective braided microcatheter

Designed to provide access and support in the treatment of intracranial aneurysms & mechanical thrombectomy.

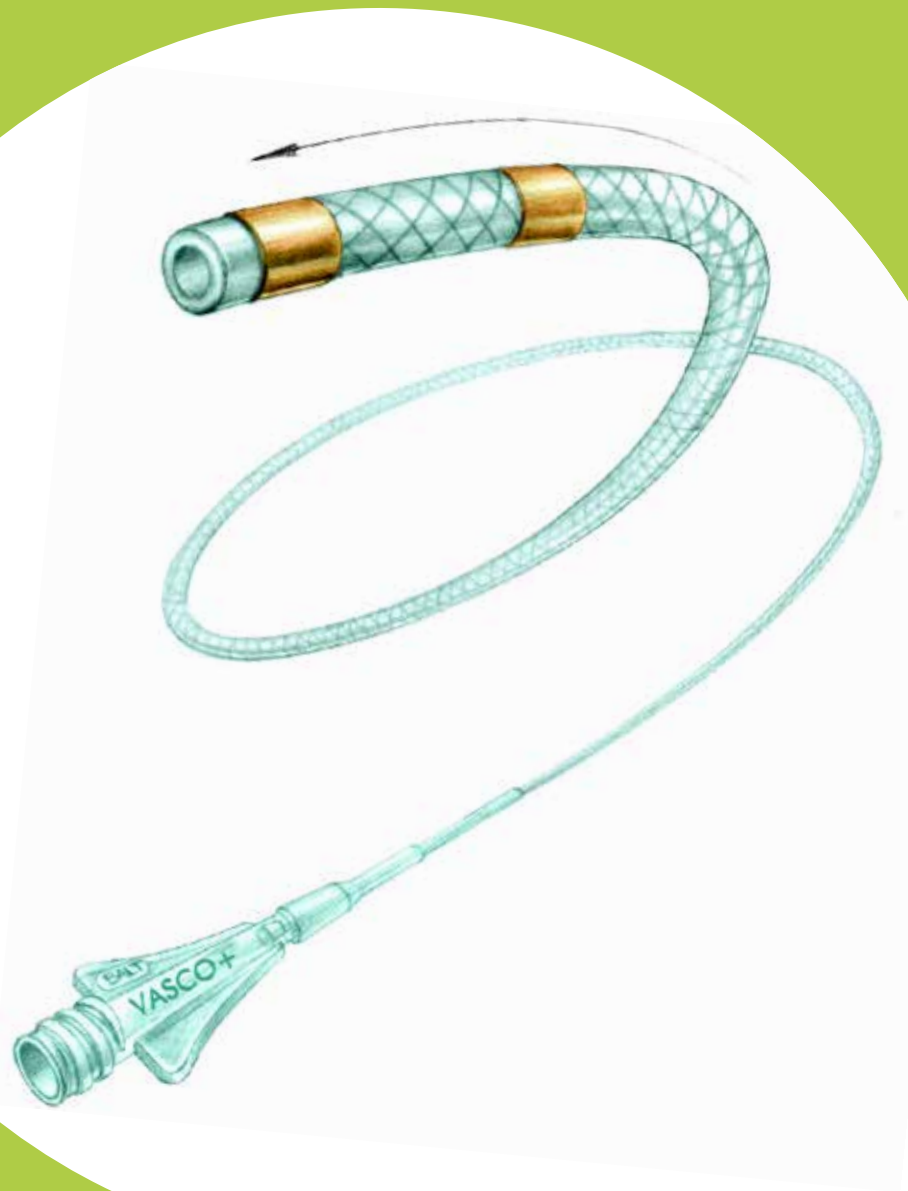

progressive
braiding

High support &
progressive suppleness

Progressive braiding along
the microcatheter:

proximal wide braiding for **more stability**


distal tight braiding for **flexibility &
kink resistance**

Ease of navigability and
controlled deliverability

Smooth navigation & deliverability
enhanced by a hydrophilic coated
distal part & the PTFE* inner coating

Gentle access
allowed by supple-tip

Visibility
full radiopaque microcatheter
(Vasco+ 21, 25, 28 & 35)

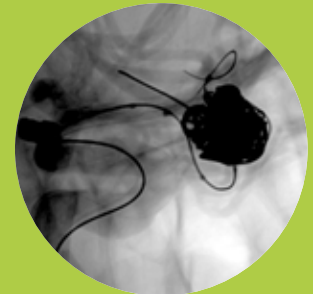

access
treatment




A 3rd marker to
assist coil delivery

Vasco MH (Michael Holt)

3 radiopaque markers
to support:

- coil positioning in
aneurysm sac
- coil selection thanks to
a visual feedback
(5mm second marker)

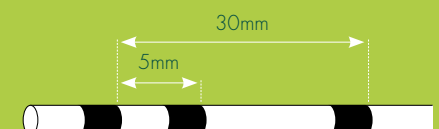

*Polytétrafluoroéthylène