




# Certificate of Conformity

KIT : **Aflatoxin B1 ELISA Kit** **RNM98007**

Release Date **Nov20<sup>th</sup> 2023**  
 Expiration Date: **Nov19<sup>th</sup> 2024**      Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	1.840	1.810	1.750	1.790	0.046	2.560	100%
0.02ppb Calibrator	1.609	1.560	1.540	1.570	0.036	2.261	87.7%
0.06ppb Calibrator	1.297	1.285	1.279	1.283	0.009	0.714	71.7%
0.2 ppb Calibrator	0.810	0.805	0.800	0.803	0.005	0.623	44.9%
0.6 ppb Calibrator	0.411	0.407	0.401	0.400	0.005	1.258	22.3%
1.5 ppb Calibrator	0.179	0.175	0.169	0.170	0.005	2.961	9.5%

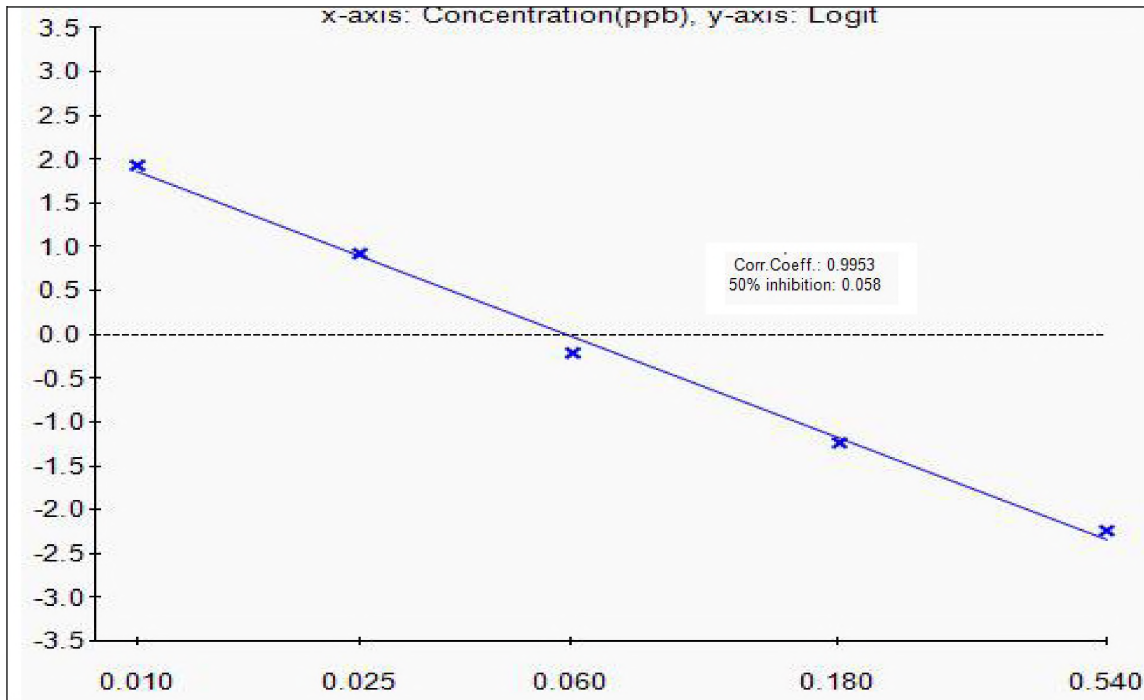

Note: The absorbance of the calibrators may Decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date Nov.20<sup>th</sup> 2023





REAGEN


# Certificate of Conformity

KIT : **Furaltadone (AMOZ) ELISA Kit RND99012**

Release Date **May.18<sup>th</sup>, 2023**  
Expiration Date: **May.17<sup>th</sup>, 2024**      Temperature: **25°C**

REAGEN LLC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2.533	2.501	2.525	2.52	0.0167	0.661	100.00%
0.05 ppb Calibrator	2.164	2.144	2.124	2.144	0.0200	0.933	85.08%
0.15 ppb Calibrator	1.703	1.658	1.685	1.682	0.0226	1.347	66.75%
0.45ppb Calibrator	0.871	0.853	0.845	0.856	0.0133	1.556	33.97%
1.35 ppb Calibrator	0.222	0.213	0.241	0.225	0.0143	6.353	8.93%
4.05 ppb Calibrator	0.089	0.095	0.088	0.091	0.0038	4.160	3.61%

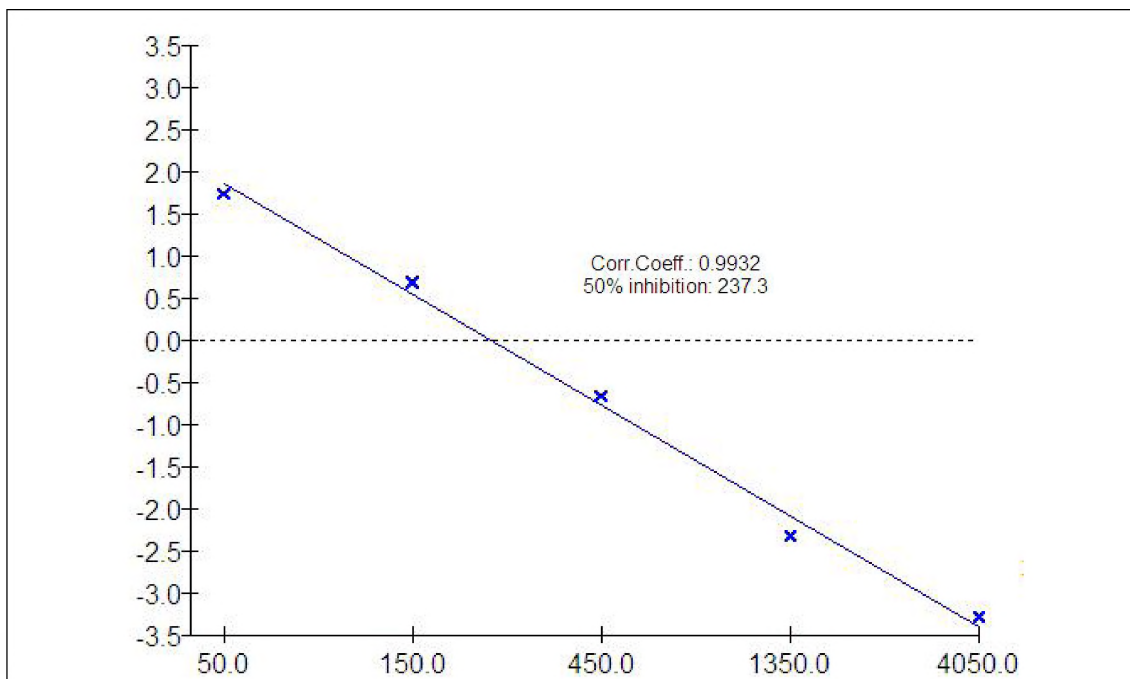

Note: The absorbance of the calibrators may decrease during the shelf life of kit. Actual values may vary; this data is for example purposes only.

QA Manager Alexis      Release Date May.18<sup>th</sup>, 2023

REAGEN



REAGEN


# Certificate of Conformity

KIT : **Furazolidone (AOZ) ELISA Kit RND99011**

Release Date: Aug.10<sup>th</sup>, 2023  
Expiration Date: Aug.09<sup>th</sup>, 2024      Temperature: 25°C

REAGEN LLC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2.285	2.24	2.254	2.26	0.0230	1.019	100.00%
0.02 ppb Calibrator	2.142	2.077	2.099	2.106	0.0331	1.570	93.19%
0.06 ppb Calibrator	1.807	1.835	1.854	1.832	0.0236	1.291	81.06%
0.18 ppb Calibrator	0.996	1.012	0.992	1.0	0.0110	1.097	44.25%
0.54 ppb Calibrator	0.403	0.426	0.425	0.418	0.0130	3.110	18.50%
1.62 ppb Calibrator	0.164	0.158	0.170	0.164	0.0108	6.326	7.26%

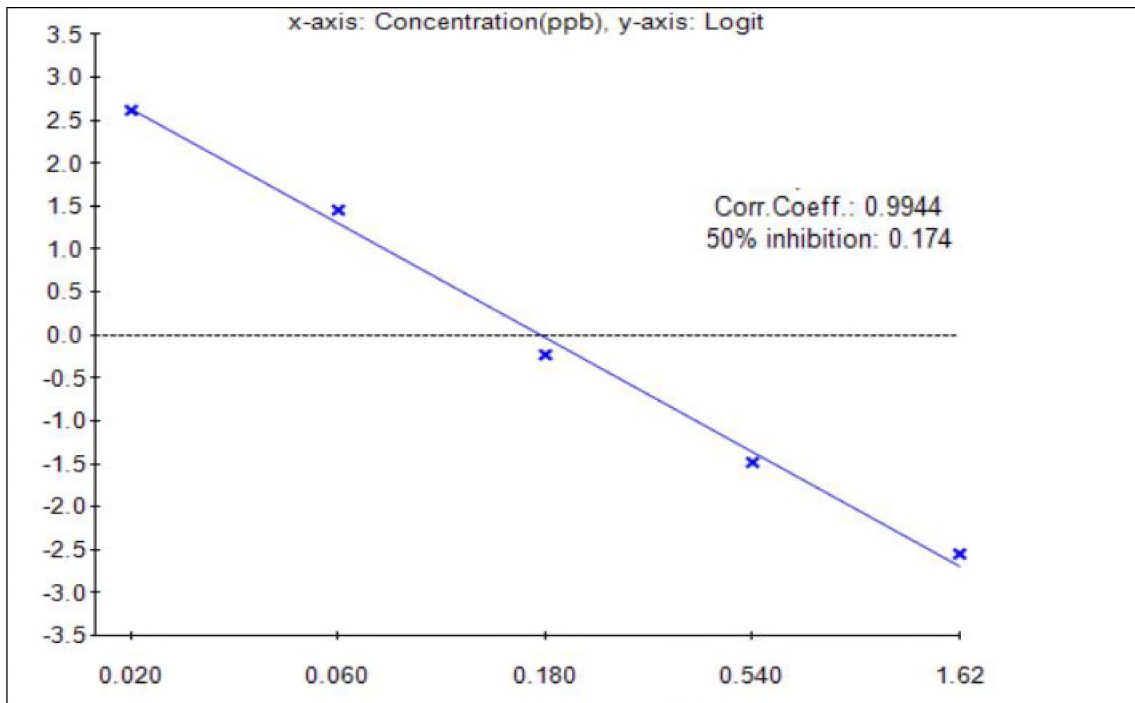

Note: The absorbance of the calibrators may decrease during the shelf life of kit. Actual values may vary; this data is for example purposes only.

QA Manager Alexis      Release Date Aug.10<sup>th</sup>, 2023






# Certificate of Conformity

KIT : **Chloramphenicol ELISA Kit RND99001**

Release Date: Oct.20<sup>th</sup> 2023  
 Expiration Date: Oct.19<sup>th</sup> 2024      Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2.189	2.129	2.165	2.161	0.0302	1.397	100.00%
0.05ppb Calibrator	1.954	1.898	1.925	1.926	0.0280	1.454	89.13%
0.15ppb Calibrator	1.623	1.624	1.632	1.626	0.0049	0.303	75.24%
0.5 ppb Calibrator	1.019	1.043	1.026	1.029	0.0123	1.199	47.62%
1.5 ppb Calibrator	0.519	0.534	0.528	0.527	0.0075	1.433	24.39%
4.5 ppb Calibrator	0.239	0.23	0.241	0.237	0.0059	2.472	10.97%

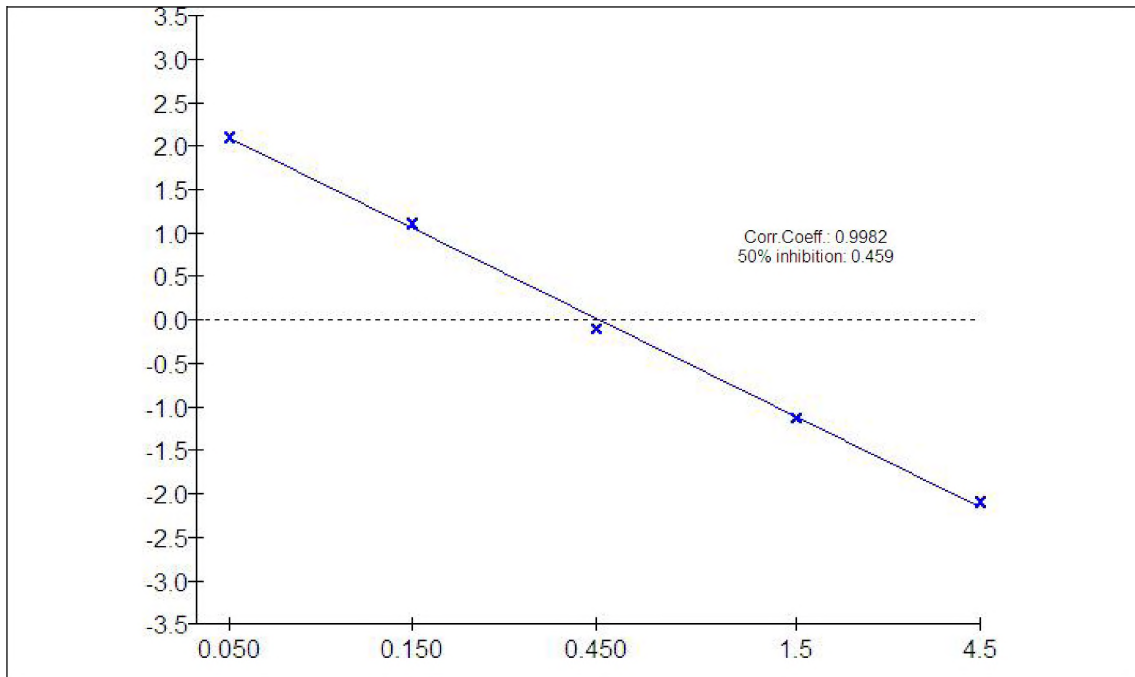

Note: The absorbance of the calibrators may Decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis      Release Date Oct.20<sup>th</sup> 2023






# Certificate of Conformity

KIT : **Deoxynivalenol (DON) ELISA Kit RNM98004**

Release Date Dec.20<sup>th</sup> 2023  
 Expiration Date: Dec.19<sup>th</sup> 2024 Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	B/Bo
Negative Control	2. 271	2. 189	2. 215	2. 225	0. 0419	1. 883	100%
2 ppb Calibrator	2. 081	1. 889	2. 011	1. 994	0. 0972	4. 874	89. 6%
6 ppb Calibrator	1. 783	1. 605	1. 718	1. 702	0. 0901	5. 292	76. 5%
18 ppb Calibrator	1. 316	1. 215	1. 289	1. 273	0. 0523	4. 107	57. 2%
54 ppb Calibrator	0. 871	0. 714	0. 758	0. 781	0. 0810	10. 370	35. 1%
162 ppb Calibrator	0. 511	0. 458	0. 496	0. 488	0. 0273	5. 594	21. 9%

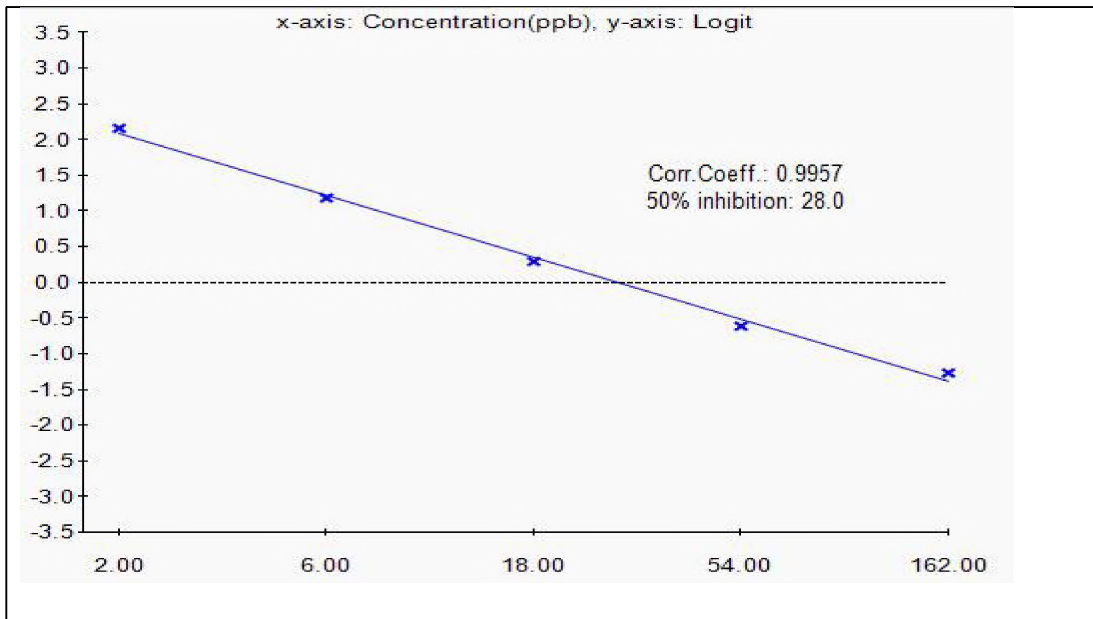

Note: The absorbance of the calibrators may decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date Dec.20<sup>th</sup> 2023






# Certificate of Conformity

KIT : **Total Aflatoxin ELISA Kit RNM98006**  
 Release Date Jan.20<sup>th</sup>, 2024  
 Expiration Date: Jan.19<sup>th</sup>, 2025 Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	1.93	1.926	1.952	1.936	0.0140	0.723	100%
0.02ppb Calibrator	1.52	1.55	1.49	1.520	0.0300	1.974	78.51%
0.06ppb Calibrator	1.08	1.09	1.091	1.087	0.0061	0.560	56.15%
0.2 ppb Calibrator	0.59	0.599	0.596	0.595	0.0046	0.770	30.73%
0.6 ppb Calibrator	0.302	0.292	0.285	0.293	0.0085	2.916	15.13%
1.5 ppb Calibrator	0.13	0.14	0.135	0.135	0.0050	3.704	6.97%

x-axis: Concentration(ppb), y-axis: Logit

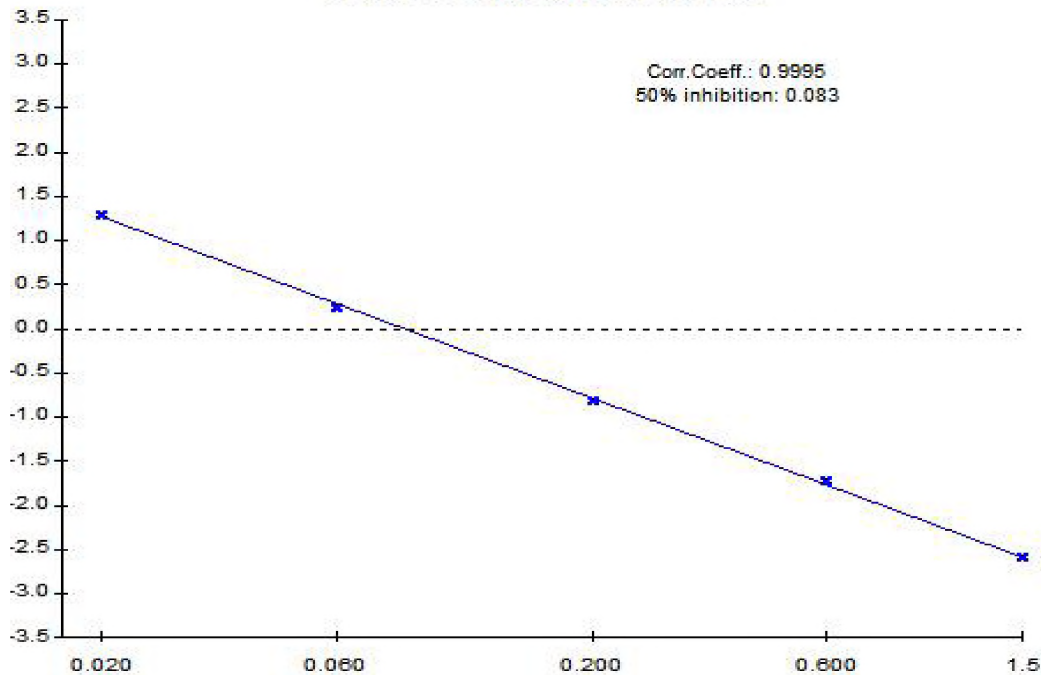

Note: The absorbance of the calibrators may Decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis

Release Date Jan.20<sup>th</sup>, 2024








# Certificate of Conformity

KIT : **Aflatoxin M1 ELISA Kit RNM98001-1**  
 Release Date: Sep.26<sup>th</sup>, 2023  
 Expiration Date: Sep.25<sup>th</sup>, 2024      Temperature: 25°C

REAGEN LLC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2.608	2.598	2.594	2.600	0.0072	0.277	100.00%
0.01 ppb Calibrator	2.20	2.19	2.15	2.18	0.0265	1.214	83.85%
0.025 ppb Calibrator	1.807	1.797	1.757	1.787	0.0265	1.481	68.73%
0.06 ppb Calibrator	1.18	1.17	1.13	1.212	0.0265	2.281	44.62%
0.18 ppb Calibrator	0.599	0.589	0.549	0.579	0.0265	4.570	22.27%
0.54ppb Calibrator	0.302	0.292	0.252	0.282	0.0265	9.382	10.85%

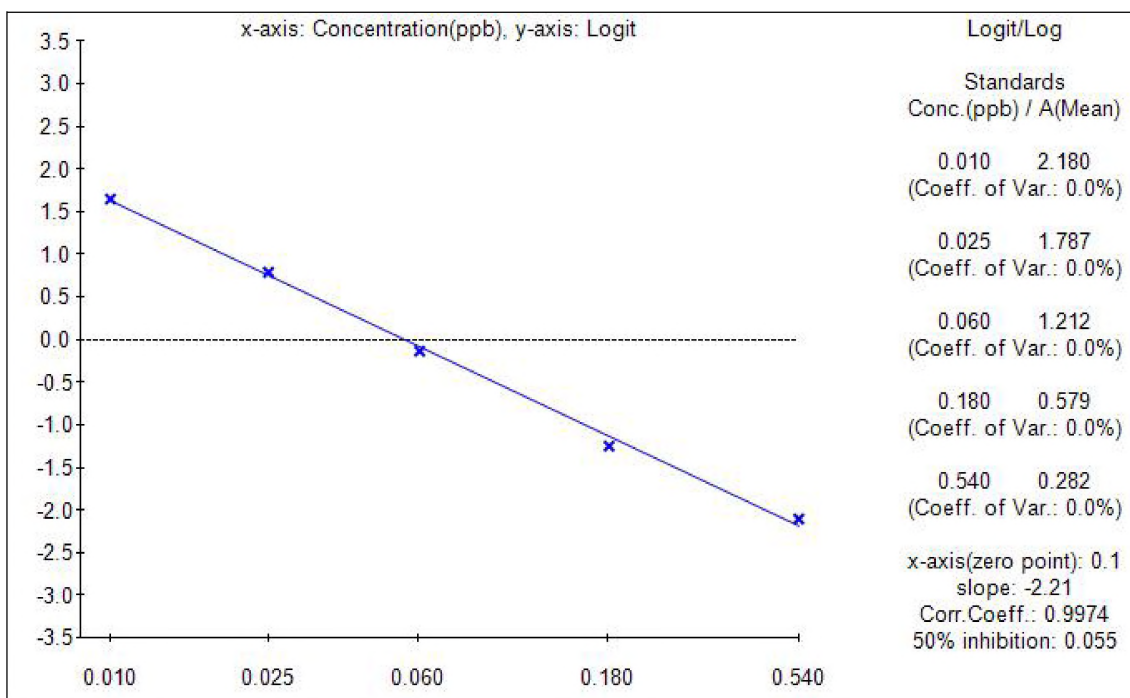

Note: The absorbance of the calibrators may decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date Sep.26<sup>th</sup>, 2023






# Certificate of Conformity

KIT : **Nitrofurantoin(AHD) ELISA Kit RND99024**

Release Date **May.18<sup>th</sup>, 2023**  
 Expiration Date: **May.17<sup>th</sup>, 2024**      Temperature: **25°C**

REAGEN LLC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	1.823	1.801	1.818	1.814	0.0115	0.636	100.00%
0.03 ppb Calibrator	1.447	1.454	1.449	1.45	0.0036	0.249	79.93%
0.1 ppb Calibrator	1.186	1.181	1.182	1.183	0.0026	0.224	65.21%
0.4ppb Calibrator	0.85	0.841	0.826	0.839	0.0121	1.445	46.25%
1.0ppb Calibrator	0.615	0.625	0.626	0.622	0.0061	0.978	34.29%
4.0ppb Calibrator	0.337	0.353	0.348	0.346	0.0082	2.366	19.07%

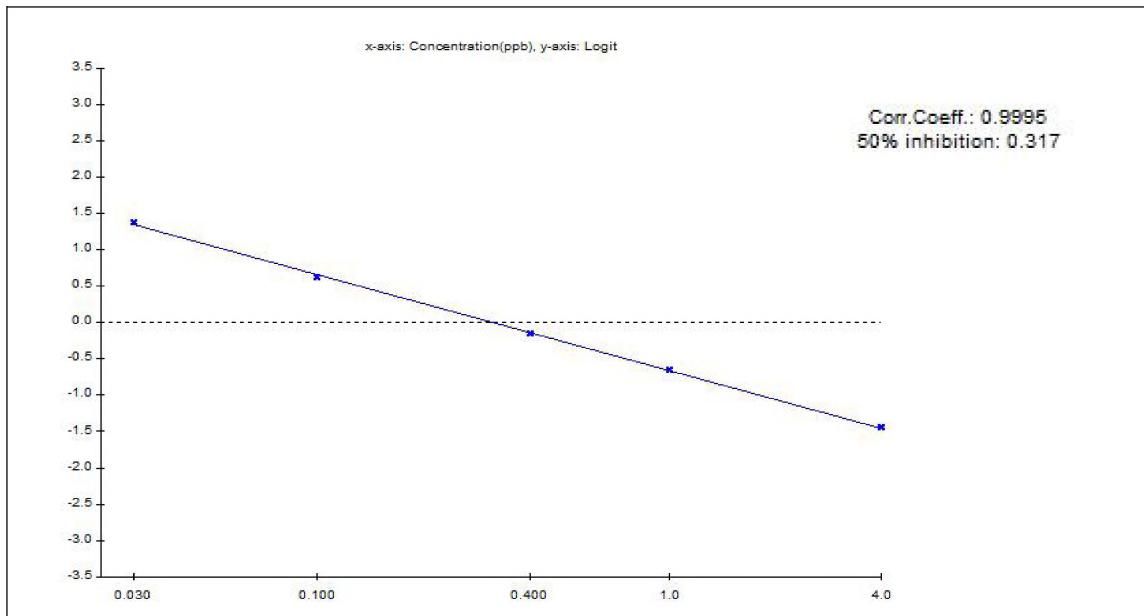

Note: The absorbance of the calibrators may decrease during the shelf life of kit. Actual values may vary; this data is for example purposes only.

QA Manager Alexis      Release Date May.18<sup>th</sup>, 2023








# Certificate of Conformity

KIT : **Nitroimidazole ELISA Kit RND99005**

Release Date Feb.18<sup>th</sup>,2021  
 Expiration Date: Feb.17<sup>th</sup>,2022 Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	1.823	1.801	1.818	1.814	0.012	0.66	<b>100%</b>
1.5 ppb Calibrator	1.447	1.454	1.449	1.450	0.035	2.44	<b>79.9%</b>
3.0 ppb Calibrator	1.186	1.181	1.182	1.183	0.002	1.04	<b>59.7%</b>
6.0 ppb Calibrator	0.850	0.841	0.826	0.839	0.012	1.55	<b>46.3%</b>
12.0 ppb Calibrator	0.615	0.625	0.626	0.622	0.011	1.74	<b>34.3%</b>
24.0 ppb Calibrator	0.337	0.353	0.348	0.346	0.008	2.31	<b>19.1%</b>

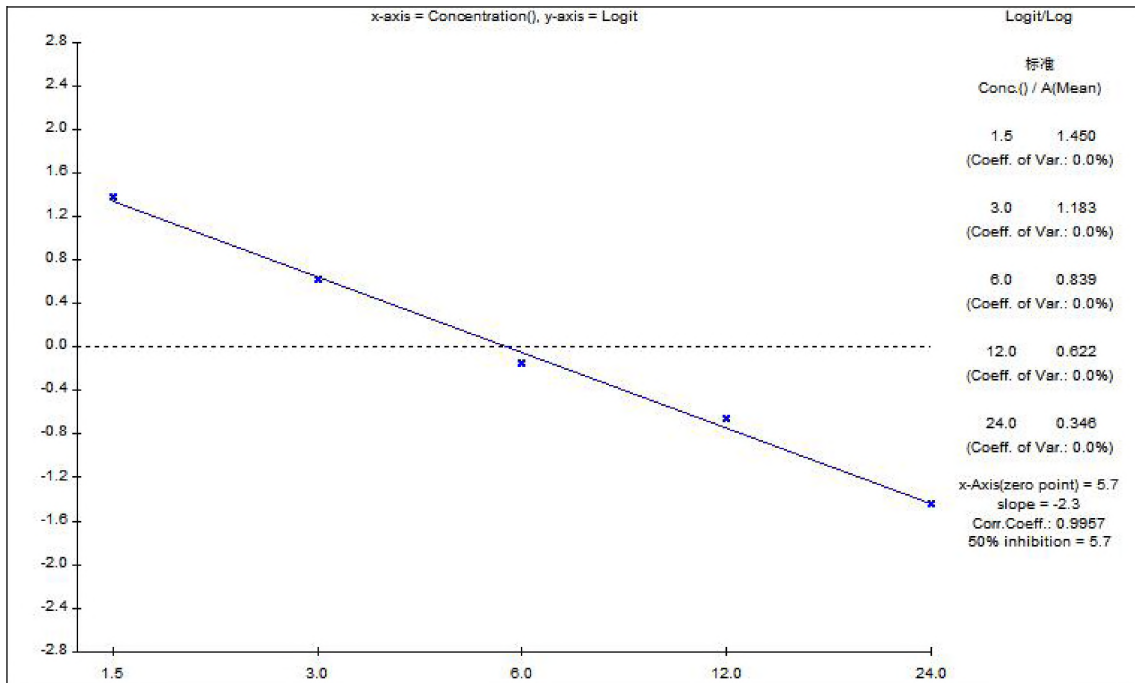

Note: The absorbance of the calibrators may decrease during the shelf life of kit. Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date Feb.18<sup>th</sup>,2021






# Certificate of Conformity

KIT : **Penicillin G ELISA Kit RND99124**

Release Date: Jan.08<sup>th</sup> 2024  
 Expiration Date: Jan.07<sup>th</sup> 2025      Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep. #3	Avg.	Std. Dev.	%RSD	B/Bo
Negative Control	2.018	2.017	2.015	2.017	0.0015	0.076	100%
0.15 ppb Calibrator	1.889	1.885	1.902	1.892	0.0089	0.470	93.8%
0.3 ppb Calibrator	1.634	1.632	1.638	1.635	0.0031	0.187	81.1%
0.6 ppb Calibrator	1.259	1.256	1.261	1.259	0.0025	0.200	62.4%
1.8 ppb Calibrator	0.415	0.412	0.419	0.415	0.0035	0.846	20.6%
5.4 ppb Calibrator	0.159	0.157	0.163	0.160	0.0031	1.913	7.9%

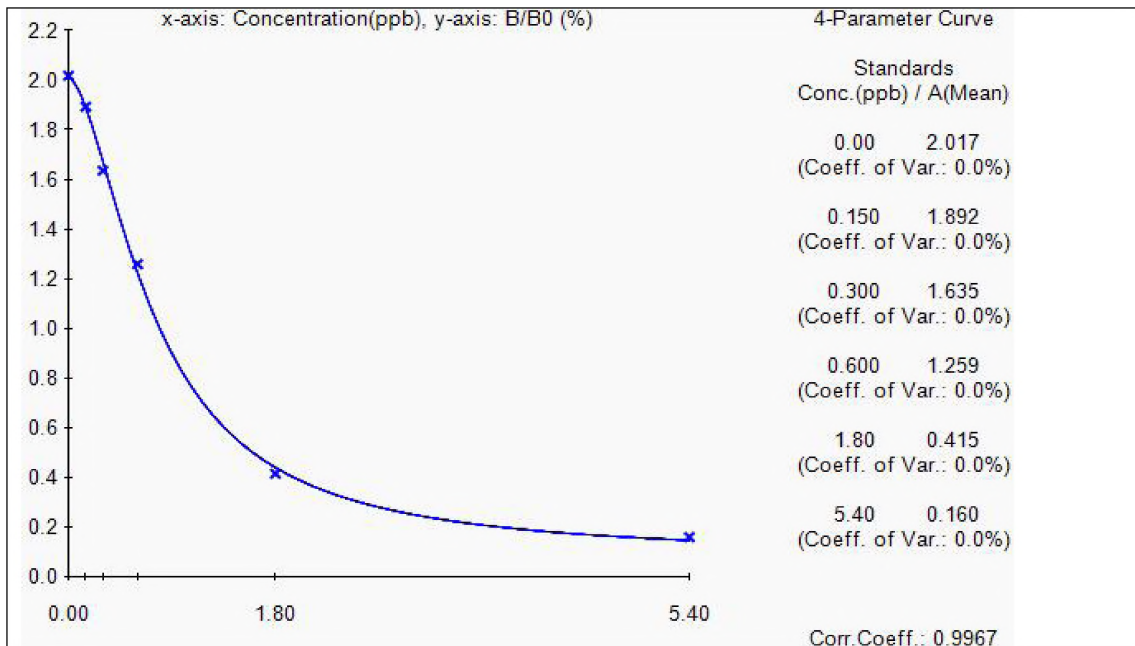

Note: The absorbance of the calibrators may decrease during the shelf life of kit. Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date Jan 08<sup>th</sup> 2024






# Certificate of Conformity

KIT : Nitrofurazone (SEM) ELISA Kit RND99023

Release Date May.26<sup>th</sup>, 2023  
 Expiration Date: May.25<sup>th</sup>, 2024 Temperature: 25°C

REAGEN LLC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	%Bo
Negative Control	2.212	2.215	2.232	2.22	0.0108	0.486	100.00%
0.025 ppb Calibrator	1.944	1.939	1.951	1.945	0.0060	0.310	87.61%
0.1 ppb Calibrator	1.411	1.461	1.436	1.436	0.0250	1.741	64.68%
0.4 ppb Calibrator	0.553	0.551	0.545	0.55	0.0042	0.757	24.77%
0.8 ppb Calibrator	0.28	0.258	0.269	0.269	0.0110	4.089	12.12%
1.6 ppb Calibrator	0.148	0.139	0.143	0.143	0.0045	3.153	6.44%

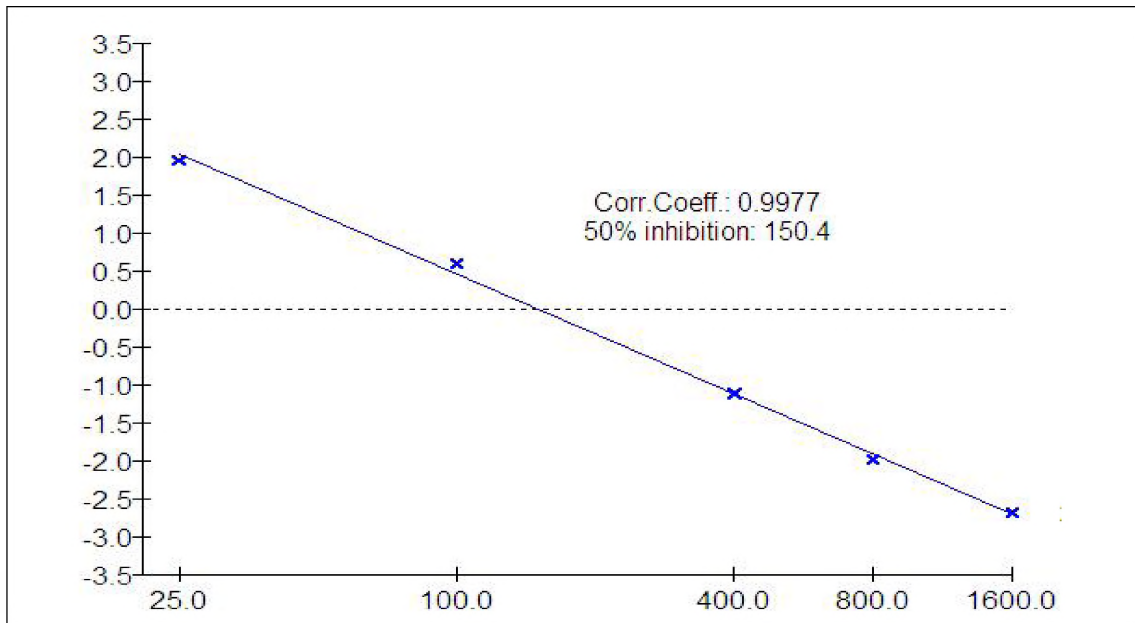

Note: The absorbance of the calibrators may decrease during the shelf life of kit. Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date May.26<sup>th</sup>, 2023






# Certificate of Conformity

KIT : **Streptomycin ELISA Kit RND99002**

Release Date: Jan.08<sup>th</sup> 2024  
 Expiration Date: Jan.07<sup>th</sup> 2025      Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep. #3	Avg.	Std. Dev.	%RSD	B/Bo
Negative Control	2.058	2.056	2.053	2.056	0.0025	0.122	100%
0.05 ppb Calibrator	1.771	1.769	1.768	1.769	0.0015	0.086	86.1%
0.15 ppb Calibrator	1.361	1.359	1.358	1.359	0.0015	0.112	66.1%
0.45 ppb Calibrator	0.698	0.692	0.695	0.695	0.0030	0.432	33.8%
1.35 ppb Calibrator	0.327	0.324	0.325	0.325	0.0015	0.470	15.8%
4.05 ppb Calibrator	0.138	0.135	0.136	0.136	0.0015	1.120	6.6%

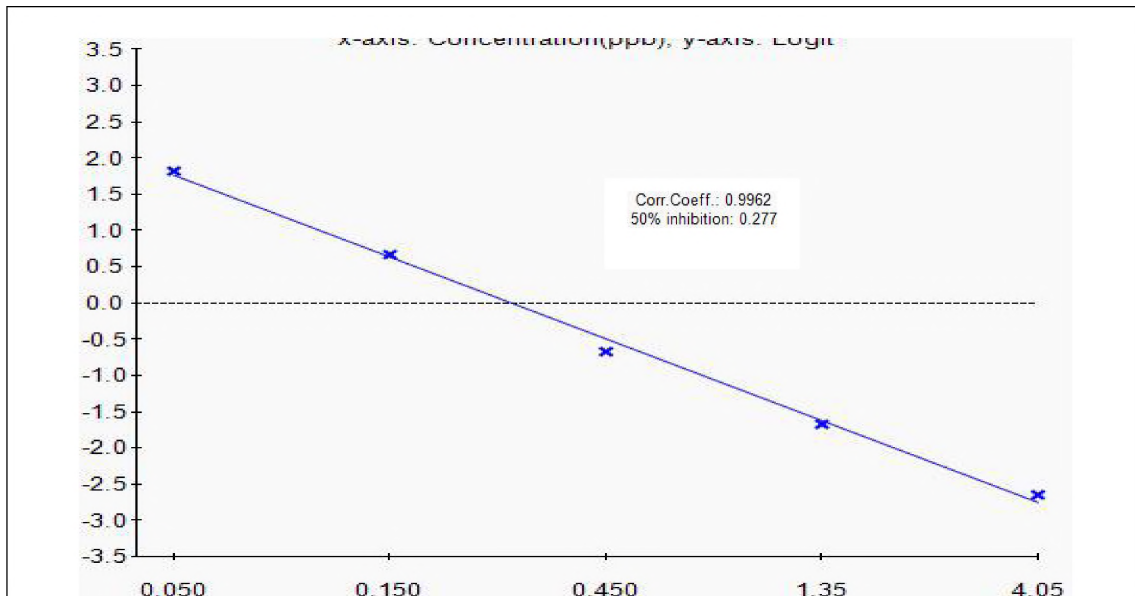

Note: The absorbance of the calibrators may decrease during the shelf life of kit. Actual values may vary; this data is for example purposes only. QA Manager Alexis Release Date Jan 08<sup>th</sup> 2024




# Certificate of Conformity

KIT : Zearalenone ELISA Kit RNM98005

Release Date Feb.12<sup>nd</sup> 2024  
 Expiration Date: Feb.11<sup>st</sup> 2025 Temperature: 25°C

REAGEN INC certifies that this lot has passed Quality control assays and conforms to product release specifications.

Standards	Rep. #1	Rep. #2	Rep.#3	Avg.	Std. Dev.	%RSD	B/Bo
Negative Control	2. 018	2. 002	2. 056	2. 025	0. 0277	1. 369	100%
0.1 ppb Calibrator	1. 819	1. 809	1. 82	1. 816	0. 0061	0. 335	89. 7%
0.4ppb Calibrator	1. 398	1. 418	1. 4	1. 405	0. 0110	0. 784	69. 4%
1.6ppb Calibrator	0. 607	0. 687	0. 65	0. 648	0. 0400	6. 179	32. 0%
6.4ppb Calibrator	0. 239	0. 29	0. 273	0. 267	0. 0260	9. 714	13. 2%
25.6 ppb Calibrator	0. 107	0. 102	0. 098	0. 102	0. 0045	4. 406	5. 1%

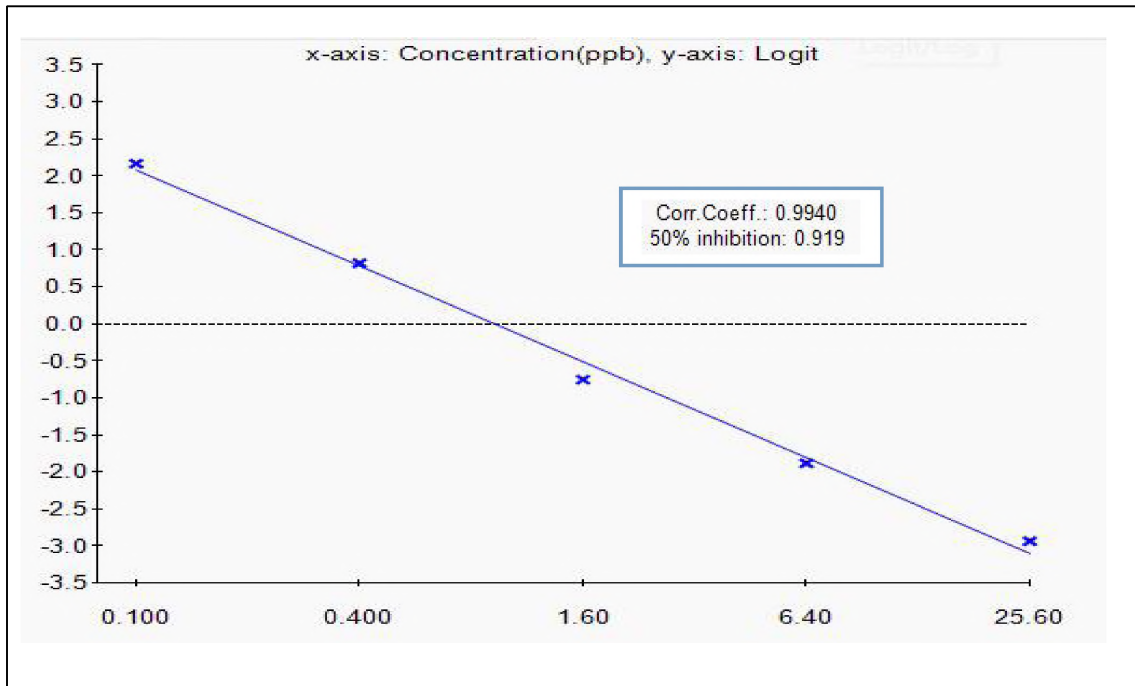

Note: The absorbance of the calibrators may Decrease during the shelf life of kit . Actual values may vary; this data is for example purposes only.

QA Manager Alexis Release Date Feb. 12<sup>nd</sup> 2024

